

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 15:15
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 03:50:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 03:48:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.562	51662886	62745442	23.508	23.637
28)	SA Decachlor...	8.761	7.627	45138229	57723768	24.337	24.047
Target Compounds							
9)	A Endosulfan I	5.834	4.825	29241462	39060136	11.264	11.655
10)	B gamma-Chl...	5.706	4.711	31454181	41828334	11.330	11.975
12)	B 4,4'-DDE	5.966	4.967	53072554	73165226	22.006	22.755
13)	MA Dieldrin	6.112	5.087	60212900	81486432	22.816	23.546
19)	B Endosulfa...	6.937	6.055	49441053	63250693	21.547	21.795
20)	A Methoxychlor	7.285	6.341	137.7E6	157.0E6	116.780	110.733
21)	B Endrin ke...	7.422	6.551	56900822	74514000	23.305	23.332


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 15:15
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 03:50:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 03:48:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

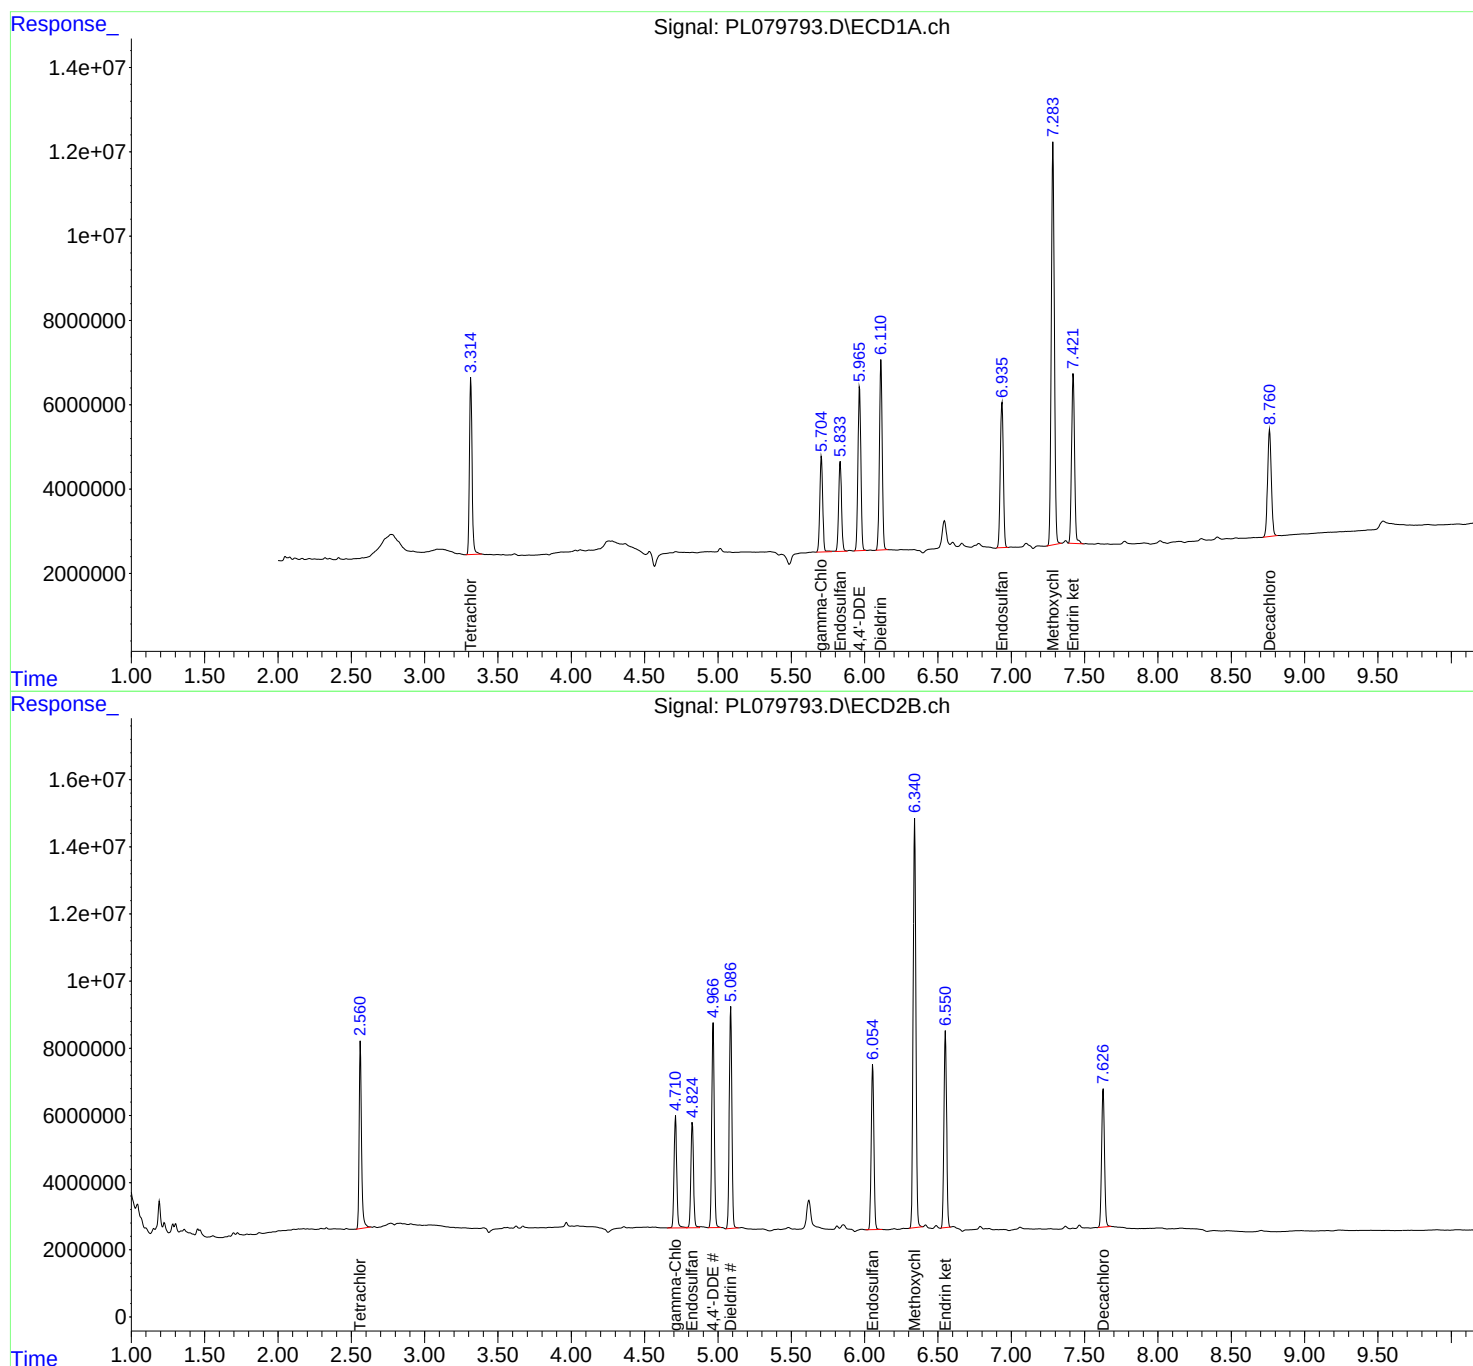


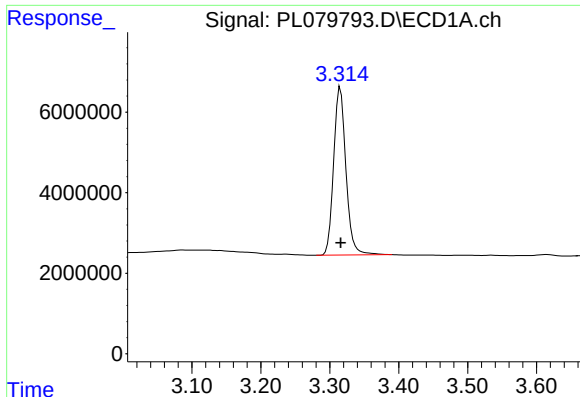

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 51662886
Conc: 23.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

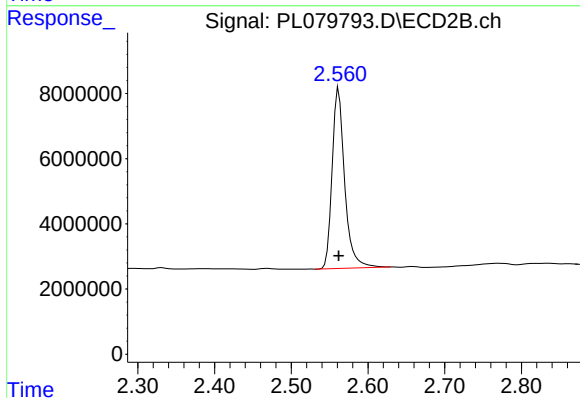


#1 Tetrachloro-m-xylene

R.T.: 2.562 min
Delta R.T.: 0.000 min
Response: 62745442
Conc: 23.64 ng/ml

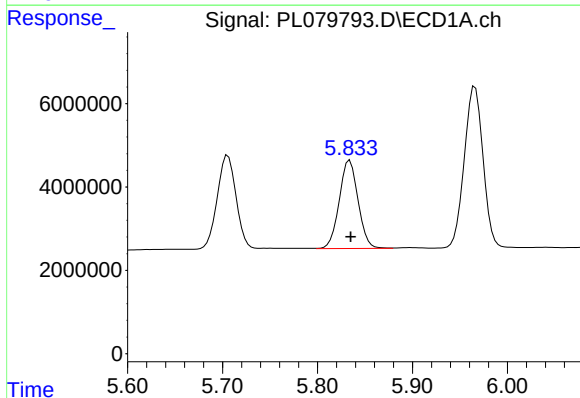


#9 Endosulfan I

R.T.: 5.834 min
Delta R.T.: -0.001 min
Response: 29241462
Conc: 11.26 ng/ml

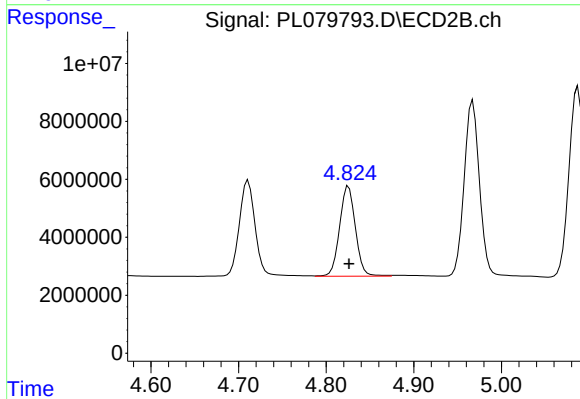

#9 Endosulfan I


R.T.: 4.825 min
Delta R.T.: 0.000 min
Response: 39060136
Conc: 11.65 ng/ml

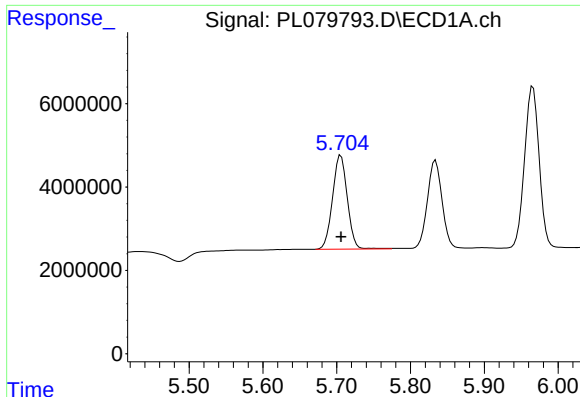

#10 gamma-Chlordane


R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 31454181
Conc: 11.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

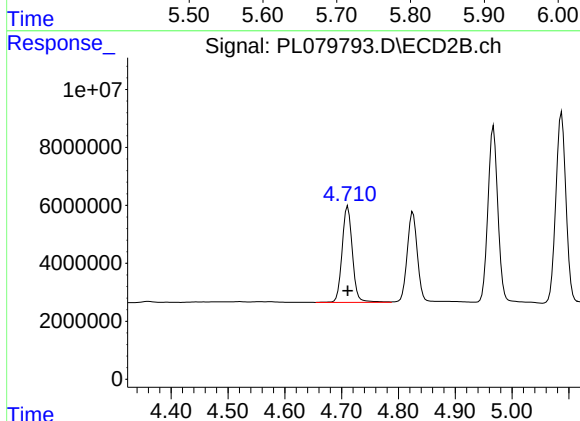


#10 gamma-Chlordane

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 41828334
Conc: 11.97 ng/ml

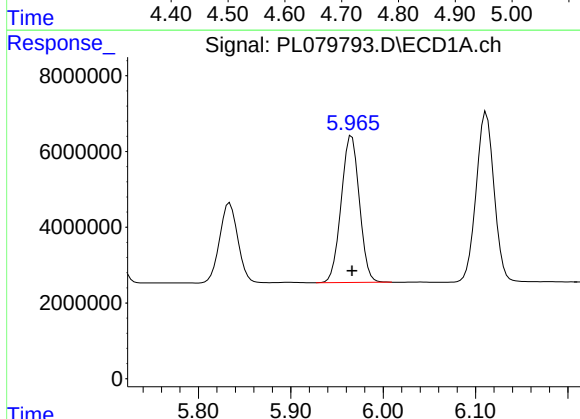


#12 4,4'-DDE

R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 53072554
Conc: 22.01 ng/ml

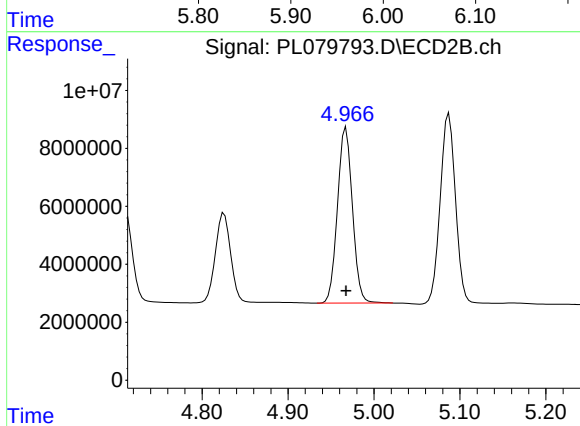

#12 4,4'-DDE


R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 73165226
Conc: 22.75 ng/ml

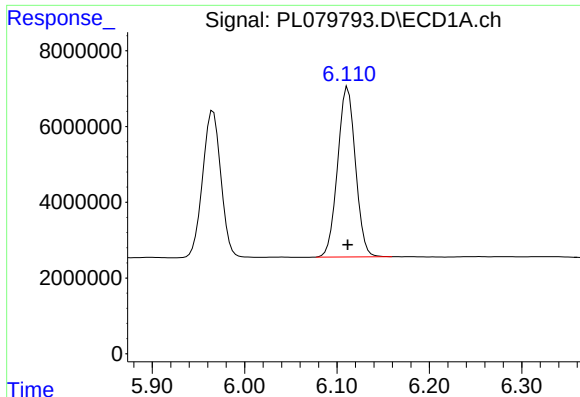

#13 Dieldrin


R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 60212900
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

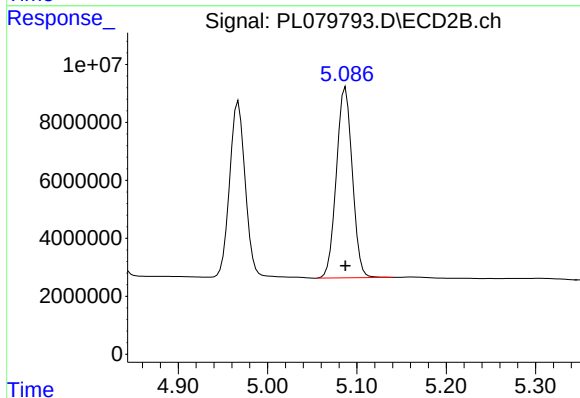


#13 Dieldrin

R.T.: 5.087 min
Delta R.T.: 0.000 min
Response: 81486432
Conc: 23.55 ng/ml

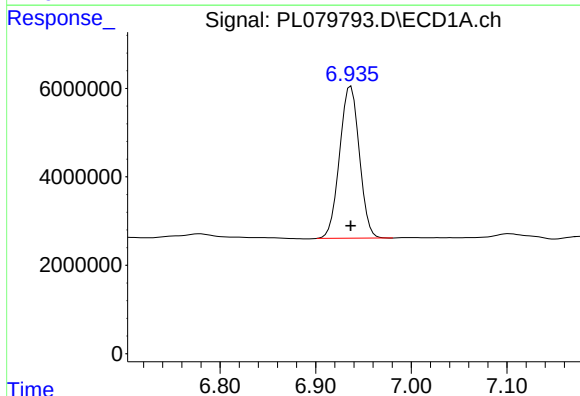


#19 Endosulfan Sulfate

R.T.: 6.937 min
Delta R.T.: 0.000 min
Response: 49441053
Conc: 21.55 ng/ml

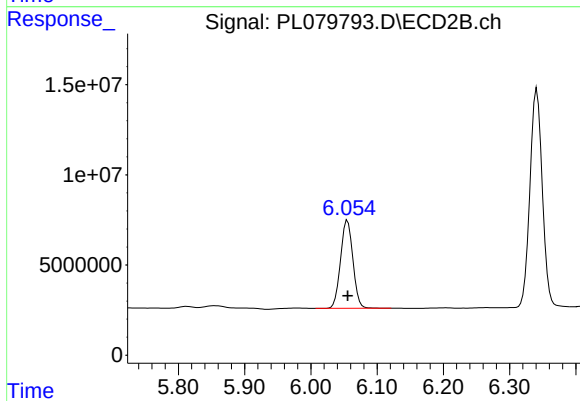

#19 Endosulfan Sulfate


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 63250693
Conc: 21.79 ng/ml

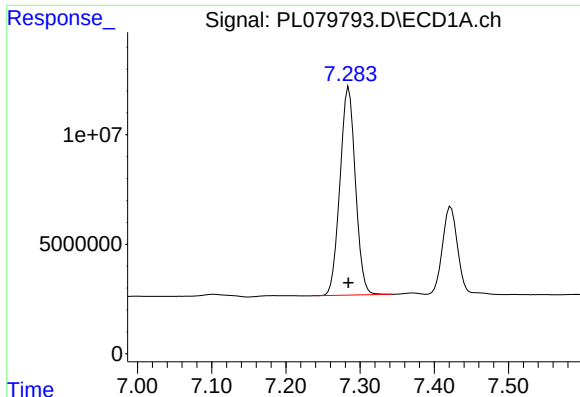

#20 Methoxychlor


R.T.: 7.285 min
Delta R.T.: 0.000 min
Response: 137650991
Conc: 116.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

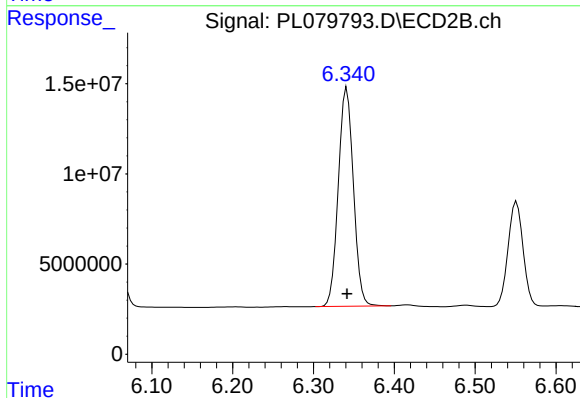


#20 Methoxychlor

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 157026424
Conc: 110.73 ng/ml

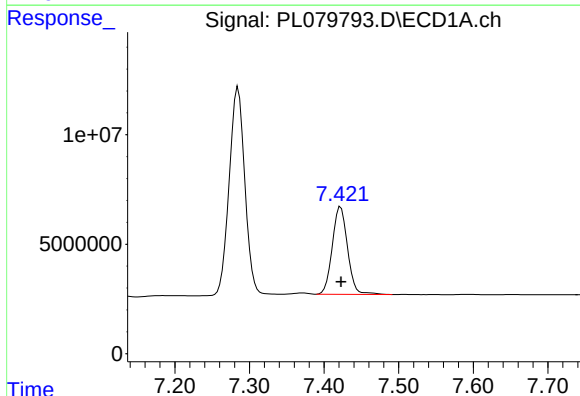


#21 Endrin ketone

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 56900822
Conc: 23.30 ng/ml

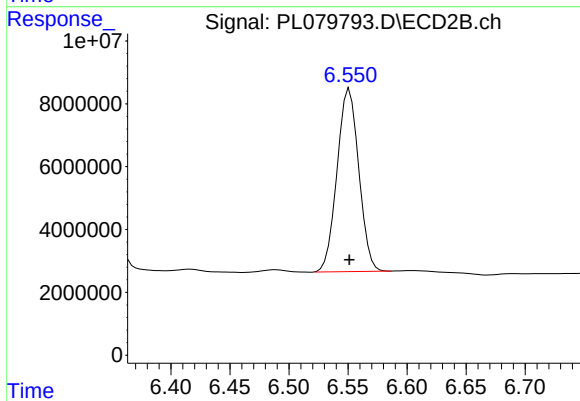

#21 Endrin ketone


R.T.: 6.551 min
Delta R.T.: 0.000 min
Response: 74514000
Conc: 23.33 ng/ml

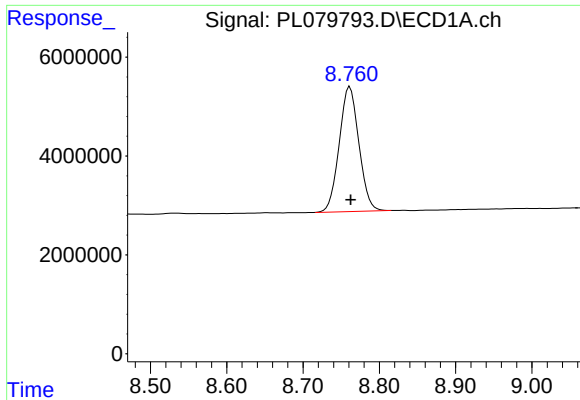

#28 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: -0.001 min
Response: 45138229
Conc: 24.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

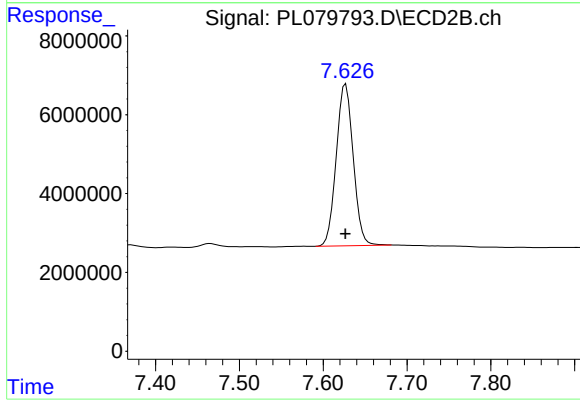

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 57723768
Conc: 24.05 ng/ml