

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 16:38
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:18:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 02:18:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.561	222.0E6	318.5E6	102.026	100.468
28)	SA Decachlor...	8.762	7.627	178.7E6	229.2E6	98.411	98.163
Target Compounds							
23)	Chlordane-1	4.464	3.526	95367821	104.5E6	1020.317	1000.305
24)	Chlordane-2	4.997	4.092	99190962	110.9E6	993.966	985.438
25)	Chlordane-3	5.706	4.711	416.3E6	343.5E6	1027.963	1007.250
26)	Chlordane-4	5.784	4.771	500.0E6	365.0E6	1020.605	1003.567
27)	Chlordane-5	6.641	5.432	83177928	91970663	1022.280	993.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 16:38
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:18:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 02:18:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

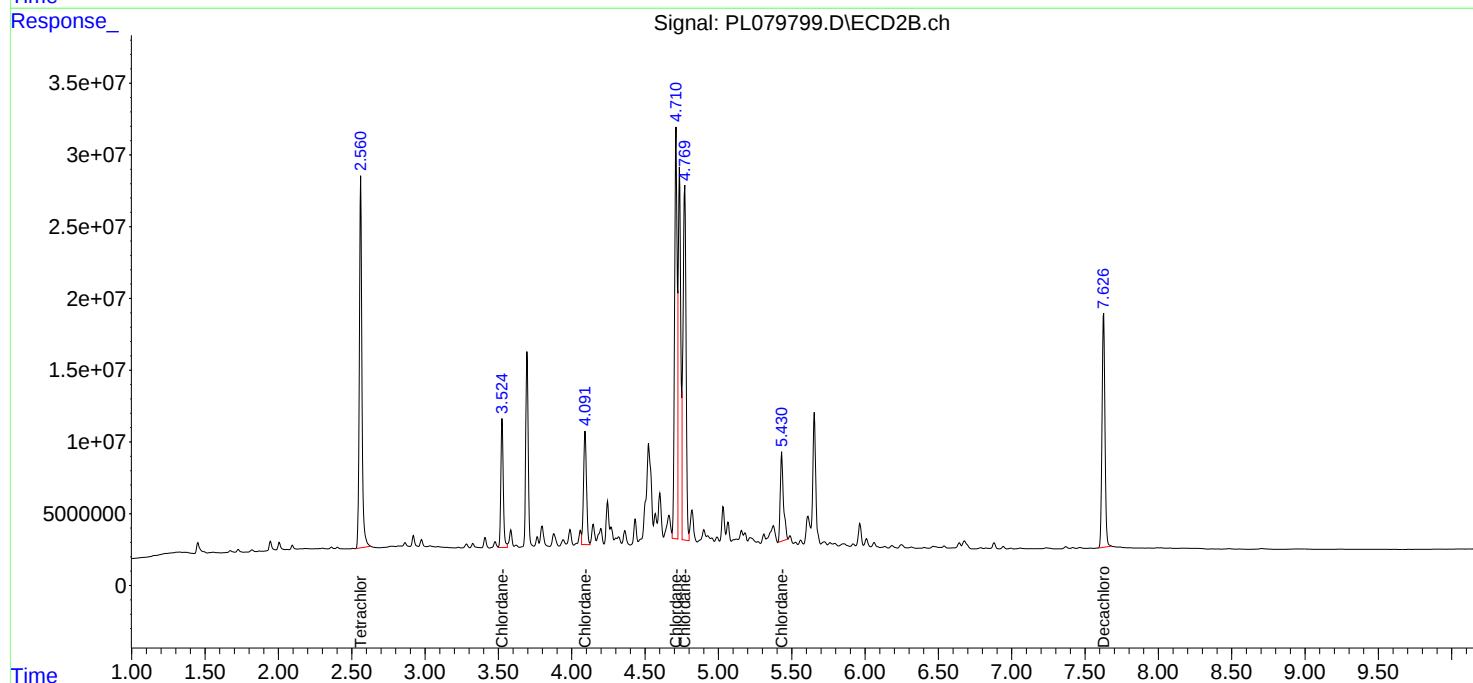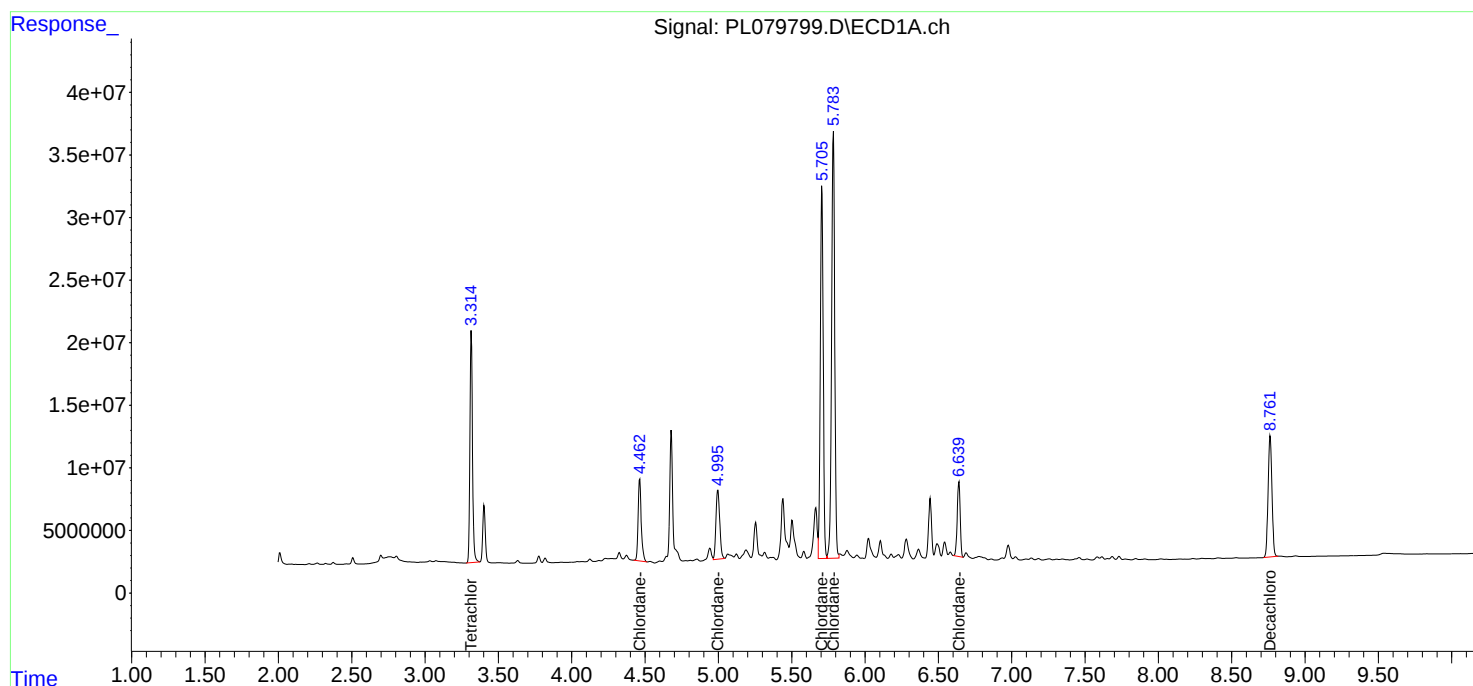


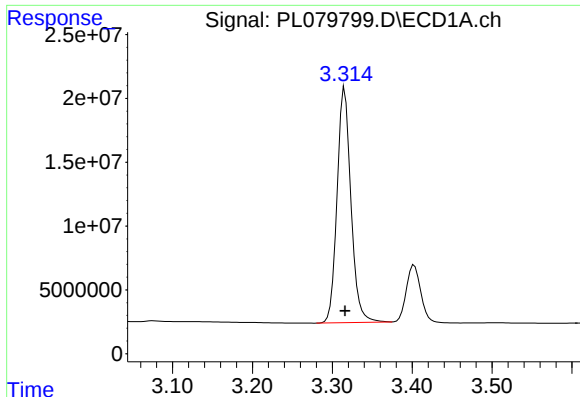

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: 0.000 min
Response: 222040285
Conc: 102.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

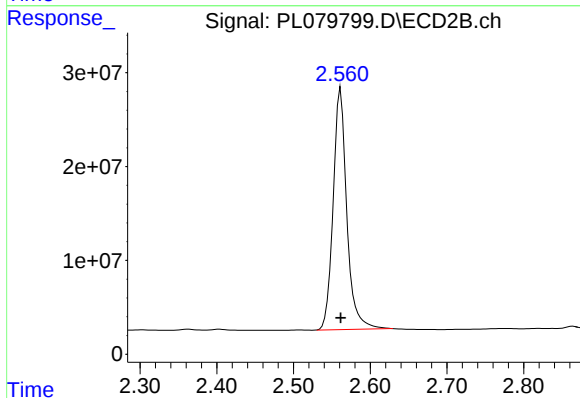


#1 Tetrachloro-m-xylene

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 318503557
Conc: 100.47 ng/ml

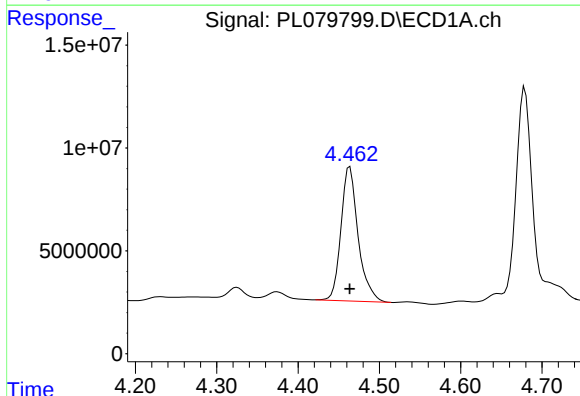


#23 Chlordane-1

R.T.: 4.464 min
Delta R.T.: 0.000 min
Response: 95367821
Conc: 1020.32 ng/ml

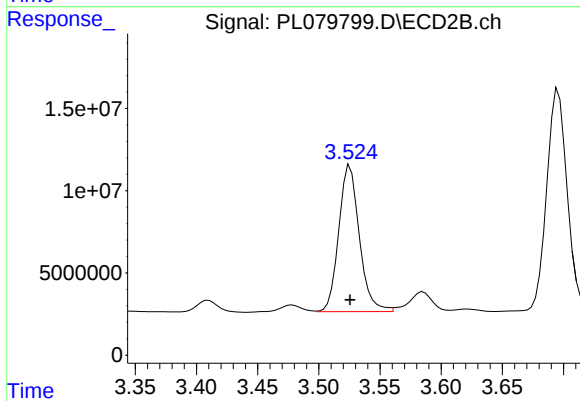

#23 Chlordane-1


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 104493758
Conc: 1000.30 ng/ml

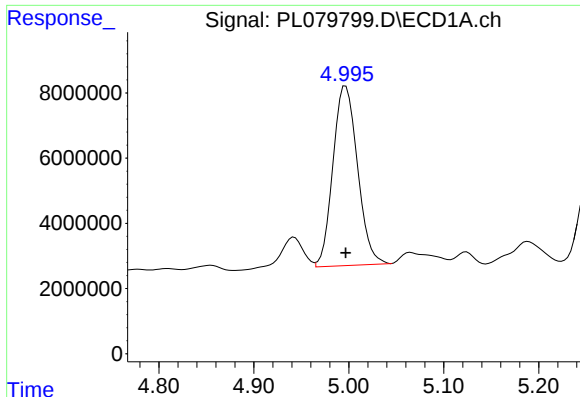

#24 Chlordane-2


R.T.: 4.997 min
Delta R.T.: 0.000 min
Response: 99190962
Conc: 993.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

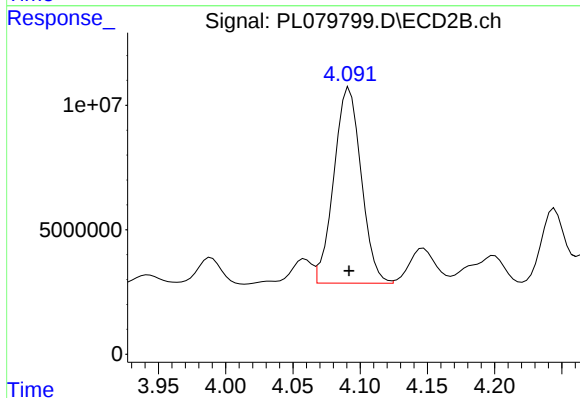


#24 Chlordane-2

R.T.: 4.092 min
Delta R.T.: 0.000 min
Response: 110910591
Conc: 985.44 ng/ml

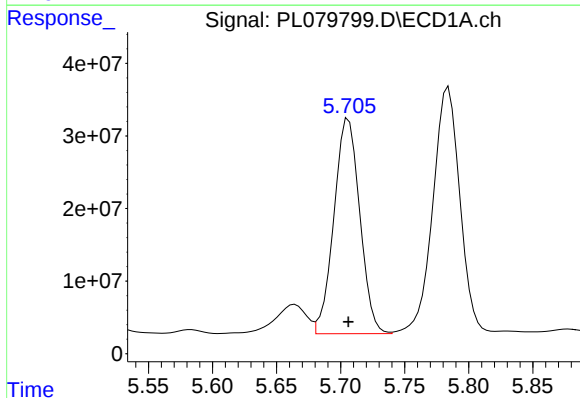


#25 Chlordane-3

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 416333008
Conc: 1027.96 ng/ml

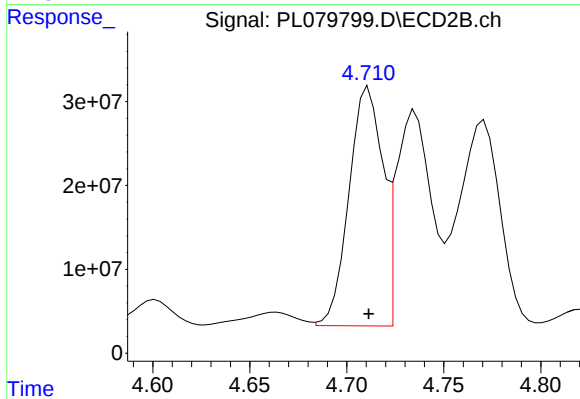

#25 Chlordane-3


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 343534565
Conc: 1007.25 ng/ml

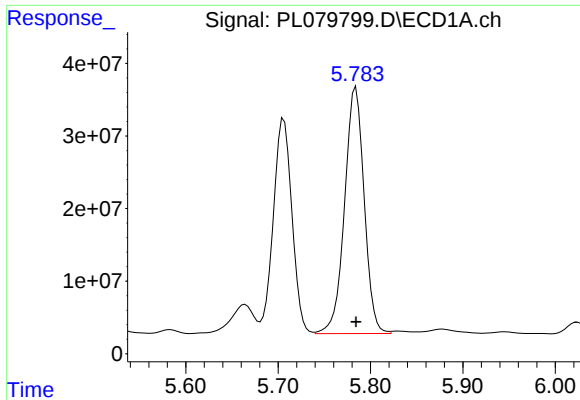

#26 Chlordane-4


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 499968796
Conc: 1020.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

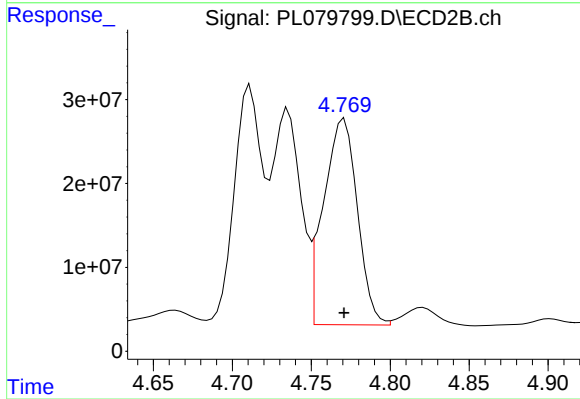


#26 Chlordane-4

R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 365011454
Conc: 1003.57 ng/ml

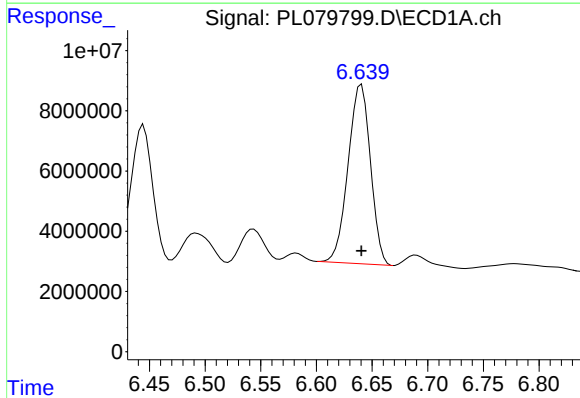


#27 Chlordane-5

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 83177928
Conc: 1022.28 ng/ml

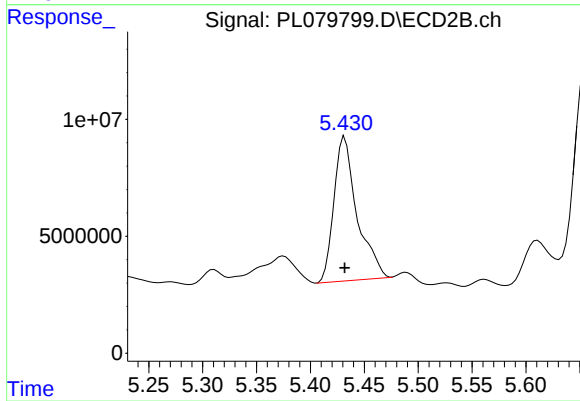

#27 Chlordane-5


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 91970663
Conc: 993.81 ng/ml

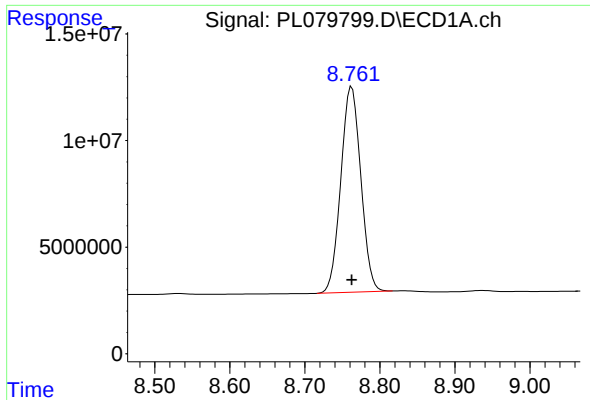

#28 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 178686863
Conc: 98.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

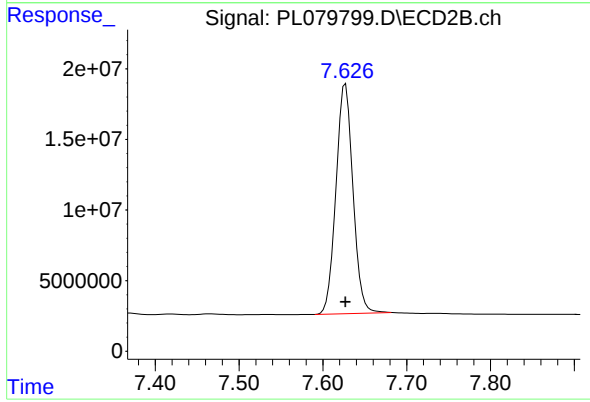

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 229188181
Conc: 98.16 ng/ml