

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 16:52
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:28:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 02:28:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.561	157.5E6	231.0E6	73.213	73.568
28)	SA Decachlor...	8.762	7.627	132.3E6	168.9E6	73.572	73.207
Target Compounds							
23)	Chlordane-1	4.463	3.525	68379004	75585982	737.612	732.174
24)	Chlordane-2	4.996	4.091	72426314	82107110	733.667	736.221
25)	Chlordane-3	5.706	4.711	295.6E6	245.3E6	736.409	729.185
26)	Chlordane-4	5.784	4.771	356.9E6	265.8E6	735.590	737.035
27)	Chlordane-5	6.640	5.432	59641090	67221613	738.584	734.083



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 16:52
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:28:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 02:28:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

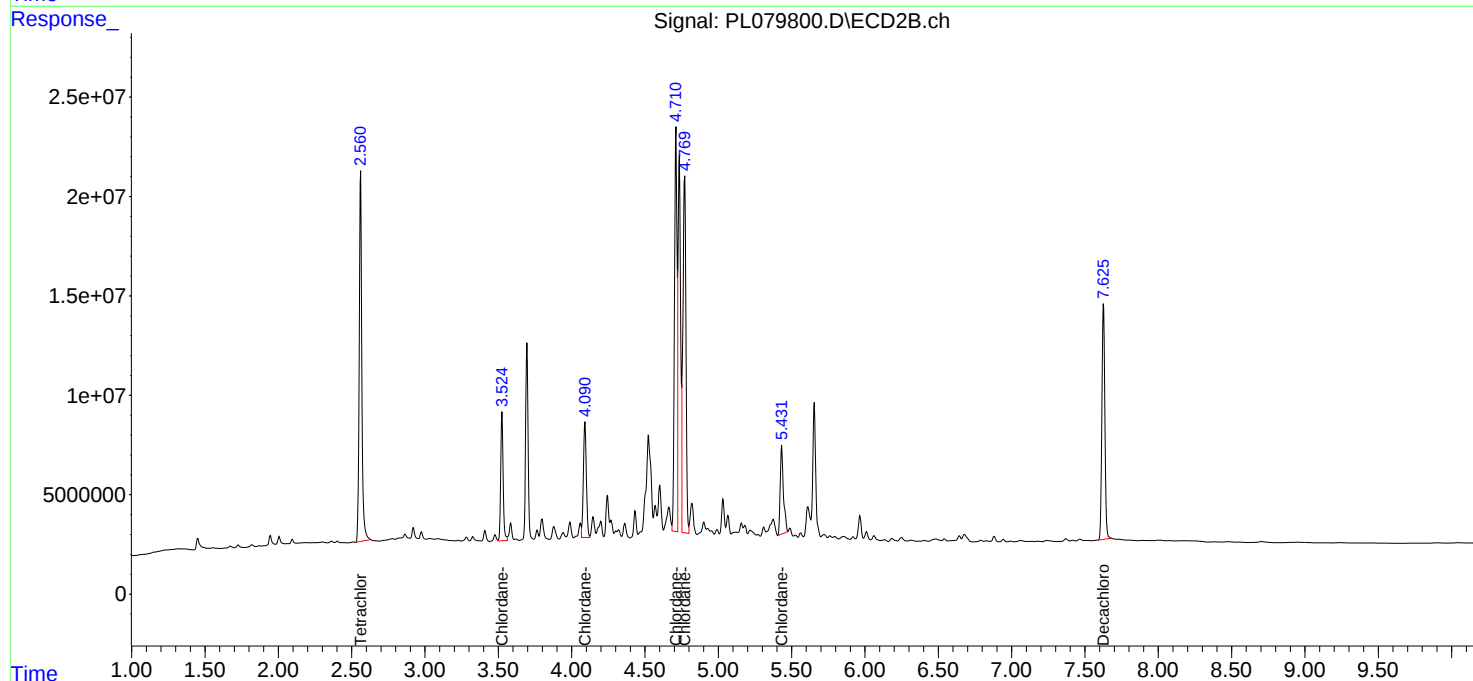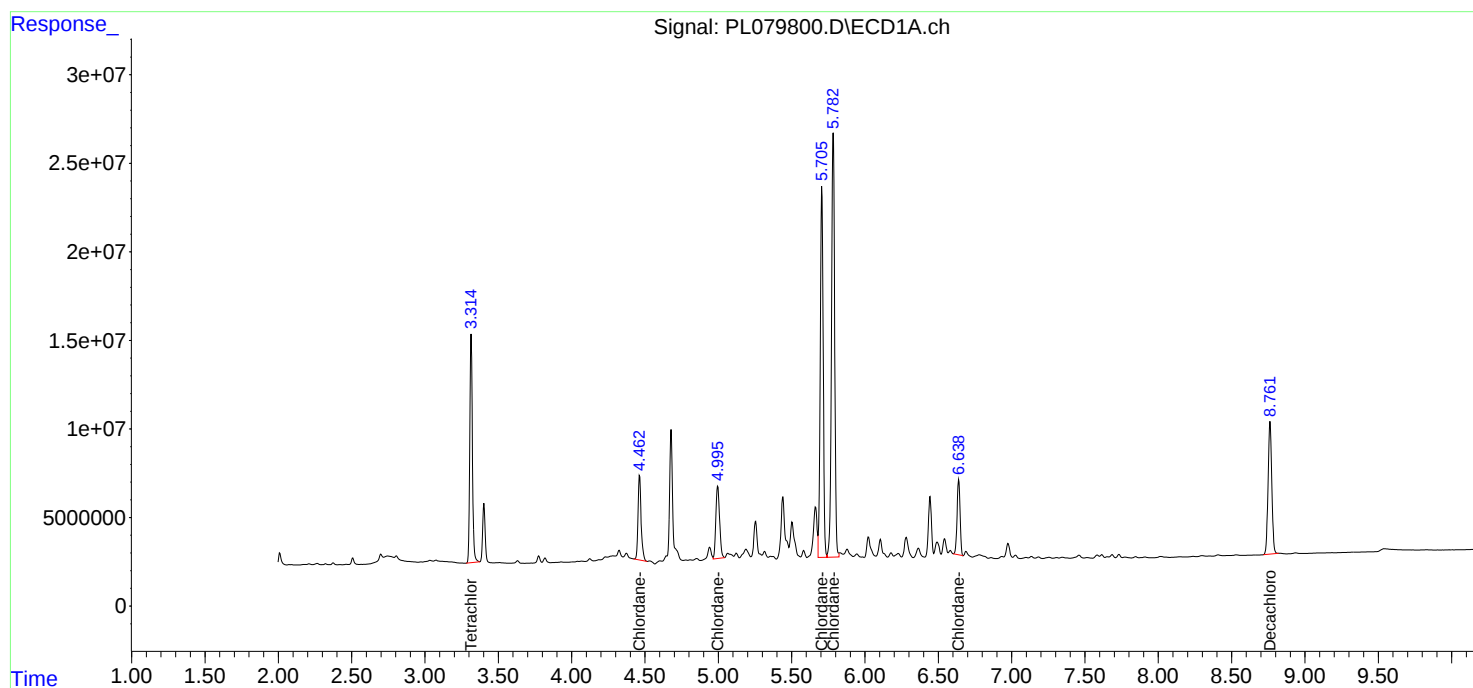


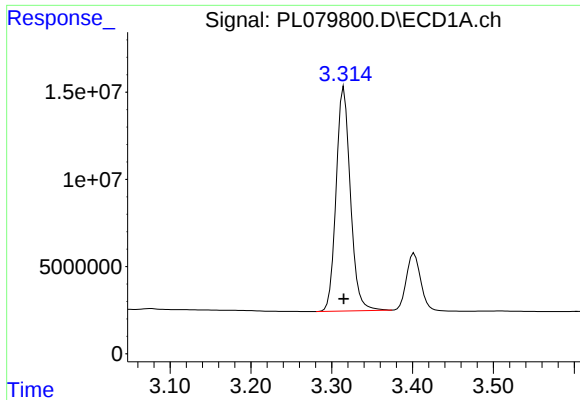

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 157457772
Conc: 73.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

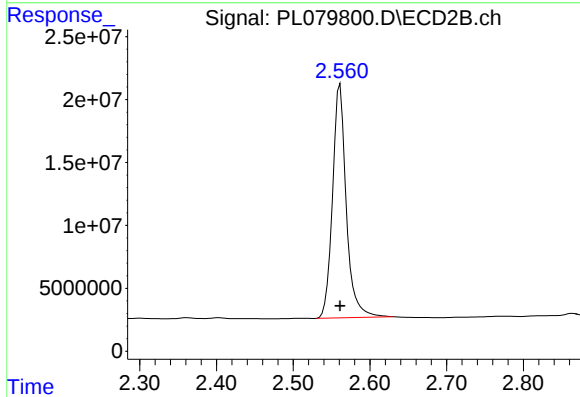


#1 Tetrachloro-m-xylene

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 231017489
Conc: 73.57 ng/ml

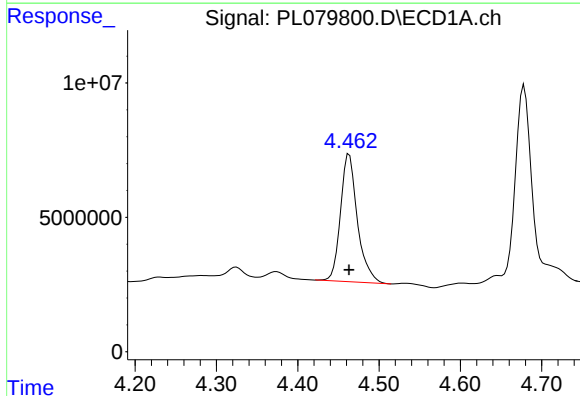


#23 Chlordane-1

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 68379004
Conc: 737.61 ng/ml

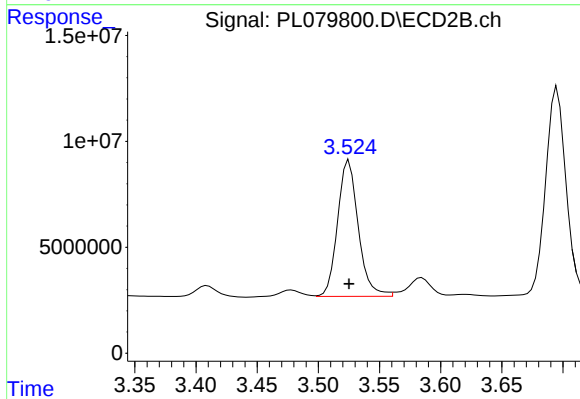

#23 Chlordane-1


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 75585982
Conc: 732.17 ng/ml

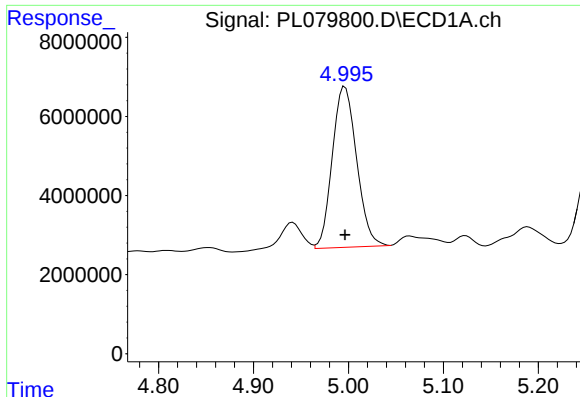

#24 Chlordane-2


R.T.: 4.996 min
Delta R.T.: 0.000 min
Response: 72426314
Conc: 733.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

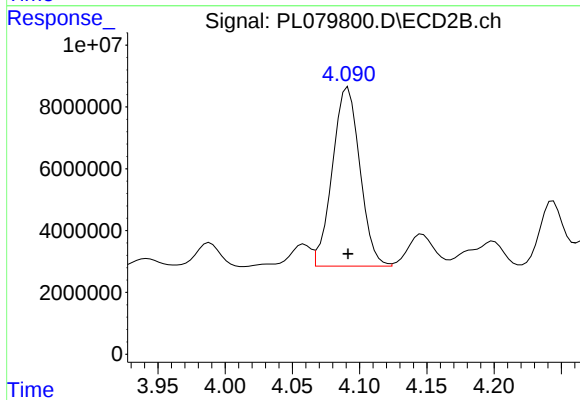


#24 Chlordane-2

R.T.: 4.091 min
Delta R.T.: 0.000 min
Response: 82107110
Conc: 736.22 ng/ml

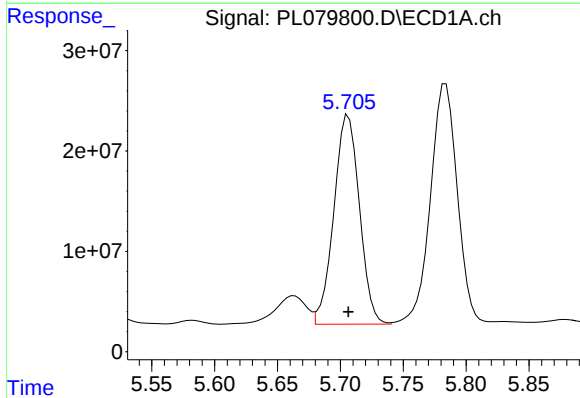


#25 Chlordane-3

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 295572983
Conc: 736.41 ng/ml

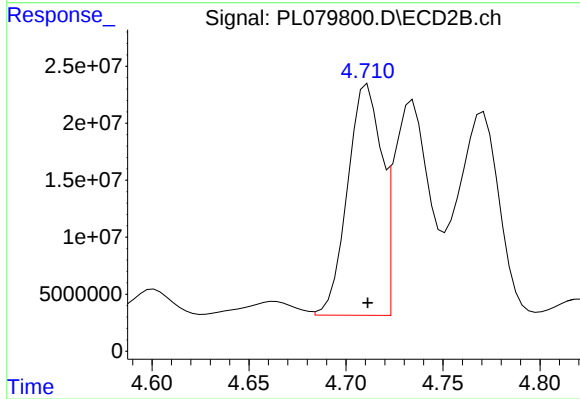

#25 Chlordane-3


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 245293413
Conc: 729.19 ng/ml

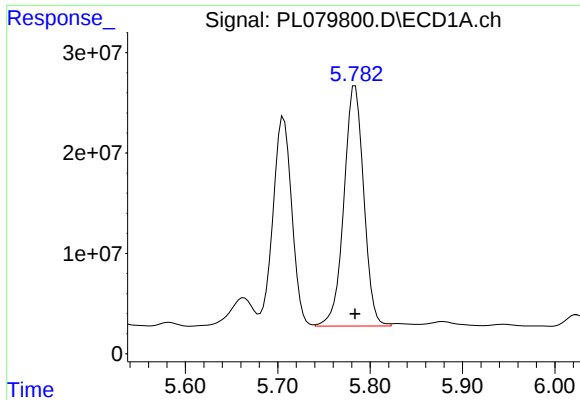

#26 Chlordane-4


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 356918656
Conc: 735.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

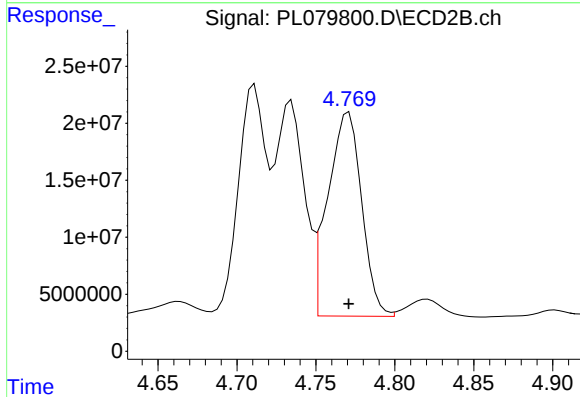


#26 Chlordane-4

R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 265772881
Conc: 737.04 ng/ml

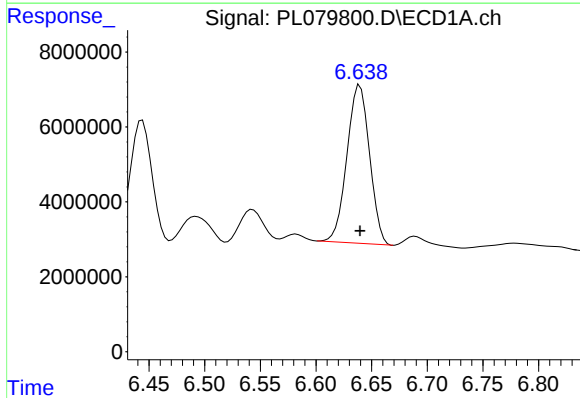


#27 Chlordane-5

R.T.: 6.640 min
Delta R.T.: 0.000 min
Response: 59641090
Conc: 738.58 ng/ml

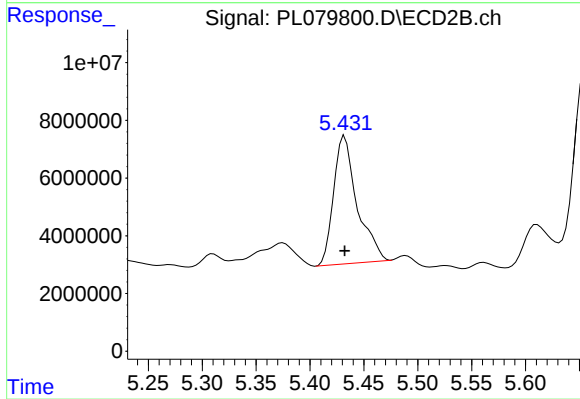

#27 Chlordane-5


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 67221613
Conc: 734.08 ng/ml

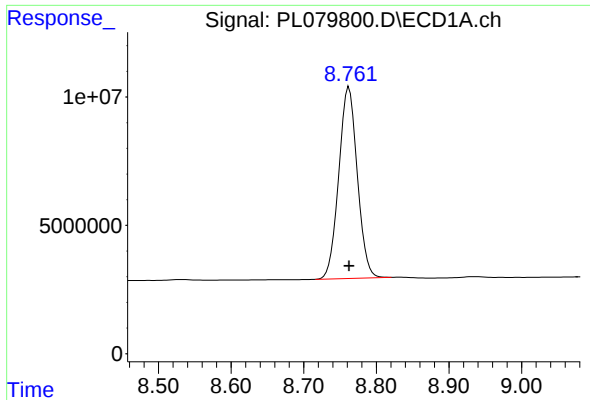

#28 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 132326961
Conc: 73.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

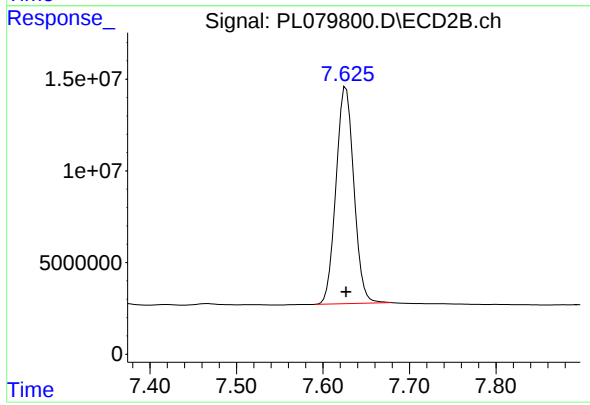

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 168902363
Conc: 73.21 ng/ml