

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 17:06
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:45:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 01:39:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.561	106.6E6	157.8E6	50.000	50.000
28)	SA Decachlor...	8.760	7.627	92228867	118.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.463	3.525	45784896	52215024	500.000	500.000
24)	Chlordane-2	4.996	4.091	50197638	57094280	500.000	500.000
25)	Chlordane-3	5.706	4.711	196.8E6	169.3E6	500.000	500.000
26)	Chlordane-4	5.784	4.771	239.9E6	181.2E6	500.000	500.000
27)	Chlordane-5	6.639	5.432	39776154	46558594	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 17:06
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:45:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 01:39:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

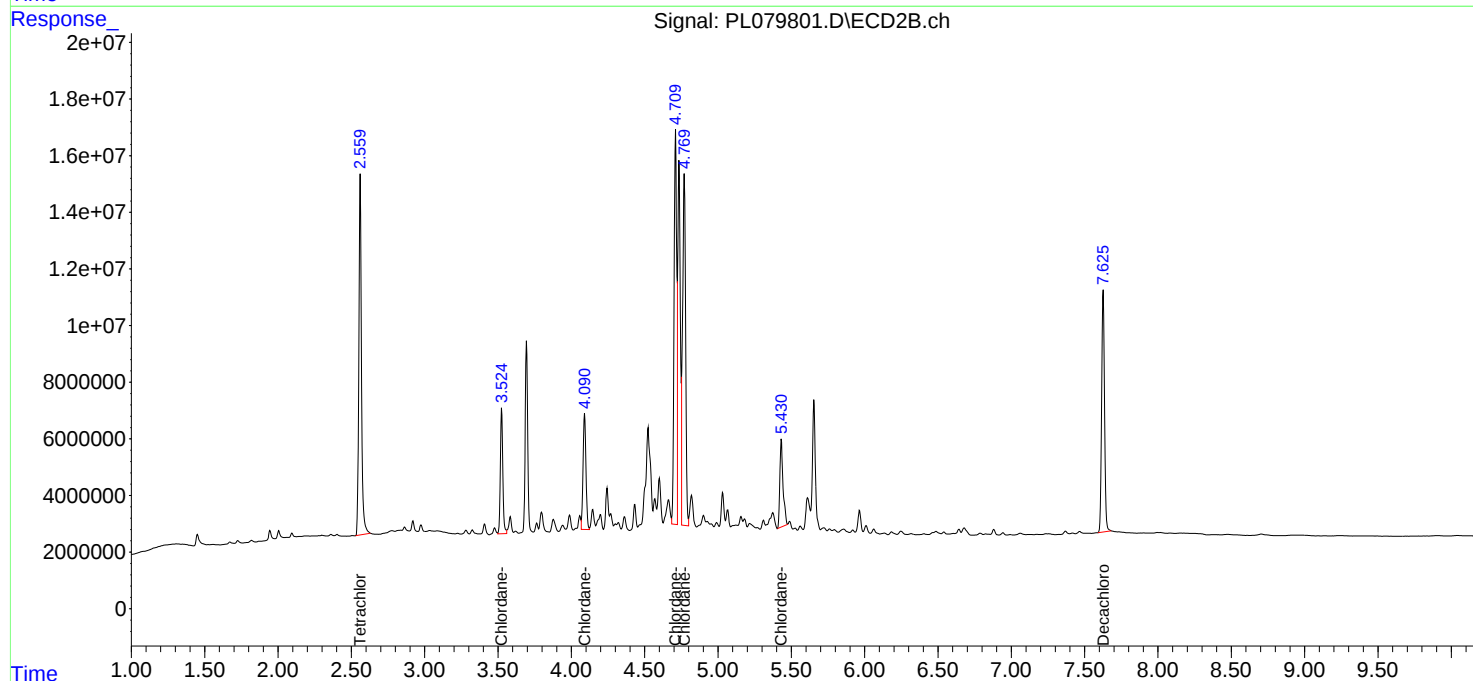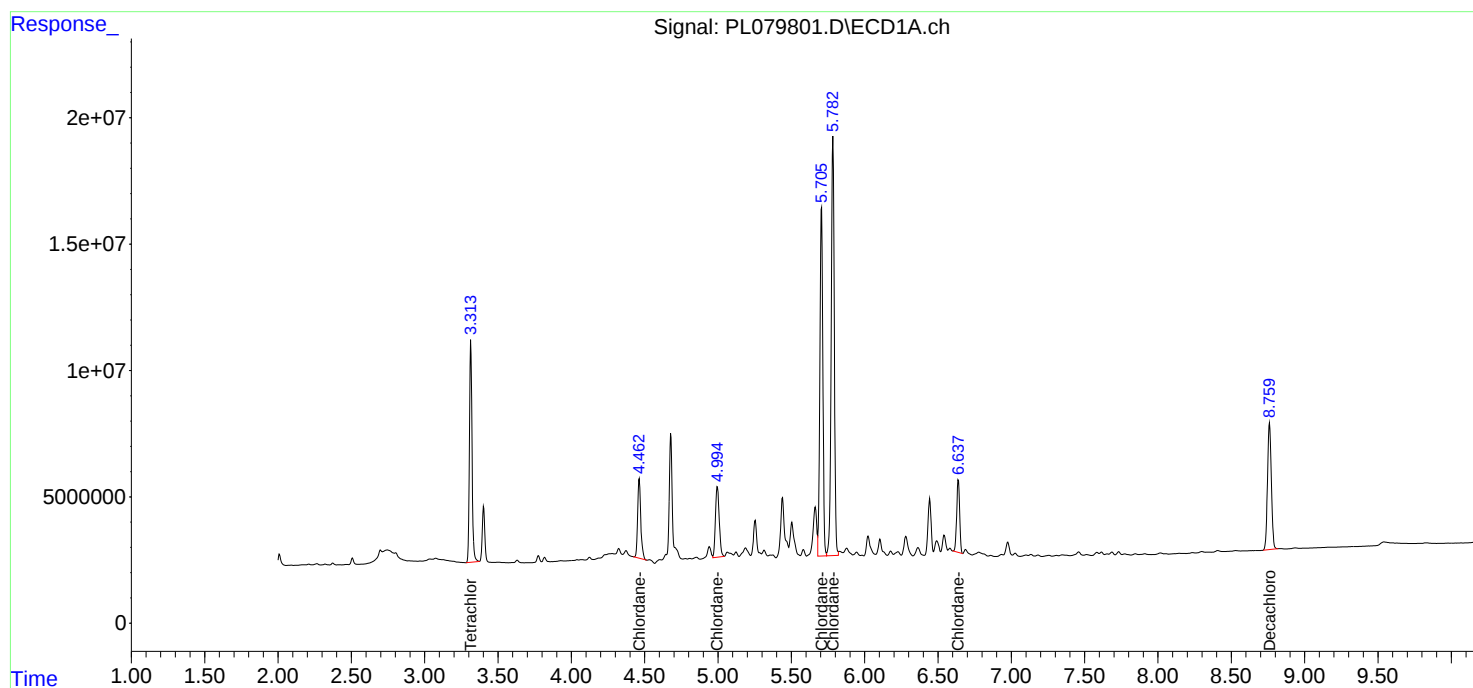


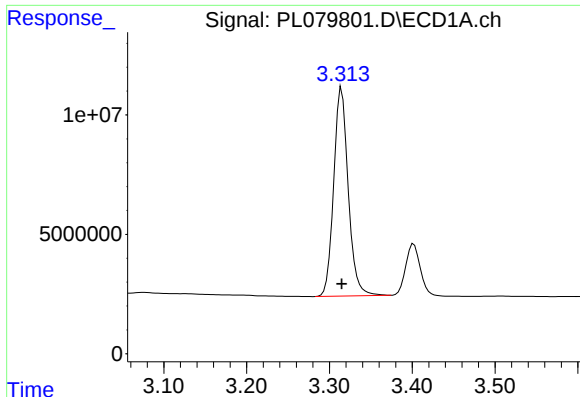

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 106611350
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

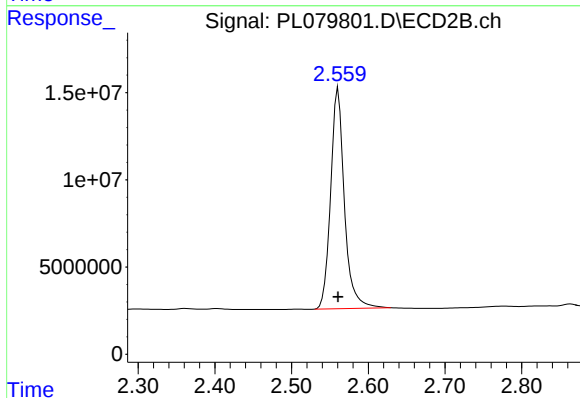


#1 Tetrachloro-m-xylene

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 157768057
Conc: 50.00 ng/ml

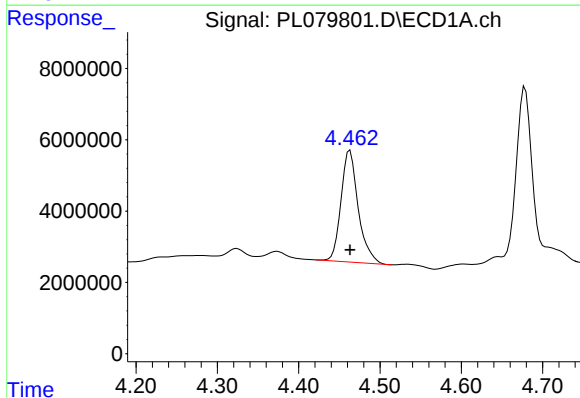


#23 Chlordane-1

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 45784896
Conc: 500.00 ng/ml

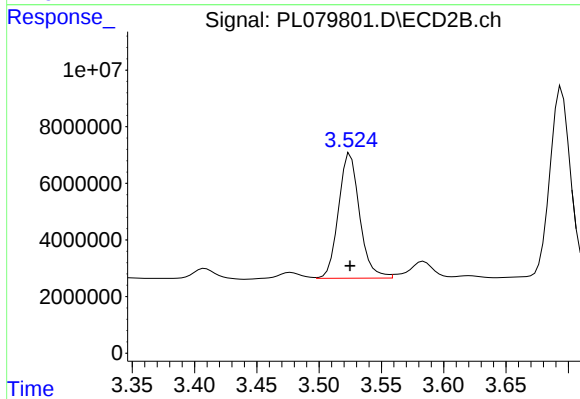

#23 Chlordane-1


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 52215024
Conc: 500.00 ng/ml

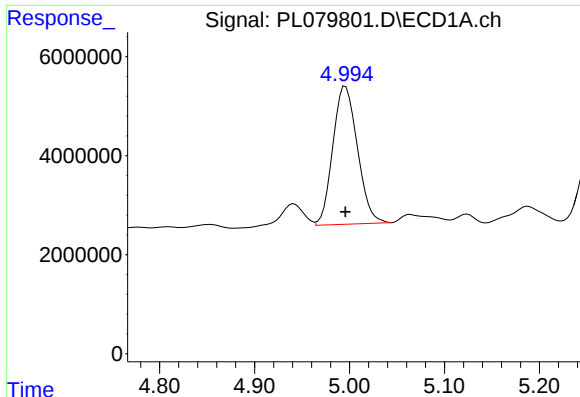

#24 Chlordane-2


R.T.: 4.996 min
Delta R.T.: 0.000 min
Response: 50197638
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

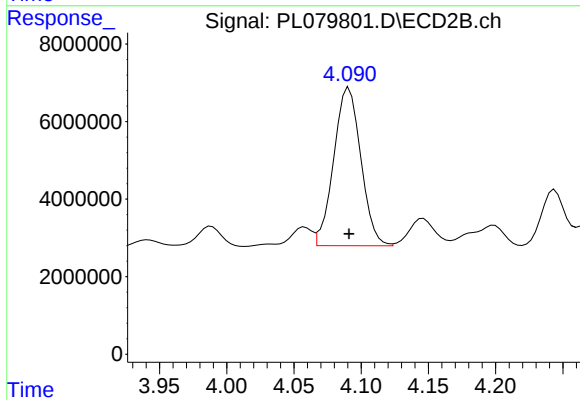


#24 Chlordane-2

R.T.: 4.091 min
Delta R.T.: 0.000 min
Response: 57094280
Conc: 500.00 ng/ml

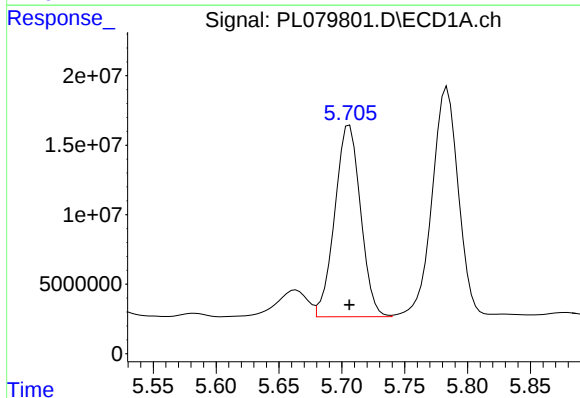


#25 Chlordane-3

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 196841216
Conc: 500.00 ng/ml

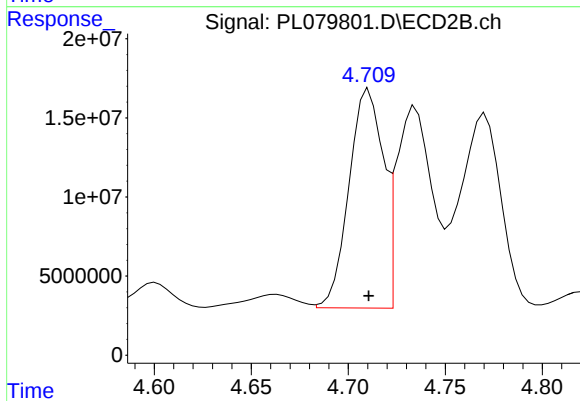

#25 Chlordane-3


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 169294491
Conc: 500.00 ng/ml

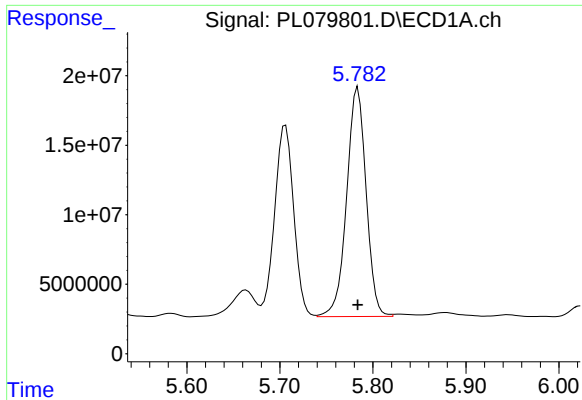

#26 Chlordane-4


R.T.: 5.784 min
Delta R.T.: 0.000 min
Response: 239890735
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

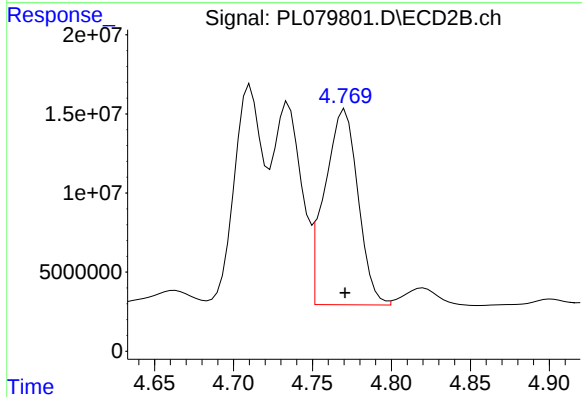


#26 Chlordane-4

R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 181208231
Conc: 500.00 ng/ml

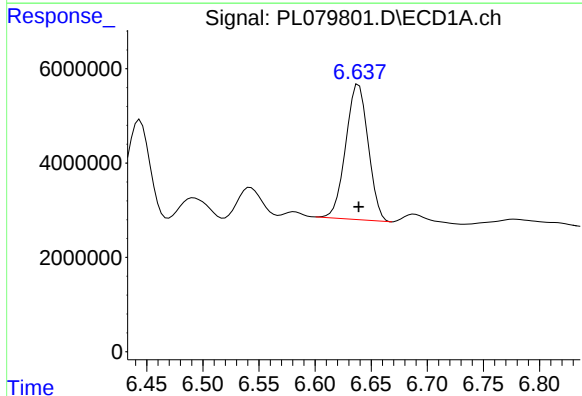


#27 Chlordane-5

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 39776154
Conc: 500.00 ng/ml

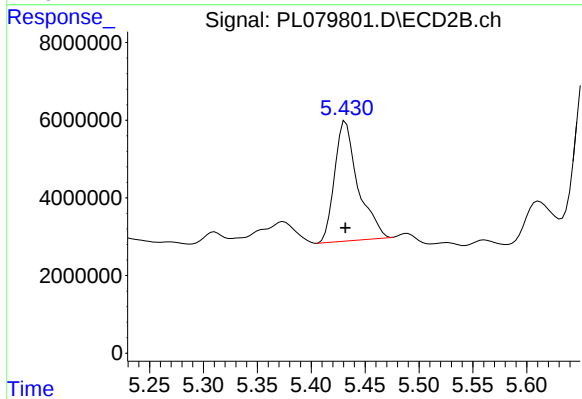

#27 Chlordane-5


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 46558594
Conc: 500.00 ng/ml

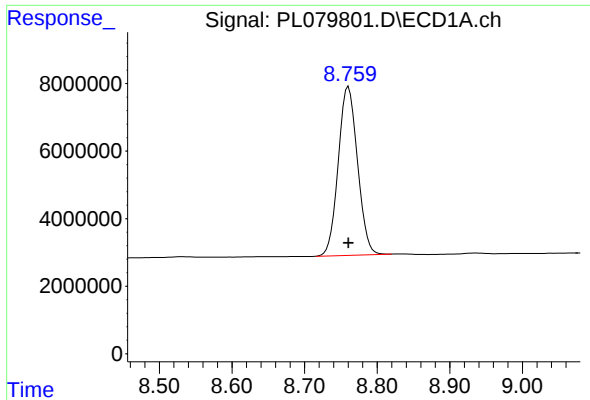

#28 Decachlorobiphenyl

R.T.: 8.760 min
Delta R.T.: 0.000 min
Response: 92228867
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

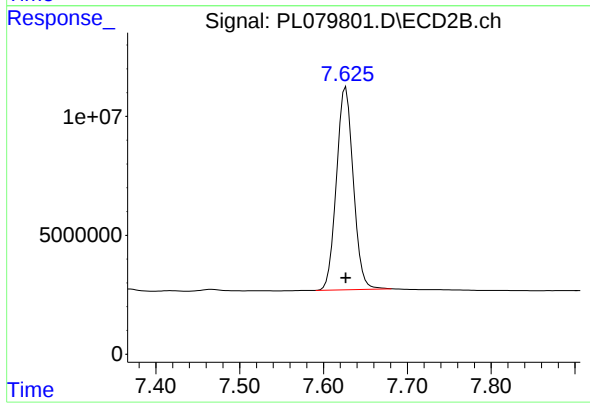

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 118882429
Conc: 50.00 ng/ml