

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 17:20
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:33:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 02:33:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	2.561	51829910	78127806	24.318	24.910
28)	SA Decachlor...	8.761	7.627	46618016	60163144	25.683	25.799
Target Compounds							
23)	Chlordane-1	4.463	3.525	22031183	26276996	240.624	253.386
24)	Chlordane-2	4.995	4.091	25093271	28875490	253.130	256.627
25)	Chlordane-3	5.705	4.711	92644515	83055091	235.334	247.667
26)	Chlordane-4	5.783	4.771	115.2E6	88881603	240.416	247.354
27)	Chlordane-5	6.639	5.432	18674333	22691905	235.676	248.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 17:20
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:33:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 02:33:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

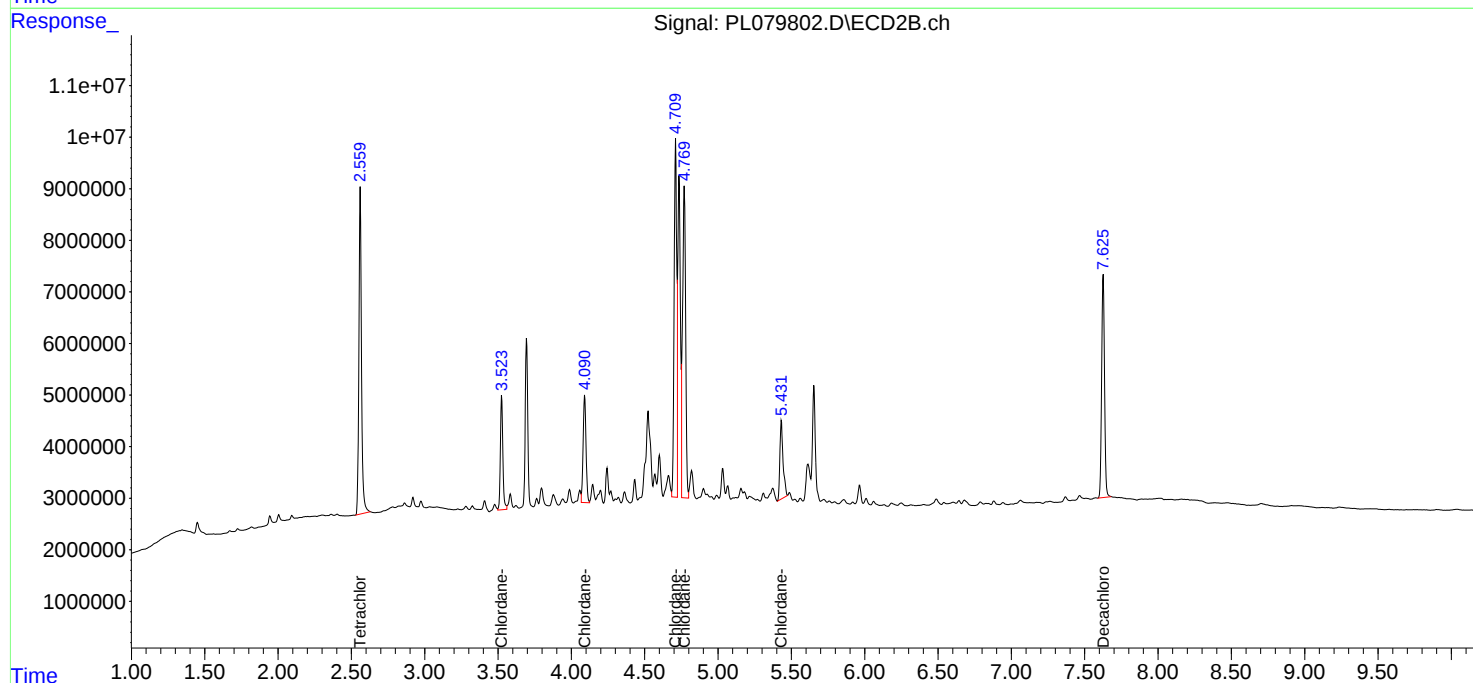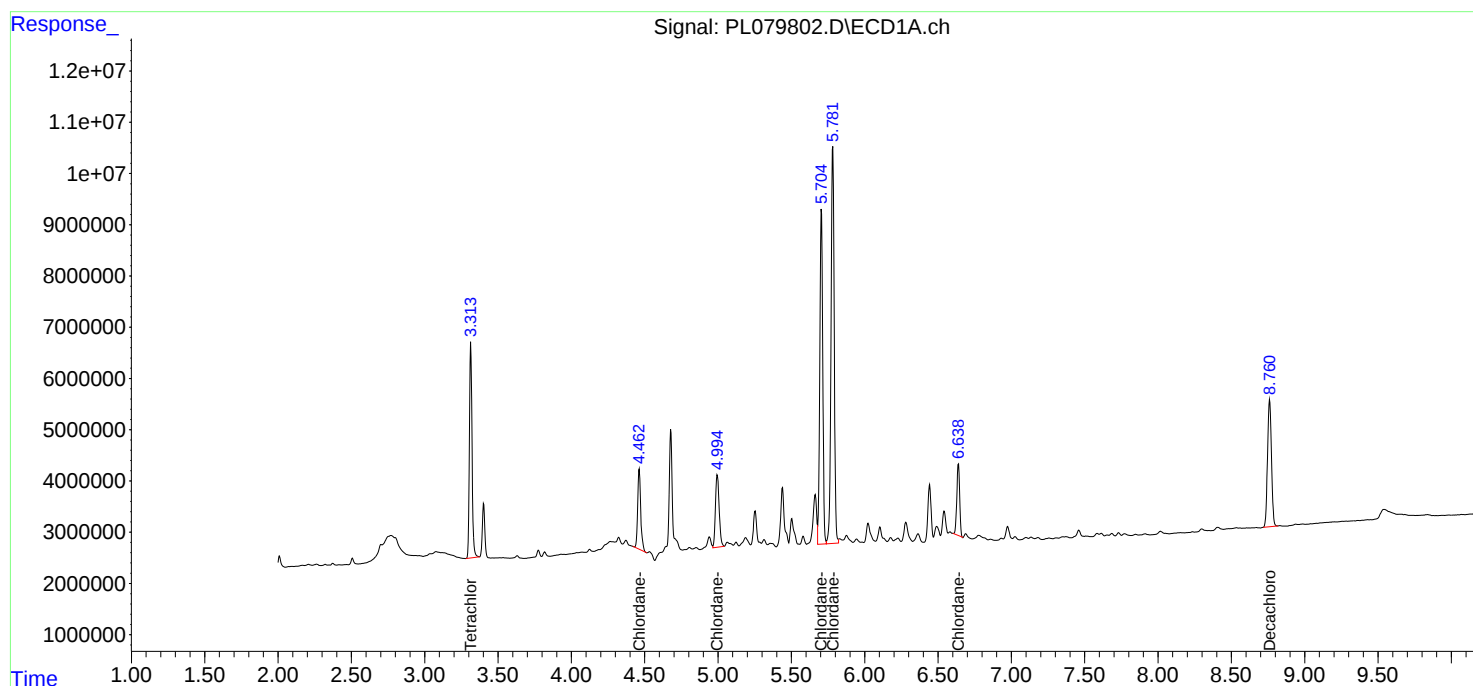


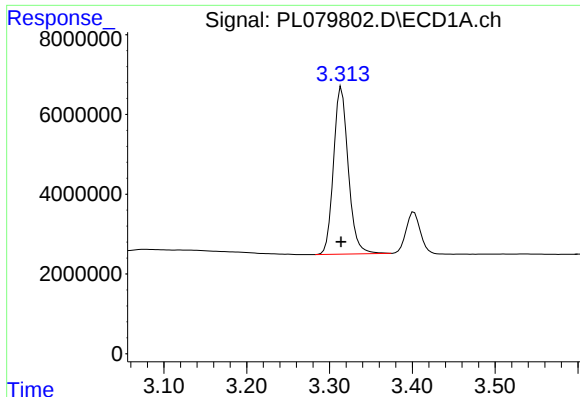

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 51829910
Conc: 24.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

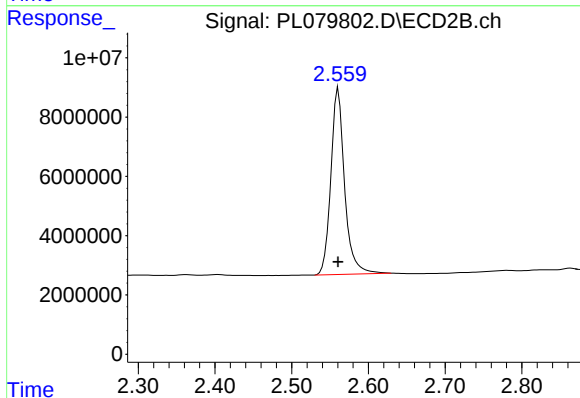


#1 Tetrachloro-m-xylene

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 78127806
Conc: 24.91 ng/ml

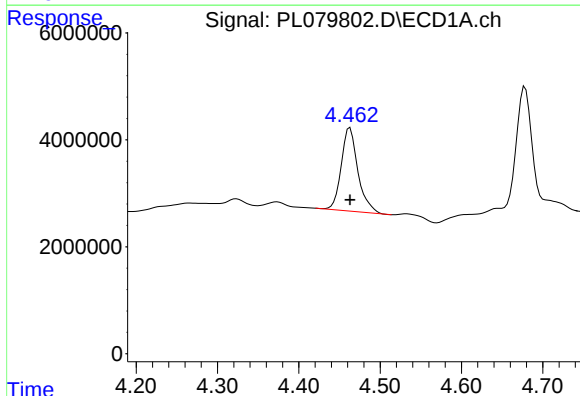


#23 Chlordane-1

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 22031183
Conc: 240.62 ng/ml

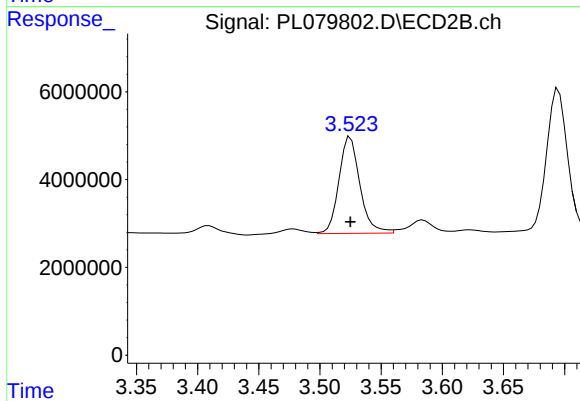

#23 Chlordane-1


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 26276996
Conc: 253.39 ng/ml

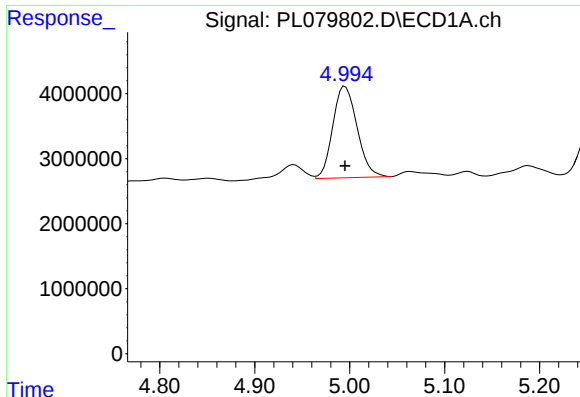

#24 Chlordane-2


R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 25093271
Conc: 253.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

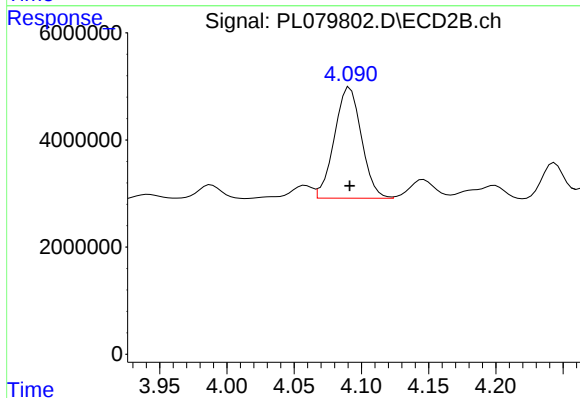


#24 Chlordane-2

R.T.: 4.091 min
Delta R.T.: 0.000 min
Response: 28875490
Conc: 256.63 ng/ml

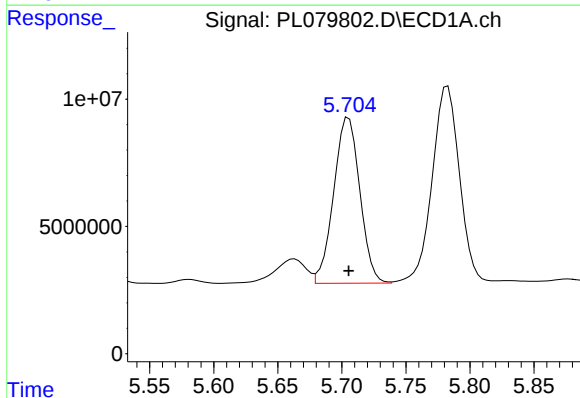


#25 Chlordane-3

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 92644515
Conc: 235.33 ng/ml

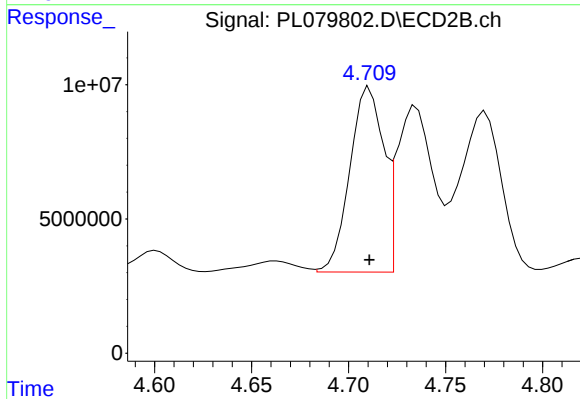

#25 Chlordane-3


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 83055091
Conc: 247.67 ng/ml

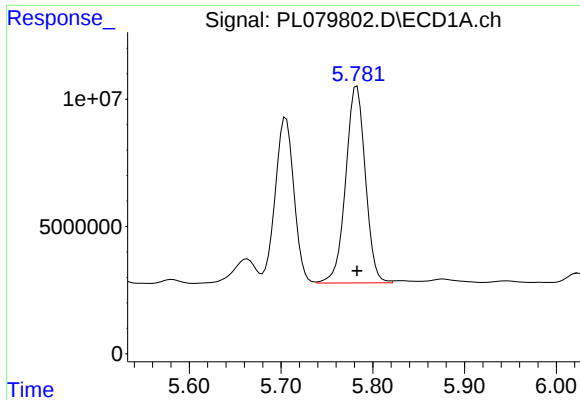

#26 Chlordane-4


R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 115181159
Conc: 240.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

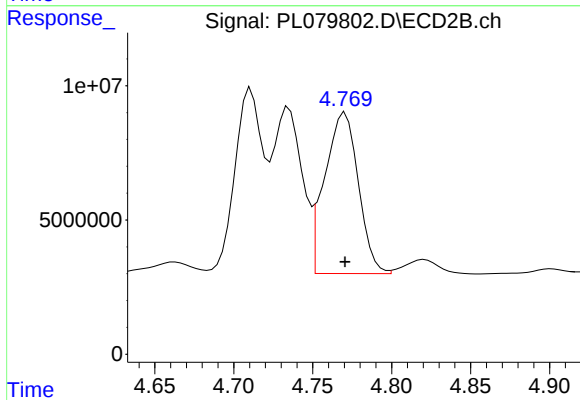


#26 Chlordane-4

R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 88881603
Conc: 247.35 ng/ml

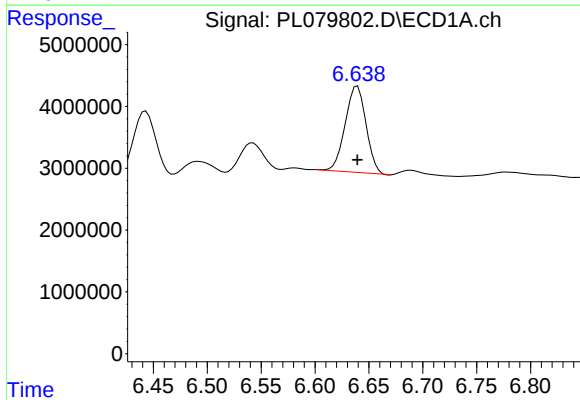


#27 Chlordane-5

R.T.: 6.639 min
Delta R.T.: 0.000 min
Response: 18674333
Conc: 235.68 ng/ml

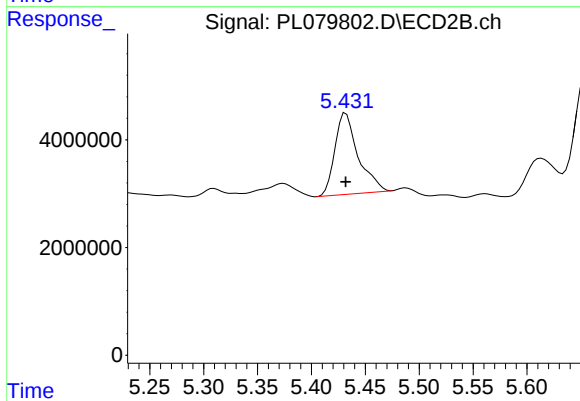

#27 Chlordane-5


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 22691905
Conc: 248.35 ng/ml

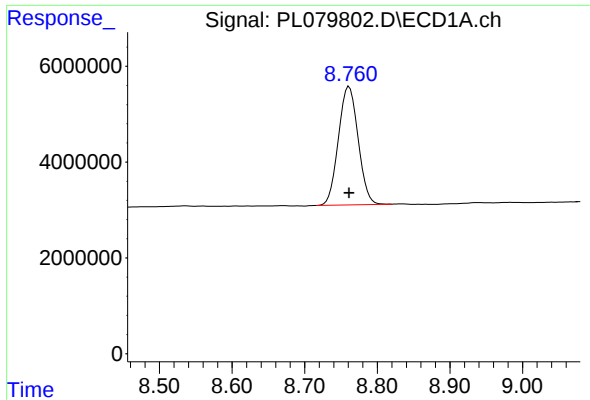

#28 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: 0.000 min
Response: 46618016
Conc: 25.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

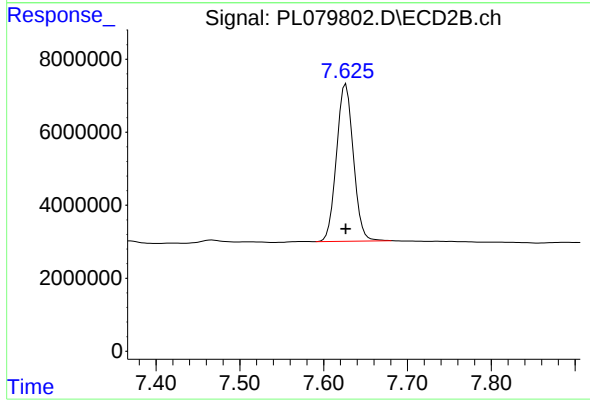

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 60163144
Conc: 25.80 ng/ml