

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
 Data File : PL079810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 19:11
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL122022CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:46:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 01:39:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.561	110.9E6	162.6E6	52.032	51.522
28)	SA Decachlor...	8.762	7.627	94168730	120.4E6	51.052	50.634
Target Compounds							
23)	Chlordane-1	4.463	3.525	47848231	53763782	522.533	514.831
24)	Chlordane-2	4.996	4.091	51570160	58867754	513.671	515.531
25)	Chlordane-3	5.706	4.711	203.4E6	173.2E6	516.759	511.621
26)	Chlordane-4	5.783	4.771	247.6E6	185.6E6	515.989	512.139
27)	Chlordane-5	6.638	5.432	40795858	47556407	512.818	510.716



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122022\
Data File : PL079810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 19:11
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL122022CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:46:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 01:39:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

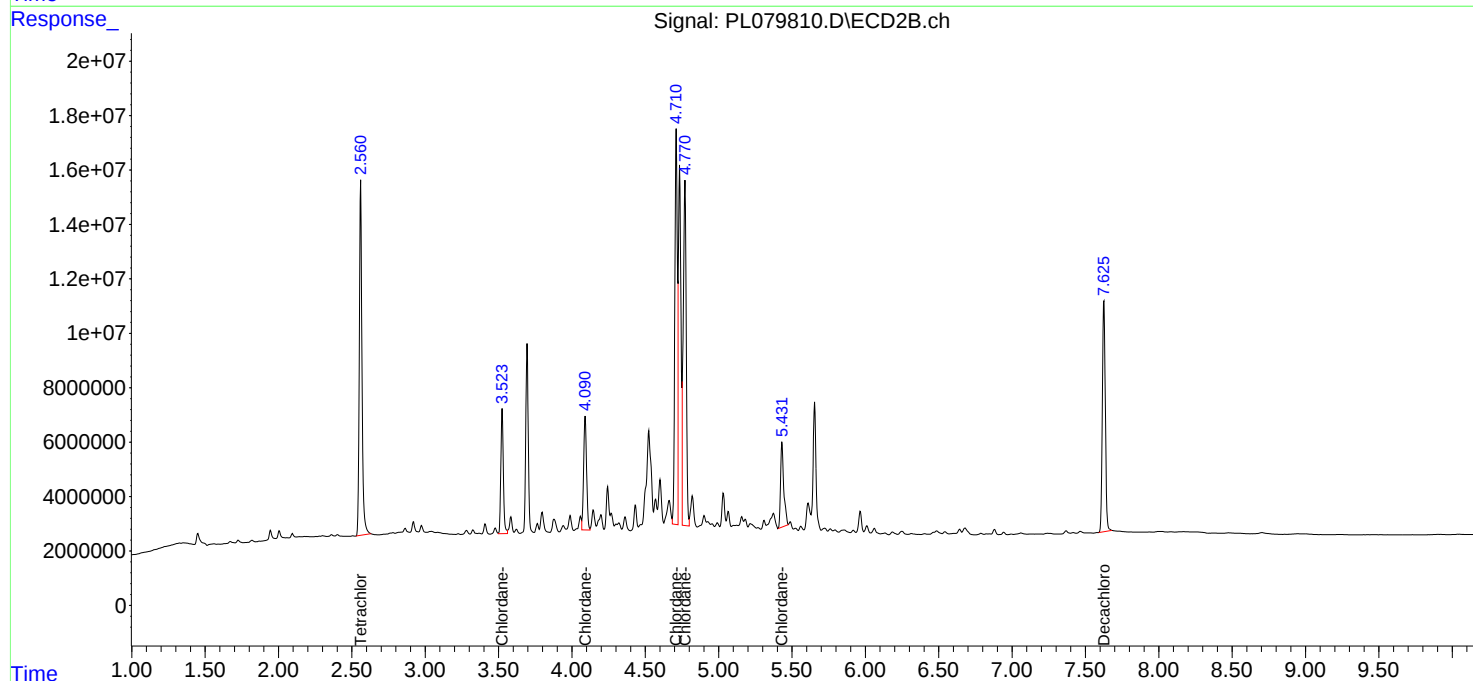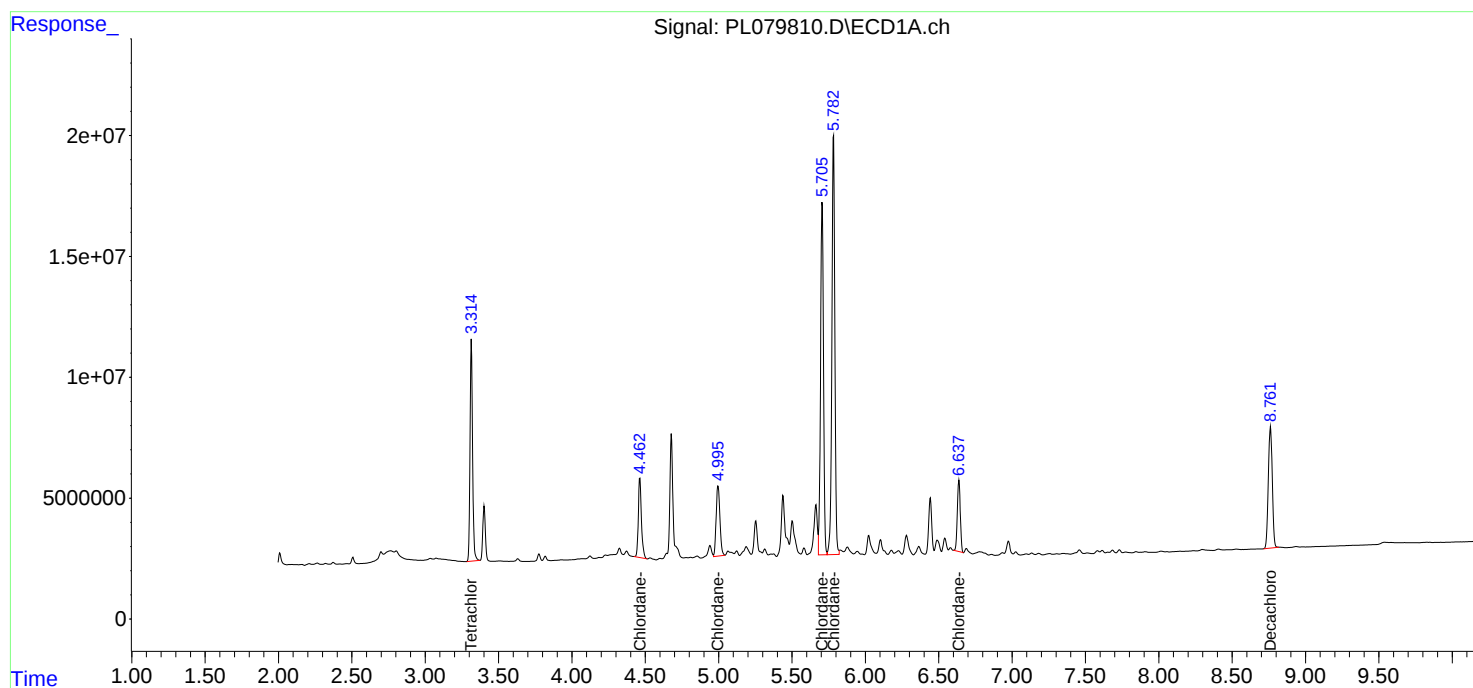


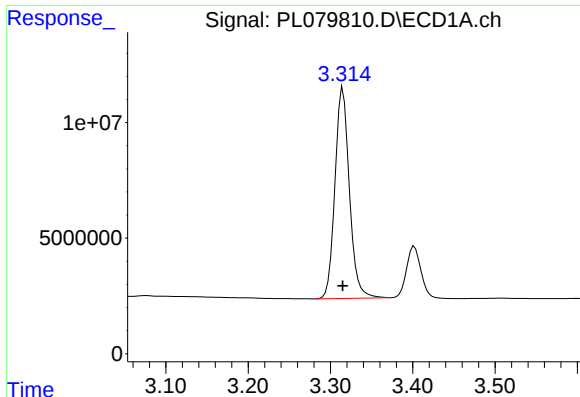

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 110943427
Conc: 52.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122022CHLOR

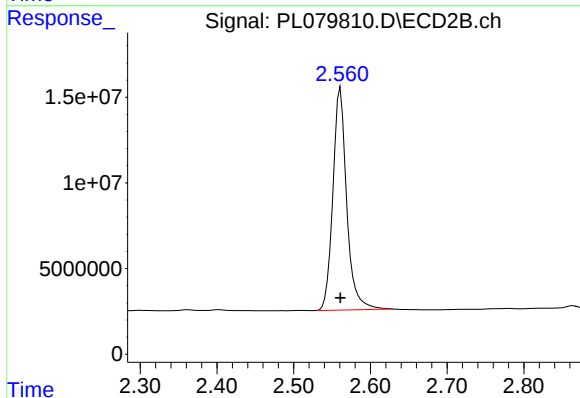


#1 Tetrachloro-m-xylene

R.T.: 2.561 min
Delta R.T.: 0.000 min
Response: 162569391
Conc: 51.52 ng/ml

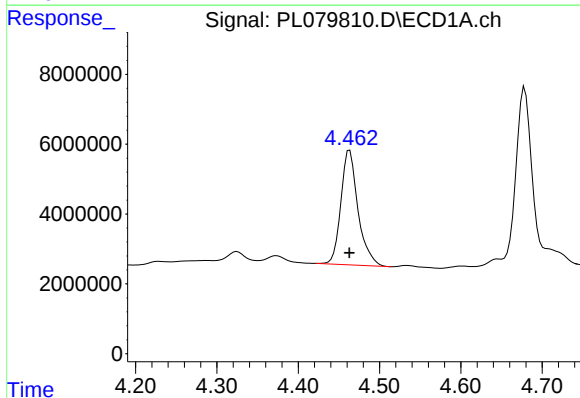


#23 Chlordane-1

R.T.: 4.463 min
Delta R.T.: 0.000 min
Response: 47848231
Conc: 522.53 ng/ml

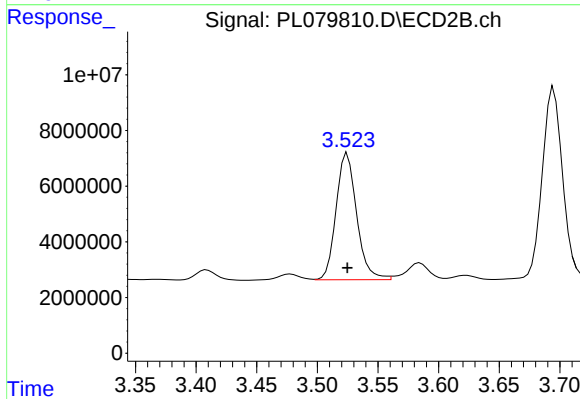

#23 Chlordane-1


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 53763782
Conc: 514.83 ng/ml

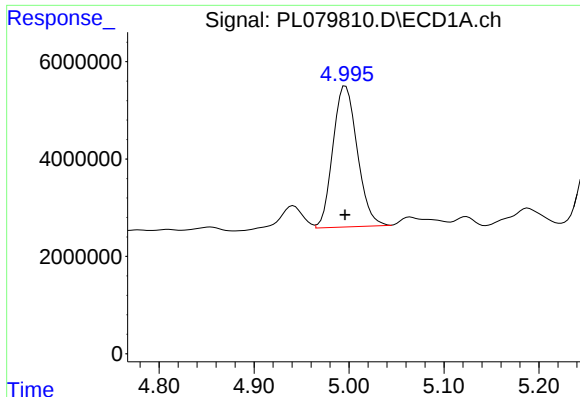

#24 Chlordane-2


R.T.: 4.996 min
Delta R.T.: 0.000 min
Response: 51570160
Conc: 513.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122022CHLOR

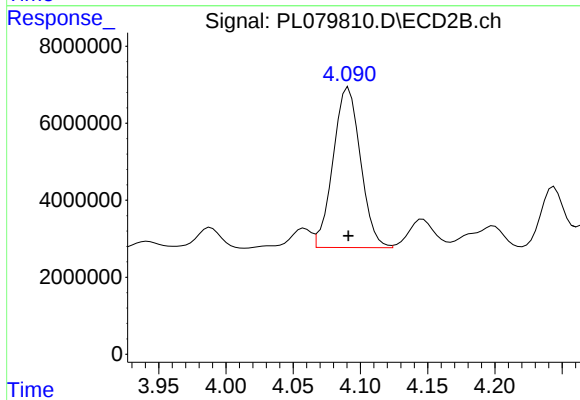


#24 Chlordane-2

R.T.: 4.091 min
Delta R.T.: 0.000 min
Response: 58867754
Conc: 515.53 ng/ml

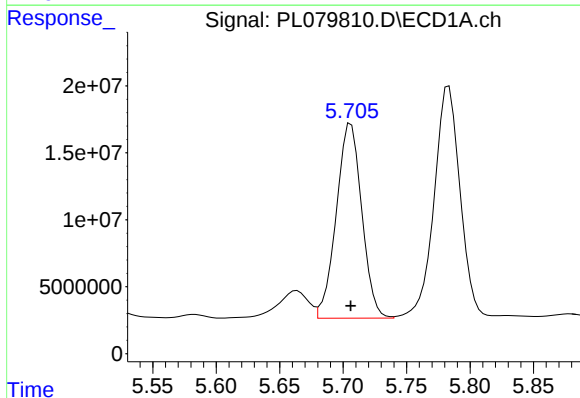


#25 Chlordane-3

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 203438845
Conc: 516.76 ng/ml

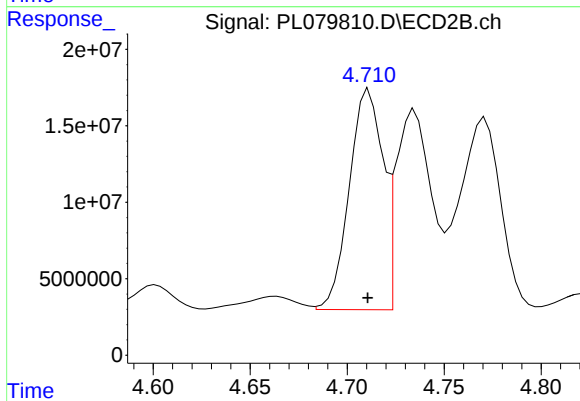

#25 Chlordane-3


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 173229392
Conc: 511.62 ng/ml

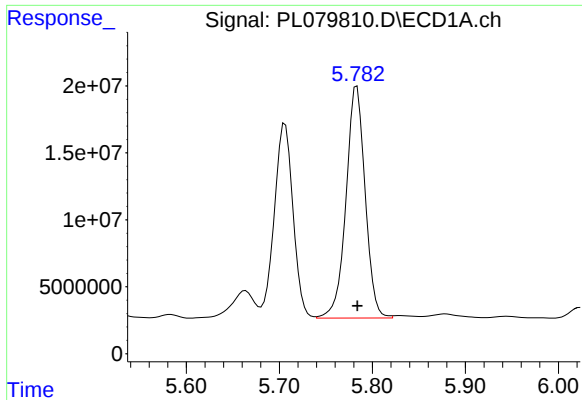

#26 Chlordane-4


R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 247561986
Conc: 515.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122022CHLOR

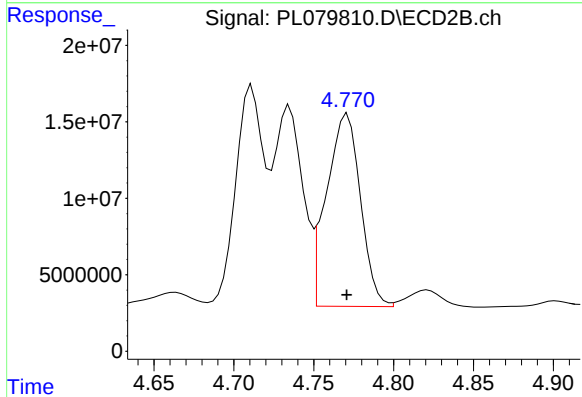


#26 Chlordane-4

R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 185607635
Conc: 512.14 ng/ml

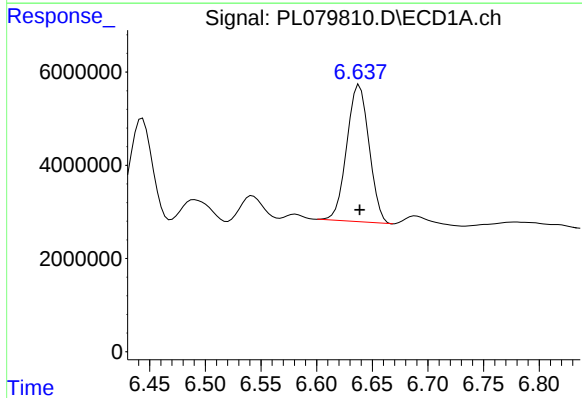


#27 Chlordane-5

R.T.: 6.638 min
Delta R.T.: 0.000 min
Response: 40795858
Conc: 512.82 ng/ml

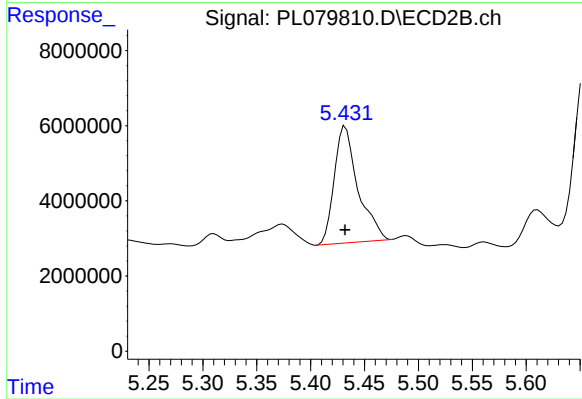

#27 Chlordane-5


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 47556407
Conc: 510.72 ng/ml

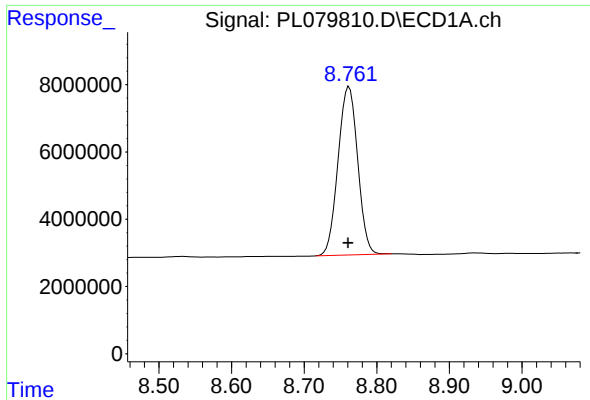

#28 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.002 min
Response: 94168730
Conc: 51.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122022CHLOR

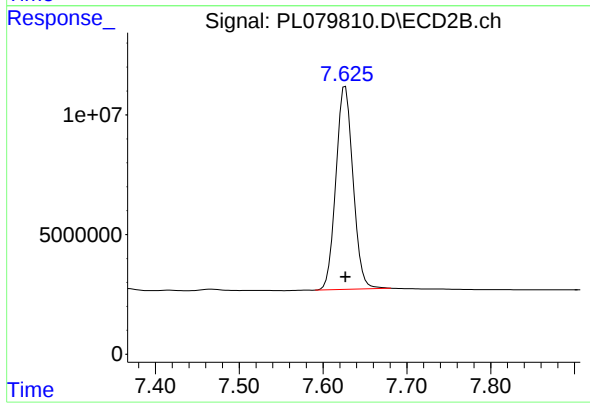

#28 Decachlorobiphenyl

R.T.: 7.627 min
Delta R.T.: 0.000 min
Response: 120390574
Conc: 50.63 ng/ml