

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122024\
 Data File : PL093466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 12:08
 Operator : AR\AJ
 Sample : P5342-03RE 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HT2651RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/23/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:22:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.794f	2700156	13784652	1.039m	4.780m#
28) SA Decachlor...	9.055	7.913	3767388	8338710	2.167m	2.919m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122024\
Data File : PL093466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 12:08
Operator : AR\AJ
Sample : P5342-03RE 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
HT2651RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/23/2024
Supervised By : Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:22:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

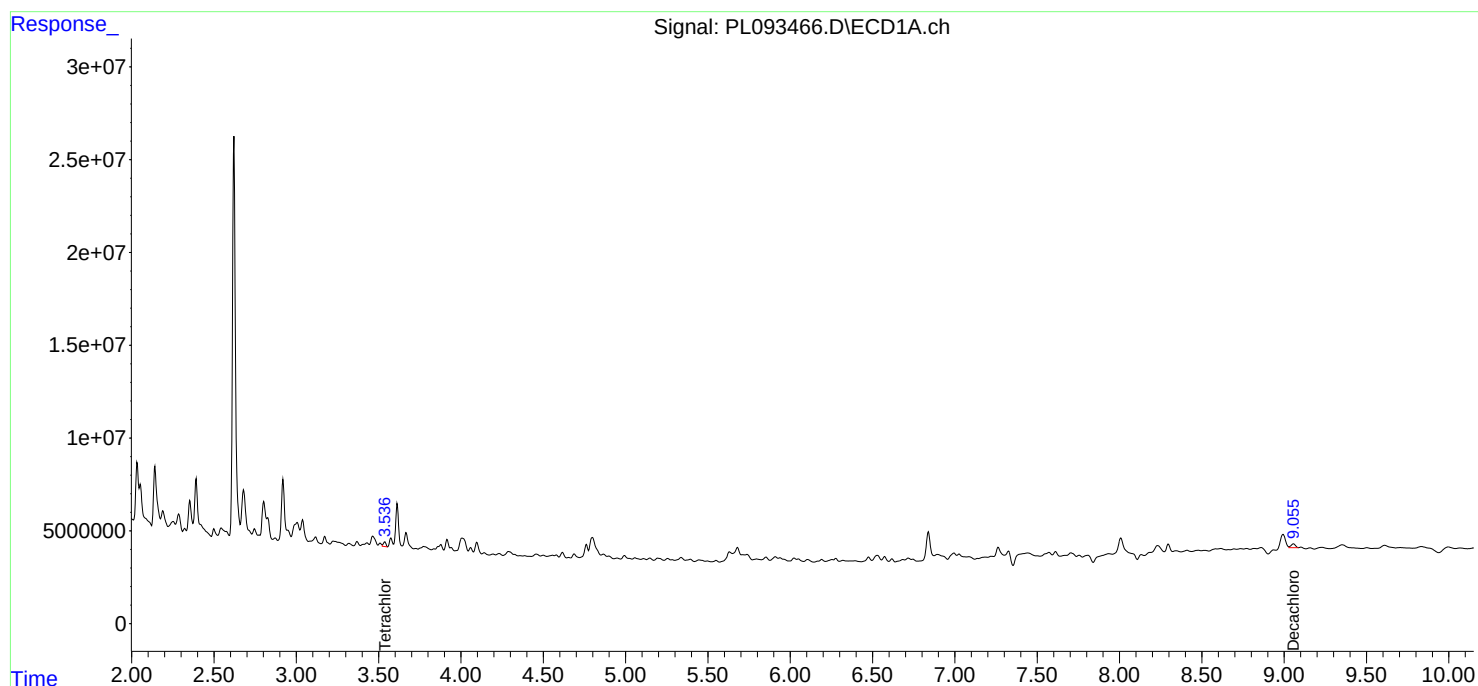

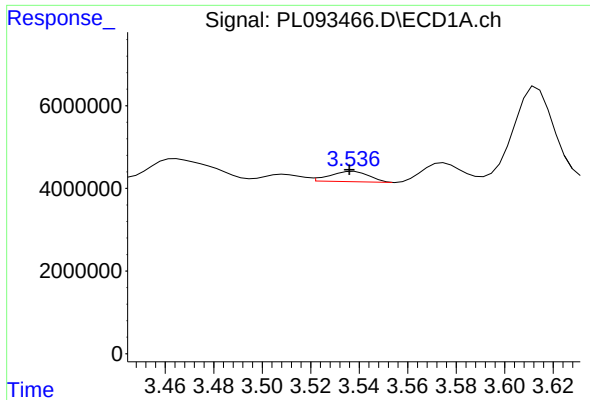


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 2700156
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HT2651RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/23/2024
Supervised By :Ankita Jodhani 12/27/2024

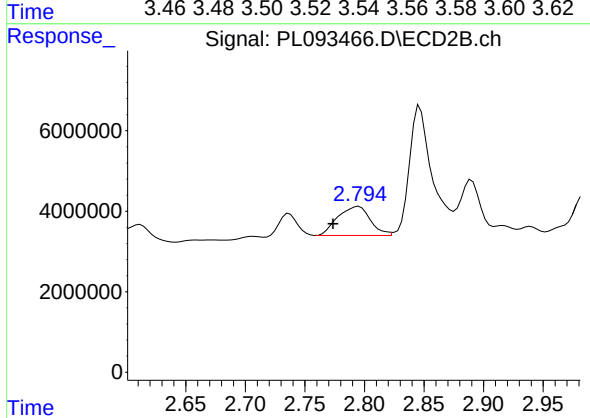


#1 Tetrachloro-m-xylene

R.T.: 2.794 min
Delta R.T.: 0.020 min
Response: 13784652
Conc: 4.78 ng/ml m

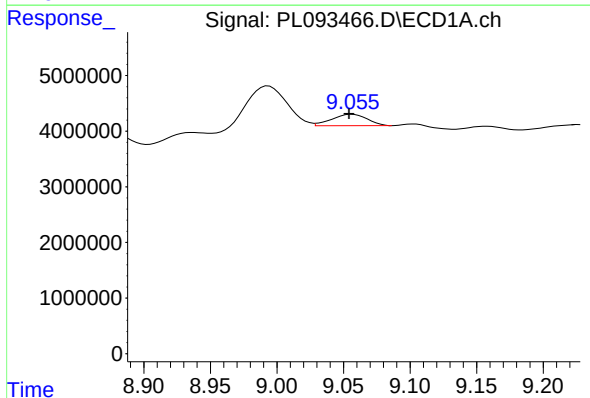

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 3767388
Conc: 2.17 ng/ml m

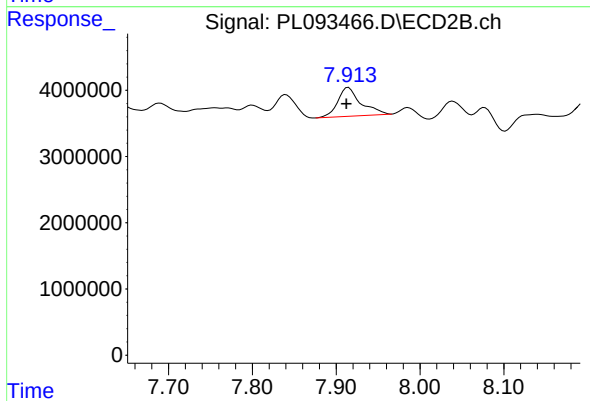

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 8338710
Conc: 2.92 ng/ml m