

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2018 11:23
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 22:14:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.100	137.5E6	71558206	22.415	24.143
28)	SA Decachlor...	8.205	9.233	122.7E6	51873345	18.797	19.886
Target Compounds							
2)	A alpha-BHC	3.897	0.000	5231916	0	0.553	N.D. #
8)	B Heptachlo...	0.000	6.016	0	1517340	N.D.	0.400 #
9)	A Endosulfan I	0.000	6.370	0	783680	N.D.	0.231 #
11)	B alpha-Chl...	0.000	6.370 ^f	0	783680	N.D.	0.218 #
20)	A Methoxychlor	6.902	0.000	6196403	0	1.847	N.D. #
26)	Chlordane-4	0.000	6.370	0	783680	N.D.	1.373 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2018 11:23
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 22:14:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

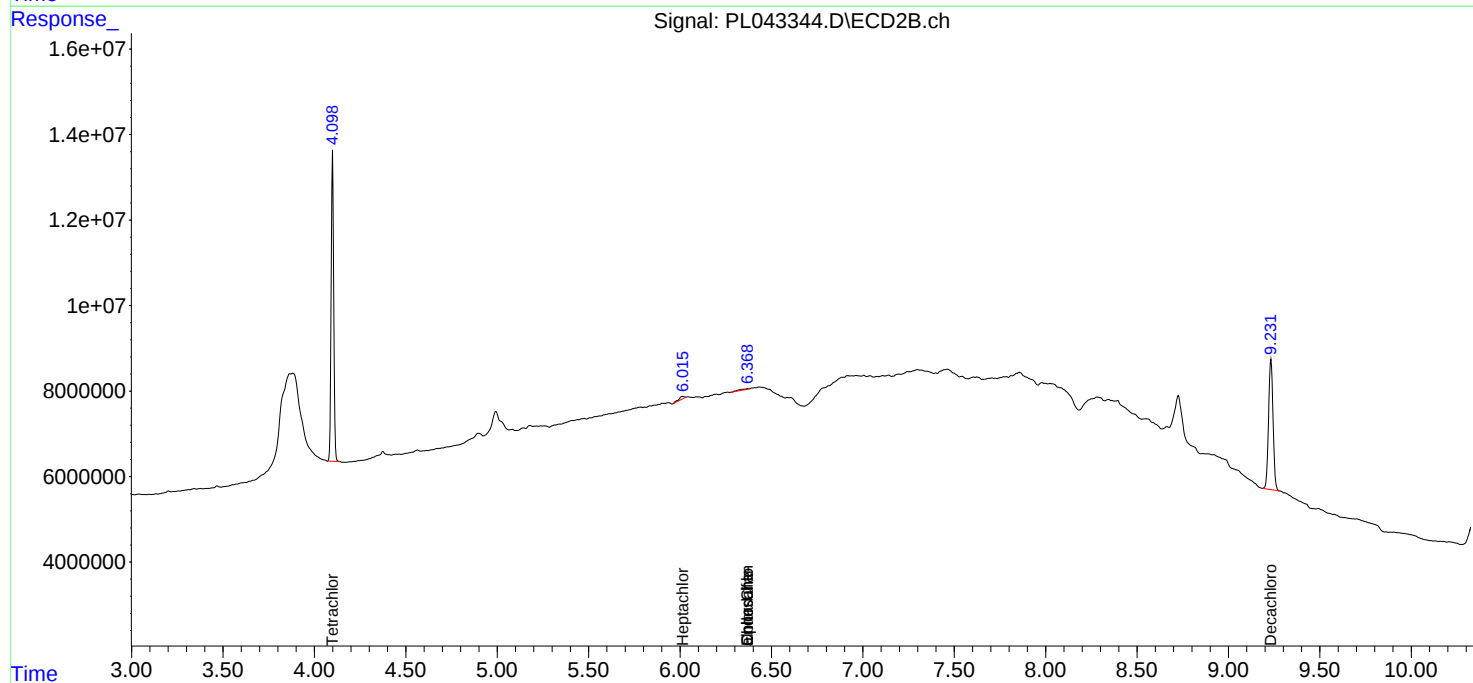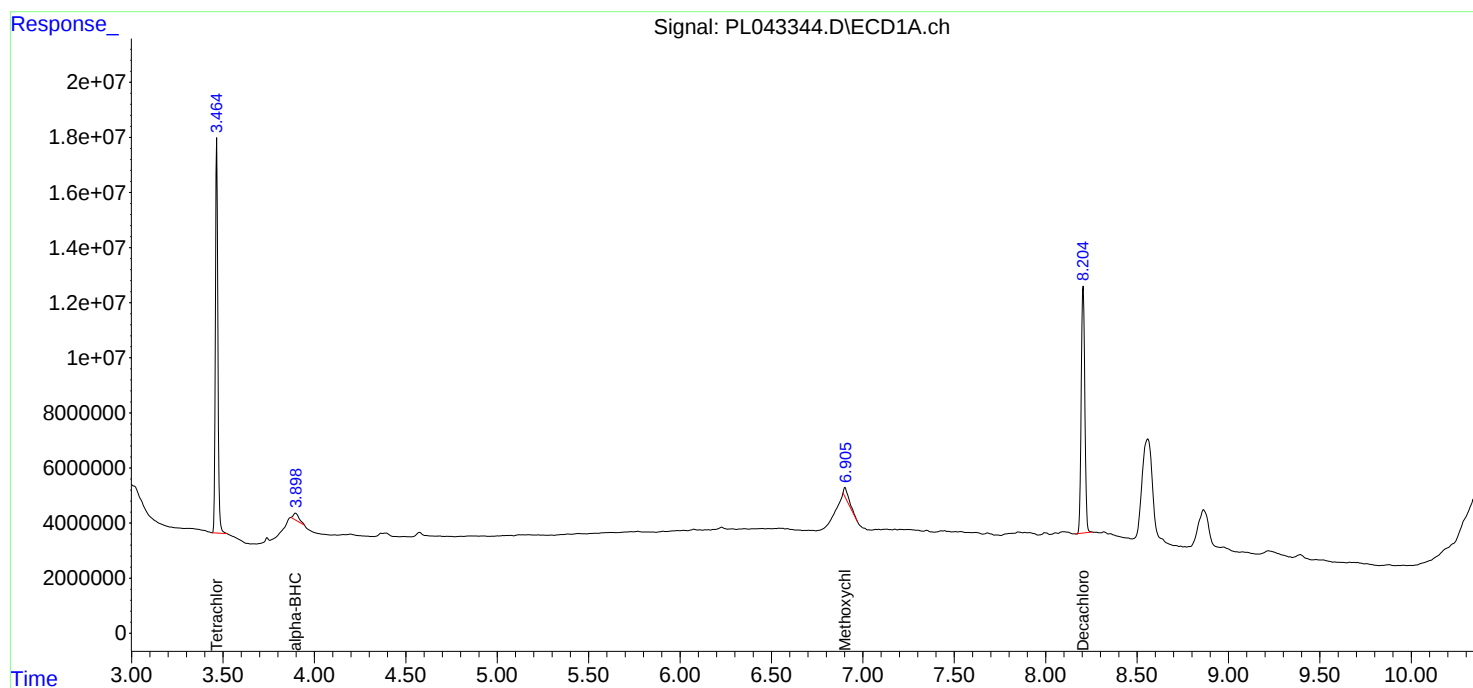


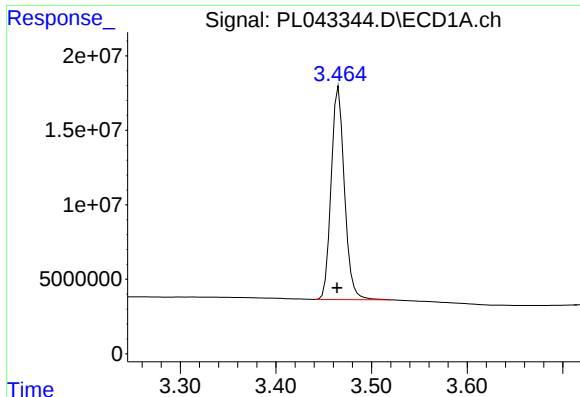

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.002 min
Response: 137470540
Conc: 22.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

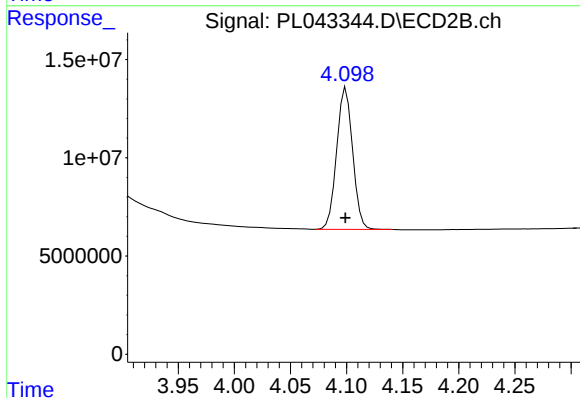


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 71558206
Conc: 24.14 ng/ml

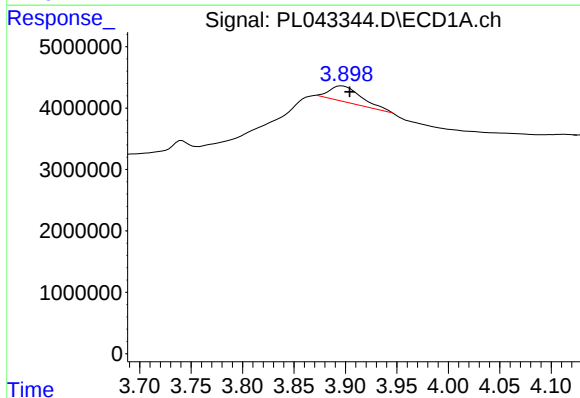


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: -0.008 min
Response: 5231916
Conc: 0.55 ng/ml

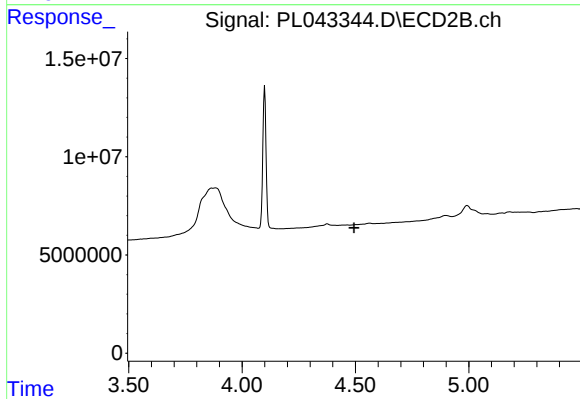

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

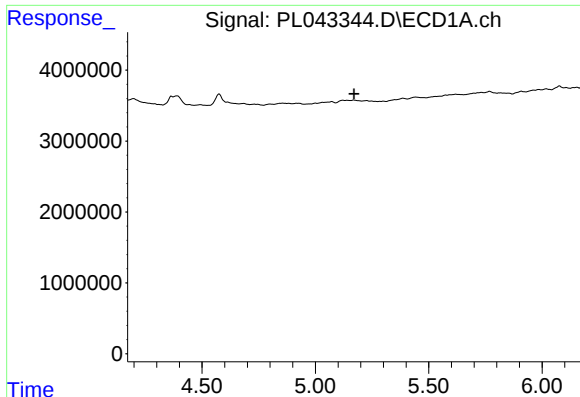

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

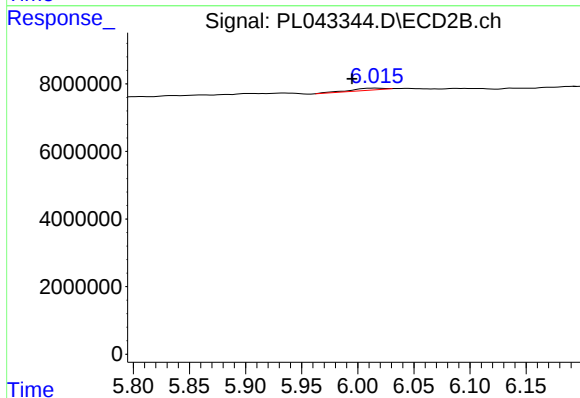


#8 Heptachlor epoxide

R.T.: 6.016 min
Delta R.T.: 0.021 min
Response: 1517340
Conc: 0.40 ng/ml

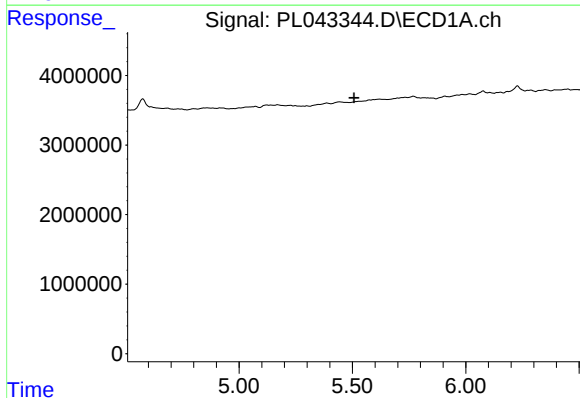


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

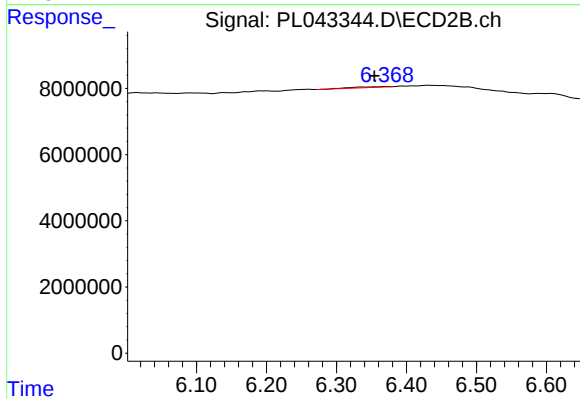

#9 Endosulfan I


R.T.: 6.370 min
Delta R.T.: 0.015 min
Response: 783680
Conc: 0.23 ng/ml

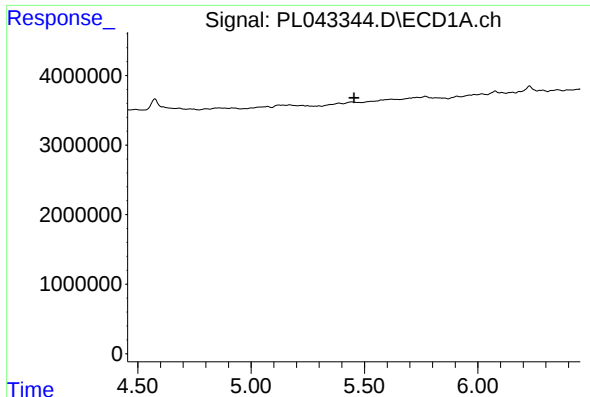

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

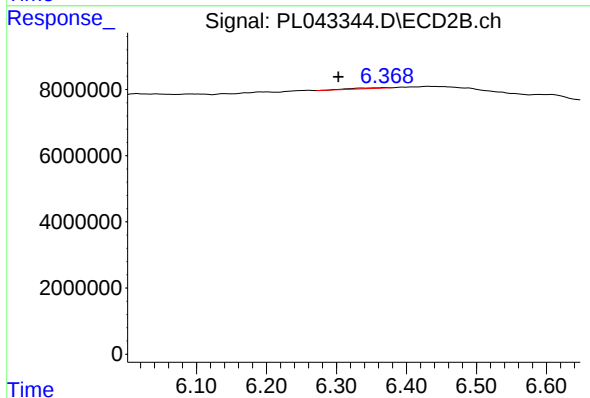


#11 alpha-Chlordane

R.T.: 6.370 min
Delta R.T.: 0.067 min
Response: 783680
Conc: 0.22 ng/ml

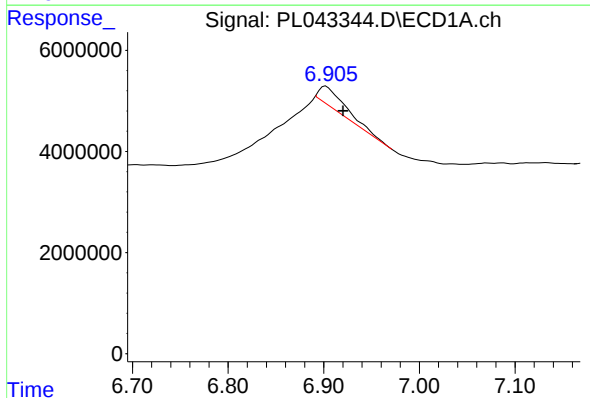


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: -0.018 min
Response: 6196403
Conc: 1.85 ng/ml

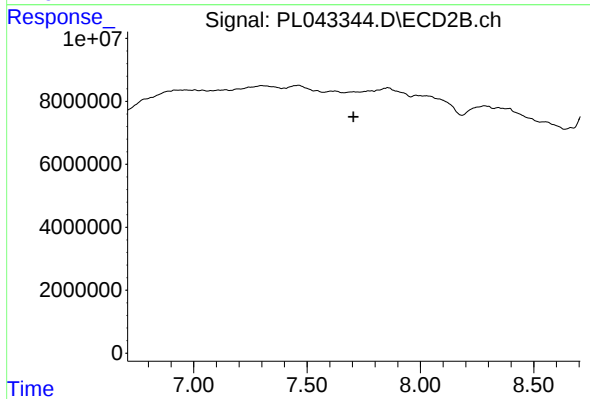

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.705 min
Response: 0
Conc: N.D.

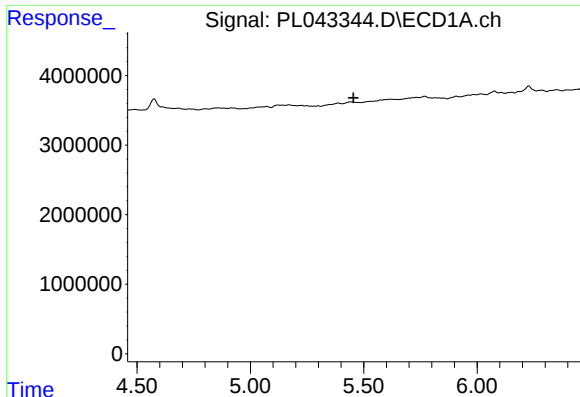

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

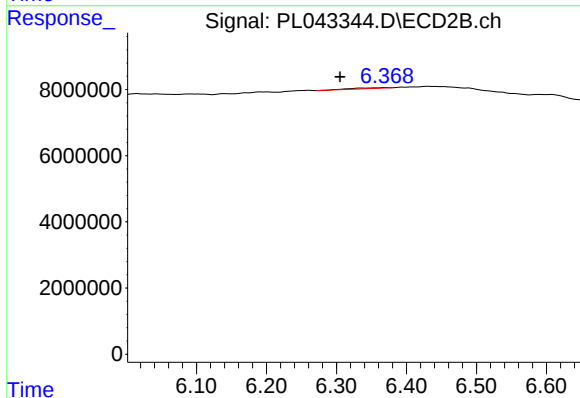


#26 Chlordane-4

R.T.: 6.370 min
Delta R.T.: 0.065 min
Response: 783680
Conc: 1.37 ng/ml

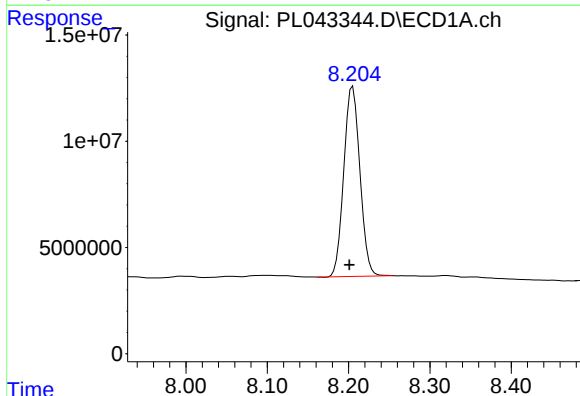

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 122745932
Conc: 18.80 ng/ml

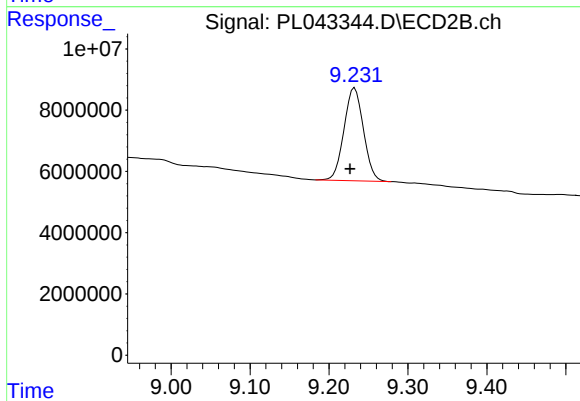

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.006 min
Response: 51873345
Conc: 19.89 ng/ml