

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2018 14:56
 Operator : AJ\SJ
 Sample : J6482-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 R20-OS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 22:37:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	45140464	23606045	7.360	7.965
28)	SA Decachlor...	8.203	9.234	74478550	37930893	11.406	14.541 #
Target Compounds							
6)	B beta-BHC	4.398f	4.902f	1728620	3329266	0.469	1.967 #
7)	B delta-BHC	0.000	5.172	0	4037174	N.D.	0.939 #
8)	B Heptachlo...	0.000	6.008	0	2176413	N.D.	0.574 #
9)	A Endosulfan I	0.000	6.414f	0	654851	N.D.	0.193 #
12)	B 4,4'-DDE	5.627	6.414f	1936136	654851	0.280	0.181 #
23)	Chlordane-1	4.398	5.172	1728620	4037174	6.433	28.565 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2018 14:56
Operator : AJ\SJ
Sample : J6482-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
R20-OS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 22:37:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

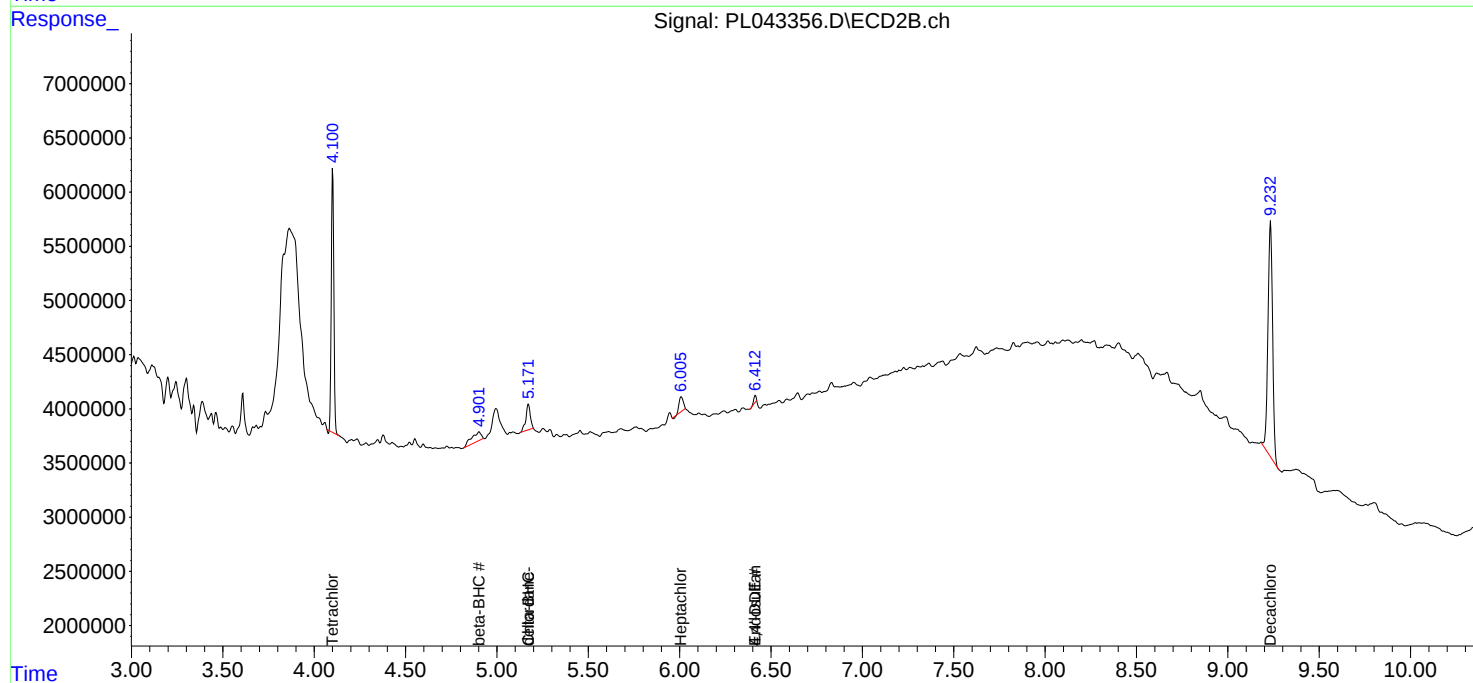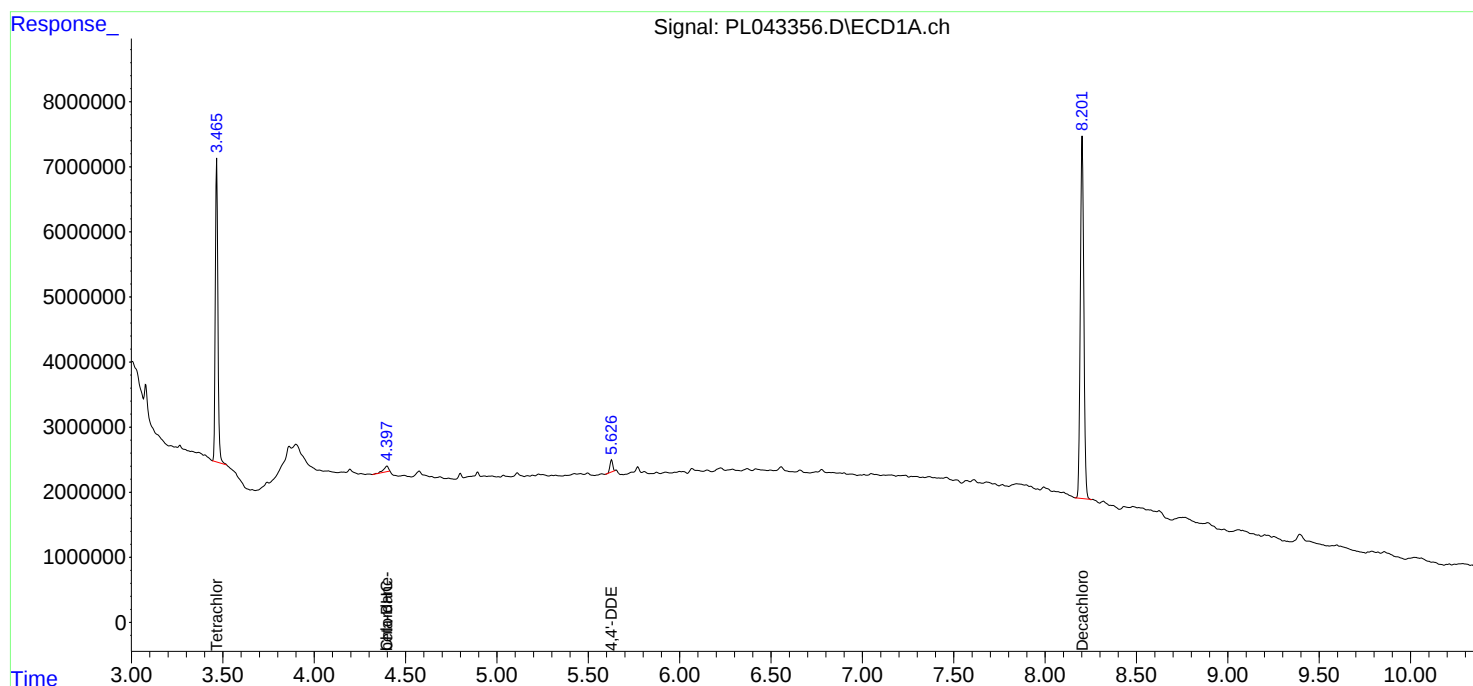


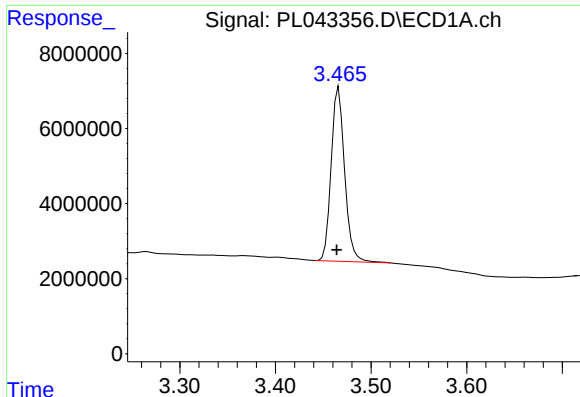

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.002 min
Response: 45140464
Conc: 7.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
R20-OS

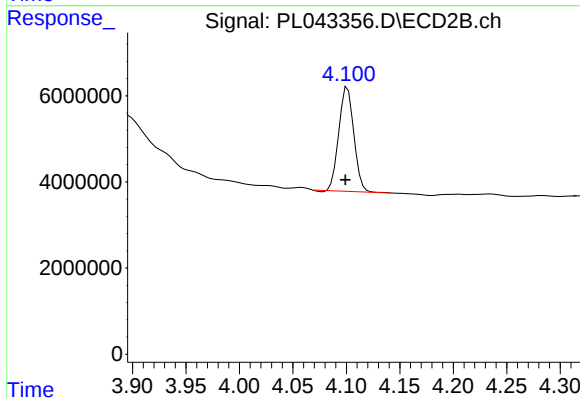


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.002 min
Response: 23606045
Conc: 7.96 ng/ml

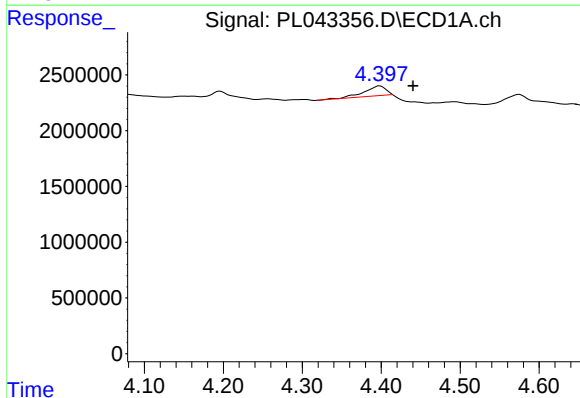


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.042 min
Response: 1728620
Conc: 0.47 ng/ml

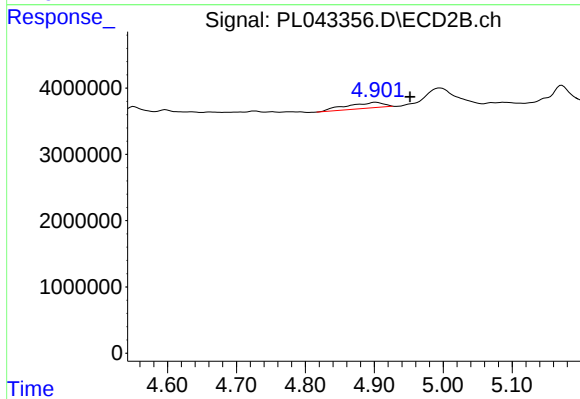

#6 beta-BHC


R.T.: 4.902 min
Delta R.T.: -0.050 min
Response: 3329266
Conc: 1.97 ng/ml

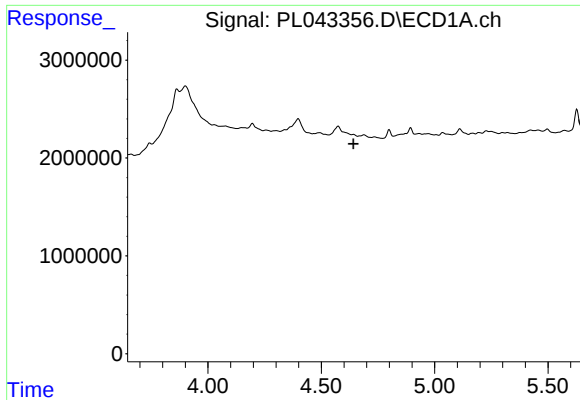

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R20-OS

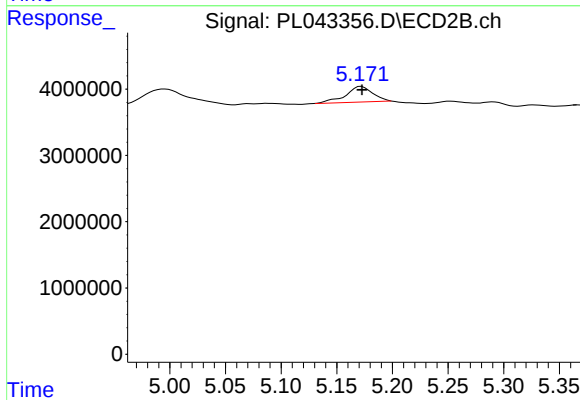


#7 delta-BHC

R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 4037174
Conc: 0.94 ng/ml

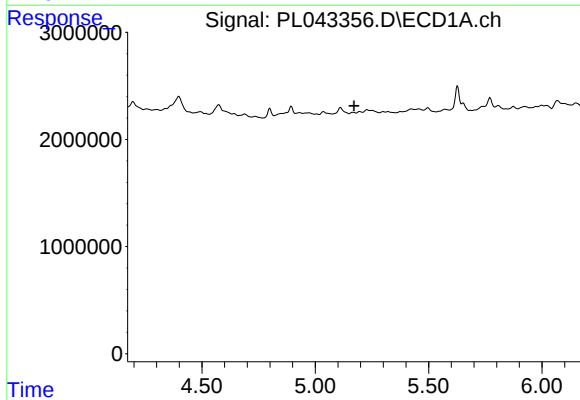


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

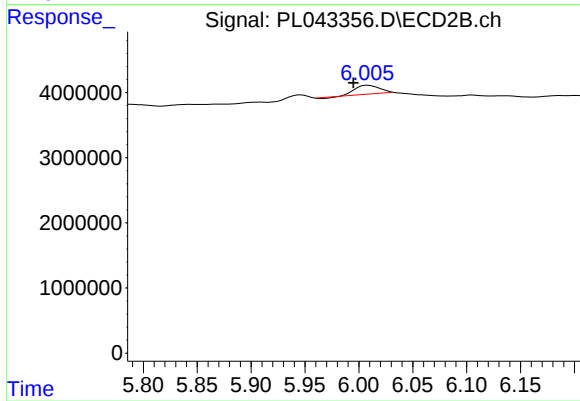

#8 Heptachlor epoxide


R.T.: 6.008 min
Delta R.T.: 0.014 min
Response: 2176413
Conc: 0.57 ng/ml

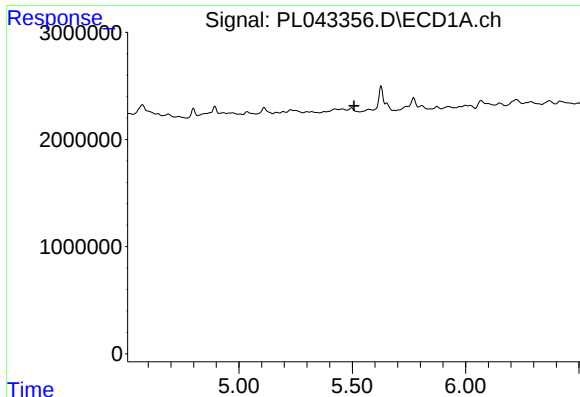

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R20-OS

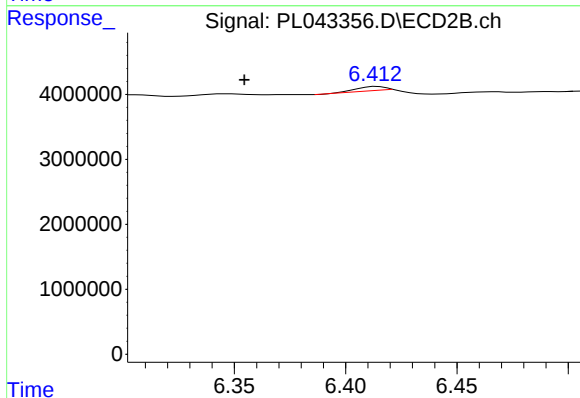


#9 Endosulfan I

R.T.: 6.414 min
Delta R.T.: 0.060 min
Response: 654851
Conc: 0.19 ng/ml

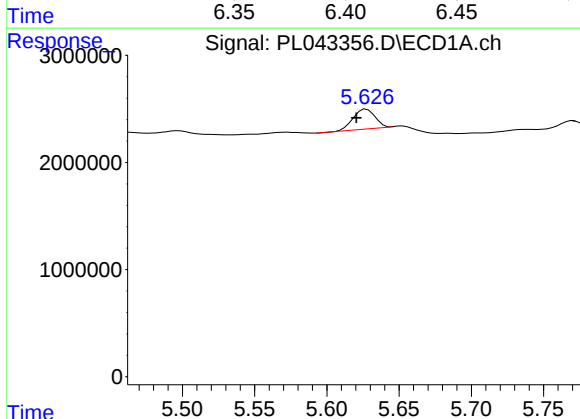


#12 4,4'-DDE

R.T.: 5.627 min
Delta R.T.: 0.007 min
Response: 1936136
Conc: 0.28 ng/ml

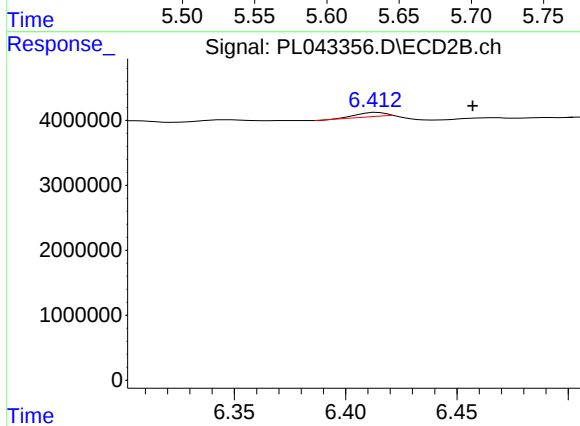

#12 4,4'-DDE


R.T.: 6.414 min
Delta R.T.: -0.043 min
Response: 654851
Conc: 0.18 ng/ml

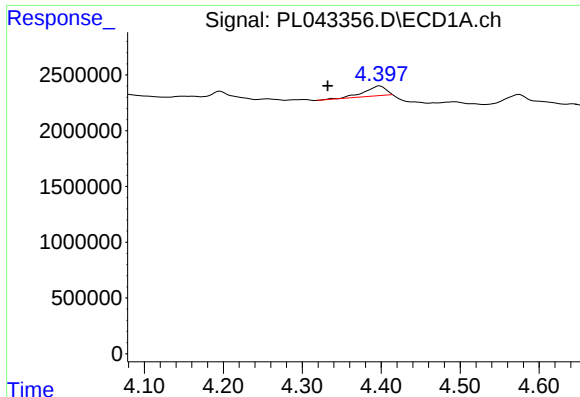

#23 Chlordane-1


R.T.: 4.398 min
Delta R.T.: 0.066 min
Response: 1728620
Conc: 6.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
R20-OS

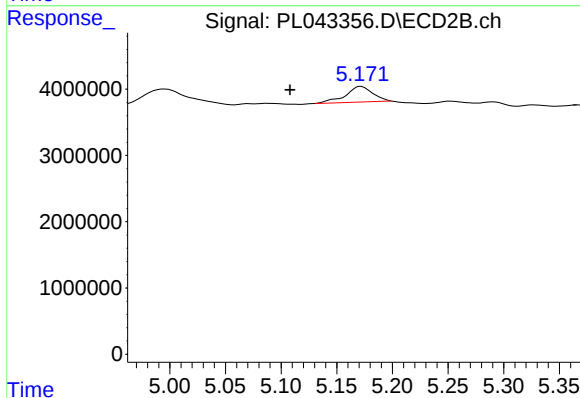


#23 Chlordane-1

R.T.: 5.172 min
Delta R.T.: 0.064 min
Response: 4037174
Conc: 28.56 ng/ml

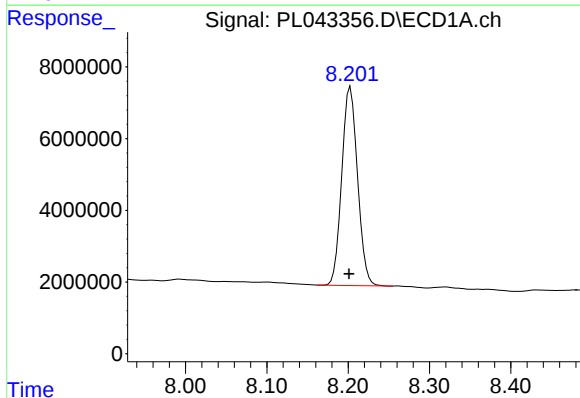

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.002 min
Response: 74478550
Conc: 11.41 ng/ml

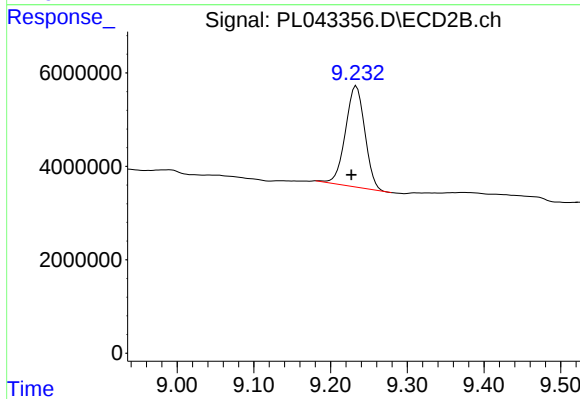

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.007 min
Response: 37930893
Conc: 14.54 ng/ml