

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 00:49
 Operator : AJ\SJ
 Sample : J6200-02
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-122018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:22:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.103	137.7E6	72010450	22.452	24.296
28)	SA Decachlor...	8.205	9.238	117.6E6	47841261	18.010	18.341
Target Compounds							
2)	A alpha-BHC	3.906	0.000	4946334	0	0.523	N.D. #
4)	MA Heptachlor	4.443f	5.265	6818032	-183505	0.768	N.D. #
6)	B beta-BHC	4.443	4.905f	6818032	1307566	1.848	0.772 #
7)	B delta-BHC	0.000	5.167	0	12762342	N.D.	2.970 #
8)	B Heptachlo...	0.000	6.001	0	10680450	N.D.	2.817 #
18)	B Endrin al...	6.456	0.000	1709029	0	0.310	N.D. #
19)	B Endosulfa...	6.674	0.000	5489117	0	0.819	N.D. #
20)	A Methoxychlor	0.000	7.646f	0	3254564	N.D.	2.158 #
23)	Chlordane-1	4.365	5.092	1267513	4187247	4.717	29.627 #
24)	Chlordane-2	4.901	0.000	14151967	0	49.305	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 00:49
Operator : AJ\SJ
Sample : J6200-02
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:22:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

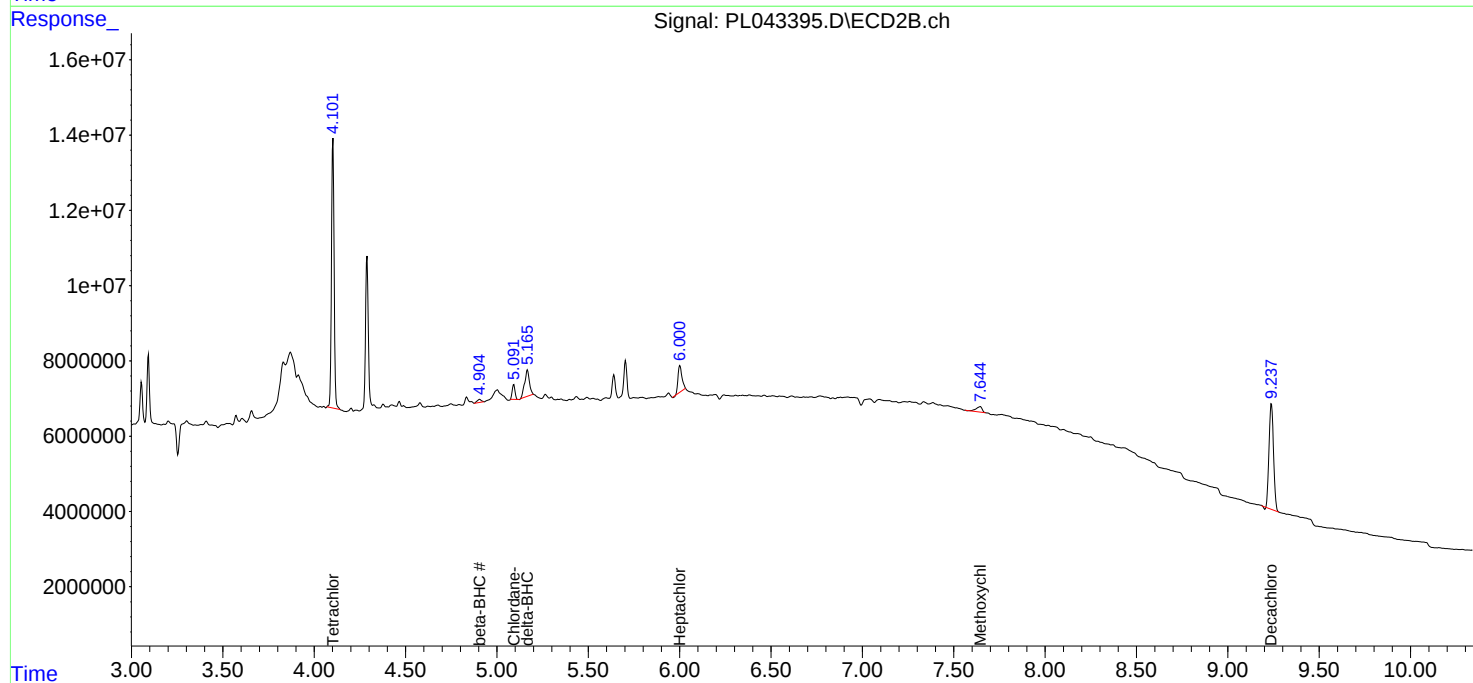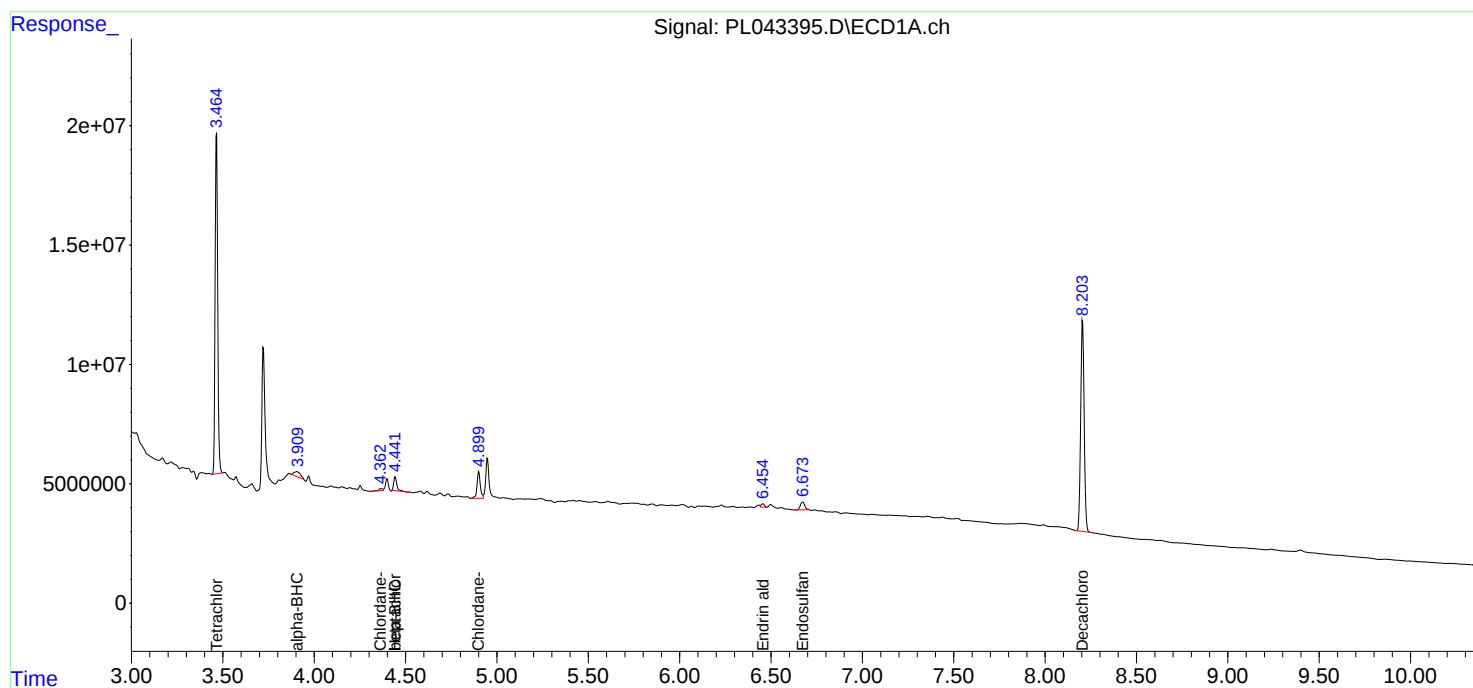


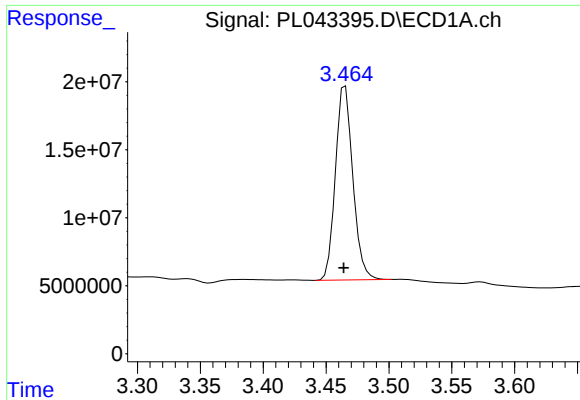

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 137696404
Conc: 22.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

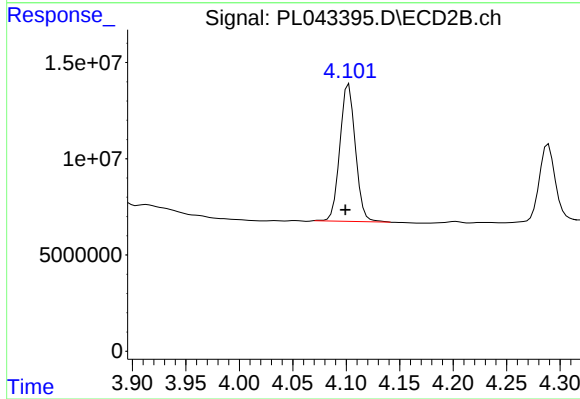


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.003 min
Response: 72010450
Conc: 24.30 ng/ml

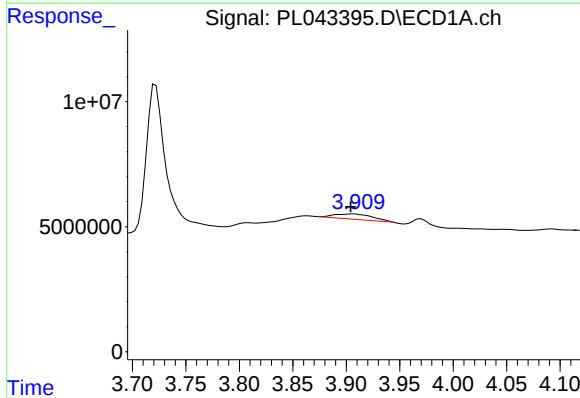


#2 alpha-BHC

R.T.: 3.906 min
Delta R.T.: 0.002 min
Response: 4946334
Conc: 0.52 ng/ml

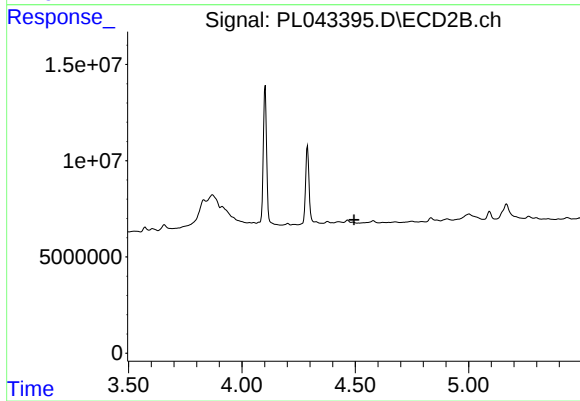

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.494 min
Response: 0
Conc: N.D.

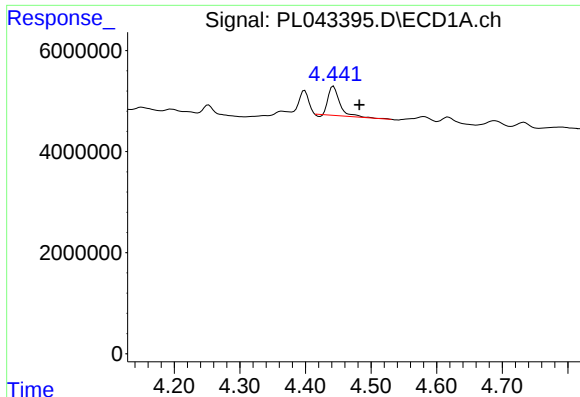

#4 Heptachlor


R.T.: 4.443 min
Delta R.T.: -0.039 min
Response: 6818032
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

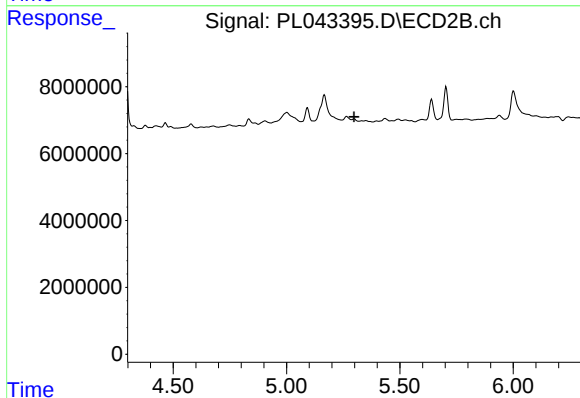


#4 Heptachlor

R.T.: 5.265 min
Delta R.T.: -0.033 min
Response: -183505
Conc: N.D.

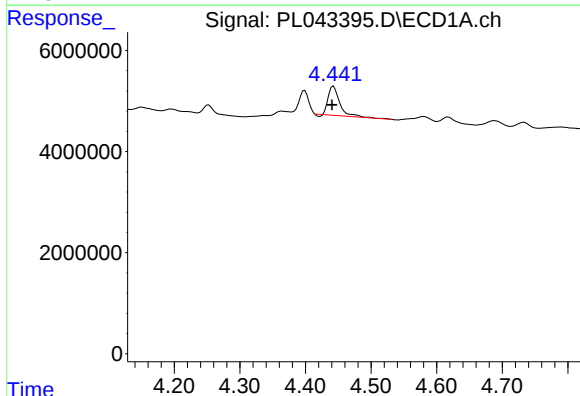


#6 beta-BHC

R.T.: 4.443 min
Delta R.T.: 0.002 min
Response: 6818032
Conc: 1.85 ng/ml

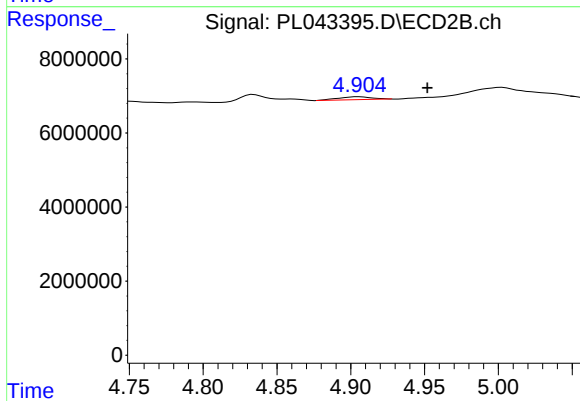

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.046 min
Response: 1307566
Conc: 0.77 ng/ml

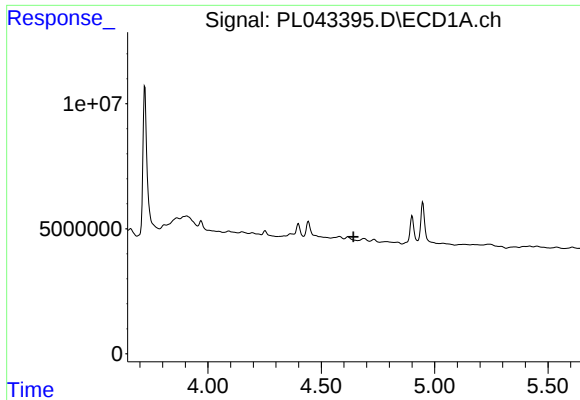

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

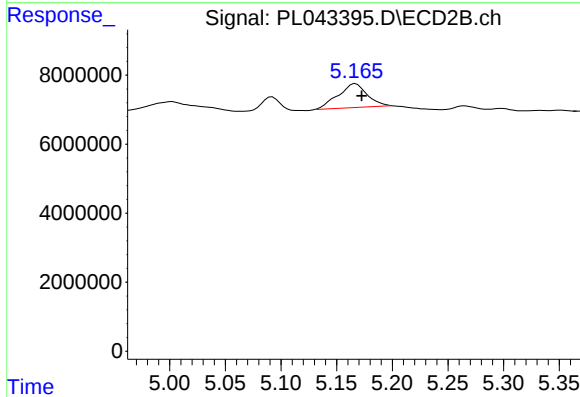


#7 delta-BHC

R.T.: 5.167 min
Delta R.T.: -0.006 min
Response: 12762342
Conc: 2.97 ng/ml

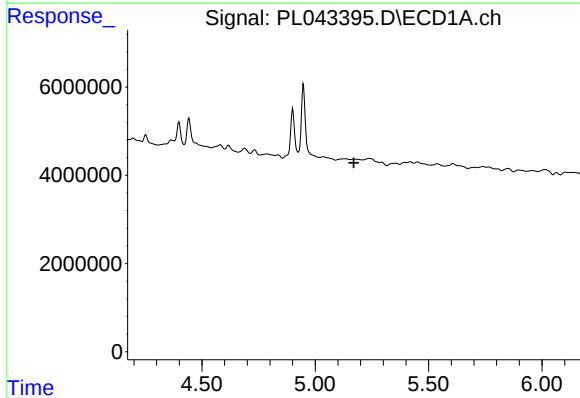


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

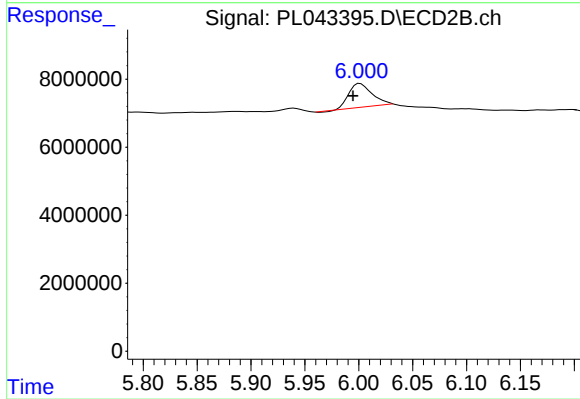

#8 Heptachlor epoxide


R.T.: 6.001 min
Delta R.T.: 0.006 min
Response: 10680450
Conc: 2.82 ng/ml

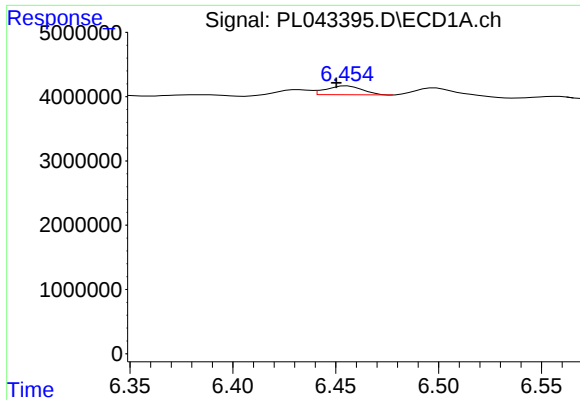

#18 Endrin aldehyde


R.T.: 6.456 min
Delta R.T.: 0.005 min
Response: 1709029
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

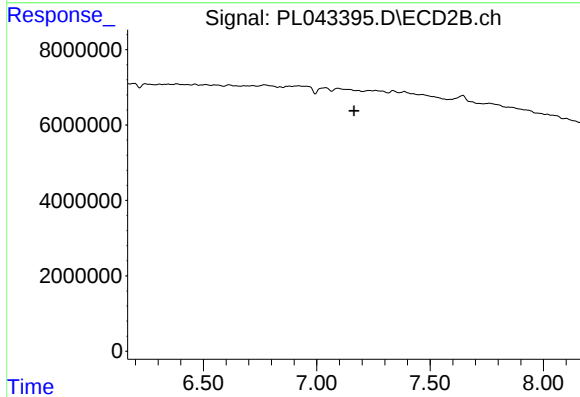


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.165 min
Response: 0
Conc: N.D.

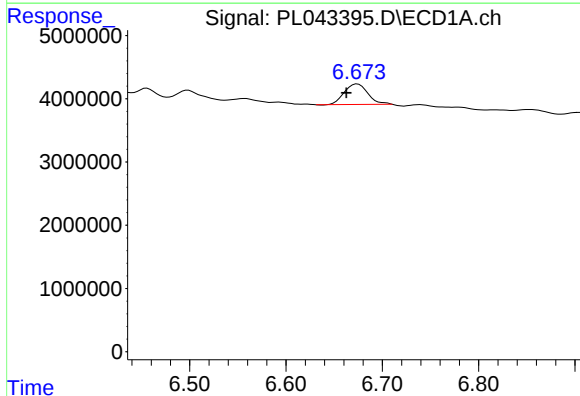


#19 Endosulfan Sulfate

R.T.: 6.674 min
Delta R.T.: 0.012 min
Response: 5489117
Conc: 0.82 ng/ml

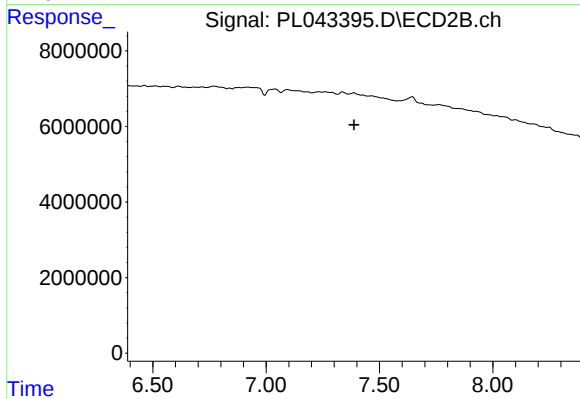

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

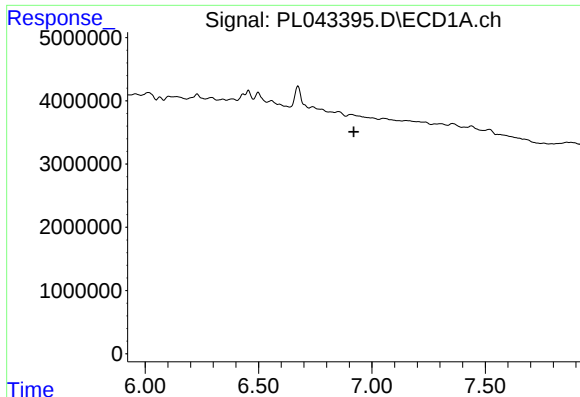

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

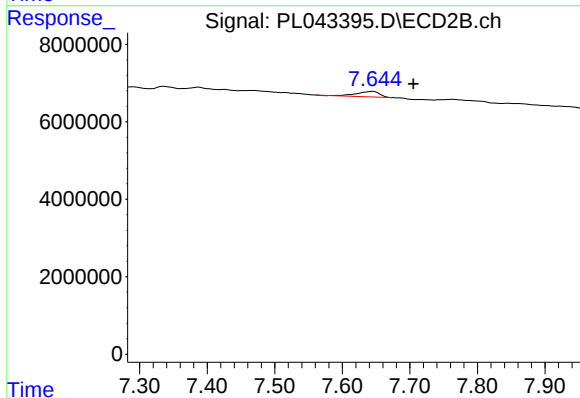


#20 Methoxychlor

R.T.: 7.646 min
Delta R.T.: -0.060 min
Response: 3254564
Conc: 2.16 ng/ml

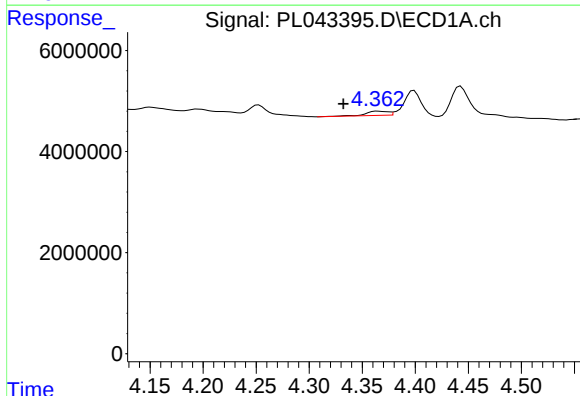


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.032 min
Response: 1267513
Conc: 4.72 ng/ml

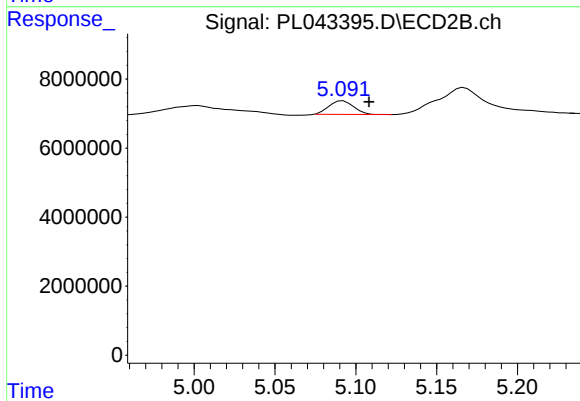

#23 Chlordane-1


R.T.: 5.092 min
Delta R.T.: -0.016 min
Response: 4187247
Conc: 29.63 ng/ml

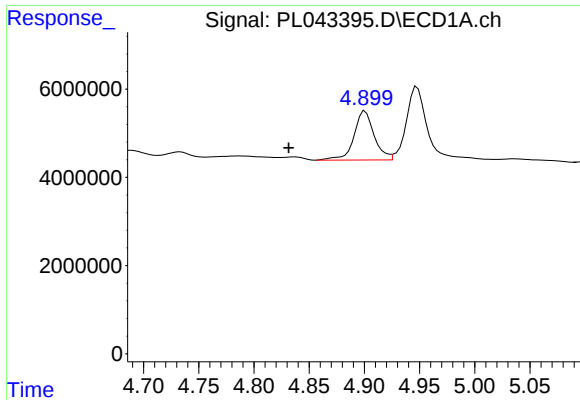

#24 Chlordane-2


R.T.: 4.901 min
Delta R.T.: 0.069 min
Response: 14151967
Conc: 49.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-122018

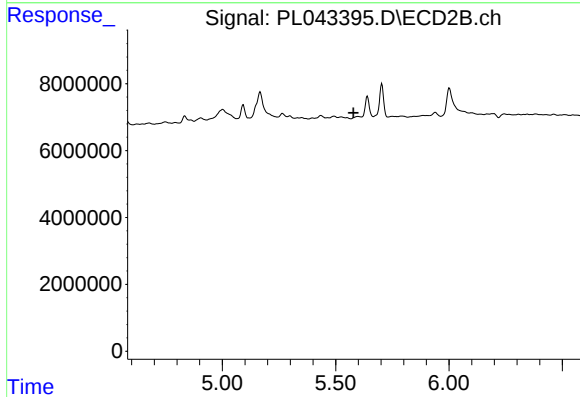


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.579 min
Response: 0
Conc: N.D.

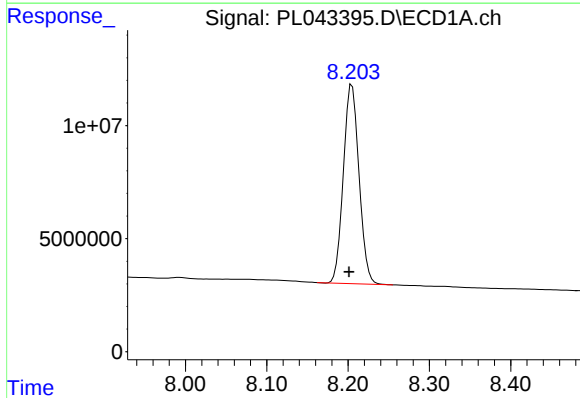

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 117604289
Conc: 18.01 ng/ml

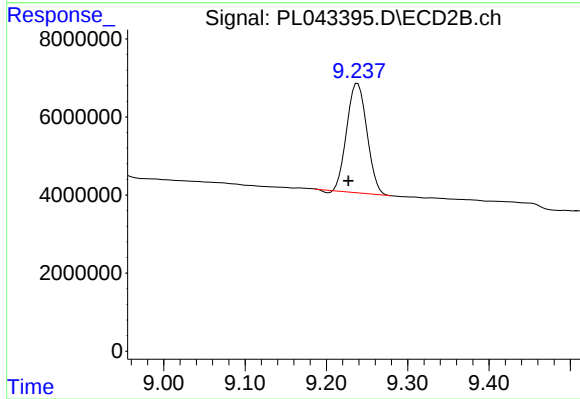

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.011 min
Response: 47841261
Conc: 18.34 ng/ml