

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 01:03
 Operator : AJ\SJ
 Sample : J6469-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DRUM-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 03:11:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.102	134.6E6	64326549	21.953	21.703
28)	SA Decachlor...	8.205	9.239	140.7E6	60659935	21.540	23.255
Target Compounds							
6)	B beta-BHC	4.399f	0.000	4066650	0	1.103	N.D. #
7)	B delta-BHC	0.000	5.170	0	3208643	N.D.	0.747 #
8)	B Heptachlo...	0.000	6.006	0	2793102	N.D.	0.737 #
9)	A Endosulfan I	0.000	6.356	0	949240	N.D.	0.280 #
11)	B alpha-Chl...	0.000	6.356f	0	949240	N.D.	0.264 #
14)	MA Endrin	6.071f	0.000	668054	0	0.093	N.D. #
16)	A 4,4'-DDD	6.071f	0.000	668054	0	0.118	N.D. #
23)	Chlordane-1	4.364	5.151	1976231	2713533	7.355	19.200 #
26)	Chlordane-4	0.000	6.356	0	949240	N.D.	1.663 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 01:03
Operator : AJ\SJ
Sample : J6469-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DRUM-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 03:11:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

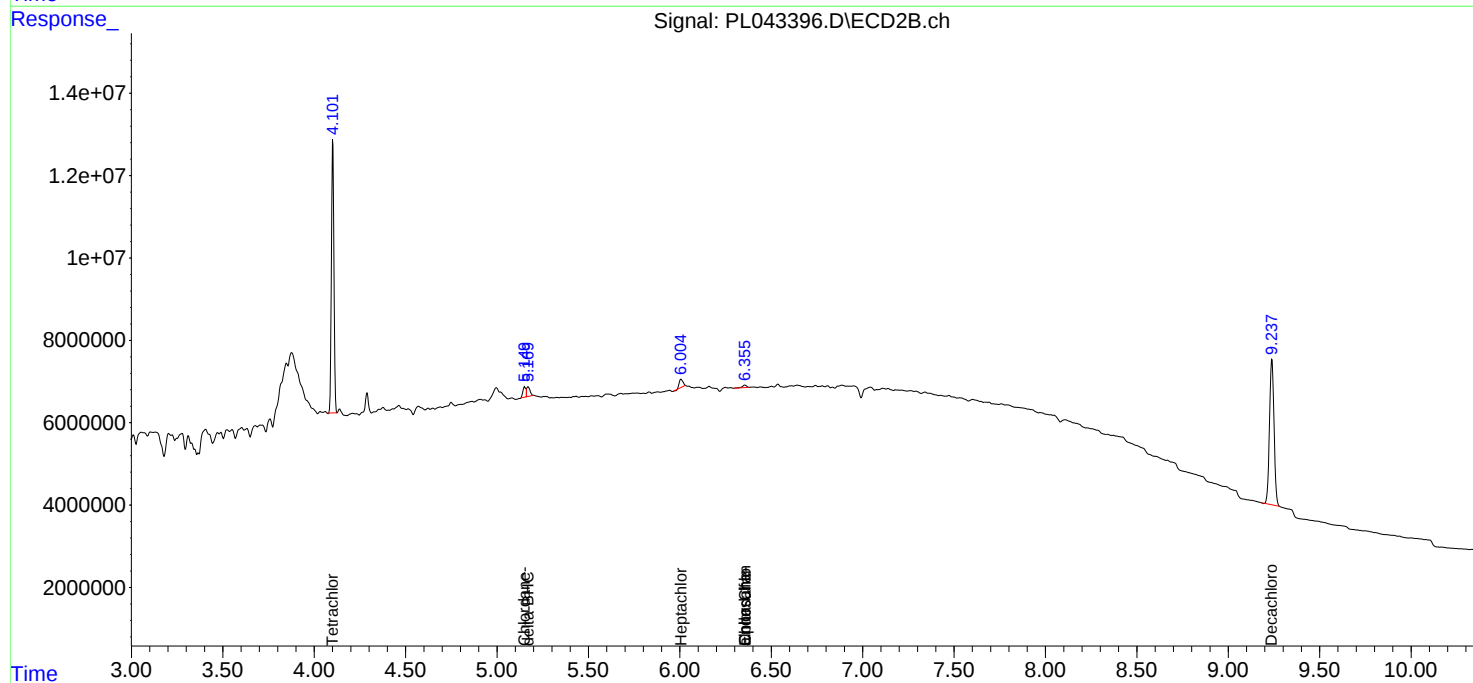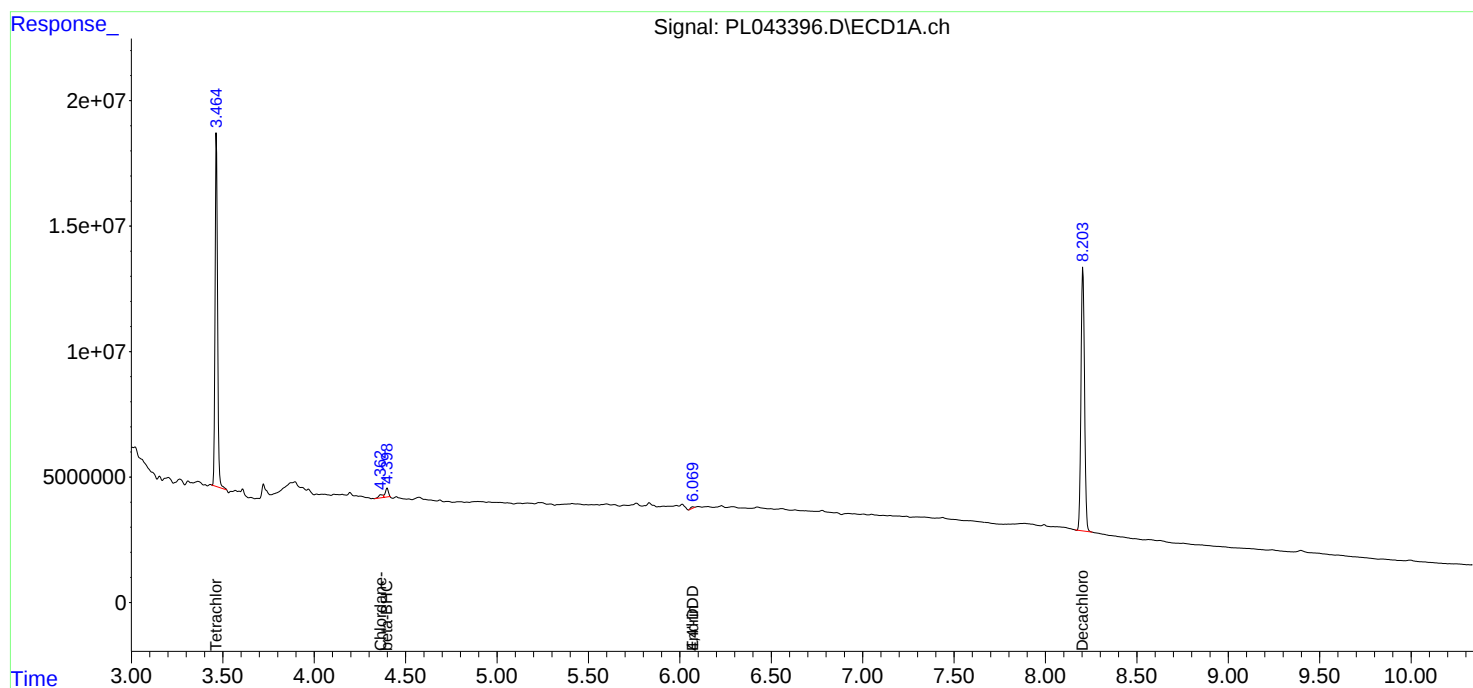


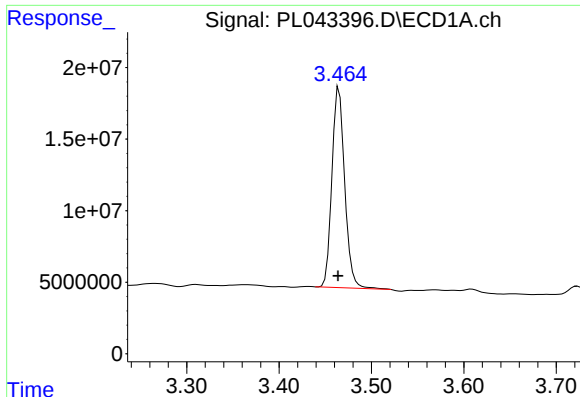

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 134634505
Conc: 21.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

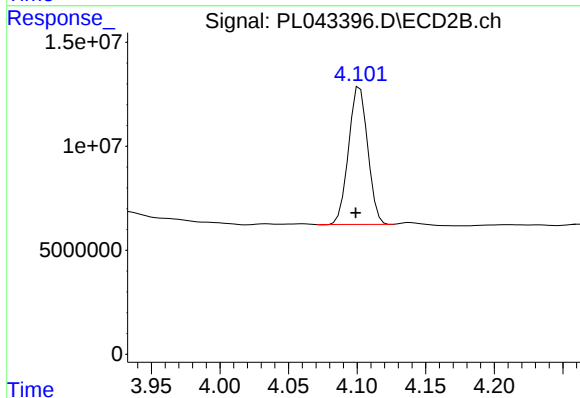


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.003 min
Response: 64326549
Conc: 21.70 ng/ml

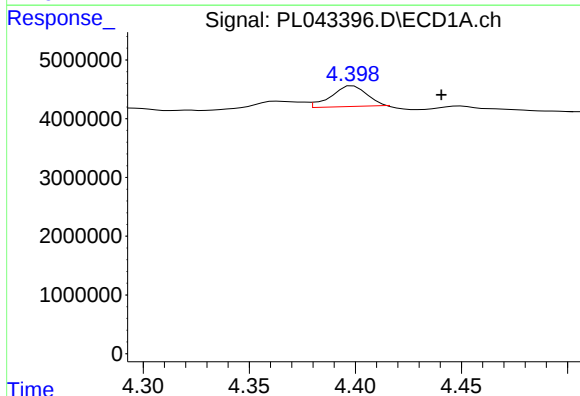


#6 beta-BHC

R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 4066650
Conc: 1.10 ng/ml

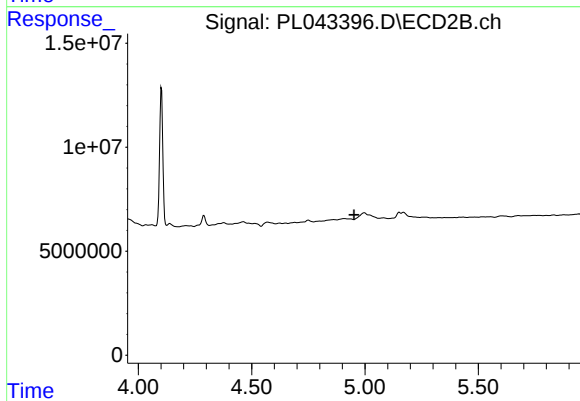

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

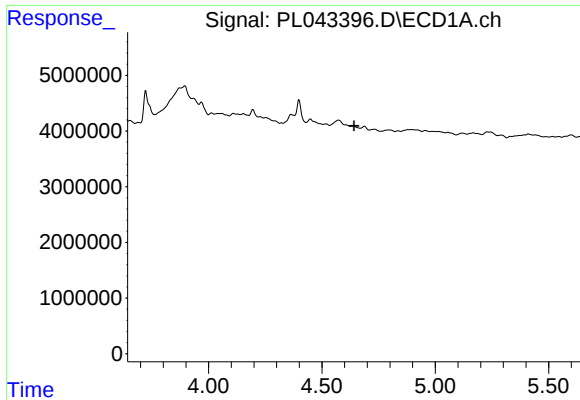

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DRUM-1

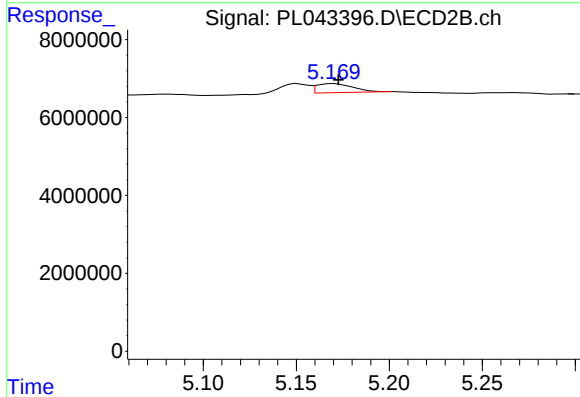


#7 delta-BHC

R.T.: 5.170 min
Delta R.T.: -0.003 min
Response: 3208643
Conc: 0.75 ng/ml

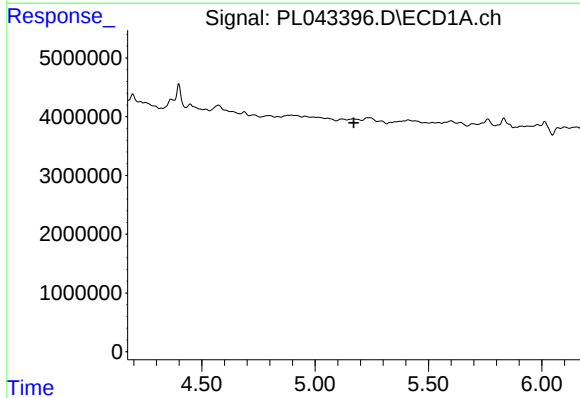


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

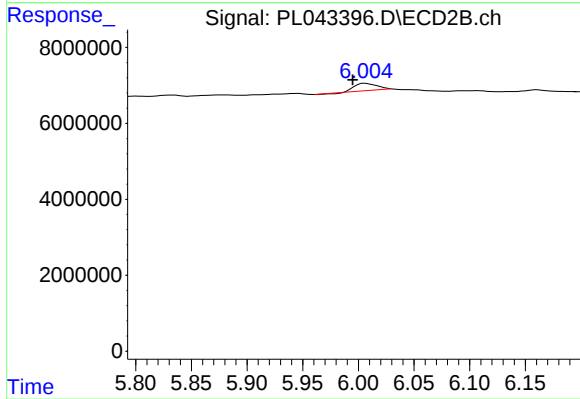

#8 Heptachlor epoxide


R.T.: 6.006 min
Delta R.T.: 0.011 min
Response: 2793102
Conc: 0.74 ng/ml

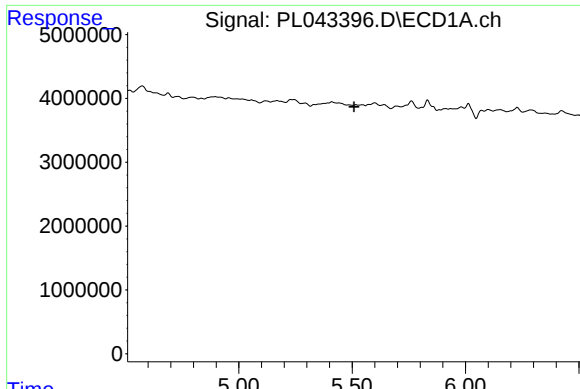

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DRUM-1

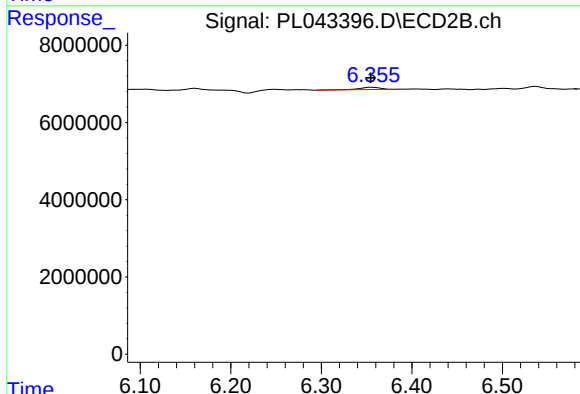


#9 Endosulfan I

R.T.: 6.356 min
Delta R.T.: 0.001 min
Response: 949240
Conc: 0.28 ng/ml

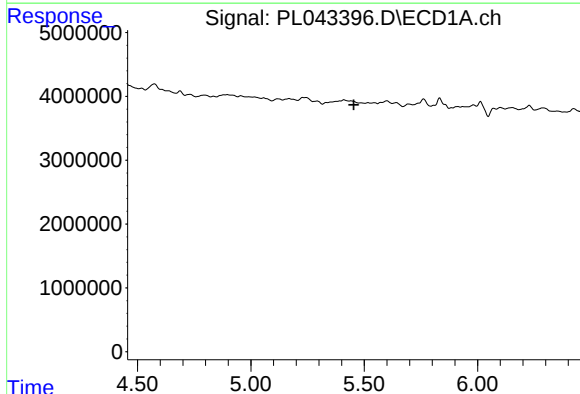


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

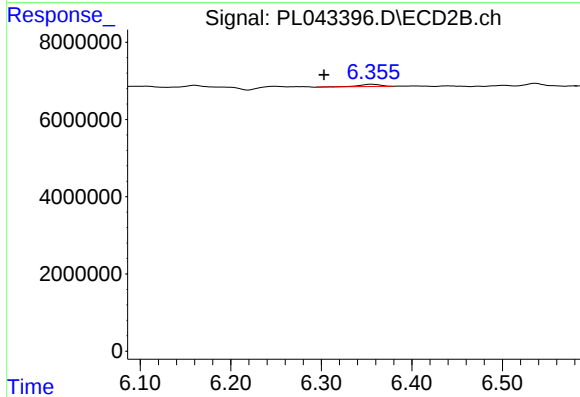

#11 alpha-Chlordane


R.T.: 6.356 min
Delta R.T.: 0.053 min
Response: 949240
Conc: 0.26 ng/ml

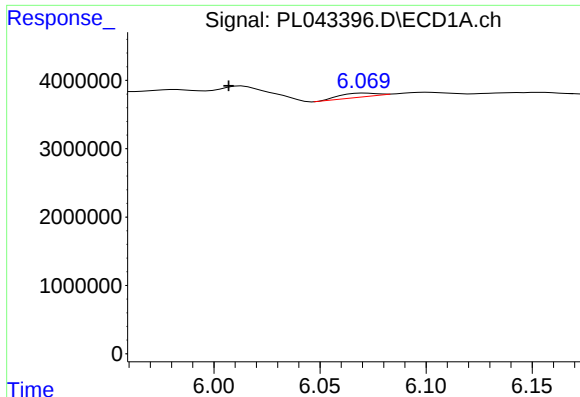

#14 Endrin


R.T.: 6.071 min
Delta R.T.: 0.064 min
Response: 668054
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

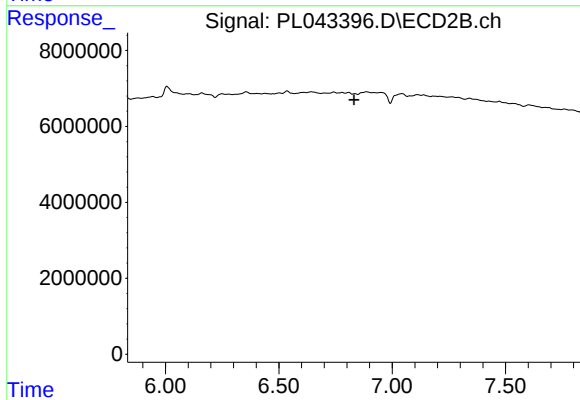


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

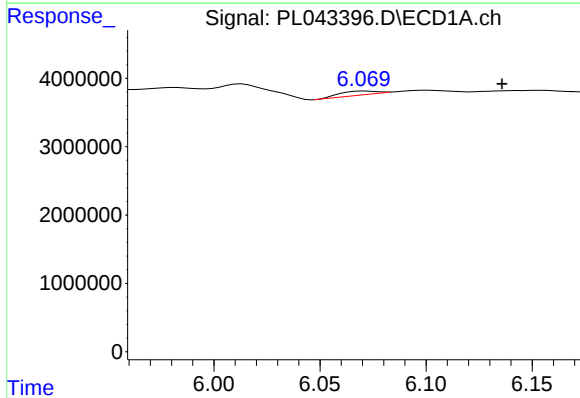


#16 4,4'-DDD

R.T.: 6.071 min
Delta R.T.: -0.065 min
Response: 668054
Conc: 0.12 ng/ml

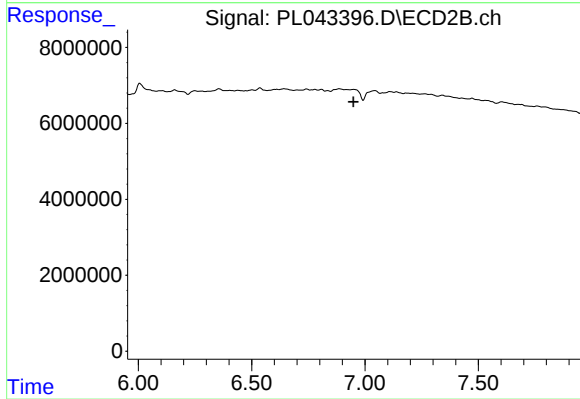

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.949 min
Response: 0
Conc: N.D.

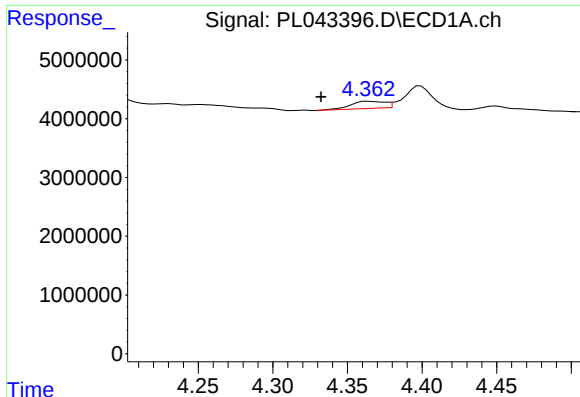

#23 Chlordane-1


R.T.: 4.364 min
Delta R.T.: 0.032 min
Response: 1976231
Conc: 7.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

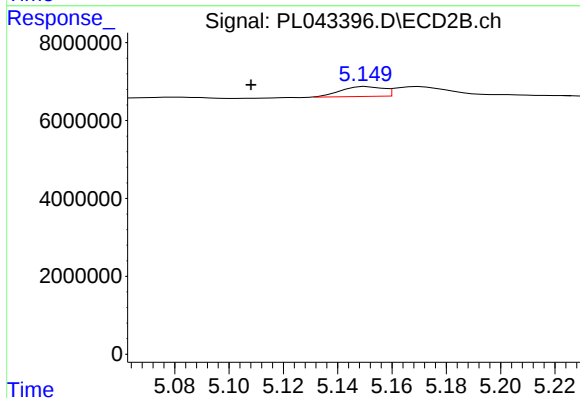


#23 Chlordane-1

R.T.: 5.151 min
Delta R.T.: 0.043 min
Response: 2713533
Conc: 19.20 ng/ml

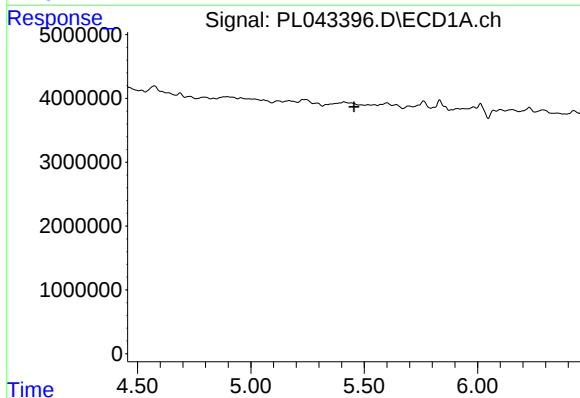


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

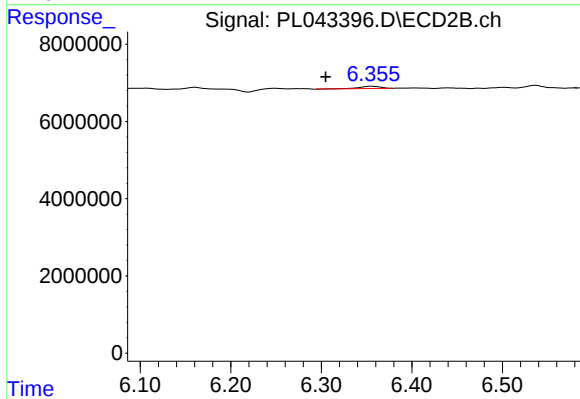

#26 Chlordane-4


R.T.: 6.356 min
Delta R.T.: 0.051 min
Response: 949240
Conc: 1.66 ng/ml

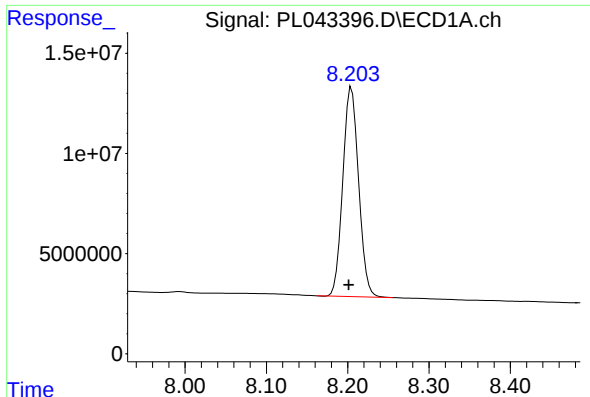

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 140656696
Conc: 21.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-1

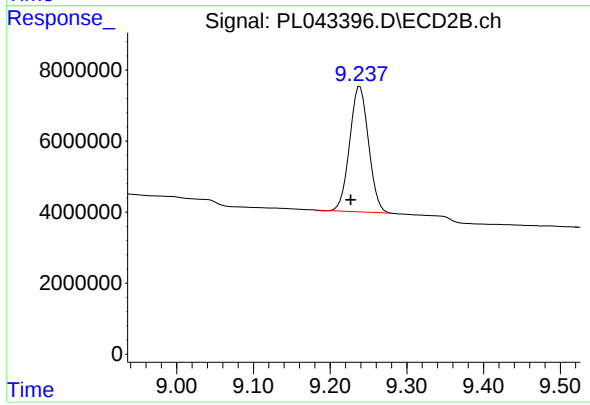

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.012 min
Response: 60659935
Conc: 23.25 ng/ml