

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 02:14
 Operator : AJ\SJ
 Sample : J6498-07
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-1219-S-TCLP-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 03:14:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.103	143.8E6	74544073	23.446	25.151
28)	SA Decachlor...	8.205	9.239	122.0E6	54158177	18.677	20.762
Target Compounds							
6)	B beta-BHC	4.399f	0.000	4344621	0	1.178	N.D. #
7)	B delta-BHC	0.000	5.170	0	3624731	N.D.	0.843 #
8)	B Heptachlo...	0.000	6.006	0	4046788	N.D.	1.067 #
14)	MA Endrin	6.016	0.000	2548066	0	0.354	N.D. #
23)	Chlordane-1	4.364	5.152	1089734	2688522	4.055	19.023 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 02:14
Operator : AJ\SJ
Sample : J6498-07
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-1219-S-TCLP-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 03:14:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

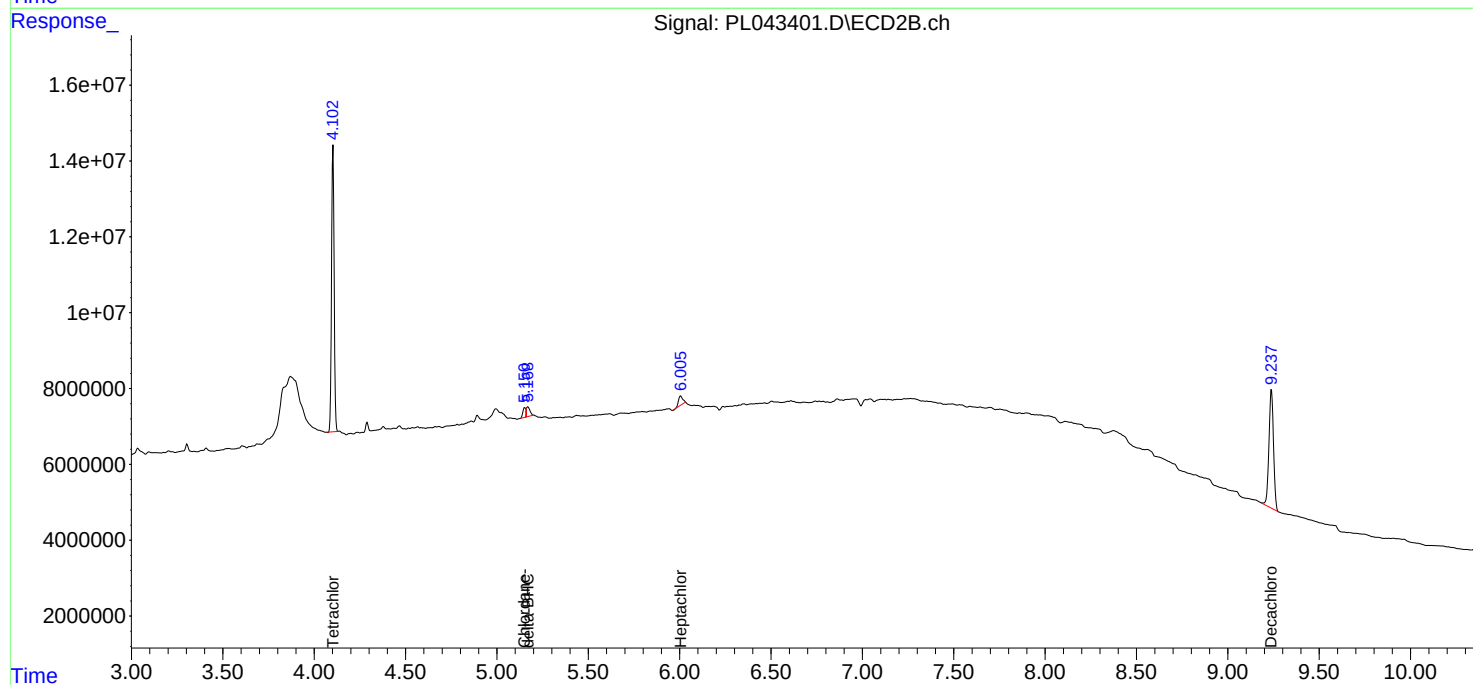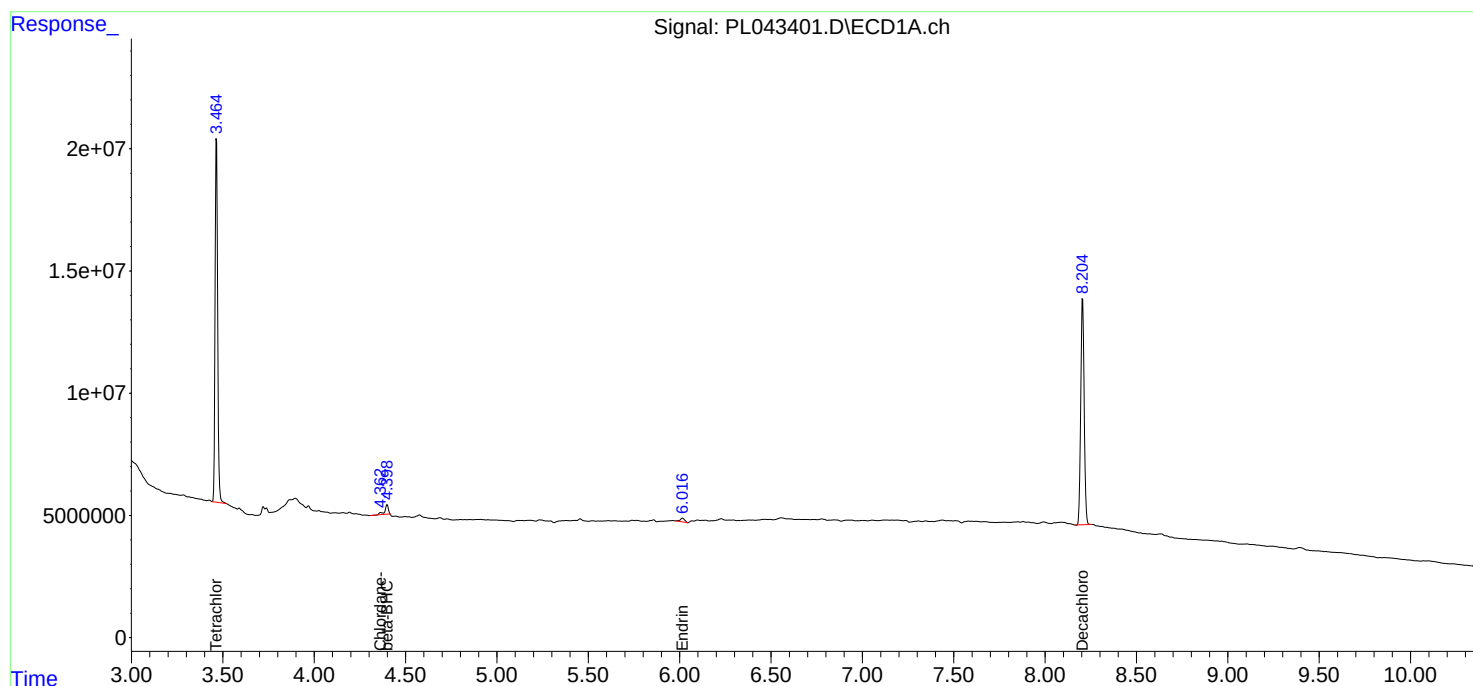


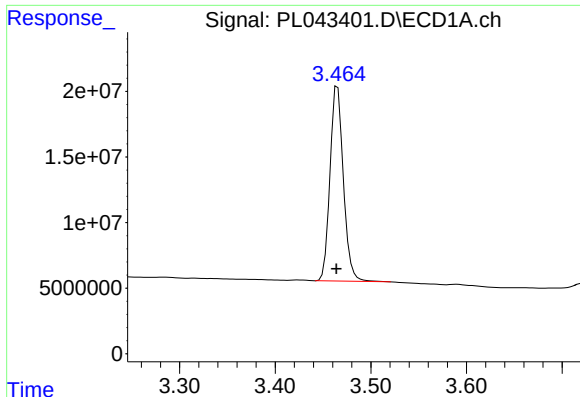

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 143793129
Conc: 23.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1219-S-TCLP-5

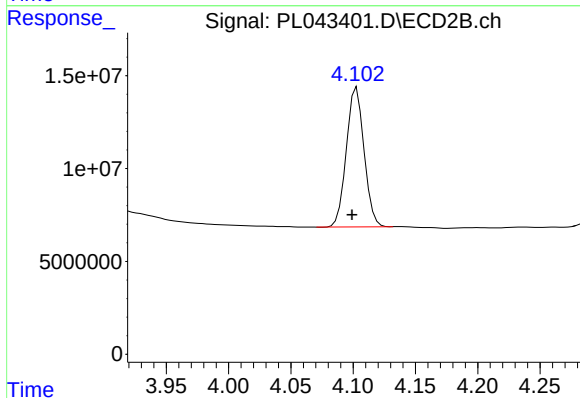


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.004 min
Response: 74544073
Conc: 25.15 ng/ml

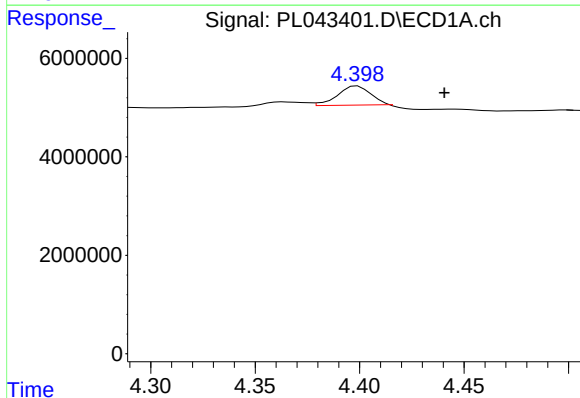


#6 beta-BHC

R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 4344621
Conc: 1.18 ng/ml

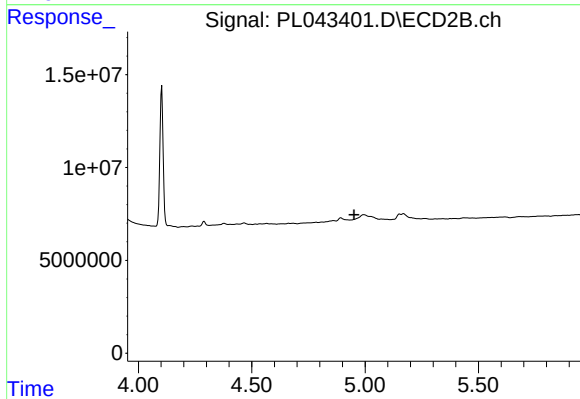

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.952 min
Response: 0
Conc: N.D.

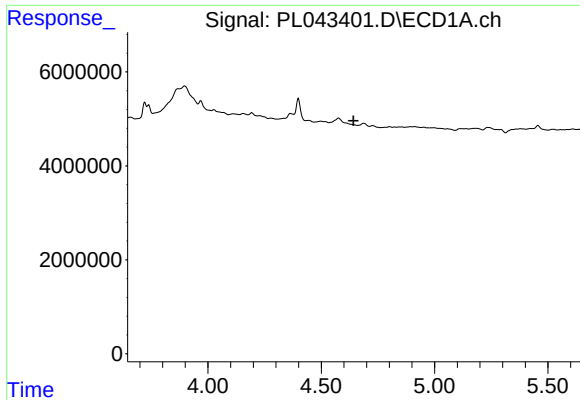

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SSSI-1219-S-TCLP-5

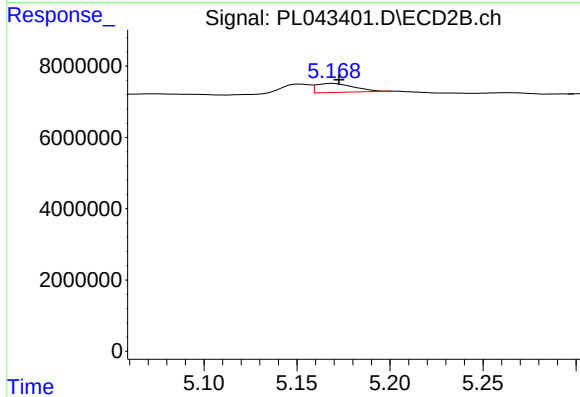


#7 delta-BHC

R.T.: 5.170 min
Delta R.T.: -0.003 min
Response: 3624731
Conc: 0.84 ng/ml

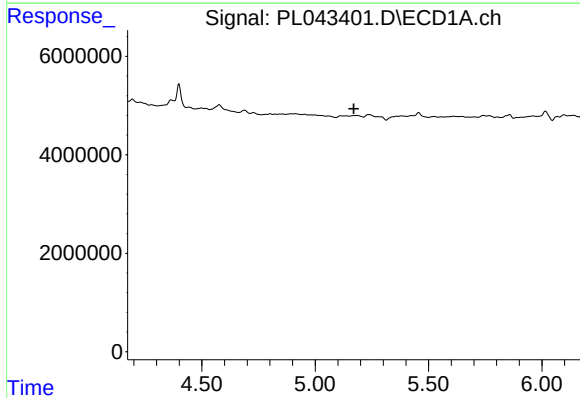


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

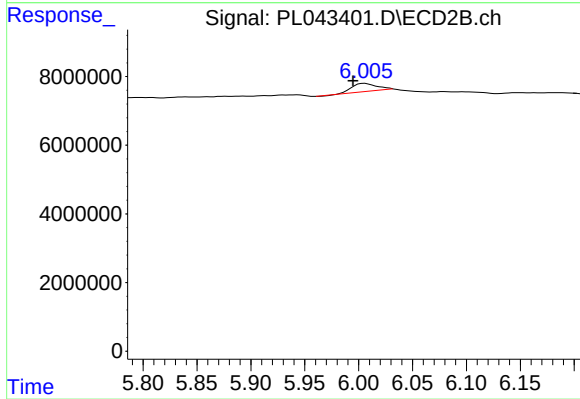

#8 Heptachlor epoxide


R.T.: 6.006 min
Delta R.T.: 0.011 min
Response: 4046788
Conc: 1.07 ng/ml

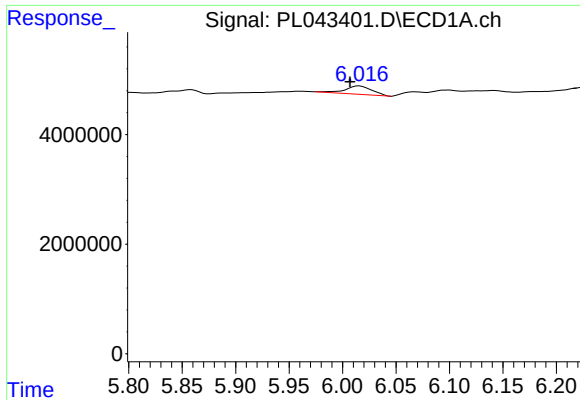

#14 Endrin


R.T.: 6.016 min
Delta R.T.: 0.009 min
Response: 2548066
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1219-S-TCLP-5

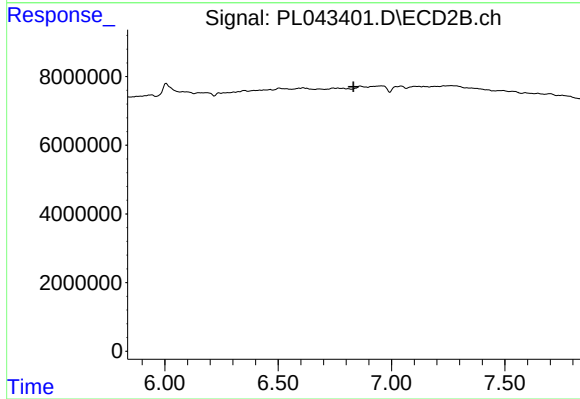


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.832 min
Response: 0
Conc: N.D.

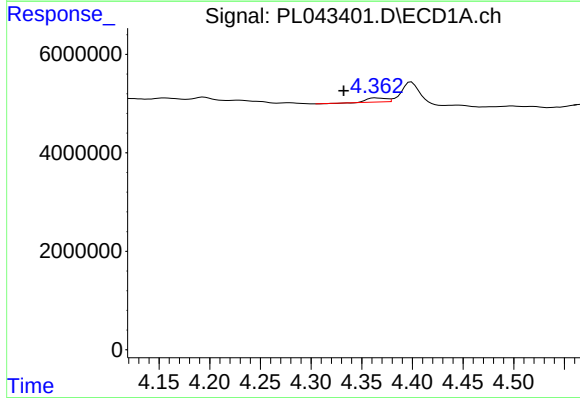


#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.031 min
Response: 1089734
Conc: 4.06 ng/ml

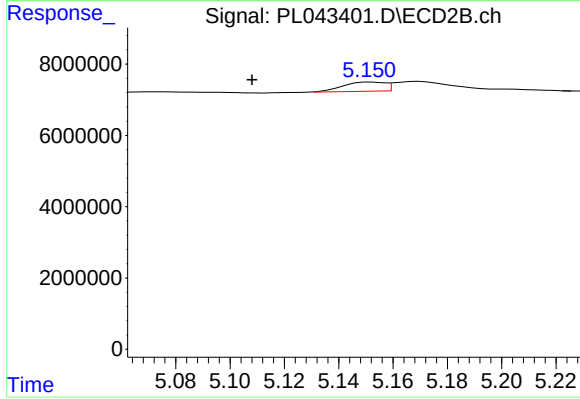

#23 Chlordane-1


R.T.: 5.152 min
Delta R.T.: 0.044 min
Response: 2688522
Conc: 19.02 ng/ml

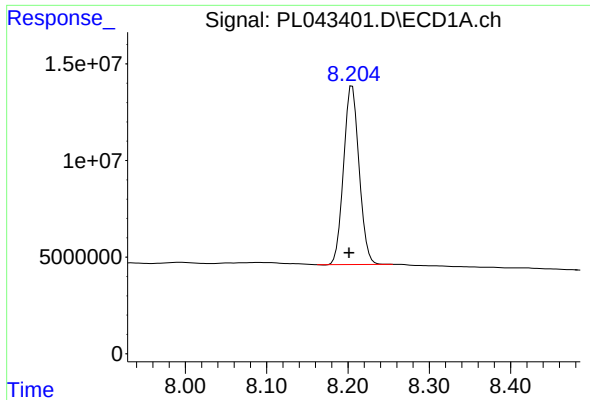

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 121963324
Conc: 18.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-1219-S-TCLP-5

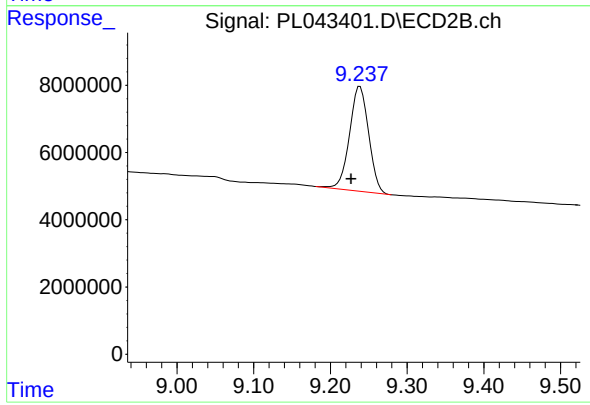

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.012 min
Response: 54158177
Conc: 20.76 ng/ml