

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 04:07
 Operator : AJ\SJ
 Sample : J6501-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 05:43:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.103	133.2E6	67072560	21.725	22.630
28)	SA Decachlor...	8.205	9.239	119.9E6	51629542	18.366	19.793
Target Compounds							
2)	A alpha-BHC	0.000	4.473	0	800729	N.D.	0.177 #
6)	B beta-BHC	4.399f	0.000	4327754	0	1.173	N.D. #
7)	B delta-BHC	0.000	5.169	0	6823764	N.D.	1.588 #
8)	B Heptachlo...	0.000	6.004	0	5233728	N.D.	1.380 #
9)	A Endosulfan I	0.000	6.318f	0	116358	N.D.	0.034 #
11)	B alpha-Chl...	0.000	6.318	0	116358	N.D.	0.032 #
15)	B Endosulfa...	6.229f	0.000	1692348	0	0.254	N.D. #
23)	Chlordane-1	4.338	5.169	3191714	6823764	11.878	48.281 #
26)	Chlordane-4	0.000	6.318	0	116358	N.D.	0.204 #
27)	Chlordane-5	6.229	0.000	1692348	0	7.056	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 04:07
Operator : AJ\SJ
Sample : J6501-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VNJ-221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 05:43:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

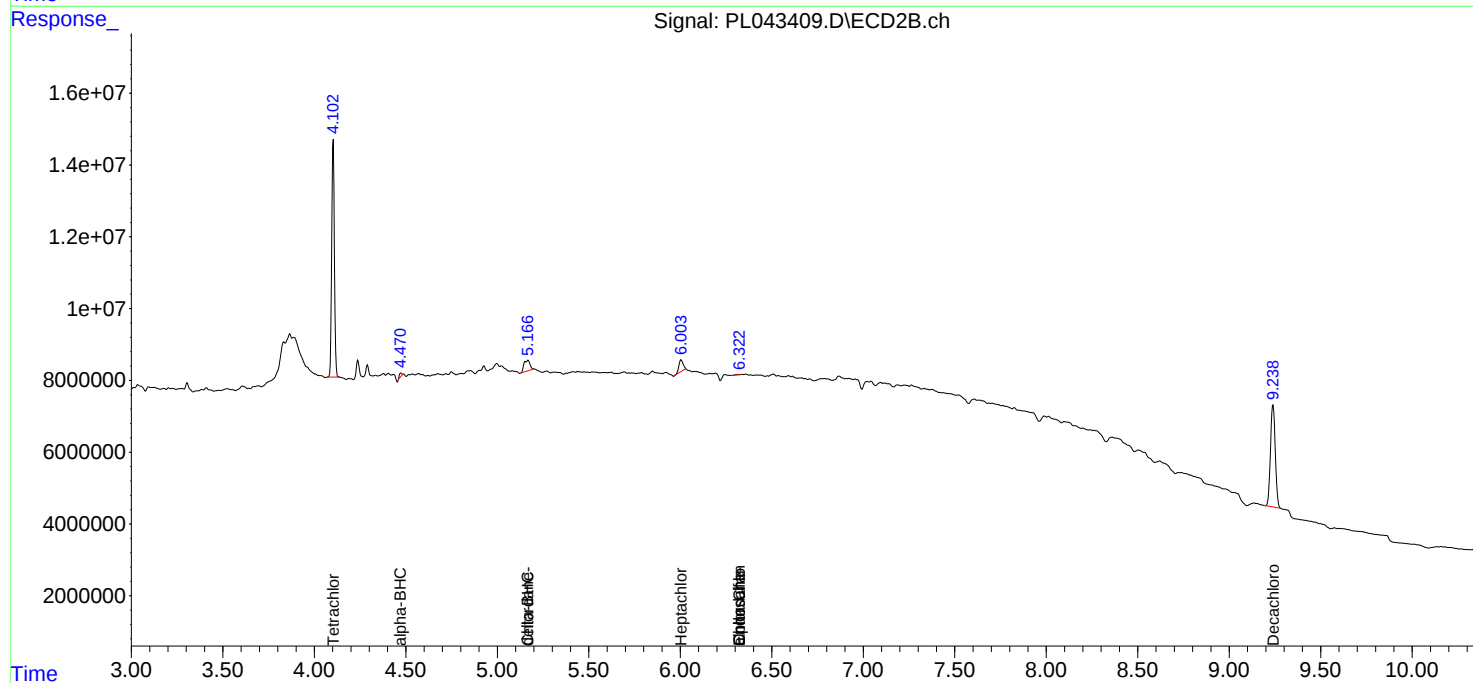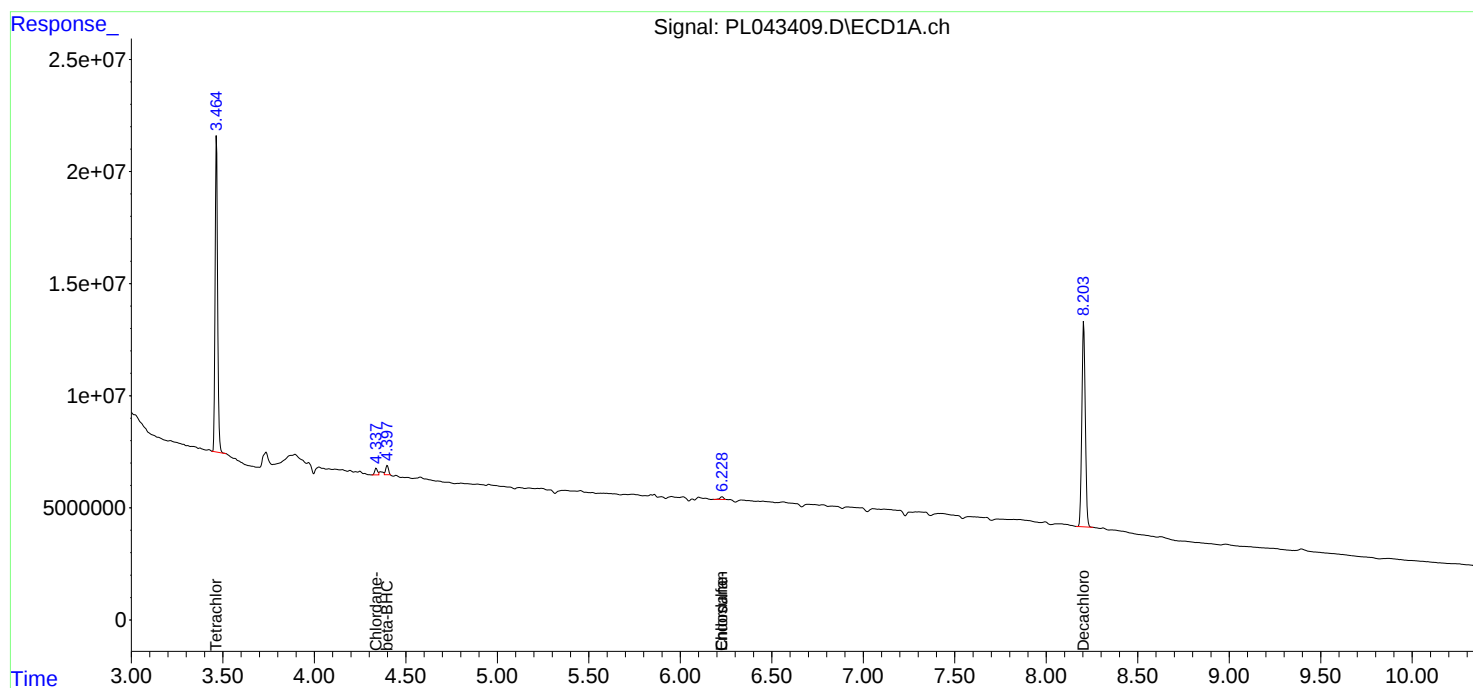


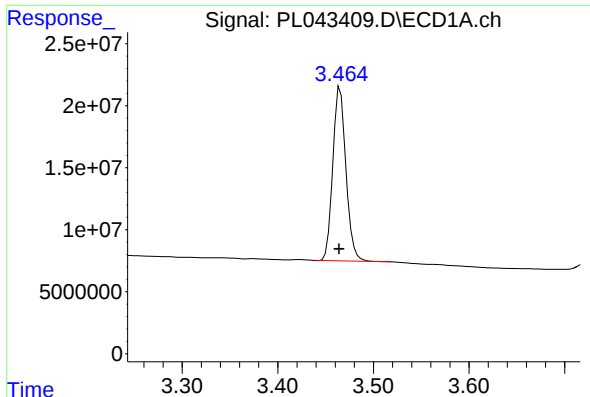

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 133236247
Conc: 21.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-221

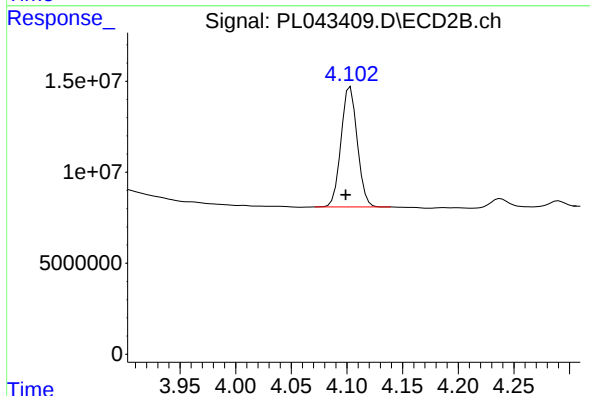


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.004 min
Response: 67072560
Conc: 22.63 ng/ml

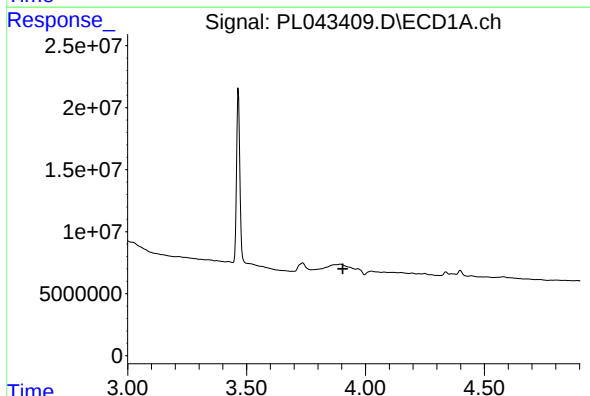


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.904 min
Response: 0
Conc: N.D.

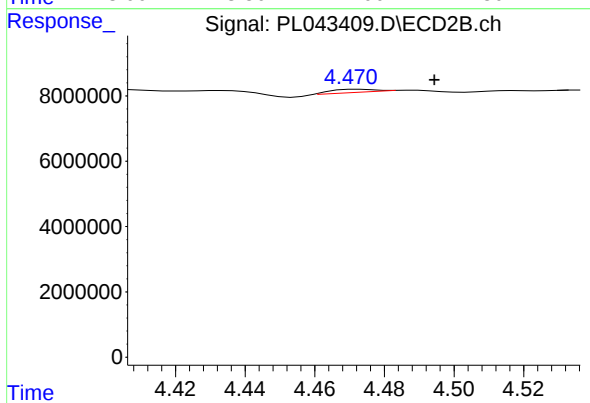

#2 alpha-BHC


R.T.: 4.473 min
Delta R.T.: -0.022 min
Response: 800729
Conc: 0.18 ng/ml

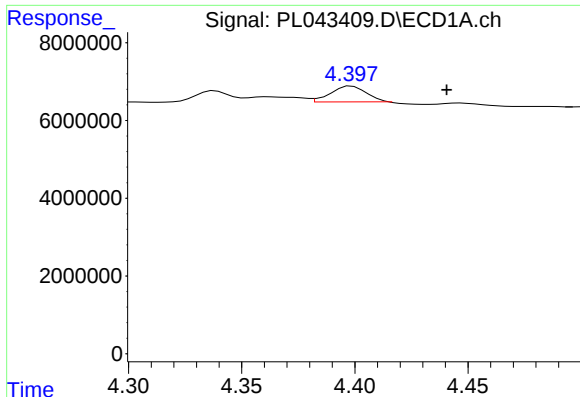

#6 beta-BHC


R.T.: 4.399 min
Delta R.T.: -0.042 min
Response: 4327754
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-221

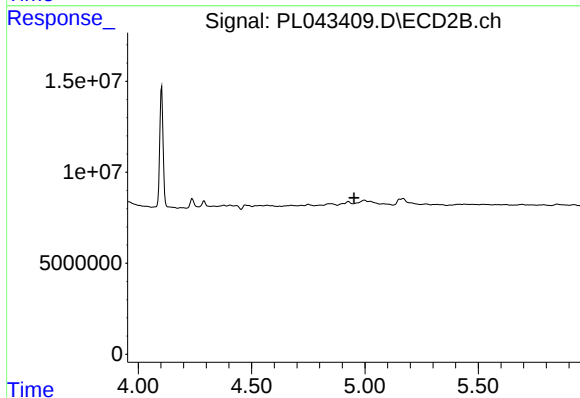


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

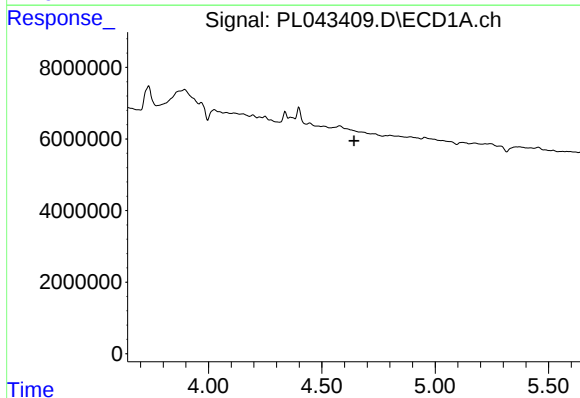


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

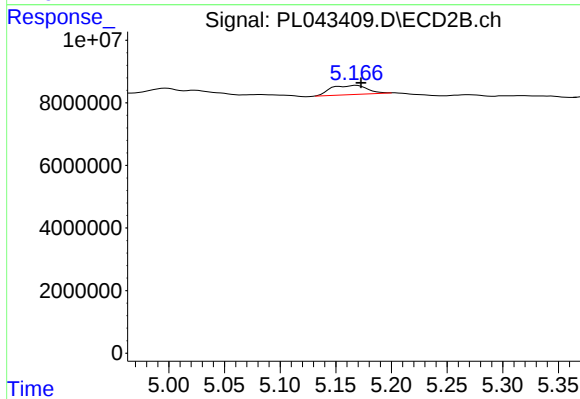

#7 delta-BHC


R.T.: 5.169 min
Delta R.T.: -0.004 min
Response: 6823764
Conc: 1.59 ng/ml

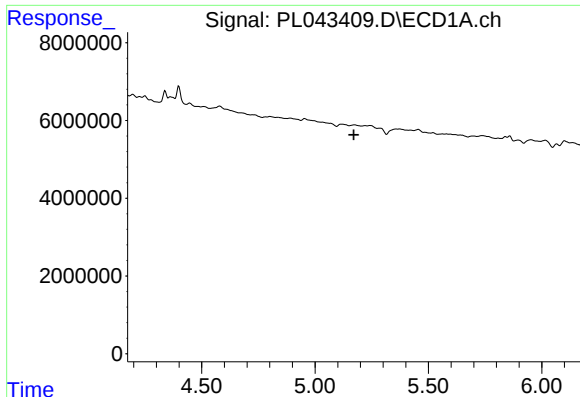

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-221

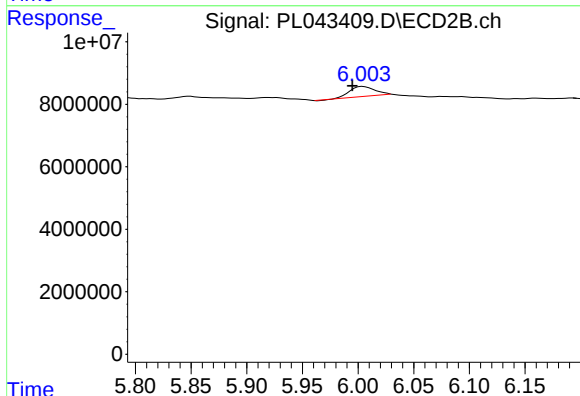


#8 Heptachlor epoxide

R.T.: 6.004 min
Delta R.T.: 0.009 min
Response: 5233728
Conc: 1.38 ng/ml

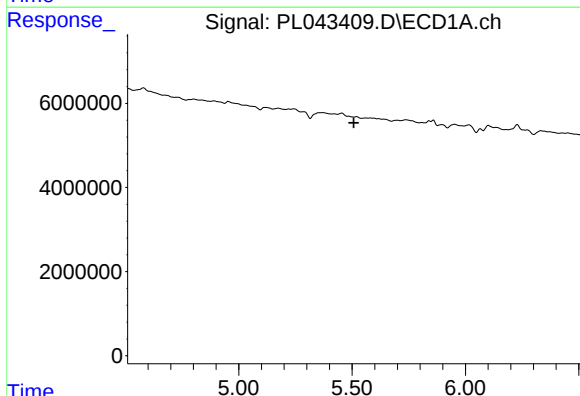


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

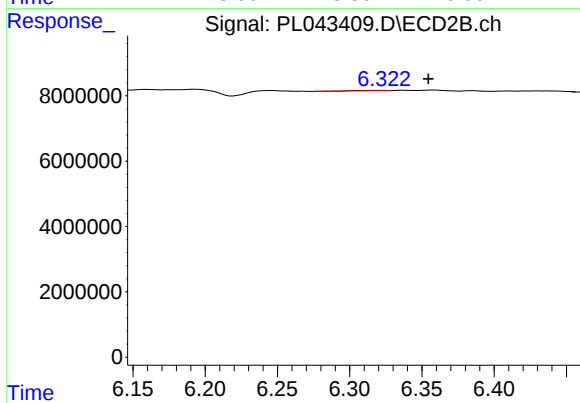

#9 Endosulfan I


R.T.: 6.318 min
Delta R.T.: -0.036 min
Response: 116358
Conc: 0.03 ng/ml

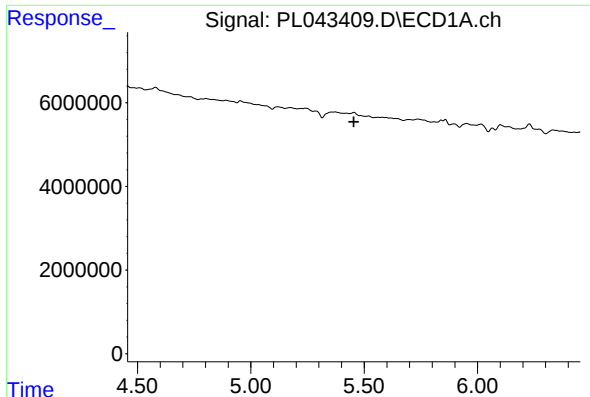

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VNJ-221

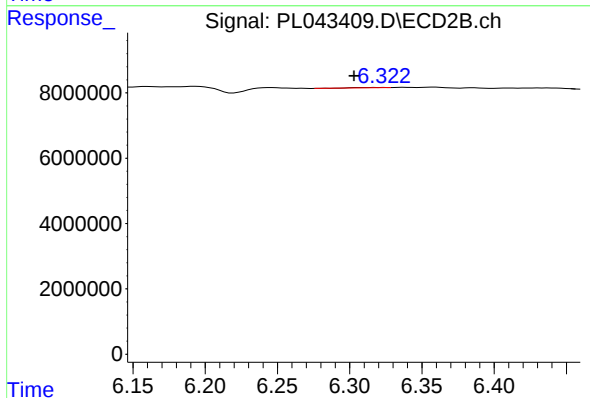


#11 alpha-Chlordane

R.T.: 6.318 min
Delta R.T.: 0.015 min
Response: 116358
Conc: 0.03 ng/ml

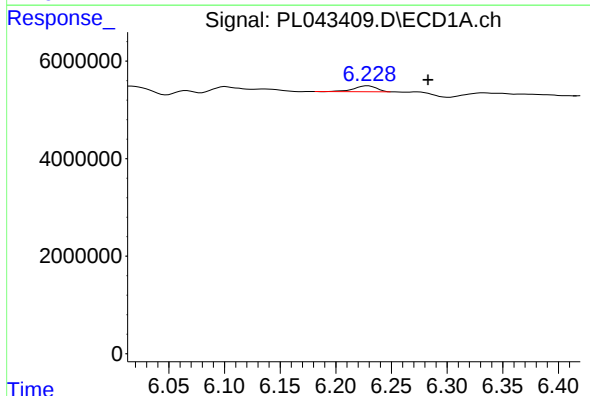


#15 Endosulfan II

R.T.: 6.229 min
Delta R.T.: -0.054 min
Response: 1692348
Conc: 0.25 ng/ml

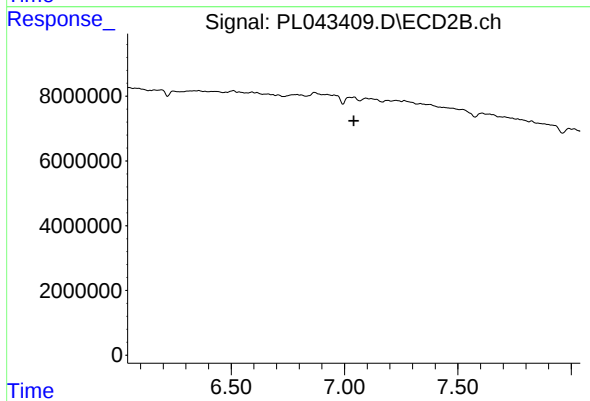

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

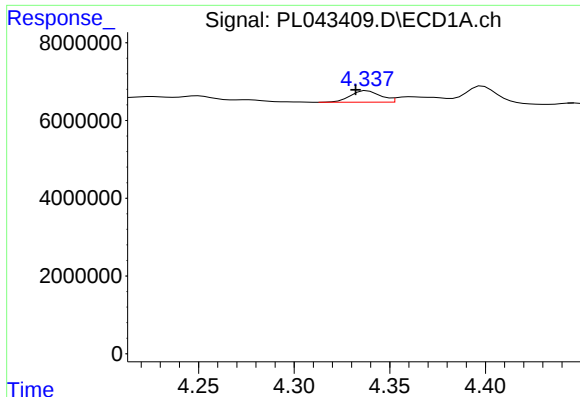

#23 Chlordane-1


R.T.: 4.338 min
Delta R.T.: 0.006 min
Response: 3191714
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-221

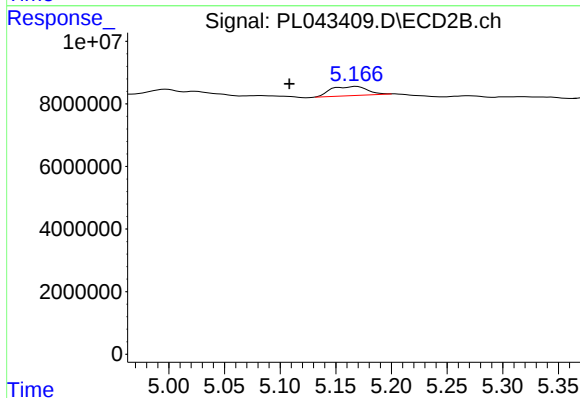


#23 Chlordane-1

R.T.: 5.169 min
Delta R.T.: 0.061 min
Response: 6823764
Conc: 48.28 ng/ml

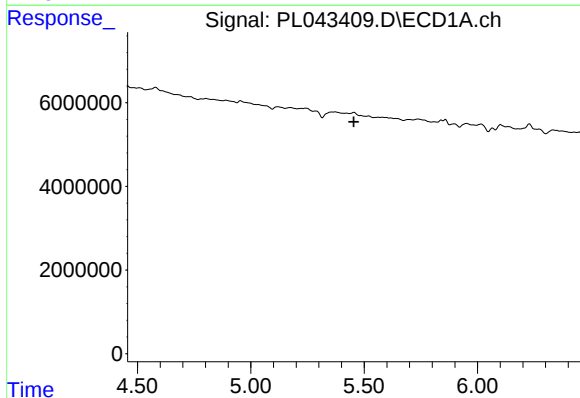


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

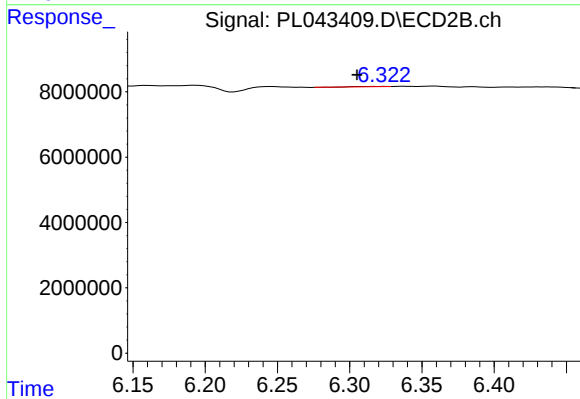

#26 Chlordane-4


R.T.: 6.318 min
Delta R.T.: 0.013 min
Response: 116358
Conc: 0.20 ng/ml

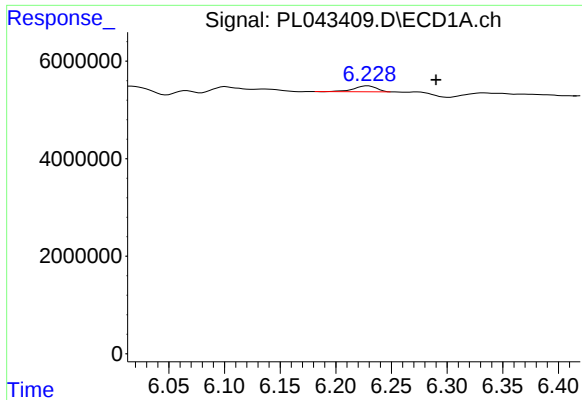

#27 Chlordane-5


R.T.: 6.229 min
Delta R.T.: -0.061 min
Response: 1692348
Conc: 7.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-221

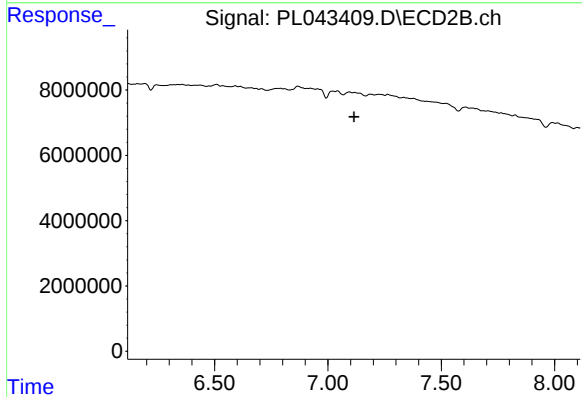


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.115 min
Response: 0
Conc: N.D.

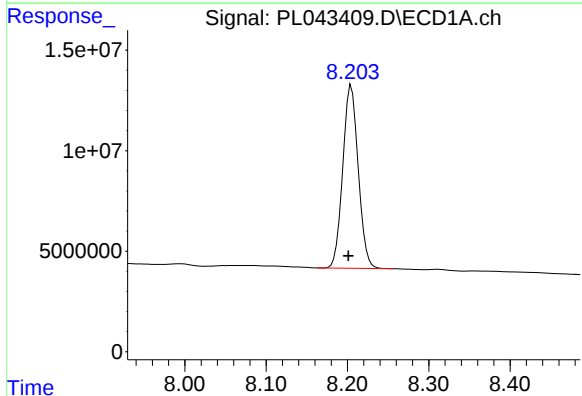

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 119930590
Conc: 18.37 ng/ml

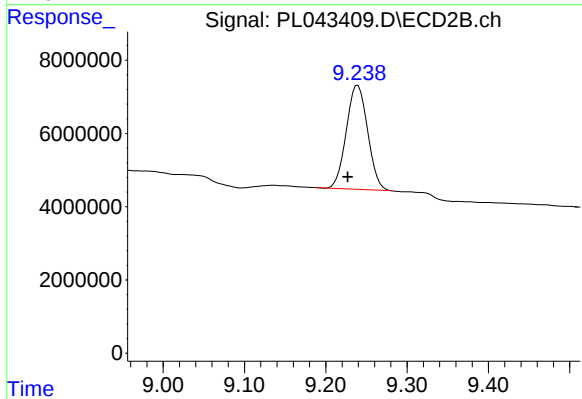

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.012 min
Response: 51629542
Conc: 19.79 ng/ml