

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 14:22
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 08:14:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.101	140.5E6	69330459	22.911	23.392
28)	SA Decachlor...	8.204	9.235	123.8E6	57060536	18.966	21.875
Target Compounds							
6)	B beta-BHC	0.000	4.907f	0	1713125	N.D.	1.012 #
8)	B Heptachlo...	0.000	5.995	0	5087056	N.D.	1.342 #
15)	B Endosulfa...	6.231f	0.000	988964	0	0.149	N.D. #
20)	A Methoxychlor	0.000	7.646f	0	5106572	N.D.	3.386 #
23)	Chlordane-1	4.362	0.000	327366	0	1.218	N.D. #
27)	Chlordane-5	6.231	0.000	988964	0	4.123	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 14:22
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 08:14:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

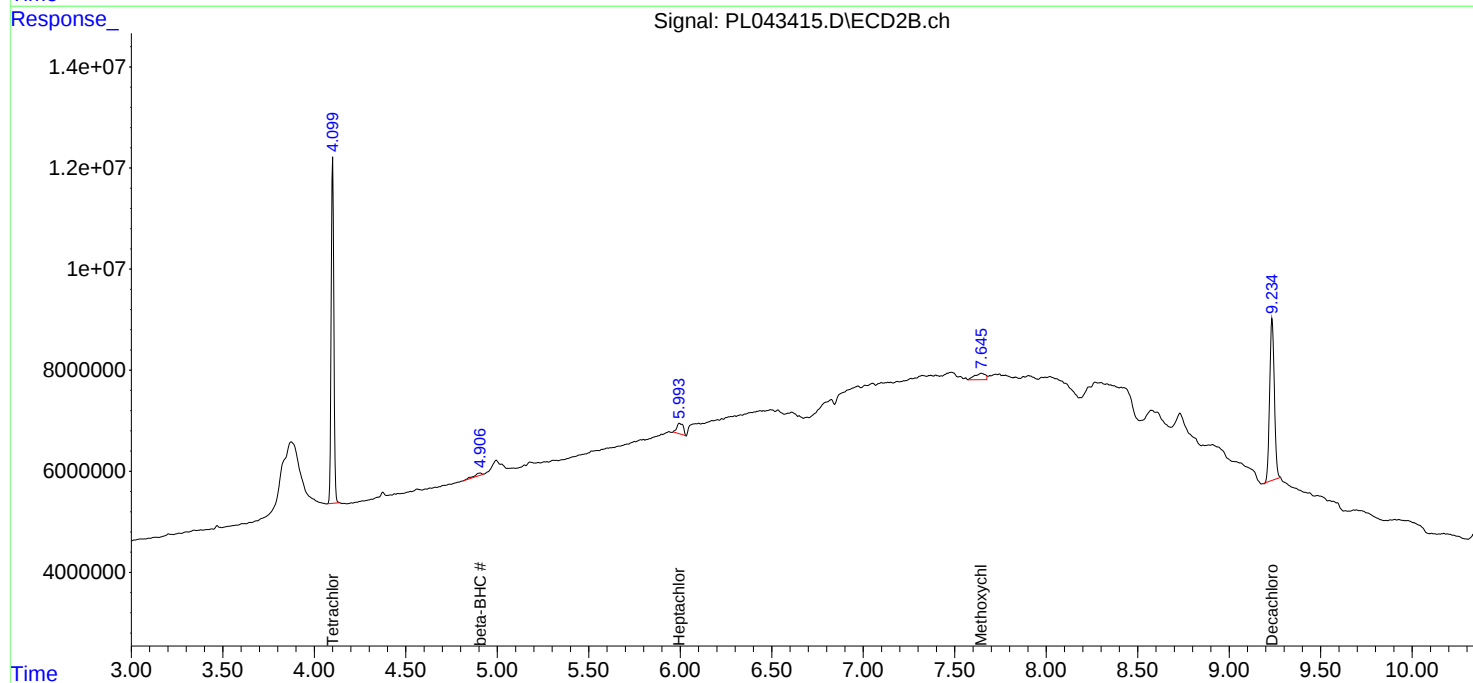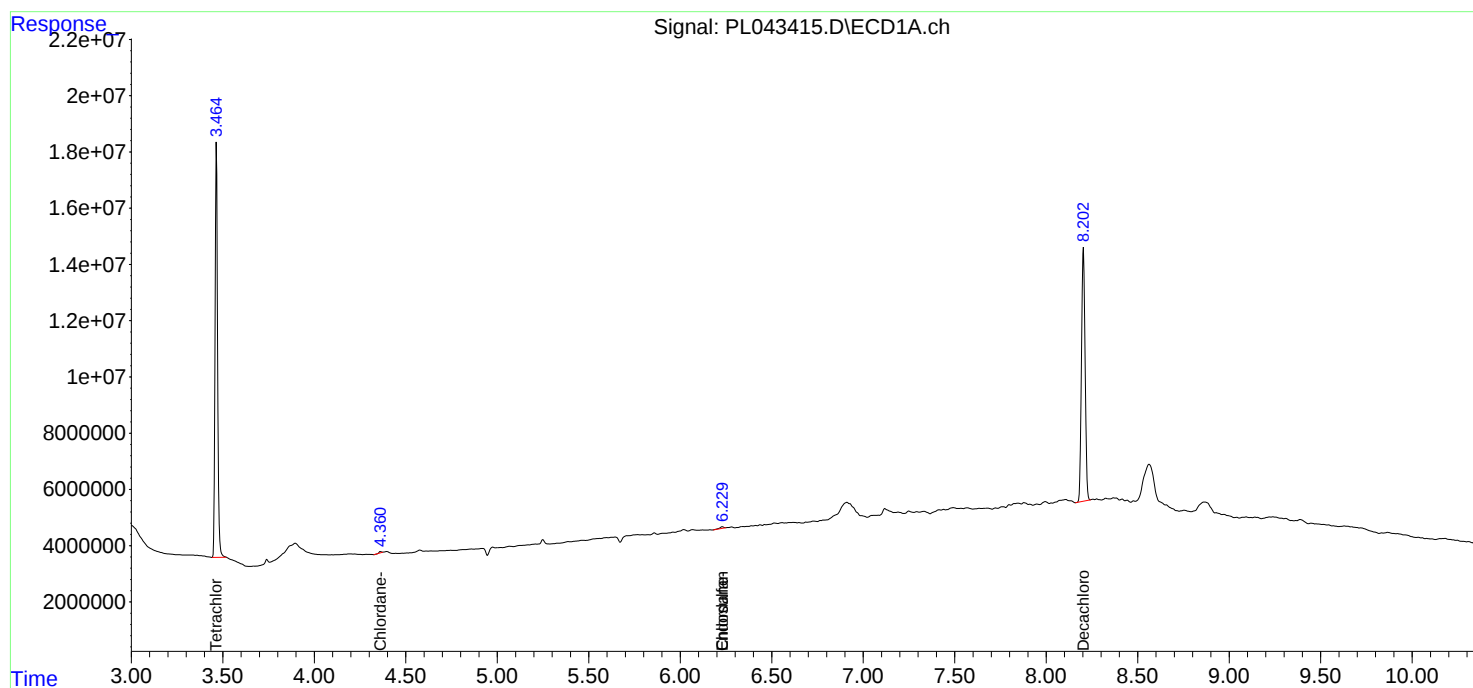


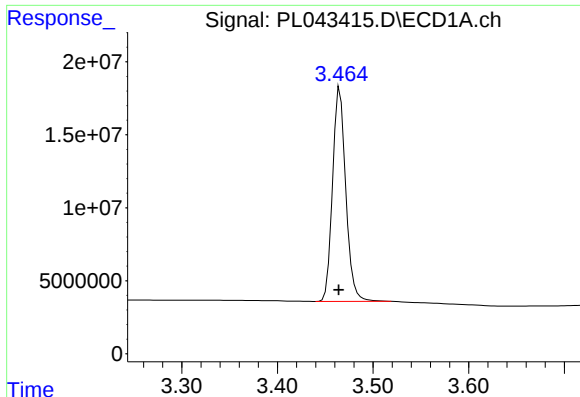

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 140508750
Conc: 22.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

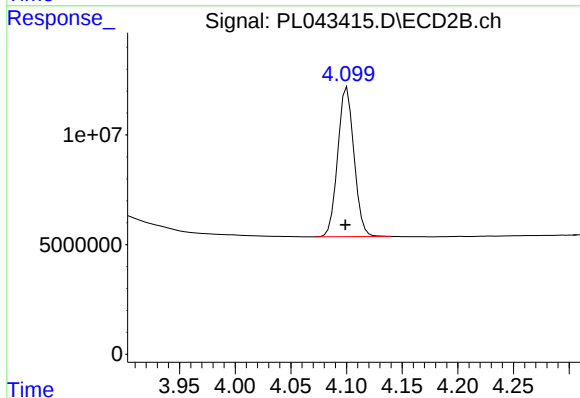


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.002 min
Response: 69330459
Conc: 23.39 ng/ml

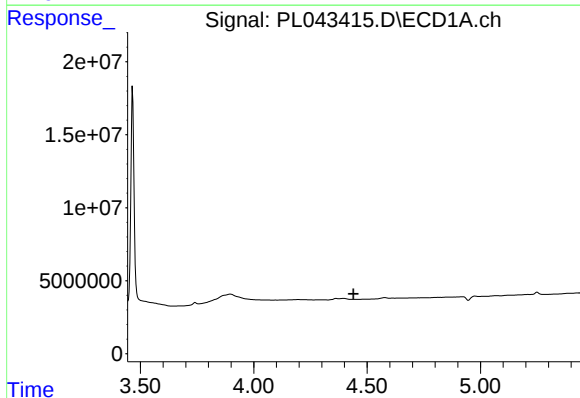


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.441 min
Response: 0
Conc: N.D.

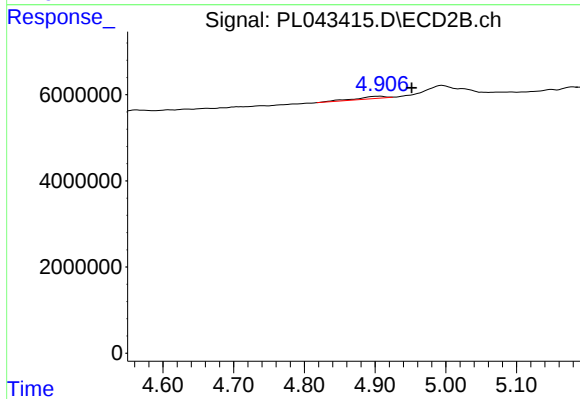

#6 beta-BHC


R.T.: 4.907 min
Delta R.T.: -0.045 min
Response: 1713125
Conc: 1.01 ng/ml

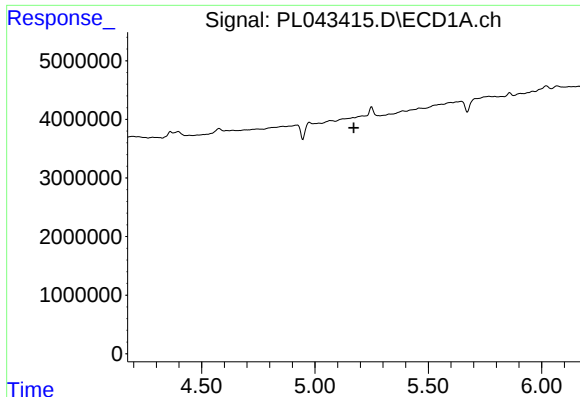

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.171 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

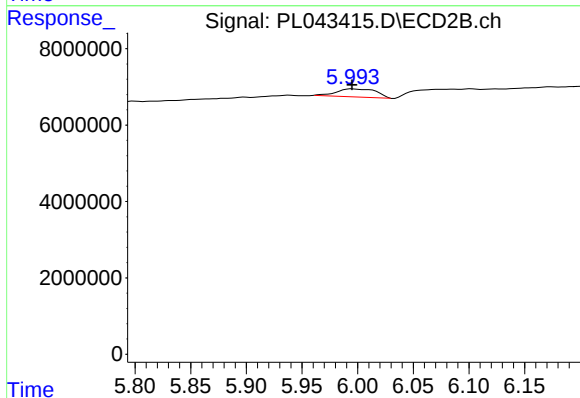


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 5087056
Conc: 1.34 ng/ml

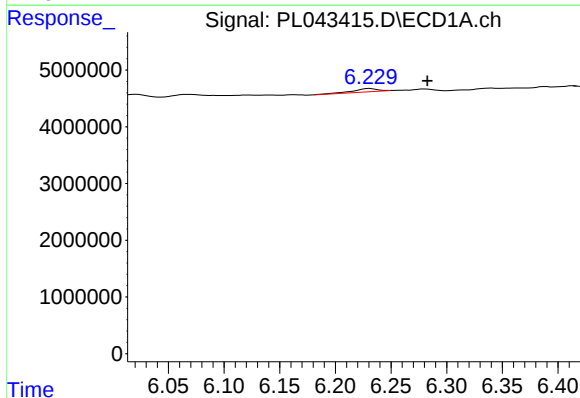


#15 Endosulfan II

R.T.: 6.231 min
Delta R.T.: -0.052 min
Response: 988964
Conc: 0.15 ng/ml

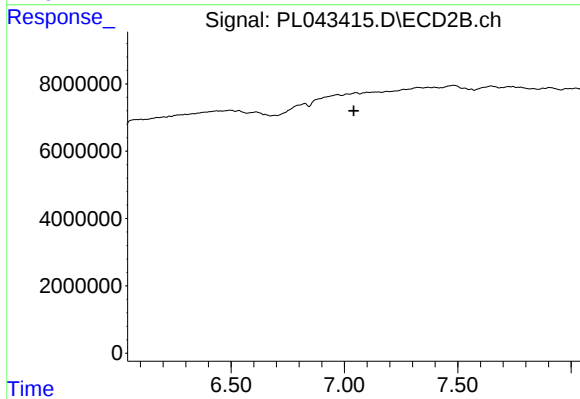

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

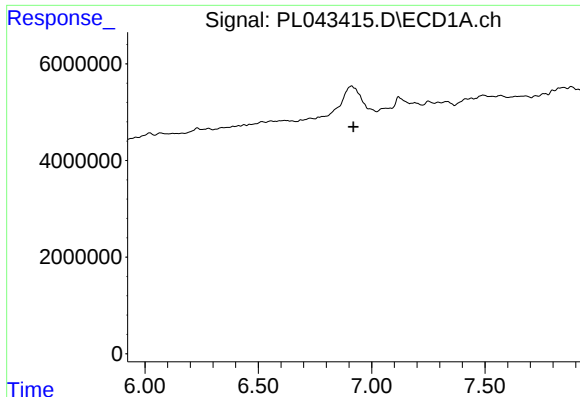

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

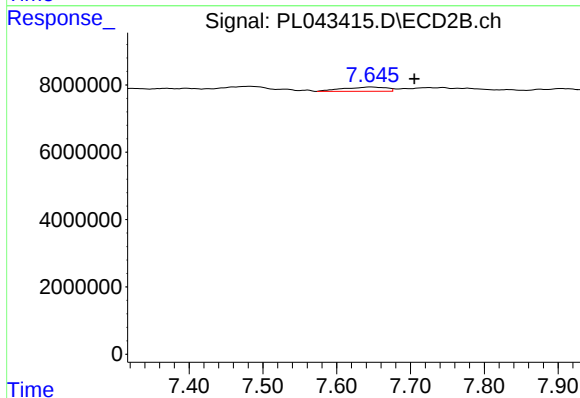


#20 Methoxychlor

R.T.: 7.646 min
Delta R.T.: -0.059 min
Response: 5106572
Conc: 3.39 ng/ml

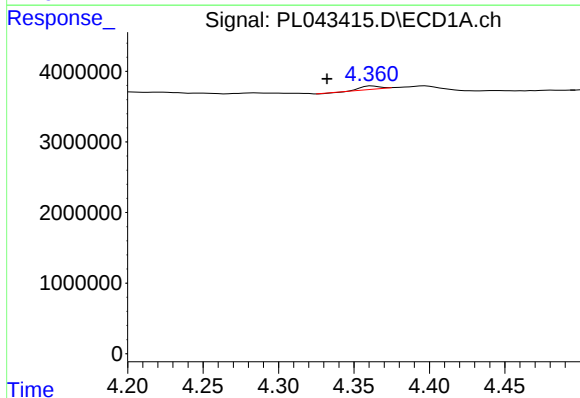


#23 Chlordane-1

R.T.: 4.362 min
Delta R.T.: 0.030 min
Response: 327366
Conc: 1.22 ng/ml

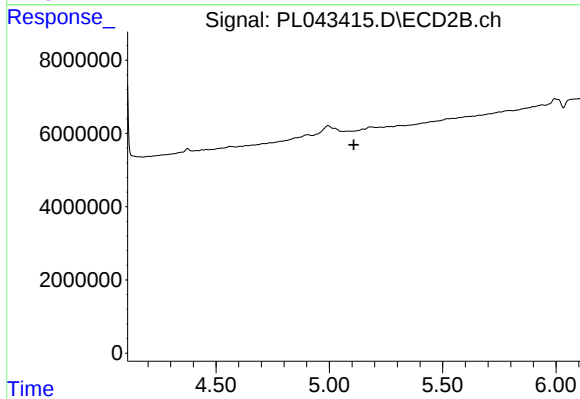

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

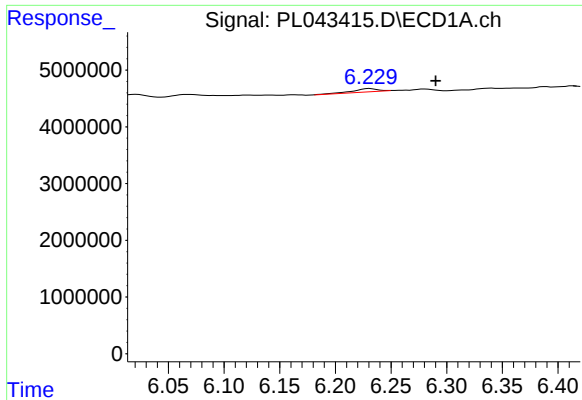

#27 Chlordane-5


R.T.: 6.231 min
Delta R.T.: -0.059 min
Response: 988964
Conc: 4.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

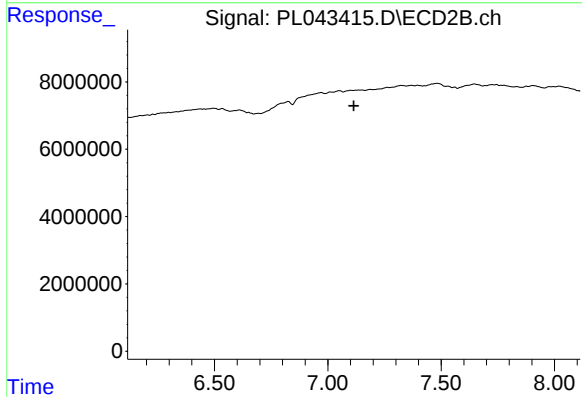


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.115 min
Response: 0
Conc: N.D.

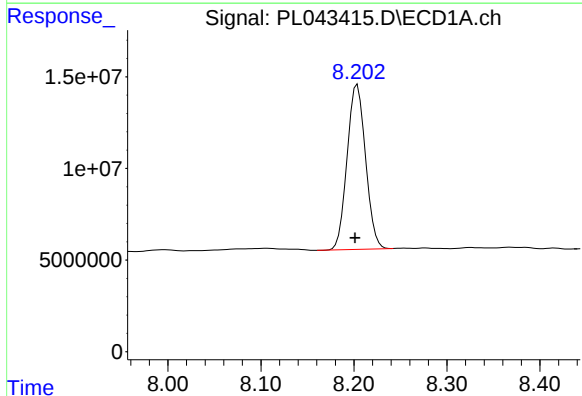

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: 0.002 min
Response: 123848884
Conc: 18.97 ng/ml

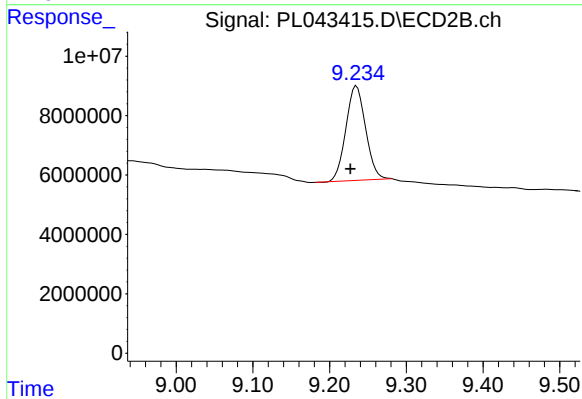

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.008 min
Response: 57060536
Conc: 21.87 ng/ml