

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 15:32
 Operator : AJ\SJ
 Sample : PB115916TB
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 08:15:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.102	140.0E6	70578890	22.833	23.813
28)	SA Decachlor...	8.202	9.234	138.6E6	61982858	21.218	23.762
Target Compounds							
6)	B beta-BHC	4.396f	4.903f	2079220	1490678	0.564	0.881 #
7)	B delta-BHC	0.000	5.174	0	2973195	N.D.	0.692 #
8)	B Heptachlo...	0.000	5.991	0	33234461	N.D.	8.764 #
14)	MA Endrin	6.018	6.771f	10958333	786606	1.522	0.252 #
17)	MA 4,4'-DDT	0.000	7.315f	0	1878528	N.D.	0.640 #
19)	B Endosulfa...	0.000	7.340f	0	862520	N.D.	0.287 #
20)	A Methoxychlor	0.000	7.642f	0	60965113	N.D.	40.419 #
23)	Chlordane-1	4.361	5.174	1327027	2973195	4.939	21.037 #
24)	Chlordane-2	0.000	5.514	0	6539093	N.D.	45.587 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 15:32
Operator : AJ\SJ
Sample : PB115916TB
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 08:15:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

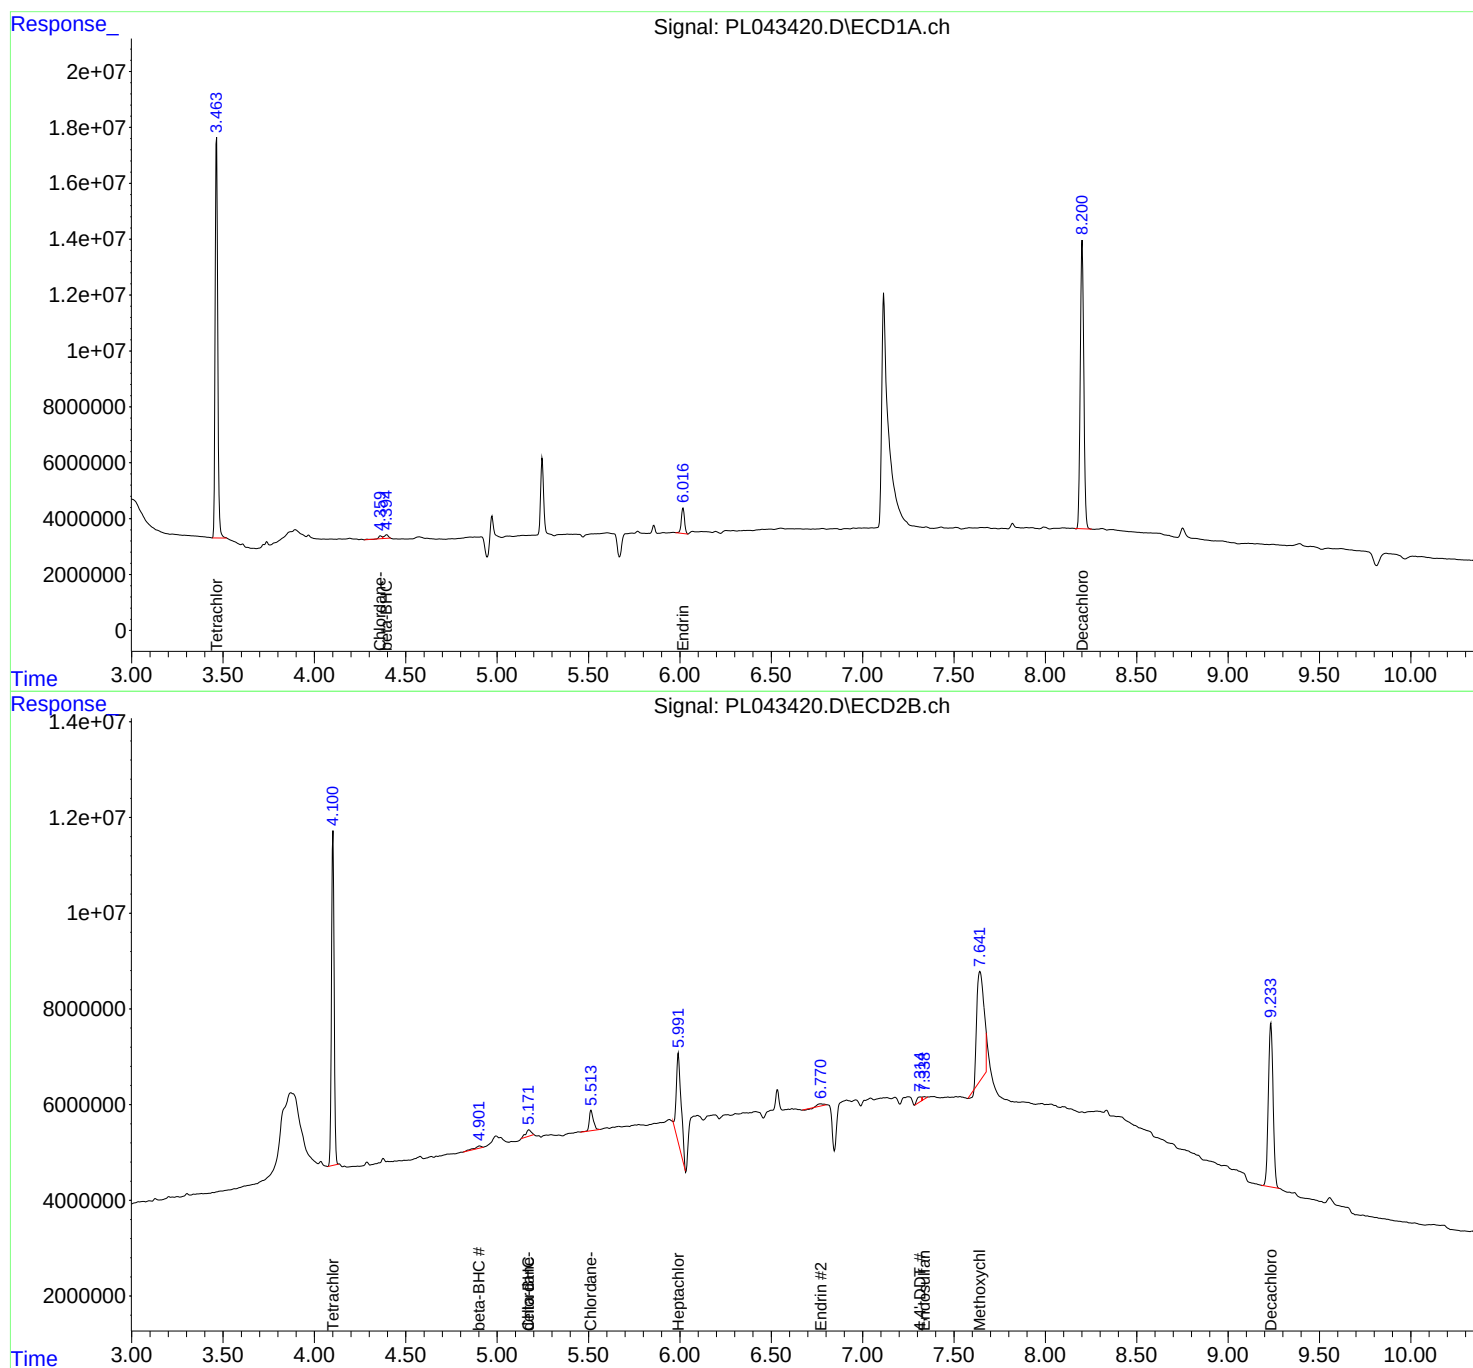


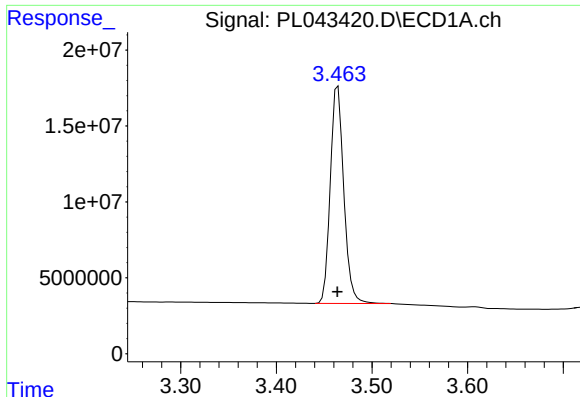

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 140035285
Conc: 22.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

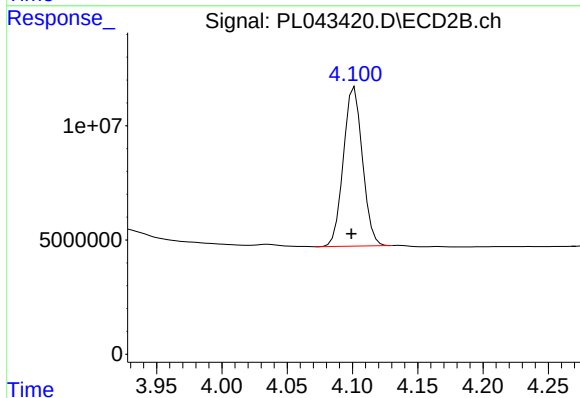


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.003 min
Response: 70578890
Conc: 23.81 ng/ml

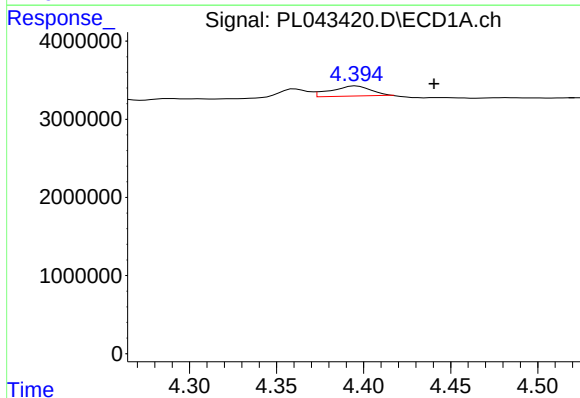


#6 beta-BHC

R.T.: 4.396 min
Delta R.T.: -0.045 min
Response: 2079220
Conc: 0.56 ng/ml

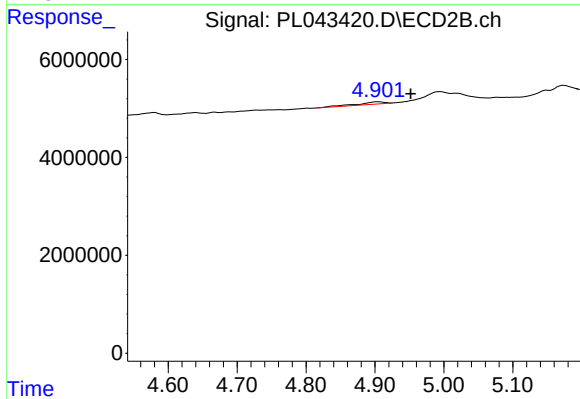

#6 beta-BHC


R.T.: 4.903 min
Delta R.T.: -0.048 min
Response: 1490678
Conc: 0.88 ng/ml

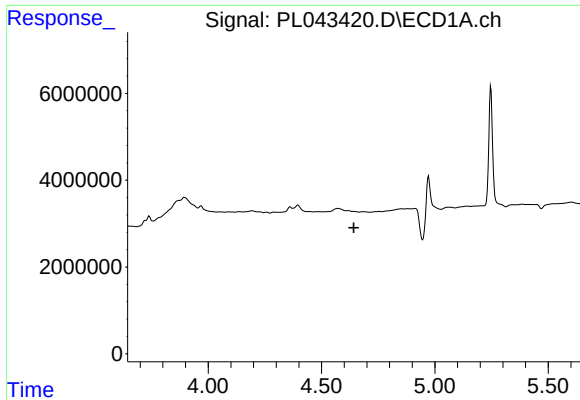

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

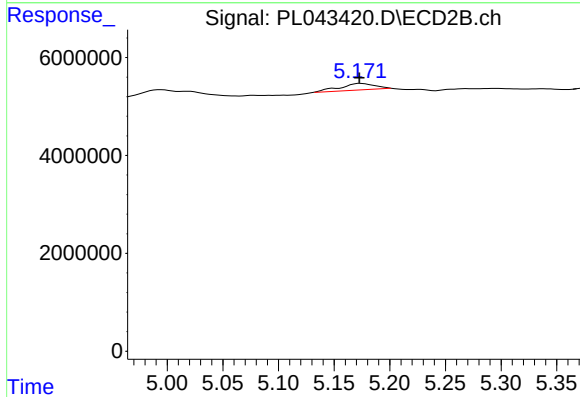


#7 delta-BHC

R.T.: 5.174 min
Delta R.T.: 0.001 min
Response: 2973195
Conc: 0.69 ng/ml

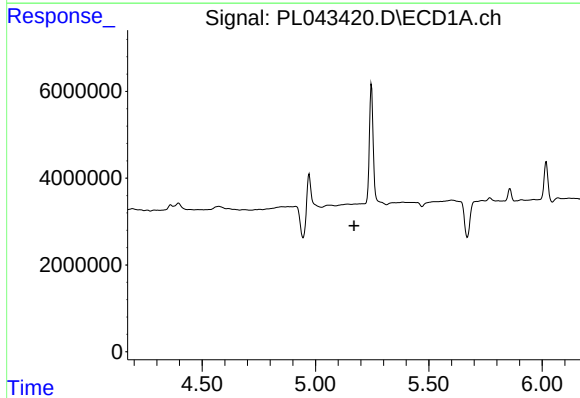


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

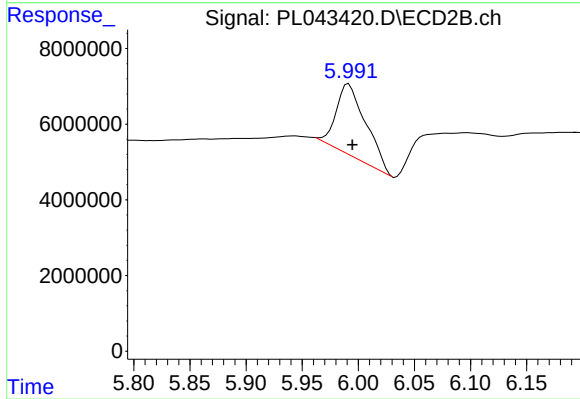

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.003 min
Response: 33234461
Conc: 8.76 ng/ml

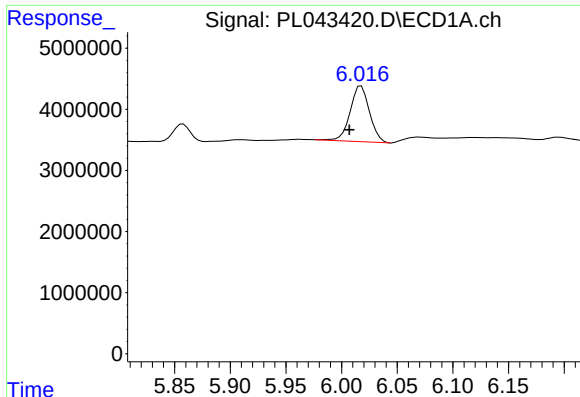

#14 Endrin


R.T.: 6.018 min
Delta R.T.: 0.011 min
Response: 10958333
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

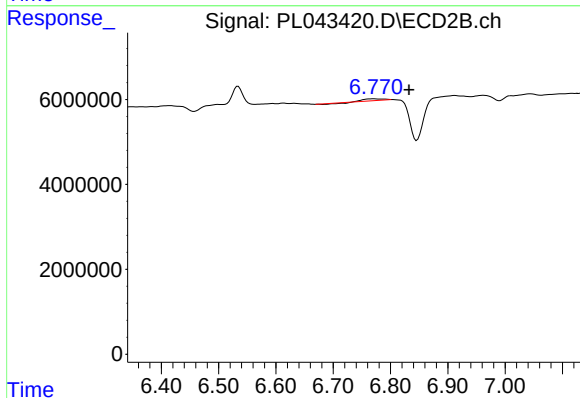


#14 Endrin

R.T.: 6.771 min
Delta R.T.: -0.061 min
Response: 786606
Conc: 0.25 ng/ml

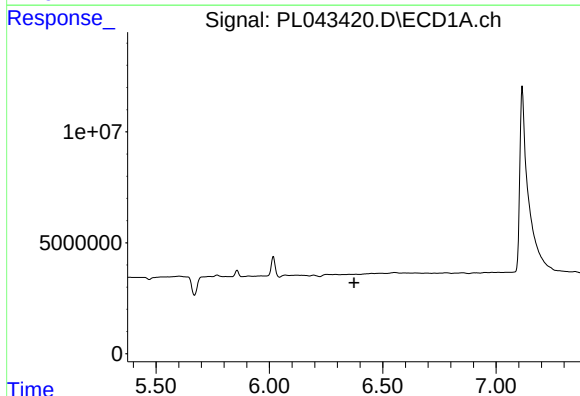


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.374 min
Response: 0
Conc: N.D.

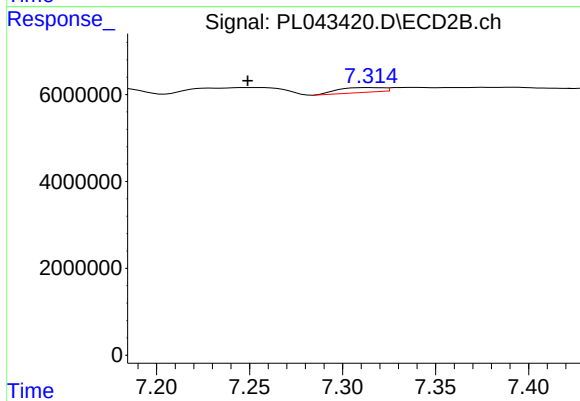

#17 4,4'-DDT


R.T.: 7.315 min
Delta R.T.: 0.066 min
Response: 1878528
Conc: 0.64 ng/ml

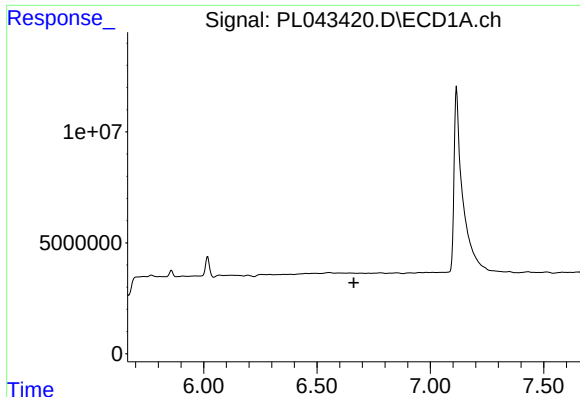

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

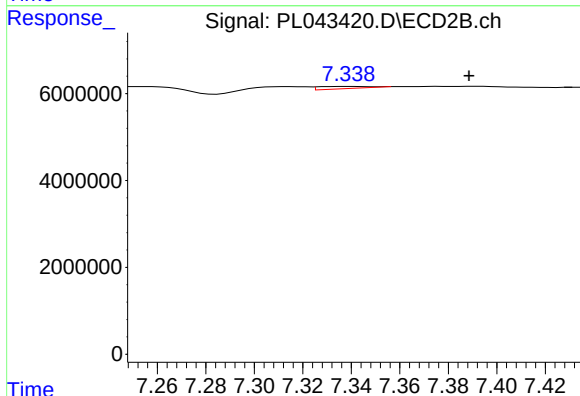


#19 Endosulfan Sulfate

R.T.: 7.340 min
Delta R.T.: -0.049 min
Response: 862520
Conc: 0.29 ng/ml

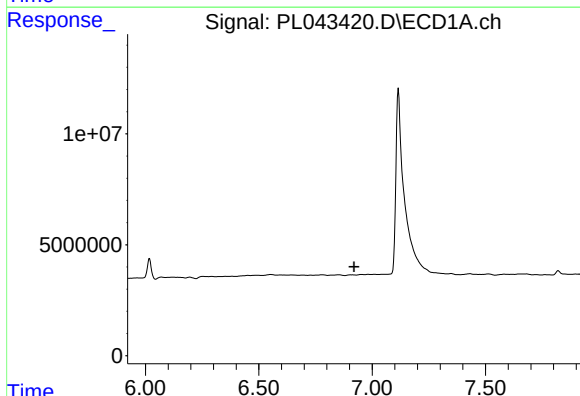


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.920 min
Response: 0
Conc: N.D.

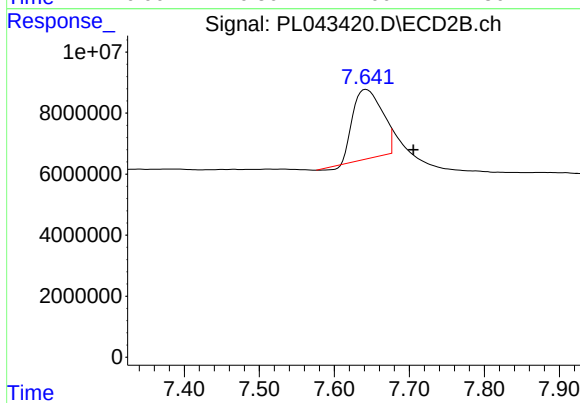

#20 Methoxychlor


R.T.: 7.642 min
Delta R.T.: -0.063 min
Response: 60965113
Conc: 40.42 ng/ml

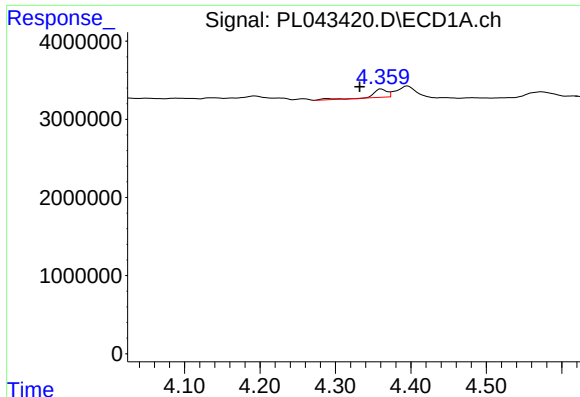

#23 Chlordane-1


R.T.: 4.361 min
Delta R.T.: 0.029 min
Response: 1327027
Conc: 4.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

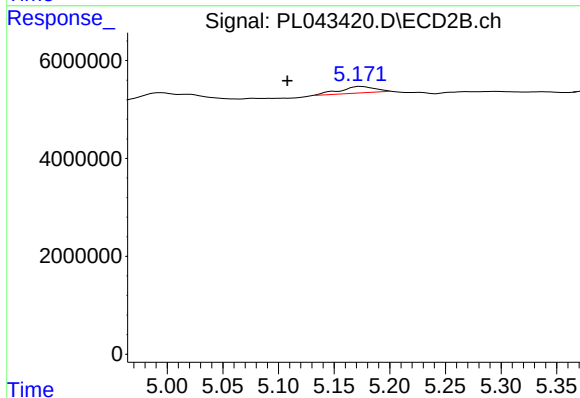


#23 Chlordane-1

R.T.: 5.174 min
Delta R.T.: 0.066 min
Response: 2973195
Conc: 21.04 ng/ml

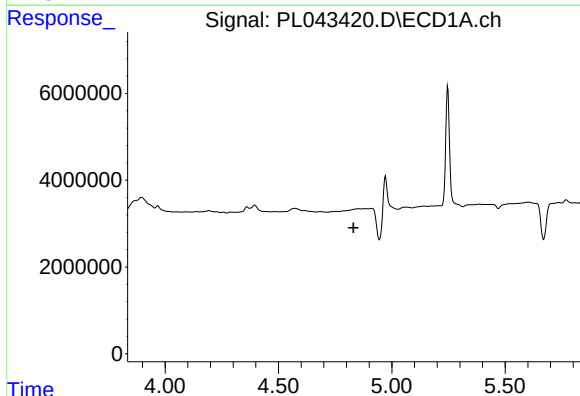


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

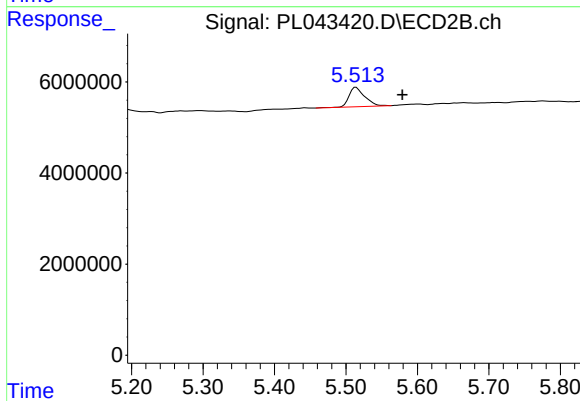

#24 Chlordane-2

R.T.: 5.514 min
Delta R.T.: -0.065 min
Response: 6539093
Conc: 45.59 ng/ml

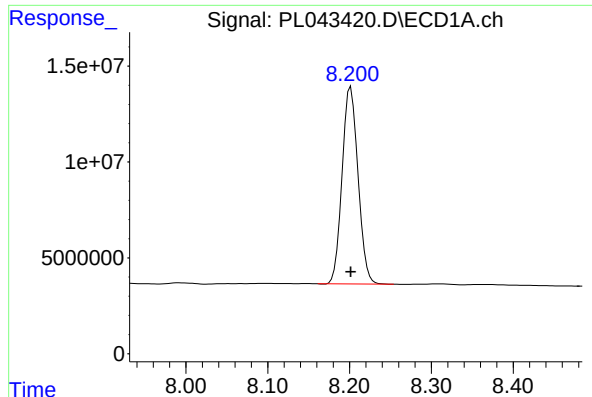

#28 Decachlorobiphenyl


R.T.: 8.202 min

Delta R.T.: 0.000 min

Response: 138556180

Conc: 21.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

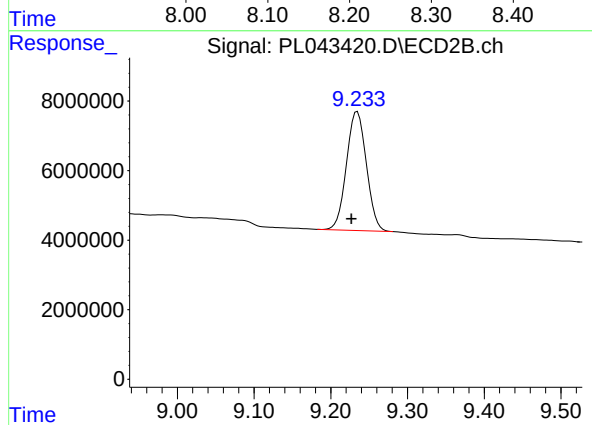

#28 Decachlorobiphenyl

R.T.: 9.234 min

Delta R.T.: 0.008 min

Response: 61982858

Conc: 23.76 ng/ml