

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
 Data File : PL043421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2018 15:46
 Operator : AJ\SJ
 Sample : J6498-07
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 08:15:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 07 00:20:08 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.102	141.5E6	72460431	23.068	24.448
28)	SA Decachlor...	8.202	9.234	127.3E6	57454483	19.494	22.026
Target Compounds							
6)	B beta-BHC	4.398f	0.000	8948982	0	2.426	N.D. #
7)	B delta-BHC	0.000	5.169	0	4241322	N.D.	0.987 #
8)	B Heptachlo...	0.000	5.993	0	35346683	N.D.	9.321 #
9)	A Endosulfan I	5.532	0.000	2925859	0	0.399	N.D. #
13)	MA Dieldrin	5.705f	0.000	5871710	0	0.755	N.D. #
14)	MA Endrin	6.018	6.773f	15867600	2741034	2.204	0.878 #
19)	B Endosulfa...	0.000	7.342f	0	279271	N.D.	0.093 #
20)	A Methoxychlor	0.000	7.643f	0	45106980	N.D.	29.905 #
23)	Chlordane-1	4.398	5.150	8948982	3122007	33.304	22.090 #
24)	Chlordane-2	0.000	5.514	0	5846403	N.D.	40.758 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122118\
Data File : PL043421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2018 15:46
Operator : AJ\SJ
Sample : J6498-07
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 08:15:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL120618.M
Quant Title : GC Extractables
QLast Update : Fri Dec 07 00:20:08 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

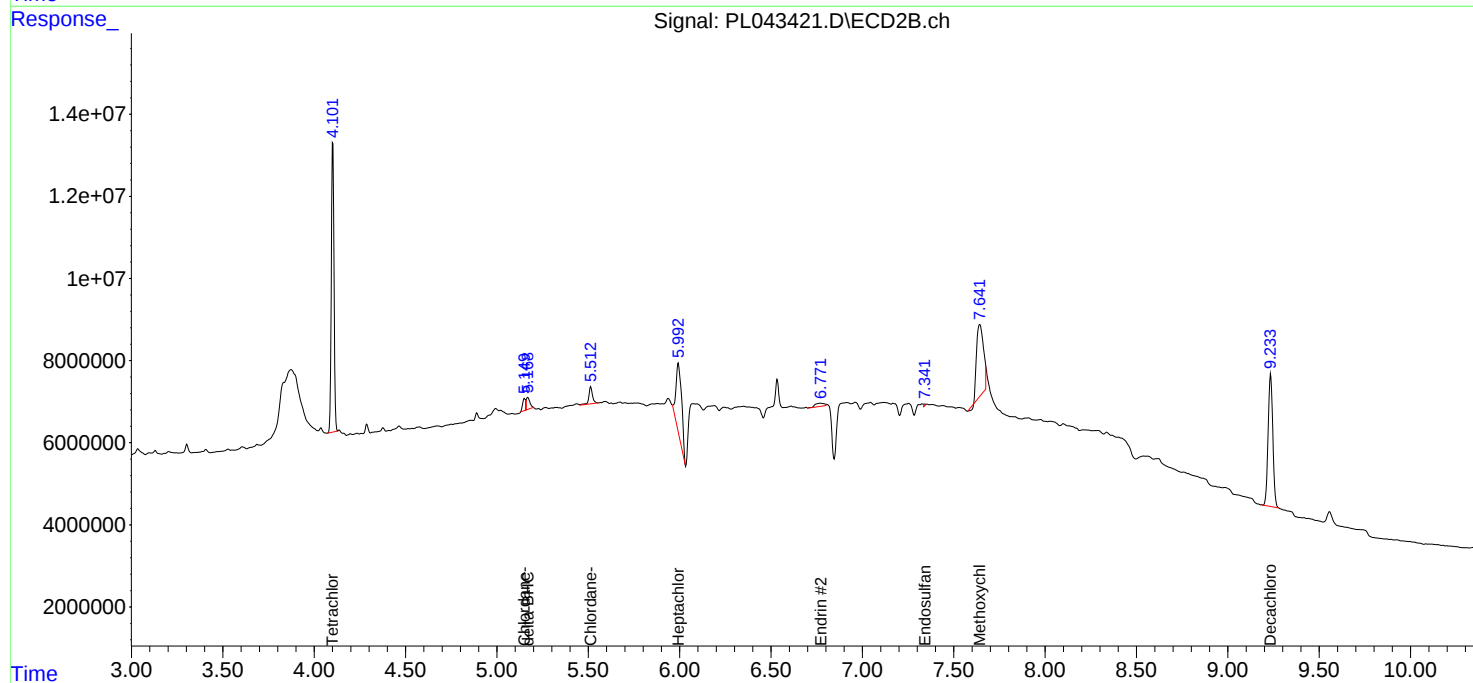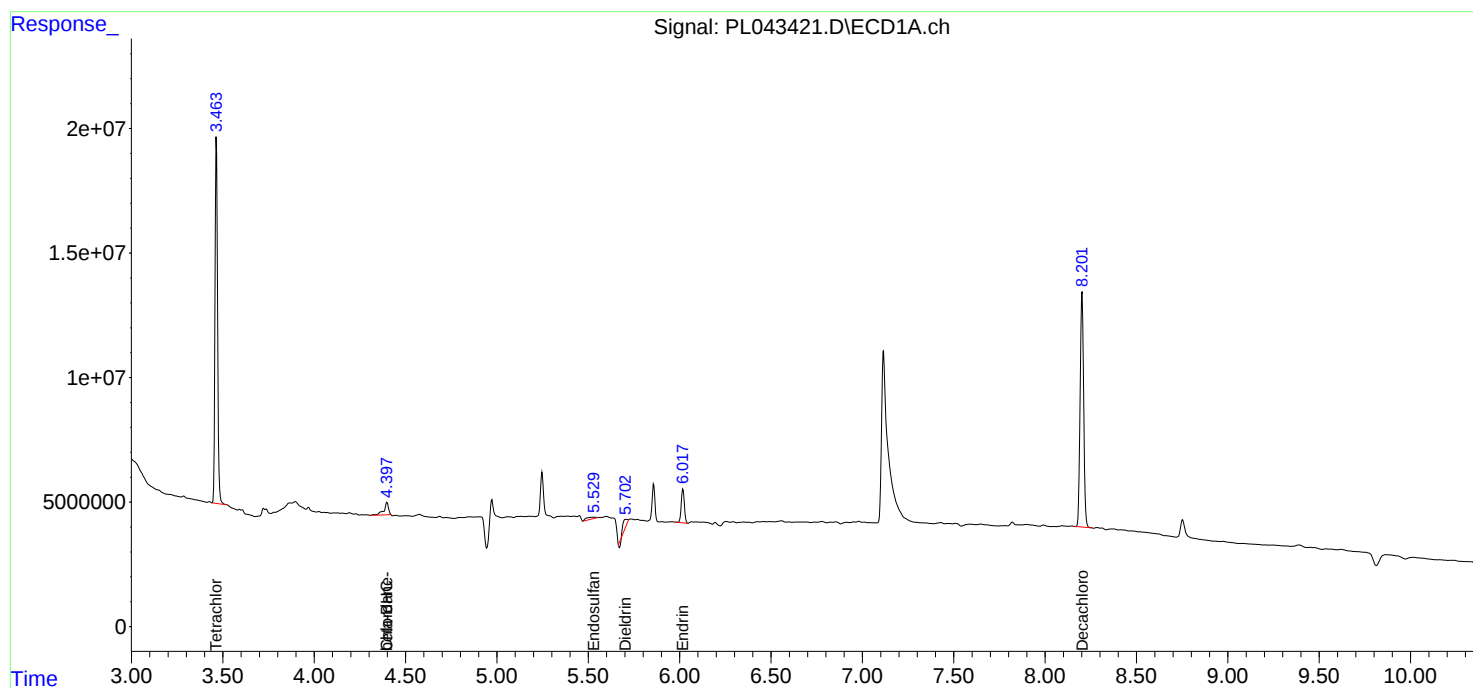


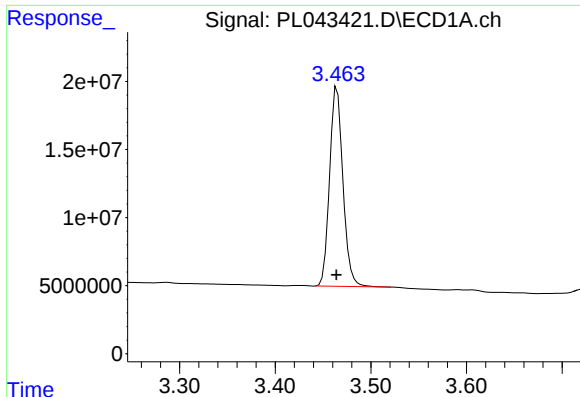

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 141475276
Conc: 23.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

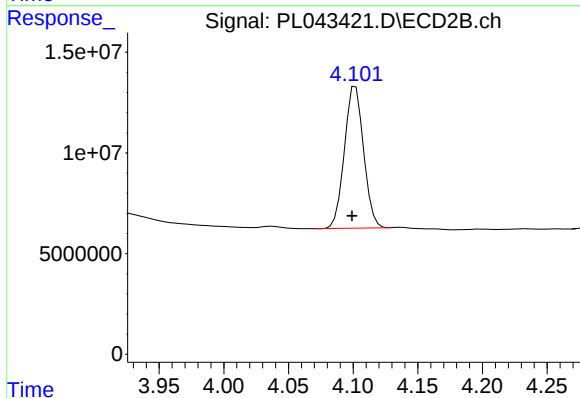


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.003 min
Response: 72460431
Conc: 24.45 ng/ml

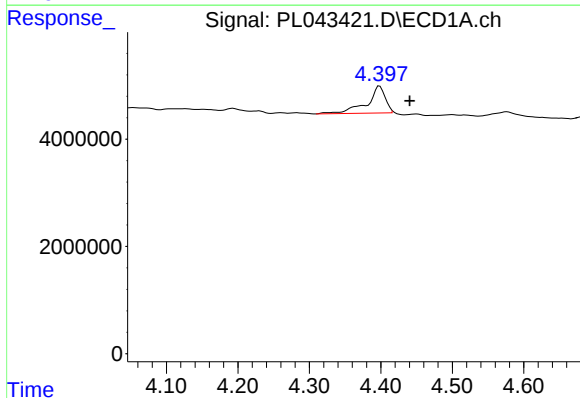


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: -0.042 min
Response: 8948982
Conc: 2.43 ng/ml

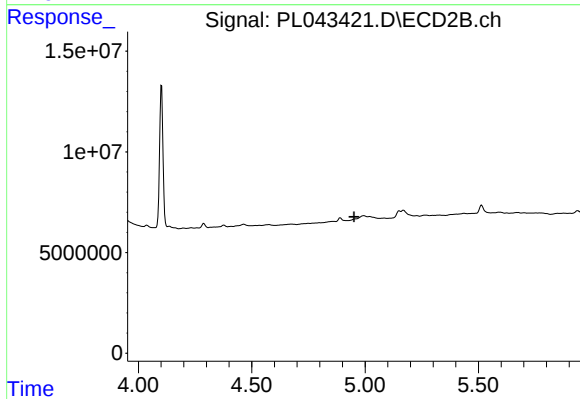

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

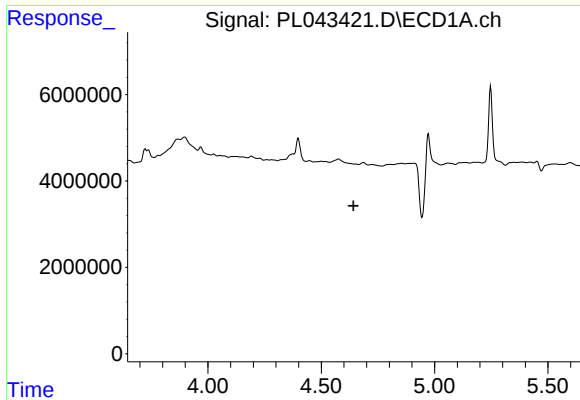

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

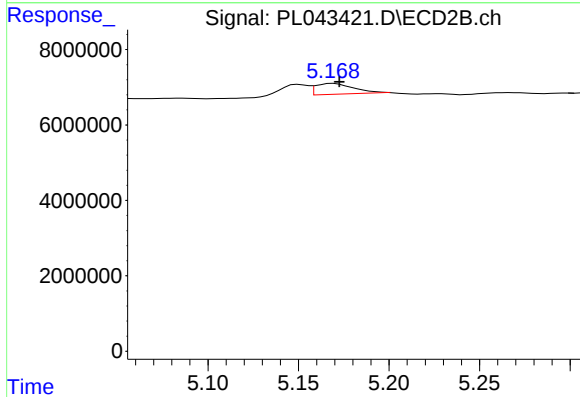


#7 delta-BHC

R.T.: 5.169 min
Delta R.T.: -0.004 min
Response: 4241322
Conc: 0.99 ng/ml

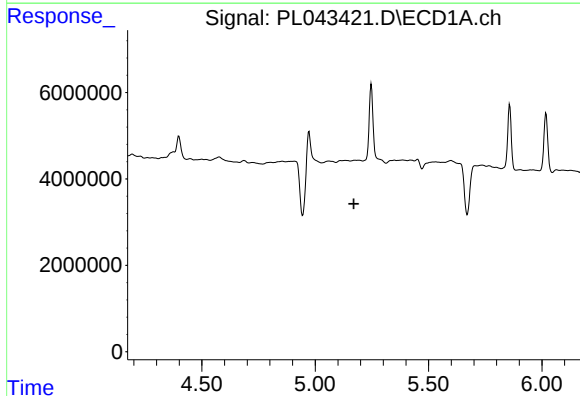


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.171 min
Response: 0
Conc: N.D.

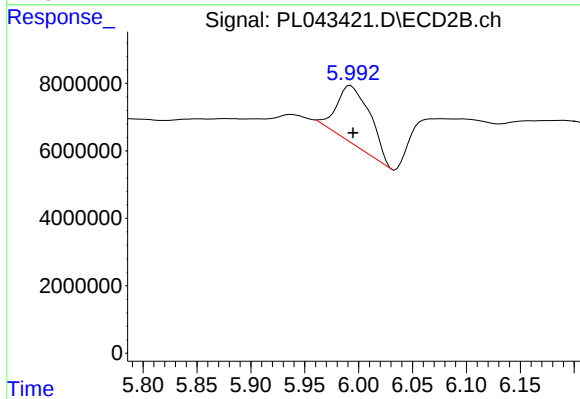

#8 Heptachlor epoxide


R.T.: 5.993 min
Delta R.T.: -0.002 min
Response: 35346683
Conc: 9.32 ng/ml

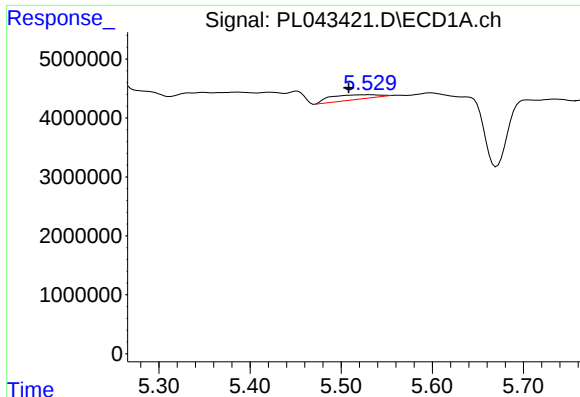

#9 Endosulfan I


R.T.: 5.532 min
Delta R.T.: 0.024 min
Response: 2925859
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

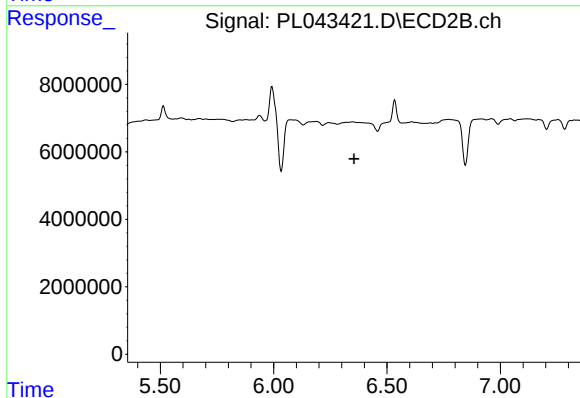


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

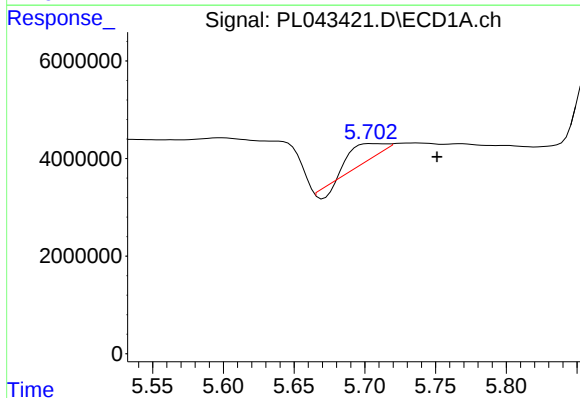


#13 Dieldrin

R.T.: 5.705 min
Delta R.T.: -0.046 min
Response: 5871710
Conc: 0.76 ng/ml

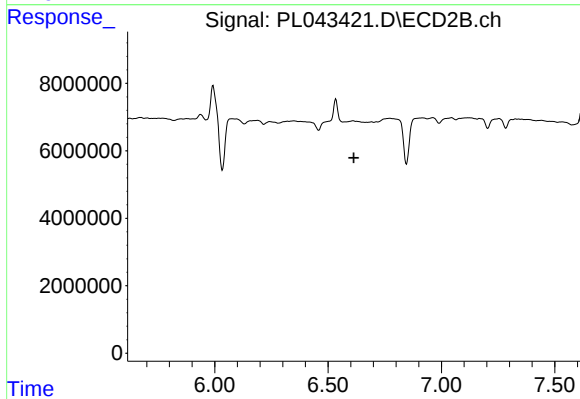

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.613 min
Response: 0
Conc: N.D.

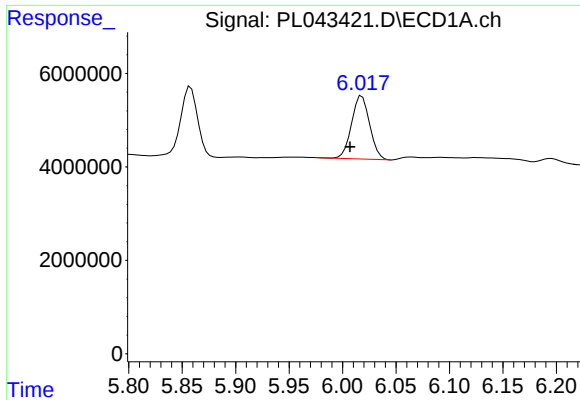

#14 Endrin


R.T.: 6.018 min
Delta R.T.: 0.011 min
Response: 15867600
Conc: 2.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

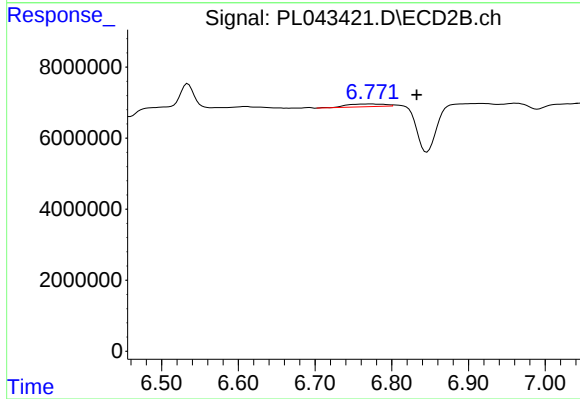


#14 Endrin

R.T.: 6.773 min
Delta R.T.: -0.060 min
Response: 2741034
Conc: 0.88 ng/ml

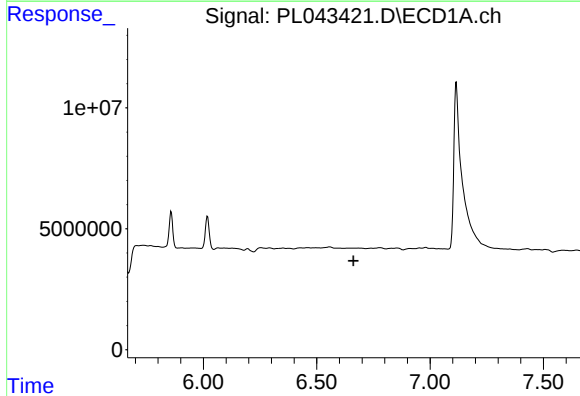


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.663 min
Response: 0
Conc: N.D.

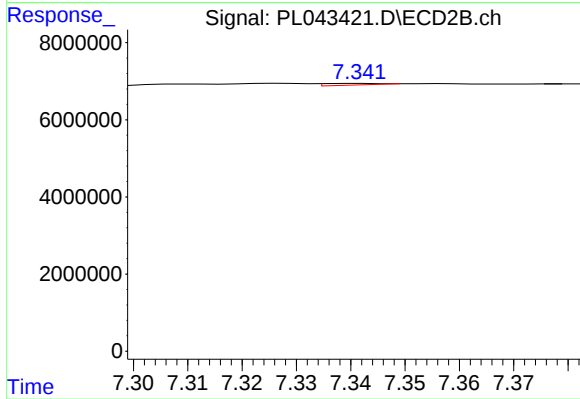

#19 Endosulfan Sulfate


R.T.: 7.342 min
Delta R.T.: -0.046 min
Response: 279271
Conc: 0.09 ng/ml

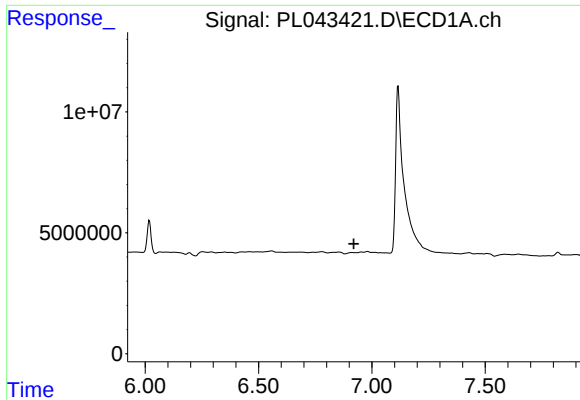

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

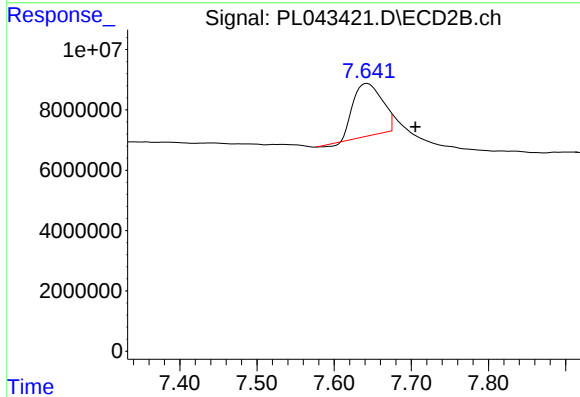


#20 Methoxychlor

R.T.: 7.643 min
Delta R.T.: -0.063 min
Response: 45106980
Conc: 29.91 ng/ml

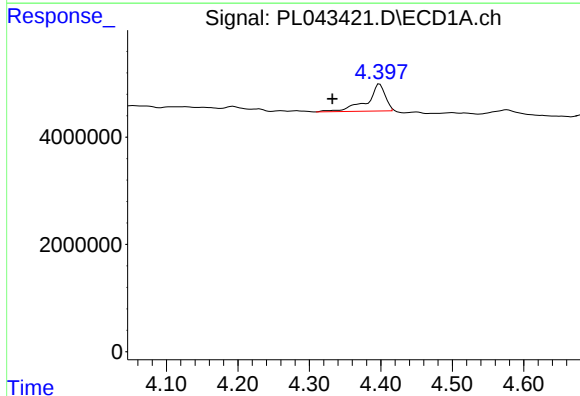


#23 Chlordane-1

R.T.: 4.398 min
Delta R.T.: 0.066 min
Response: 8948982
Conc: 33.30 ng/ml

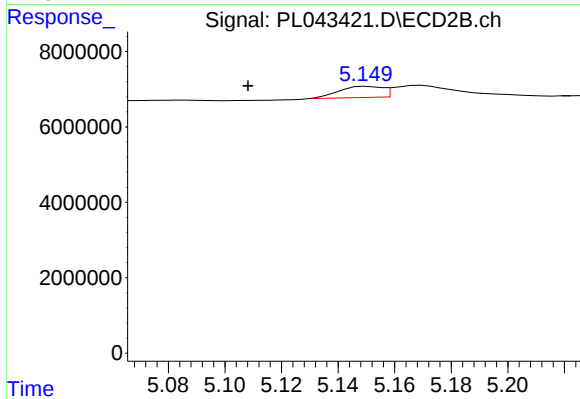

#23 Chlordane-1


R.T.: 5.150 min
Delta R.T.: 0.042 min
Response: 3122007
Conc: 22.09 ng/ml

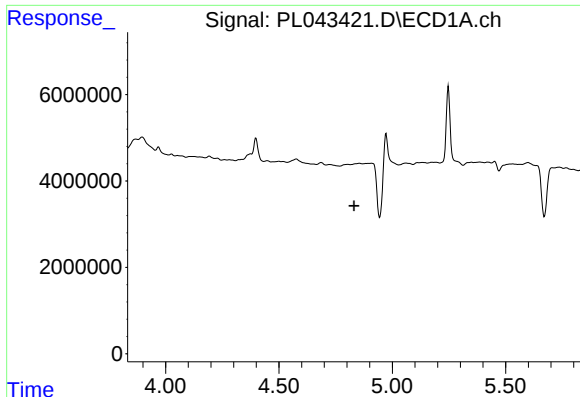

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.832 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

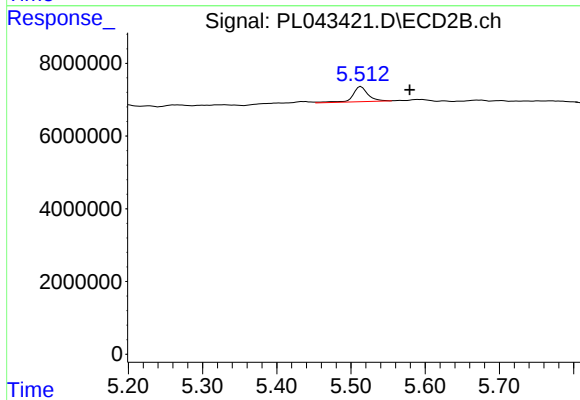


#24 Chlordane-2

R.T.: 5.514 min
Delta R.T.: -0.066 min
Response: 5846403
Conc: 40.76 ng/ml

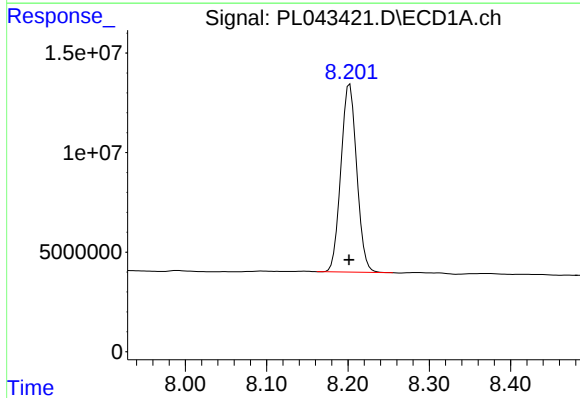

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: 0.001 min
Response: 127292877
Conc: 19.49 ng/ml

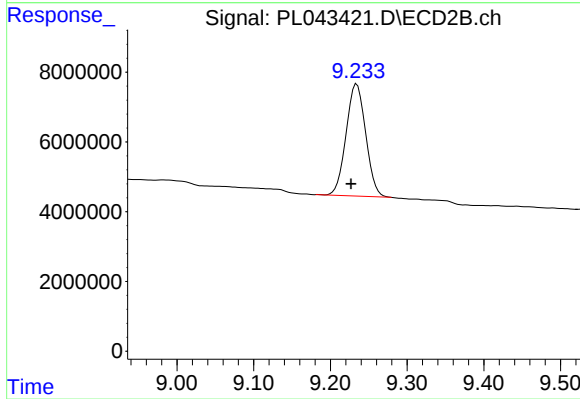

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.007 min
Response: 57454483
Conc: 22.03 ng/ml