

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122119\
 Data File : PL055140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 12:57
 Operator : SG\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 05:29:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.047	198.2E6	51685927	18.848	19.561
28)	SA Decachlor...	8.311	9.143	177.0E6	42840895	19.071	19.407
Target Compounds							
9)	A Endosulfan I	5.606	6.282	119.3E6	23912470	9.029	9.654
10)	B gamma-Chl...	5.493	6.159	132.5E6	26357645	9.093	9.931
12)	B 4,4'-DDE	5.714	6.389	254.0E6	46281295	19.064	18.981
13)	MA Dieldrin	5.850	6.540	263.2E6	48791742	18.851	19.119
19)	B Endosulfa...	6.763	7.317	168.0E6	38193281	16.706	18.287
20)	A Methoxychlor	7.017	7.640	464.1E6	98161803	96.307	90.952
21)	B Endrin ke...	7.257	7.790	186.7E6	41093773	17.812	18.453
25)	Chlordane-3	5.493	6.159	132.5E6	26357645	104.525	81.903



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122119\
Data File : PL055140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 12:57
Operator : SG\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 05:29:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

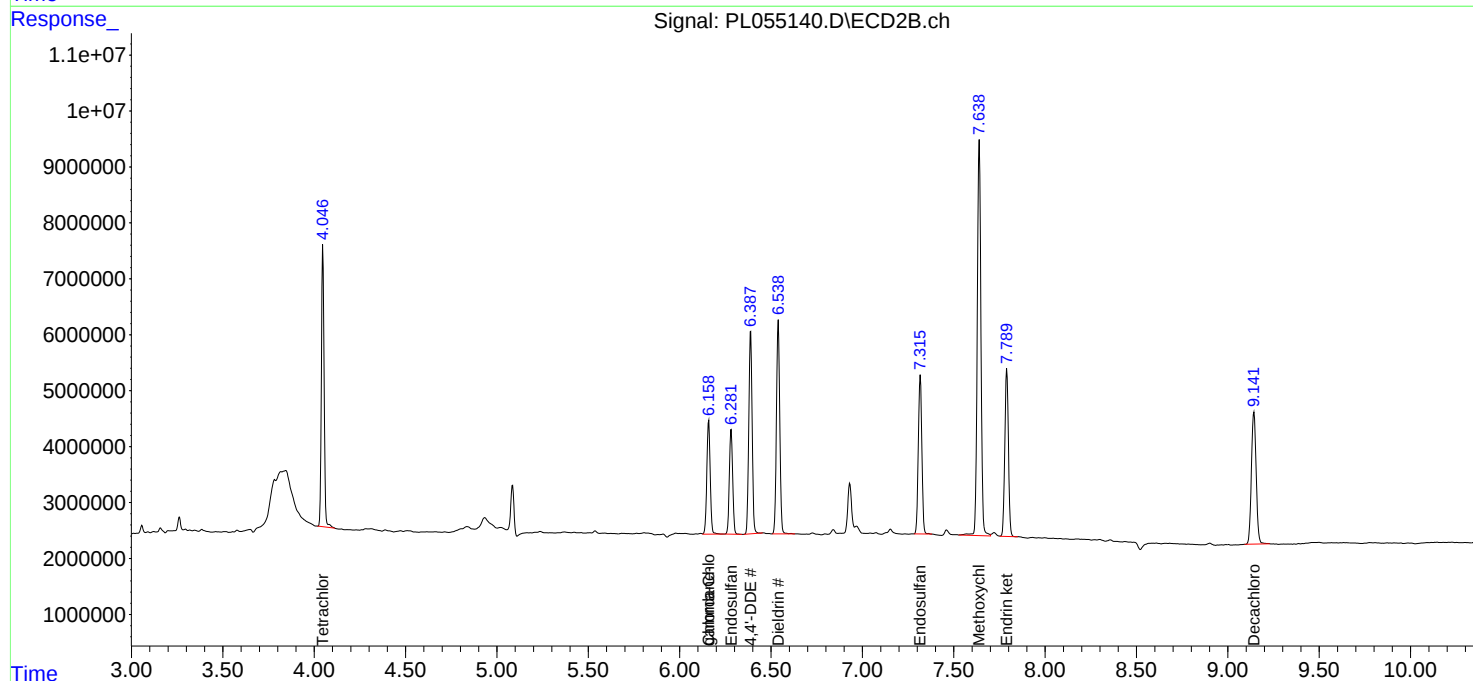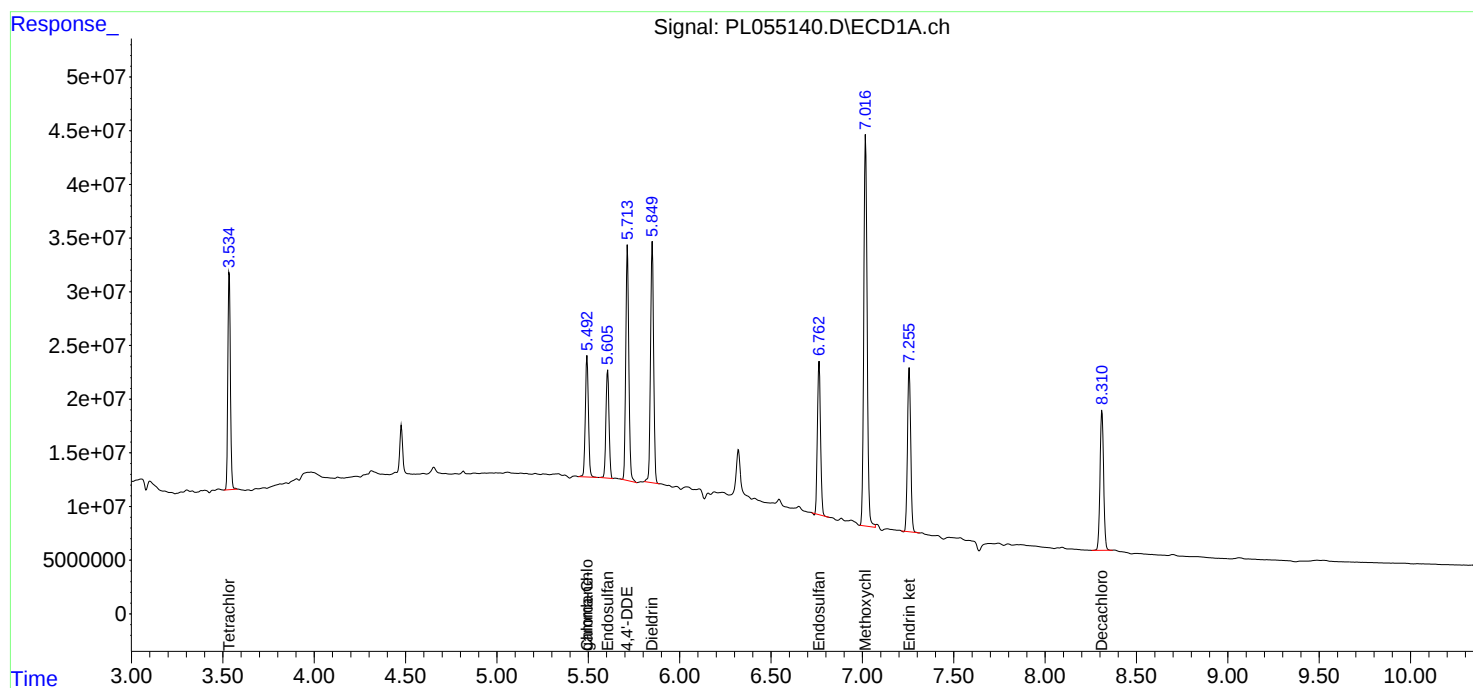


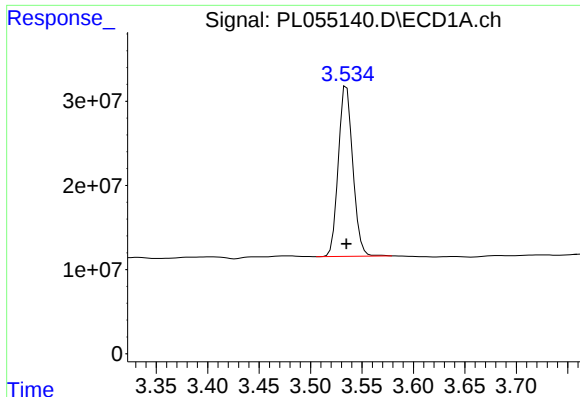

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 198214206
Conc: 18.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

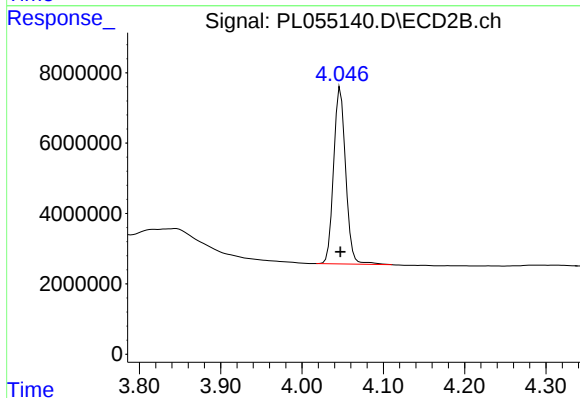


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 51685927
Conc: 19.56 ng/ml

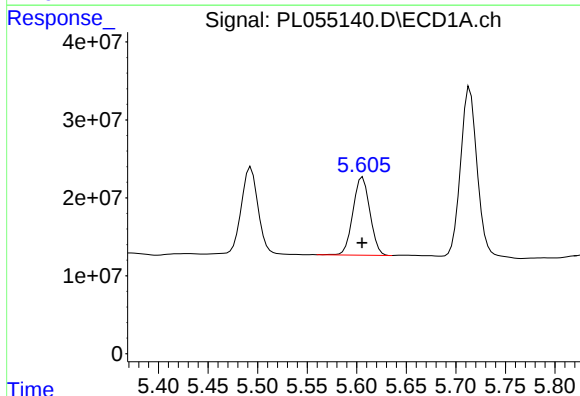


#9 Endosulfan I

R.T.: 5.606 min
Delta R.T.: 0.000 min
Response: 119301877
Conc: 9.03 ng/ml

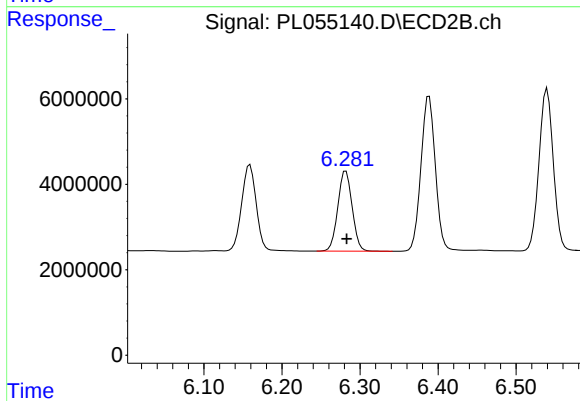

#9 Endosulfan I


R.T.: 6.282 min
Delta R.T.: 0.000 min
Response: 23912470
Conc: 9.65 ng/ml

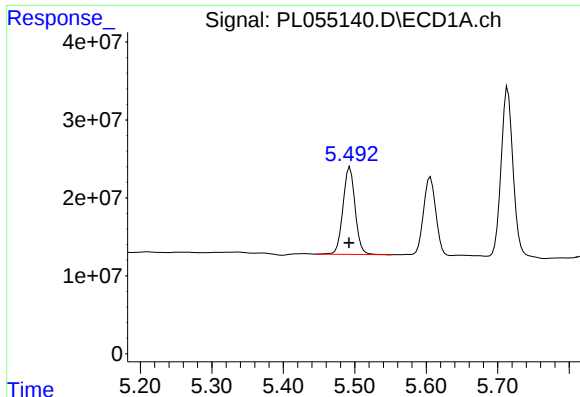

#10 gamma-Chlordane


R.T.: 5.493 min
Delta R.T.: 0.001 min
Response: 132481770
Conc: 9.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

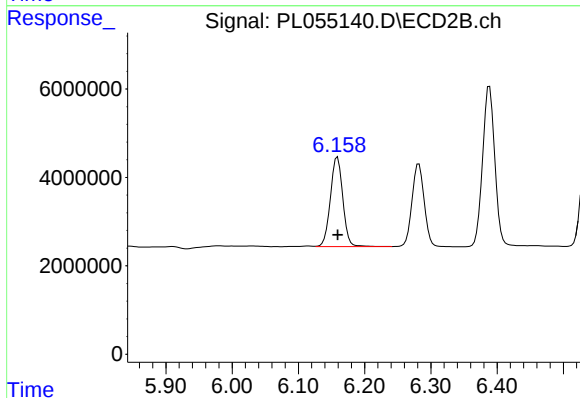


#10 gamma-Chlordane

R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 26357645
Conc: 9.93 ng/ml

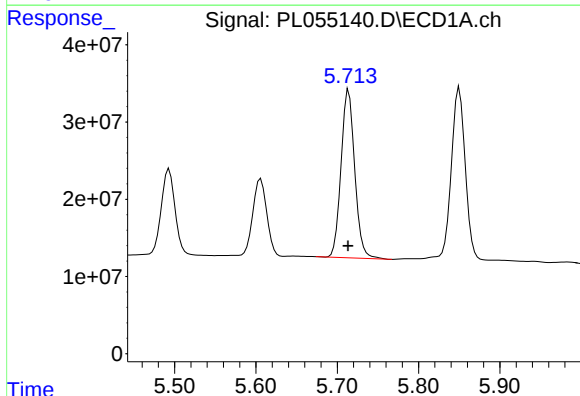


#12 4,4'-DDE

R.T.: 5.714 min
Delta R.T.: 0.000 min
Response: 254046488
Conc: 19.06 ng/ml

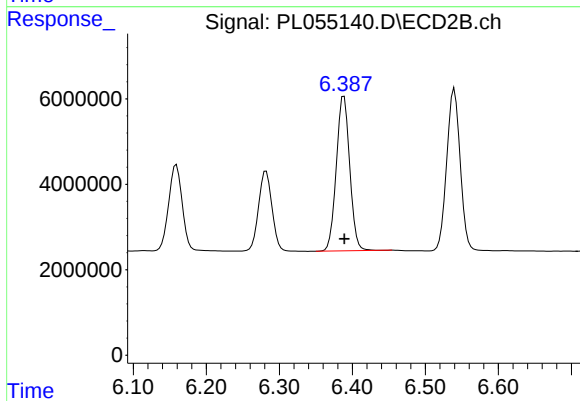

#12 4,4'-DDE


R.T.: 6.389 min
Delta R.T.: 0.000 min
Response: 46281295
Conc: 18.98 ng/ml

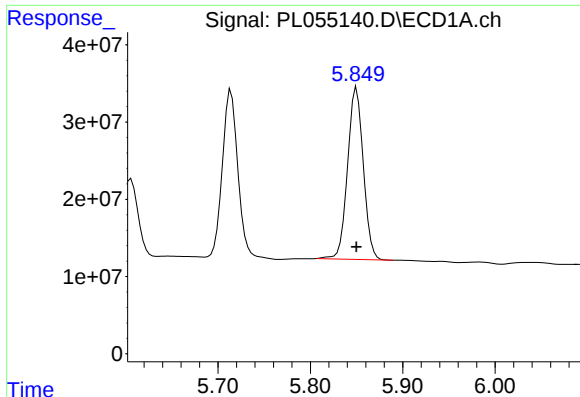

#13 Dieldrin


R.T.: 5.850 min
Delta R.T.: 0.000 min
Response: 263159238
Conc: 18.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

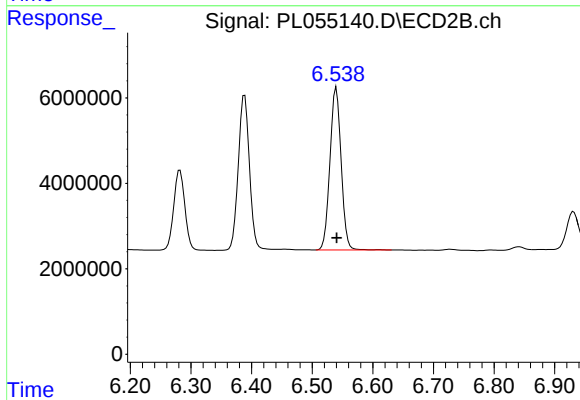


#13 Dieldrin

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 48791742
Conc: 19.12 ng/ml

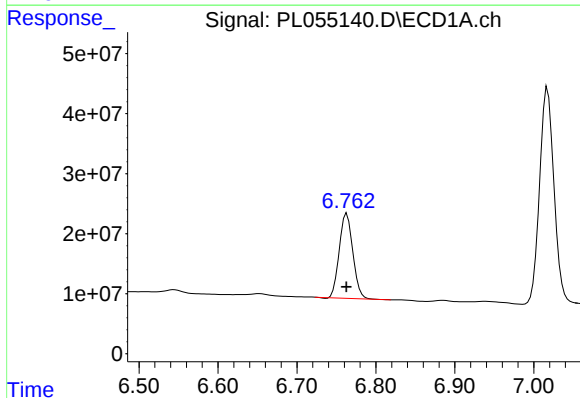


#19 Endosulfan Sulfate

R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 168046611
Conc: 16.71 ng/ml

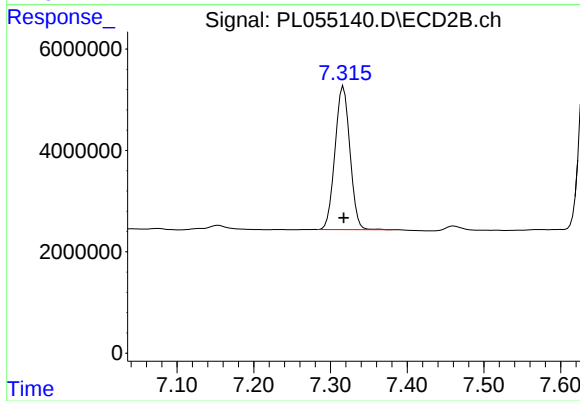

#19 Endosulfan Sulfate


R.T.: 7.317 min
Delta R.T.: 0.000 min
Response: 38193281
Conc: 18.29 ng/ml

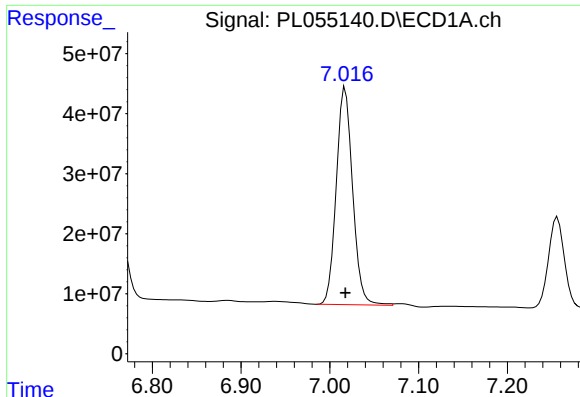

#20 Methoxychlor


R.T.: 7.017 min
Delta R.T.: 0.000 min
Response: 464143348
Conc: 96.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

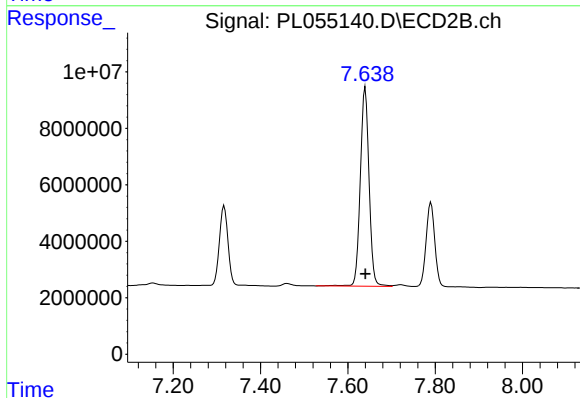


#20 Methoxychlor

R.T.: 7.640 min
Delta R.T.: 0.000 min
Response: 98161803
Conc: 90.95 ng/ml

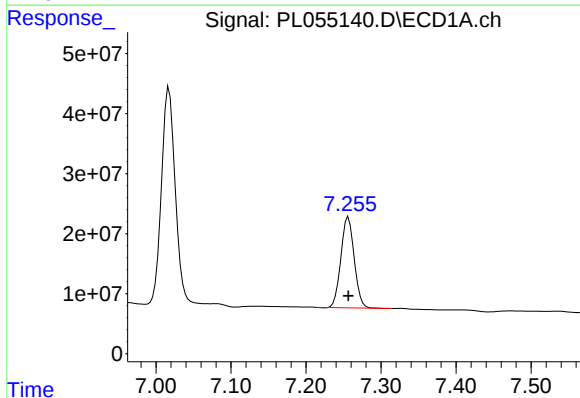


#21 Endrin ketone

R.T.: 7.257 min
Delta R.T.: 0.000 min
Response: 186702265
Conc: 17.81 ng/ml

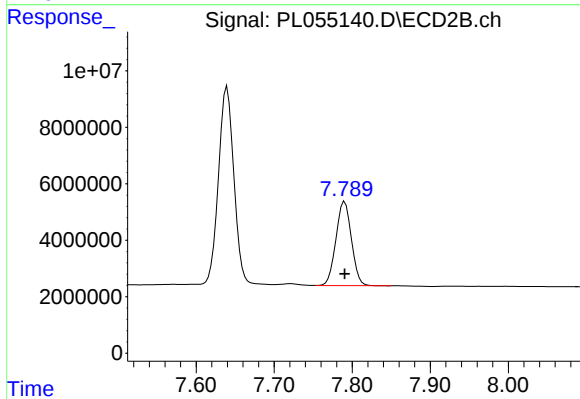

#21 Endrin ketone


R.T.: 7.790 min
Delta R.T.: 0.000 min
Response: 41093773
Conc: 18.45 ng/ml

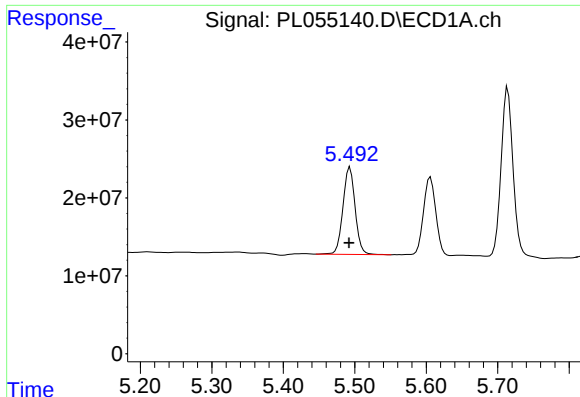

#25 Chlordane-3


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 132481770
Conc: 104.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

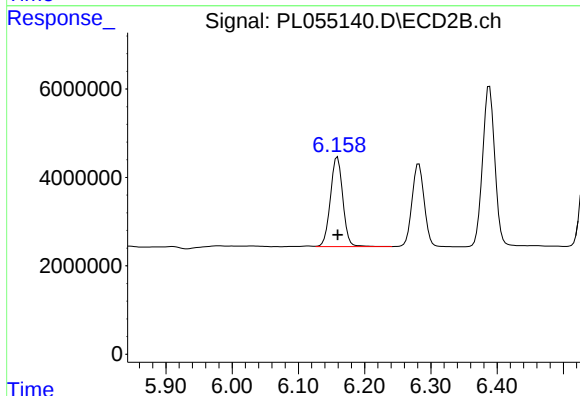


#25 Chlordane-3

R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 26357645
Conc: 81.90 ng/ml

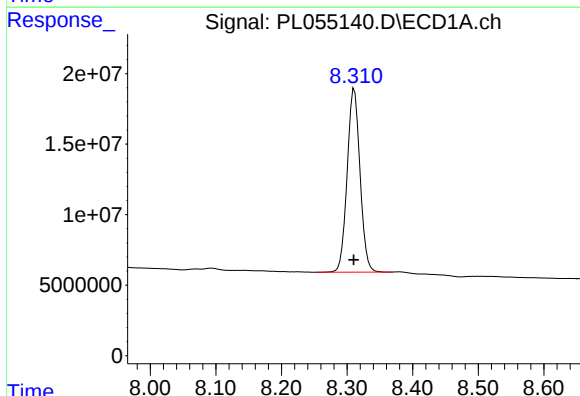

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 176951676
Conc: 19.07 ng/ml

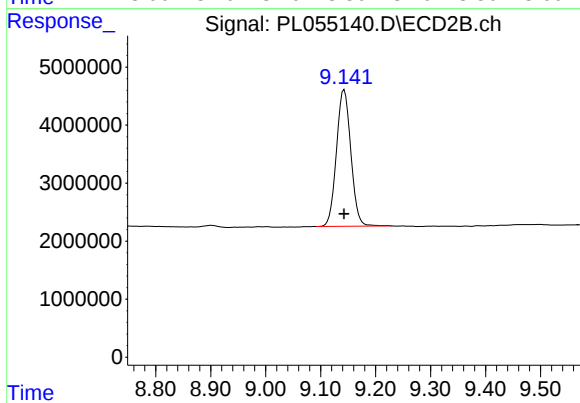

#28 Decachlorobiphenyl

R.T.: 9.143 min
Delta R.T.: 0.000 min
Response: 42840895
Conc: 19.41 ng/ml