

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122119\
 Data File : PL055146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 14:21
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 04:45:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 04:44:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	4.048	602.9E6	124.6E6	50.000	50.000
28)	SA Decachlor...	8.310	9.142	444.5E6	103.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.415	5.044	190.2E6	43949824	500.000	500.000
24)	Chlordane-2	4.919	5.512	211.8E6	47594587	500.000	500.000
25)	Chlordane-3	5.492	6.160	633.7E6	160.9E6	500.000	500.000
26)	Chlordane-4	5.551	6.233	523.4E6	192.2E6	500.000	500.000
27)	Chlordane-5	6.391	7.041	194.8E6	34886798	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122119\
Data File : PL055146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 14:21
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 04:45:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 04:44:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

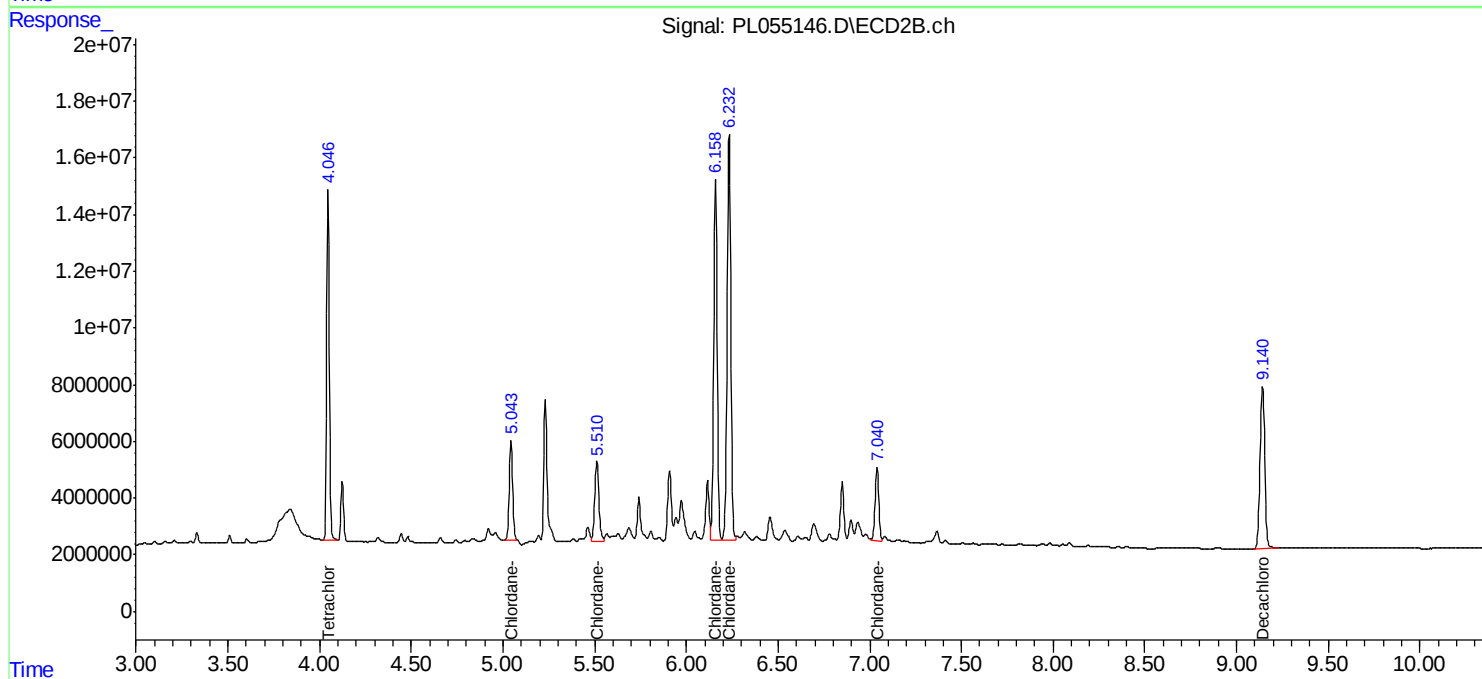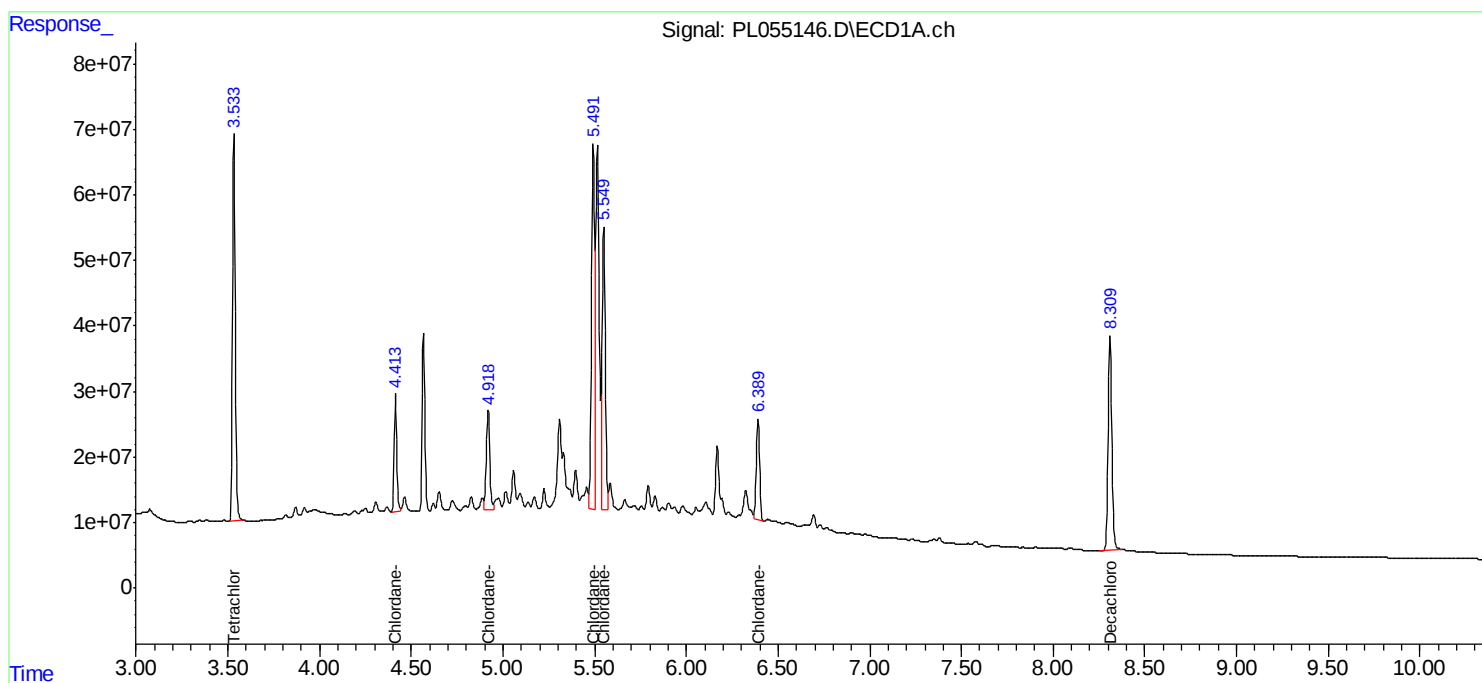


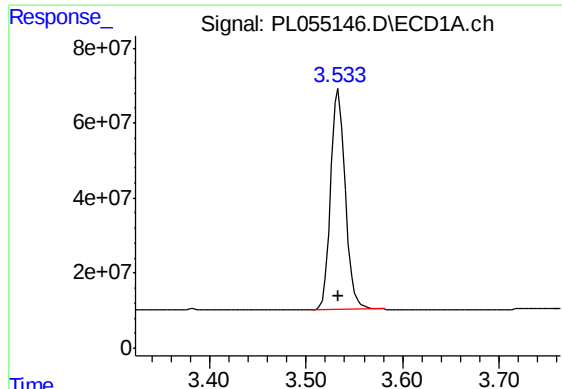

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 602850213
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

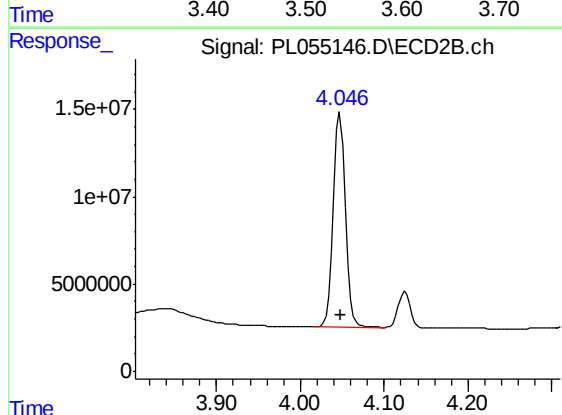


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 124592127
Conc: 50.00 ng/ml

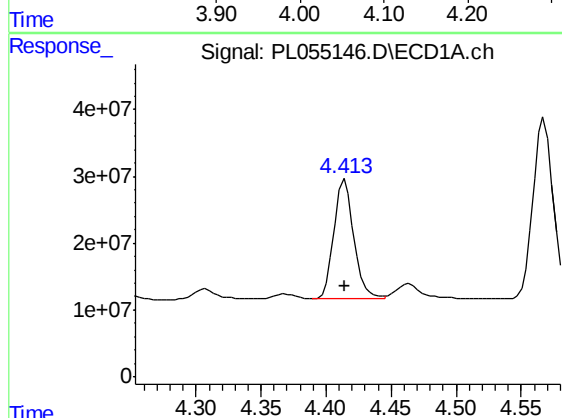


#23 Chlordane-1

R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 190192058
Conc: 500.00 ng/ml

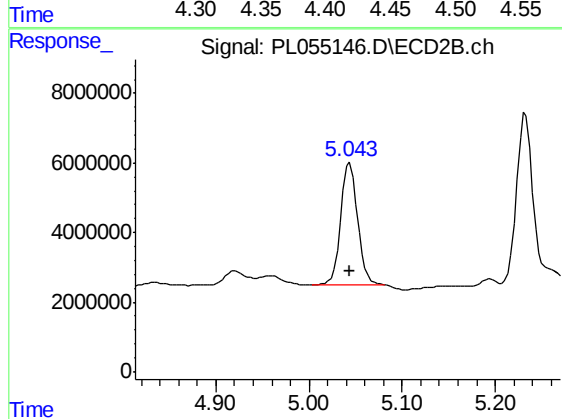

#23 Chlordane-1


R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 43949824
Conc: 500.00 ng/ml

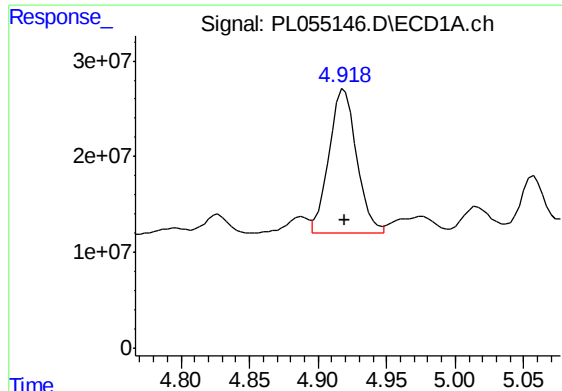

#24 Chlordane-2


R.T.: 4.919 min
Delta R.T.: 0.000 min
Response: 211767879
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

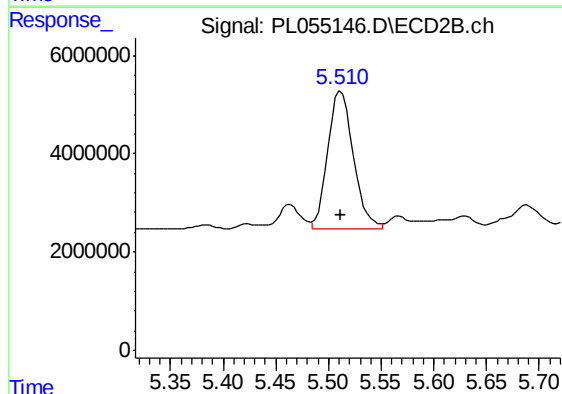


#24 Chlordane-2

R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 47594587
Conc: 500.00 ng/ml

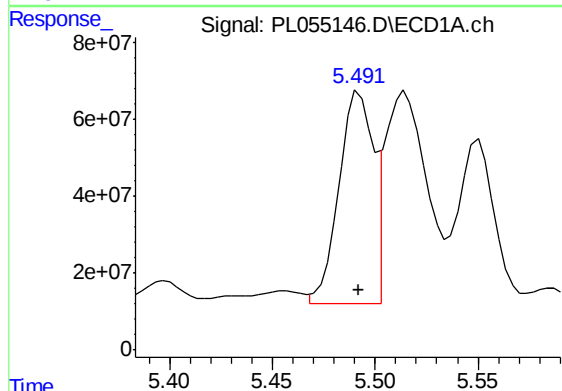


#25 Chlordane-3

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 633731835
Conc: 500.00 ng/ml

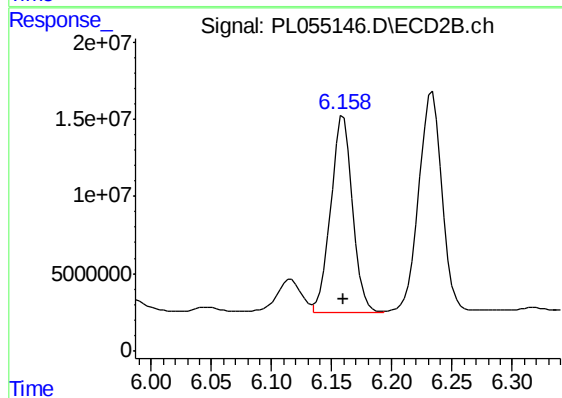

#25 Chlordane-3


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 160907243
Conc: 500.00 ng/ml

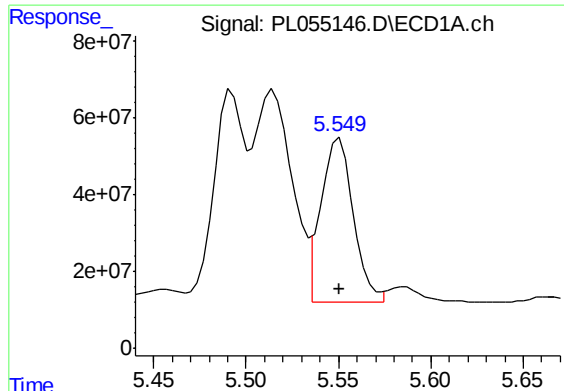

#26 Chlordane-4


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 523371911
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

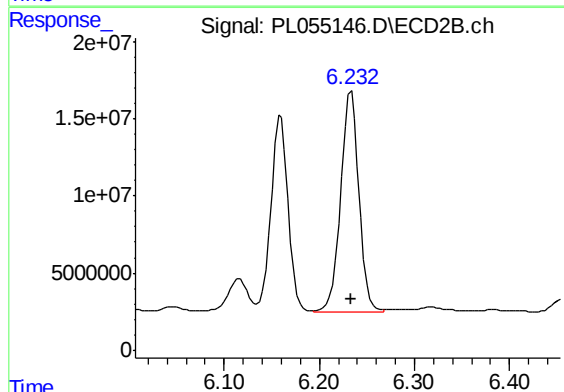


#26 Chlordane-4

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 192189180
Conc: 500.00 ng/ml

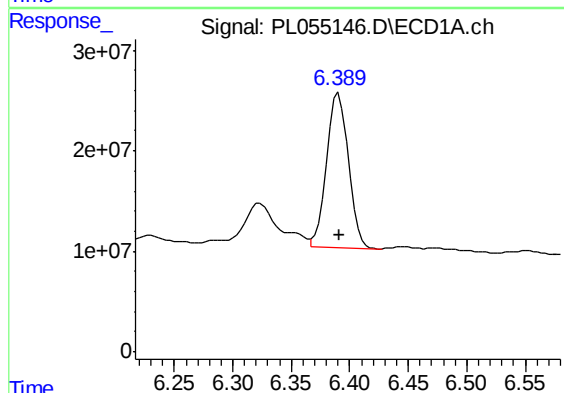


#27 Chlordane-5

R.T.: 6.391 min
Delta R.T.: 0.000 min
Response: 194834125
Conc: 500.00 ng/ml

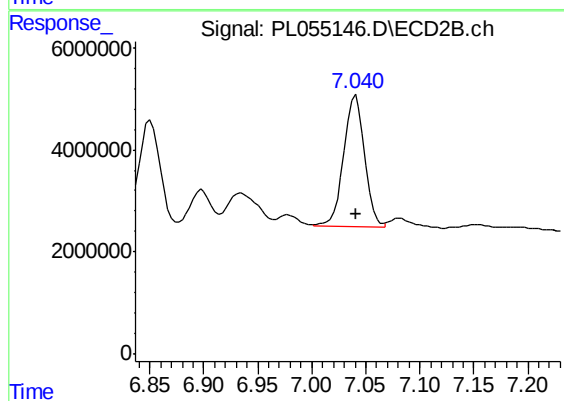

#27 Chlordane-5


R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 34886798
Conc: 500.00 ng/ml

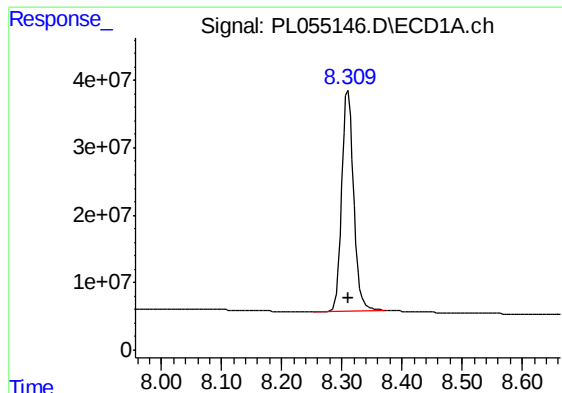

#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 444493092
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

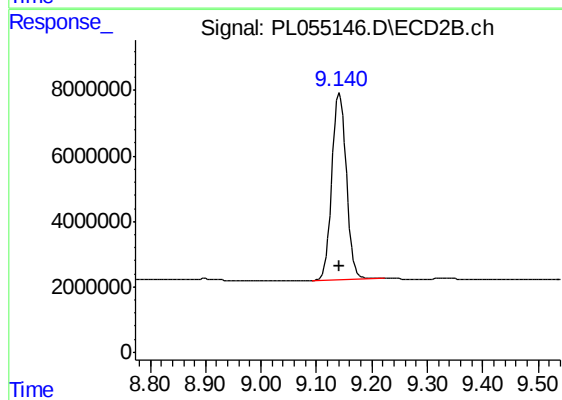

#28 Decachlorobiphenyl

R.T.: 9.142 min
Delta R.T.: 0.000 min
Response: 103696520
Conc: 50.00 ng/ml