

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122119\
 Data File : PL055162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 18:14
 Operator : SG\AJ
 Sample : K6370-01RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP1-3RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 05:32:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.048	104.7E6	28597594	9.954	10.823
28)	SA Decachlor...	8.310	9.143	1108.4E6	262.5E6	119.461	118.932
Target Compounds							
16)	A 4,4'-DDD	0.000	6.881	0	59673375	N.D.	31.389 #
17)	MA 4,4'-DDT	6.464	7.206f	128.6E6	31786949	12.778	16.196 #
18)	B Endrin al...	6.572f	7.107	392.6E6	7889177	40.309	4.088 #
19)	B Endosulfa...	6.757	0.000	66778703	0	6.639	N.D. #
20)	A Methoxychlor	0.000	7.613f	0	12480797	N.D.	11.564 #
21)	B Endrin ke...	7.279f	0.000	316.0E6	0	30.147	N.D. #
22)	Mirex	0.000	8.272f	0	217.1E6	N.D.	130.931 #
27)	Chlordane-5	0.000	7.049	0	1693990	N.D.	24.278 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122119\
Data File : PL055162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 18:14
Operator : SG\AJ
Sample : K6370-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP1-3RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 05:32:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

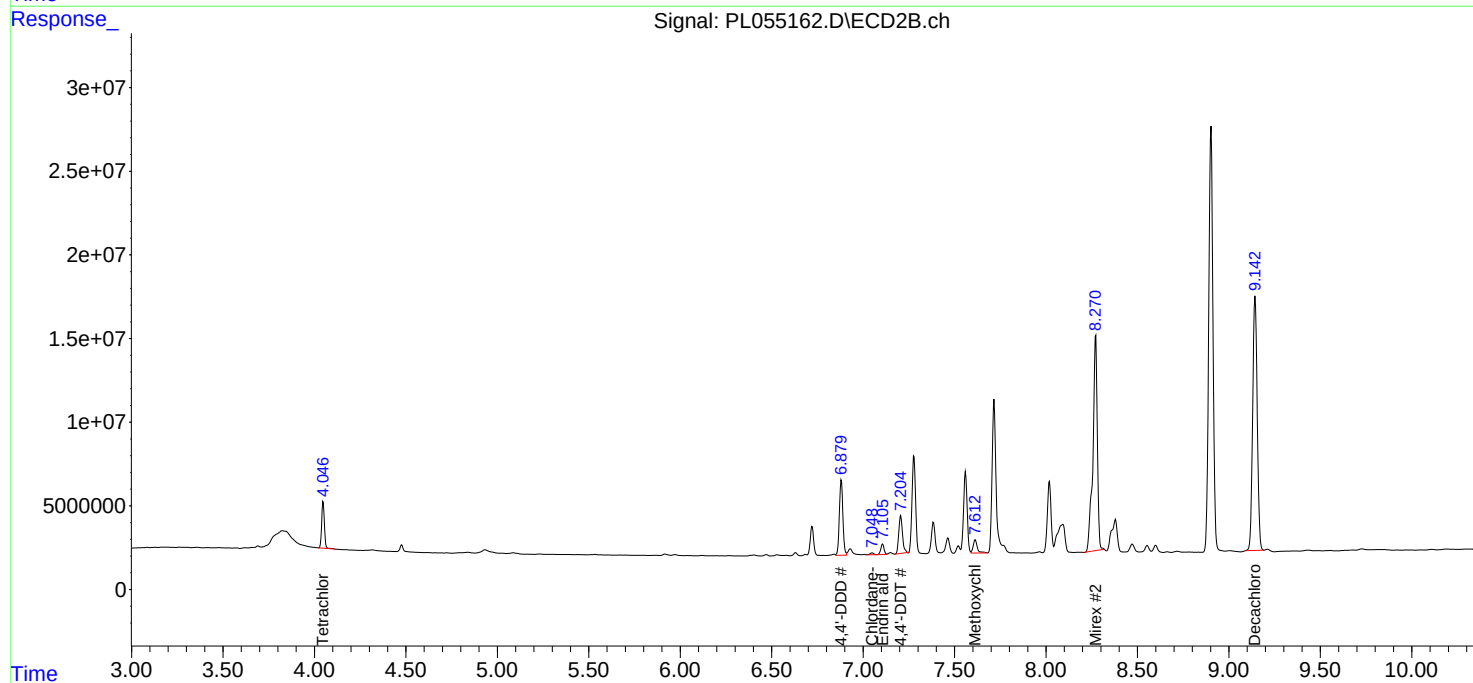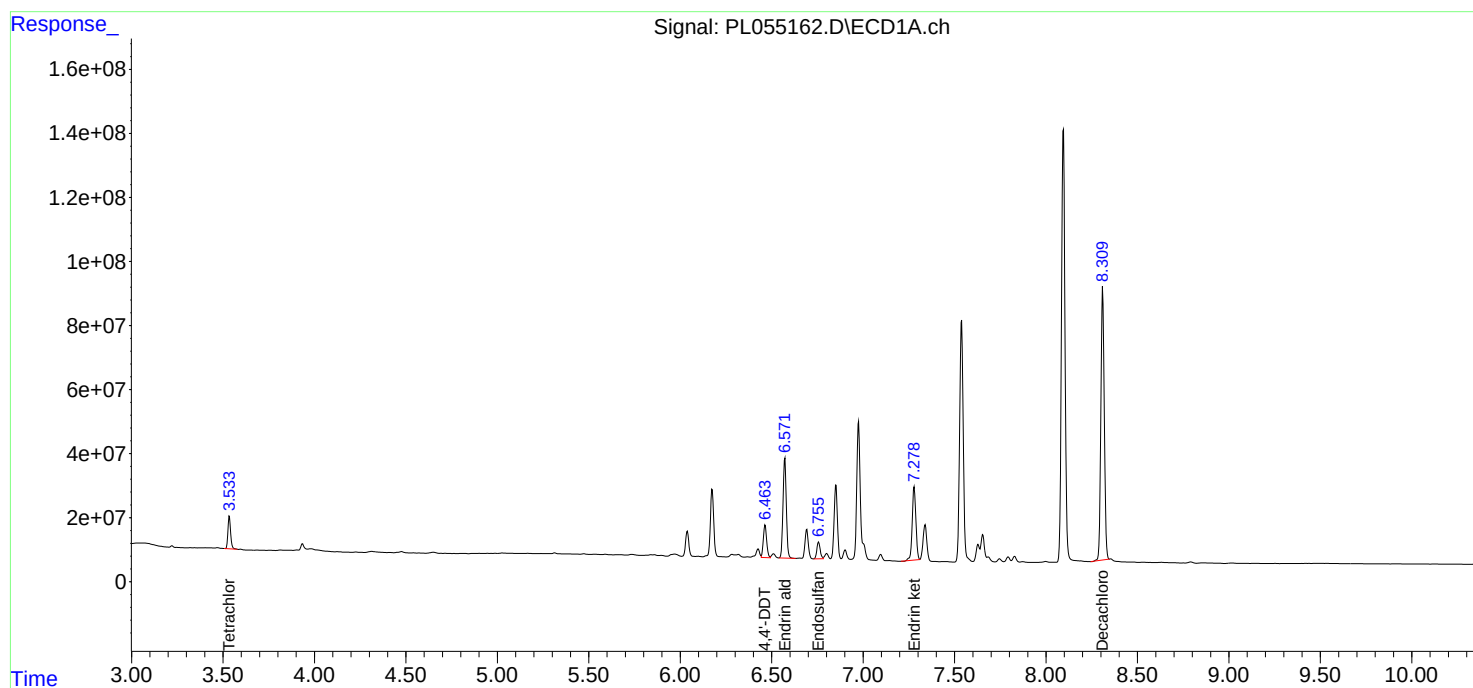


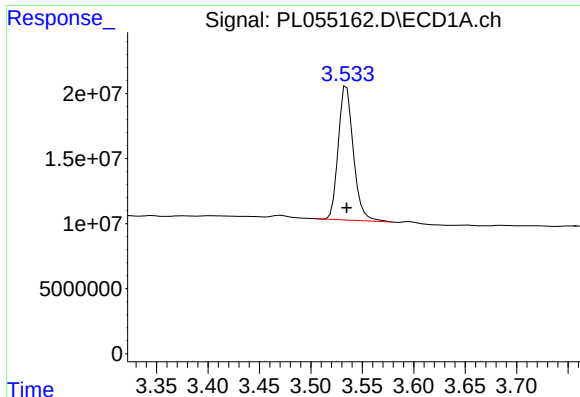

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 104681468
Conc: 9.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-3RE

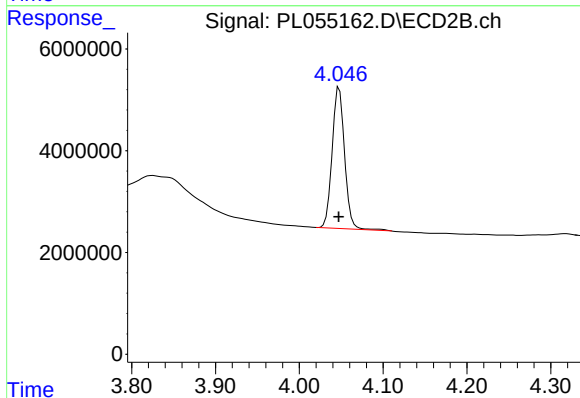


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 28597594
Conc: 10.82 ng/ml

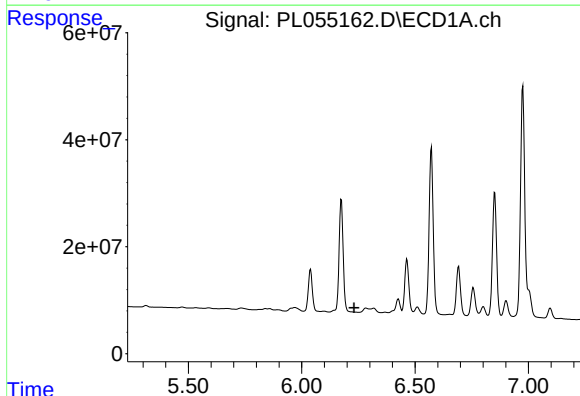


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

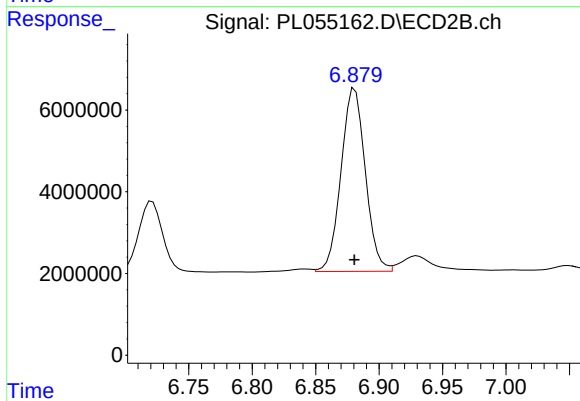

#16 4,4'-DDD


R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 59673375
Conc: 31.39 ng/ml

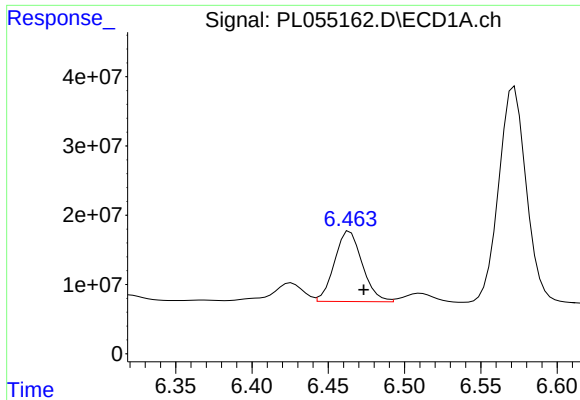

#17 4,4'-DDT


R.T.: 6.464 min
Delta R.T.: -0.009 min
Response: 128635409
Conc: 12.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-3RE

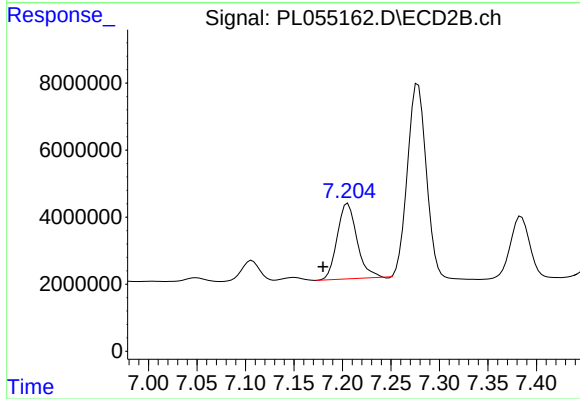


#17 4,4'-DDT

R.T.: 7.206 min
Delta R.T.: 0.026 min
Response: 31786949
Conc: 16.20 ng/ml

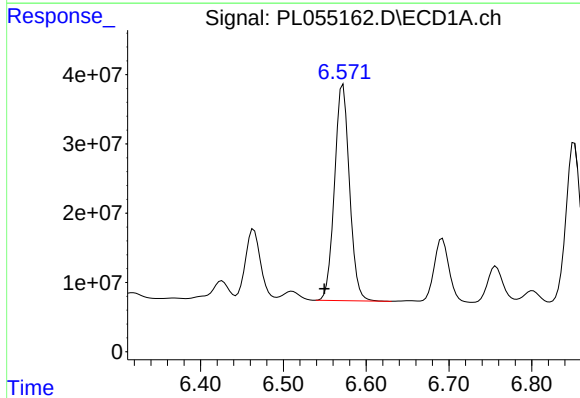


#18 Endrin aldehyde

R.T.: 6.572 min
Delta R.T.: 0.022 min
Response: 392582319
Conc: 40.31 ng/ml

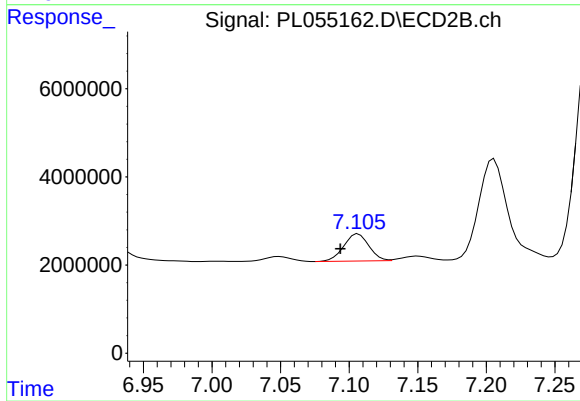

#18 Endrin aldehyde


R.T.: 7.107 min
Delta R.T.: 0.013 min
Response: 7889177
Conc: 4.09 ng/ml

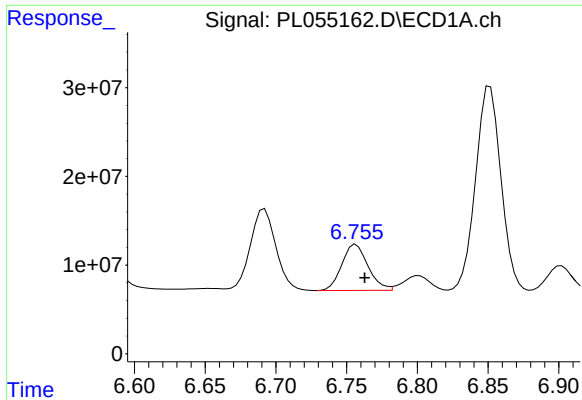

#19 Endosulfan Sulfate


R.T.: 6.757 min
Delta R.T.: -0.006 min
Response: 66778703
Conc: 6.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-3RE

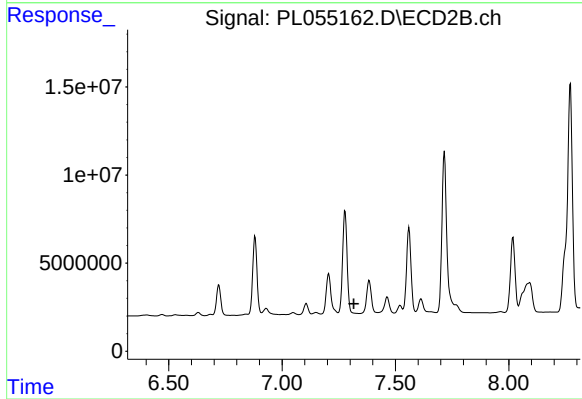


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.

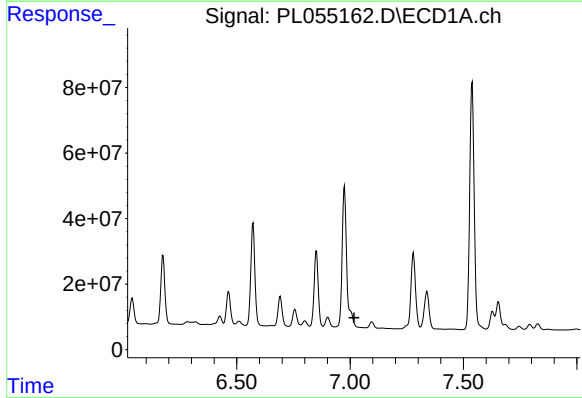


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.018 min
Response: 0
Conc: N.D.

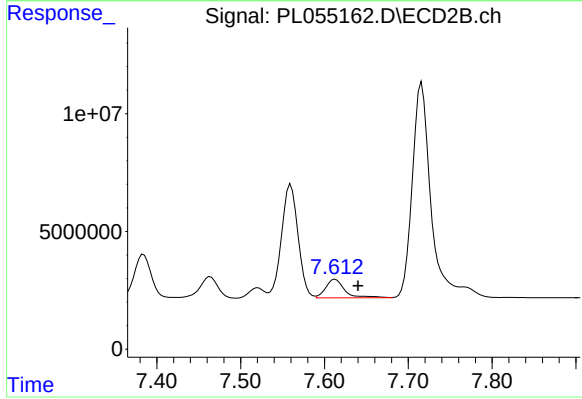

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: -0.027 min
Response: 12480797
Conc: 11.56 ng/ml

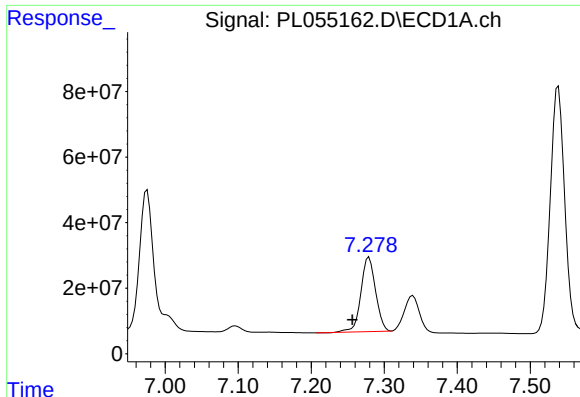

#21 Endrin ketone


R.T.: 7.279 min
Delta R.T.: 0.023 min
Response: 315988039
Conc: 30.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-3RE

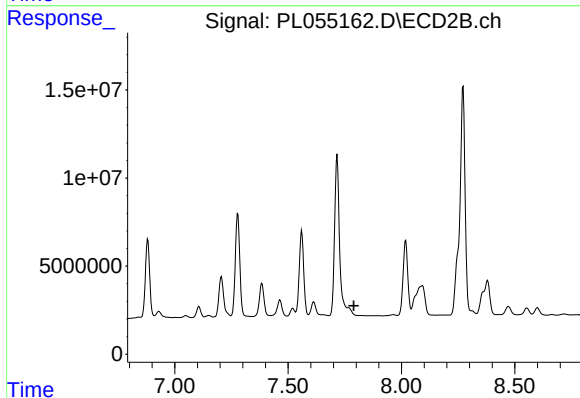


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.790 min
Response: 0
Conc: N.D.

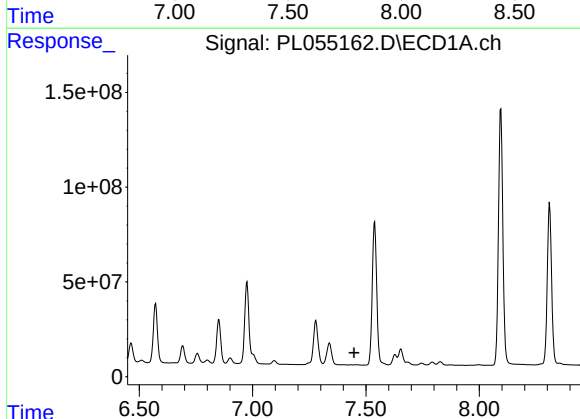


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.448 min
Response: 0
Conc: N.D.

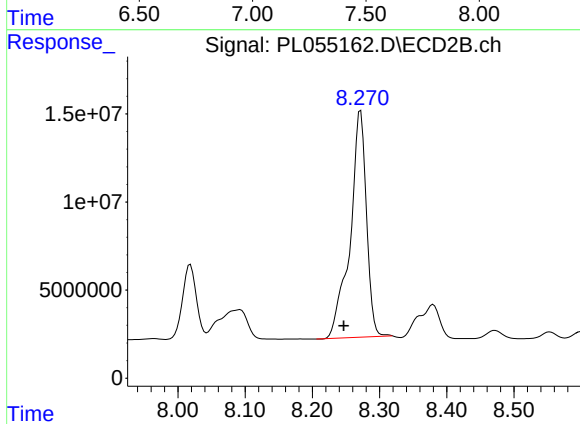

#22 Mirex


R.T.: 8.272 min
Delta R.T.: 0.025 min
Response: 217092254
Conc: 130.93 ng/ml

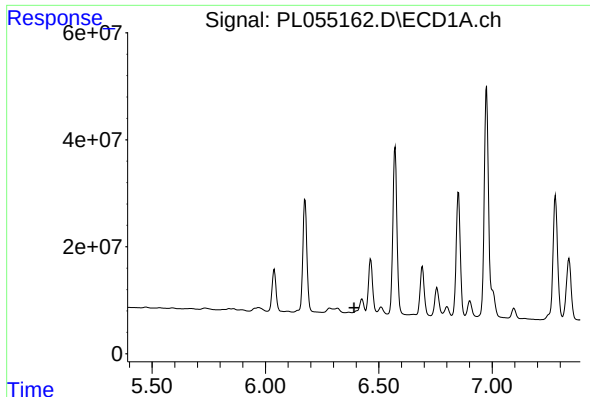

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP1-3RE

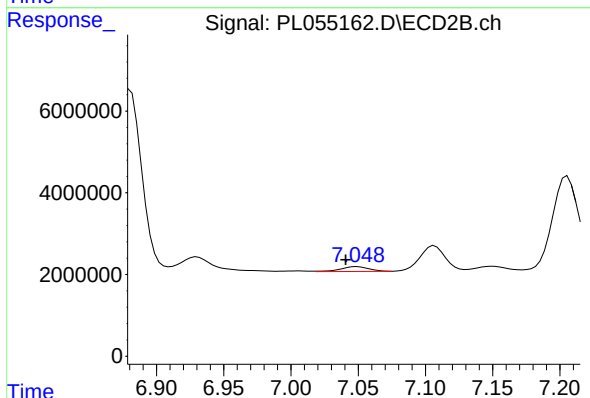


#27 Chlordane-5

R.T.: 7.049 min
Delta R.T.: 0.008 min
Response: 1693990
Conc: 24.28 ng/ml

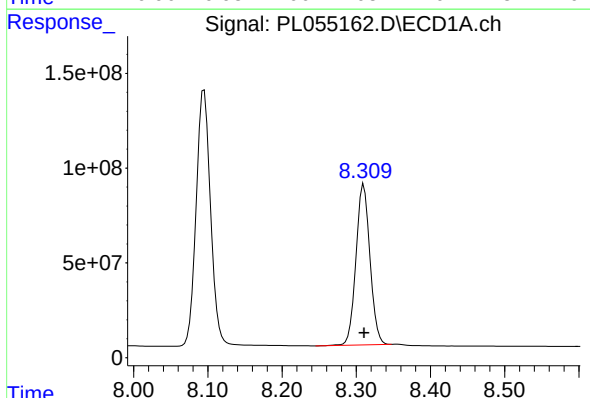

#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: 0.000 min
Response: 1108442881
Conc: 119.46 ng/ml

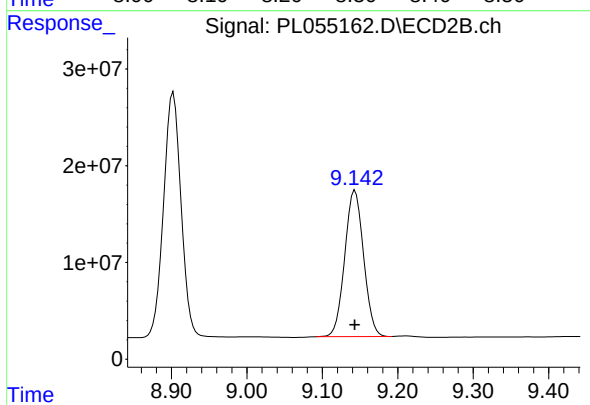

#28 Decachlorobiphenyl

R.T.: 9.143 min
Delta R.T.: 0.000 min
Response: 262538762
Conc: 118.93 ng/ml