

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122121\
 Data File : PL071545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2021 09:54
 Operator : AR\AJ
 Sample : PB141590BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 00:31:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.570	5.499	9547929	23603515	20.143	19.813
28)	SA Decachlor...	10.330	11.395	15216894	23367447	22.903	21.507
Target Compounds							
6)	B beta-BHC	6.048f	0.000	246646	0	0.864	N.D. #
7)	B delta-BHC	0.000	6.979f	0	220226	N.D.	0.144 #
10)	B gamma-Chl...	0.000	8.234	0	308957	N.D.	0.239 #
15)	B Endosulfa...	0.000	9.151f	0	574796	N.D.	0.570 #
16)	A 4,4'-DDD	0.000	9.057f	0	134862	N.D.	0.153 #
18)	B Endrin al...	0.000	9.275f	0	71587	N.D.	0.095 #
19)	B Endosulfa...	0.000	9.524f	0	185163	N.D.	0.189 #
25)	Chlordane-3	0.000	8.234	0	308957	N.D.	1.765 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122121\
Data File : PL071545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2021 09:54
Operator : AR\AJ
Sample : PB141590BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 00:31:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

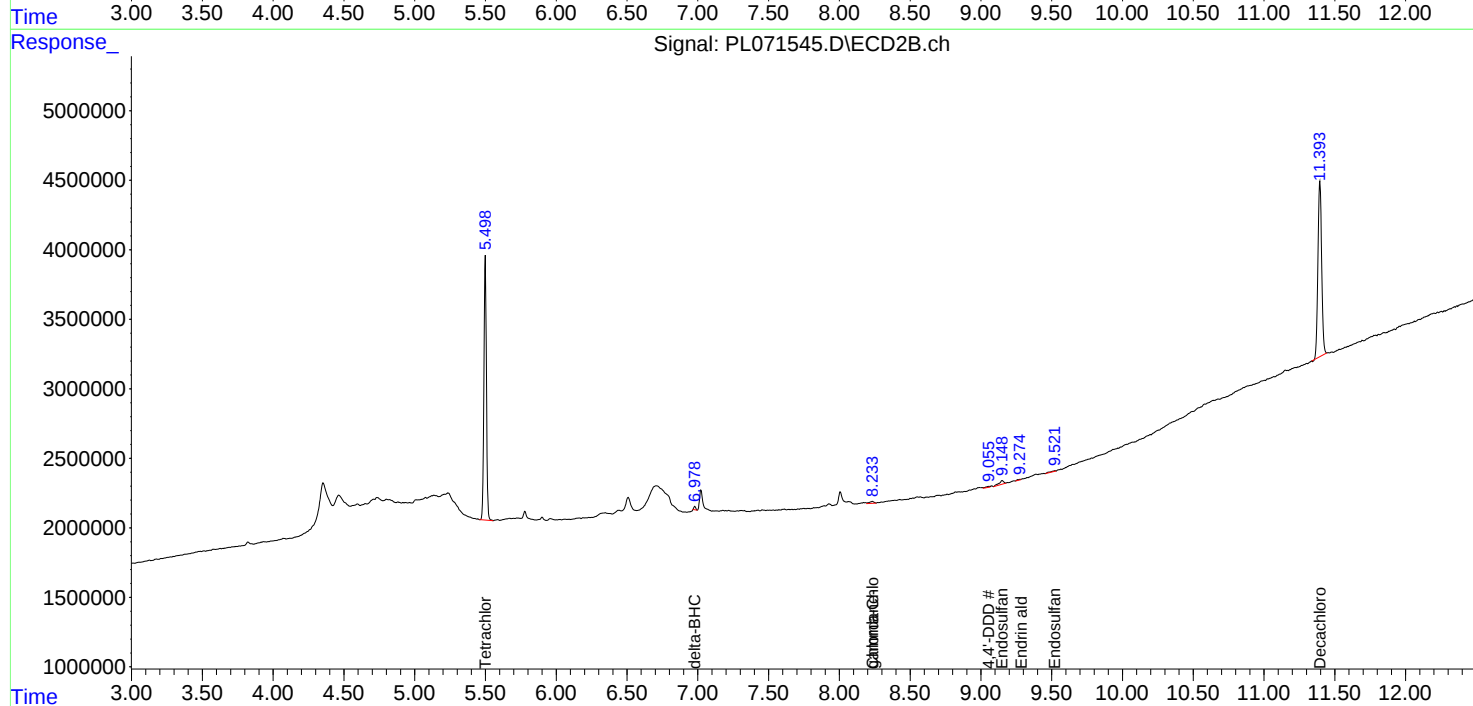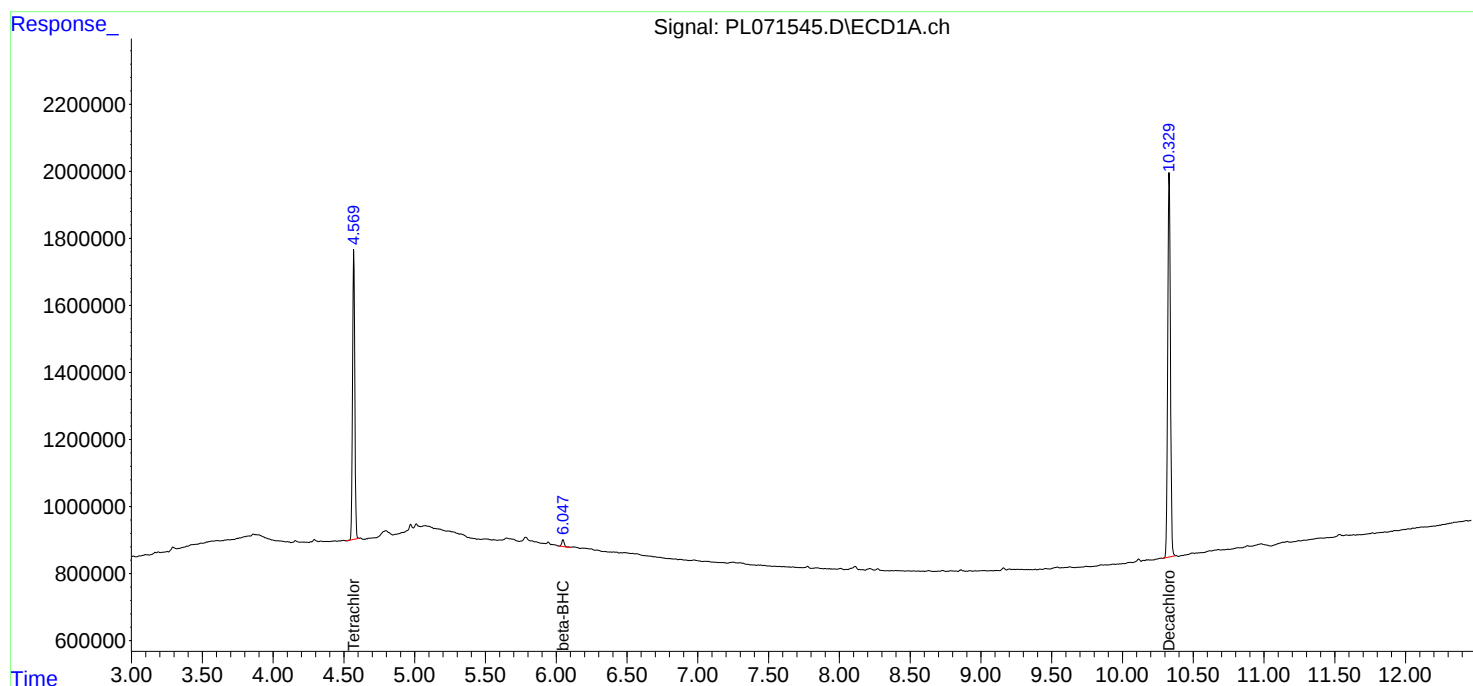


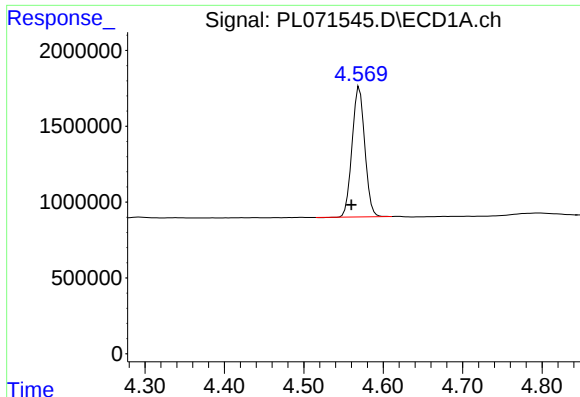

#1 Tetrachloro-m-xylene


R.T.: 4.570 min
Delta R.T.: 0.010 min
Response: 9547929
Conc: 20.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

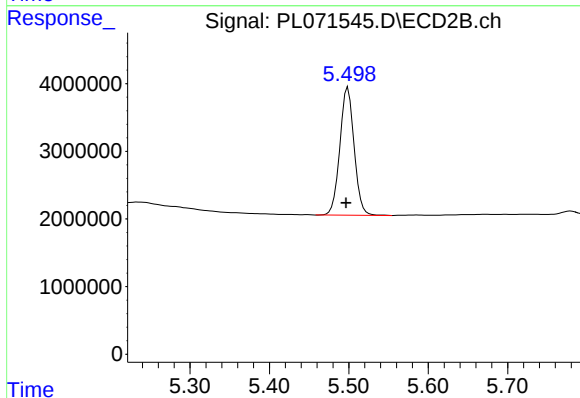


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: 0.002 min
Response: 23603515
Conc: 19.81 ng/ml

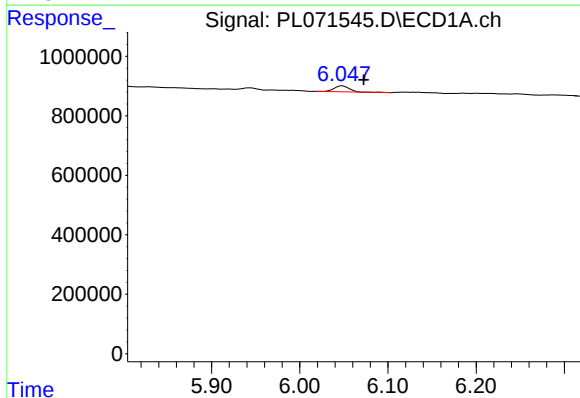


#6 beta-BHC

R.T.: 6.048 min
Delta R.T.: -0.024 min
Response: 246646
Conc: 0.86 ng/ml

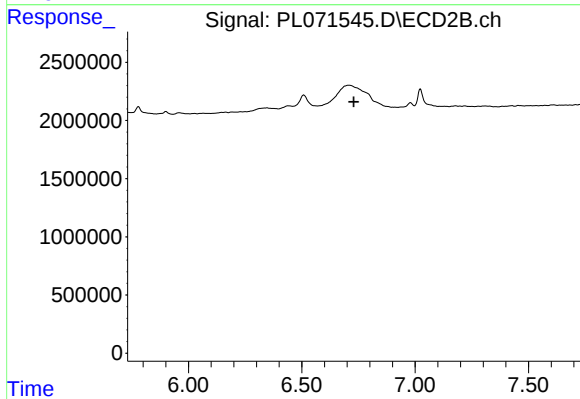

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.730 min
Response: 0
Conc: N.D.

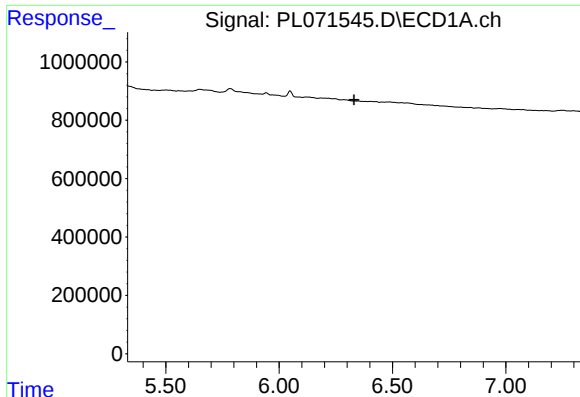

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

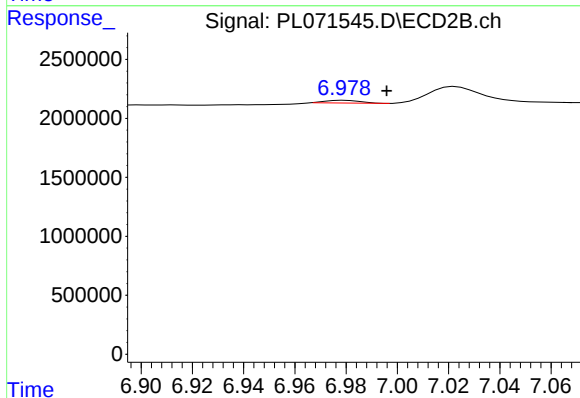


#7 delta-BHC

R.T.: 6.979 min
Delta R.T.: -0.016 min
Response: 220226
Conc: 0.14 ng/ml

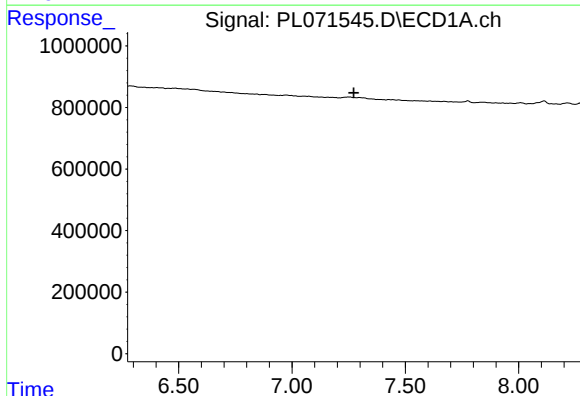


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

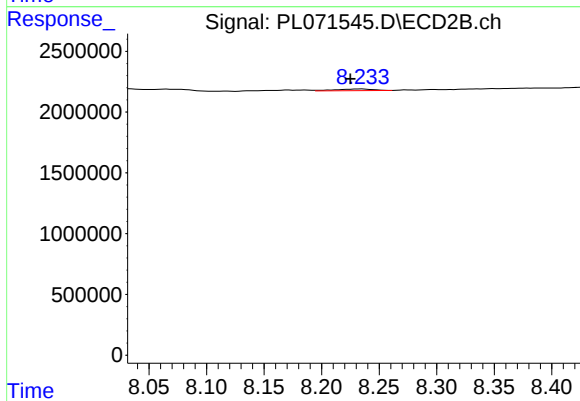

#10 gamma-Chlordane


R.T.: 8.234 min
Delta R.T.: 0.009 min
Response: 308957
Conc: 0.24 ng/ml

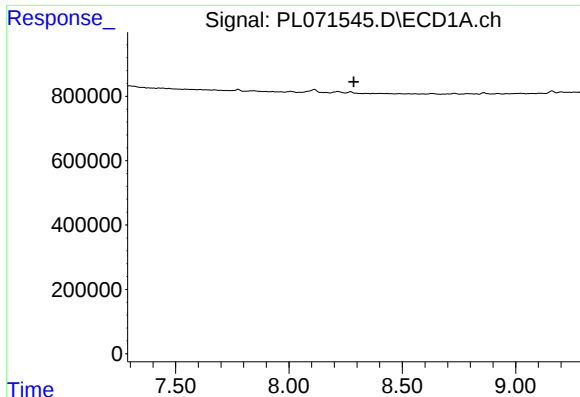

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

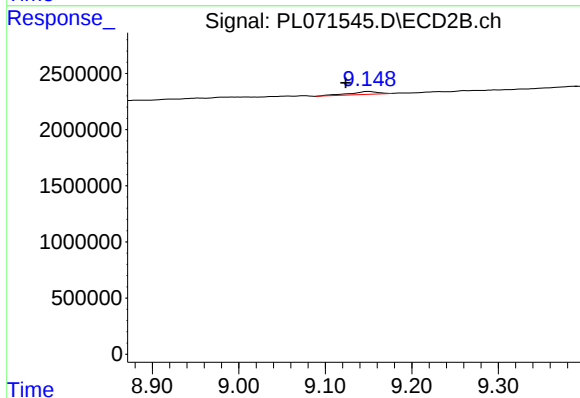


#15 Endosulfan II

R.T.: 9.151 min
Delta R.T.: 0.027 min
Response: 574796
Conc: 0.57 ng/ml

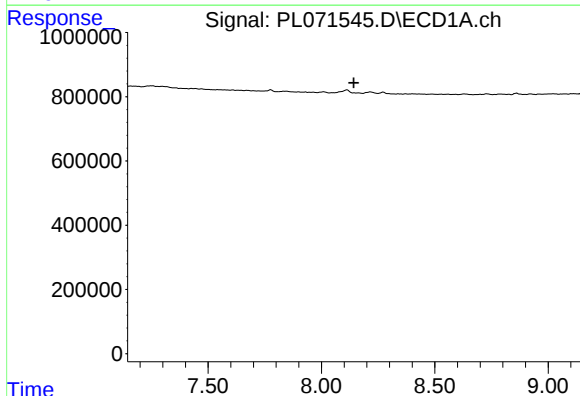


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.143 min
Response: 0
Conc: N.D.

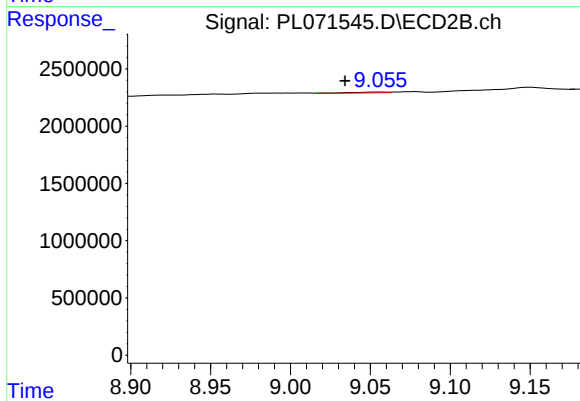

#16 4,4'-DDD


R.T.: 9.057 min
Delta R.T.: 0.023 min
Response: 134862
Conc: 0.15 ng/ml

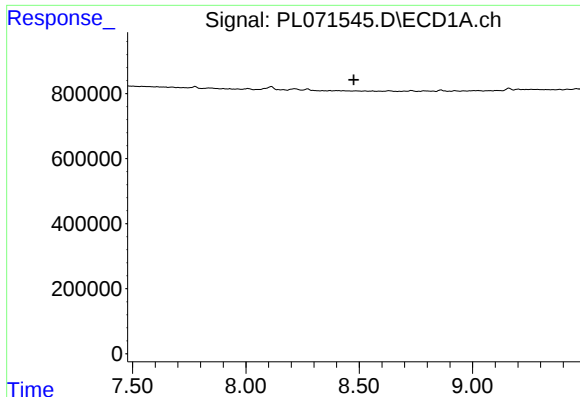

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

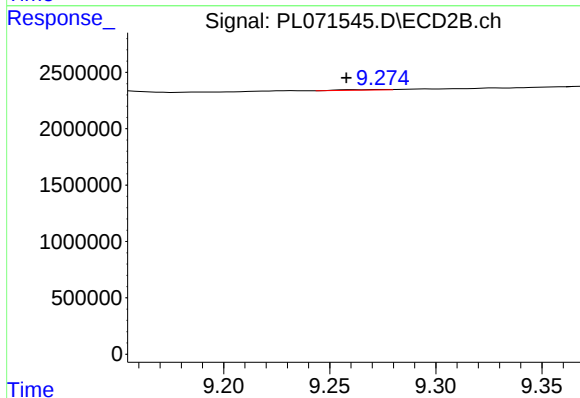


#18 Endrin aldehyde

R.T.: 9.275 min
Delta R.T.: 0.017 min
Response: 71587
Conc: 0.10 ng/ml

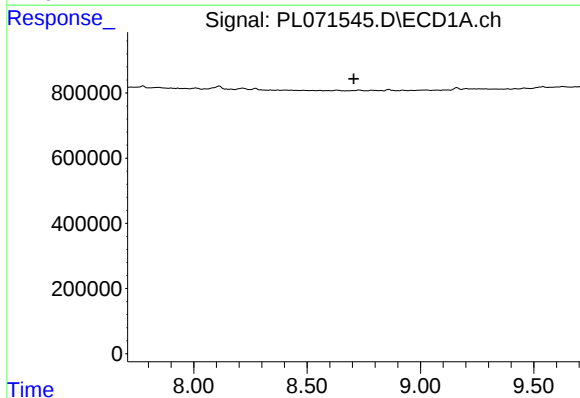


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

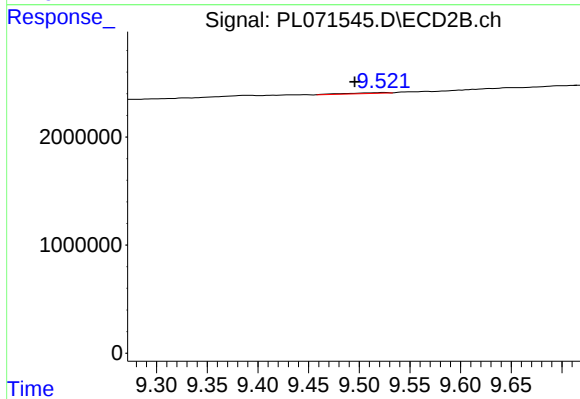

#19 Endosulfan Sulfate


R.T.: 9.524 min
Delta R.T.: 0.029 min
Response: 185163
Conc: 0.19 ng/ml

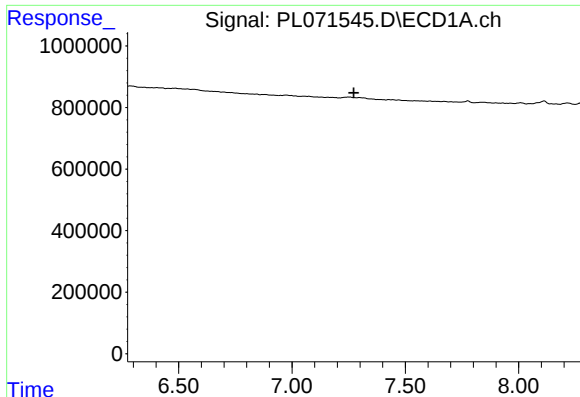

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

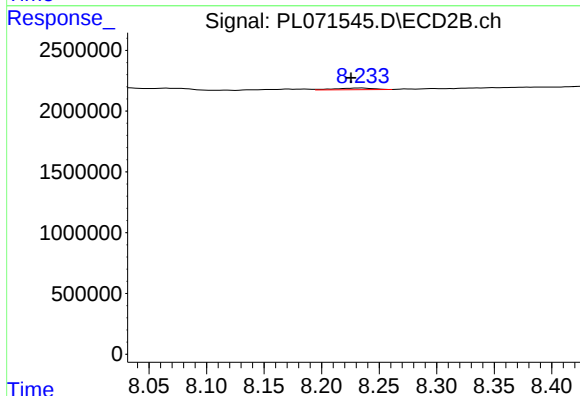


#25 Chlordane-3

R.T.: 8.234 min
Delta R.T.: 0.009 min
Response: 308957
Conc: 1.76 ng/ml

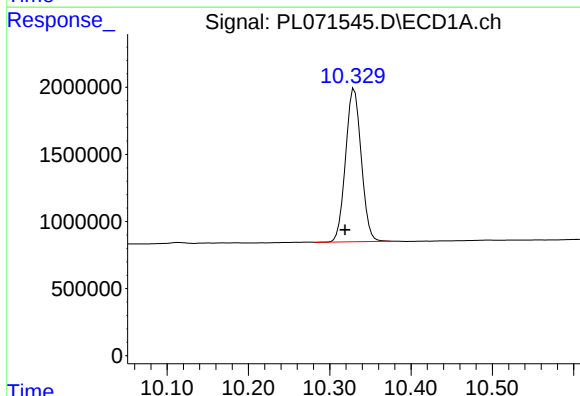

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.011 min
Response: 15216894
Conc: 22.90 ng/ml

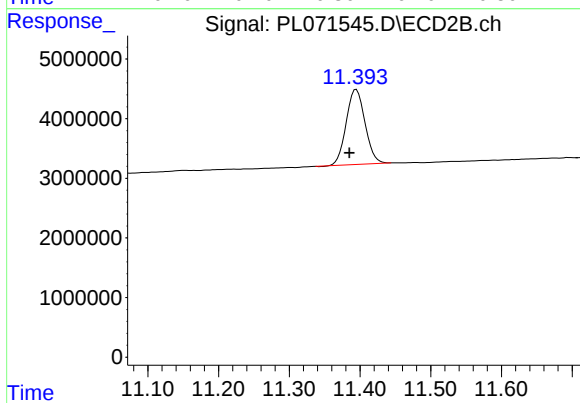

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.010 min
Response: 23367447
Conc: 21.51 ng/ml