

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122121\
 Data File : PL071550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2021 12:41
 Operator : AR\AJ
 Sample : PB141539TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 00:32:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.562	5.498	9732940	24127893	20.534	20.253
28)	SA Decachlor...	10.324	11.389	15282639	24072246	23.002	22.156
Target Compounds							
2)	A alpha-BHC	5.258	0.000	527137	0	0.829	N.D. #
7)	B delta-BHC	0.000	7.021f	0	1511906	N.D.	0.990 #
9)	A Endosulfan I	0.000	8.345f	0	71033	N.D.	0.059 #
10)	B gamma-Chl...	0.000	8.228	0	222672	N.D.	0.172 #
14)	MA Endrin	0.000	8.913f	0	151282	N.D.	0.149 #
15)	B Endosulfa...	0.000	9.102f	0	145433	N.D.	0.144 #
16)	A 4,4'-DDD	0.000	9.005f	0	292245	N.D.	0.331 #
25)	Chlordane-3	0.000	8.228	0	222672	N.D.	1.272 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122121\
Data File : PL071550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2021 12:41
Operator : AR\AJ
Sample : PB141539TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 00:32:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

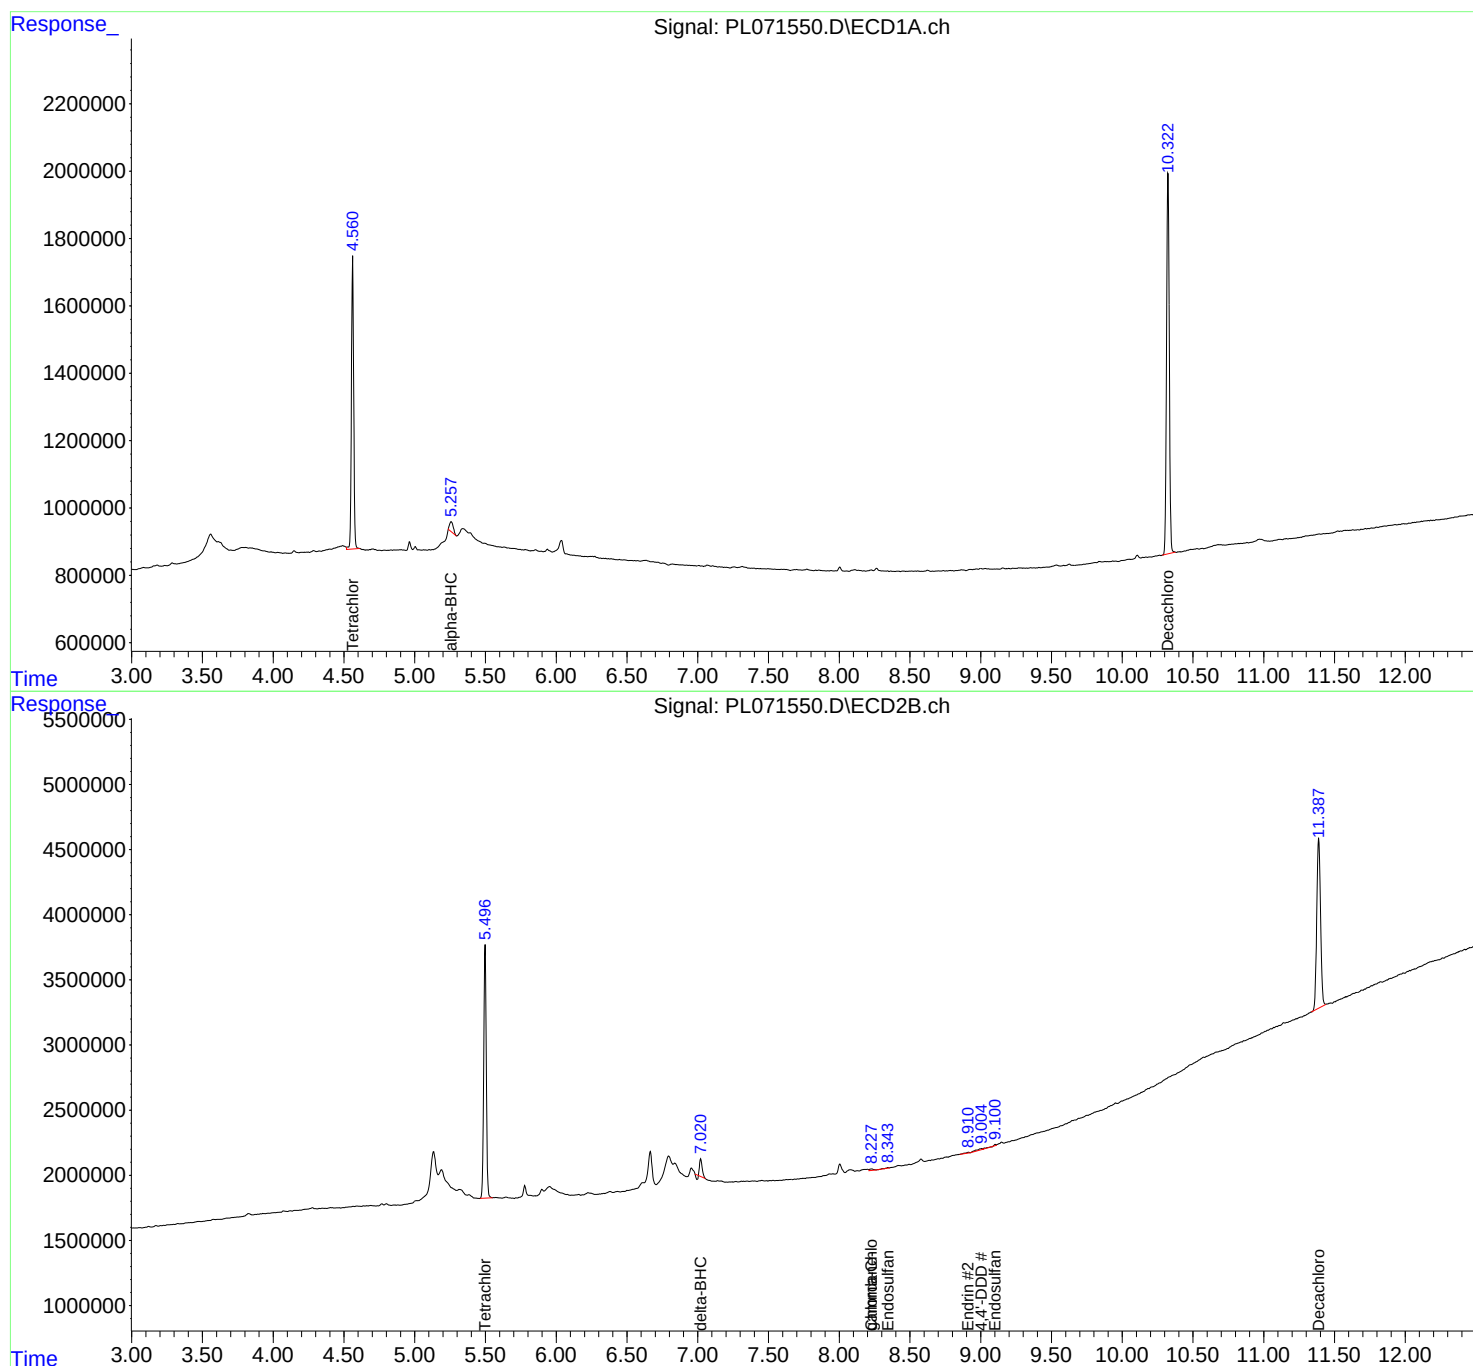


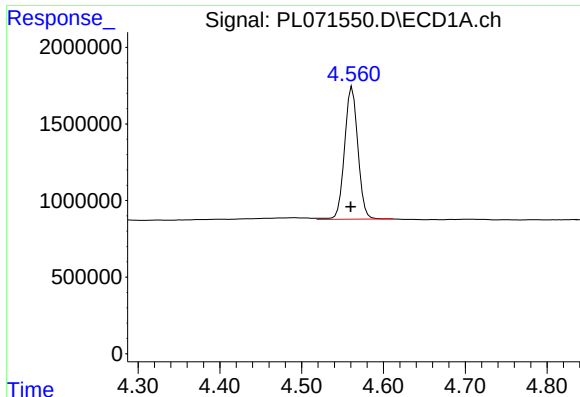

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: 0.002 min
Response: 9732940
Conc: 20.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

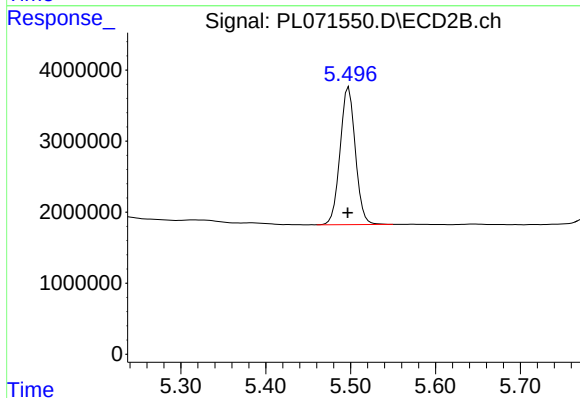


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: 0.001 min
Response: 24127893
Conc: 20.25 ng/ml

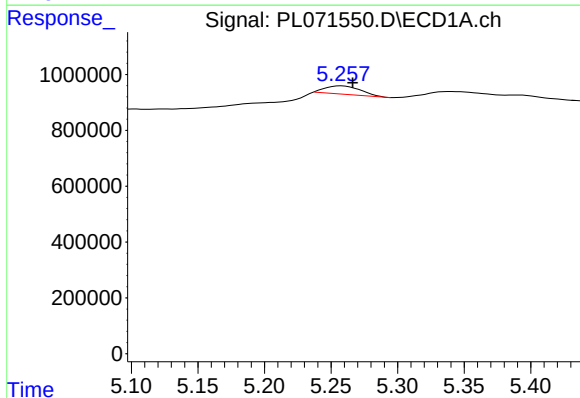


#2 alpha-BHC

R.T.: 5.258 min
Delta R.T.: -0.008 min
Response: 527137
Conc: 0.83 ng/ml

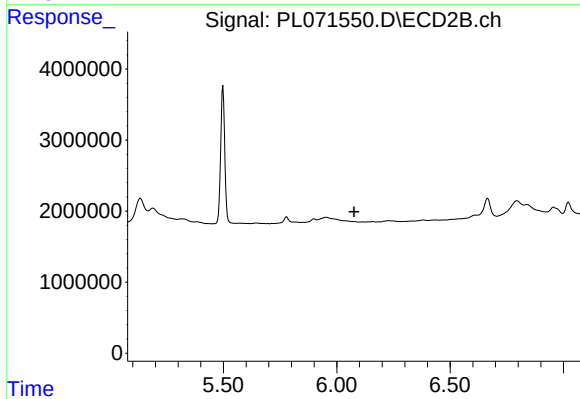

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.077 min
Response: 0
Conc: N.D.

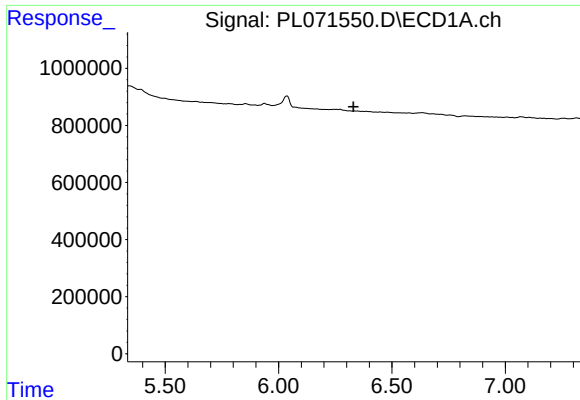

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

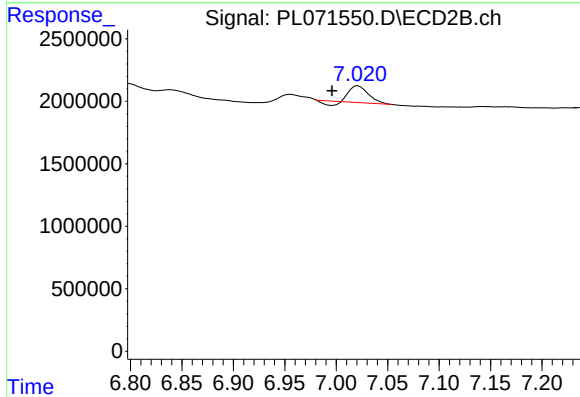


#7 delta-BHC

R.T.: 7.021 min
Delta R.T.: 0.026 min
Response: 1511906
Conc: 0.99 ng/ml

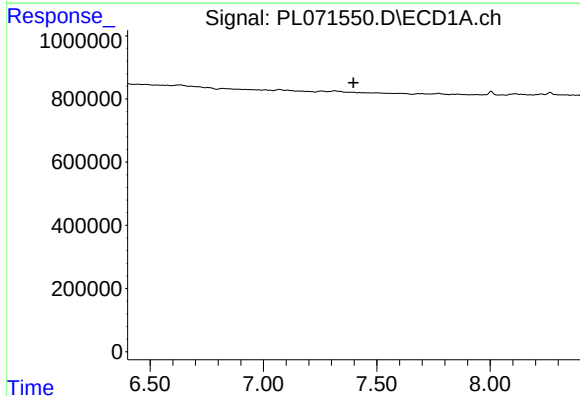


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.398 min
Response: 0
Conc: N.D.

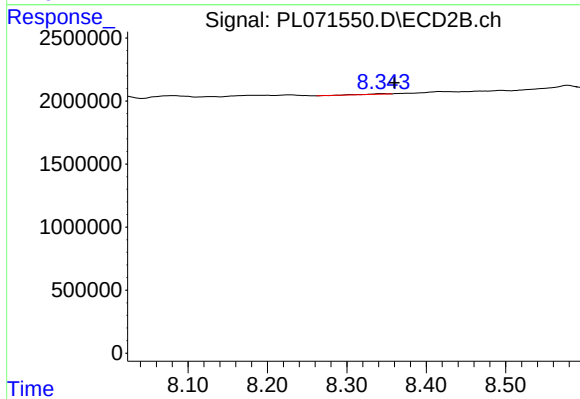

#9 Endosulfan I


R.T.: 8.345 min
Delta R.T.: -0.015 min
Response: 71033
Conc: 0.06 ng/ml

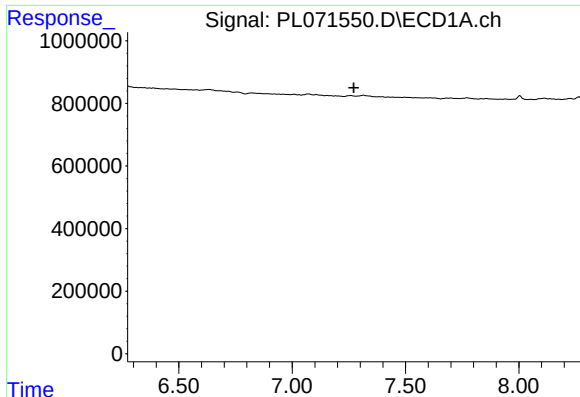

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

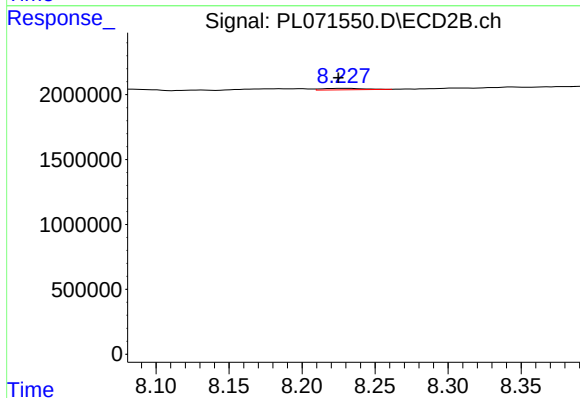


#10 gamma-Chlordane

R.T.: 8.228 min
Delta R.T.: 0.003 min
Response: 222672
Conc: 0.17 ng/ml

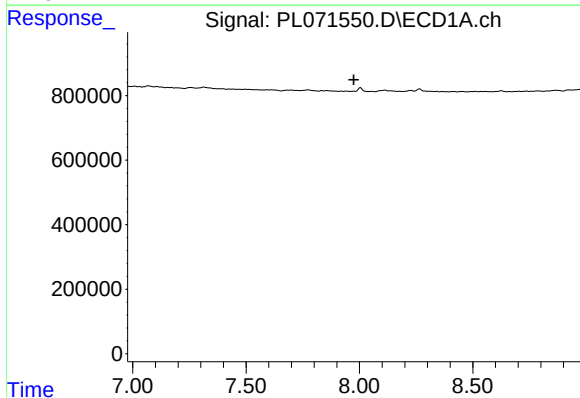


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

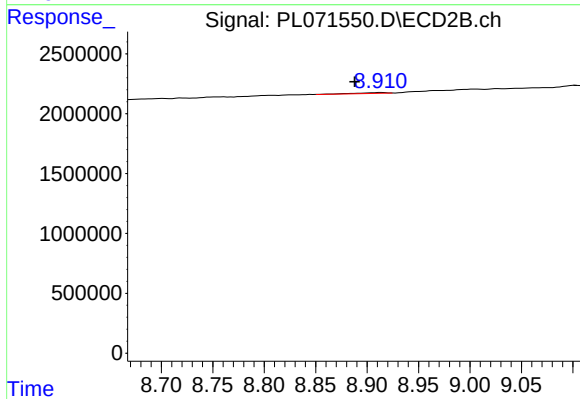

#14 Endrin


R.T.: 8.913 min
Delta R.T.: 0.025 min
Response: 151282
Conc: 0.15 ng/ml

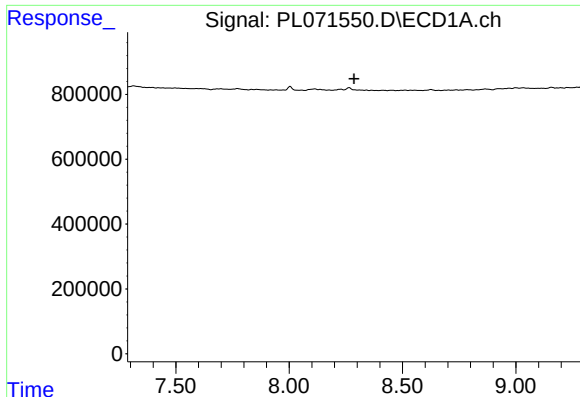

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

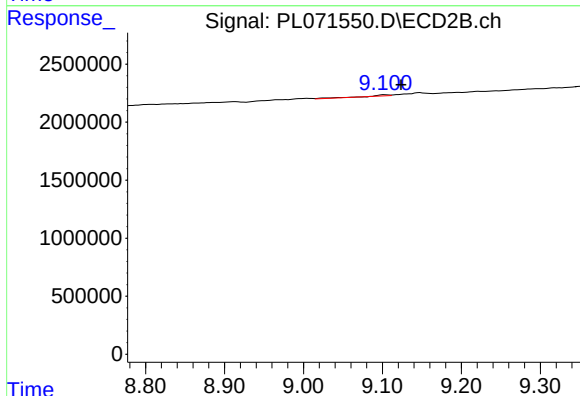


#15 Endosulfan II

R.T.: 9.102 min
Delta R.T.: -0.021 min
Response: 145433
Conc: 0.14 ng/ml

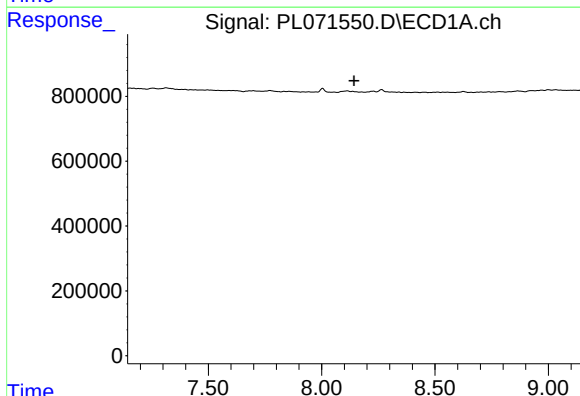


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.143 min
Response: 0
Conc: N.D.

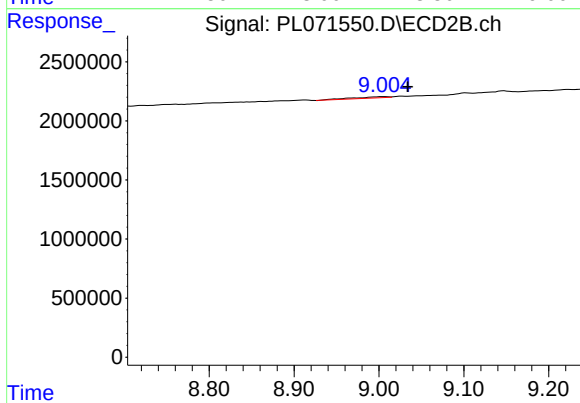

#16 4,4'-DDD


R.T.: 9.005 min
Delta R.T.: -0.029 min
Response: 292245
Conc: 0.33 ng/ml

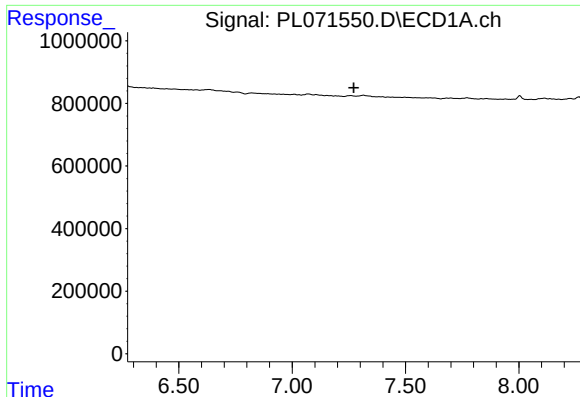

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

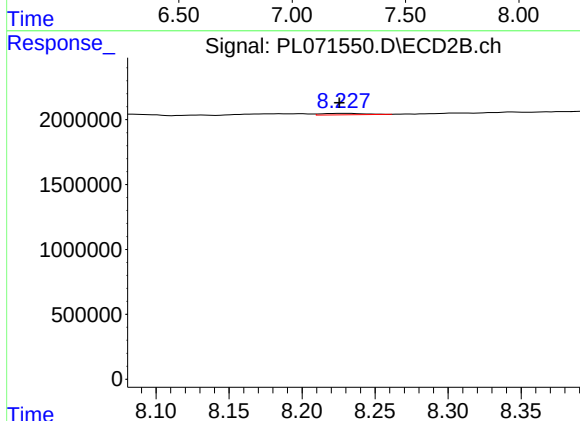


#25 Chlordane-3

R.T.: 8.228 min
Delta R.T.: 0.003 min
Response: 222672
Conc: 1.27 ng/ml

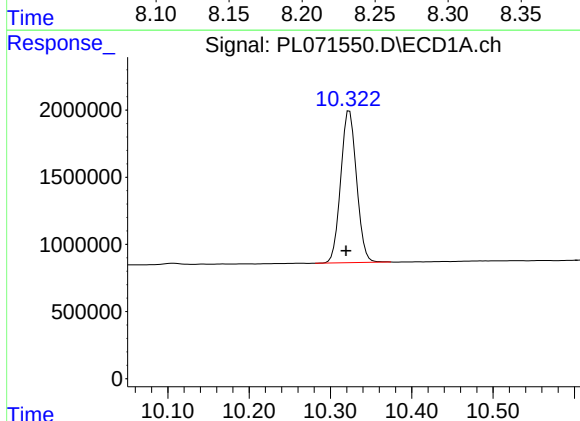

#28 Decachlorobiphenyl

R.T.: 10.324 min
Delta R.T.: 0.004 min
Response: 15282639
Conc: 23.00 ng/ml

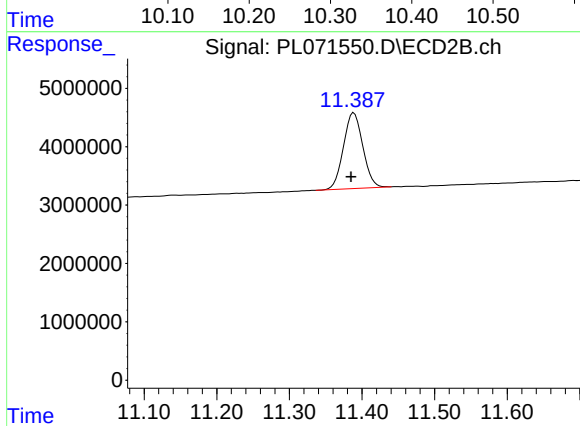

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.004 min
Response: 24072246
Conc: 22.16 ng/ml