

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122122\
 Data File : PL079830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 13:41
 Operator : AR\AJ
 Sample : N6157-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 21:34:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 10:00:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.562	19178621	24094715	8.727	9.077
28)	SA Decachlor...	8.762	7.626	14787281	18807716	7.973	7.835
Target Compounds							
2)	A alpha-BHC	3.773	0.000	58828	0	0.017	N.D. #
5)	MB Aldrin	0.000	3.957	0	179338	N.D.	0.047 #
8)	B Heptachlo...	0.000	4.452	0	338465	N.D.	0.097 #
9)	A Endosulfan I	5.848	0.000	287089	0	0.111	N.D. #
11)	B alpha-Chl...	0.000	4.745f	0	693704	N.D.	0.202 #
12)	B 4,4'-DDE	5.965	4.967	188019	176041	0.078	0.055 #
15)	B Endosulfa...	6.543f	0.000	638661	0	0.262	N.D. #
23)	Chlordane-1	0.000	3.529	0	252023	N.D.	2.413 #
26)	Chlordane-4	0.000	4.745f	0	693704	N.D.	1.908 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122122\
Data File : PL079830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 13:41
Operator : AR\AJ
Sample : N6157-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 21:34:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 10:00:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

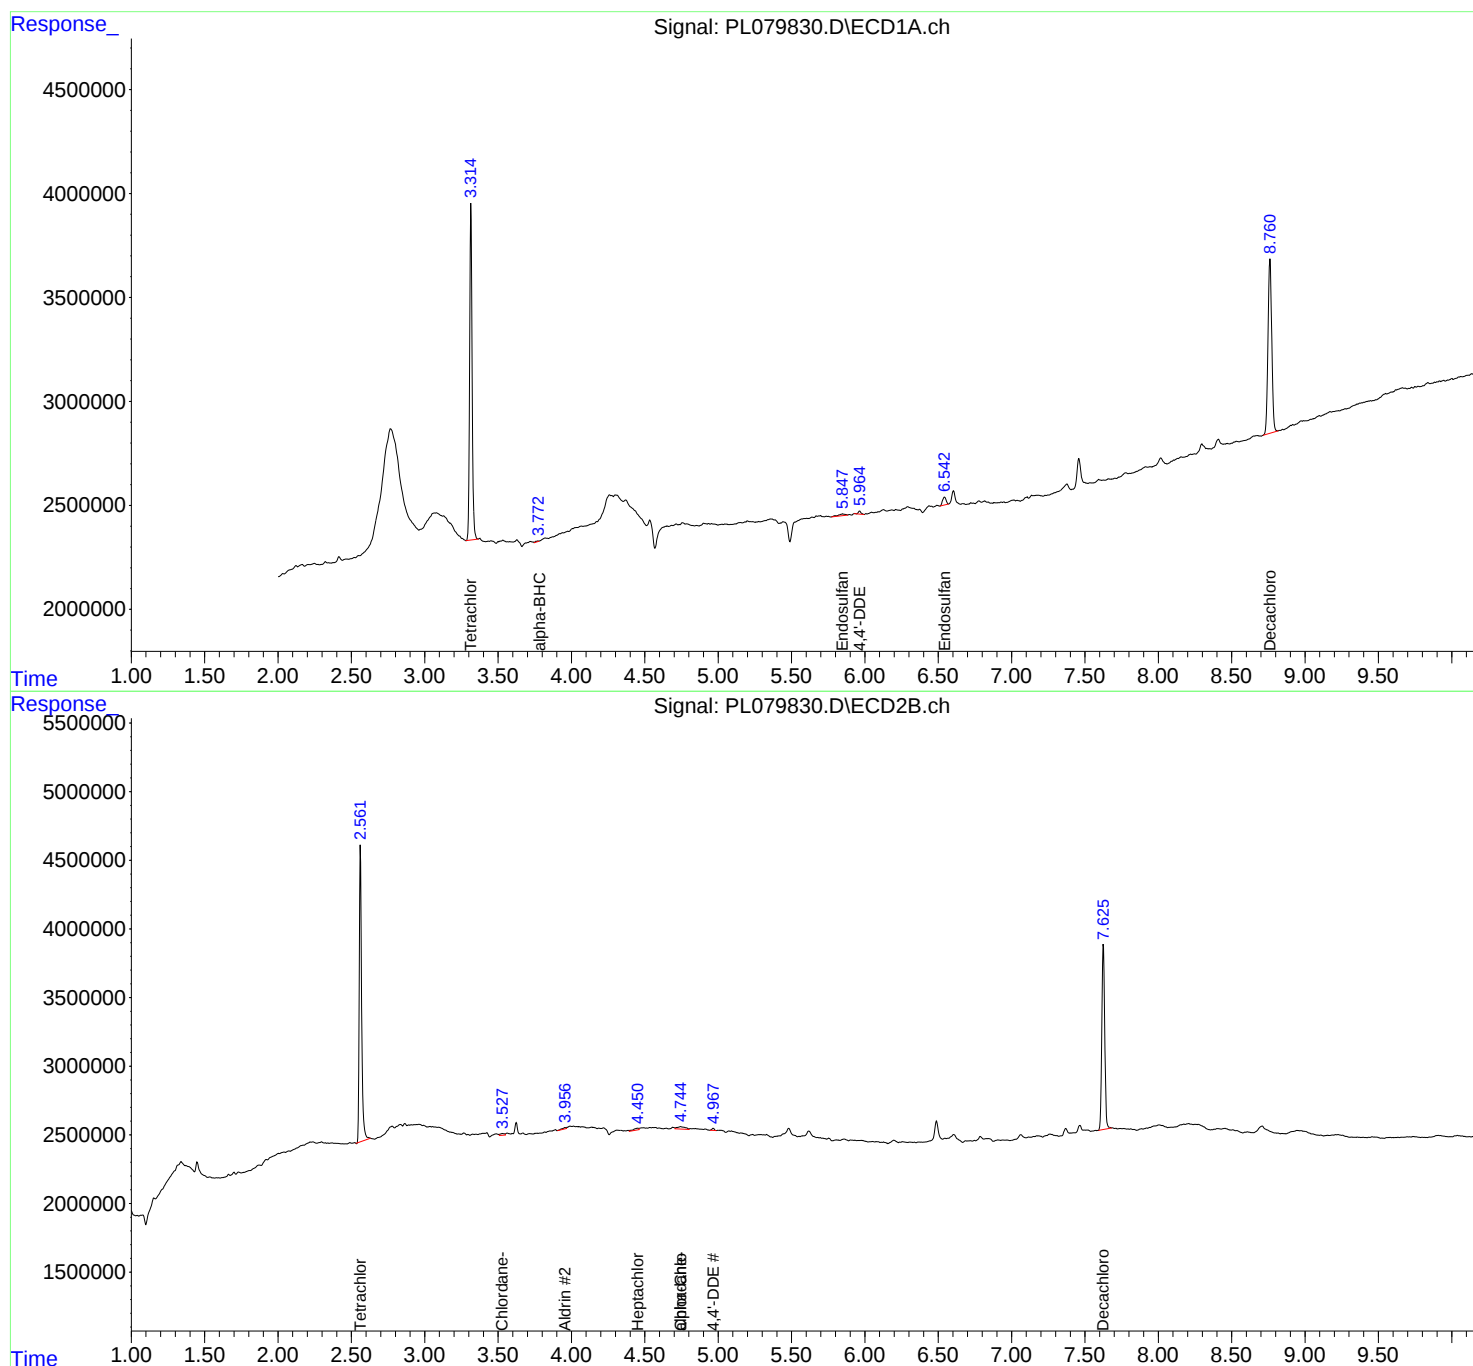


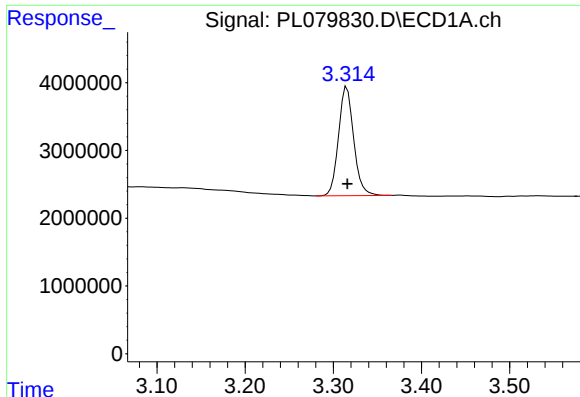

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 19178621
Conc: 8.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

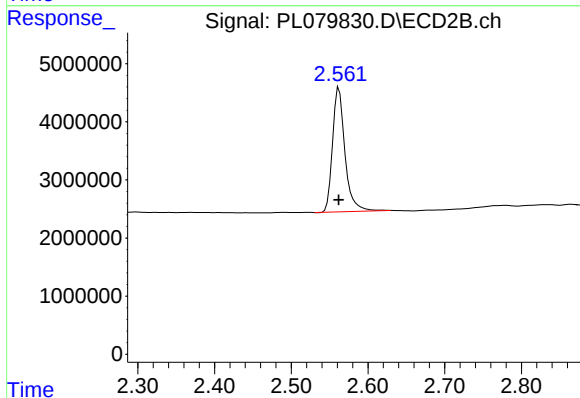


#1 Tetrachloro-m-xylene

R.T.: 2.562 min
Delta R.T.: 0.000 min
Response: 24094715
Conc: 9.08 ng/ml

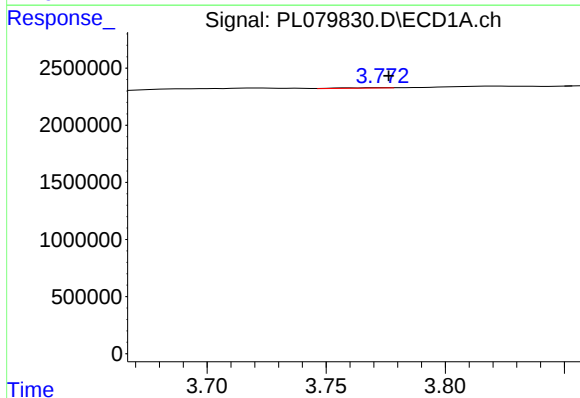


#2 alpha-BHC

R.T.: 3.773 min
Delta R.T.: -0.003 min
Response: 58828
Conc: 0.02 ng/ml

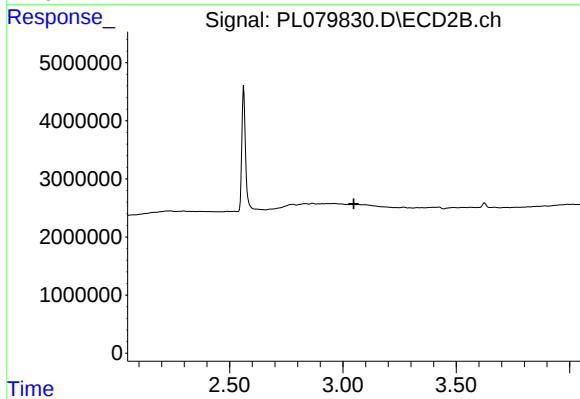

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

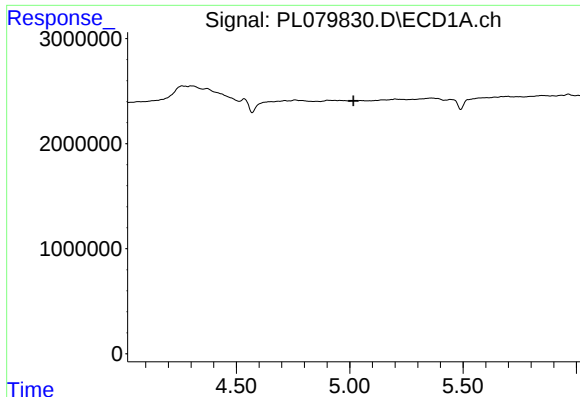

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

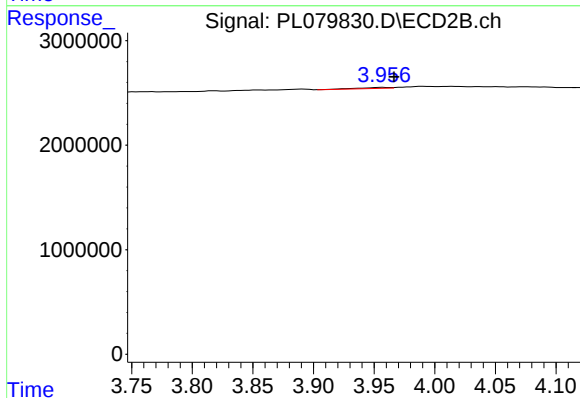


#5 Aldrin

R.T.: 3.957 min
Delta R.T.: -0.009 min
Response: 179338
Conc: 0.05 ng/ml

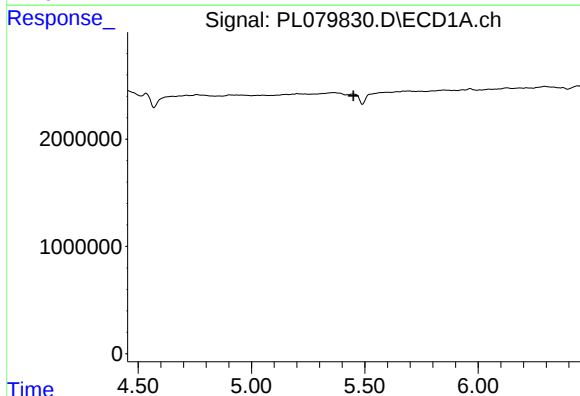


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.450 min
Response: 0
Conc: N.D.

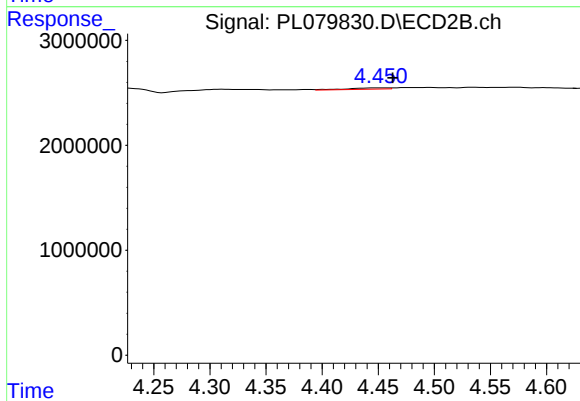

#8 Heptachlor epoxide


R.T.: 4.452 min
Delta R.T.: -0.011 min
Response: 338465
Conc: 0.10 ng/ml

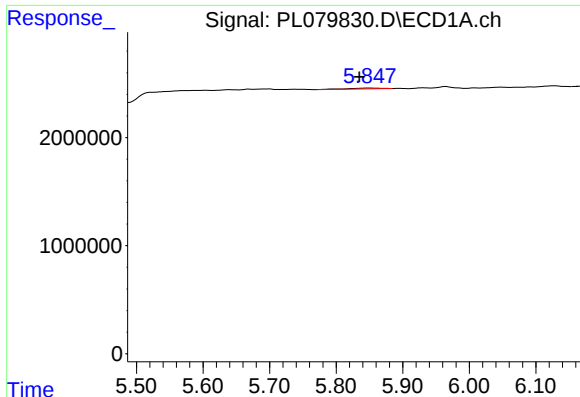

#9 Endosulfan I


R.T.: 5.848 min
Delta R.T.: 0.013 min
Response: 287089
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

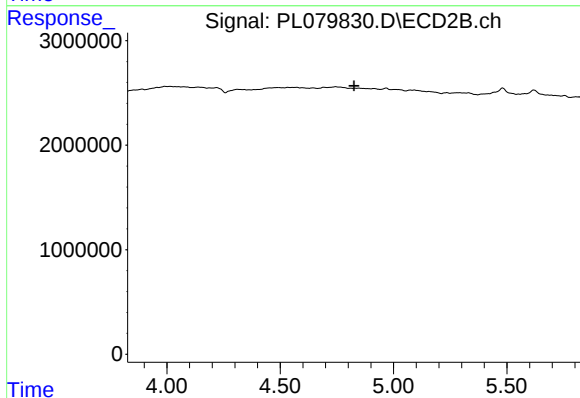


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.826 min
Response: 0
Conc: N.D.

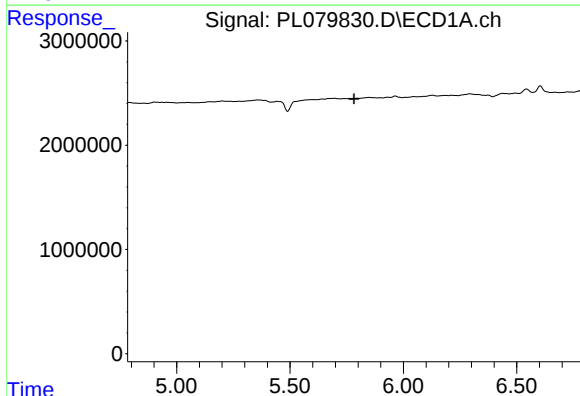


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.783 min
Response: 0
Conc: N.D.

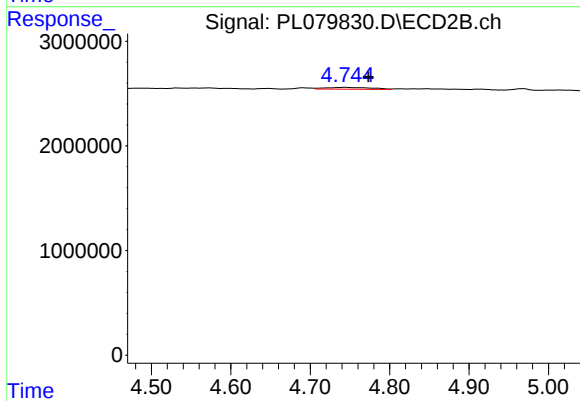

#11 alpha-Chlordane


R.T.: 4.745 min
Delta R.T.: -0.028 min
Response: 693704
Conc: 0.20 ng/ml

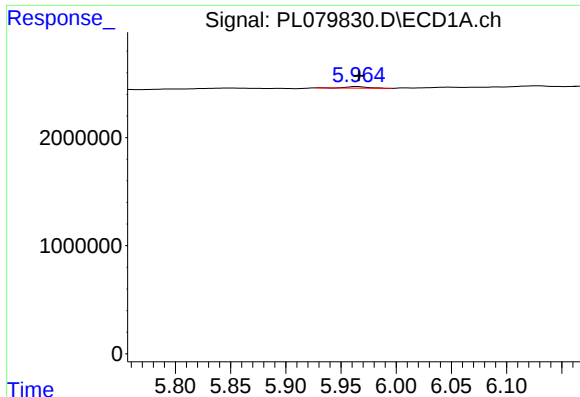

#12 4,4'-DDE


R.T.: 5.965 min
Delta R.T.: -0.001 min
Response: 188019
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

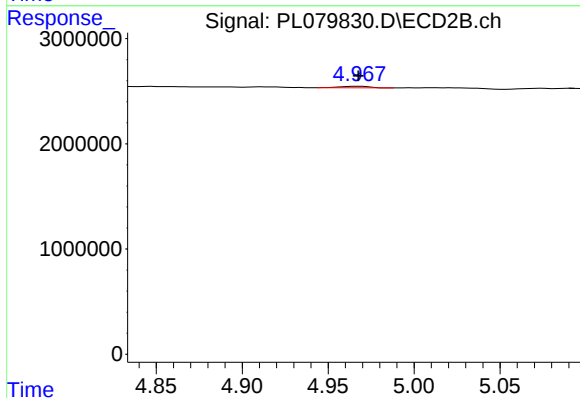


#12 4,4'-DDE

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 176041
Conc: 0.05 ng/ml

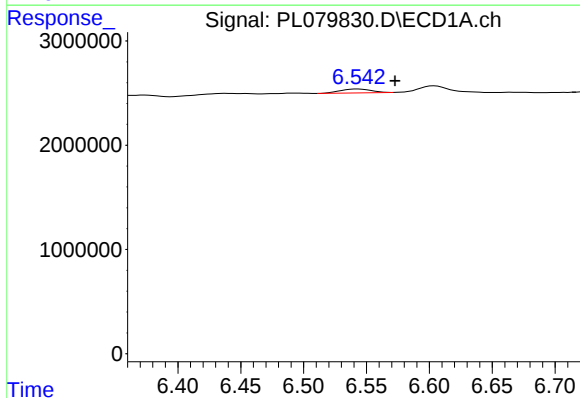


#15 Endosulfan II

R.T.: 6.543 min
Delta R.T.: -0.030 min
Response: 638661
Conc: 0.26 ng/ml

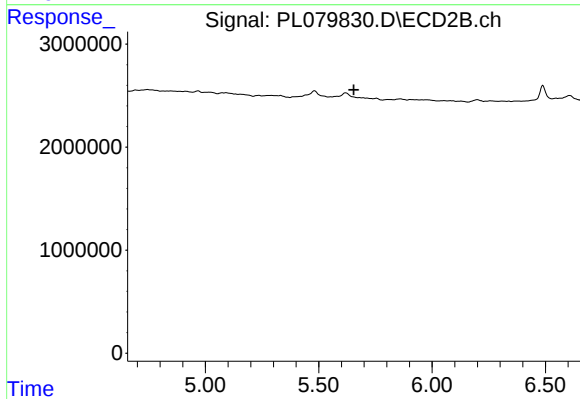

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.655 min
Response: 0
Conc: N.D.

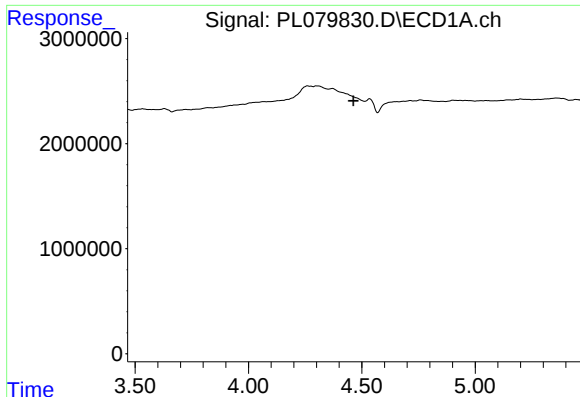

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

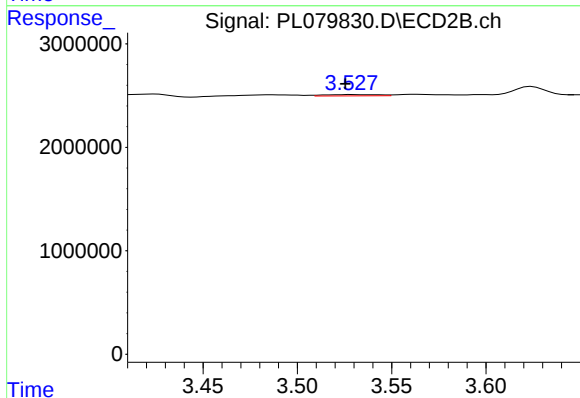


#23 Chlordane-1

R.T.: 3.529 min
Delta R.T.: 0.003 min
Response: 252023
Conc: 2.41 ng/ml

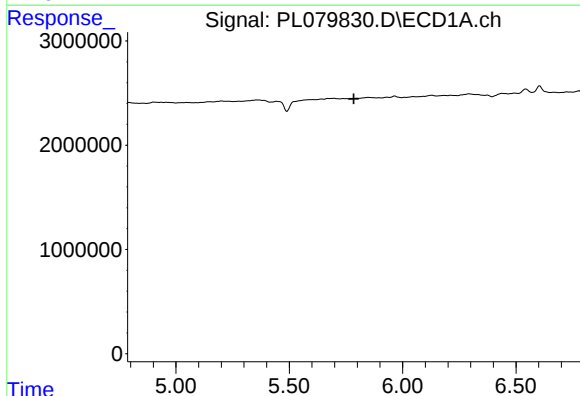


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.784 min
Response: 0
Conc: N.D.

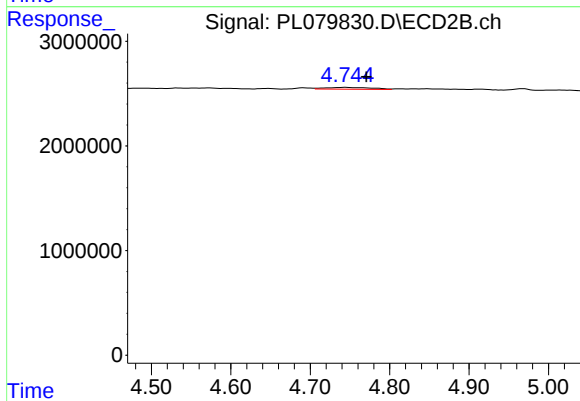

#26 Chlordane-4


R.T.: 4.745 min
Delta R.T.: -0.026 min
Response: 693704
Conc: 1.91 ng/ml

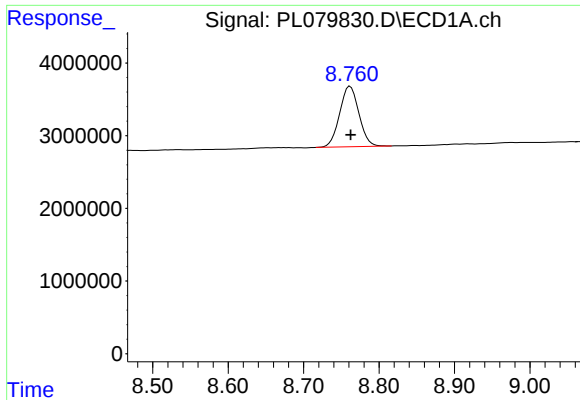

#28 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 14787281
Conc: 7.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

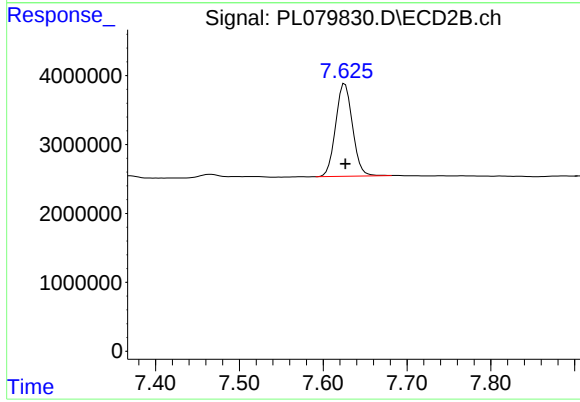

#28 Decachlorobiphenyl

R.T.: 7.626 min
Delta R.T.: 0.000 min
Response: 18807716
Conc: 7.83 ng/ml