

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122122\
 Data File : PL079831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 13:55
 Operator : AR\AJ
 Sample : N6157-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 21:35:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 10:00:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.562	19125389	24117485	8.703	9.085
28)	SA Decachlor...	8.762	7.626	17947139	22890049	9.676	9.536
Target Compounds							
5)	MB Aldrin	0.000	3.996f	0	212952	N.D.	0.056 #
8)	B Heptachlo...	5.463	4.481f	925152	82912	0.349	0.024 #
9)	A Endosulfan I	5.844	0.000	175962	0	0.068	N.D. #
10)	B gamma-Chl...	0.000	4.740f	0	590156	N.D.	0.169 #
12)	B 4,4'-DDE	5.966	4.966	258525	331817	0.107	0.103
13)	MA Dieldrin	0.000	5.094	0	480308	N.D.	0.139 #
15)	B Endosulfa...	6.543f	0.000	630731	0	0.259	N.D. #
25)	Chlordane-3	0.000	4.740f	0	590156	N.D.	1.748 #
27)	Chlordane-5	0.000	5.449f	0	12559	N.D.	0.140 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122122\
Data File : PL079831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 13:55
Operator : AR\AJ
Sample : N6157-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 21:35:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 10:00:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

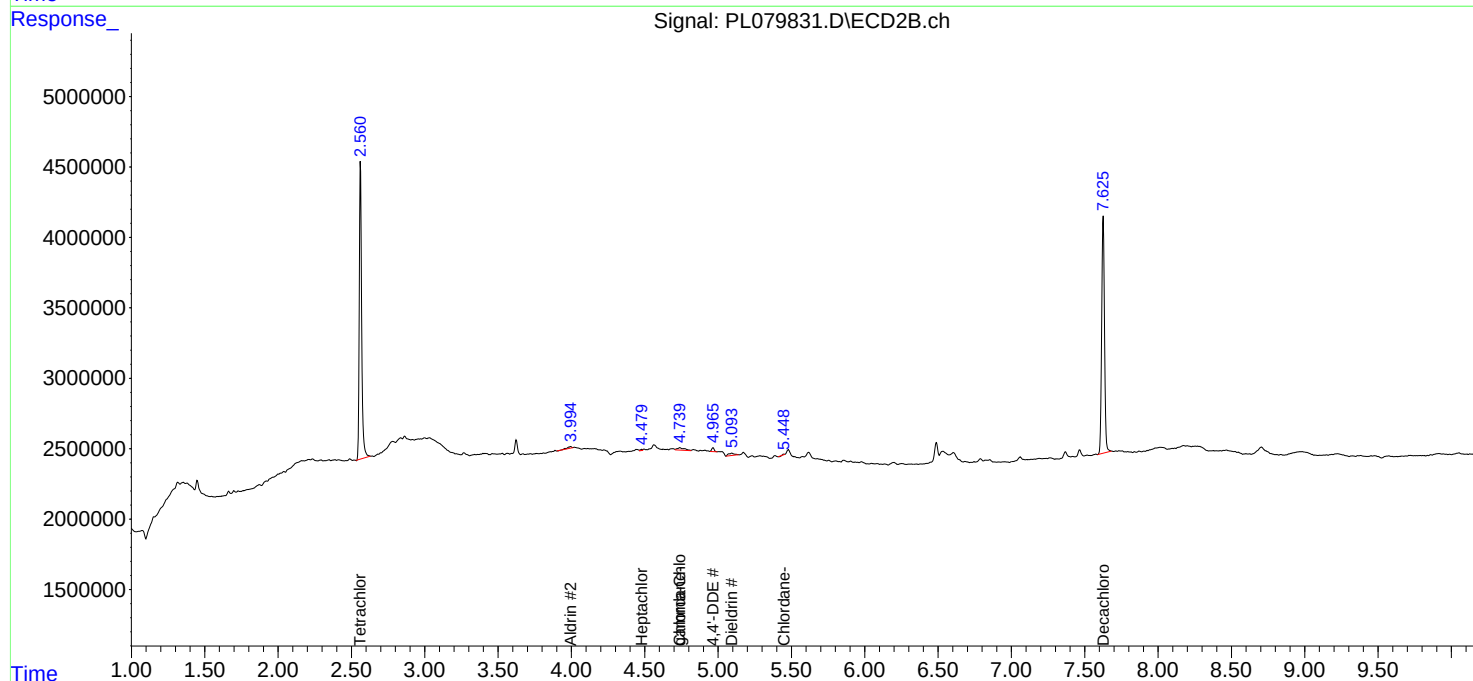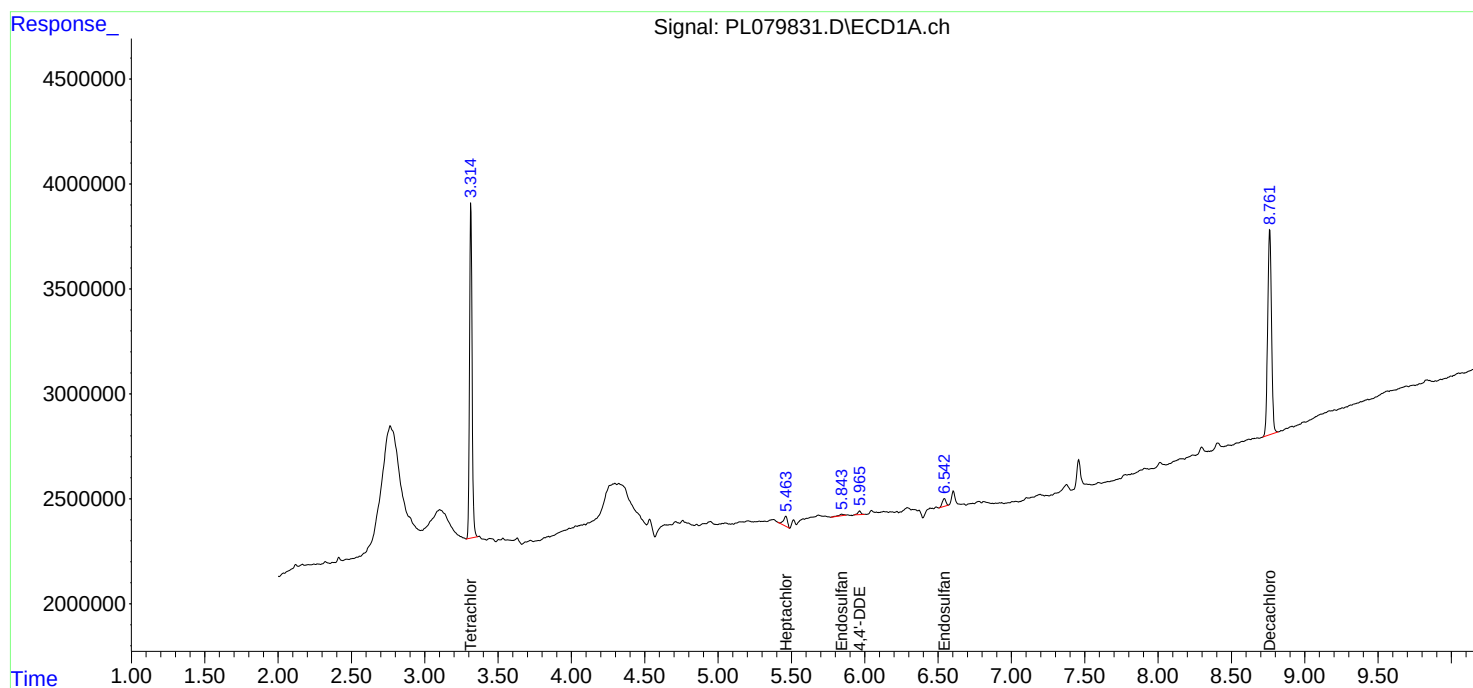


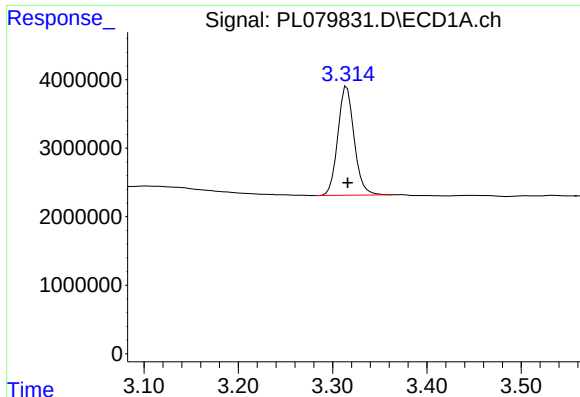

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 19125389
Conc: 8.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

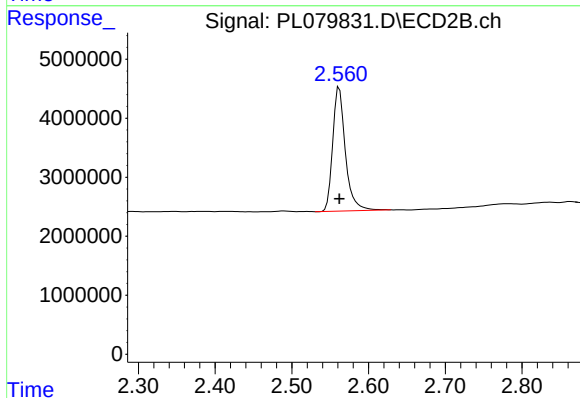


#1 Tetrachloro-m-xylene

R.T.: 2.562 min
Delta R.T.: 0.000 min
Response: 24117485
Conc: 9.09 ng/ml

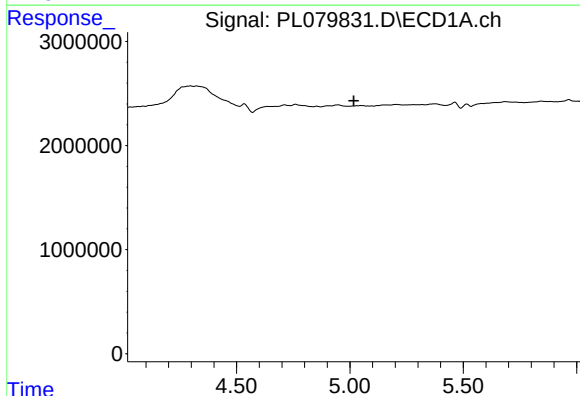


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.017 min
Response: 0
Conc: N.D.

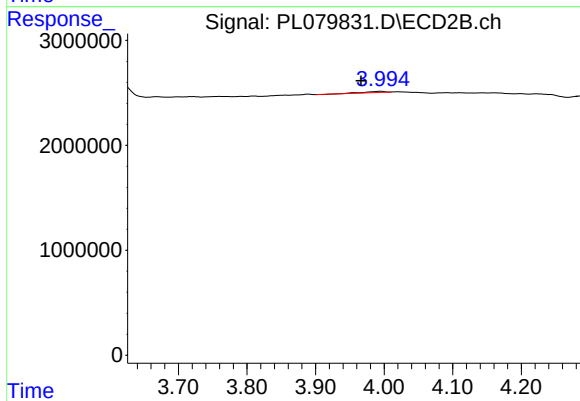

#5 Aldrin


R.T.: 3.996 min
Delta R.T.: 0.029 min
Response: 212952
Conc: 0.06 ng/ml

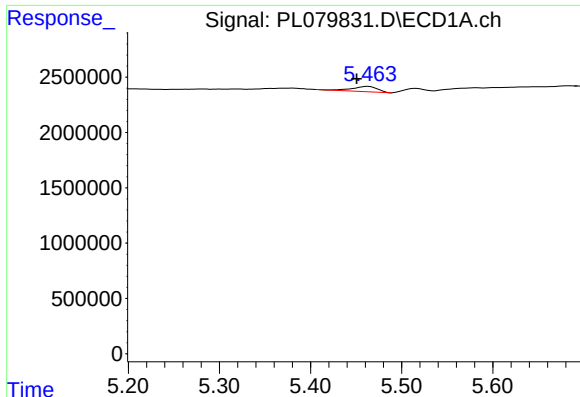

#8 Heptachlor epoxide


R.T.: 5.463 min
Delta R.T.: 0.013 min
Response: 925152
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

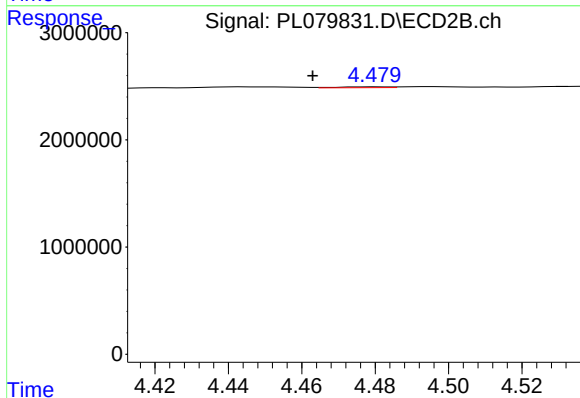


#8 Heptachlor epoxide

R.T.: 4.481 min
Delta R.T.: 0.018 min
Response: 82912
Conc: 0.02 ng/ml

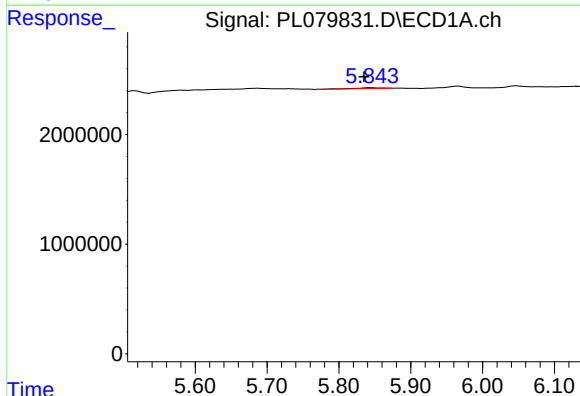


#9 Endosulfan I

R.T.: 5.844 min
Delta R.T.: 0.009 min
Response: 175962
Conc: 0.07 ng/ml

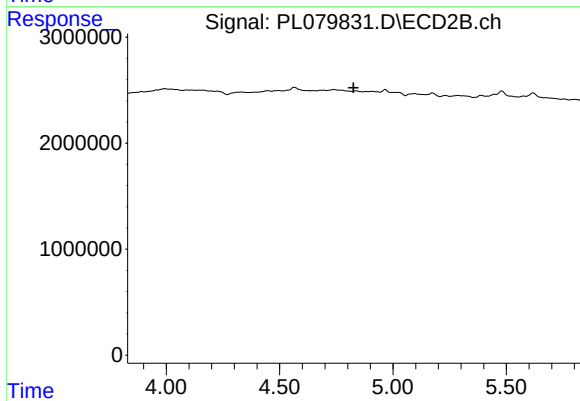

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 4.826 min
Response: 0
Conc: N.D.

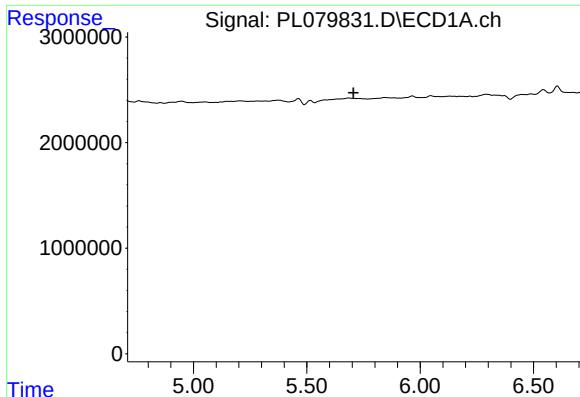

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

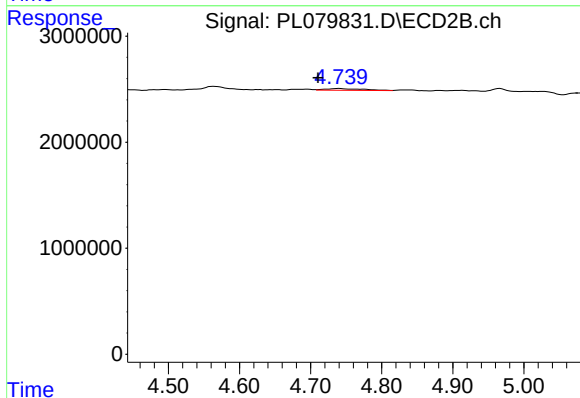


#10 gamma-Chlordane

R.T.: 4.740 min
Delta R.T.: 0.030 min
Response: 590156
Conc: 0.17 ng/ml

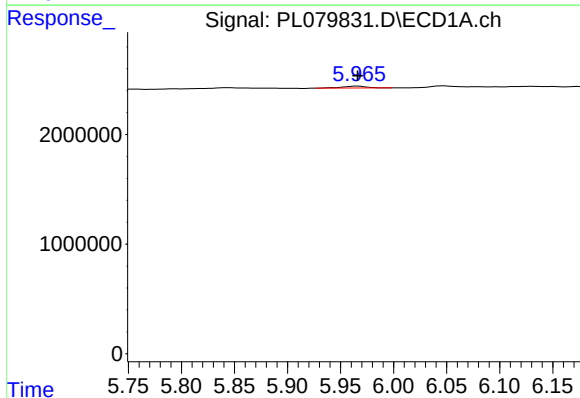


#12 4,4'-DDE

R.T.: 5.966 min
Delta R.T.: 0.000 min
Response: 258525
Conc: 0.11 ng/ml

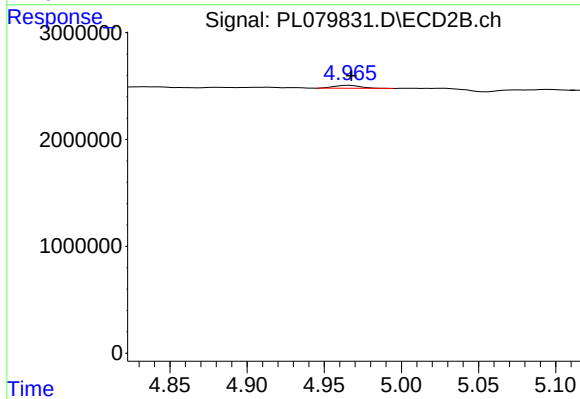

#12 4,4'-DDE


R.T.: 4.966 min
Delta R.T.: -0.001 min
Response: 331817
Conc: 0.10 ng/ml

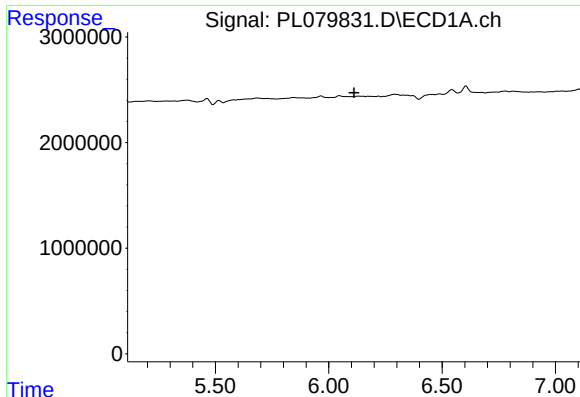

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.112 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

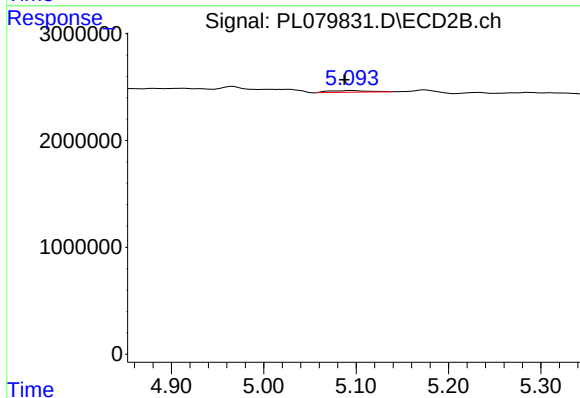


#13 Dieldrin

R.T.: 5.094 min
Delta R.T.: 0.007 min
Response: 480308
Conc: 0.14 ng/ml

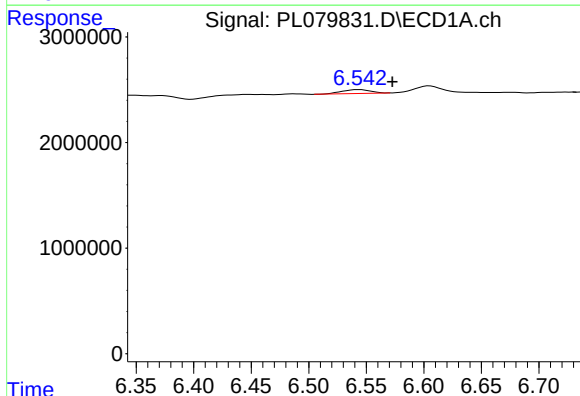


#15 Endosulfan II

R.T.: 6.543 min
Delta R.T.: -0.029 min
Response: 630731
Conc: 0.26 ng/ml

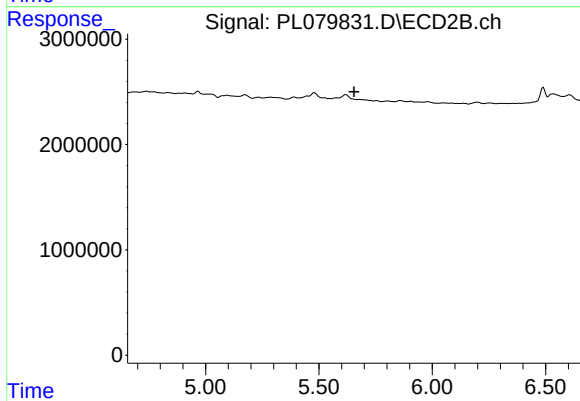

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.655 min
Response: 0
Conc: N.D.

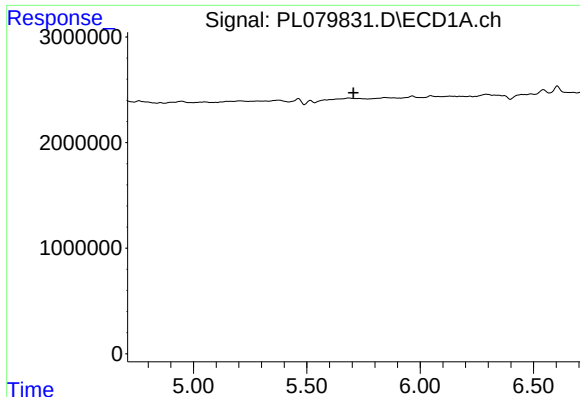

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

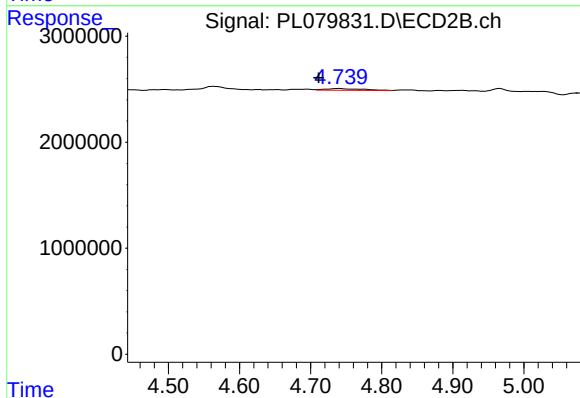


#25 Chlordane-3

R.T.: 4.740 min
Delta R.T.: 0.029 min
Response: 590156
Conc: 1.75 ng/ml

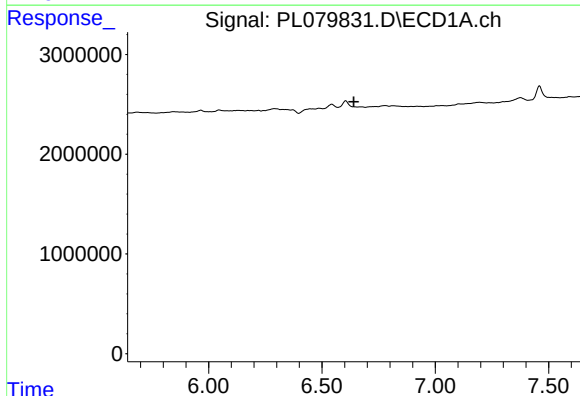


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.641 min
Response: 0
Conc: N.D.

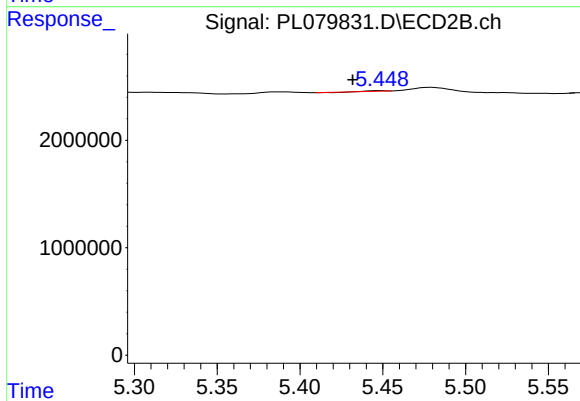

#27 Chlordane-5


R.T.: 5.449 min
Delta R.T.: 0.017 min
Response: 12559
Conc: 0.14 ng/ml

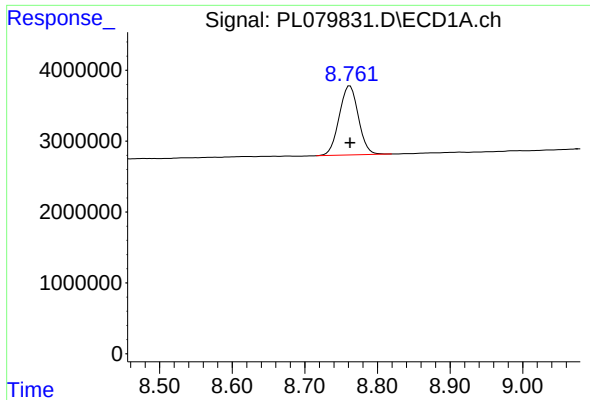

#28 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.000 min
Response: 17947139
Conc: 9.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

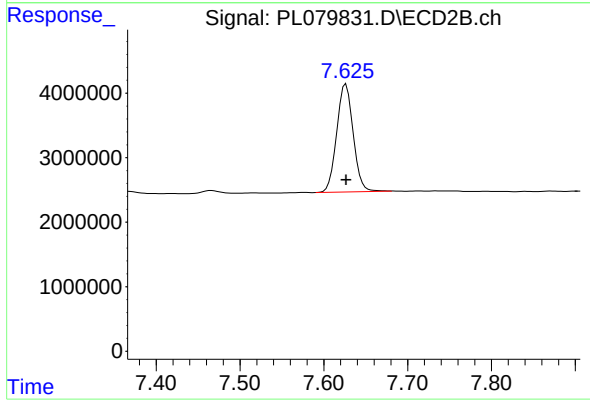

#28 Decachlorobiphenyl

R.T.: 7.626 min
Delta R.T.: 0.000 min
Response: 22890049
Conc: 9.54 ng/ml