

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122123\
 Data File : PL087360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 23:59
 Operator : AR\AJ
 Sample : 05970-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-12202023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:38:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.679	23651745	9933047	6.285	5.901
28)	SA Decachlor...	8.979	7.867	19335283	7881196	5.670	4.666
Target Compounds							
3)	MA gamma-BHC...	0.000	3.546f	0	174049	N.D.	0.072 #
4)	MA Heptachlor	4.832f	3.854	453339	41941	0.085	0.018 #
5)	MB Aldrin	0.000	4.133	0	111236	N.D.	0.046 #
7)	B delta-BHC	0.000	4.053	0	50229	N.D.	0.021 #
9)	A Endosulfan I	0.000	5.027	0	12618106	N.D.	5.839 #
10)	B gamma-Chl...	0.000	4.921f	0	581993	N.D.	0.254 #
11)	B alpha-Chl...	5.917	0.000	857518	0	0.178	N.D. #
12)	B 4,4'-DDE	6.096	5.159	2464911	794175	0.595	0.400 #
13)	MA Dieldrin	0.000	5.286	0	62636	N.D.	0.028 #
14)	MA Endrin	0.000	5.580	0	170979	N.D.	0.086 #
16)	A 4,4'-DDD	0.000	5.717	0	152257	N.D.	0.092 #
17)	MA 4,4'-DDT	0.000	5.968	0	347156	N.D.	0.188 #
18)	B Endrin al...	0.000	6.063f	0	88932	N.D.	0.061 #
19)	B Endosulfa...	0.000	6.266	0	54814	N.D.	0.029 #
23)	Chlordane-1	0.000	3.679	0	254048	N.D.	4.095 #
24)	Chlordane-2	0.000	4.263	0	167139	N.D.	2.177 #
25)	Chlordane-3	0.000	4.921f	0	581993	N.D.	2.633 #
26)	Chlordane-4	5.917	0.000	857518	0	1.003	N.D. #
27)	Chlordane-5	0.000	5.635	0	92350	N.D.	1.427 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122123\
Data File : PL087360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 23:59
Operator : AR\AJ
Sample : 05970-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:38:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

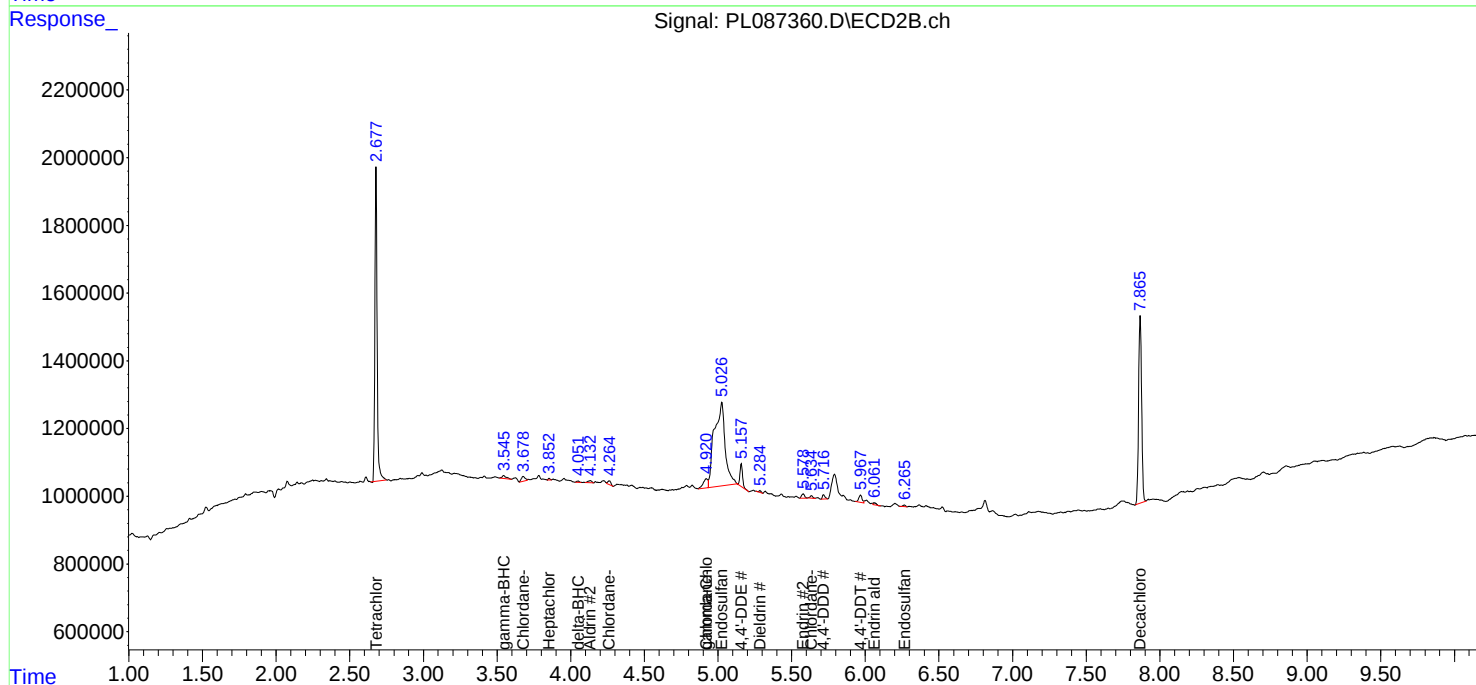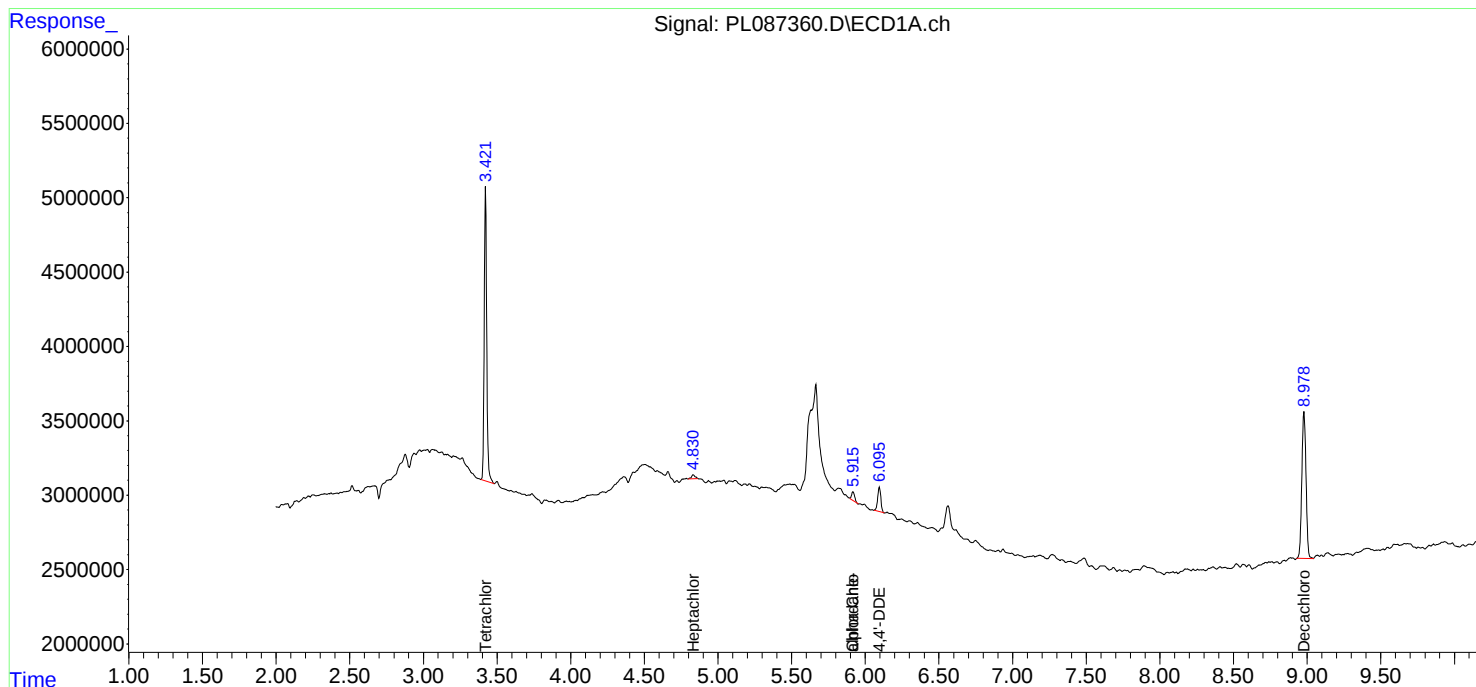


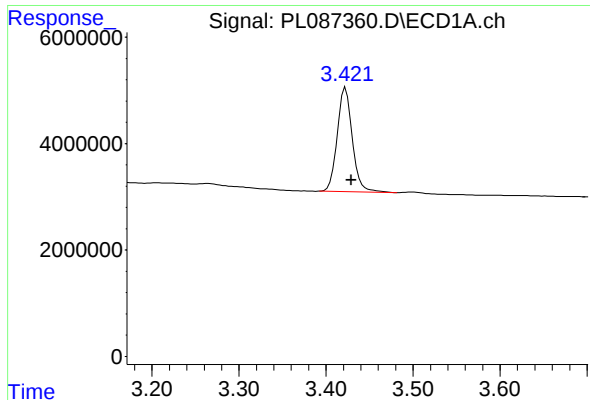

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 23651745
Conc: 6.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

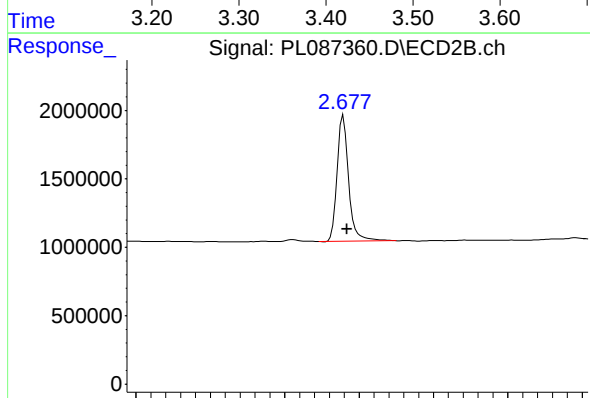


#1 Tetrachloro-m-xylene

R.T.: 2.679 min
Delta R.T.: -0.005 min
Response: 9933047
Conc: 5.90 ng/ml

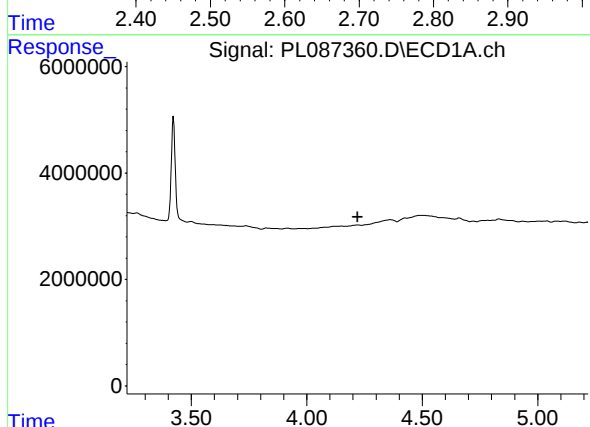


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.220 min
Response: 0
Conc: N.D.

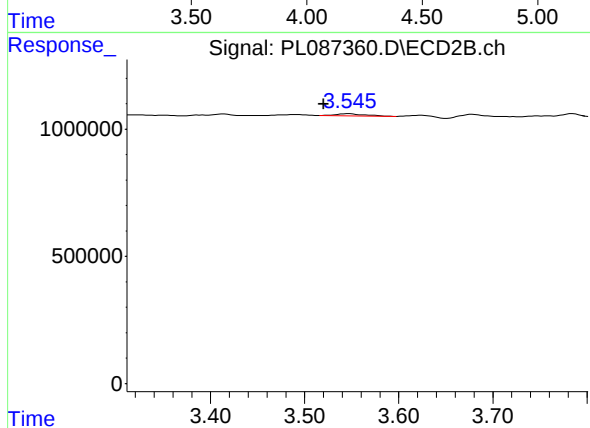

#3 gamma-BHC (Lindane)


R.T.: 3.546 min
Delta R.T.: 0.026 min
Response: 174049
Conc: 0.07 ng/ml

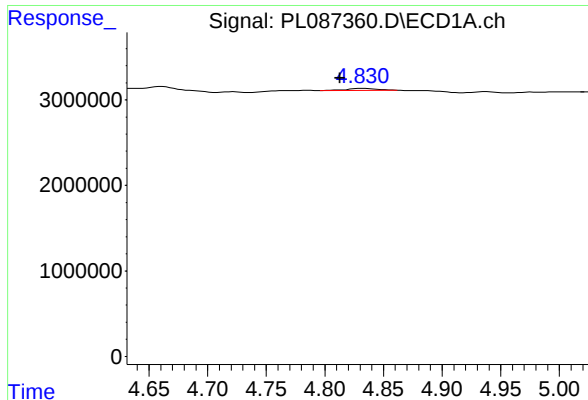

#4 Heptachlor


R.T.: 4.832 min
Delta R.T.: 0.019 min
Response: 453339
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

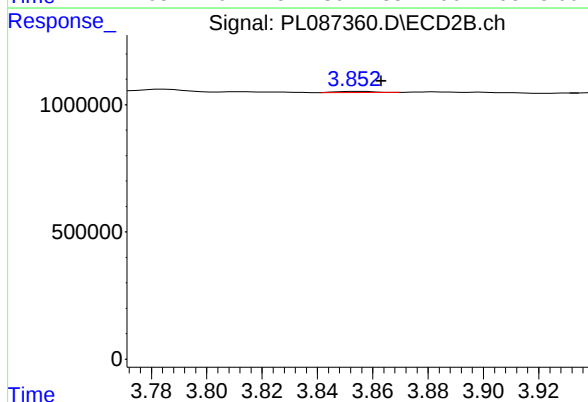


#4 Heptachlor

R.T.: 3.854 min
Delta R.T.: -0.009 min
Response: 41941
Conc: 0.02 ng/ml

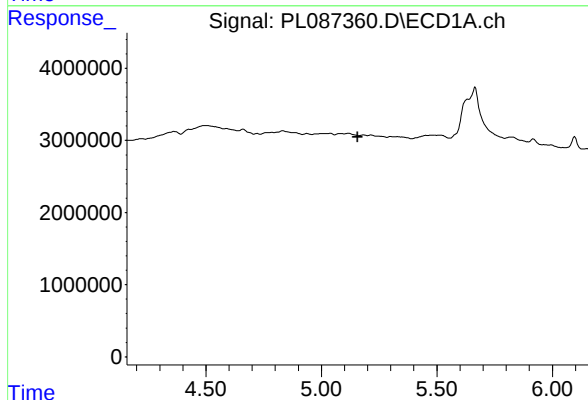


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.156 min
Response: 0
Conc: N.D.

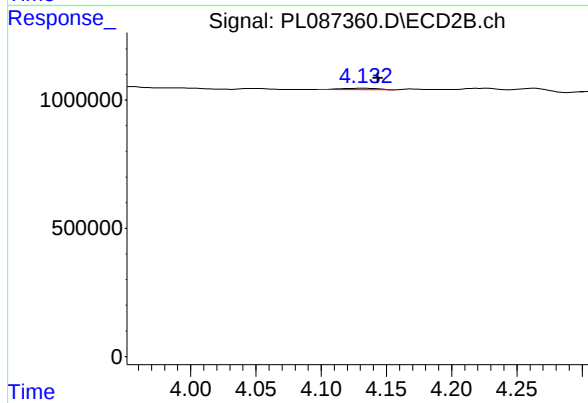

#5 Aldrin


R.T.: 4.133 min
Delta R.T.: -0.010 min
Response: 111236
Conc: 0.05 ng/ml

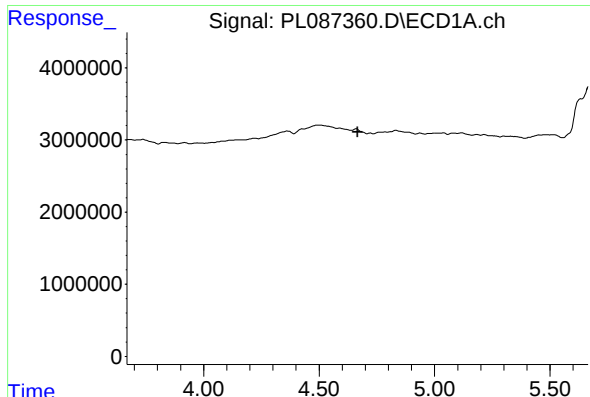

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

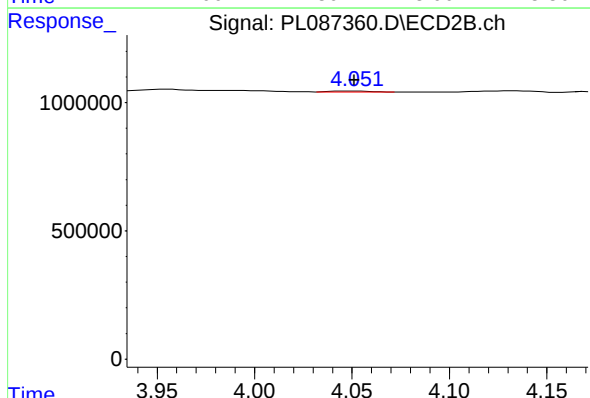


#7 delta-BHC

R.T.: 4.053 min
Delta R.T.: 0.001 min
Response: 50229
Conc: 0.02 ng/ml

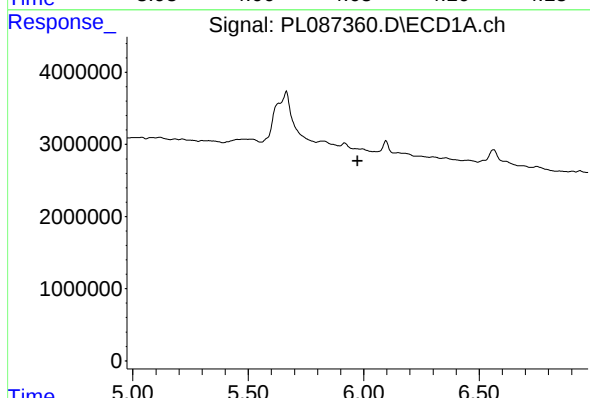


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.973 min
Response: 0
Conc: N.D.

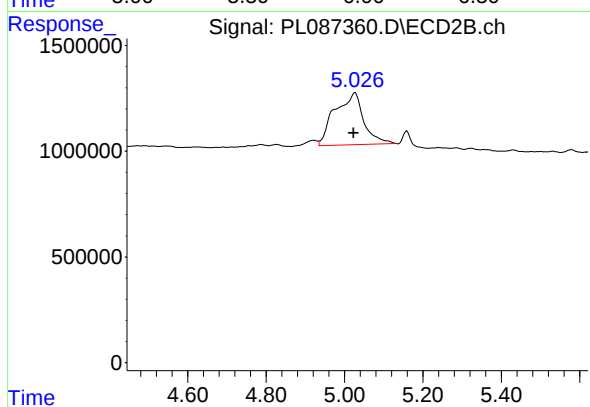

#9 Endosulfan I


R.T.: 5.027 min
Delta R.T.: 0.004 min
Response: 12618106
Conc: 5.84 ng/ml

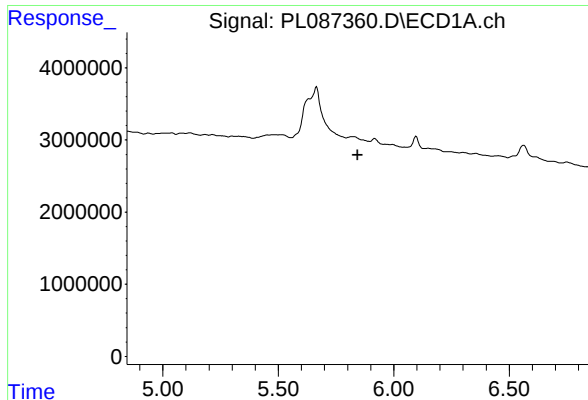

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

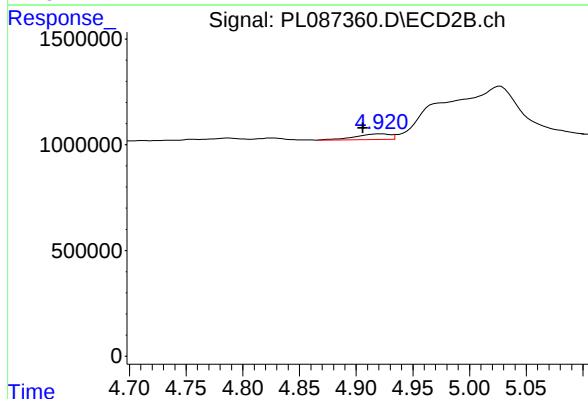


#10 gamma-Chlordane

R.T.: 4.921 min
Delta R.T.: 0.015 min
Response: 581993
Conc: 0.25 ng/ml

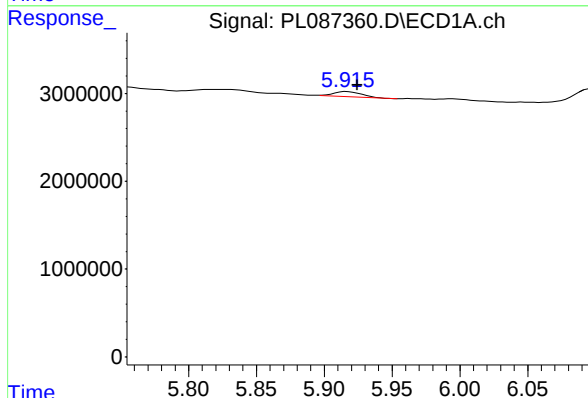


#11 alpha-Chlordane

R.T.: 5.917 min
Delta R.T.: -0.008 min
Response: 857518
Conc: 0.18 ng/ml

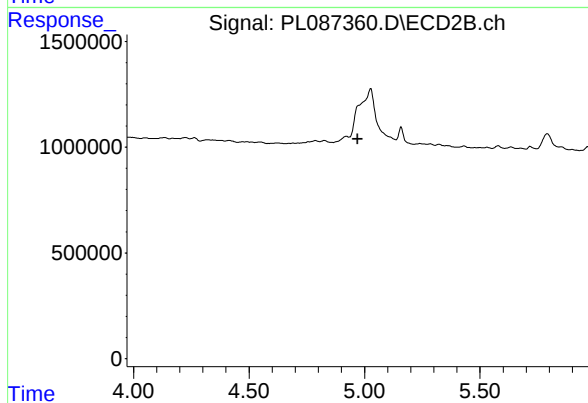

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.970 min
Response: 0
Conc: N.D.

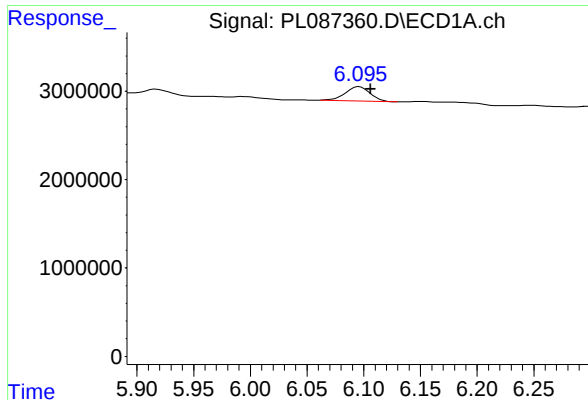

#12 4,4'-DDE


R.T.: 6.096 min
Delta R.T.: -0.010 min
Response: 2464911
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

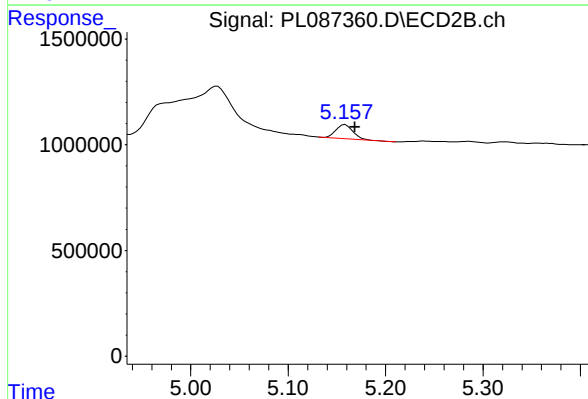


#12 4,4'-DDE

R.T.: 5.159 min
Delta R.T.: -0.010 min
Response: 794175
Conc: 0.40 ng/ml

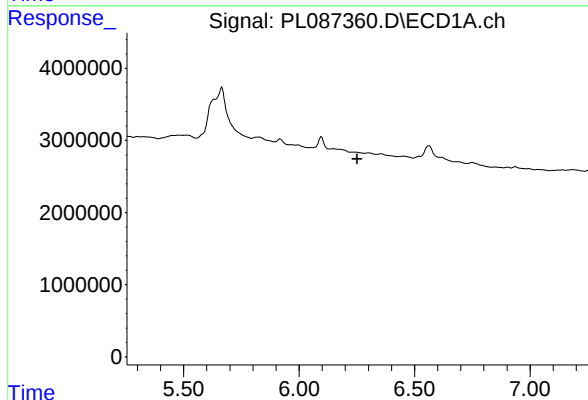


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.251 min
Response: 0
Conc: N.D.

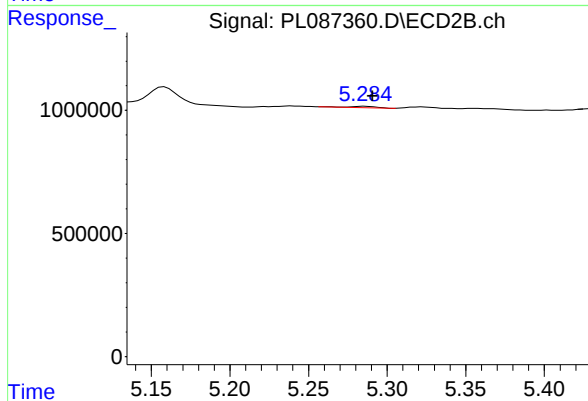

#13 Dieldrin


R.T.: 5.286 min
Delta R.T.: -0.005 min
Response: 62636
Conc: 0.03 ng/ml

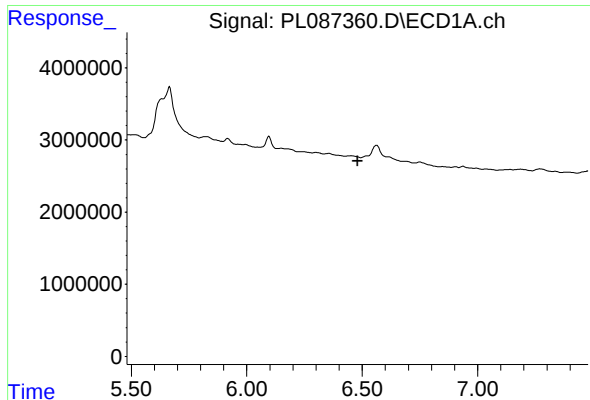

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

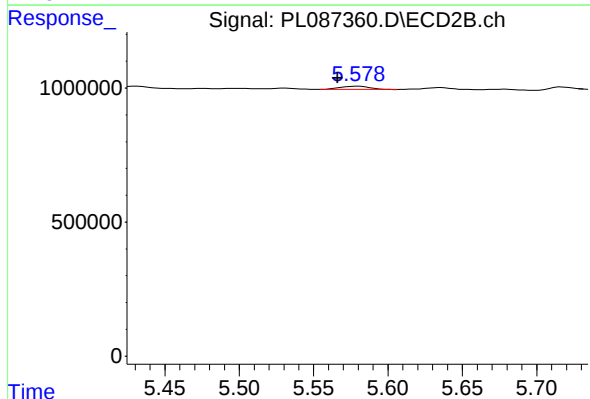


#14 Endrin

R.T.: 5.580 min
Delta R.T.: 0.013 min
Response: 170979
Conc: 0.09 ng/ml

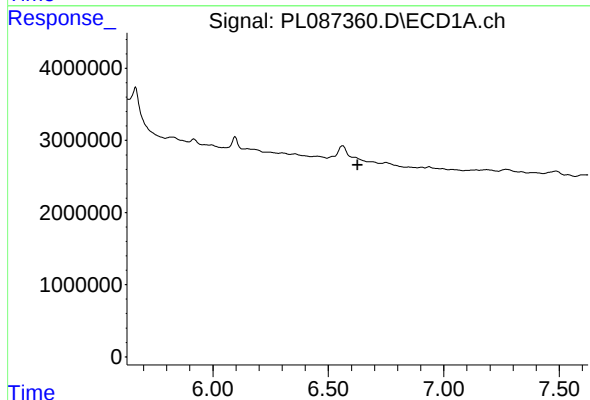


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.626 min
Response: 0
Conc: N.D.

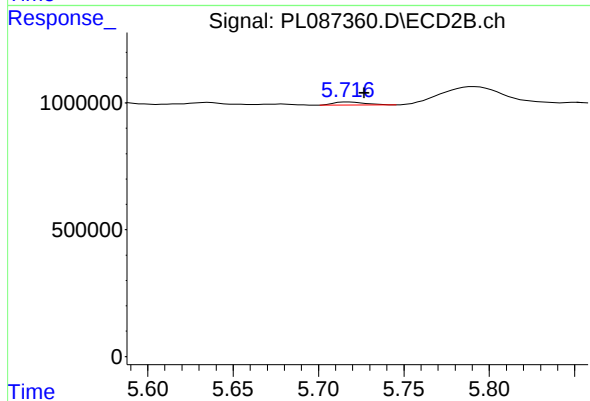

#16 4,4'-DDD


R.T.: 5.717 min
Delta R.T.: -0.010 min
Response: 152257
Conc: 0.09 ng/ml

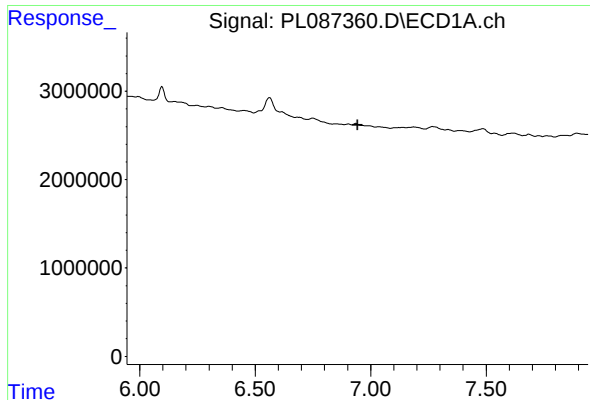

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

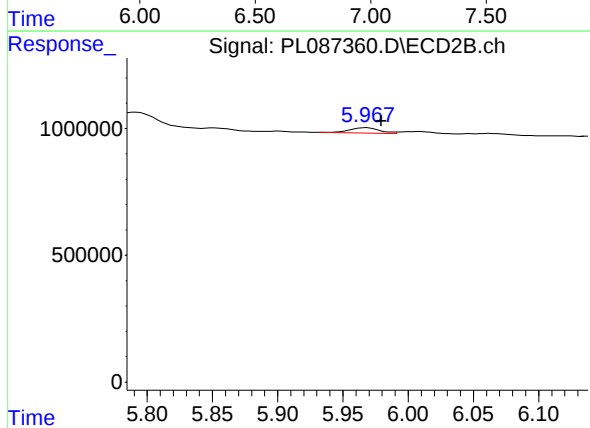


#17 4,4'-DDT

R.T.: 5.968 min
Delta R.T.: -0.011 min
Response: 347156
Conc: 0.19 ng/ml

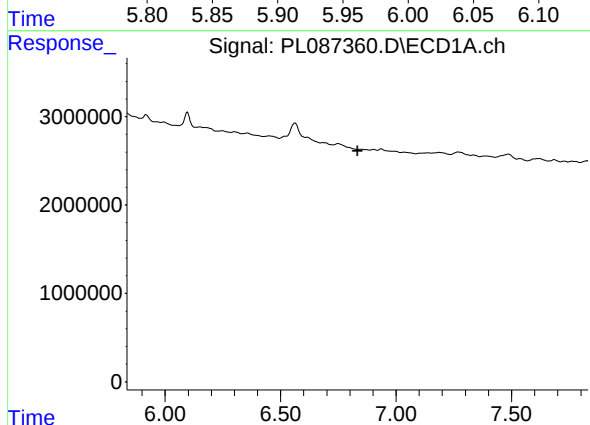


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.833 min
Response: 0
Conc: N.D.

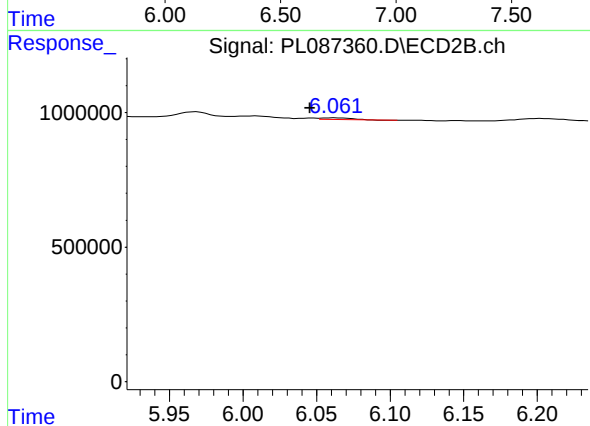

#18 Endrin aldehyde


R.T.: 6.063 min
Delta R.T.: 0.018 min
Response: 88932
Conc: 0.06 ng/ml

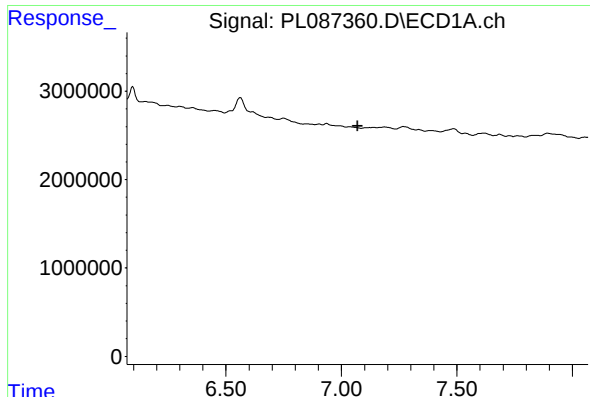

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

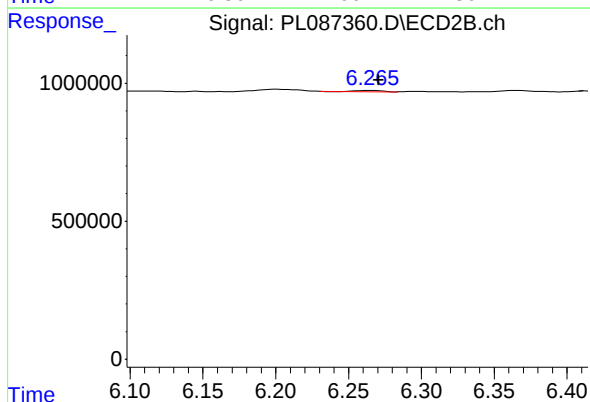


#19 Endosulfan Sulfate

R.T.: 6.266 min
Delta R.T.: -0.004 min
Response: 54814
Conc: 0.03 ng/ml

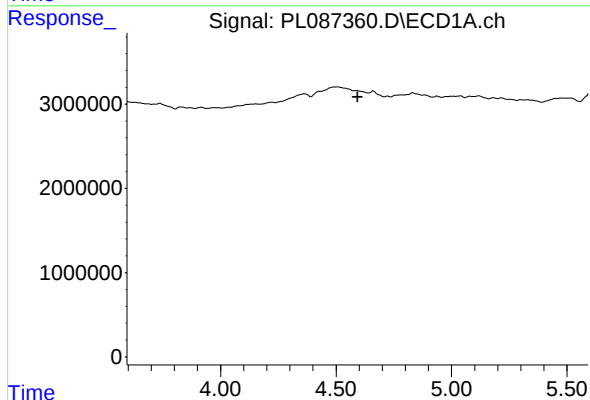


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.594 min
Response: 0
Conc: N.D.

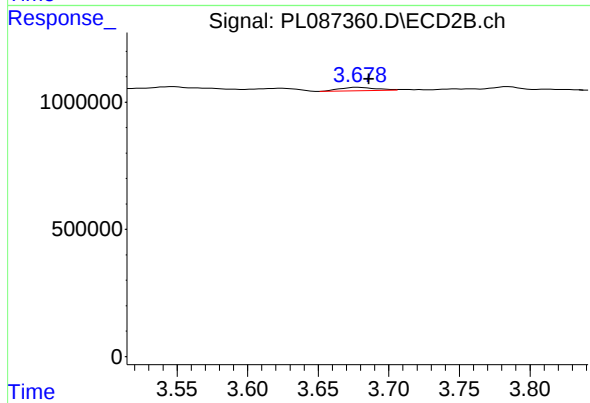

#23 Chlordane-1


R.T.: 3.679 min
Delta R.T.: -0.007 min
Response: 254048
Conc: 4.10 ng/ml

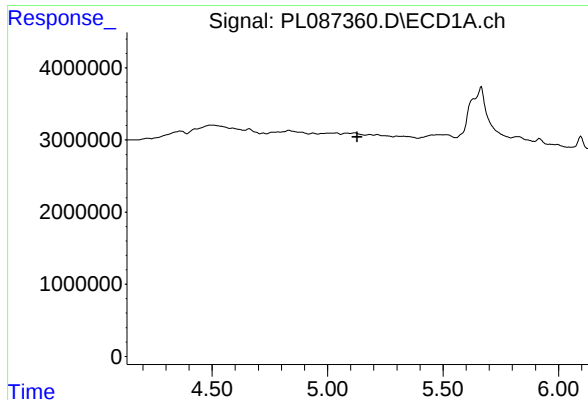

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

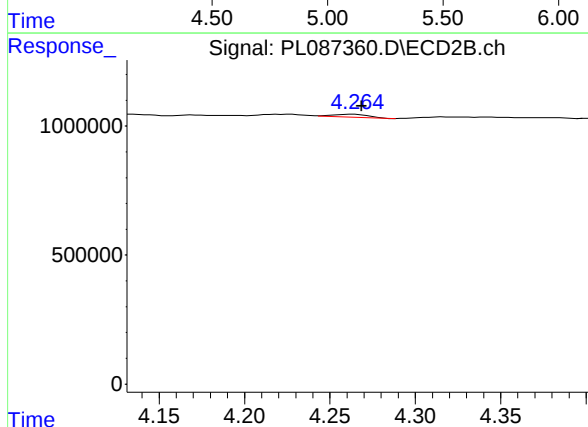


#24 Chlordane-2

R.T.: 4.263 min
Delta R.T.: -0.005 min
Response: 167139
Conc: 2.18 ng/ml

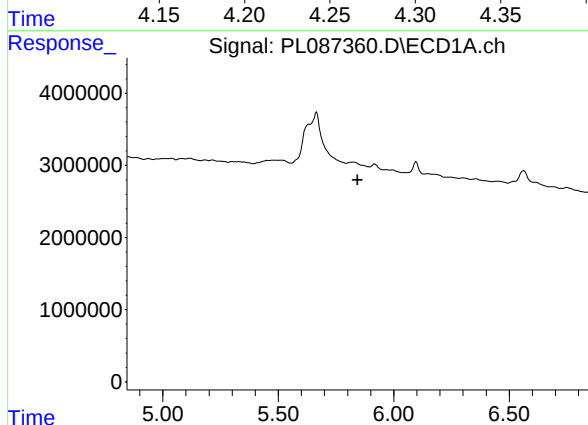


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.843 min
Response: 0
Conc: N.D.

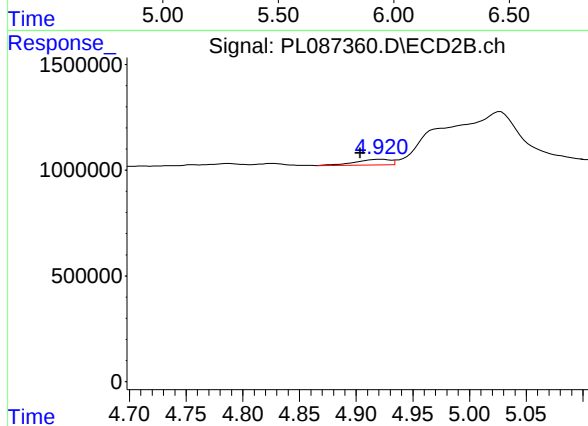

#25 Chlordane-3


R.T.: 4.921 min
Delta R.T.: 0.017 min
Response: 581993
Conc: 2.63 ng/ml

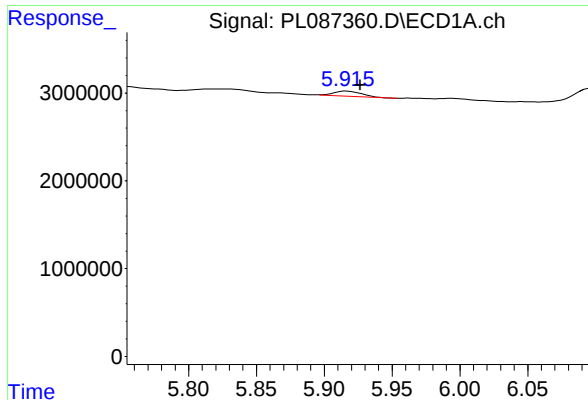

#26 Chlordane-4


R.T.: 5.917 min
Delta R.T.: -0.010 min
Response: 857518
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

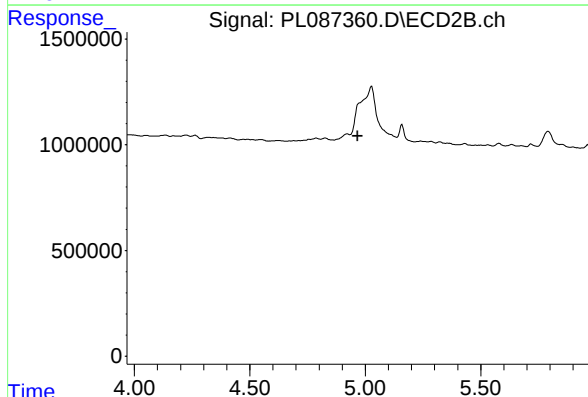


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 4.967 min
Response: 0
Conc: N.D.

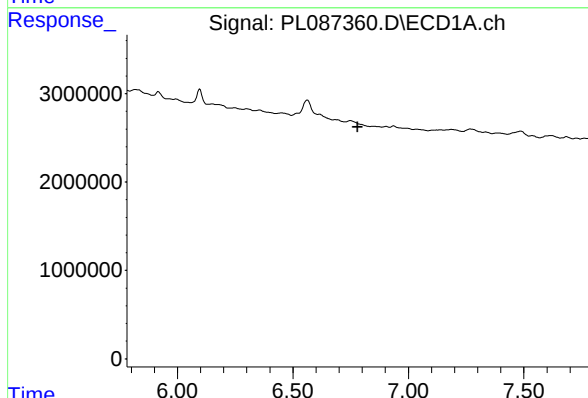


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.779 min
Response: 0
Conc: N.D.

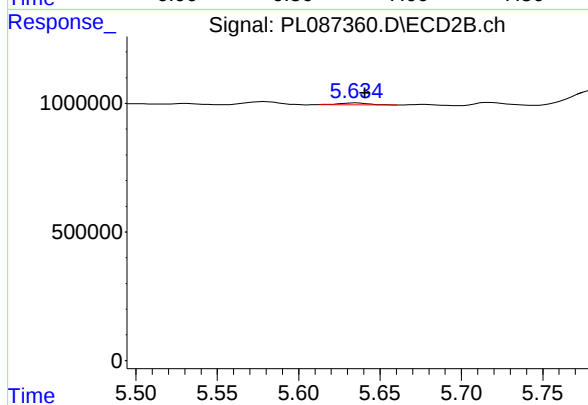

#27 Chlordane-5


R.T.: 5.635 min
Delta R.T.: -0.006 min
Response: 92350
Conc: 1.43 ng/ml

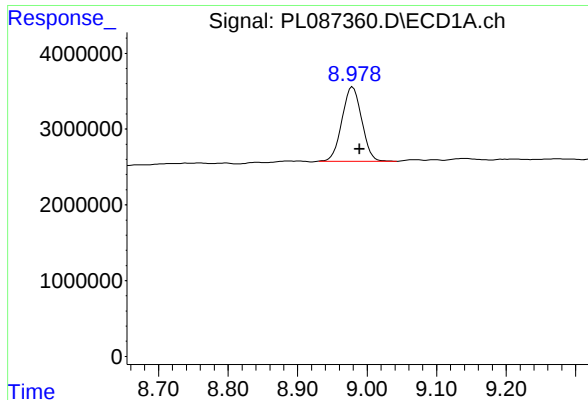

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.010 min
Response: 19335283
Conc: 5.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

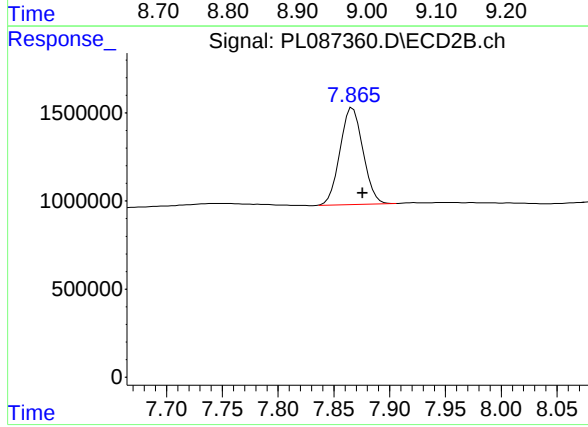

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: -0.009 min
Response: 7881196
Conc: 4.67 ng/ml