

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122123\
 Data File : PL087349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 20:44
 Operator : AR\AJ
 Sample : 05900-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GHL-SS-63

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/22/2023
 Supervised By : Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:35:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.677	32206944	14379675	8.558	8.543
28)	SA Decachlor...	8.978	7.868	16468704	7719264	4.830m	4.570
Target Compounds							
13)	MA Dieldrin	6.240	5.285	5510125	5412067	1.187m	2.429m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122123\
Data File : PL087349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 20:44
Operator : AR\AJ
Sample : 05900-10
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GHL-SS-63


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/22/2023
Supervised By : Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:35:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

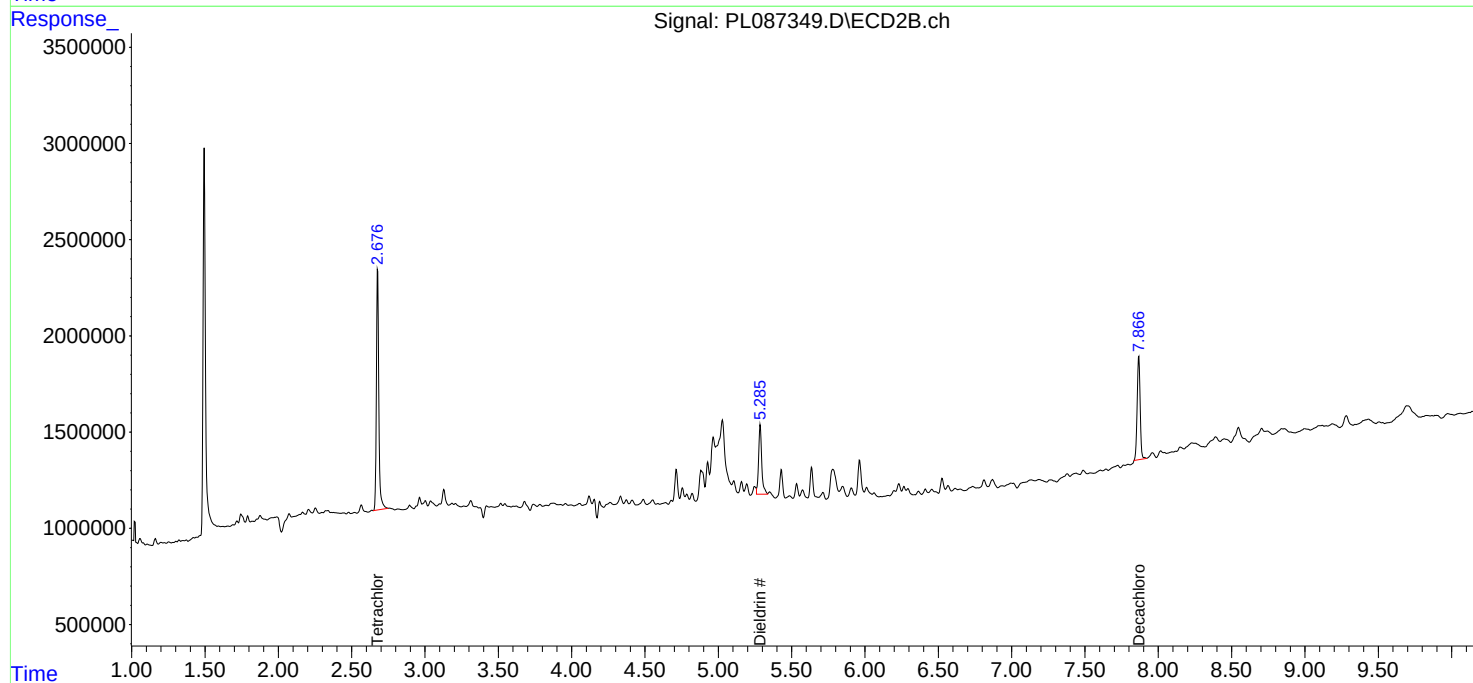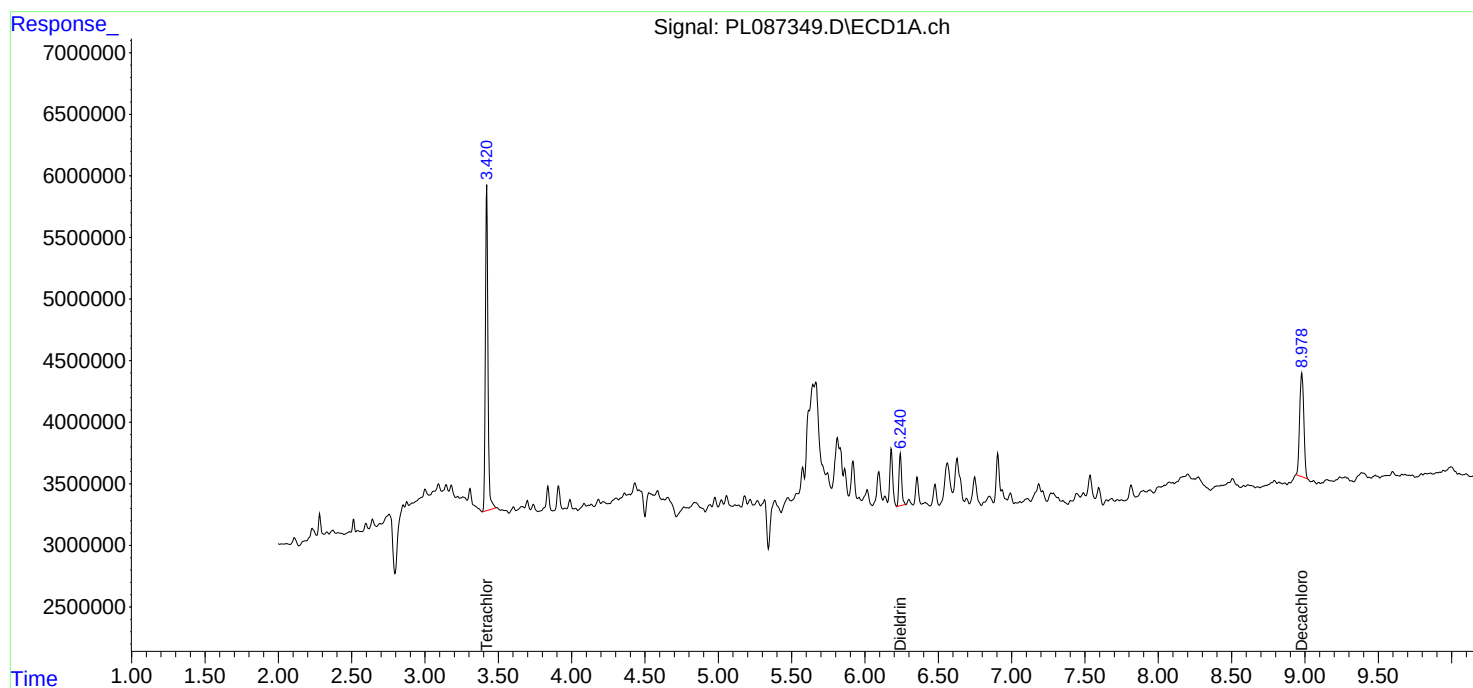

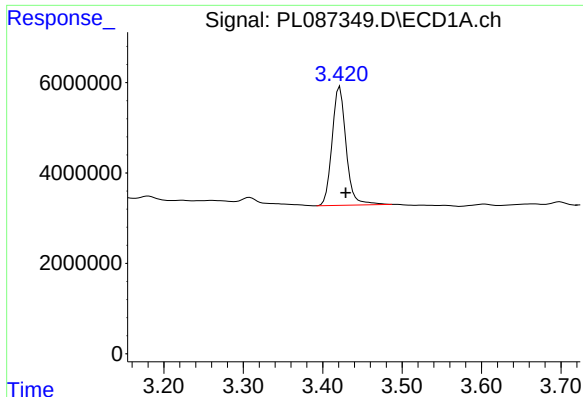


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 32206944
Conc: 8.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
GHL-SS-63


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

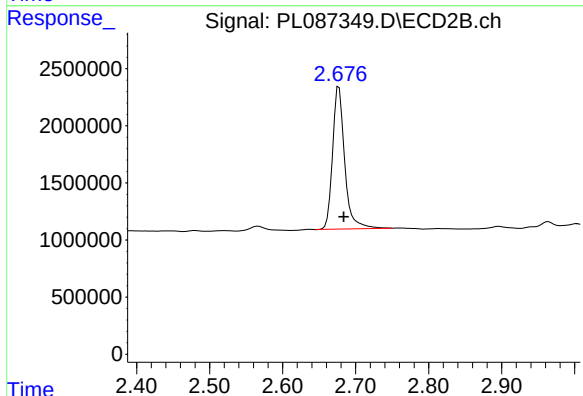


#1 Tetrachloro-m-xylene

R.T.: 2.677 min
Delta R.T.: -0.006 min
Response: 14379675
Conc: 8.54 ng/ml

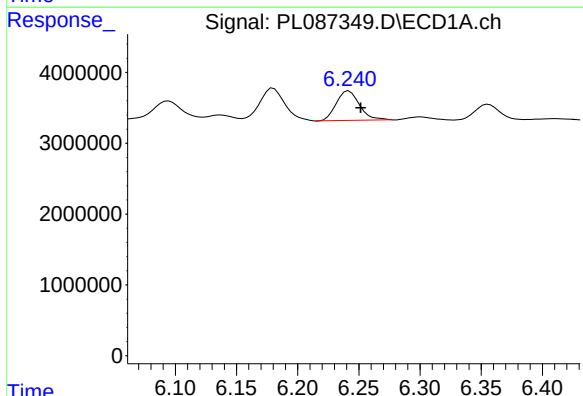


#13 Dieldrin

R.T.: 6.240 min
Delta R.T.: -0.011 min
Response: 5510125
Conc: 1.19 ng/ml m

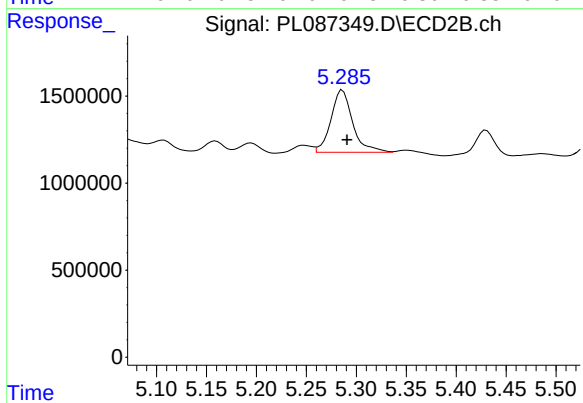

#13 Dieldrin

R.T.: 5.285 min
Delta R.T.: -0.006 min
Response: 5412067
Conc: 2.43 ng/ml m

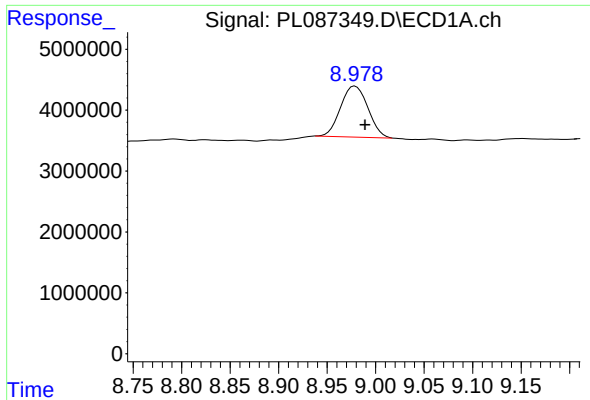


#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.012 min
Response: 16468704
Conc: 4.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
GHL-SS-63

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

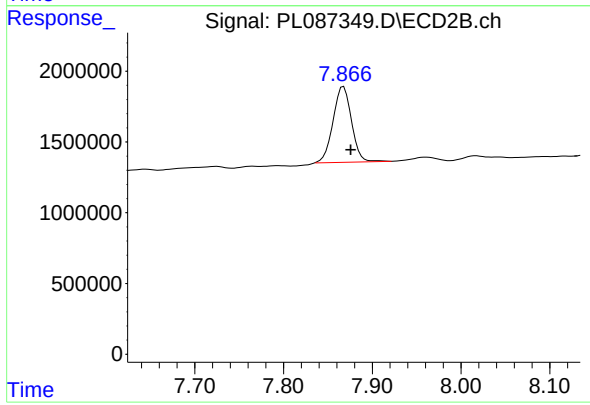

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: -0.008 min
Response: 7719264
Conc: 4.57 ng/ml