

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122123\
 Data File : PL087360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 23:59
 Operator : AR\AJ
 Sample : 05970-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-12202023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/22/2023
 Supervised By : Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 01:38:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.679	23651745	9933047	6.285	5.901
28)	SA Decachlor...	8.979	7.867	19335283	7881196	5.670	4.666
Target Compounds							
12)	B 4,4'-DDE	6.096	5.157	2464911	807188	0.595	0.407m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122123\
Data File : PL087360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 23:59
Operator : AR\AJ
Sample : 05970-01
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-12202023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 01:38:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

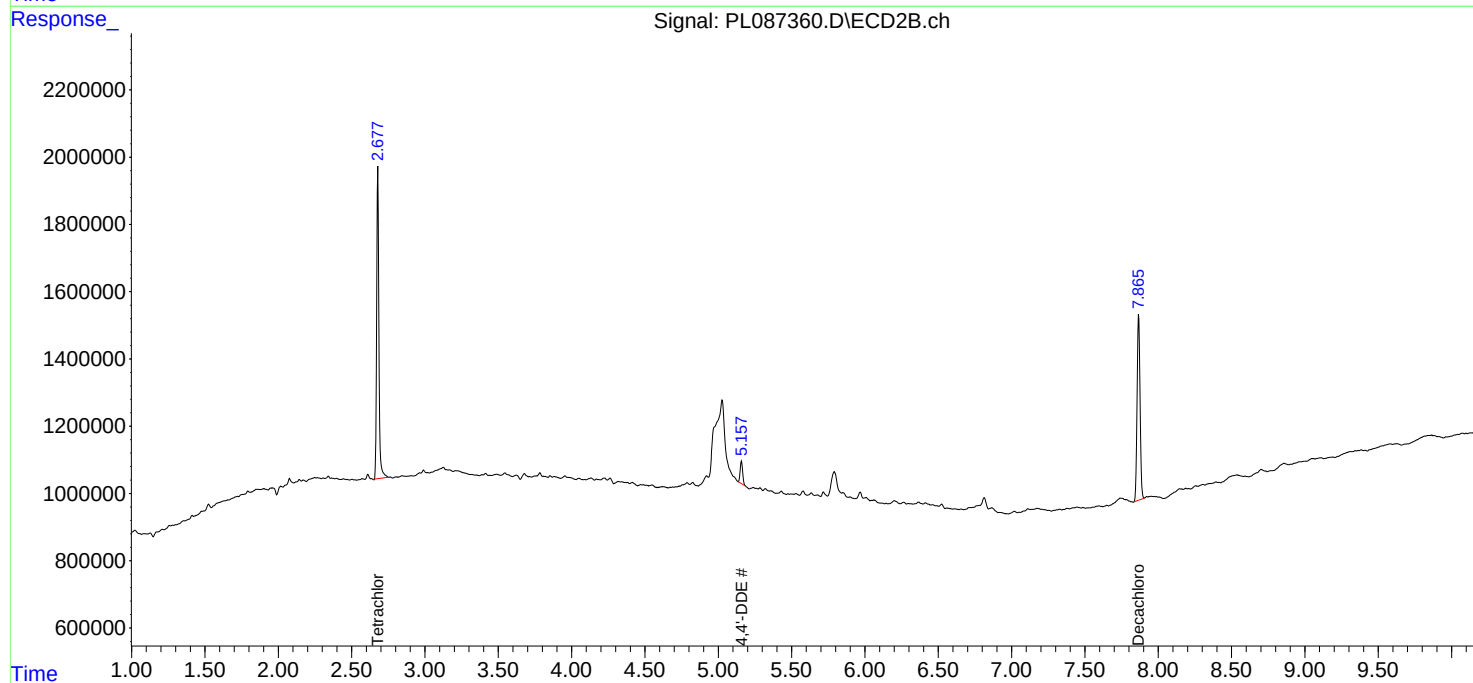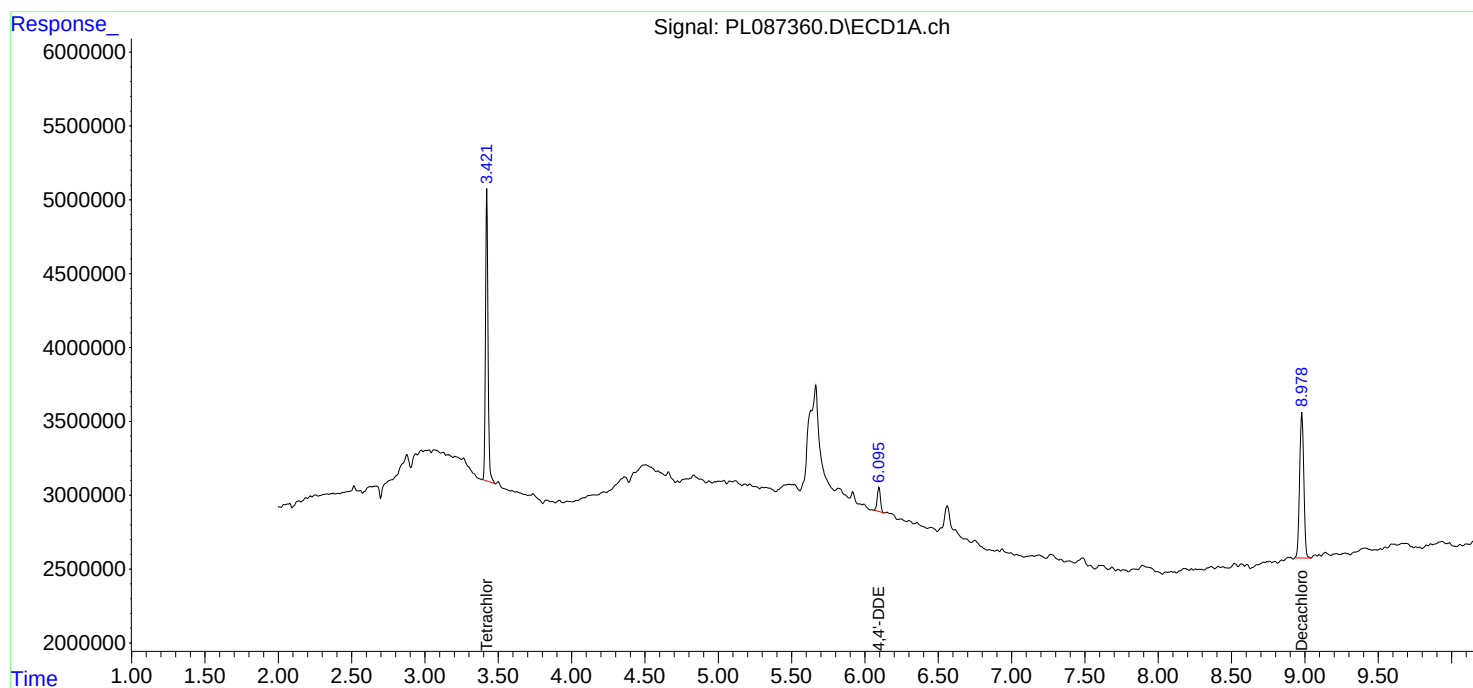

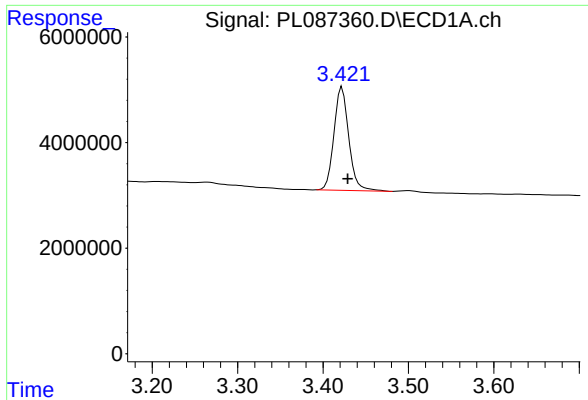


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 23651745
Conc: 6.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

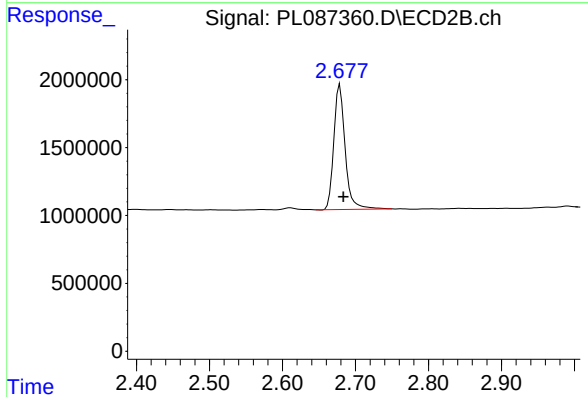


#1 Tetrachloro-m-xylene

R.T.: 2.679 min
Delta R.T.: -0.005 min
Response: 9933047
Conc: 5.90 ng/ml

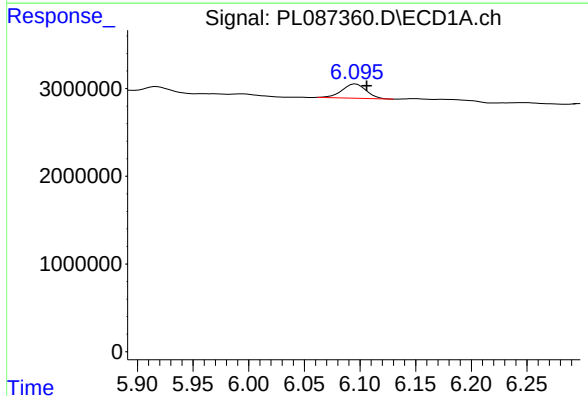


#12 4,4'-DDE

R.T.: 6.096 min
Delta R.T.: -0.010 min
Response: 2464911
Conc: 0.59 ng/ml

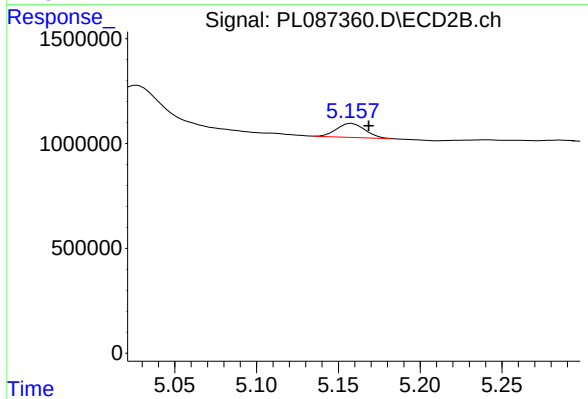

#12 4,4'-DDE

R.T.: 5.157 min
Delta R.T.: -0.011 min
Response: 807188
Conc: 0.41 ng/ml m

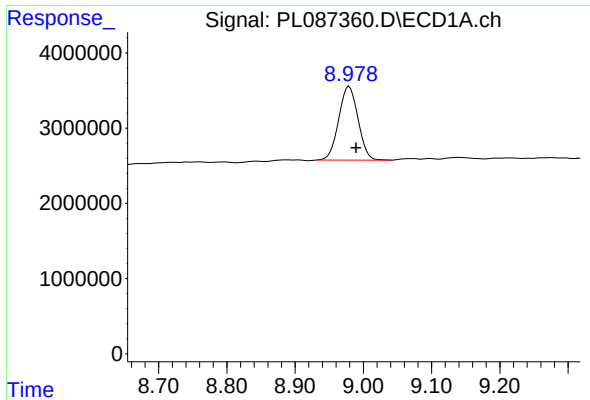


#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.010 min
Response: 19335283
Conc: 5.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-12202023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

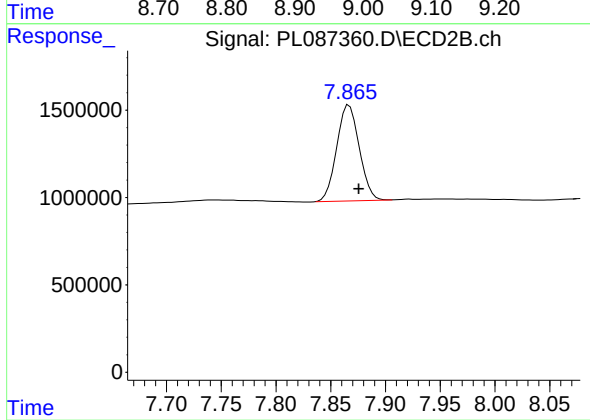

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: -0.009 min
Response: 7881196
Conc: 4.67 ng/ml