

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 10:50
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 11:37:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 11:36:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.113	349.2E6	253.2E6	97.071	96.801
28)	SA Decachlor...	8.191	9.276	287.4E6	206.9E6	102.860	104.465
Target Compounds							
23)	Chlordane-1	4.312	5.128	102.6E6	87736780	950.366	939.524
24)	Chlordane-2	4.812	5.603	109.5E6	93596061	902.124	920.938
25)	Chlordane-3	5.379	6.259	327.2E6	348.6E6	942.384	981.854
26)	Chlordane-4	5.437	6.333	267.3E6	413.2E6	948.915	967.459
27)	Chlordane-5	6.267	7.152	99374890	65511281	891.047	963.353



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 10:50
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 11:37:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 11:36:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

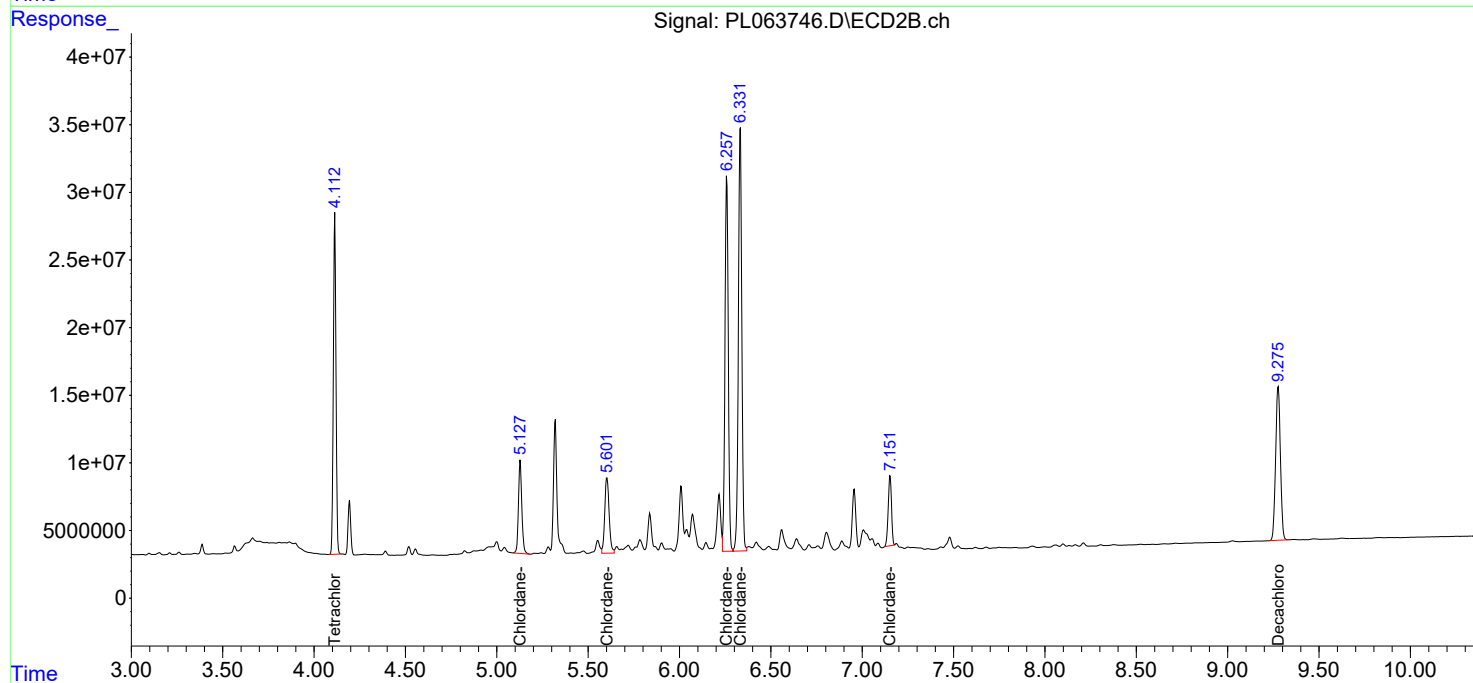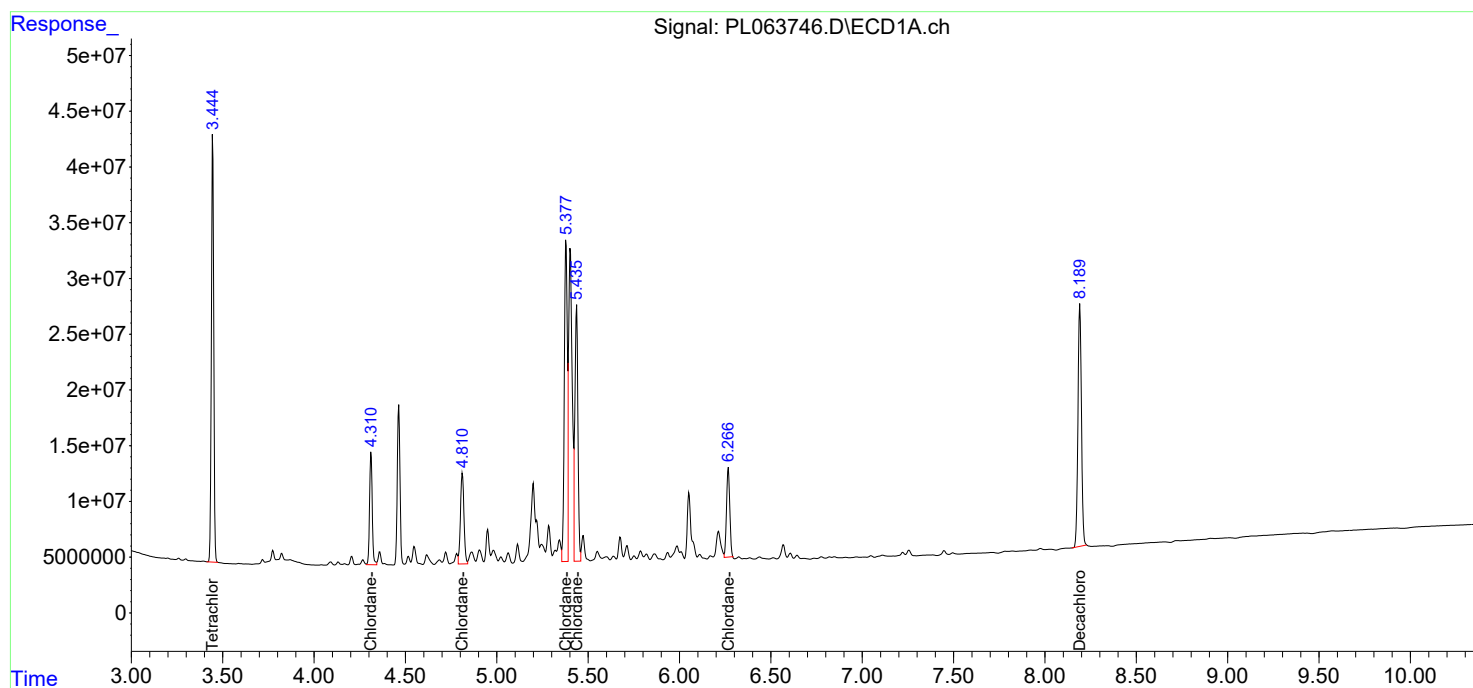


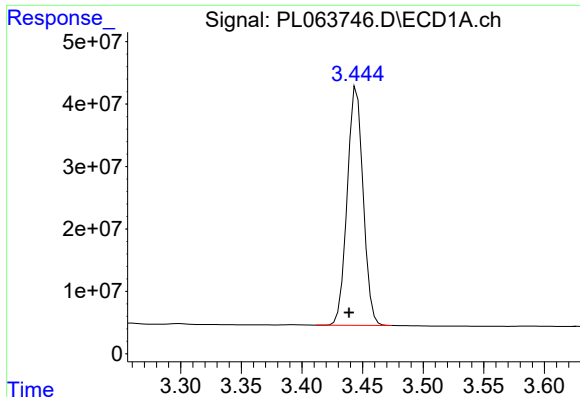

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.006 min
Response: 349185944
Conc: 97.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

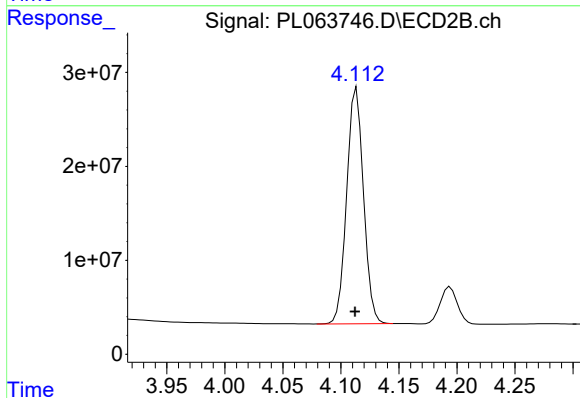


#1 Tetrachloro-m-xylene

R.T.: 4.113 min
Delta R.T.: 0.001 min
Response: 253173718
Conc: 96.80 ng/ml

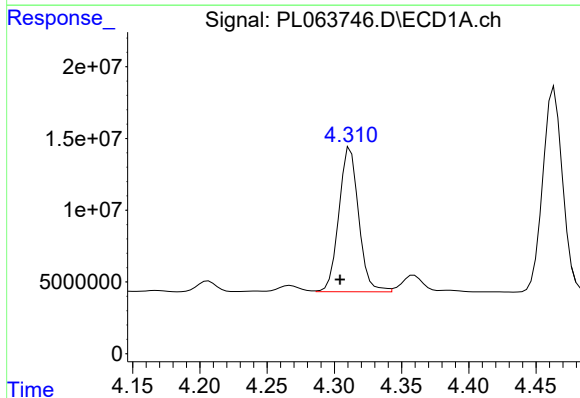


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.008 min
Response: 102588122
Conc: 950.37 ng/ml

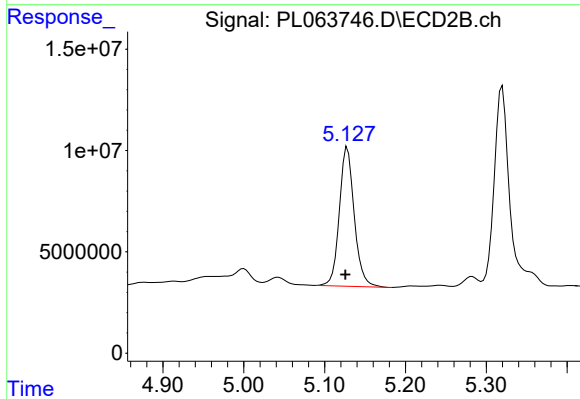

#23 Chlordane-1


R.T.: 5.128 min
Delta R.T.: 0.002 min
Response: 87736780
Conc: 939.52 ng/ml

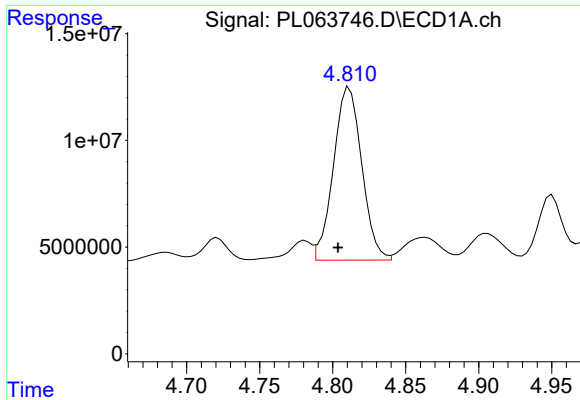

#24 Chlordane-2


R.T.: 4.812 min
Delta R.T.: 0.008 min
Response: 109480042
Conc: 902.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

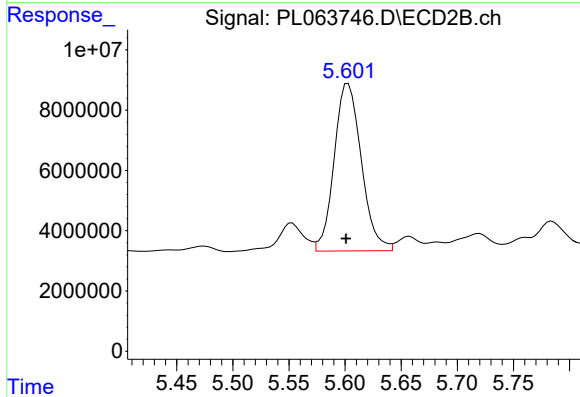


#24 Chlordane-2

R.T.: 5.603 min
Delta R.T.: 0.002 min
Response: 93596061
Conc: 920.94 ng/ml

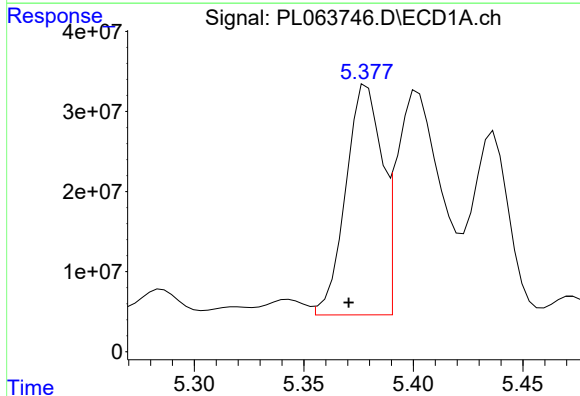


#25 Chlordane-3

R.T.: 5.379 min
Delta R.T.: 0.009 min
Response: 327175409
Conc: 942.38 ng/ml

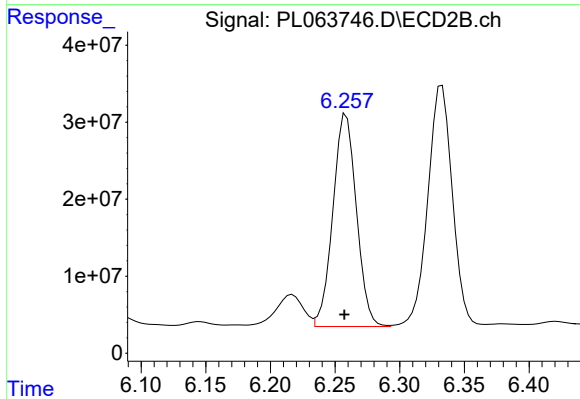

#25 Chlordane-3


R.T.: 6.259 min
Delta R.T.: 0.001 min
Response: 348591734
Conc: 981.85 ng/ml

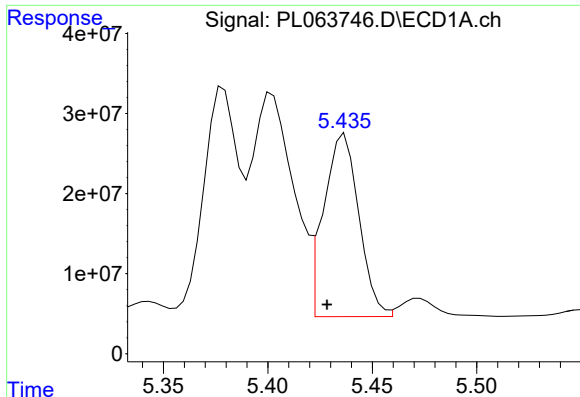

#26 Chlordane-4


R.T.: 5.437 min
Delta R.T.: 0.008 min
Response: 267282764
Conc: 948.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

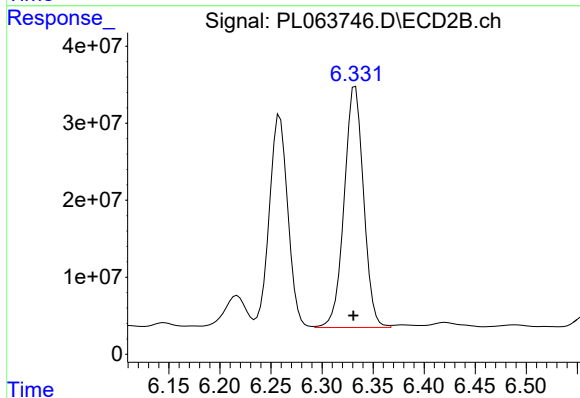


#26 Chlordane-4

R.T.: 6.333 min
Delta R.T.: 0.002 min
Response: 413241139
Conc: 967.46 ng/ml

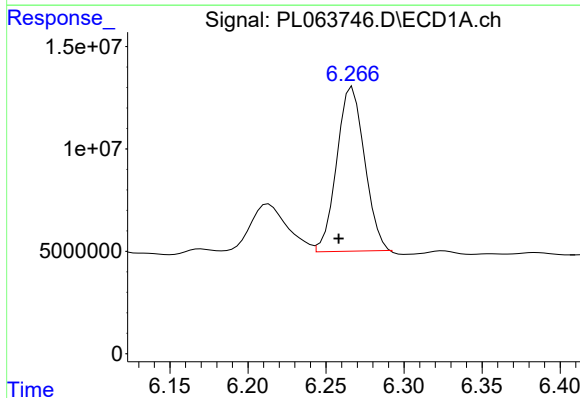


#27 Chlordane-5

R.T.: 6.267 min
Delta R.T.: 0.009 min
Response: 99374890
Conc: 891.05 ng/ml

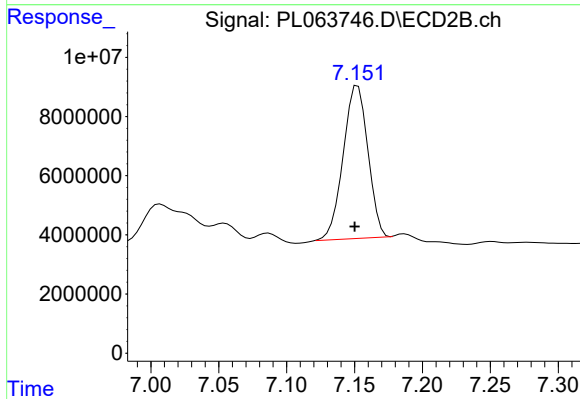

#27 Chlordane-5


R.T.: 7.152 min
Delta R.T.: 0.002 min
Response: 65511281
Conc: 963.35 ng/ml

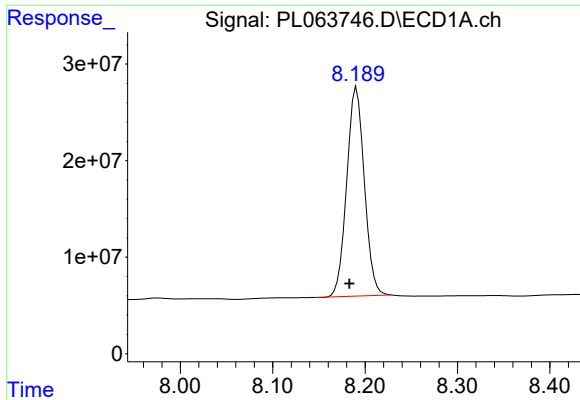

#28 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: 0.008 min
Response: 287388739
Conc: 102.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

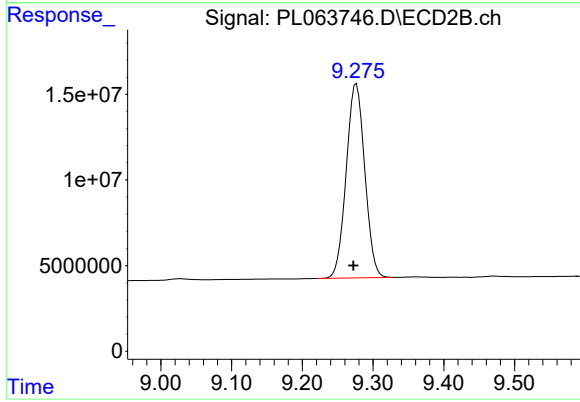

#28 Decachlorobiphenyl

R.T.: 9.276 min
Delta R.T.: 0.004 min
Response: 206925847
Conc: 104.46 ng/ml