

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 11:33
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 11:45:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 11:36:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.112	86174099	63568047	22.409	21.875
28)	SA Decachlor...	8.182	9.272	71034600	50698354	25.633	26.771
Target Compounds							
23)	Chlordane-1	4.304	5.126	26172465	22988177	220.881	210.612
24)	Chlordane-2	4.803	5.601	31065989	25513572	204.905	202.741
25)	Chlordane-3	5.370	6.257	83607154	84422749	214.759	224.648
26)	Chlordane-4	5.428	6.330	69748583	102.1E6	226.617	217.570
27)	Chlordane-5	6.259	7.150	28047588	17182280	183.149	233.226 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 11:33
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 11:45:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 11:36:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

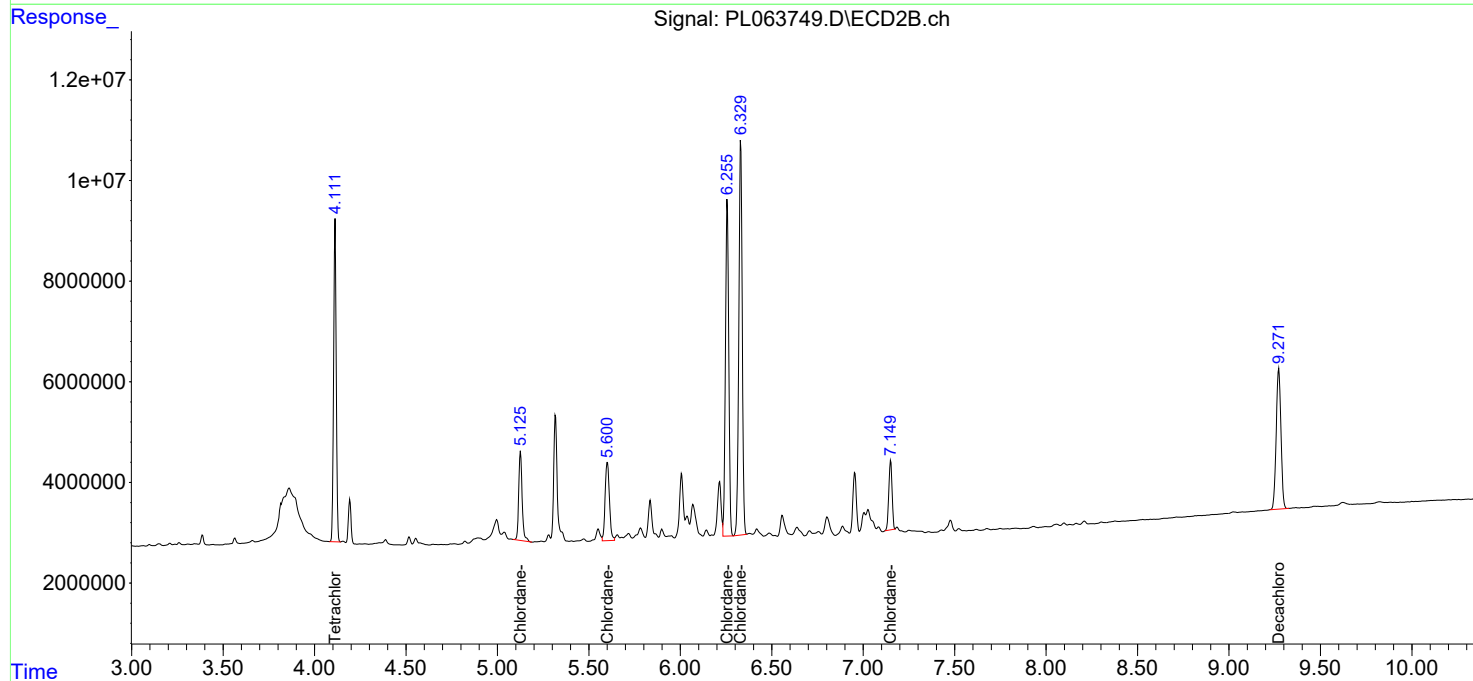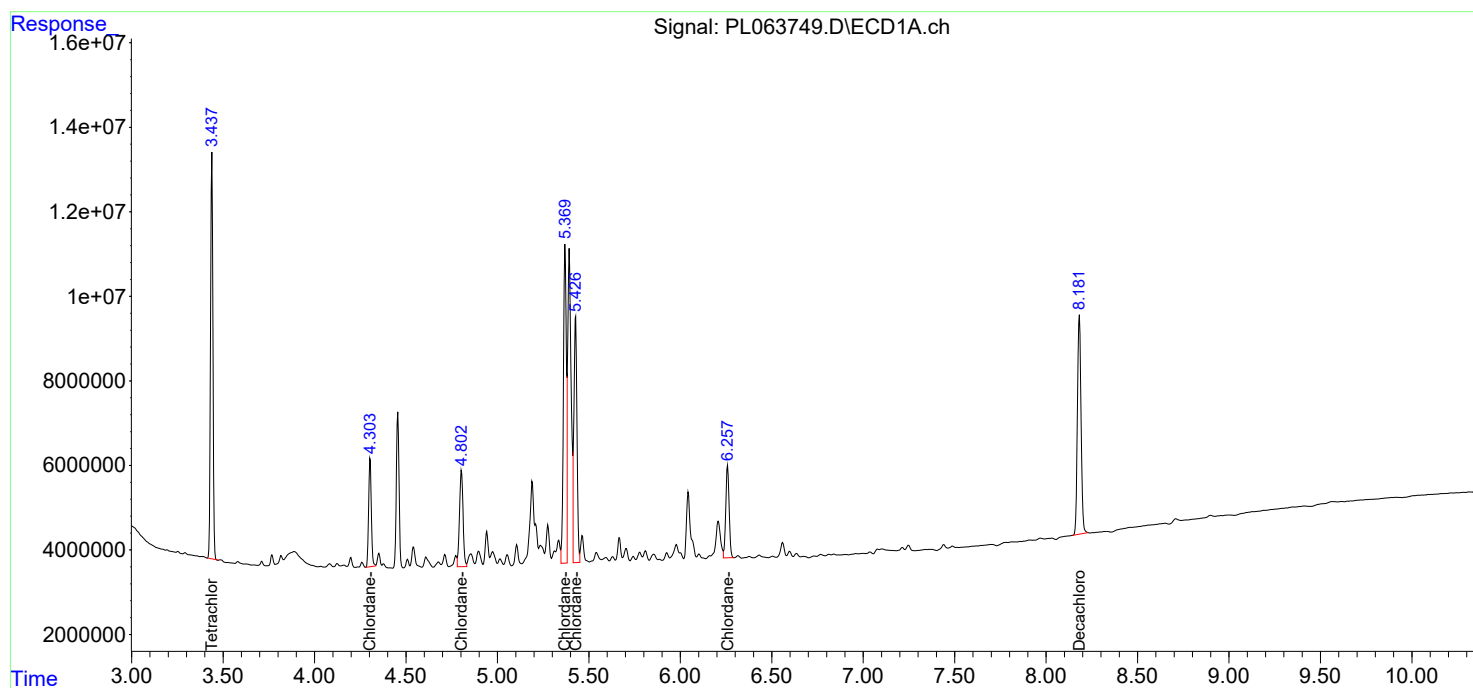


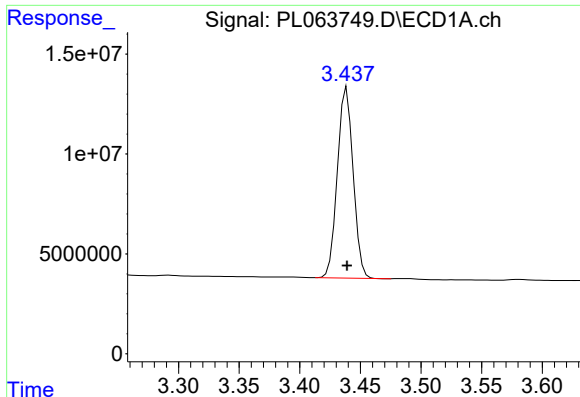

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 86174099
Conc: 22.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

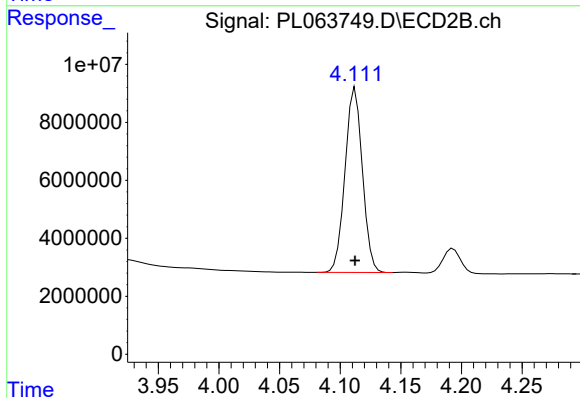


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 63568047
Conc: 21.88 ng/ml

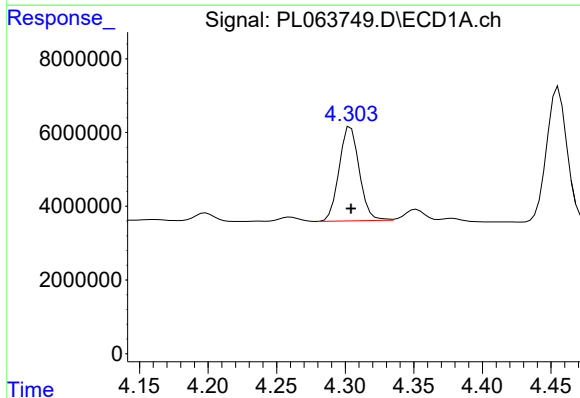


#23 Chlordane-1

R.T.: 4.304 min
Delta R.T.: 0.000 min
Response: 26172465
Conc: 220.88 ng/ml

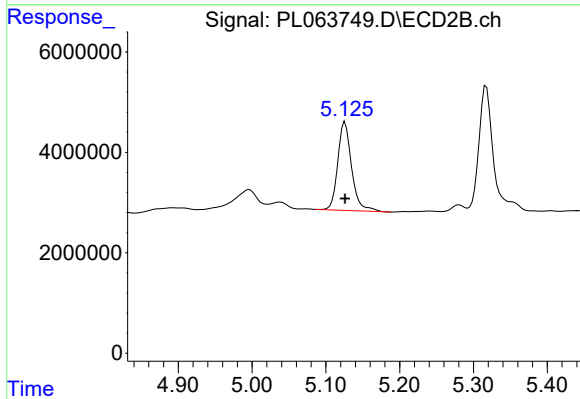

#23 Chlordane-1


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 22988177
Conc: 210.61 ng/ml

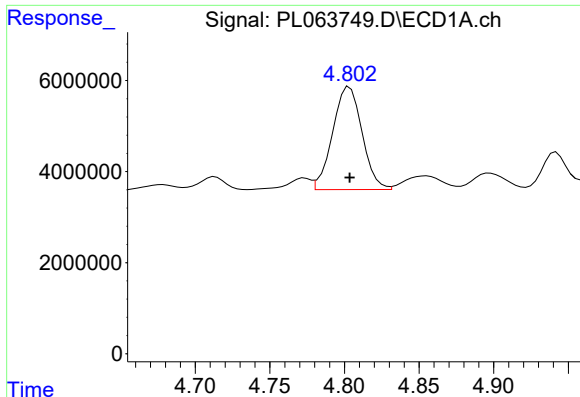

#24 Chlordane-2


R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 31065989
Conc: 204.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

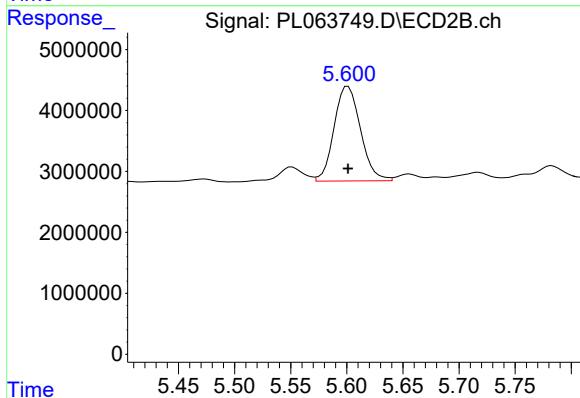


#24 Chlordane-2

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 25513572
Conc: 202.74 ng/ml

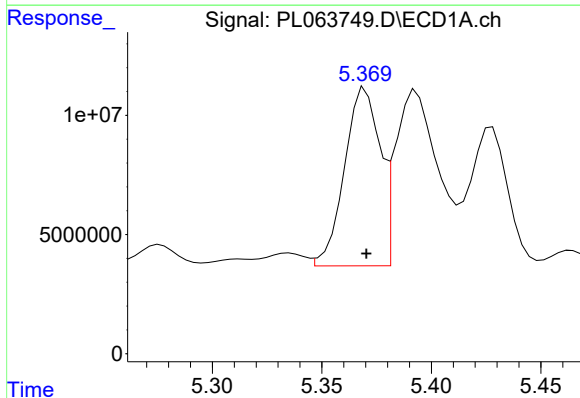


#25 Chlordane-3

R.T.: 5.370 min
Delta R.T.: 0.000 min
Response: 83607154
Conc: 214.76 ng/ml

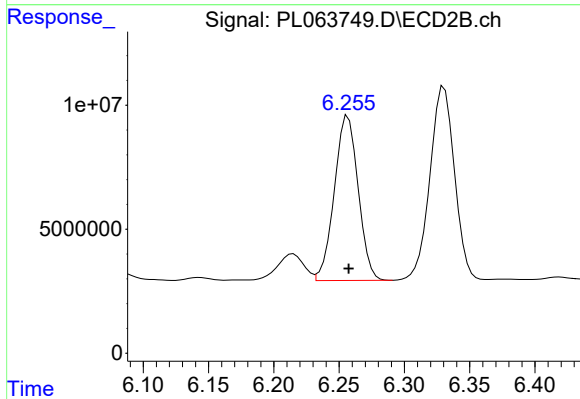

#25 Chlordane-3


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 84422749
Conc: 224.65 ng/ml

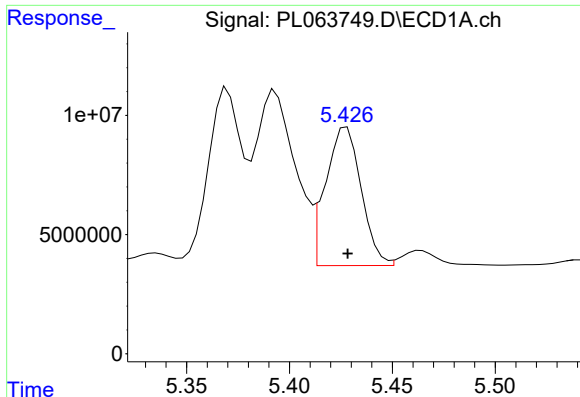

#26 Chlordane-4


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 69748583
Conc: 226.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

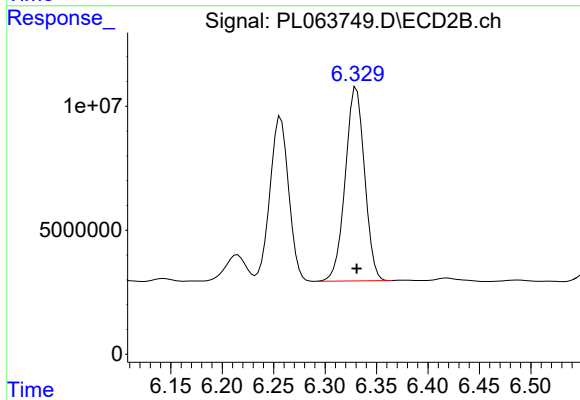


#26 Chlordane-4

R.T.: 6.330 min
Delta R.T.: 0.000 min
Response: 102059799
Conc: 217.57 ng/ml

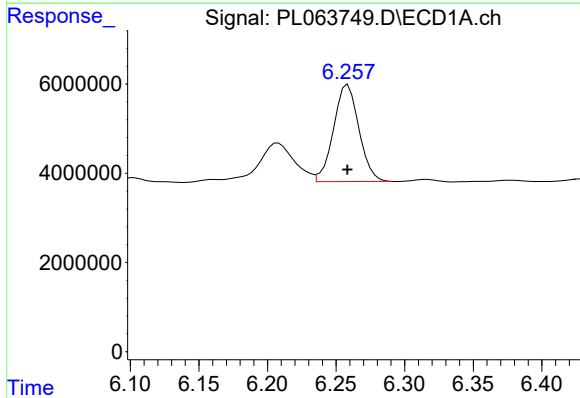


#27 Chlordane-5

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 28047588
Conc: 183.15 ng/ml

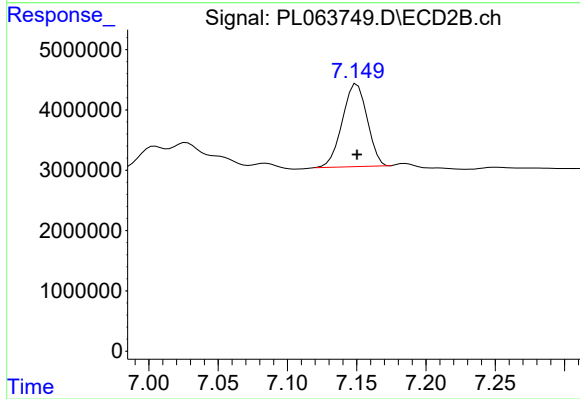

#27 Chlordane-5


R.T.: 7.150 min
Delta R.T.: 0.000 min
Response: 17182280
Conc: 233.23 ng/ml

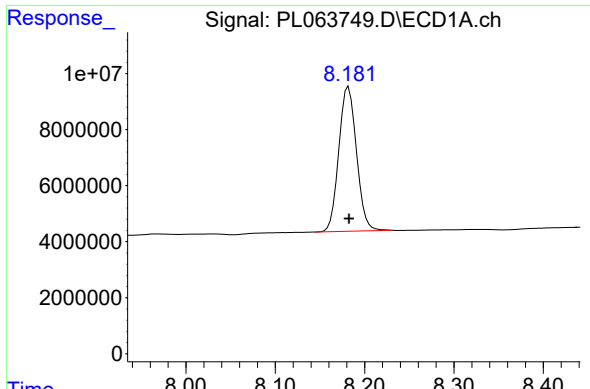

#28 Decachlorobiphenyl

R.T.: 8.182 min
Delta R.T.: 0.000 min
Response: 71034600
Conc: 25.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

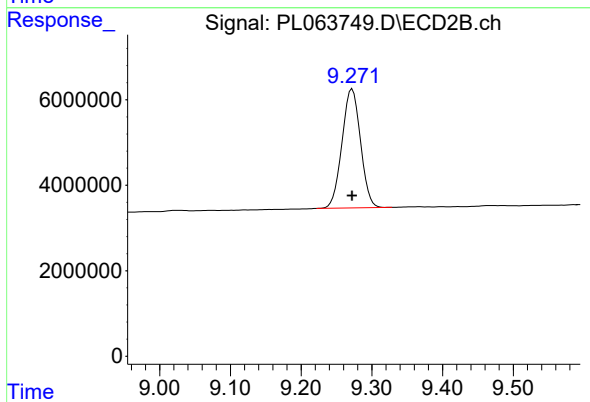

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 50698354
Conc: 26.77 ng/ml