

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 12:05
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 13:47:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 13:46:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.113	15497302	11599935	4.411	4.498
28)	SA Decachlor...	8.189	9.277	14278394	10164195	4.971	4.965
Target Compounds							
23)	Chlordane-1	4.310	5.127	4772898	3687049	45.789	40.640
24)	Chlordane-2	4.810	5.603	6714926	4417868	57.726	44.842
25)	Chlordane-3	5.377	6.259	15033860	15833079	45.107	45.350
26)	Chlordane-4	5.435	6.332	12279364	19178105	44.970	45.892
27)	Chlordane-5	6.266	7.152	5574705	3083863	52.320	45.933



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 12:05
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 13:47:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 13:46:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

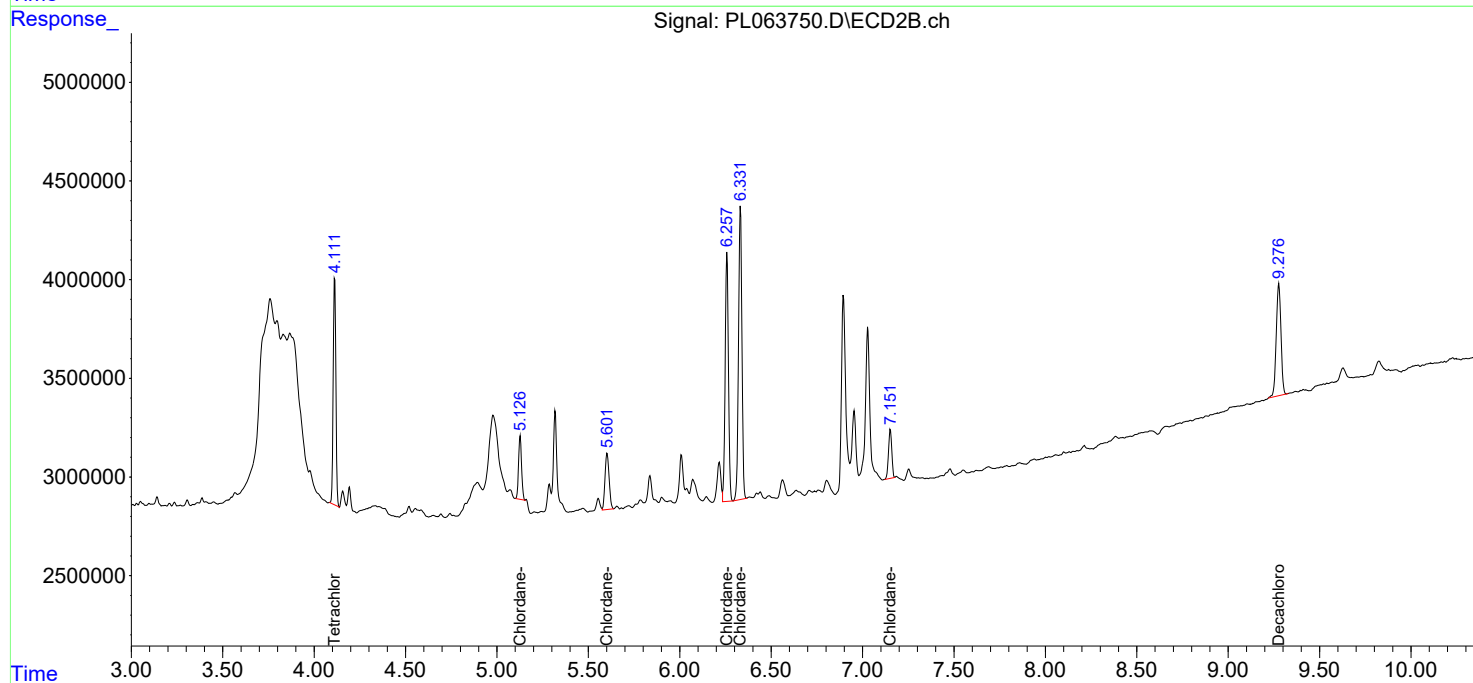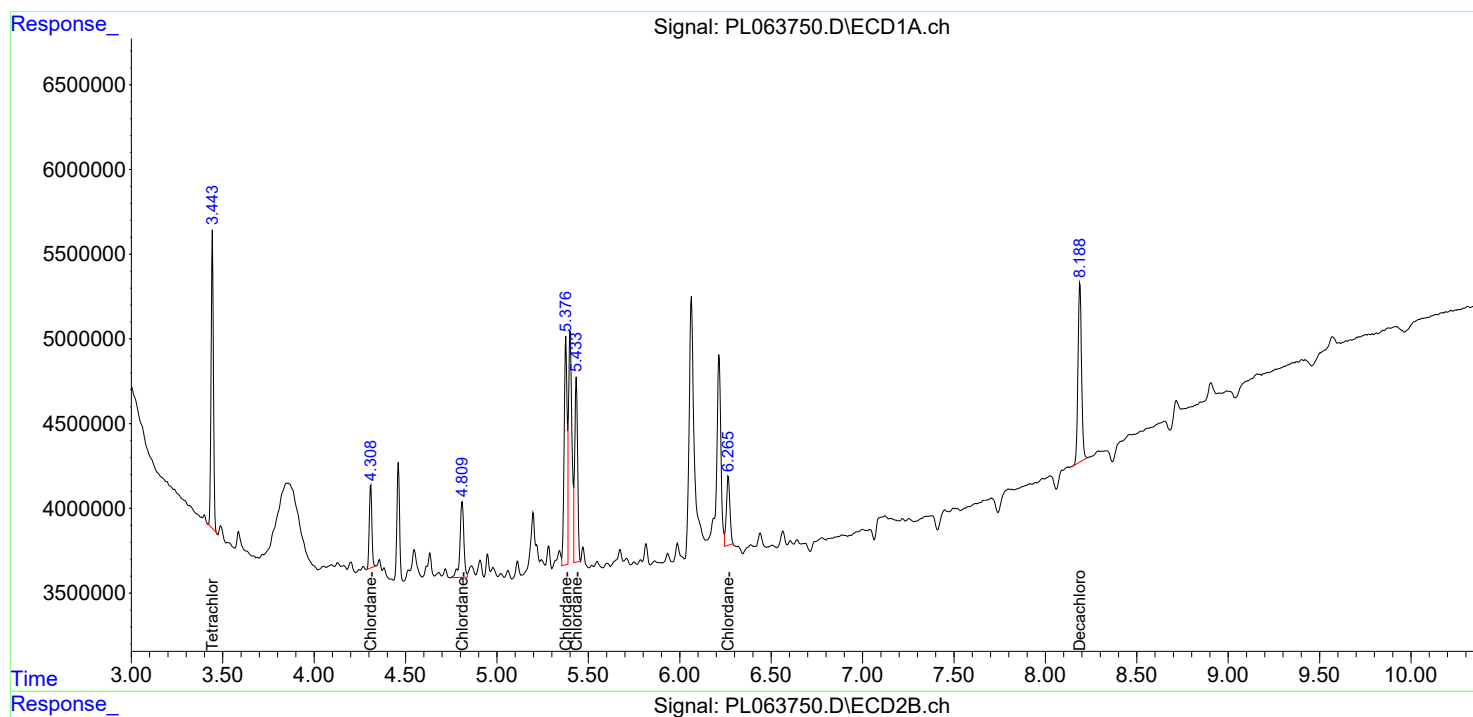


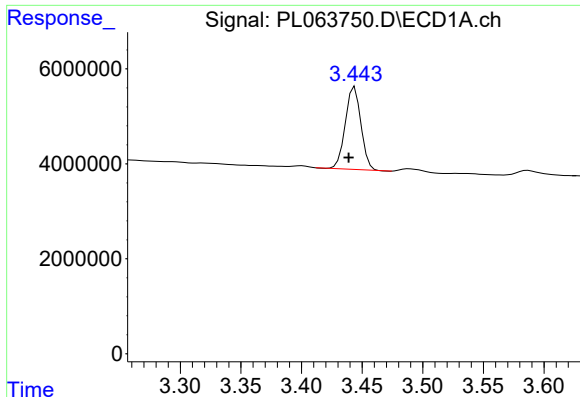

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.005 min
Response: 15497302
Conc: 4.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

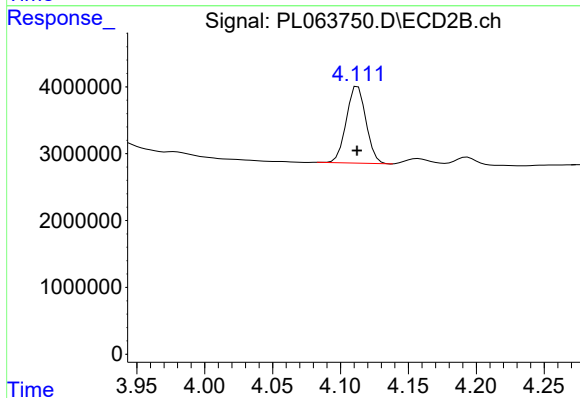


#1 Tetrachloro-m-xylene

R.T.: 4.113 min
Delta R.T.: 0.000 min
Response: 11599935
Conc: 4.50 ng/ml

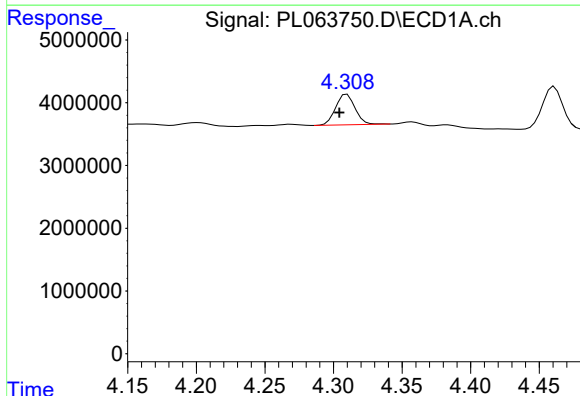


#23 Chlordane-1

R.T.: 4.310 min
Delta R.T.: 0.006 min
Response: 4772898
Conc: 45.79 ng/ml

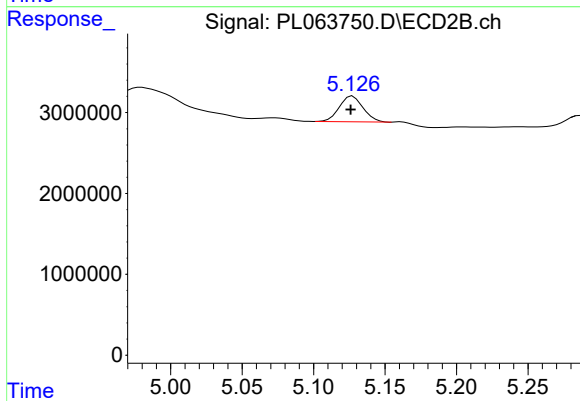

#23 Chlordane-1


R.T.: 5.127 min
Delta R.T.: 0.001 min
Response: 3687049
Conc: 40.64 ng/ml

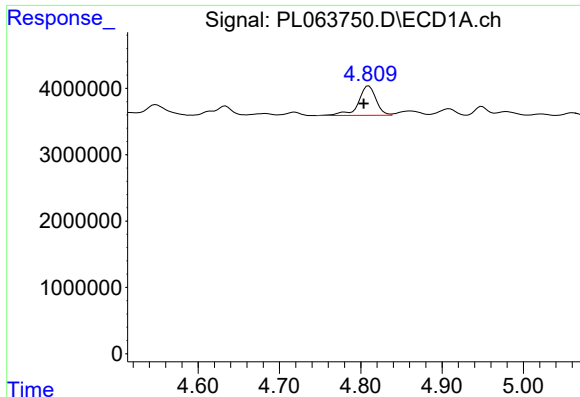

#24 Chlordane-2


R.T.: 4.810 min
Delta R.T.: 0.006 min
Response: 6714926
Conc: 57.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

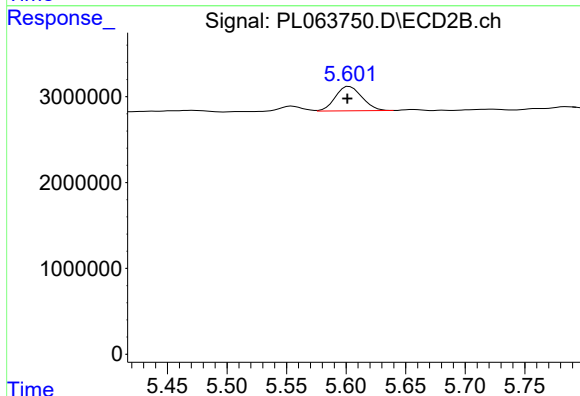


#24 Chlordane-2

R.T.: 5.603 min
Delta R.T.: 0.002 min
Response: 4417868
Conc: 44.84 ng/ml

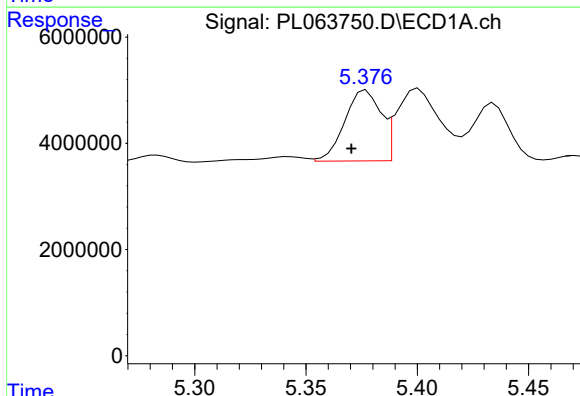


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.007 min
Response: 15033860
Conc: 45.11 ng/ml

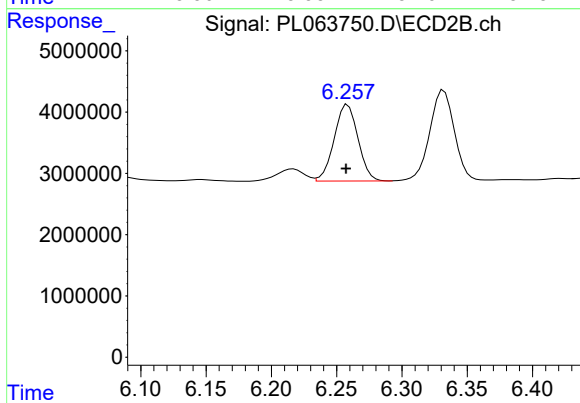

#25 Chlordane-3


R.T.: 6.259 min
Delta R.T.: 0.001 min
Response: 15833079
Conc: 45.35 ng/ml

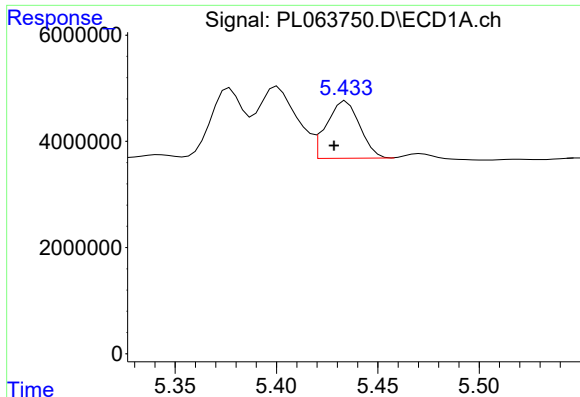

#26 Chlordane-4


R.T.: 5.435 min
Delta R.T.: 0.006 min
Response: 12279364
Conc: 44.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

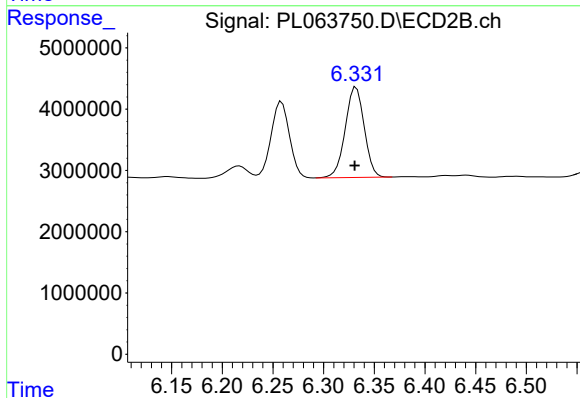


#26 Chlordane-4

R.T.: 6.332 min
Delta R.T.: 0.001 min
Response: 19178105
Conc: 45.89 ng/ml

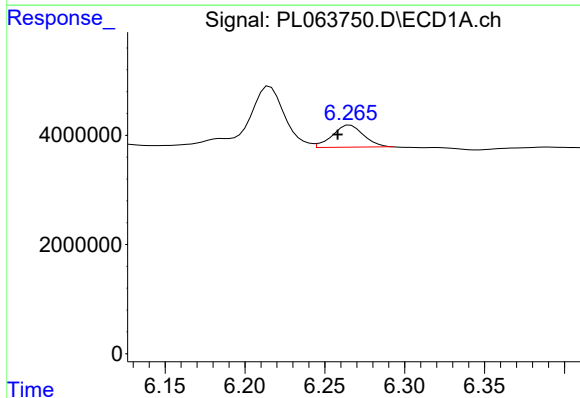


#27 Chlordane-5

R.T.: 6.266 min
Delta R.T.: 0.008 min
Response: 5574705
Conc: 52.32 ng/ml

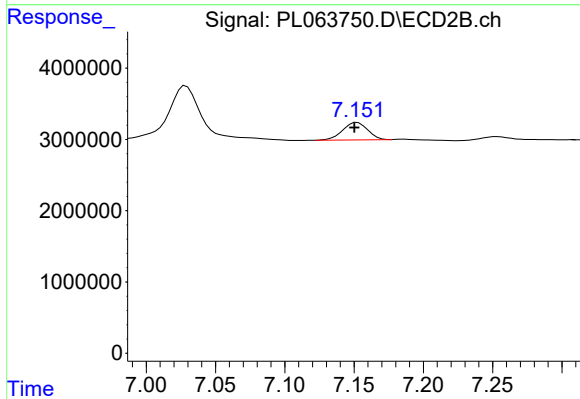

#27 Chlordane-5


R.T.: 7.152 min
Delta R.T.: 0.002 min
Response: 3083863
Conc: 45.93 ng/ml

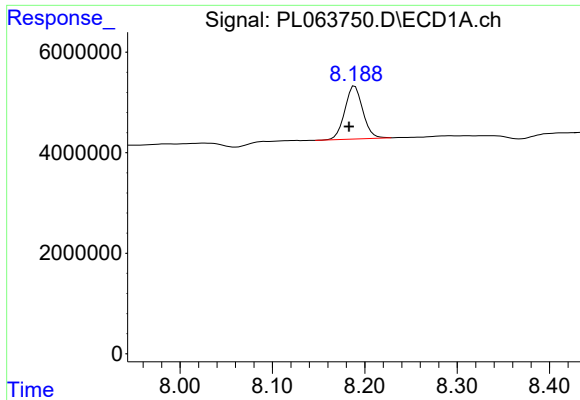

#28 Decachlorobiphenyl

R.T.: 8.189 min
Delta R.T.: 0.006 min
Response: 14278394
Conc: 4.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

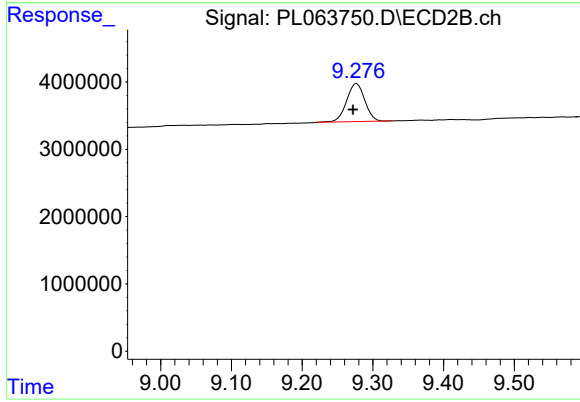

#28 Decachlorobiphenyl

R.T.: 9.277 min
Delta R.T.: 0.005 min
Response: 10164195
Conc: 4.96 ng/ml