

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 17:20
 Operator : AR\AJ
 Sample : L5176-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 00:55:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.112	23300107	20176160	7.772	7.903
28)	SA Decachlor...	8.182	9.272	16487921	12092609	5.984	6.133
Target Compounds							
19)	B Endosulfa...	6.633	0.000	2454239	0	0.779	N.D. #
20)	A Methoxychlor	6.877f	0.000	4228444	0	3.219	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 17:20
Operator : AR\AJ
Sample : L5176-07
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 00:55:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

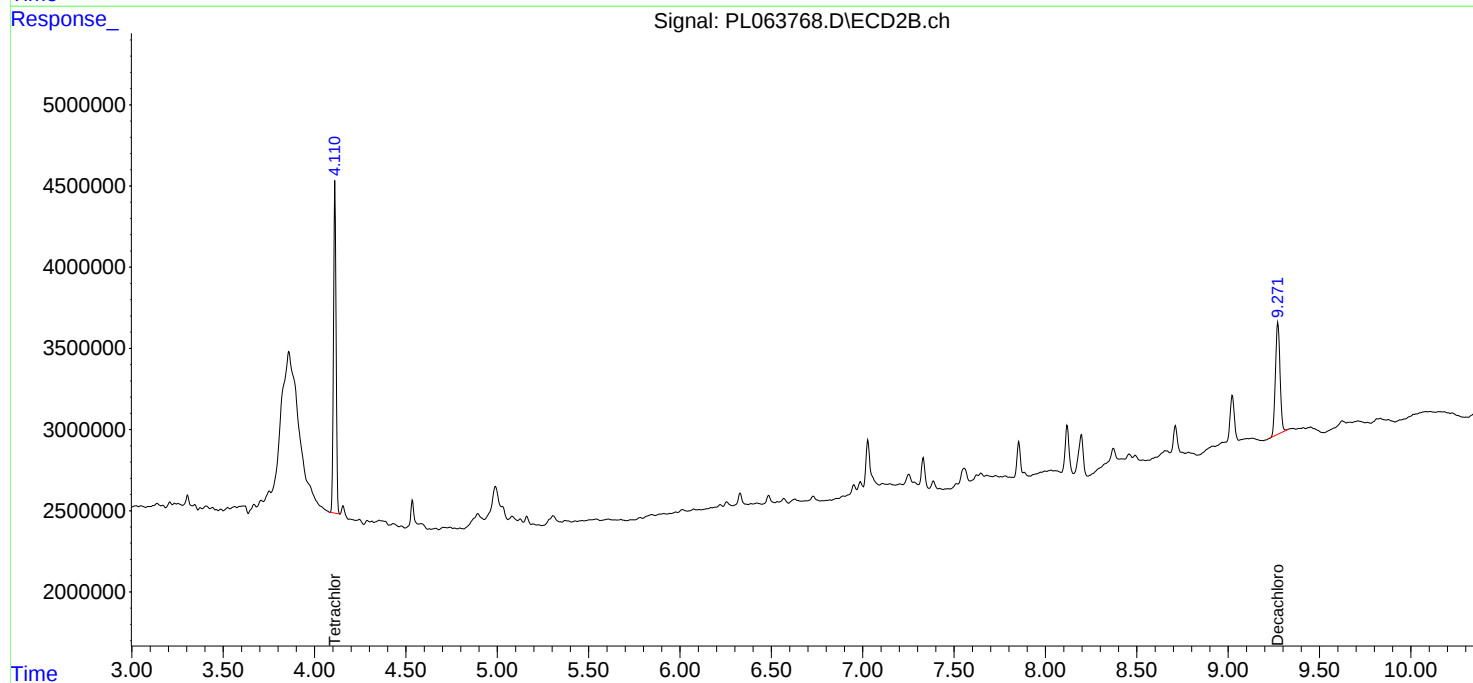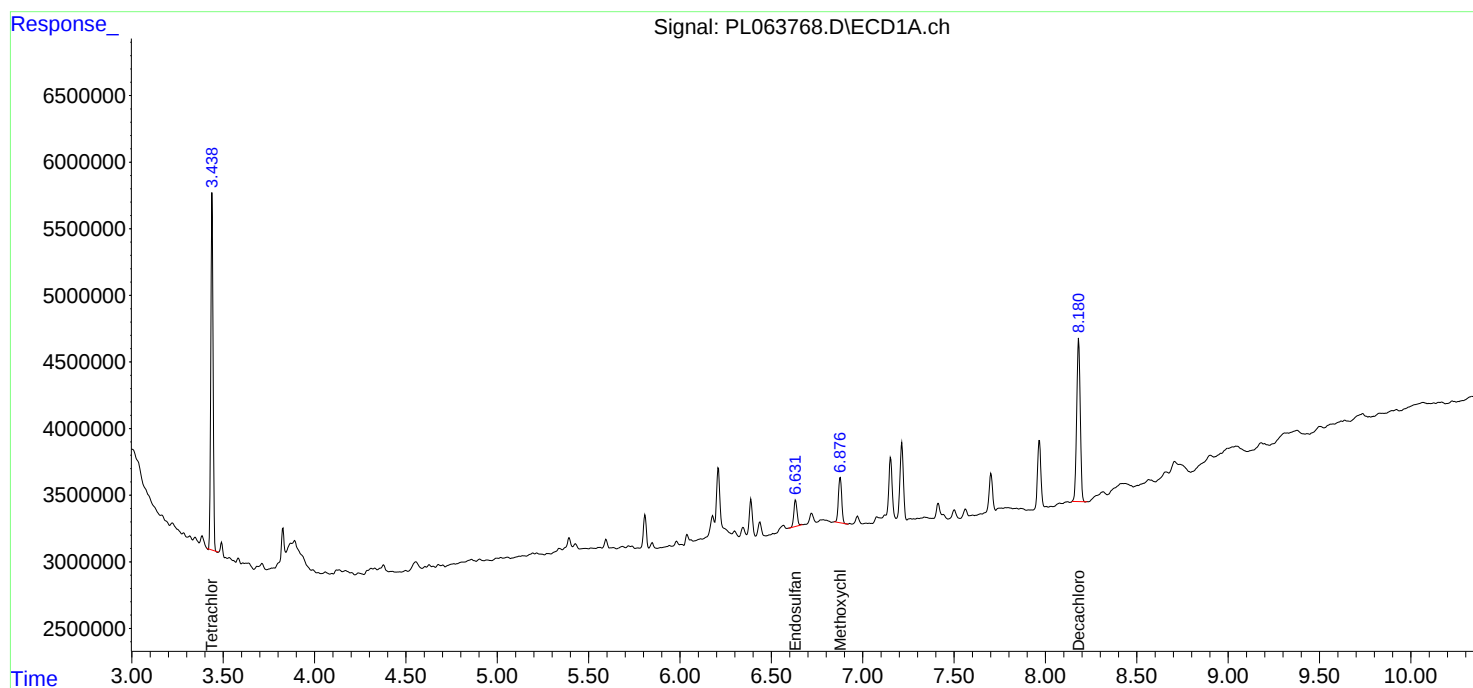


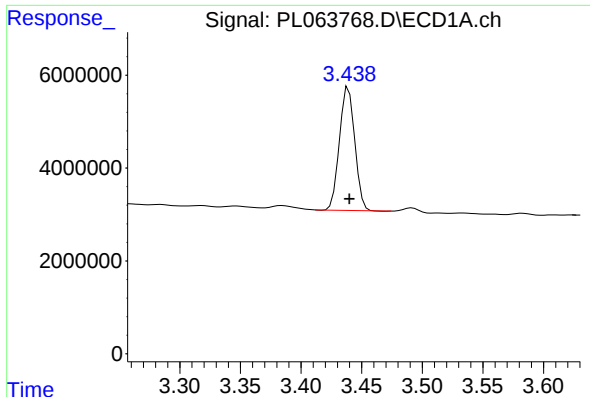

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 23300107
Conc: 7.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

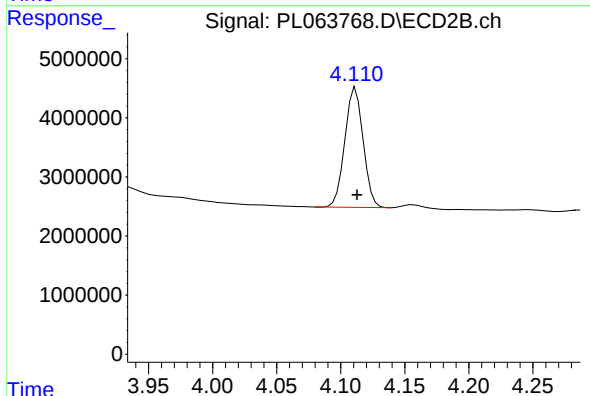


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 20176160
Conc: 7.90 ng/ml

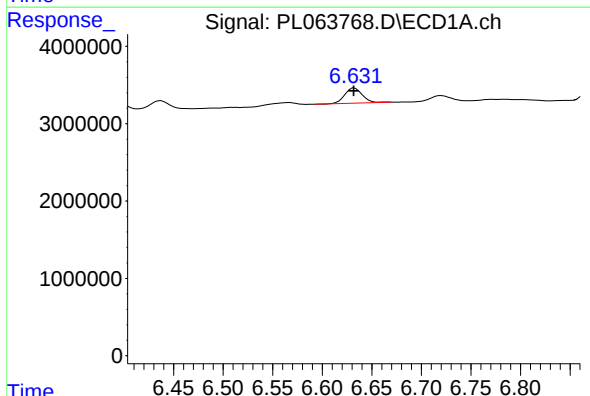


#19 Endosulfan Sulfate

R.T.: 6.633 min
Delta R.T.: 0.000 min
Response: 2454239
Conc: 0.78 ng/ml

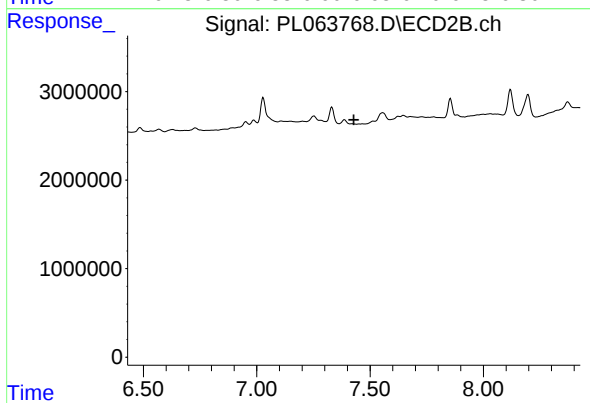

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.428 min
Response: 0
Conc: N.D.

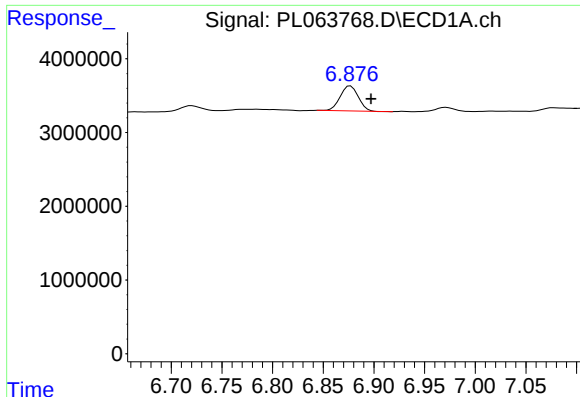

#20 Methoxychlor


R.T.: 6.877 min
Delta R.T.: -0.020 min
Response: 4228444
Conc: 3.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

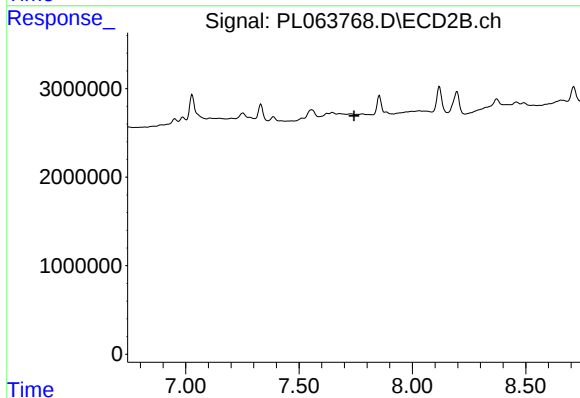


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.743 min
Response: 0
Conc: N.D.

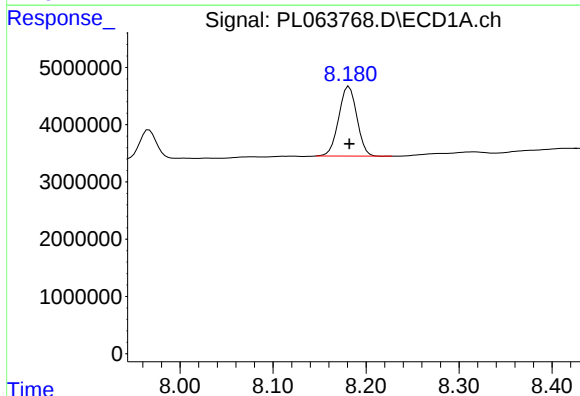

#28 Decachlorobiphenyl

R.T.: 8.182 min
Delta R.T.: 0.000 min
Response: 16487921
Conc: 5.98 ng/ml

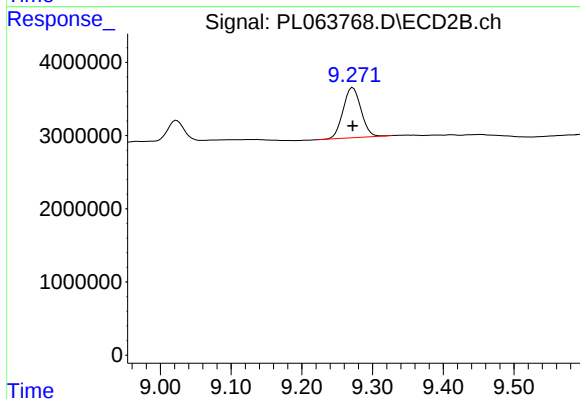

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 12092609
Conc: 6.13 ng/ml