

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 11:05
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 11:37:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 11:36:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.112	263.8E6	196.9E6	73.328	75.292
28)	SA Decachlor...	8.183	9.273	223.5E6	158.3E6	79.984	79.925
Target Compounds							
23)	Chlordane-1	4.305	5.126	76295676	67369549	706.795	721.423
24)	Chlordane-2	4.804	5.602	82646117	72601079	681.011	714.358
25)	Chlordane-3	5.371	6.257	243.3E6	266.4E6	700.764	750.367
26)	Chlordane-4	5.429	6.331	198.2E6	317.2E6	703.680	742.687
27)	Chlordane-5	6.259	7.151	77333803	49733923	693.415	731.345



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 11:05
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 11:37:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 11:36:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

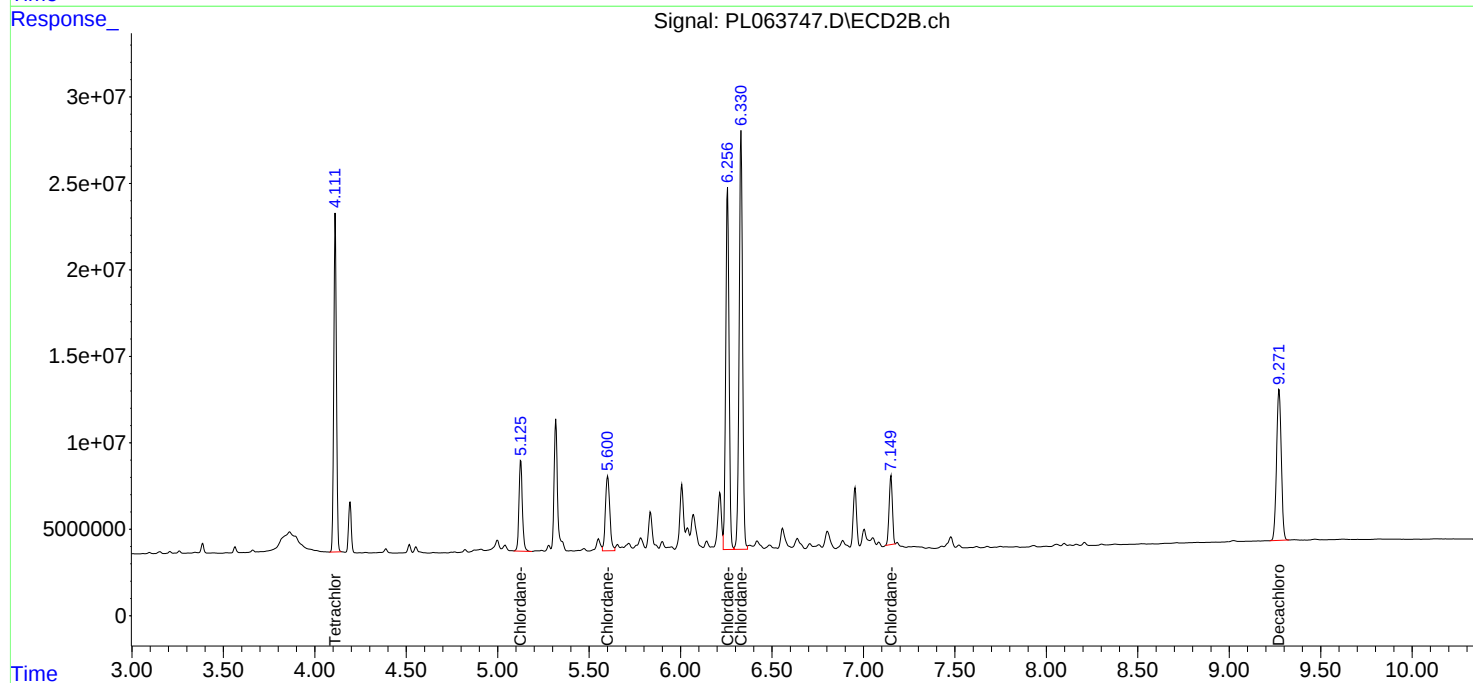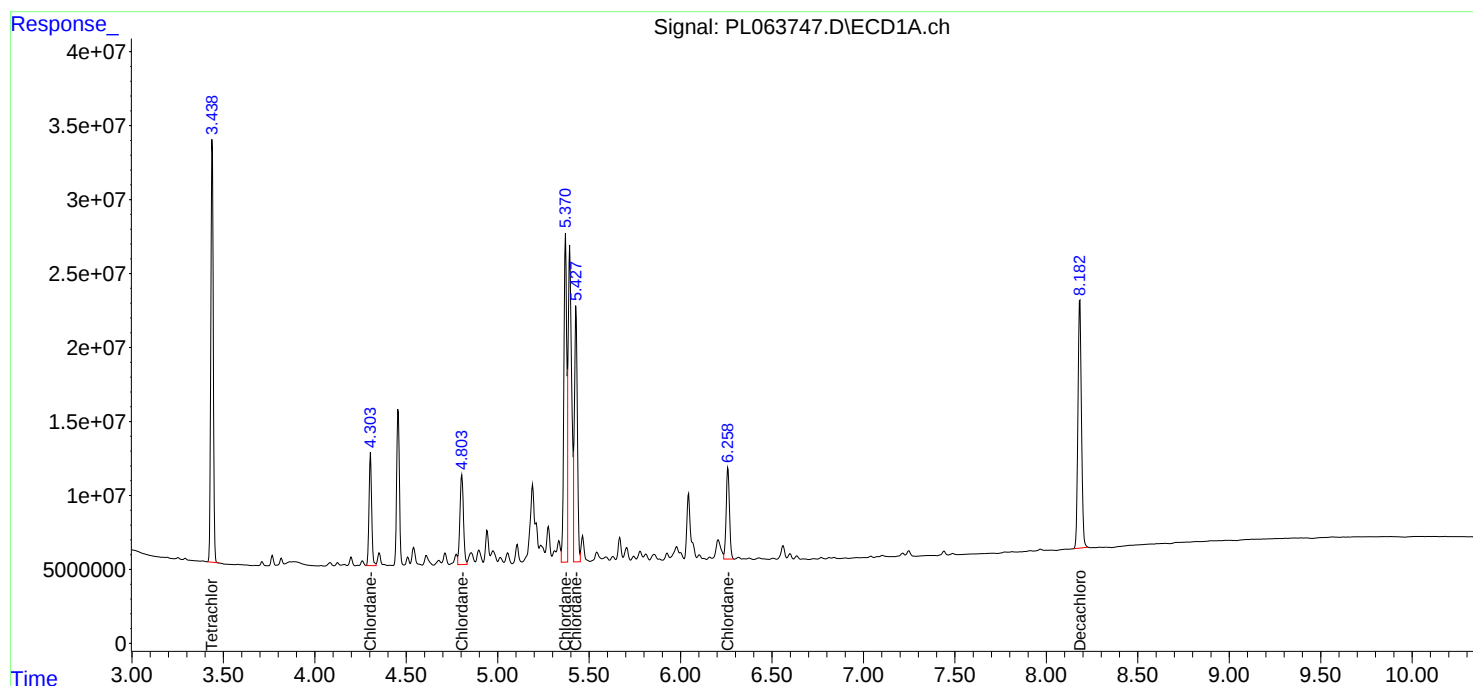


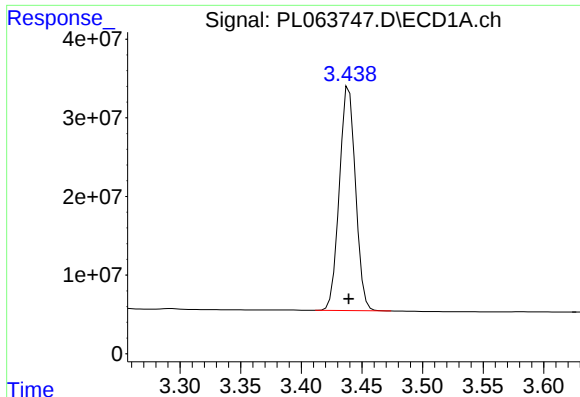

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 263776045
Conc: 73.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

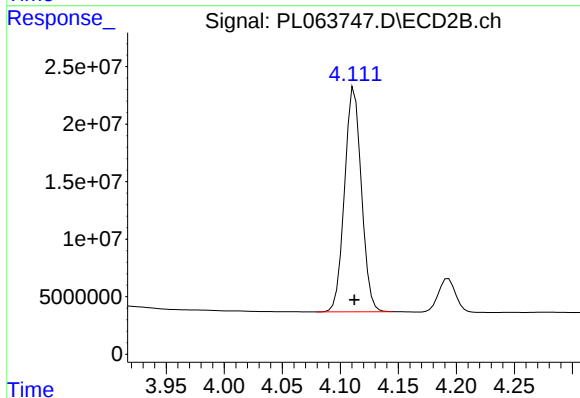


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 196918898
Conc: 75.29 ng/ml

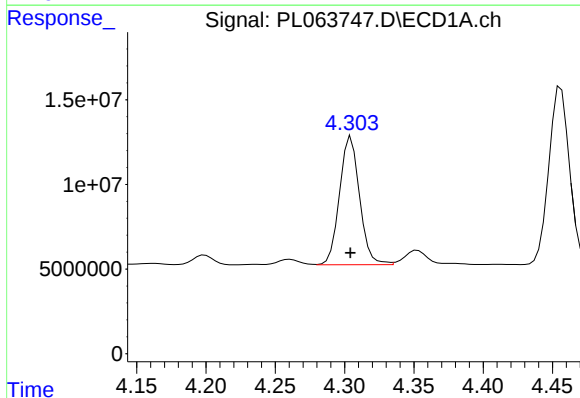


#23 Chlordane-1

R.T.: 4.305 min
Delta R.T.: 0.000 min
Response: 76295676
Conc: 706.80 ng/ml

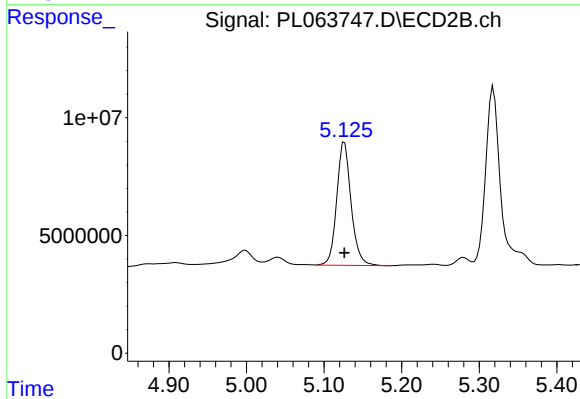

#23 Chlordane-1


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 67369549
Conc: 721.42 ng/ml

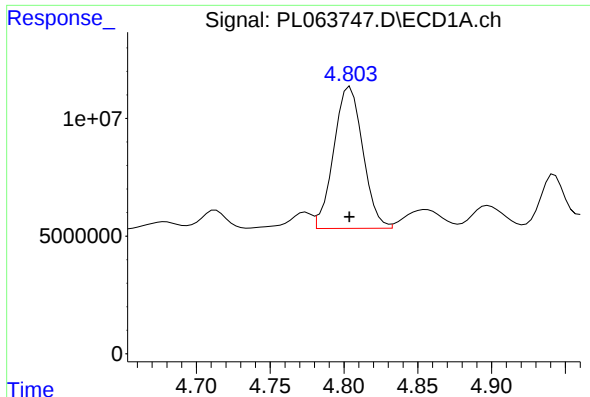

#24 Chlordane-2


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 82646117
Conc: 681.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

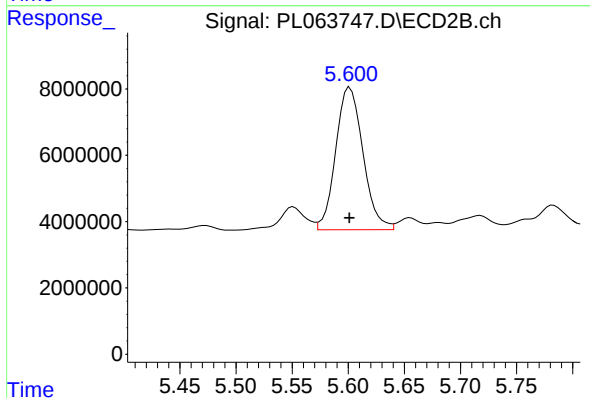


#24 Chlordane-2

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 72601079
Conc: 714.36 ng/ml

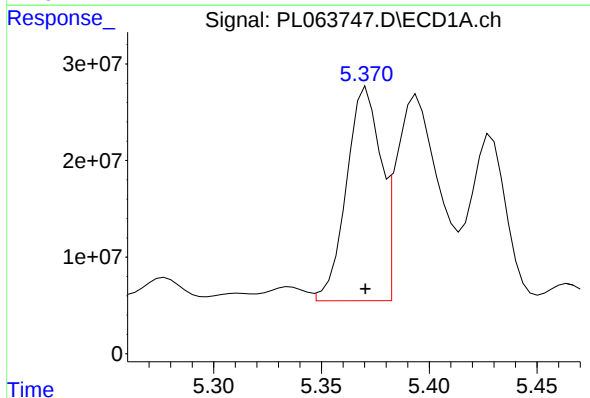


#25 Chlordane-3

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 243290107
Conc: 700.76 ng/ml

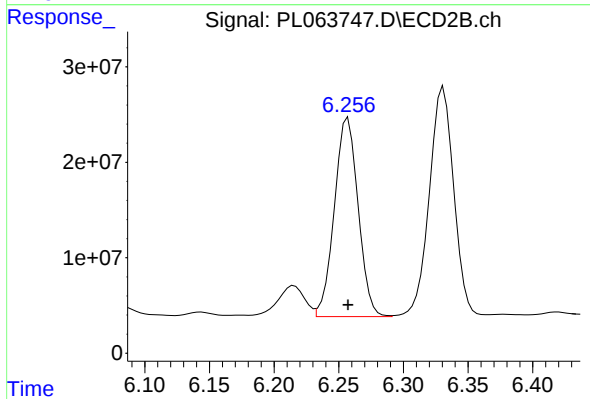

#25 Chlordane-3


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 266406004
Conc: 750.37 ng/ml

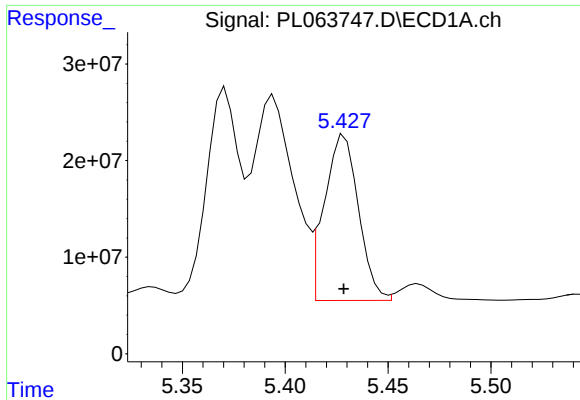

#26 Chlordane-4


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 198206942
Conc: 703.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

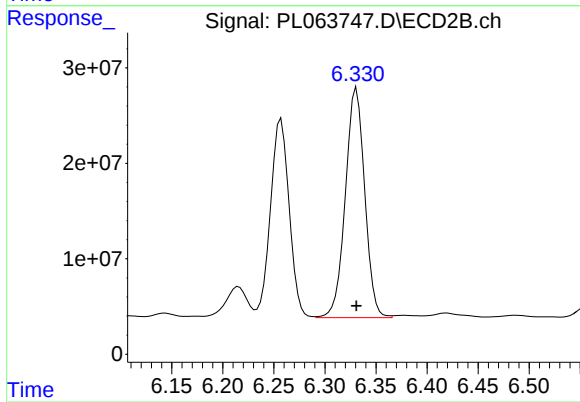


#26 Chlordane-4

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 317231830
Conc: 742.69 ng/ml

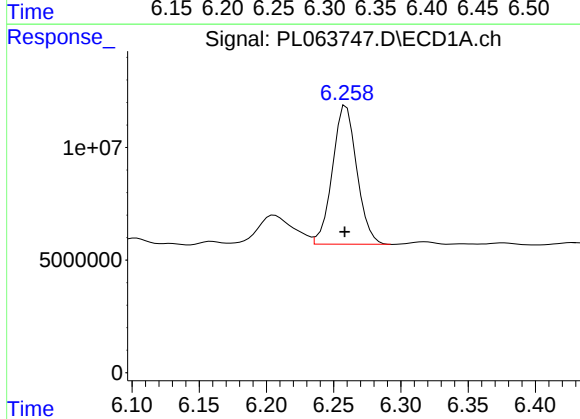


#27 Chlordane-5

R.T.: 6.259 min
Delta R.T.: 0.001 min
Response: 77333803
Conc: 693.42 ng/ml

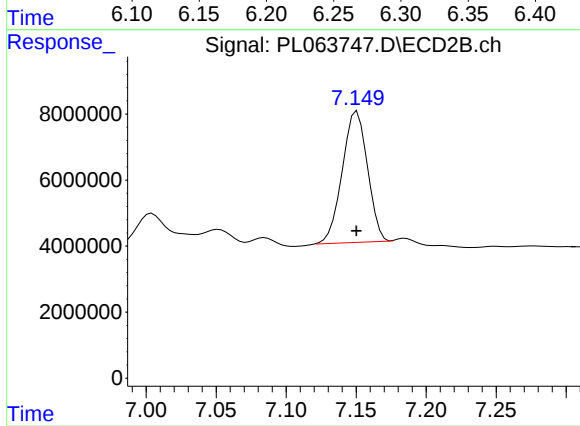

#27 Chlordane-5


R.T.: 7.151 min
Delta R.T.: 0.000 min
Response: 49733923
Conc: 731.34 ng/ml

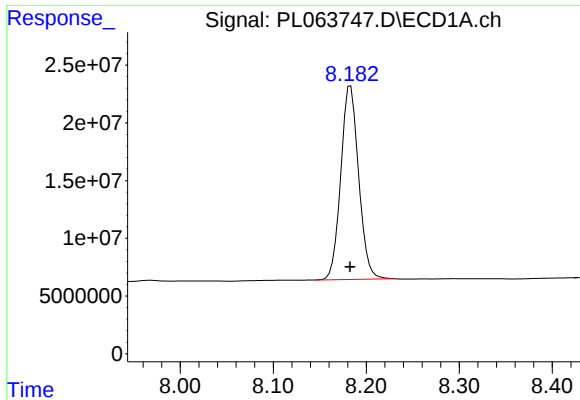

#28 Decachlorobiphenyl

R.T.: 8.183 min
Delta R.T.: 0.000 min
Response: 223475328
Conc: 79.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

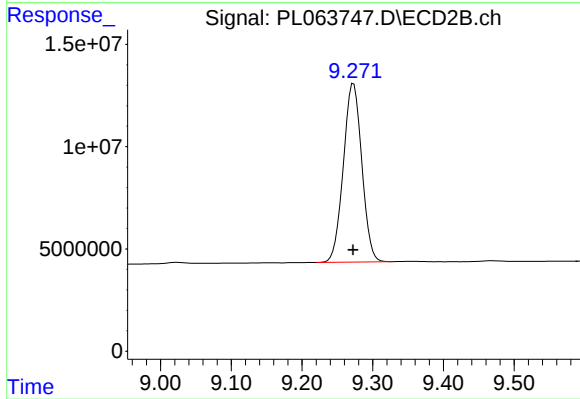

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 158317657
Conc: 79.93 ng/ml