

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 13:49
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL122220CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 14:01:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 13:48:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.113	173.5E6	124.4E6	50.588	49.213
28)	SA Decachlor...	8.183	9.273	135.6E6	96171117	47.273	47.042
Target Compounds							
23)	Chlordane-1	4.304	5.127	51265469	43842541	500.239	502.044
24)	Chlordane-2	4.804	5.601	59394349	47692573	506.177	494.285
25)	Chlordane-3	5.371	6.257	167.8E6	168.4E6	513.571	491.546
26)	Chlordane-4	5.429	6.331	137.6E6	202.9E6	514.275	493.740
27)	Chlordane-5	6.259	7.150	54428978	33024269	506.131	500.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 13:49
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL122220CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 14:01:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 13:48:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

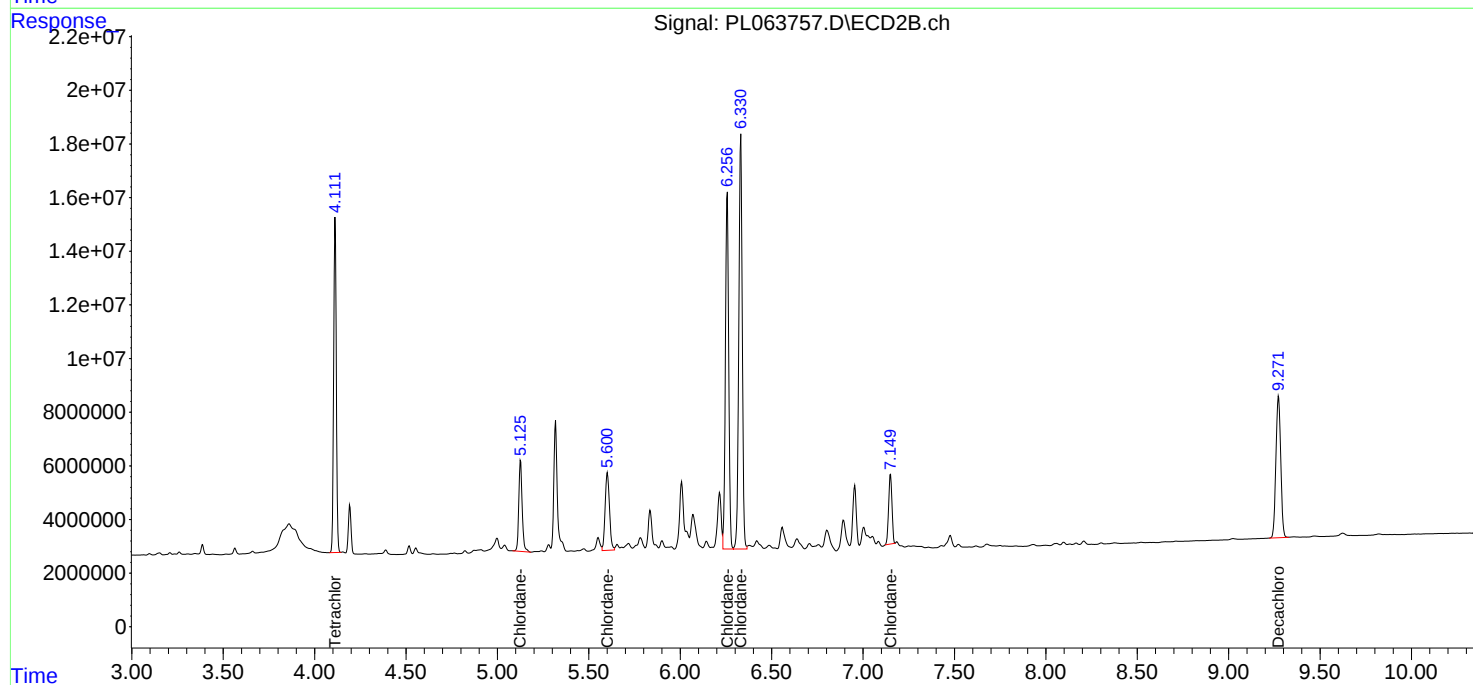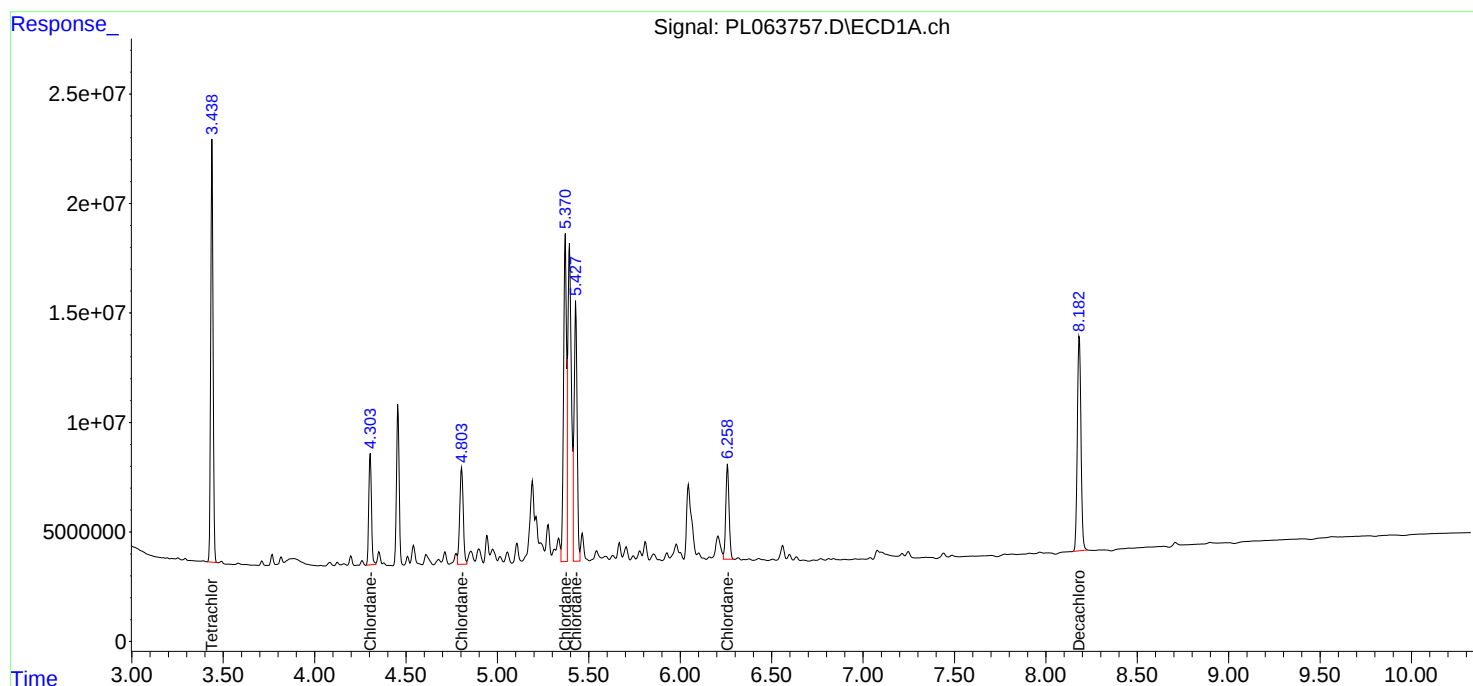


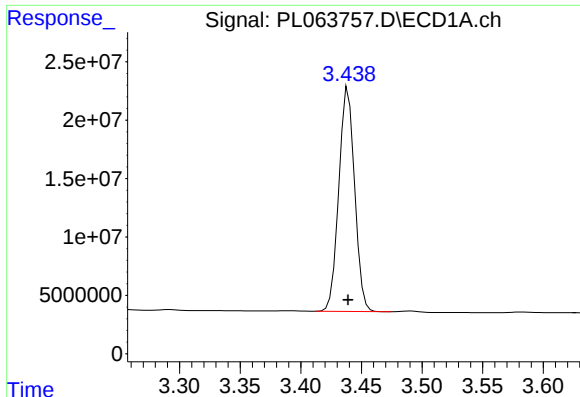

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 173541639
Conc: 50.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122220CHLOR

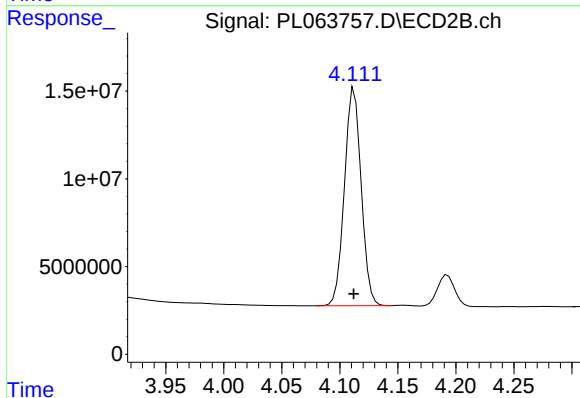


#1 Tetrachloro-m-xylene

R.T.: 4.113 min
Delta R.T.: 0.000 min
Response: 124364664
Conc: 49.21 ng/ml

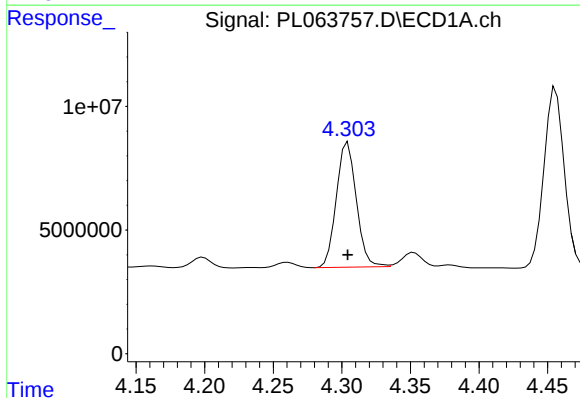


#23 Chlordane-1

R.T.: 4.304 min
Delta R.T.: 0.000 min
Response: 51265469
Conc: 500.24 ng/ml

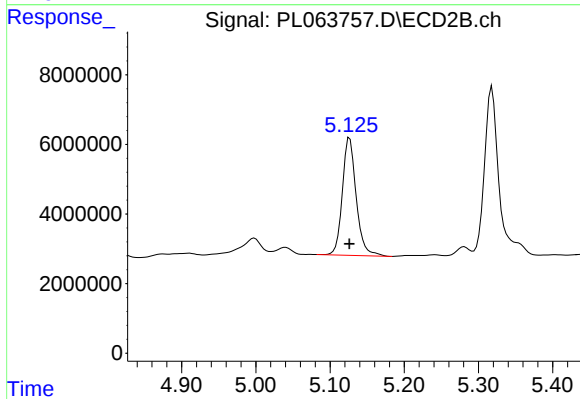

#23 Chlordane-1


R.T.: 5.127 min
Delta R.T.: 0.000 min
Response: 43842541
Conc: 502.04 ng/ml

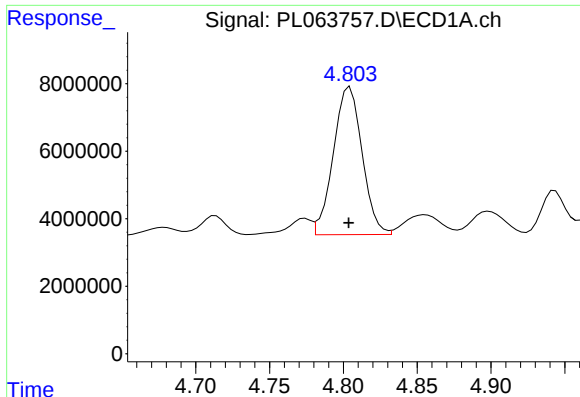

#24 Chlordane-2


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 59394349
Conc: 506.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122220CHLOR

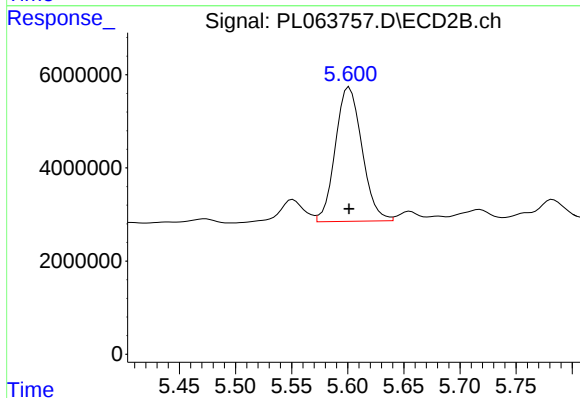


#24 Chlordane-2

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 47692573
Conc: 494.28 ng/ml

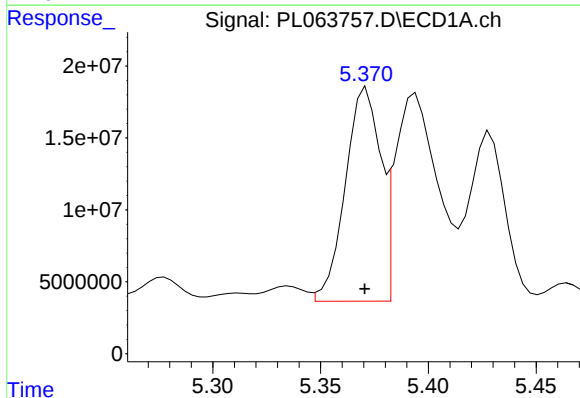


#25 Chlordane-3

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 167819197
Conc: 513.57 ng/ml

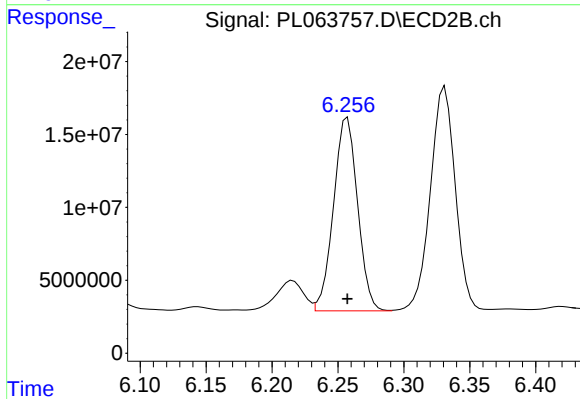

#25 Chlordane-3


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 168422064
Conc: 491.55 ng/ml

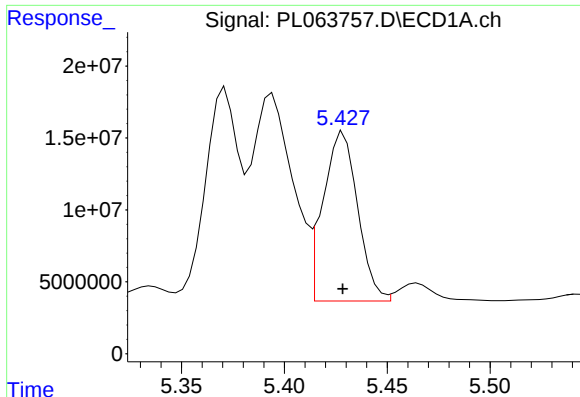

#26 Chlordane-4


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 137600682
Conc: 514.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122220CHLOR

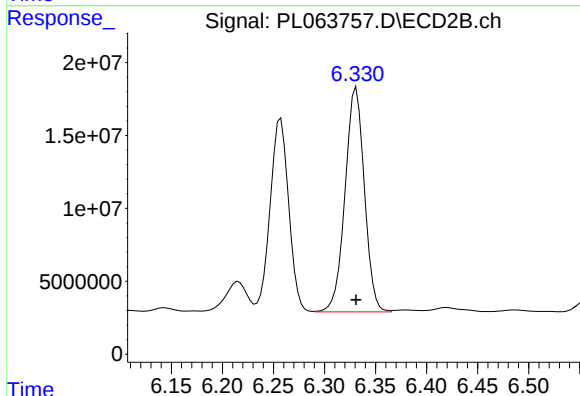


#26 Chlordane-4

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 202942986
Conc: 493.74 ng/ml

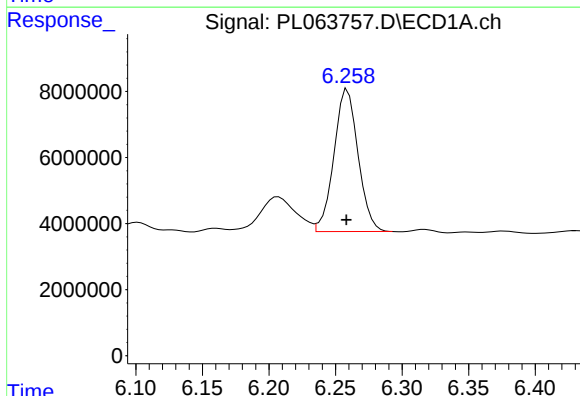


#27 Chlordane-5

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 54428978
Conc: 506.13 ng/ml

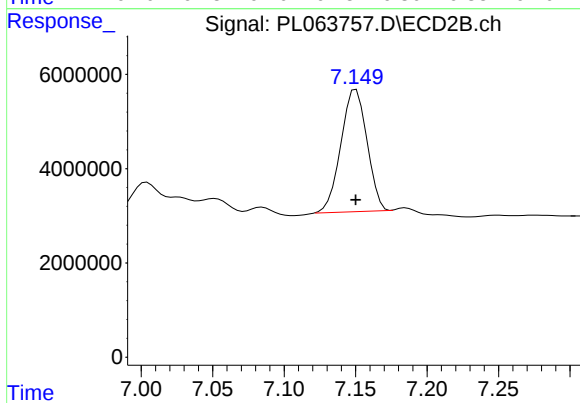

#27 Chlordane-5

R.T.: 7.150 min
Delta R.T.: 0.000 min
Response: 33024269
Conc: 500.01 ng/ml

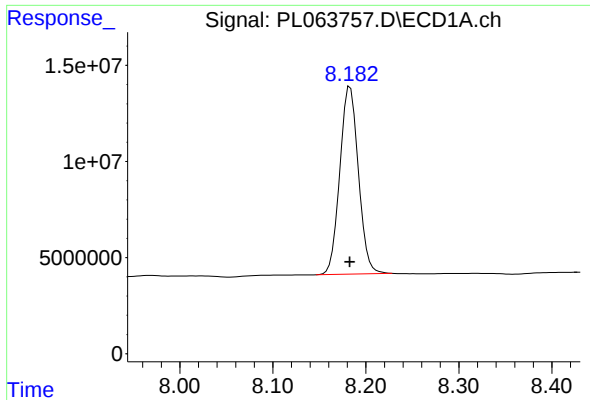

#28 Decachlorobiphenyl


R.T.: 8.183 min

Delta R.T.: 0.000 min

Response: 135621855

Conc: 47.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL122220CHLOR

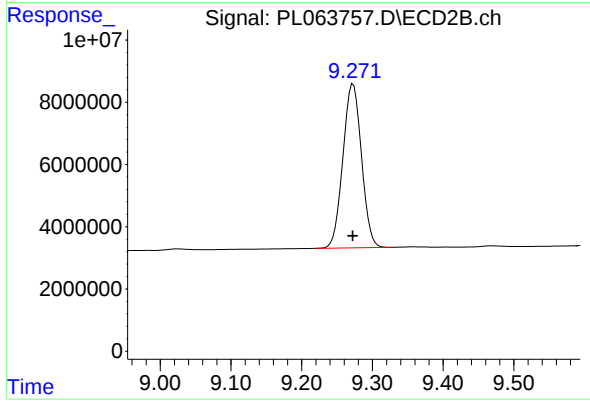

#28 Decachlorobiphenyl

R.T.: 9.273 min

Delta R.T.: 0.000 min

Response: 96171117

Conc: 47.04 ng/ml