

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
 Data File : PL063764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2020 15:51
 Operator : AR\AJ
 Sample : L5176-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26878

Manual Integrations
 APPROVED

Ankita
 12/23/2020 1:15:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 00:54:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	4.112	35767448	32893757	11.931	12.884
28) SA Decachlor...	8.181	9.271	31162283	31578301	11.311	16.017 #
Target Compounds						
11) B alpha-Chl...	5.424	6.330	1956740	3477929	0.522m	1.260 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122220\
Data File : PL063764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2020 15:51
Operator : AR\AJ
Sample : L5176-01
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
CHRT-26878


Manual Integrations
APPROVED

Ankita
12/23/2020 1:15:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 00:54:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

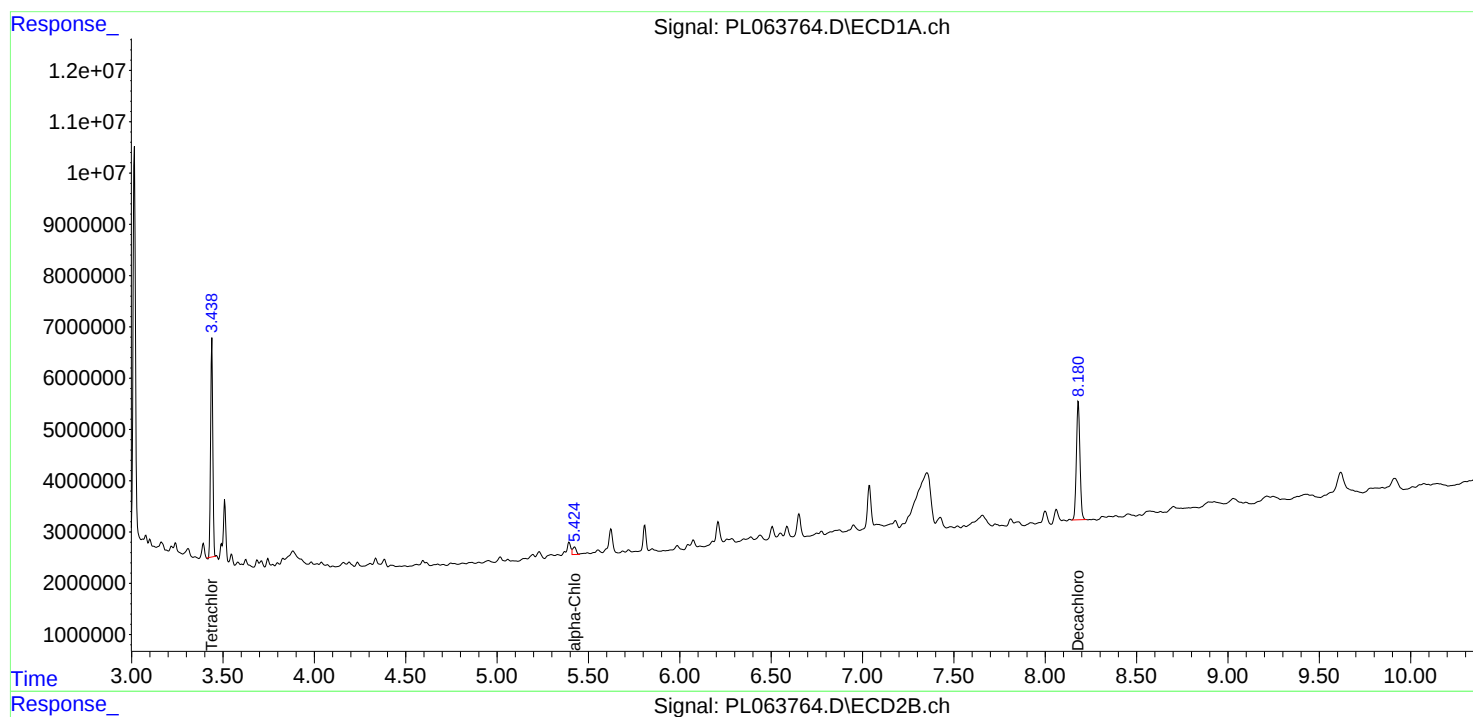

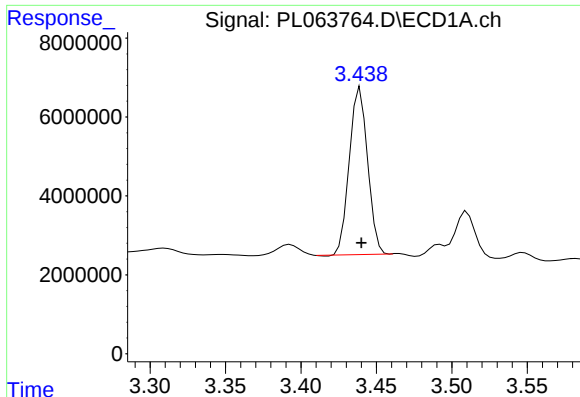


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 35767448
Conc: 11.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26878


Manual Integrations
APPROVED

Ankita
12/23/2020 1:15:35 PM

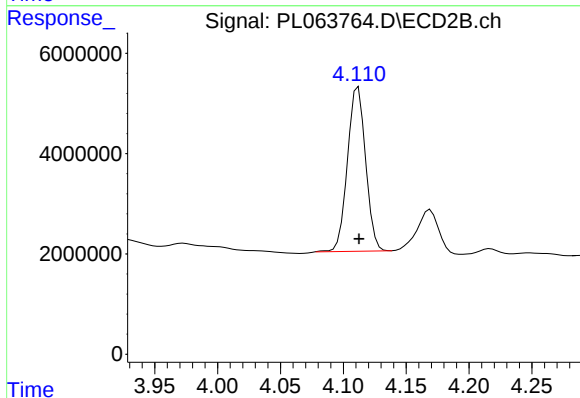


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 32893757
Conc: 12.88 ng/ml

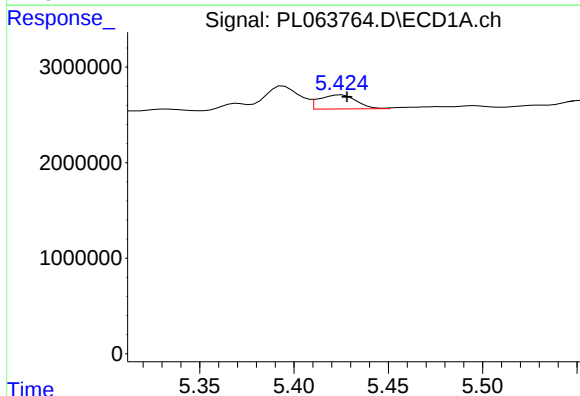


#11 alpha-Chlordane

R.T.: 5.424 min
Delta R.T.: -0.004 min
Response: 1956740
Conc: 0.52 ng/ml m

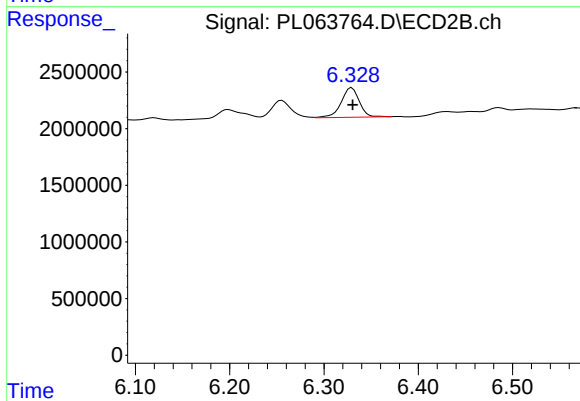

#11 alpha-Chlordane

R.T.: 6.330 min
Delta R.T.: -0.001 min
Response: 3477929
Conc: 1.26 ng/ml

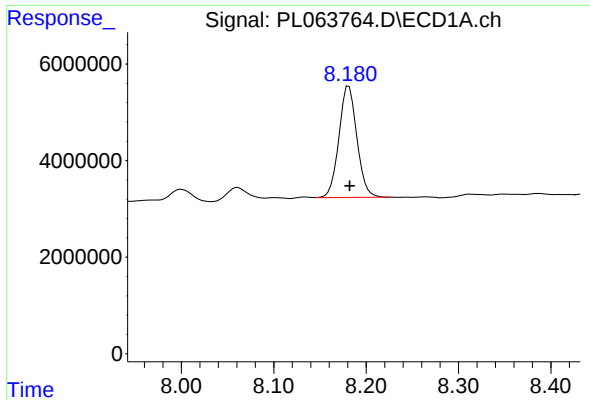


#28 Decachlorobiphenyl

R.T.: 8.181 min
Delta R.T.: 0.000 min
Response: 31162283
Conc: 11.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26878

Manual Integrations
APPROVED

Ankita
12/23/2020 1:15:35 PM

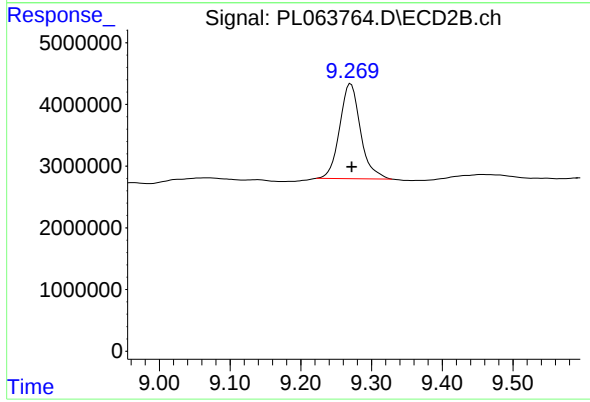

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: -0.001 min
Response: 31578301
Conc: 16.02 ng/ml