

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
 Data File : PL071564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 13:03
 Operator : AR\AJ
 Sample : PB141628BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 01:12:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.562	5.500	10184565	25606774	21.487	21.495
28)	SA Decachlor...	10.327	11.395	15328746	24509834	23.072	22.559
Target Compounds							
7)	B delta-BHC	0.000	7.023f	0	2322999	N.D.	1.520 #
8)	B Heptachlo...	0.000	7.938f	0	237965	N.D.	0.177 #
9)	A Endosulfan I	0.000	8.347	0	99664	N.D.	0.083 #
10)	B gamma-Chl...	0.000	8.233	0	251583	N.D.	0.195 #
11)	B alpha-Chl...	0.000	8.284f	0	68187	N.D.	0.054 #
19)	B Endosulfa...	0.000	9.502	0	64289	N.D.	0.066 #
25)	Chlordane-3	0.000	8.233	0	251583	N.D.	1.437 #
26)	Chlordane-4	0.000	8.284f	0	68187	N.D.	0.325 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
Data File : PL071564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 13:03
Operator : AR\AJ
Sample : PB141628BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 01:12:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

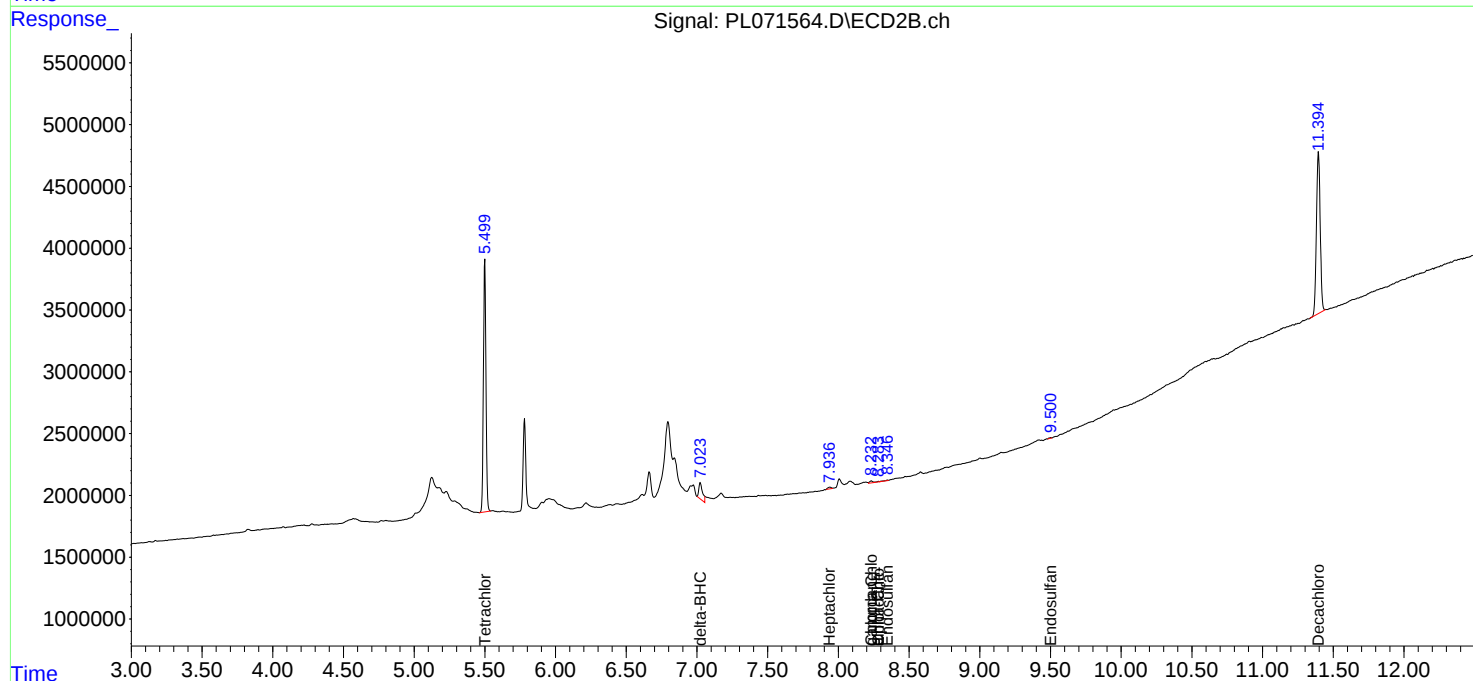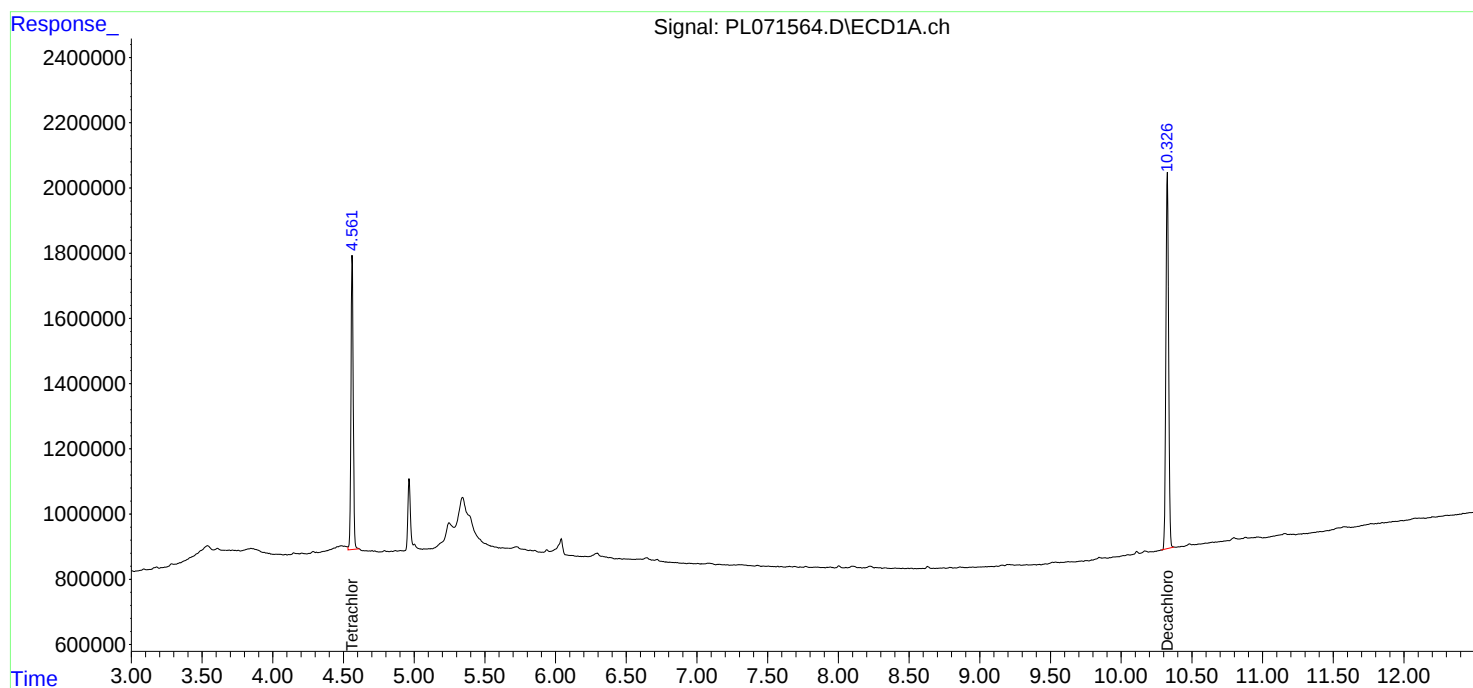


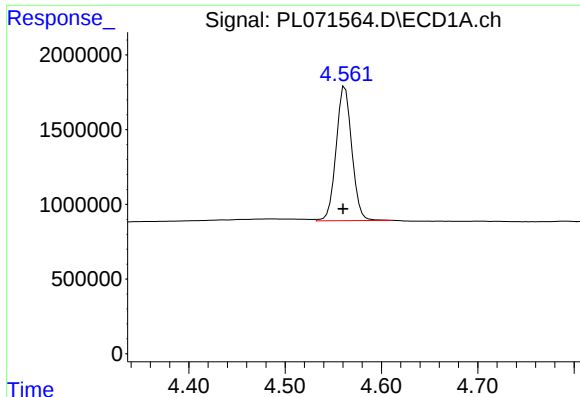

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: 0.002 min
Response: 10184565
Conc: 21.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

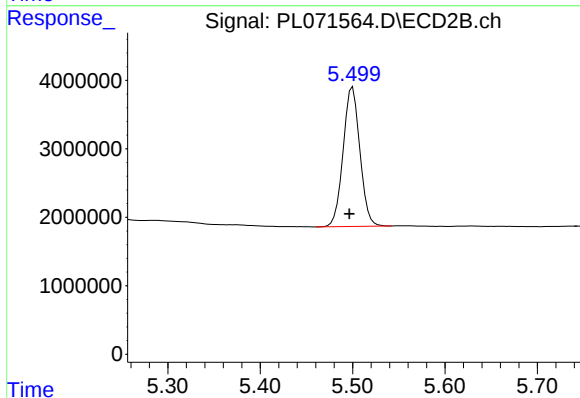


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.004 min
Response: 25606774
Conc: 21.49 ng/ml

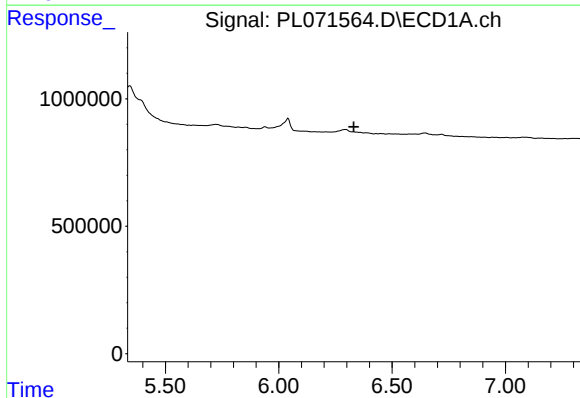


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

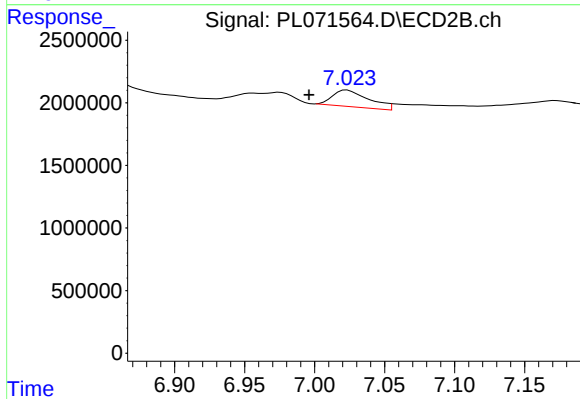

#7 delta-BHC


R.T.: 7.023 min
Delta R.T.: 0.027 min
Response: 2322999
Conc: 1.52 ng/ml

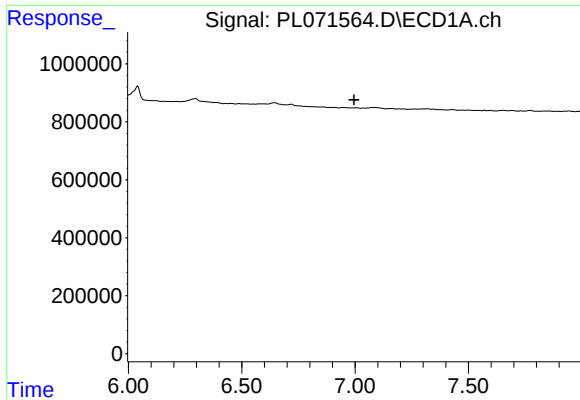

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

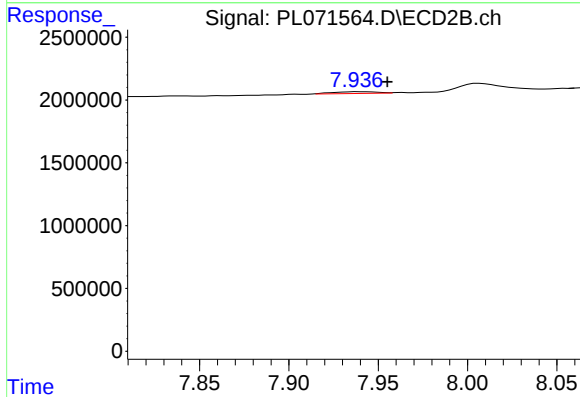


#8 Heptachlor epoxide

R.T.: 7.938 min
Delta R.T.: -0.017 min
Response: 237965
Conc: 0.18 ng/ml

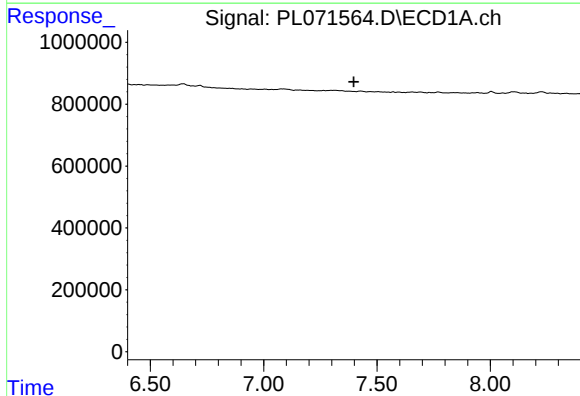


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

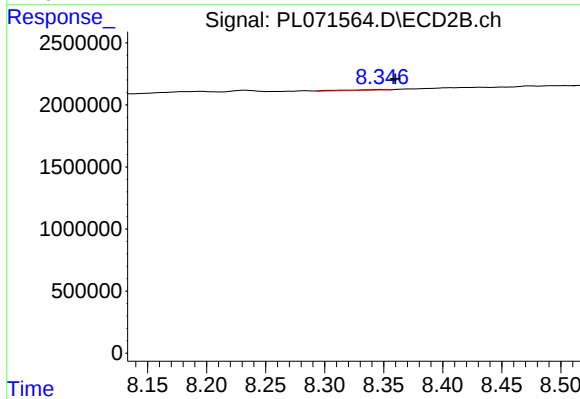

#9 Endosulfan I


R.T.: 8.347 min
Delta R.T.: -0.012 min
Response: 99664
Conc: 0.08 ng/ml

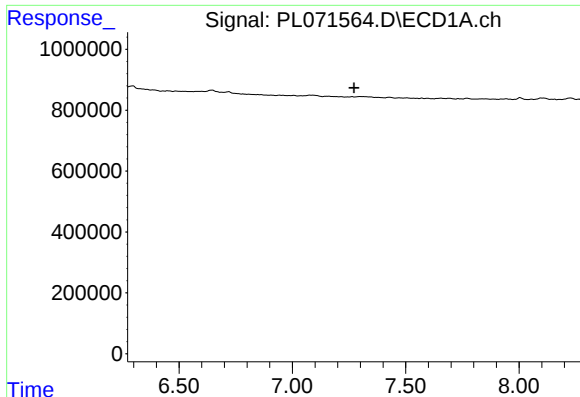

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

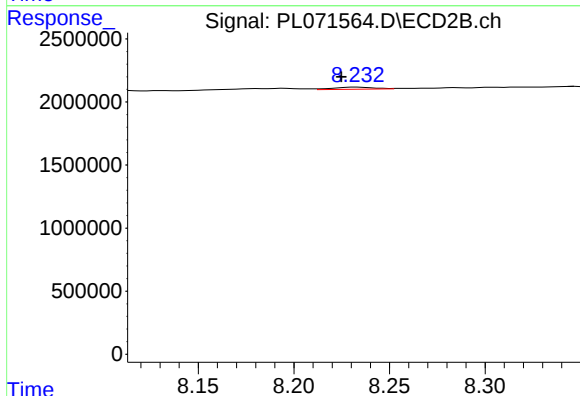


#10 gamma-Chlordane

R.T.: 8.233 min
Delta R.T.: 0.008 min
Response: 251583
Conc: 0.19 ng/ml

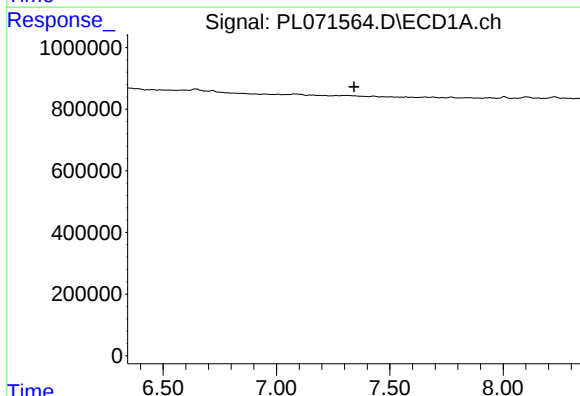


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.342 min
Response: 0
Conc: N.D.

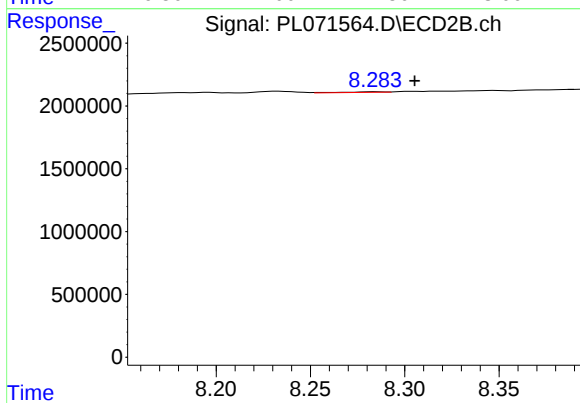

#11 alpha-Chlordane


R.T.: 8.284 min
Delta R.T.: -0.021 min
Response: 68187
Conc: 0.05 ng/ml

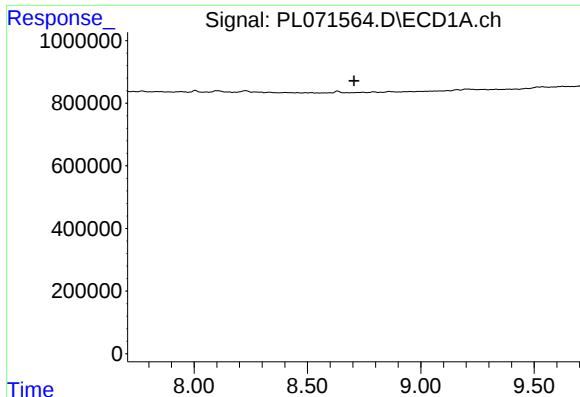

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

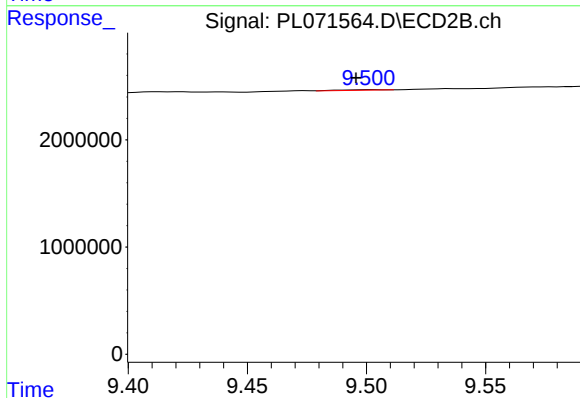


#19 Endosulfan Sulfate

R.T.: 9.502 min
Delta R.T.: 0.007 min
Response: 64289
Conc: 0.07 ng/ml

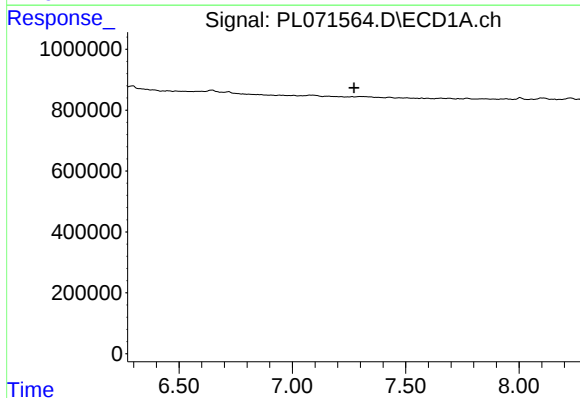


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

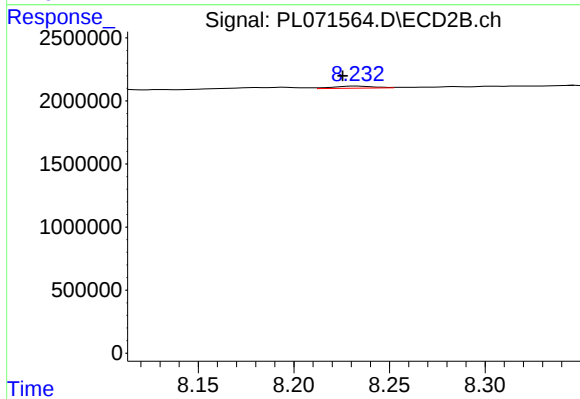

#25 Chlordane-3


R.T.: 8.233 min
Delta R.T.: 0.008 min
Response: 251583
Conc: 1.44 ng/ml

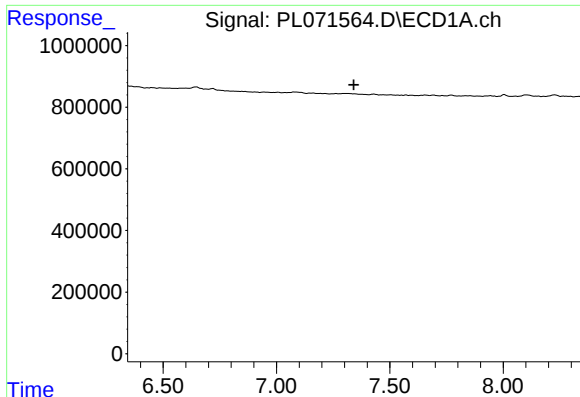

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

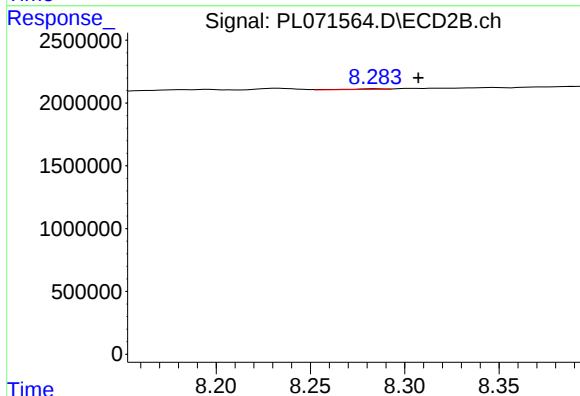


#26 Chlordane-4

R.T.: 8.284 min
Delta R.T.: -0.023 min
Response: 68187
Conc: 0.32 ng/ml

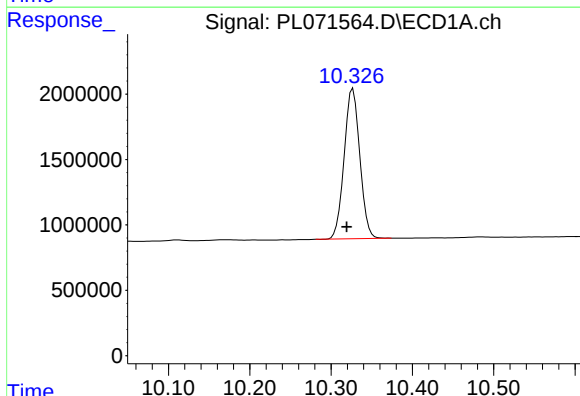

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.008 min
Response: 15328746
Conc: 23.07 ng/ml

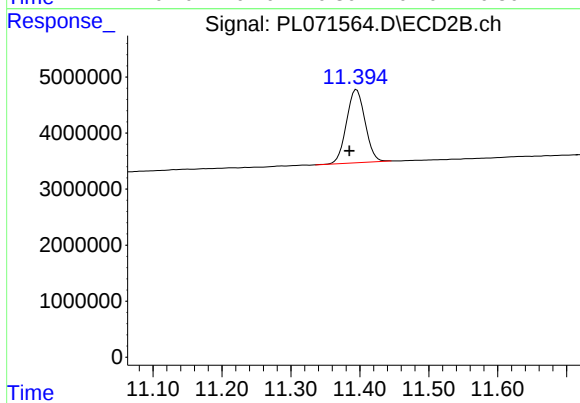

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.010 min
Response: 24509834
Conc: 22.56 ng/ml