

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
 Data File : PL071570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 16:02
 Operator : AR\AJ
 Sample : M5187-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 01:14:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.562	5.500	11509204	30027451	24.281	25.205
28)	SA Decachlor...	10.326	11.394	14640055	23968749	22.035	22.061
Target Compounds							
5)	MB Aldrin	0.000	7.477	0	271710	N.D.	0.186 #
10)	B gamma-Chl...	0.000	8.230	0	842468	N.D.	0.652 #
11)	B alpha-Chl...	0.000	8.316	0	179123	N.D.	0.141 #
12)	B 4,4'-DDE	0.000	8.504	0	72956	N.D.	0.061 #
23)	Chlordane-1	0.000	6.886	0	138416	N.D.	3.011 #
24)	Chlordane-2	0.000	7.477	0	271710	N.D.	5.762 #
25)	Chlordane-3	0.000	8.230	0	842468	N.D.	4.813 #
26)	Chlordane-4	0.000	8.316	0	179123	N.D.	0.853 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
Data File : PL071570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 16:02
Operator : AR\AJ
Sample : M5187-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 01:14:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

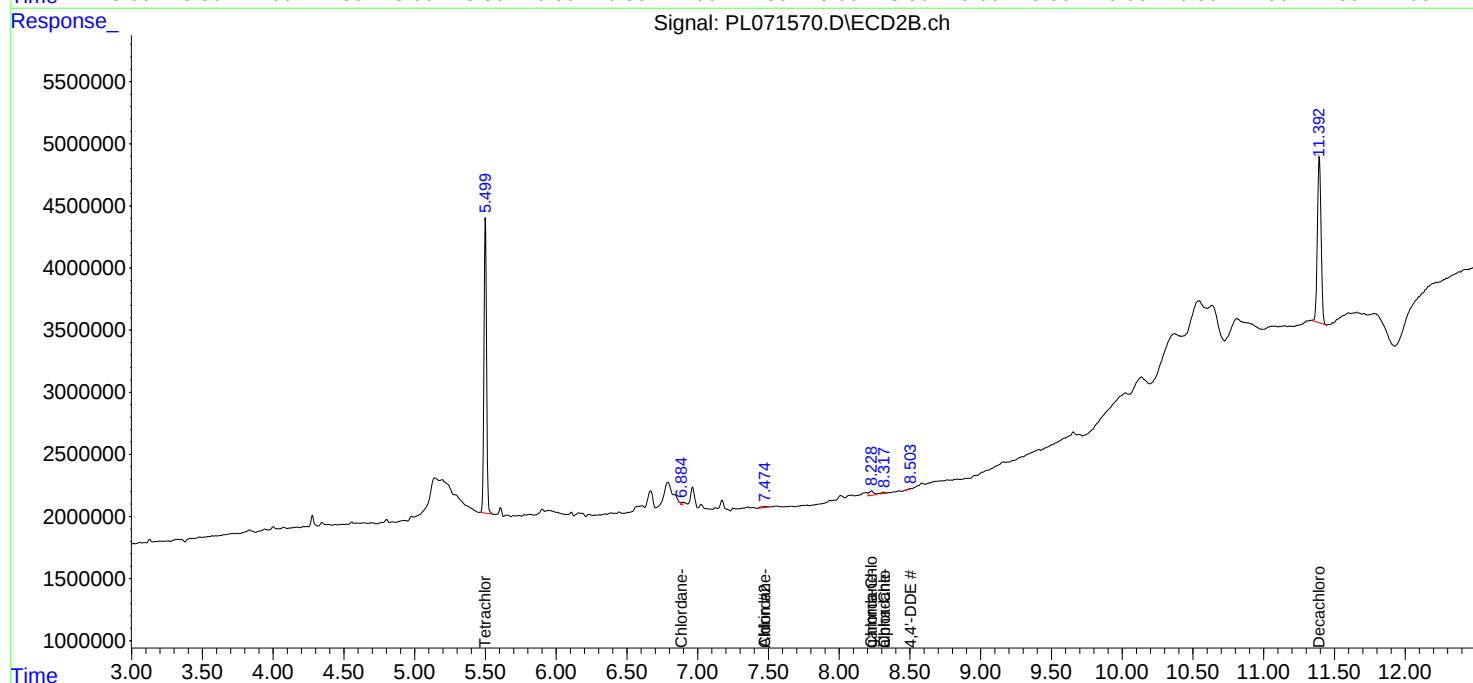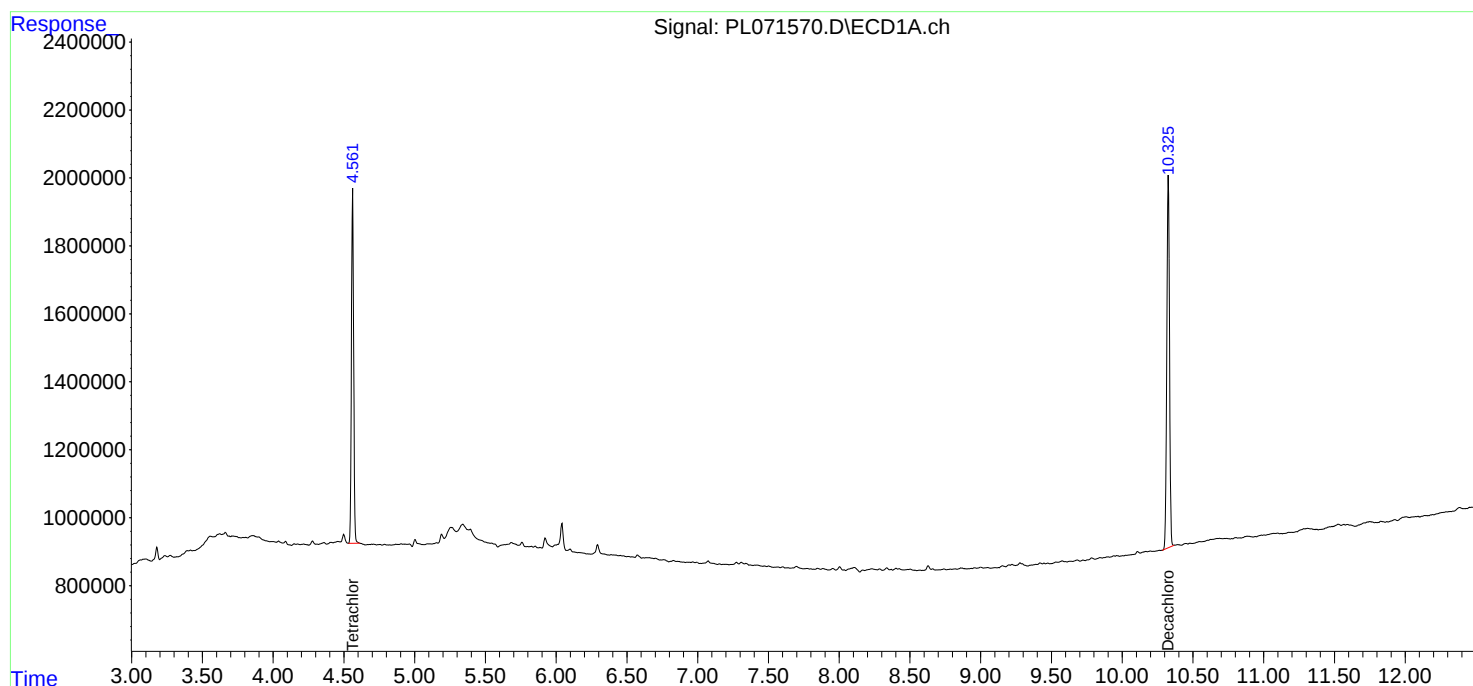


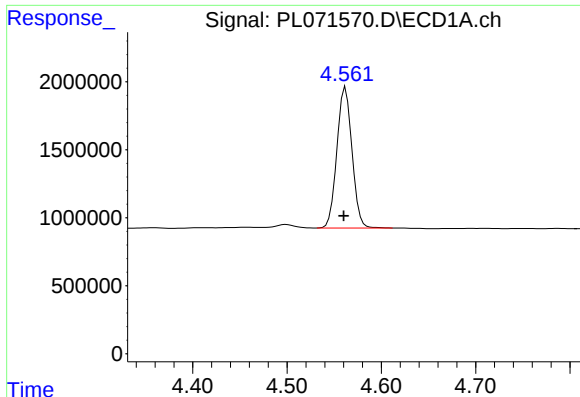

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: 0.002 min
Response: 11509204
Conc: 24.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

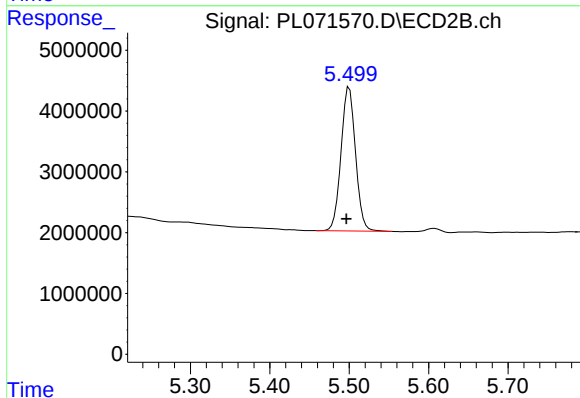


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: 0.004 min
Response: 30027451
Conc: 25.21 ng/ml

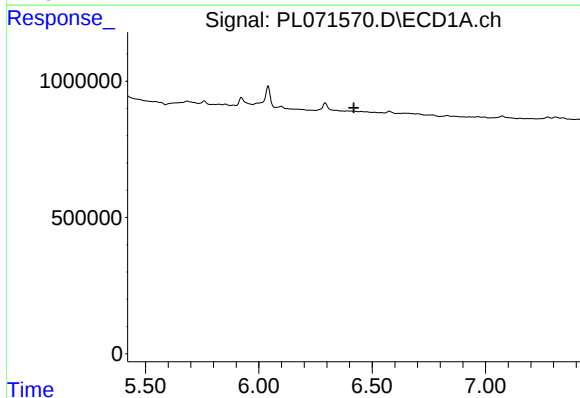


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

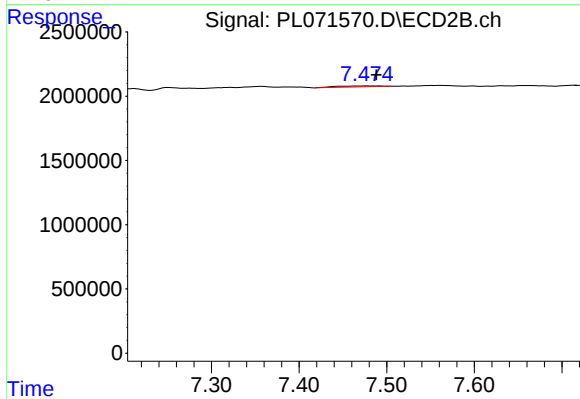

#5 Aldrin


R.T.: 7.477 min
Delta R.T.: -0.011 min
Response: 271710
Conc: 0.19 ng/ml

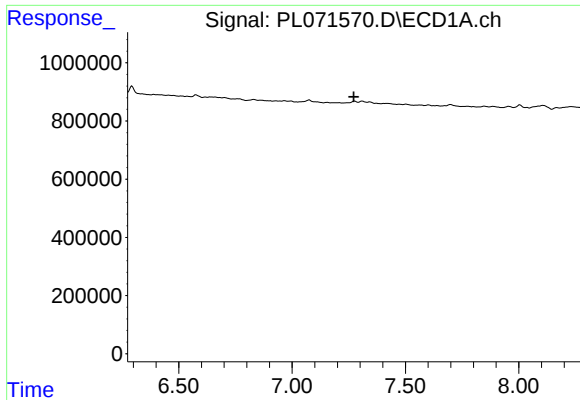

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

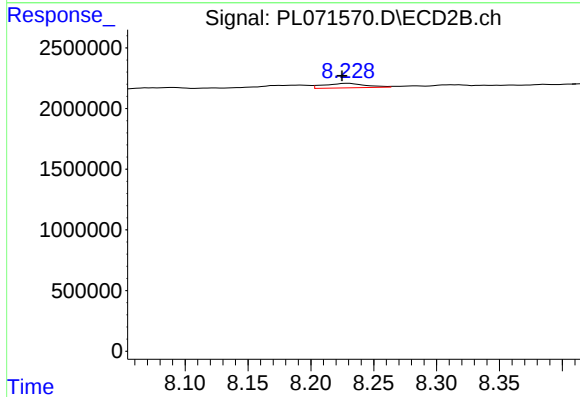


#10 gamma-Chlordane

R.T.: 8.230 min
Delta R.T.: 0.005 min
Response: 842468
Conc: 0.65 ng/ml

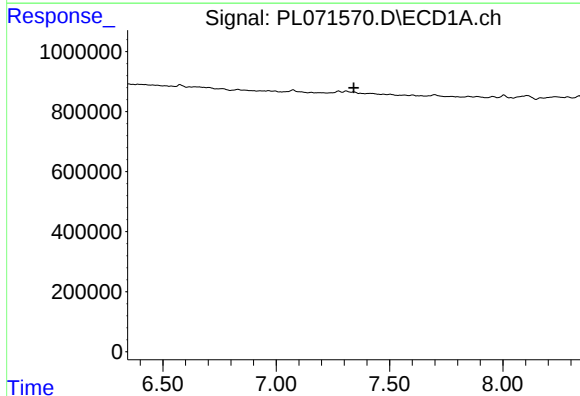


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.342 min
Response: 0
Conc: N.D.

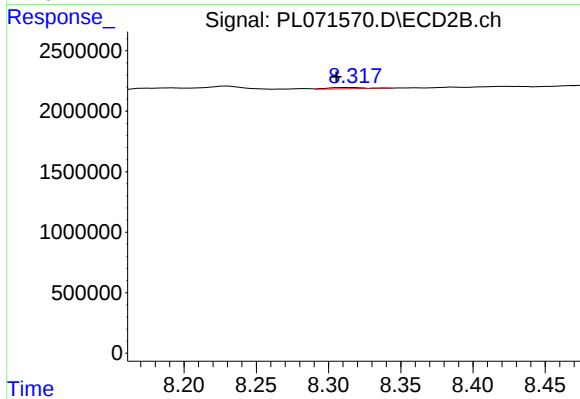

#11 alpha-Chlordane


R.T.: 8.316 min
Delta R.T.: 0.010 min
Response: 179123
Conc: 0.14 ng/ml

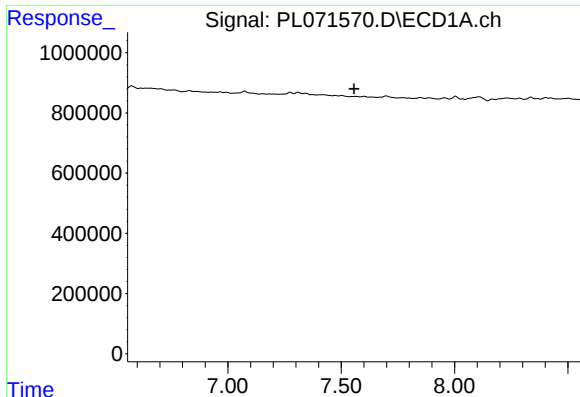

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.557 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

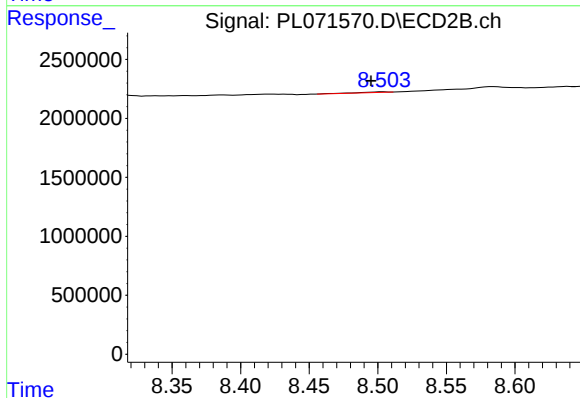


#12 4,4'-DDE

R.T.: 8.504 min
Delta R.T.: 0.009 min
Response: 72956
Conc: 0.06 ng/ml

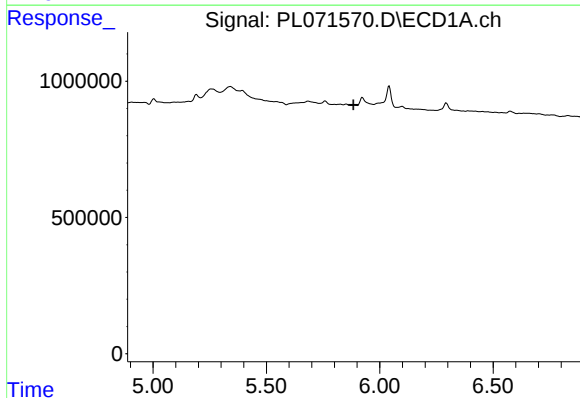


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

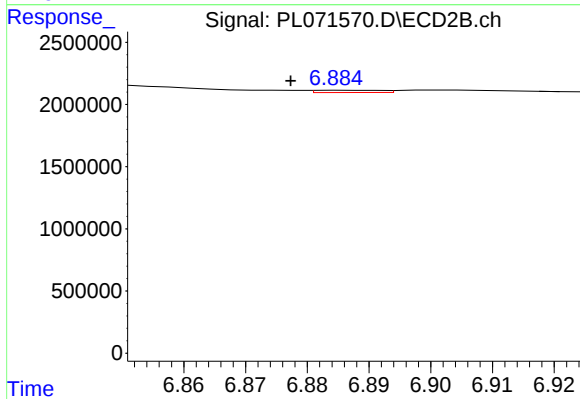

#23 Chlordane-1


R.T.: 6.886 min
Delta R.T.: 0.008 min
Response: 138416
Conc: 3.01 ng/ml

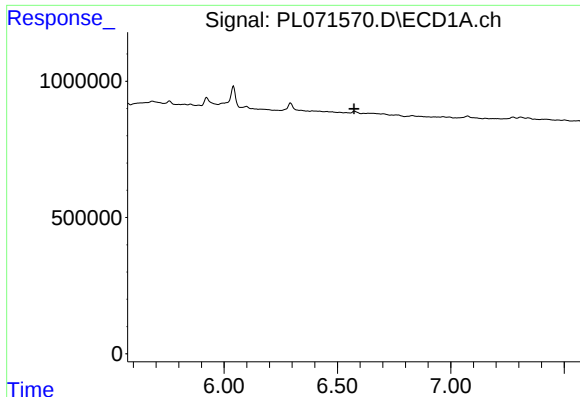

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

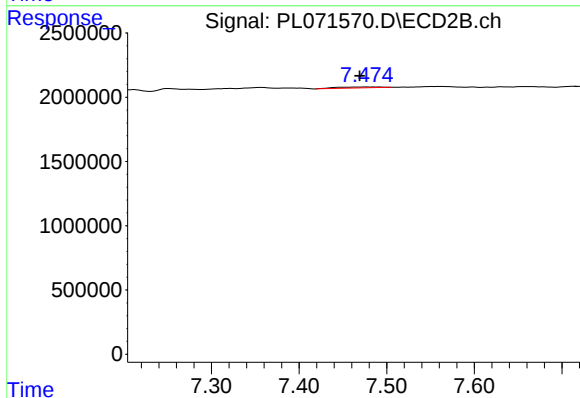


#24 Chlordane-2

R.T.: 7.477 min
Delta R.T.: 0.008 min
Response: 271710
Conc: 5.76 ng/ml

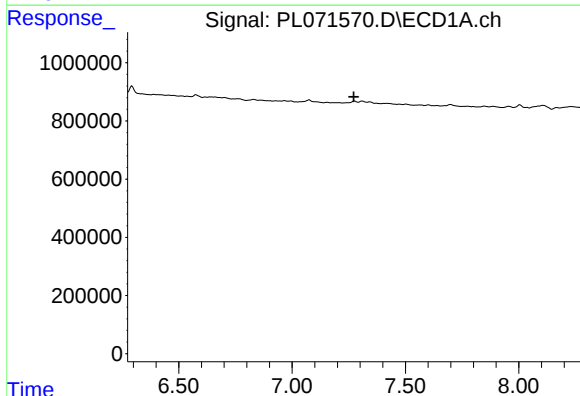


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

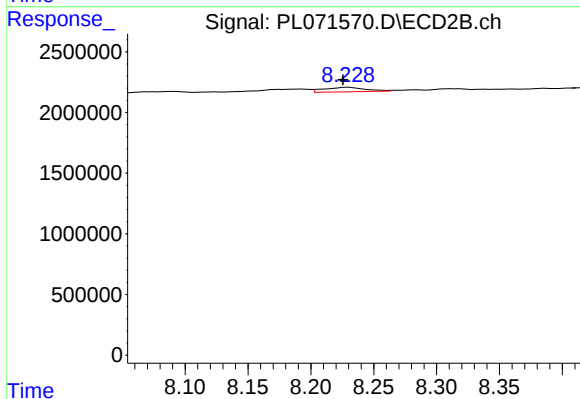

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.004 min
Response: 842468
Conc: 4.81 ng/ml

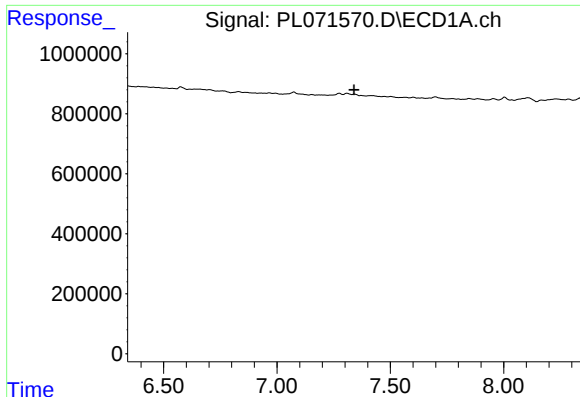

#26 Chlorine-4


R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

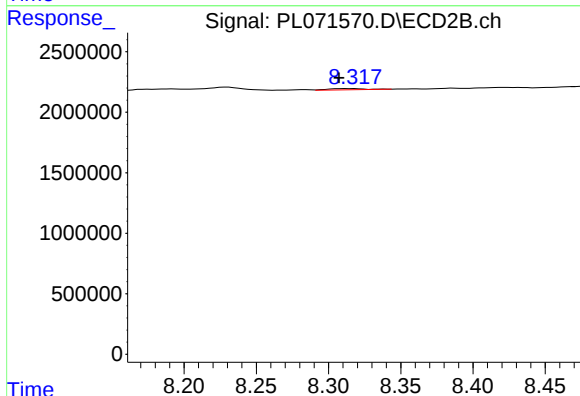


#26 Chlorine-4

R.T.: 8.316 min
Delta R.T.: 0.008 min
Response: 179123
Conc: 0.85 ng/ml

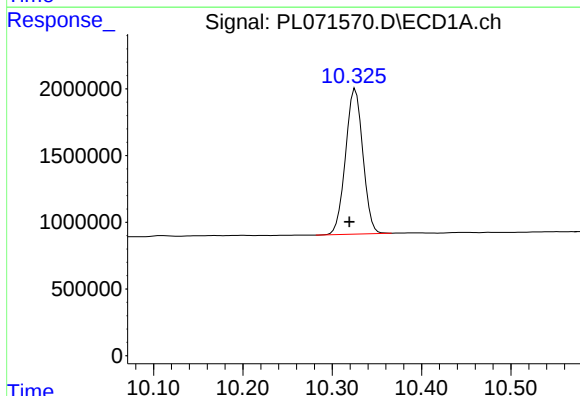

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.007 min
Response: 14640055
Conc: 22.04 ng/ml

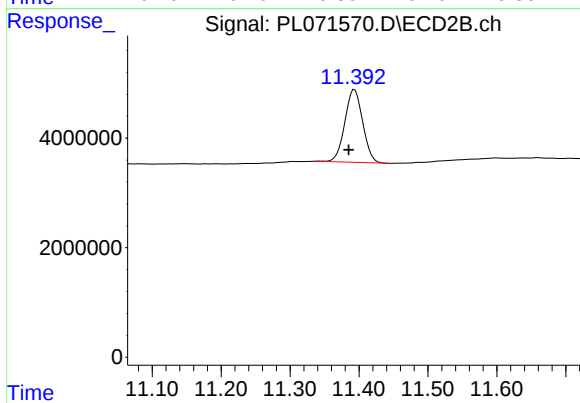

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.008 min
Response: 23968749
Conc: 22.06 ng/ml