

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
 Data File : PL071589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 22:40
 Operator : AR\AJ
 Sample : M5196-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 01:20:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.497	5334402	13362044	11.254	11.216
28)	SA Decachlor...	10.323	11.390	7972263	13641657	11.999	12.556
Target Compounds							
7)	B delta-BHC	0.000	7.023f	0	13035	N.D.	0.009 #
8)	B Heptachlo...	0.000	7.929f	0	255257	N.D.	0.190 #
9)	A Endosulfan I	0.000	8.331f	0	22287	N.D.	0.019 #
11)	B alpha-Chl...	0.000	8.303	0	61898	N.D.	0.049 #
13)	MA Dieldrin	0.000	8.674f	0	96295	N.D.	0.079 #
15)	B Endosulfa...	0.000	9.153f	0	247006	N.D.	0.245 #
26)	Chlordane-4	0.000	8.303	0	61898	N.D.	0.295 #
27)	Chlordane-5	0.000	9.203	0	669178	N.D.	19.046 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
Data File : PL071589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 22:40
Operator : AR\AJ
Sample : M5196-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 01:20:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

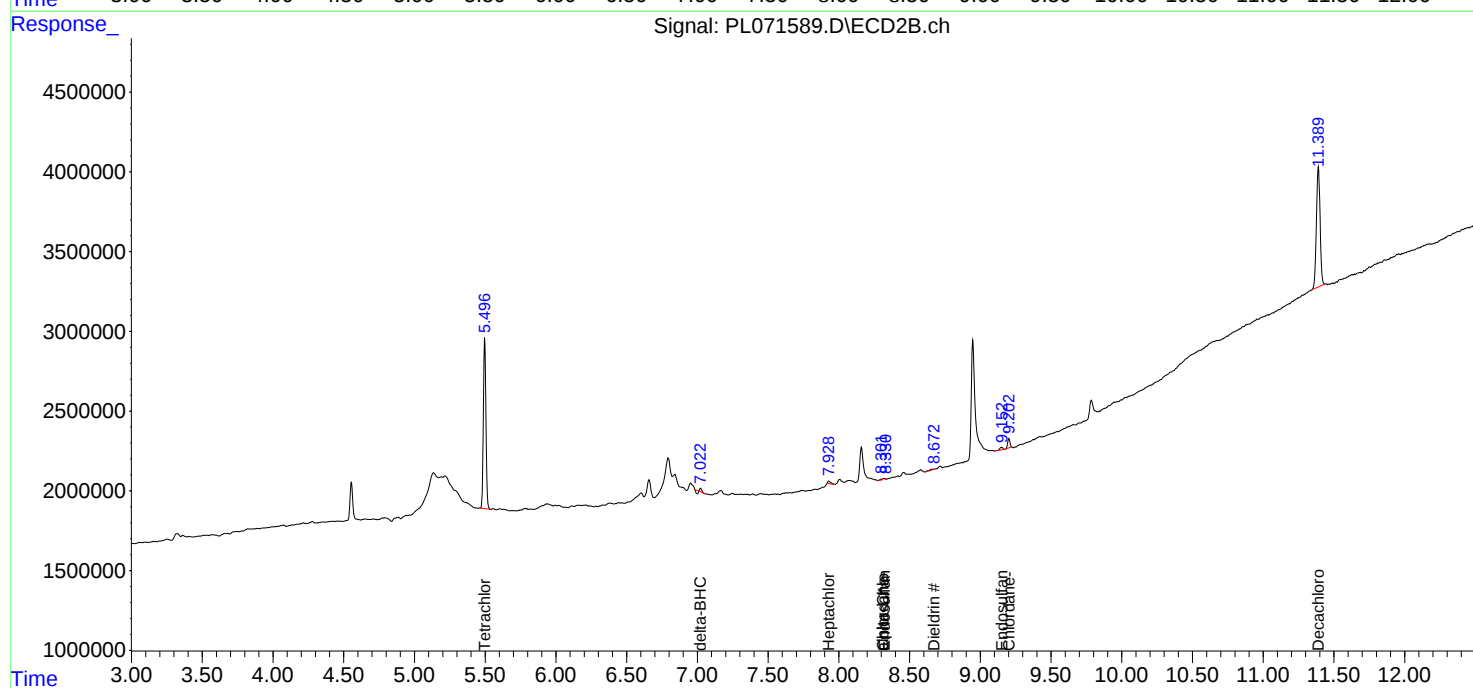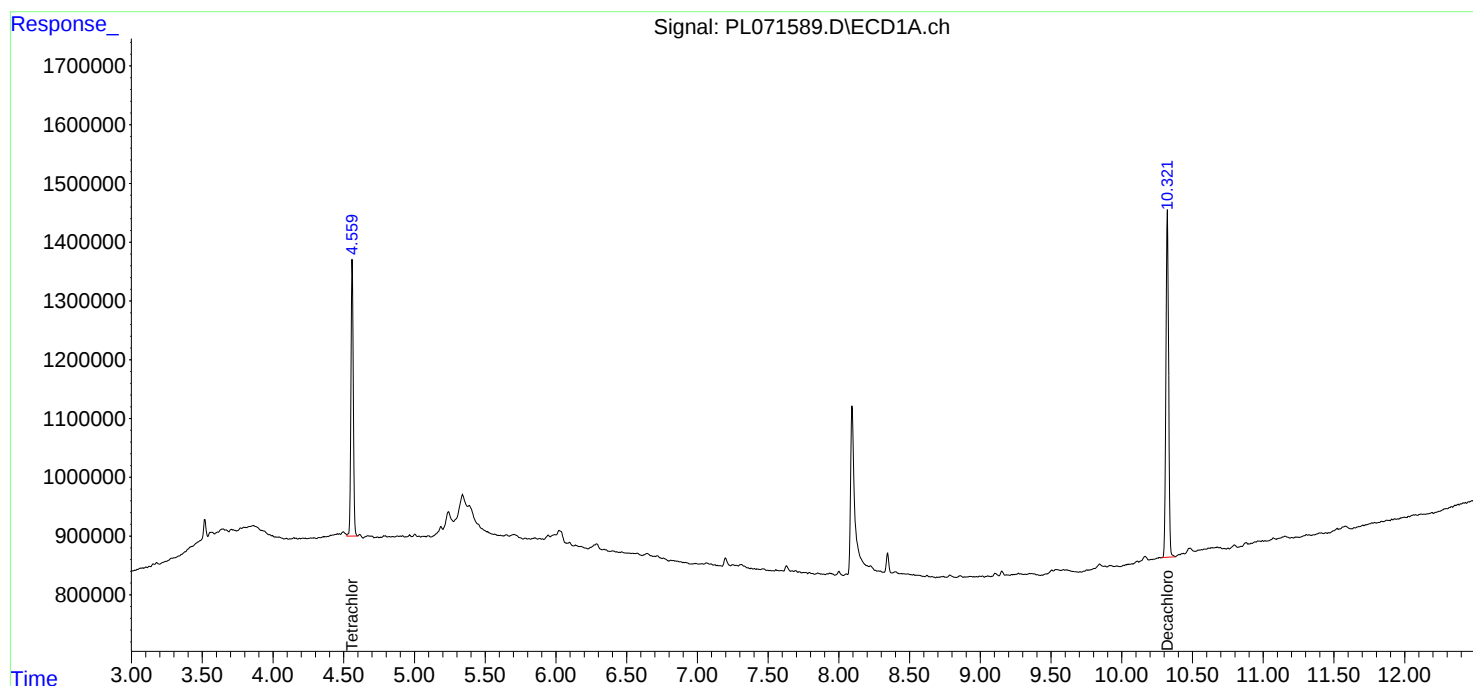


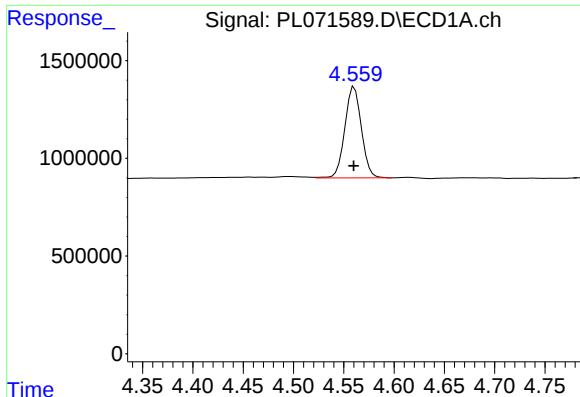

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 5334402
Conc: 11.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

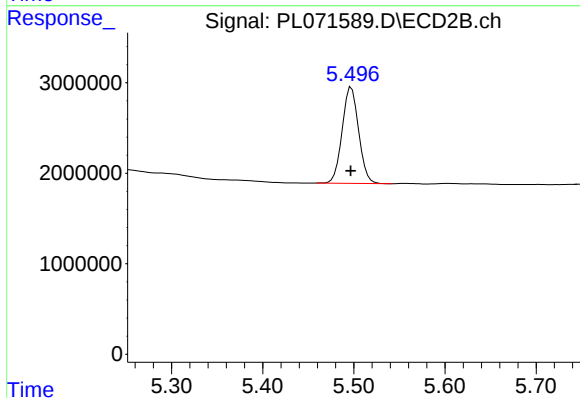


#1 Tetrachloro-m-xylene

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 13362044
Conc: 11.22 ng/ml

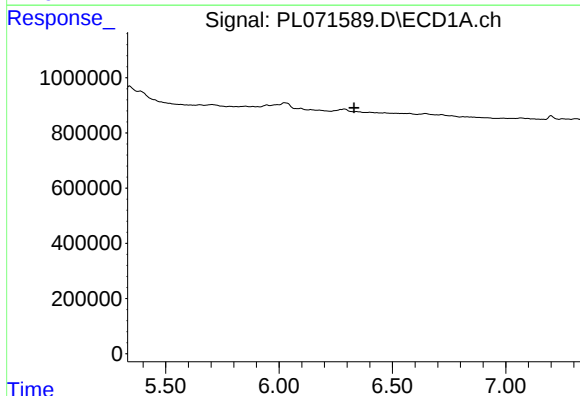


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

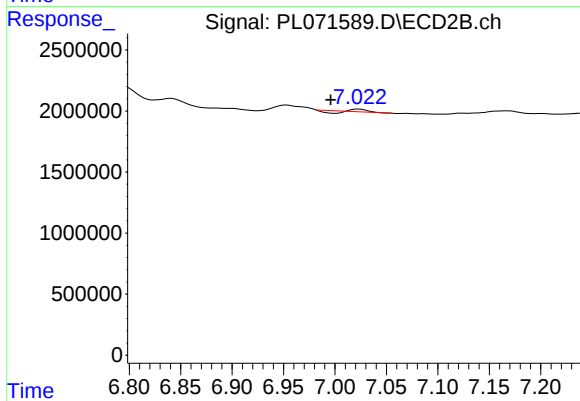

#7 delta-BHC


R.T.: 7.023 min
Delta R.T.: 0.027 min
Response: 13035
Conc: 0.01 ng/ml

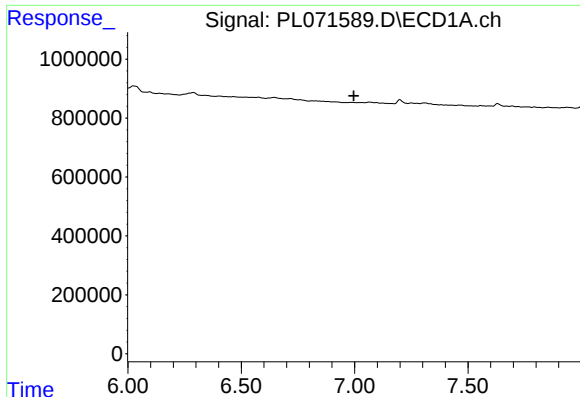

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

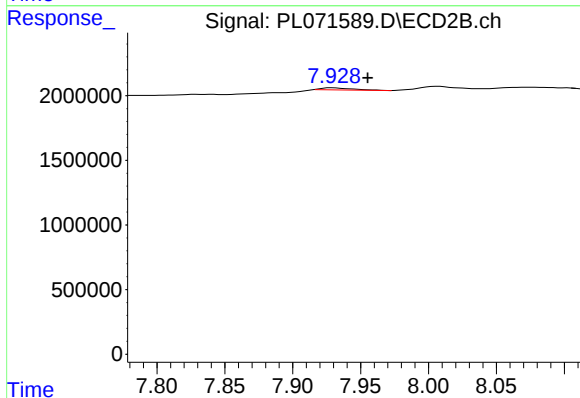


#8 Heptachlor epoxide

R.T.: 7.929 min
Delta R.T.: -0.026 min
Response: 255257
Conc: 0.19 ng/ml

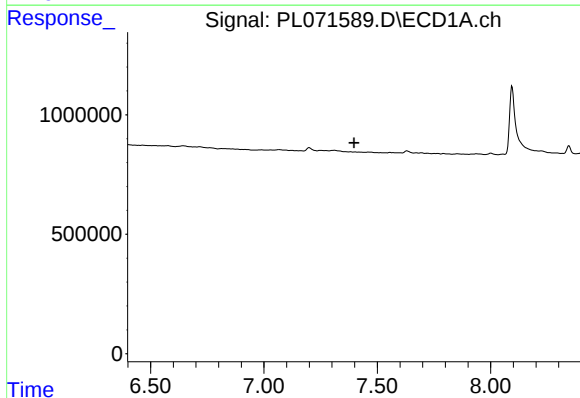


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

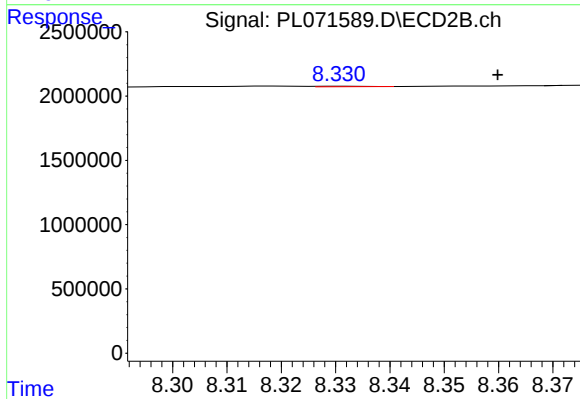

#9 Endosulfan I


R.T.: 8.331 min
Delta R.T.: -0.029 min
Response: 22287
Conc: 0.02 ng/ml

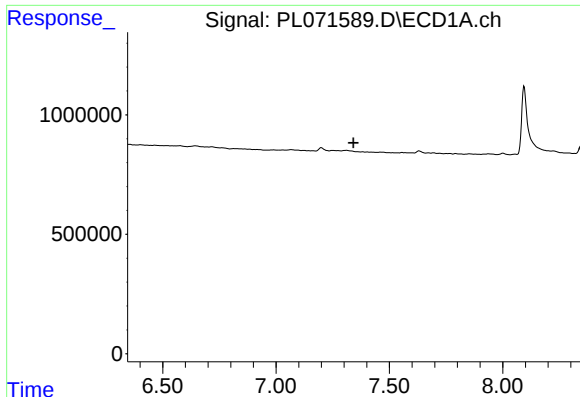

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

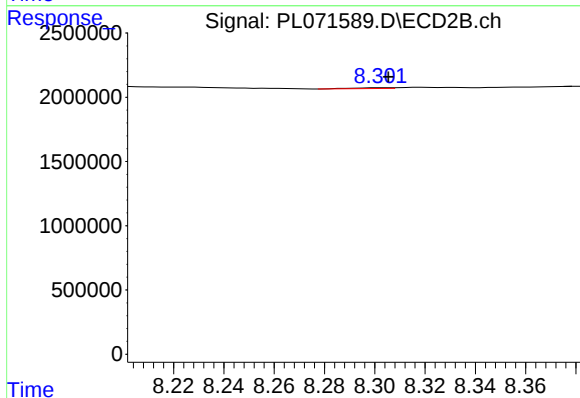


#11 alpha-Chlordane

R.T.: 8.303 min
Delta R.T.: -0.003 min
Response: 61898
Conc: 0.05 ng/ml

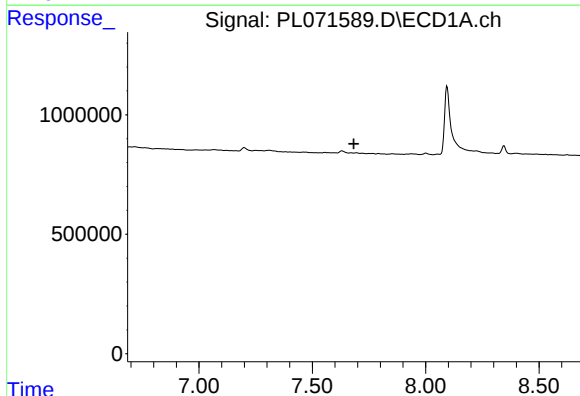


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.684 min
Response: 0
Conc: N.D.

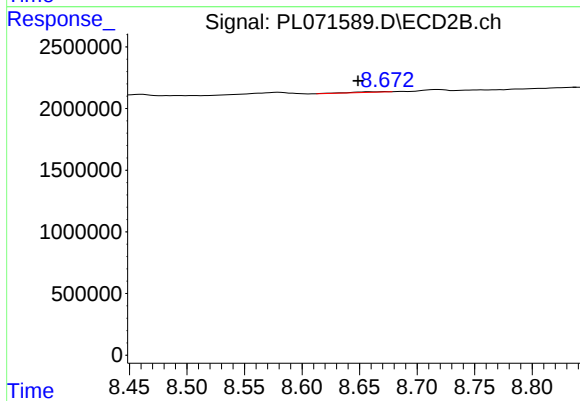

#13 Dieldrin


R.T.: 8.674 min
Delta R.T.: 0.025 min
Response: 96295
Conc: 0.08 ng/ml

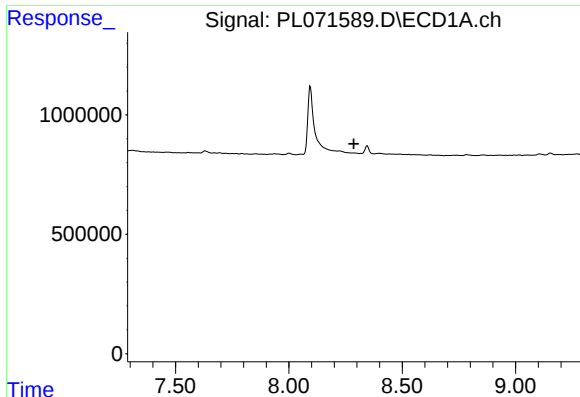

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

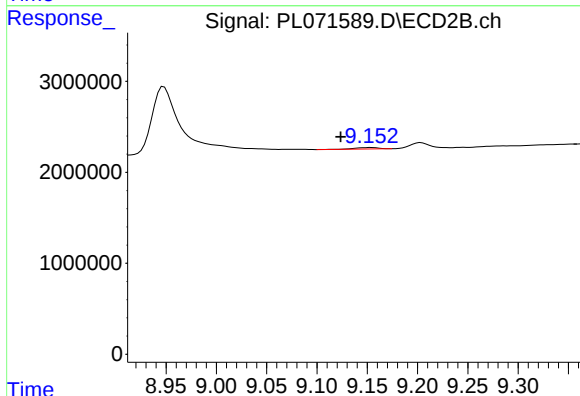


#15 Endosulfan II

R.T.: 9.153 min
Delta R.T.: 0.030 min
Response: 247006
Conc: 0.24 ng/ml

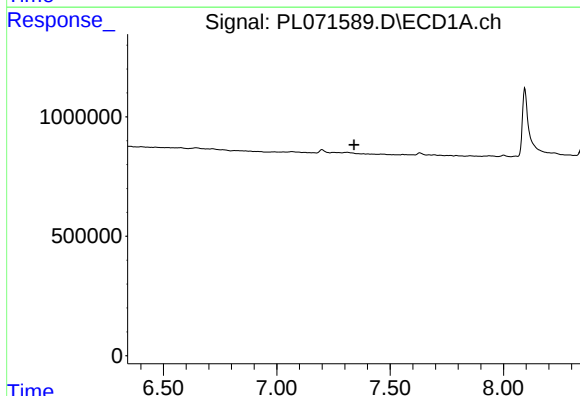


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

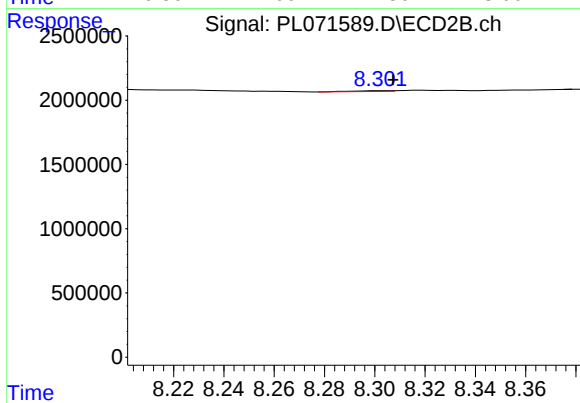

#26 Chlordane-4


R.T.: 8.303 min
Delta R.T.: -0.004 min
Response: 61898
Conc: 0.29 ng/ml

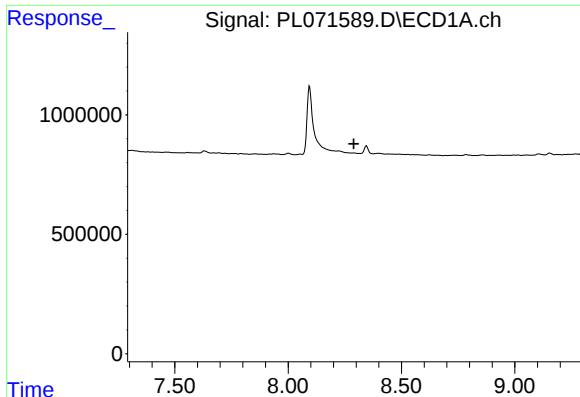

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

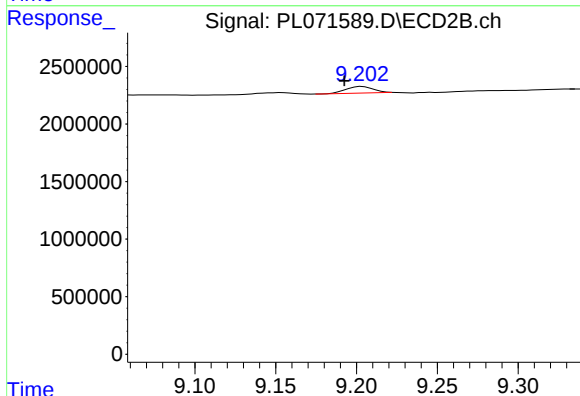


#27 Chlordane-5

R.T.: 9.203 min
Delta R.T.: 0.011 min
Response: 669178
Conc: 19.05 ng/ml

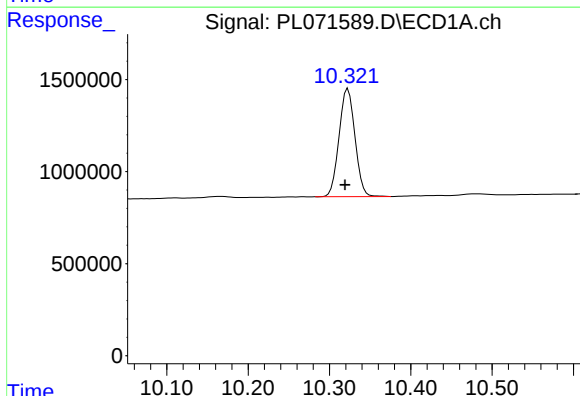

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: 0.004 min
Response: 7972263
Conc: 12.00 ng/ml

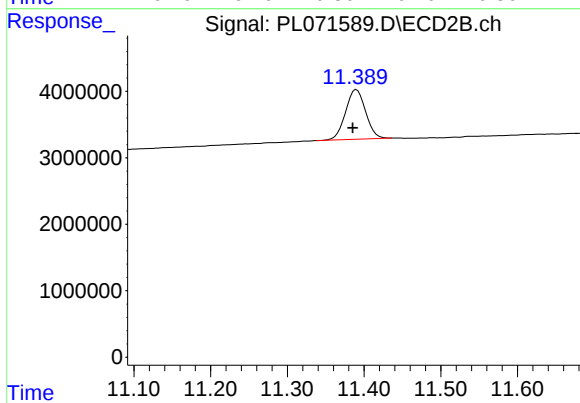

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.005 min
Response: 13641657
Conc: 12.56 ng/ml