

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
 Data File : PL071590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 22:57
 Operator : AR\AJ
 Sample : M5196-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 01:21:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.560	5.498	5736804	14246346	12.103	11.959
28)	SA Decachlor...	10.323	11.390	8429114	14623545	12.687	13.460
Target Compounds							
7)	B delta-BHC	0.000	7.026f	0	1311000	N.D.	0.858 #
8)	B Heptachlo...	0.000	7.929f	0	1716054	N.D.	1.279 #
12)	B 4,4'-DDE	7.576f	0.000	158265	0	0.290	N.D. #
15)	B Endosulfa...	0.000	9.151f	0	590223	N.D.	0.585 #
23)	Chlordane-1	0.000	6.896f	0	363016	N.D.	7.898 #
27)	Chlordane-5	0.000	9.204	0	179979	N.D.	5.123 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
Data File : PL071590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 22:57
Operator : AR\AJ
Sample : M5196-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 01:21:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

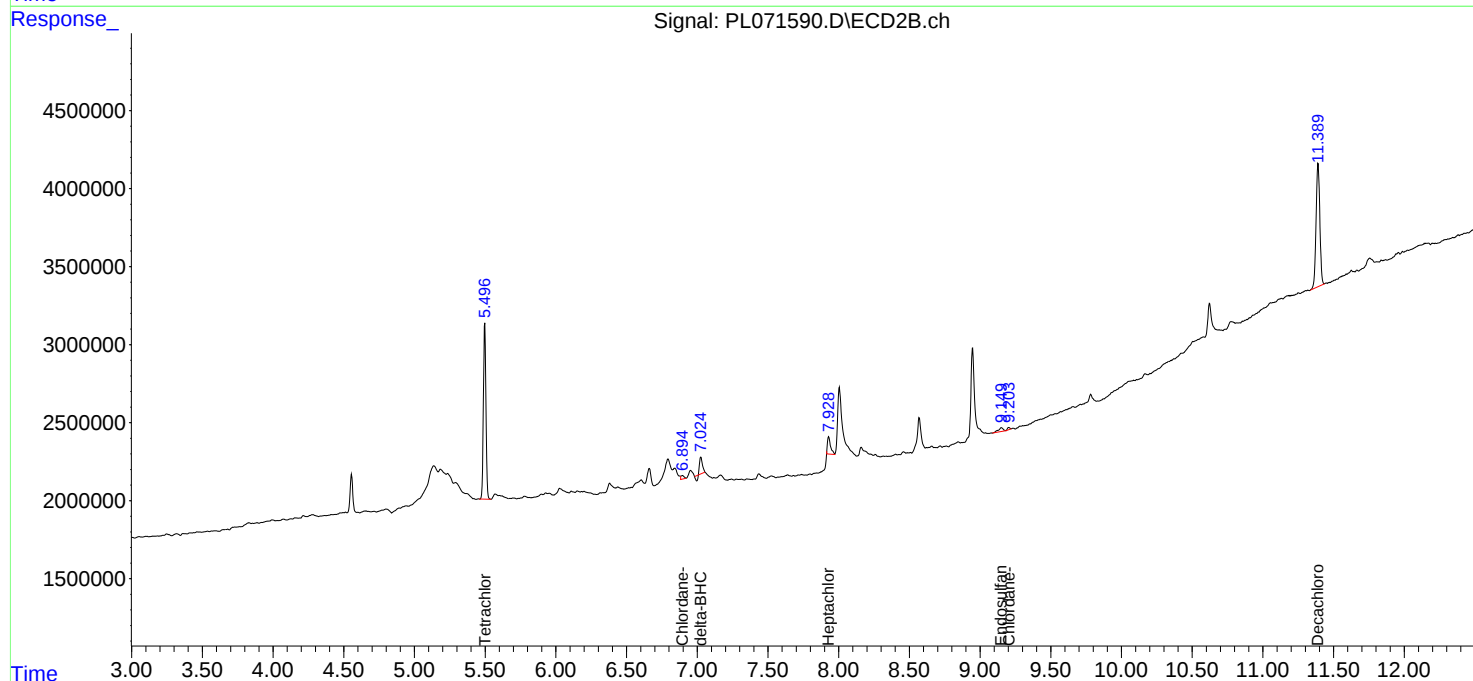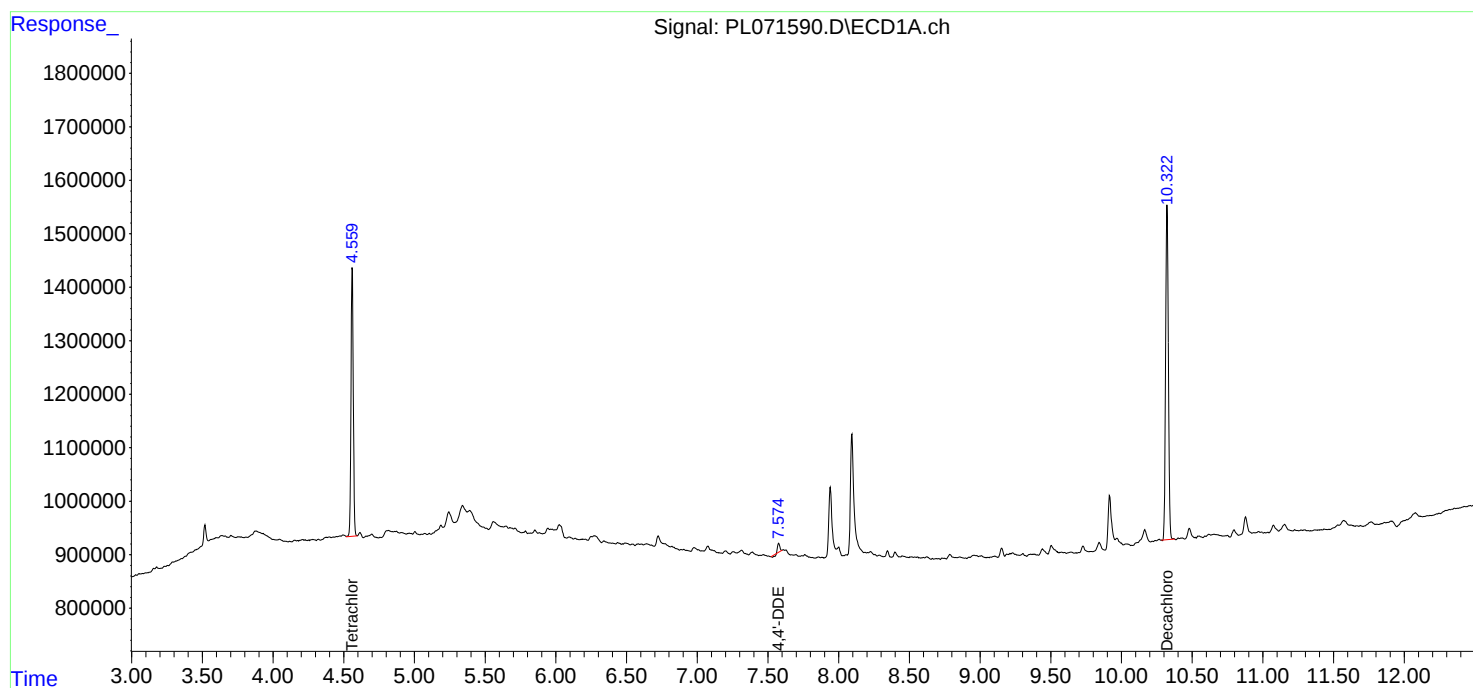


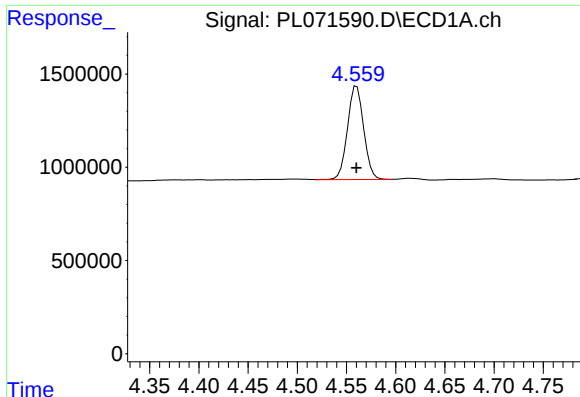

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 5736804
Conc: 12.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

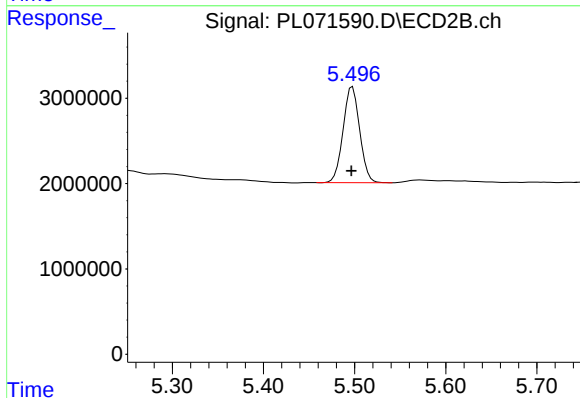


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: 0.001 min
Response: 14246346
Conc: 11.96 ng/ml

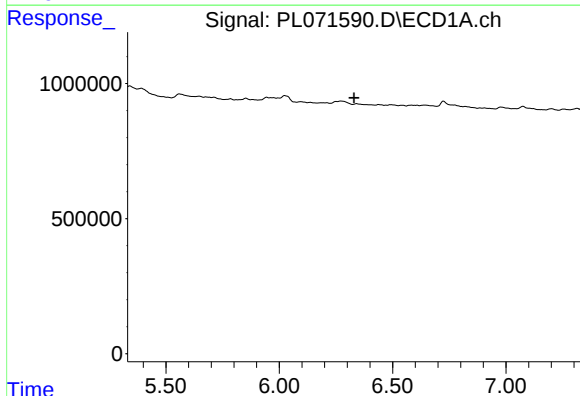


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.331 min
Response: 0
Conc: N.D.

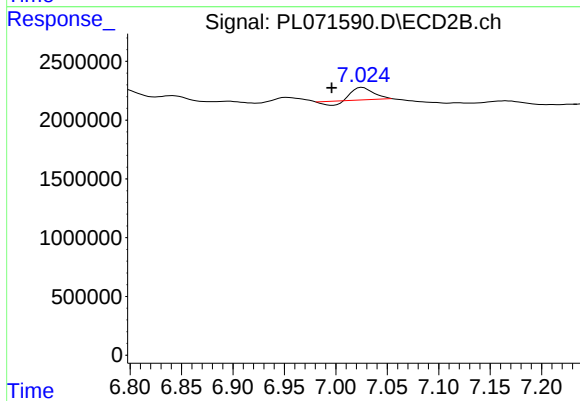

#7 delta-BHC


R.T.: 7.026 min
Delta R.T.: 0.030 min
Response: 1311000
Conc: 0.86 ng/ml

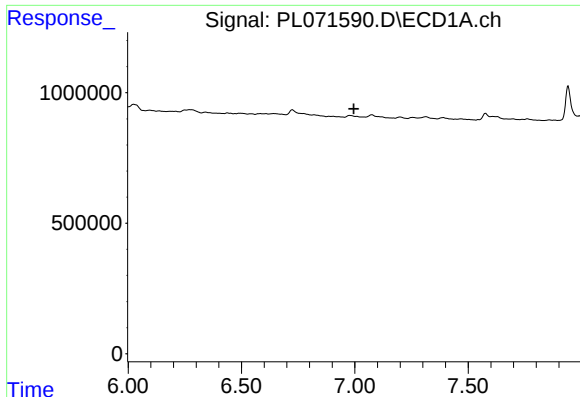

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

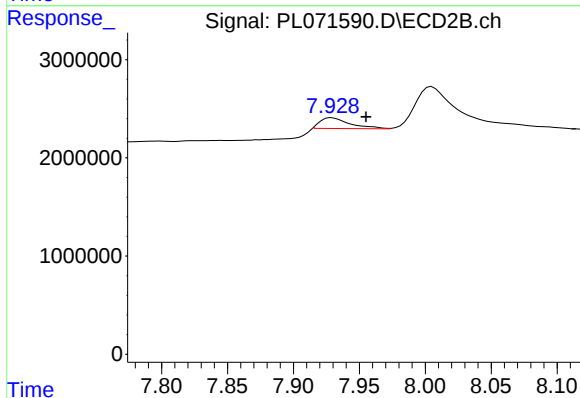


#8 Heptachlor epoxide

R.T.: 7.929 min
Delta R.T.: -0.026 min
Response: 1716054
Conc: 1.28 ng/ml

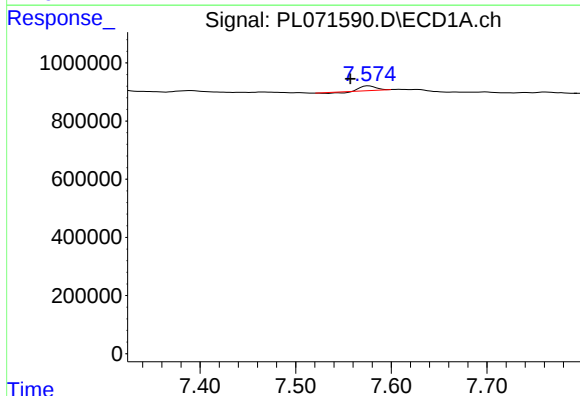


#12 4,4'-DDE

R.T.: 7.576 min
Delta R.T.: 0.019 min
Response: 158265
Conc: 0.29 ng/ml

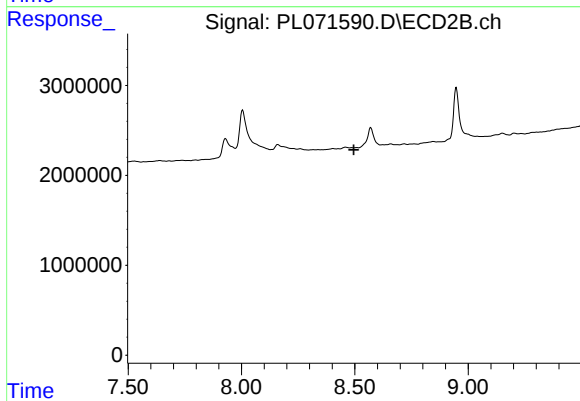

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 8.495 min
Response: 0
Conc: N.D.

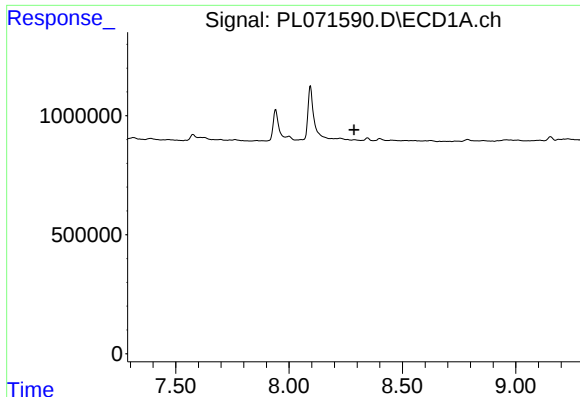

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

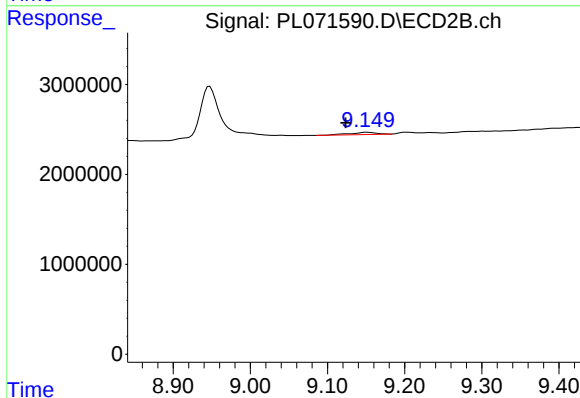


#15 Endosulfan II

R.T.: 9.151 min
Delta R.T.: 0.027 min
Response: 590223
Conc: 0.58 ng/ml

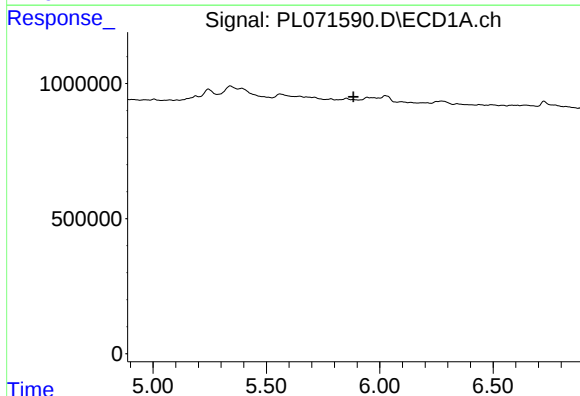


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

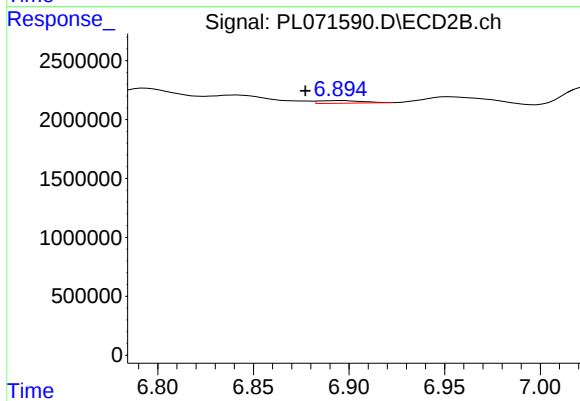

#23 Chlordane-1


R.T.: 6.896 min
Delta R.T.: 0.019 min
Response: 363016
Conc: 7.90 ng/ml

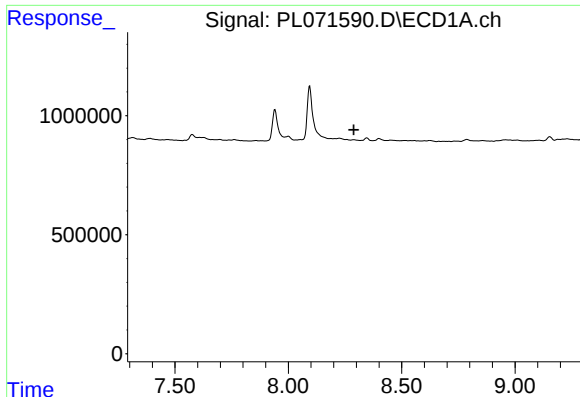

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

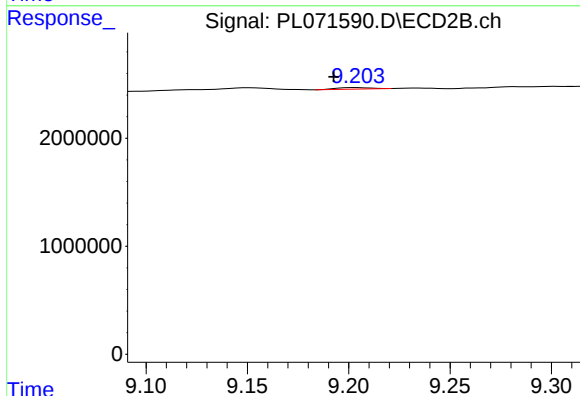


#27 Chlordane-5

R.T.: 9.204 min
Delta R.T.: 0.011 min
Response: 179979
Conc: 5.12 ng/ml

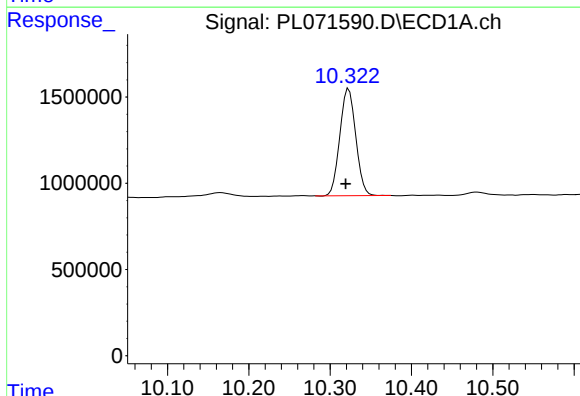

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: 0.004 min
Response: 8429114
Conc: 12.69 ng/ml

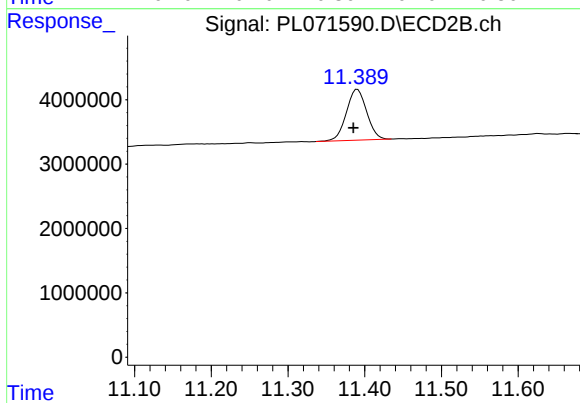

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.005 min
Response: 14623545
Conc: 13.46 ng/ml