

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
 Data File : PL071567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2021 15:12
 Operator : AR\AJ
 Sample : M5178-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-122021

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/23/2021
 Supervised By : Ankita Jodhani 12/23/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 01:13:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.498	8666945	20531961	18.285	17.235m
28)	SA Decachlor...	10.331	11.397	10207340	21262517	15.363	19.570m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122221\
Data File : PL071567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2021 15:12
Operator : AR\AJ
Sample : M5178-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-122021


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/23/2021
Supervised By : Ankita Jodhani 12/23/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 01:13:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

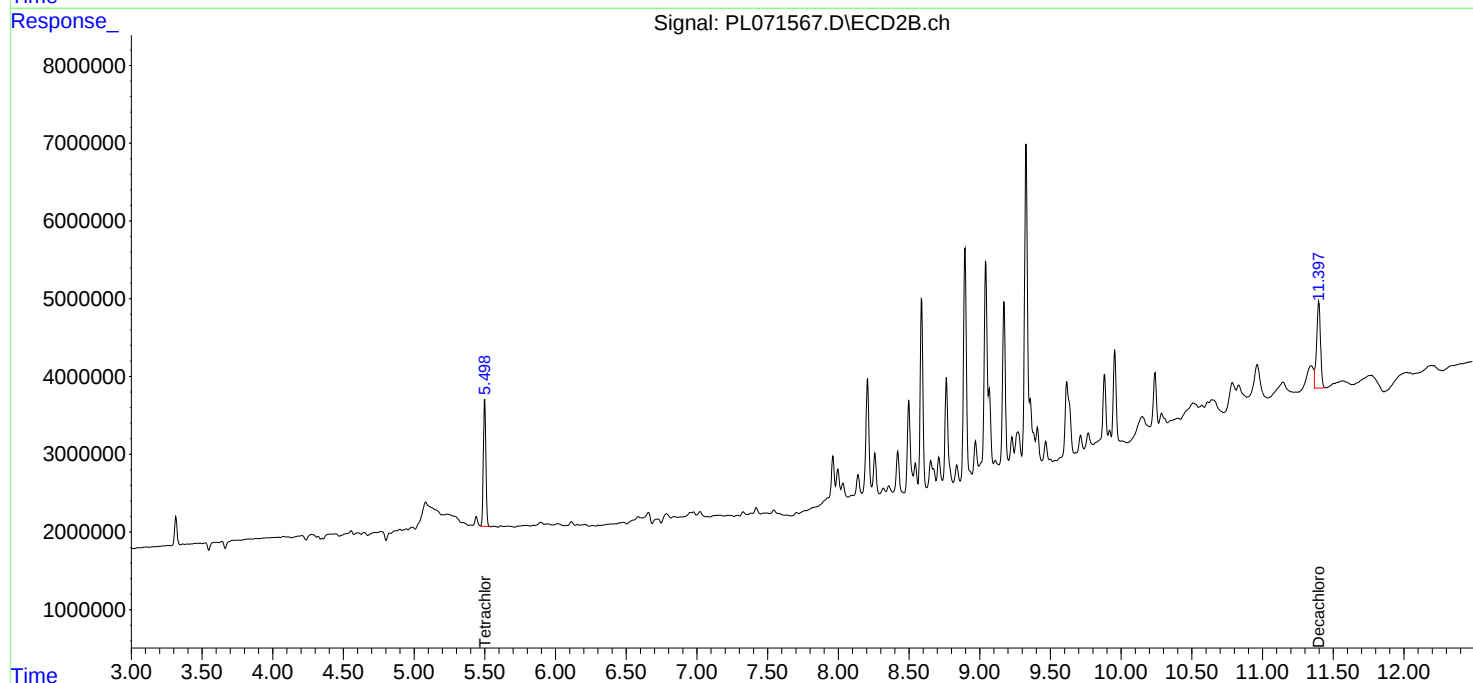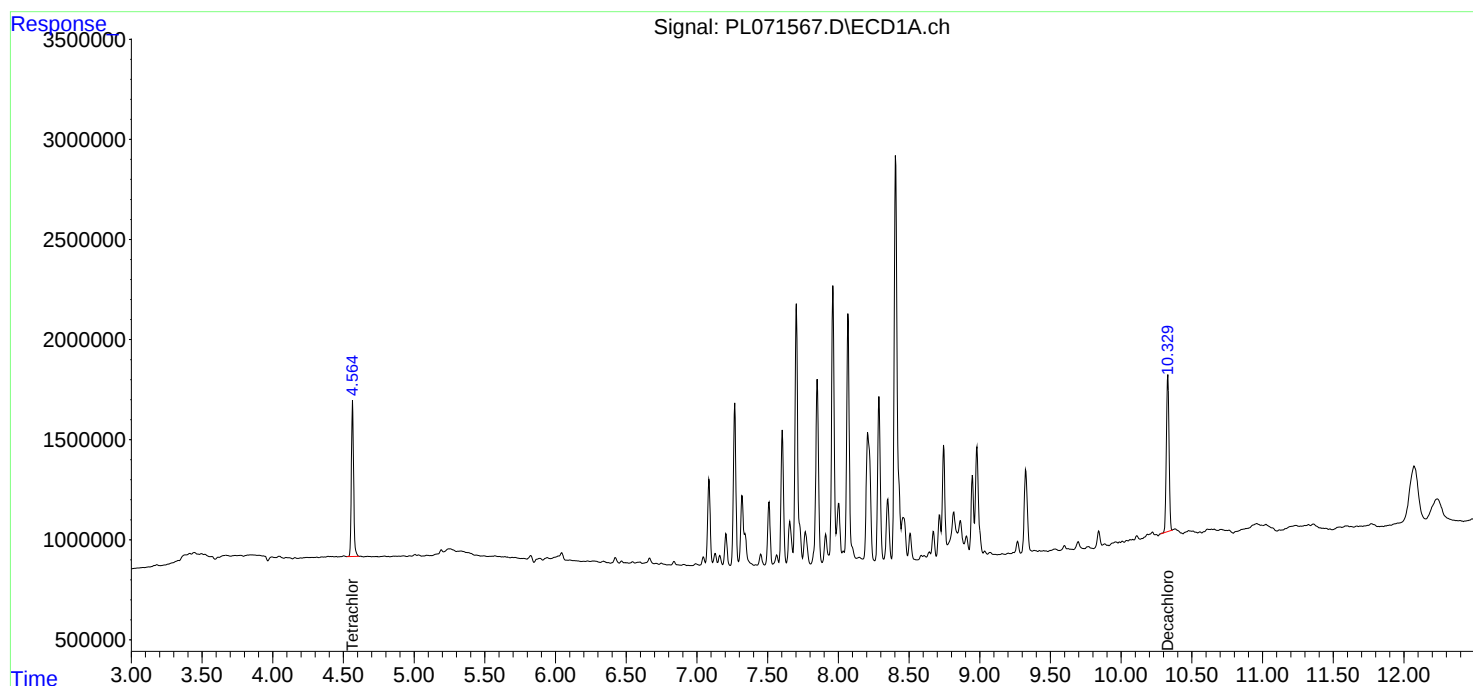

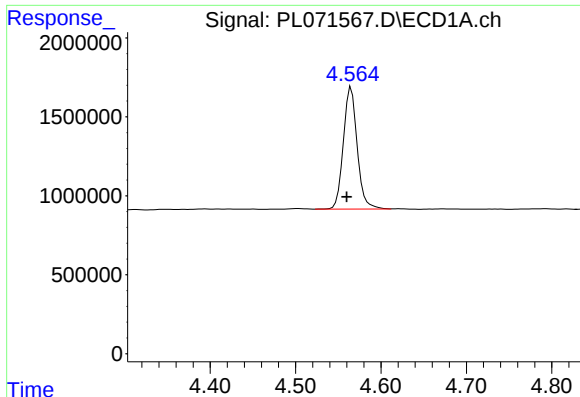


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: 0.005 min
Response: 8666945
Conc: 18.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-122021


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/23/2021
Supervised By :Ankita Jodhani 12/23/2021

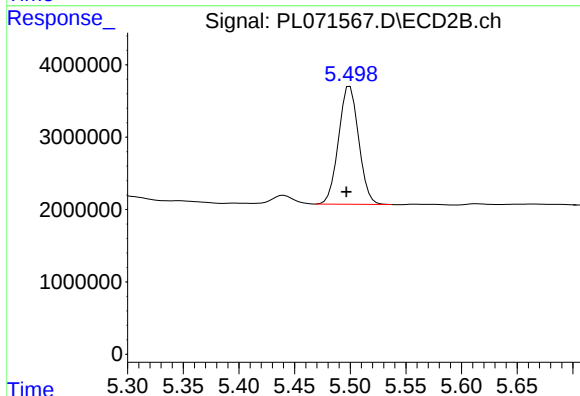


#1 Tetrachloro-m-xylene

R.T.: 5.498 min
Delta R.T.: 0.002 min
Response: 20531961
Conc: 17.23 ng/ml m

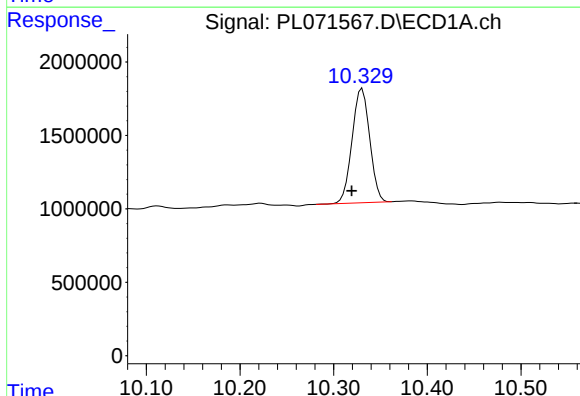

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.011 min
Response: 10207340
Conc: 15.36 ng/ml

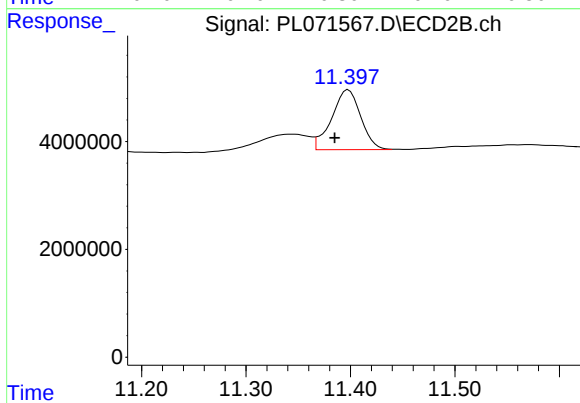

#28 Decachlorobiphenyl

R.T.: 11.397 min
Delta R.T.: 0.012 min
Response: 21262517
Conc: 19.57 ng/ml m