

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122222\
 Data File : PL079866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2022 18:18
 Operator : AR\AJ
 Sample : PB149800TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 21:03:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 21 10:00:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.562	41506849	52046247	18.887	19.607
28)	SA Decachlor...	8.763	7.628	40493580	49371498	21.832	20.567
Target Compounds							
2)	A alpha-BHC	0.000	3.037	0	516635	N.D.	0.120 #
3)	MA gamma-BHC...	0.000	3.390f	0	561976	N.D.	0.143 #
4)	MA Heptachlor	0.000	3.668f	0	421088	N.D.	0.104 #
5)	MB Aldrin	0.000	3.961	0	22304	N.D.	0.006 #
6)	B beta-BHC	0.000	3.668	0	421088	N.D.	0.278 #
8)	B Heptachlo...	5.462	4.480f	1110531	220936	0.419	0.063 #
9)	A Endosulfan I	5.854f	0.000	170735	0	0.066	N.D. #
11)	B alpha-Chl...	0.000	4.746f	0	75977	N.D.	0.022 #
15)	B Endosulfa...	6.543f	0.000	257897	0	0.106	N.D. #
26)	Chlordane-4	0.000	4.746f	0	75977	N.D.	0.209 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122222\
Data File : PL079866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2022 18:18
Operator : AR\AJ
Sample : PB149800TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 21:03:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122022.M
Quant Title : GC Extractables
QLast Update : Wed Dec 21 10:00:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

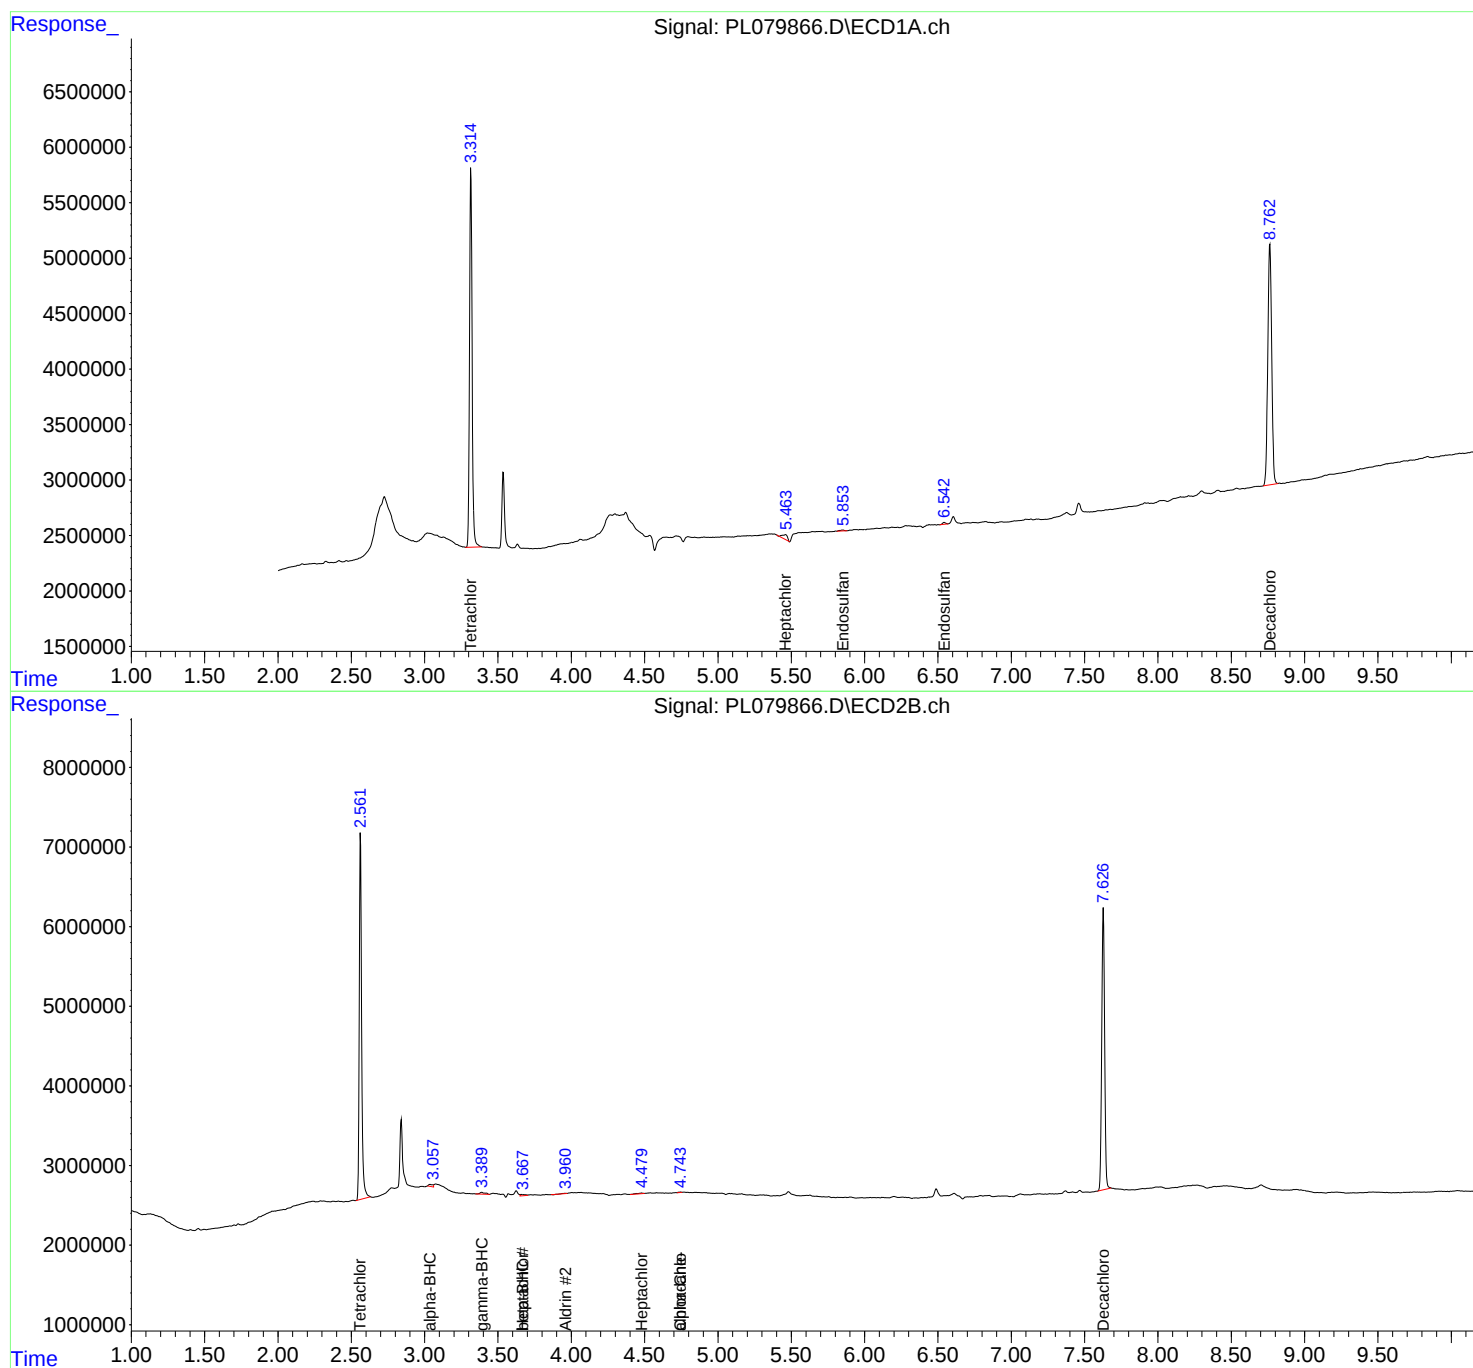


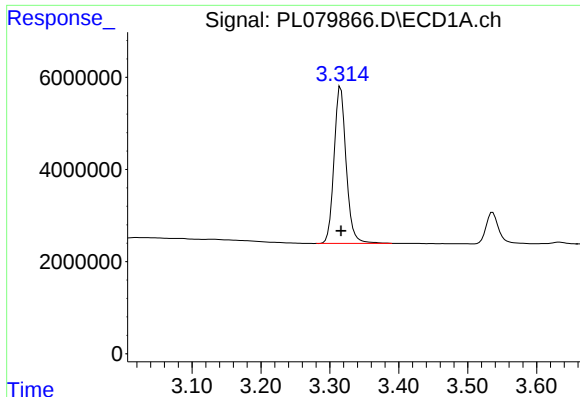

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: 0.000 min
Response: 41506849
Conc: 18.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

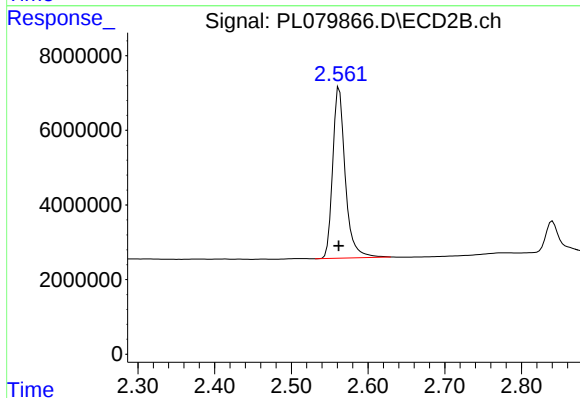


#1 Tetrachloro-m-xylene

R.T.: 2.562 min
Delta R.T.: 0.000 min
Response: 52046247
Conc: 19.61 ng/ml

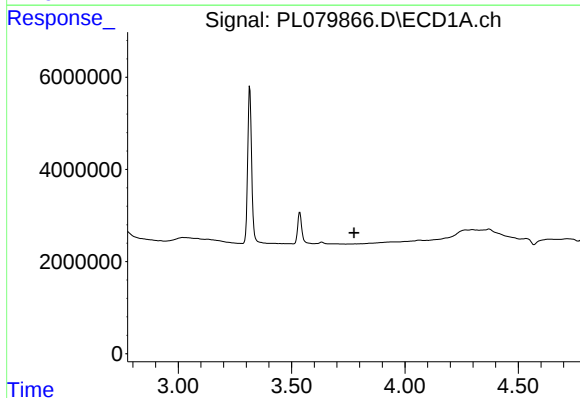


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.776 min
Response: 0
Conc: N.D.

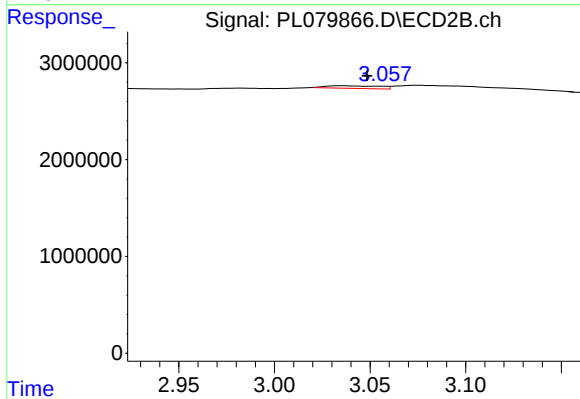

#2 alpha-BHC


R.T.: 3.037 min
Delta R.T.: -0.012 min
Response: 516635
Conc: 0.12 ng/ml

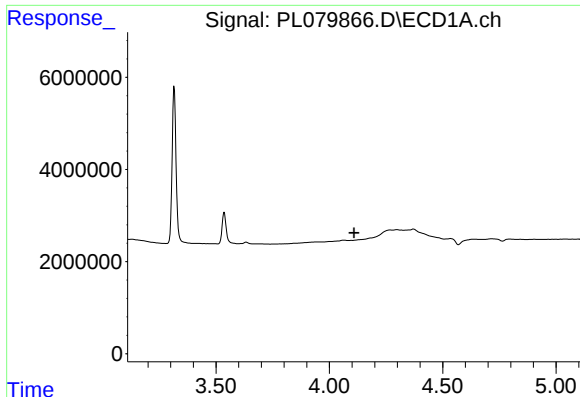

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

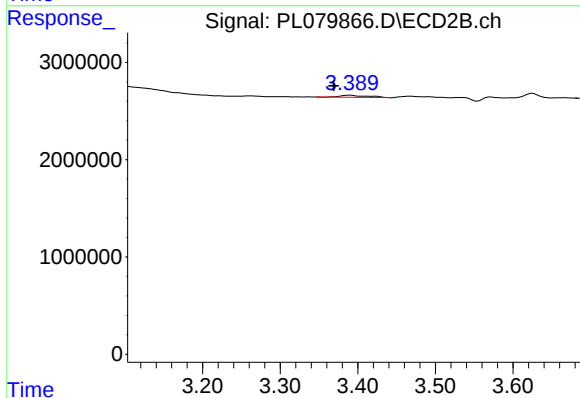


#3 gamma-BHC (Lindane)

R.T.: 3.390 min
Delta R.T.: 0.021 min
Response: 561976
Conc: 0.14 ng/ml

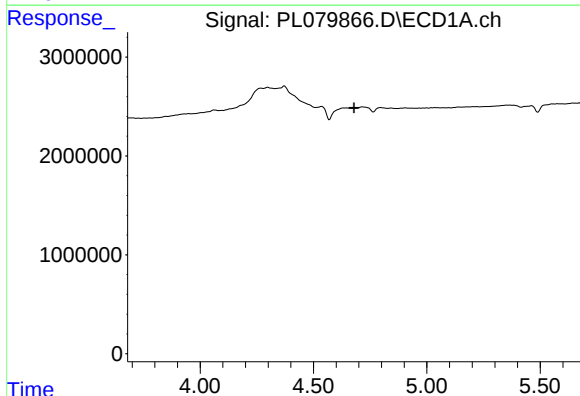


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.679 min
Response: 0
Conc: N.D.

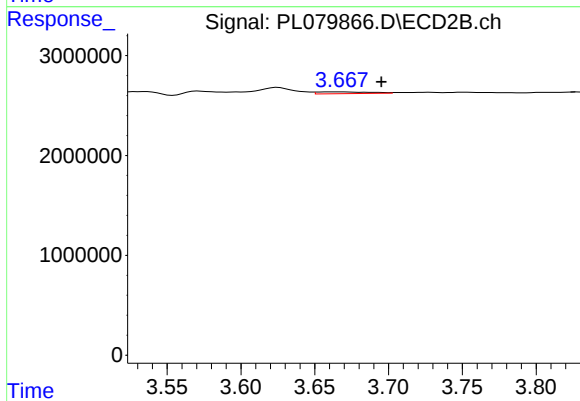

#4 Heptachlor


R.T.: 3.668 min
Delta R.T.: -0.027 min
Response: 421088
Conc: 0.10 ng/ml

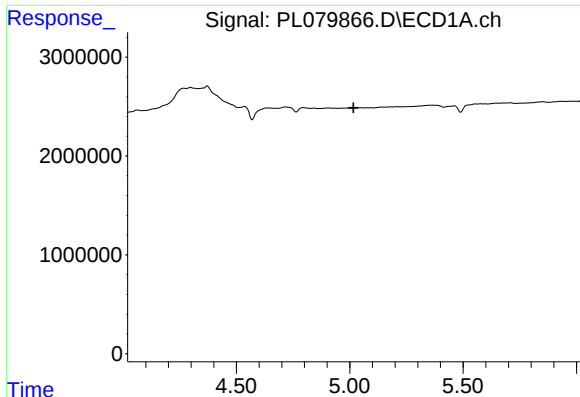

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

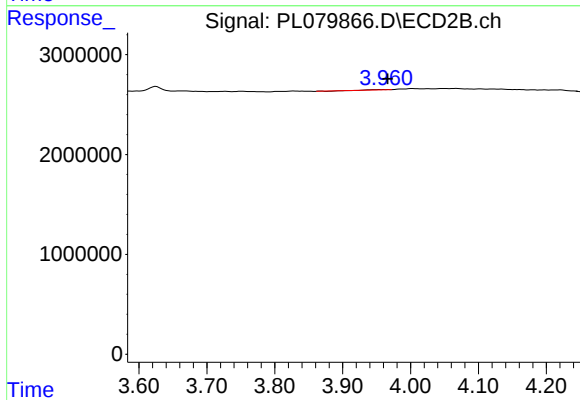


#5 Aldrin

R.T.: 3.961 min
Delta R.T.: -0.005 min
Response: 22304
Conc: 0.01 ng/ml

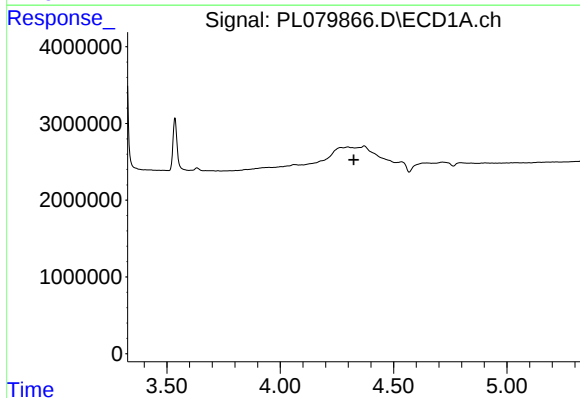


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.325 min
Response: 0
Conc: N.D.

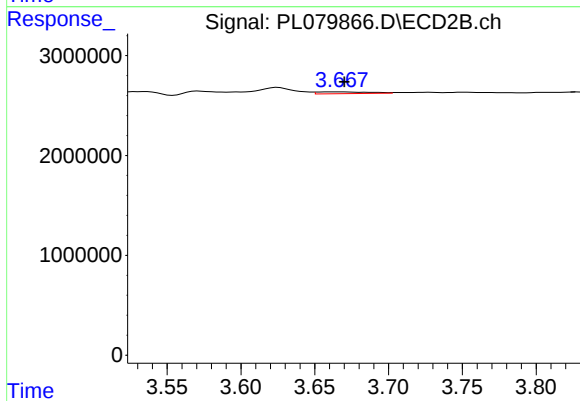

#6 beta-BHC


R.T.: 3.668 min
Delta R.T.: -0.002 min
Response: 421088
Conc: 0.28 ng/ml

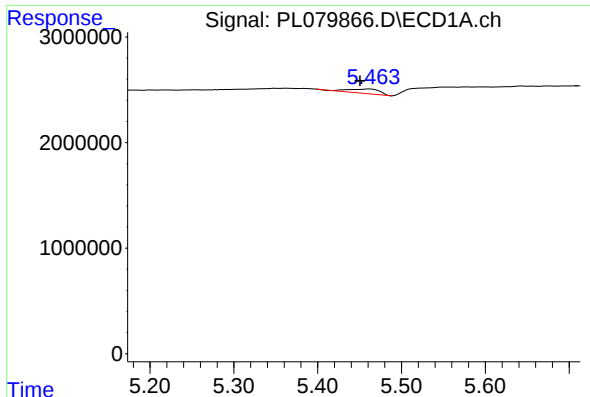

#8 Heptachlor epoxide


R.T.: 5.462 min
Delta R.T.: 0.011 min
Response: 1110531
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

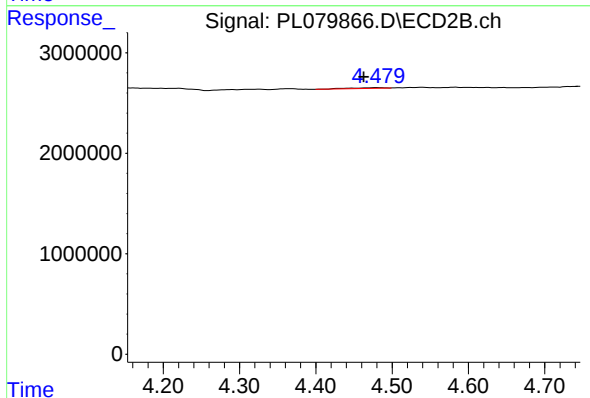


#8 Heptachlor epoxide

R.T.: 4.480 min
Delta R.T.: 0.017 min
Response: 220936
Conc: 0.06 ng/ml

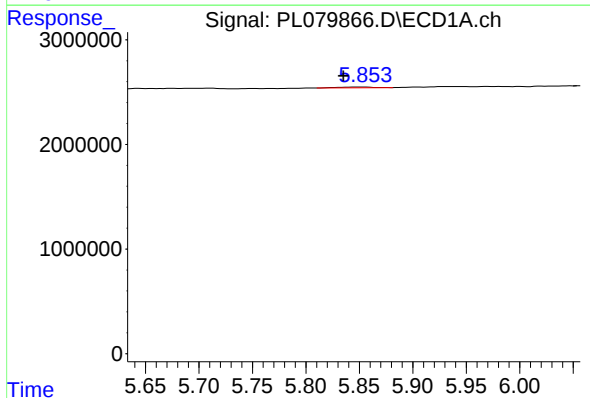


#9 Endosulfan I

R.T.: 5.854 min
Delta R.T.: 0.019 min
Response: 170735
Conc: 0.07 ng/ml

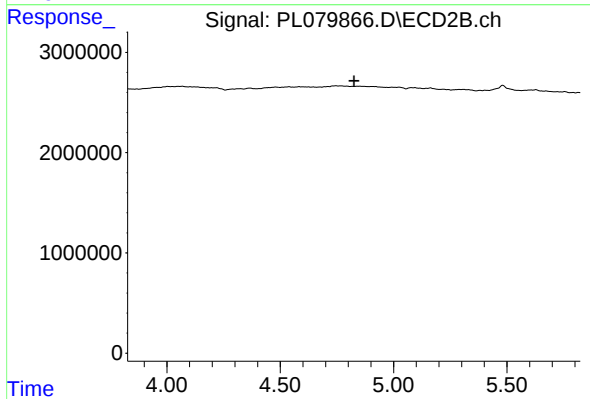

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 4.826 min
Response: 0
Conc: N.D.

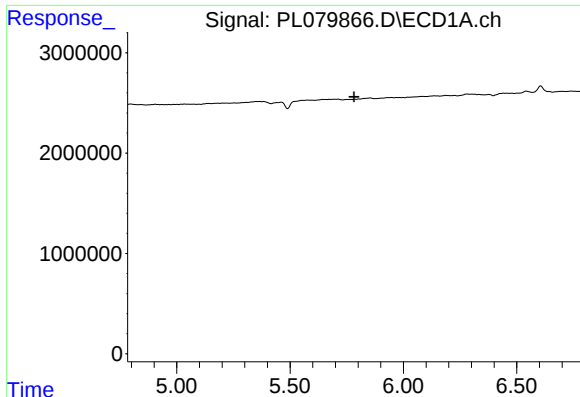

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.783 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

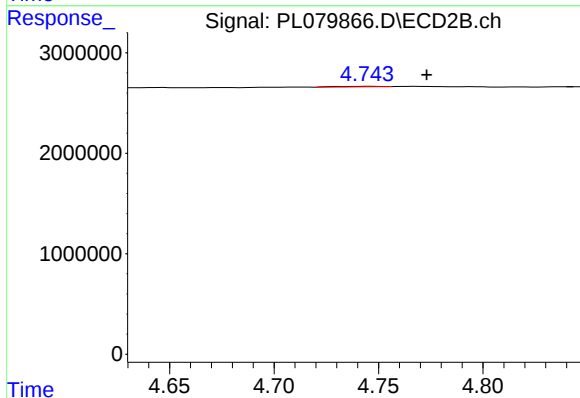


#11 alpha-Chlordane

R.T.: 4.746 min
Delta R.T.: -0.027 min
Response: 75977
Conc: 0.02 ng/ml

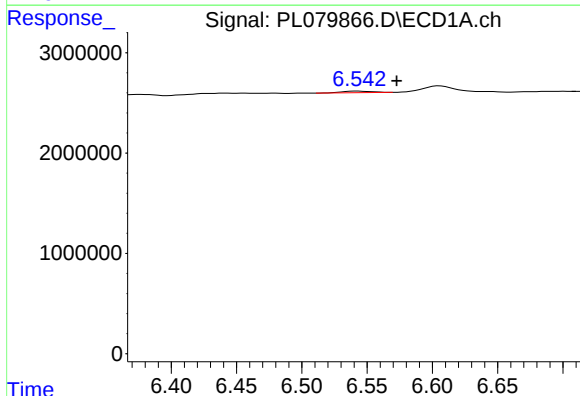


#15 Endosulfan II

R.T.: 6.543 min
Delta R.T.: -0.030 min
Response: 257897
Conc: 0.11 ng/ml

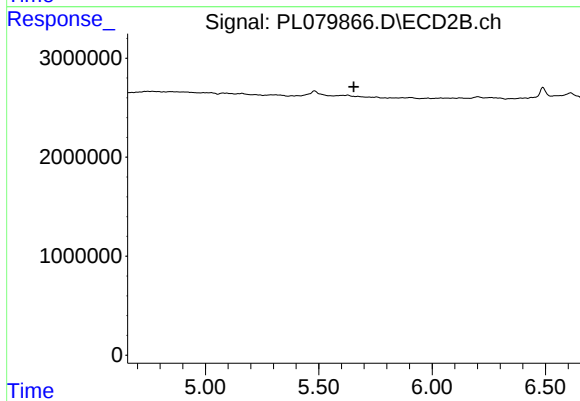

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.655 min
Response: 0
Conc: N.D.

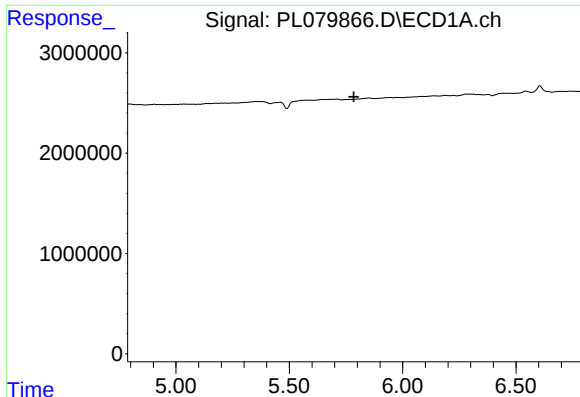

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.784 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

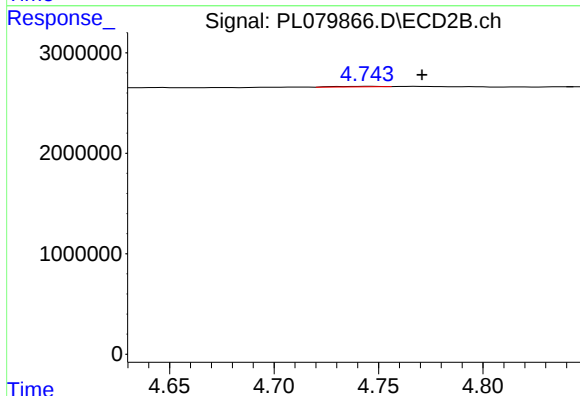


#26 Chlordane-4

R.T.: 4.746 min
Delta R.T.: -0.025 min
Response: 75977
Conc: 0.21 ng/ml

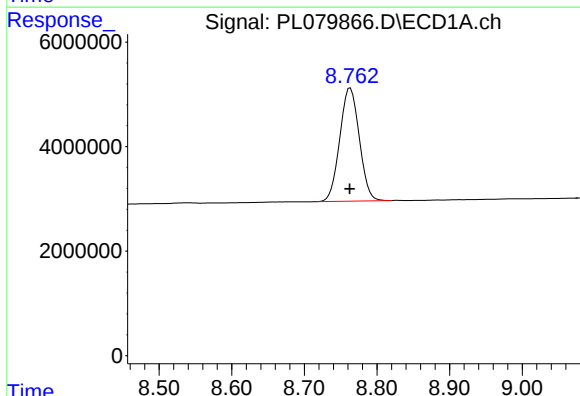

#28 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: 0.000 min
Response: 40493580
Conc: 21.83 ng/ml

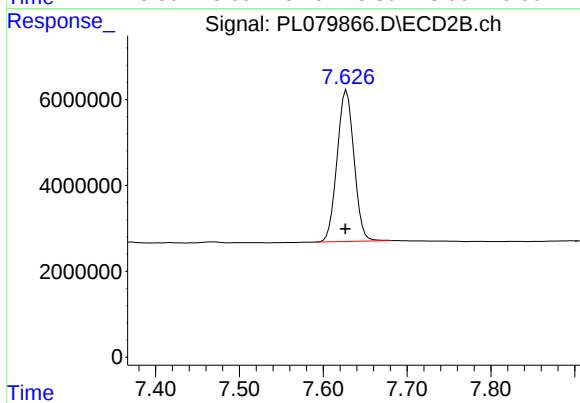

#28 Decachlorobiphenyl

R.T.: 7.628 min
Delta R.T.: 0.001 min
Response: 49371498
Conc: 20.57 ng/ml