

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122223\
 Data File : PL087403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2023 01:42
 Operator : AR\AJ
 Sample : PB158025BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB158025BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 05:13:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.678	51795376	21107189	13.763	12.539
28)	SA Decachlor...	8.978	7.865	48615999	20662921	14.257	12.234
Target Compounds							
3)	MA gamma-BHC...	0.000	3.510	0	27982	N.D.	0.012 #
4)	MA Heptachlor	0.000	3.887f	0	27722	N.D.	0.012 #
5)	MB Aldrin	5.158	4.173f	113687	46398	0.022	0.019
7)	B delta-BHC	4.660	4.050	1578627	47232	0.302	0.019 #
8)	B Heptachlo...	0.000	4.642	0	8825	N.D.	0.004 #
9)	A Endosulfan I	0.000	5.024	0	4518268	N.D.	2.091 #
14)	MA Endrin	0.000	5.579	0	40031	N.D.	0.020 #
18)	B Endrin al...	0.000	6.034	0	340526	N.D.	0.232 #
23)	Chlordane-1	0.000	3.704f	0	16131	N.D.	0.260 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122223\
Data File : PL087403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2023 01:42
Operator : AR\AJ
Sample : PB158025BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB158025BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 05:13:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

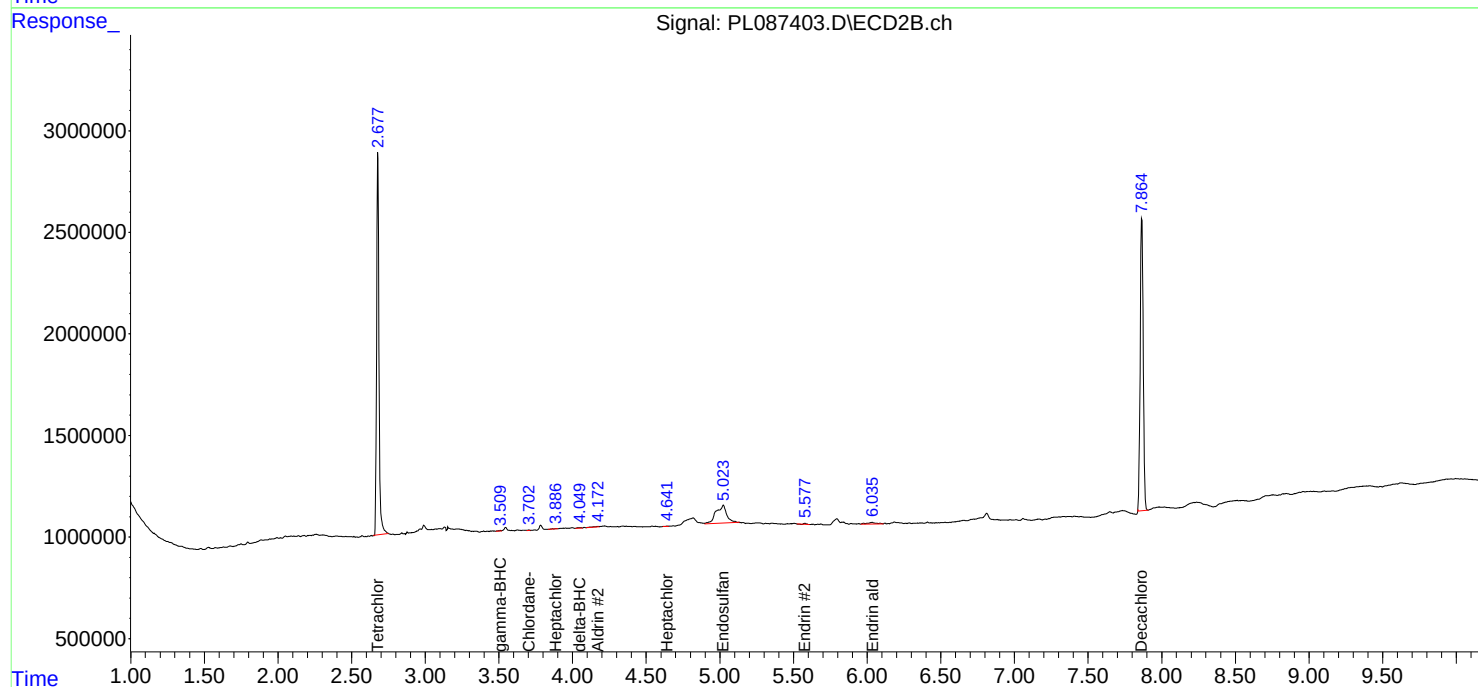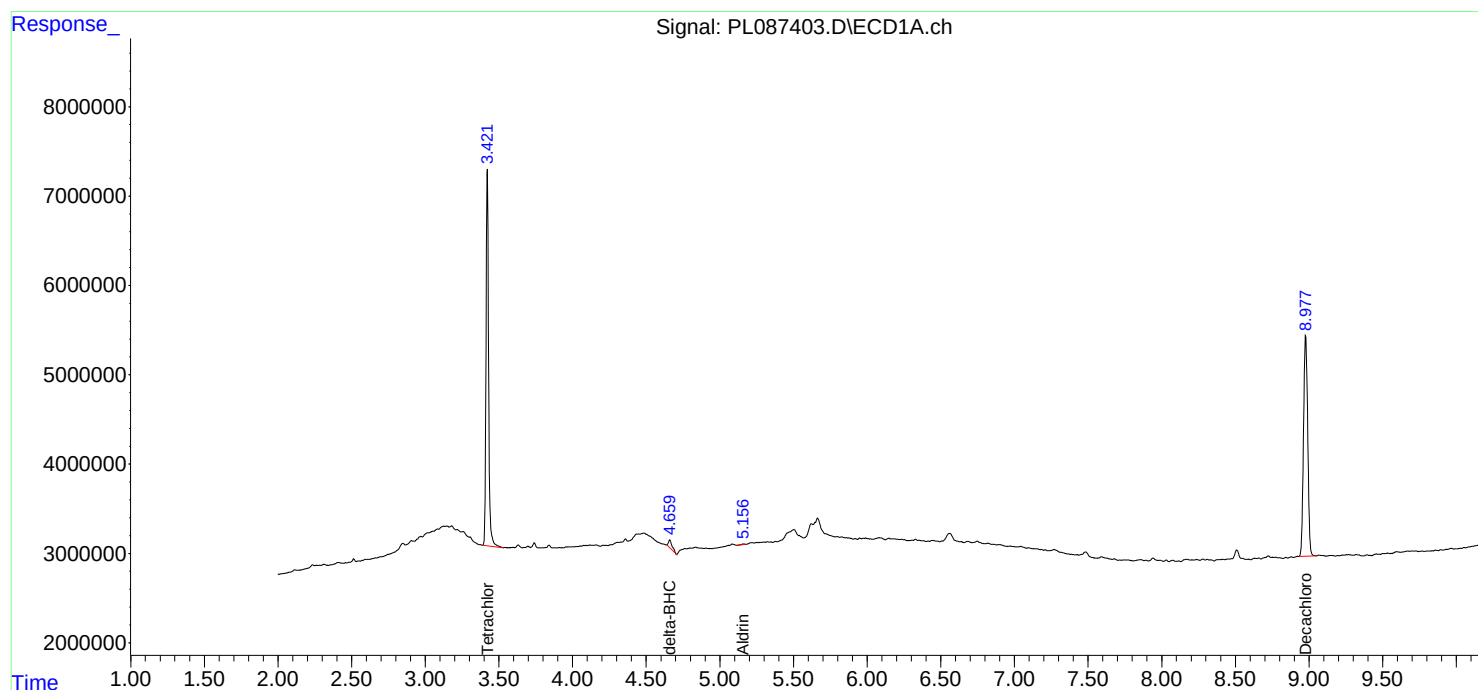


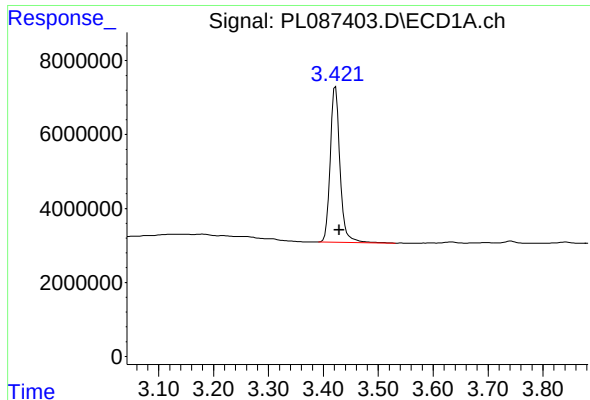

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 51795376
Conc: 13.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB158025BL

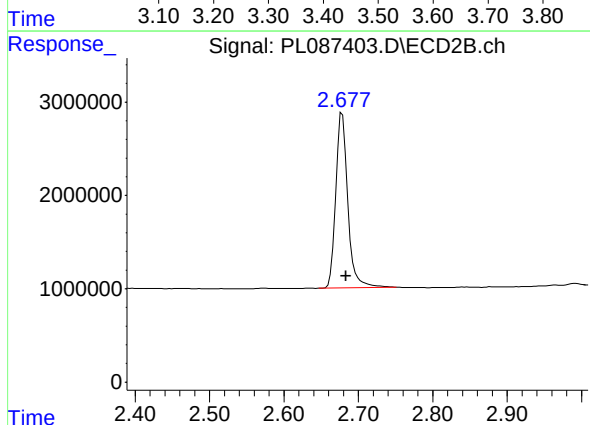


#1 Tetrachloro-m-xylene

R.T.: 2.678 min
Delta R.T.: -0.005 min
Response: 21107189
Conc: 12.54 ng/ml

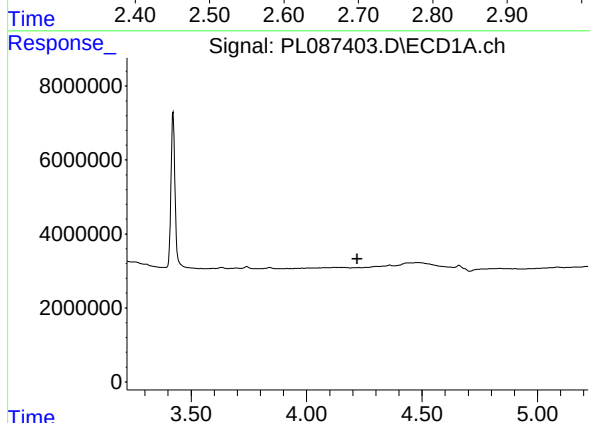


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.220 min
Response: 0
Conc: N.D.

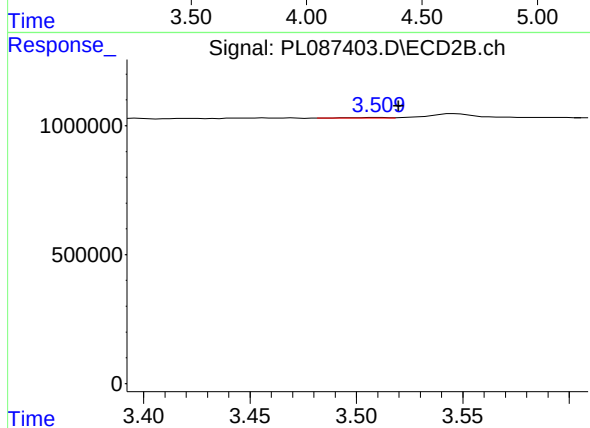

#3 gamma-BHC (Lindane)


R.T.: 3.510 min
Delta R.T.: -0.010 min
Response: 27982
Conc: 0.01 ng/ml

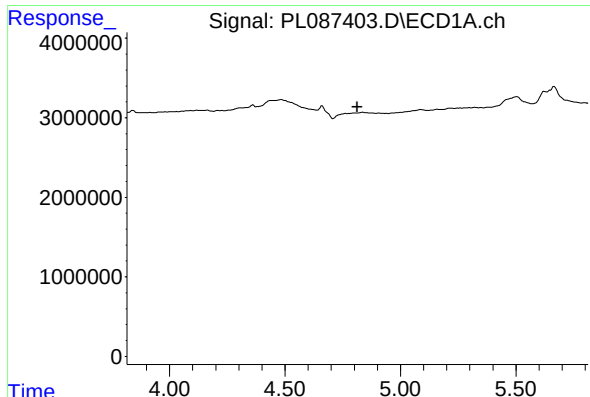

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.813 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB158025BL

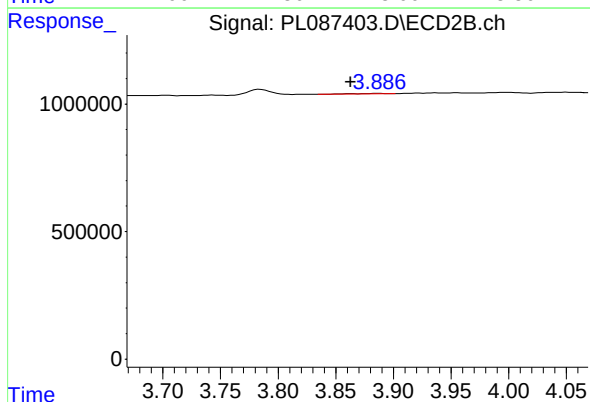


#4 Heptachlor

R.T.: 3.887 min
Delta R.T.: 0.024 min
Response: 27722
Conc: 0.01 ng/ml

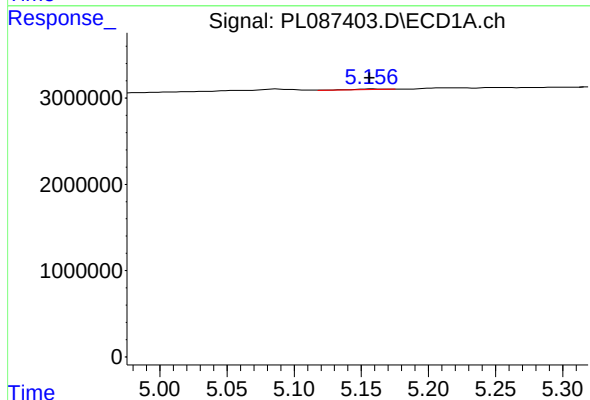


#5 Aldrin

R.T.: 5.158 min
Delta R.T.: 0.002 min
Response: 113687
Conc: 0.02 ng/ml

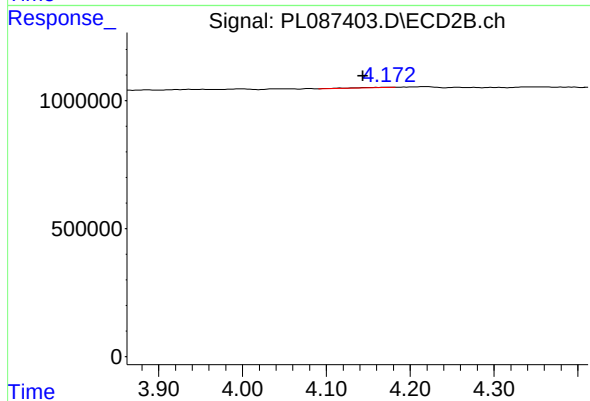

#5 Aldrin


R.T.: 4.173 min
Delta R.T.: 0.029 min
Response: 46398
Conc: 0.02 ng/ml

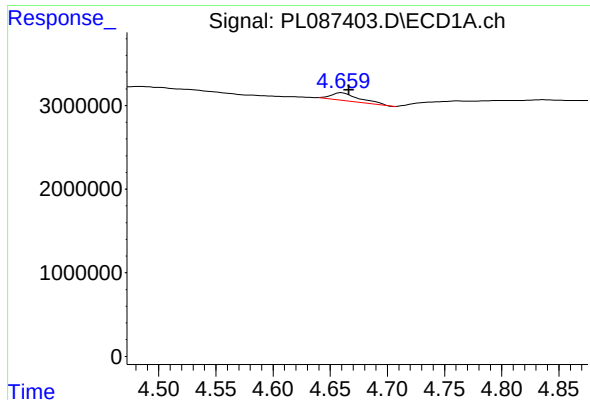

#7 delta-BHC


R.T.: 4.660 min
Delta R.T.: -0.006 min
Response: 1578627
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB158025BL

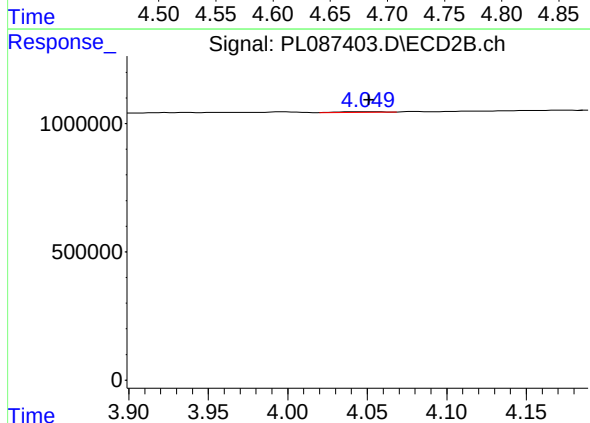


#7 delta-BHC

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 47232
Conc: 0.02 ng/ml

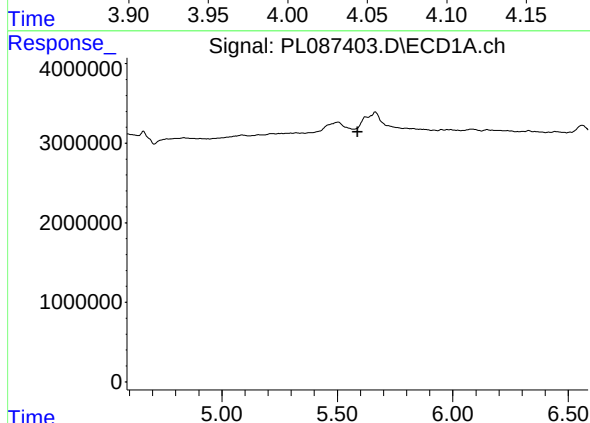


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.587 min
Response: 0
Conc: N.D.

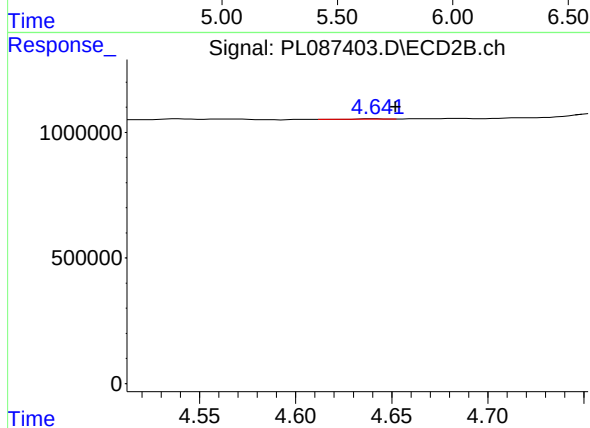

#8 Heptachlor epoxide


R.T.: 4.642 min
Delta R.T.: -0.010 min
Response: 8825
Conc: 0.00 ng/ml

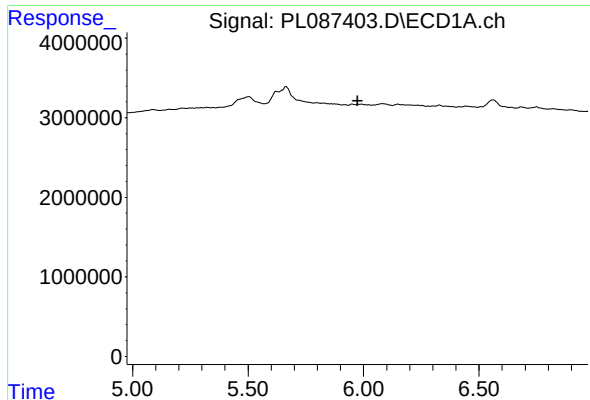

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.973 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB158025BL

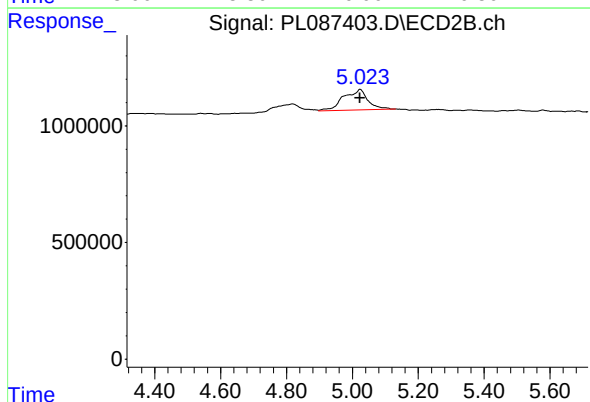


#9 Endosulfan I

R.T.: 5.024 min
Delta R.T.: 0.000 min
Response: 4518268
Conc: 2.09 ng/ml

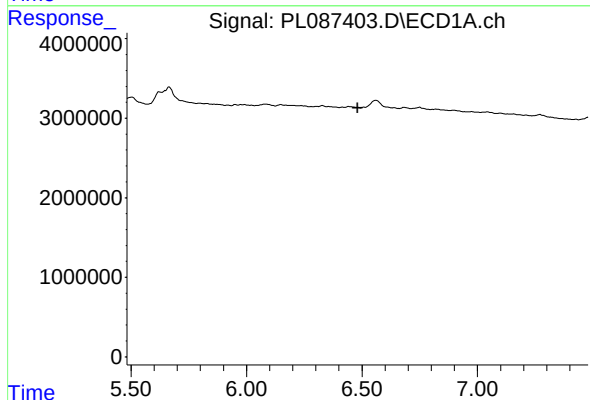


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.480 min
Response: 0
Conc: N.D.

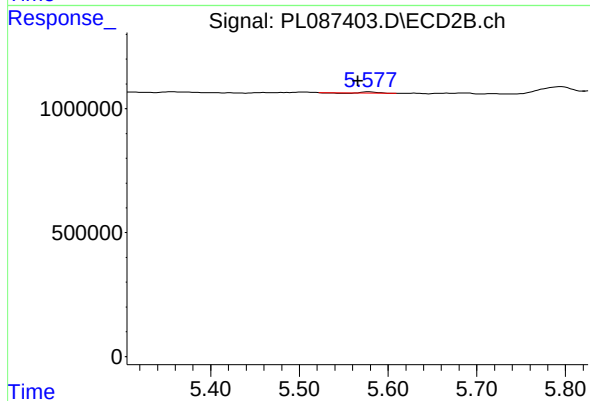

#14 Endrin


R.T.: 5.579 min
Delta R.T.: 0.013 min
Response: 40031
Conc: 0.02 ng/ml

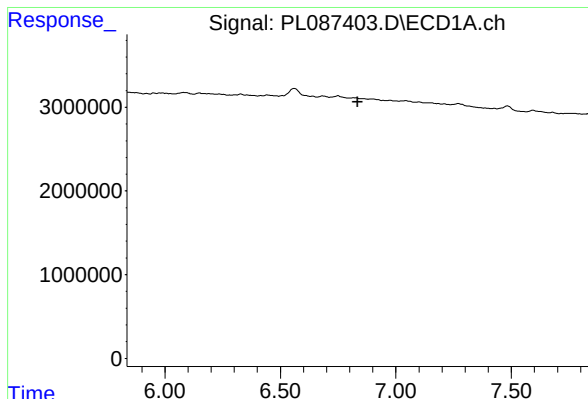

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.833 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB158025BL

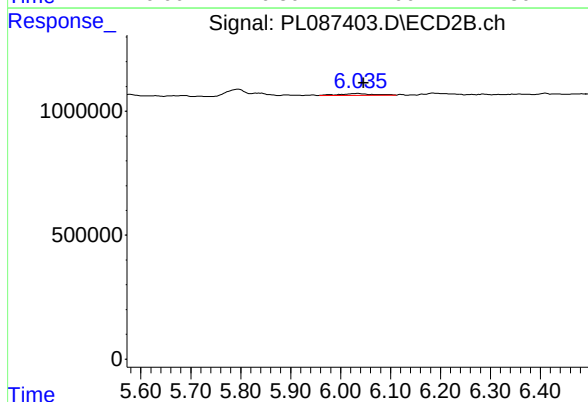


#18 Endrin aldehyde

R.T.: 6.034 min
Delta R.T.: -0.011 min
Response: 340526
Conc: 0.23 ng/ml

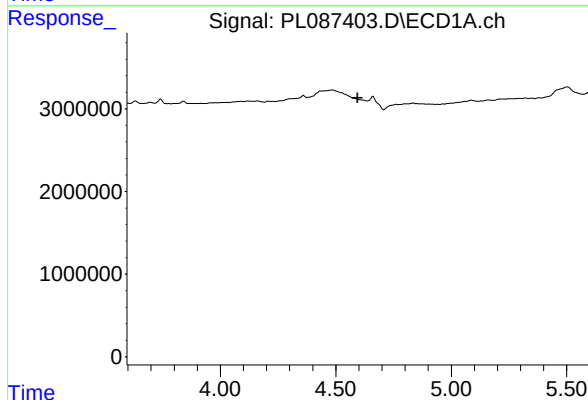


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.594 min
Response: 0
Conc: N.D.

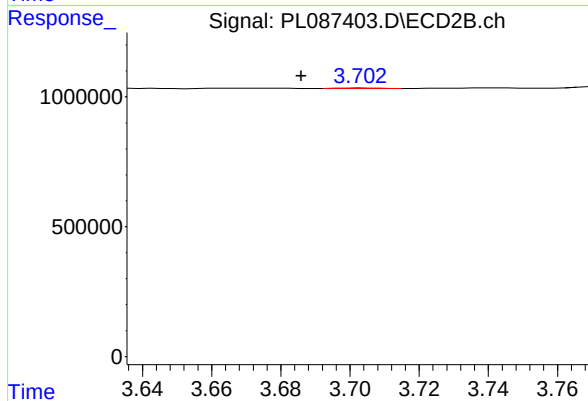

#23 Chlordane-1


R.T.: 3.704 min
Delta R.T.: 0.018 min
Response: 16131
Conc: 0.26 ng/ml

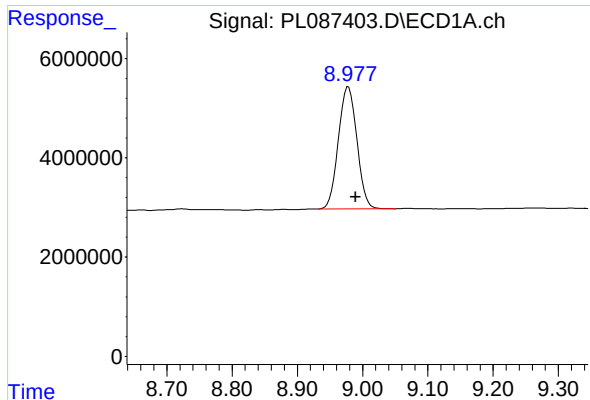

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.011 min
Response: 48615999
Conc: 14.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB158025BL

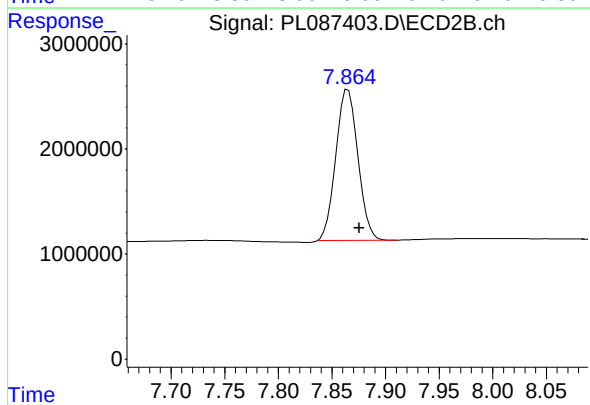

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.011 min
Response: 20662921
Conc: 12.23 ng/ml