

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122223\
 Data File : PL087388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 21:31
 Operator : AR\AJ
 Sample : 05909-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GHL-SD-46

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 05:09:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	2.678	57371713	23467458	15.245	13.941
28) SA Decachlor...	8.979	7.865	48281839	21885710	14.159	12.958m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122223\
Data File : PL087388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 21:31
Operator : AR\AJ
Sample : 05909-08
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GHL-SD-46


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/26/2023
Supervised By : Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 05:09:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

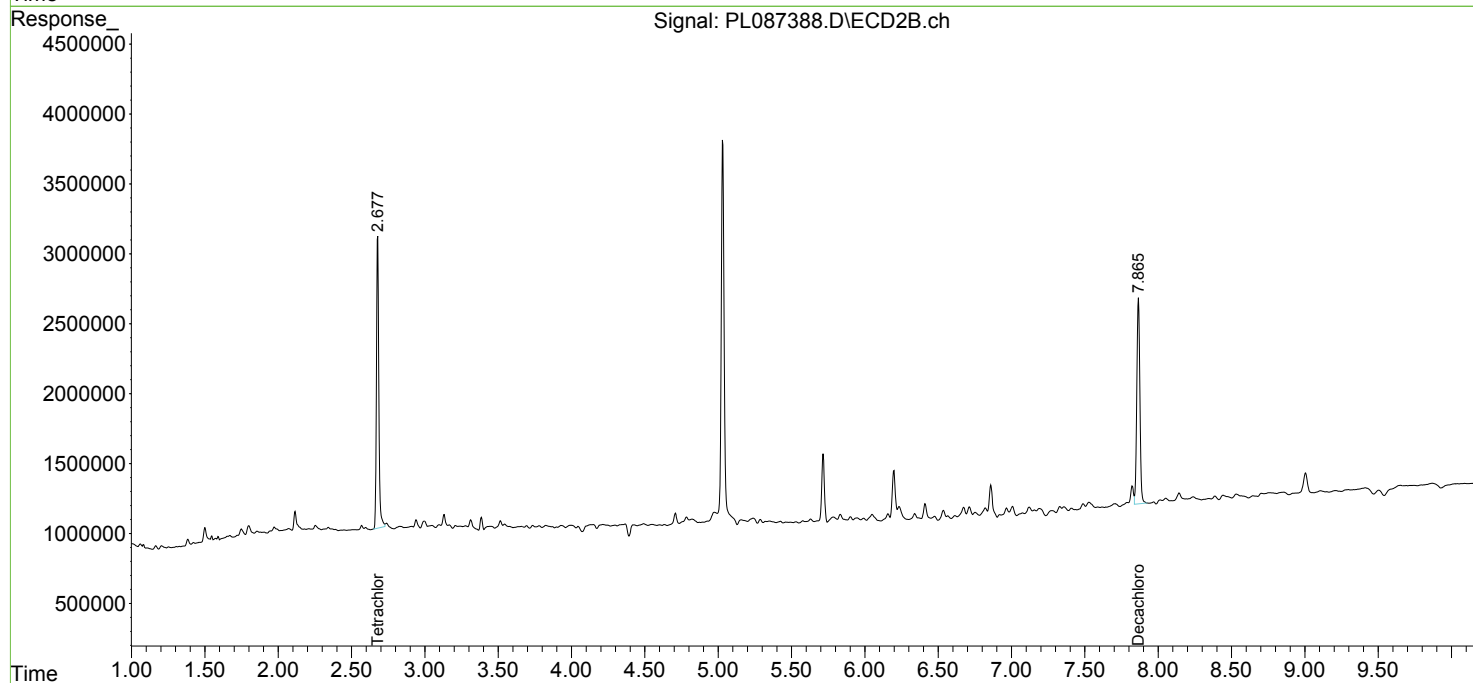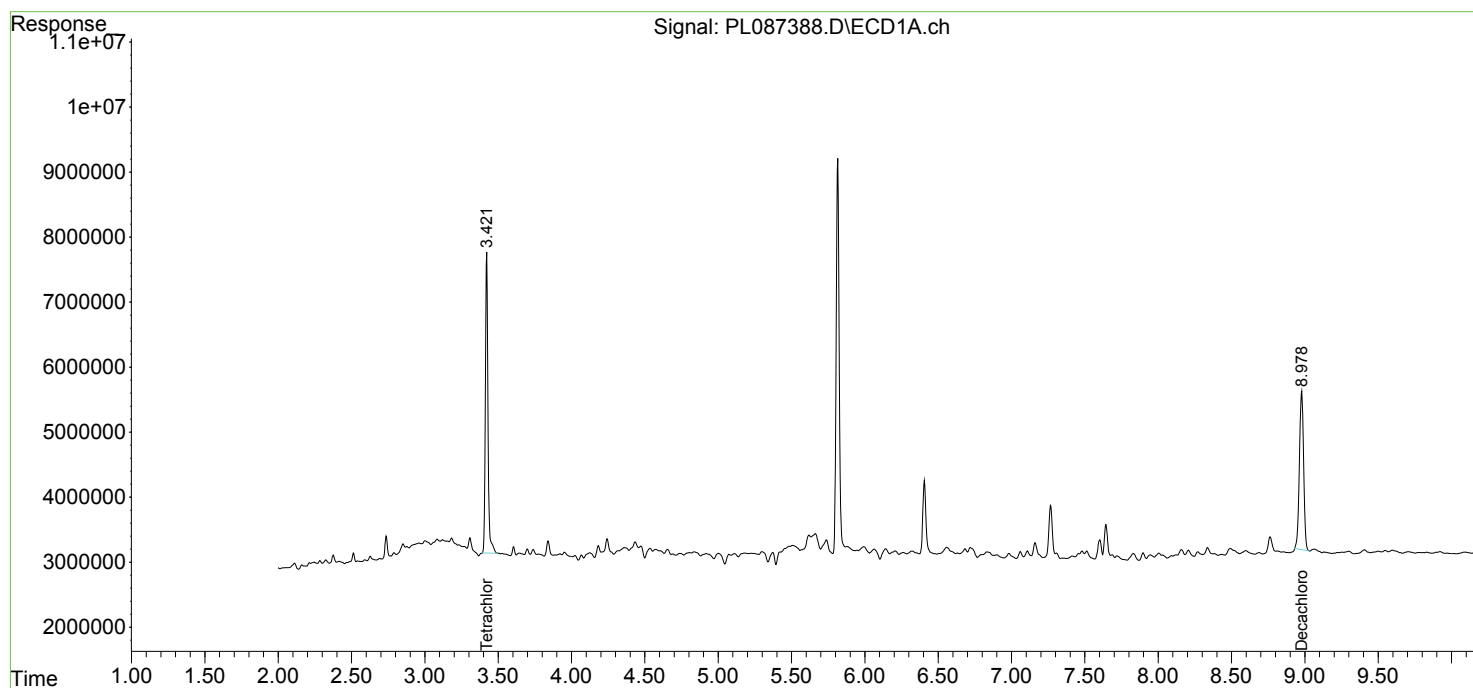

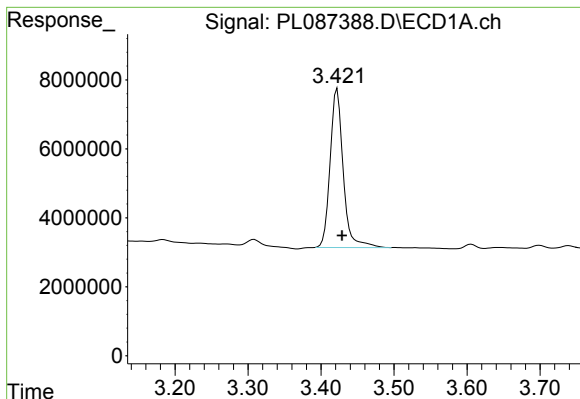


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.007 min
Response: 57371713
Conc: 15.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
GHL-SD-46


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

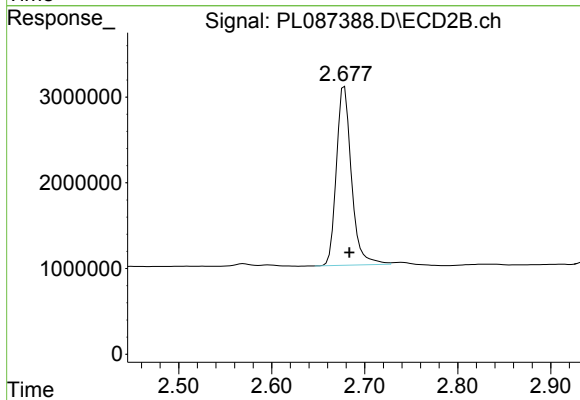


#1 Tetrachloro-m-xylene

R.T.: 2.678 min
Delta R.T.: -0.005 min
Response: 23467458
Conc: 13.94 ng/ml

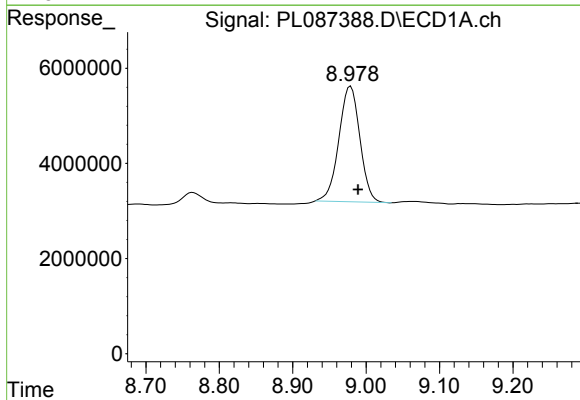

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.010 min
Response: 48281839
Conc: 14.16 ng/ml

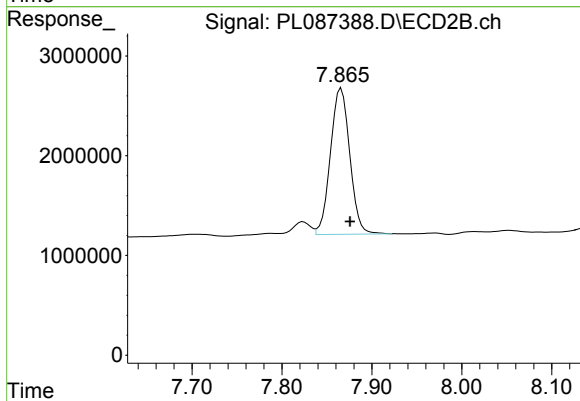

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.011 min
Response: 21885710
Conc: 12.96 ng/ml m