

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122223\
 Data File : PL087398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 23:51
 Operator : AR\AJ
 Sample : 05909-16
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 GHL-SD-52-D

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 05:11:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 04:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.679	32632926	13462427	8.671	7.998
28)	SA Decachlor...	8.976	7.865	13207491	5594106	3.873	3.312
Target Compounds							
11)	B alpha-Chl...	5.919	4.958	4992075	2245302	1.039	0.973m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122223\
Data File : PL087398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 23:51
Operator : AR\AJ
Sample : 05909-16
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
GHL-SD-52-D


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/26/2023
Supervised By : Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 05:11:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121523.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 04:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

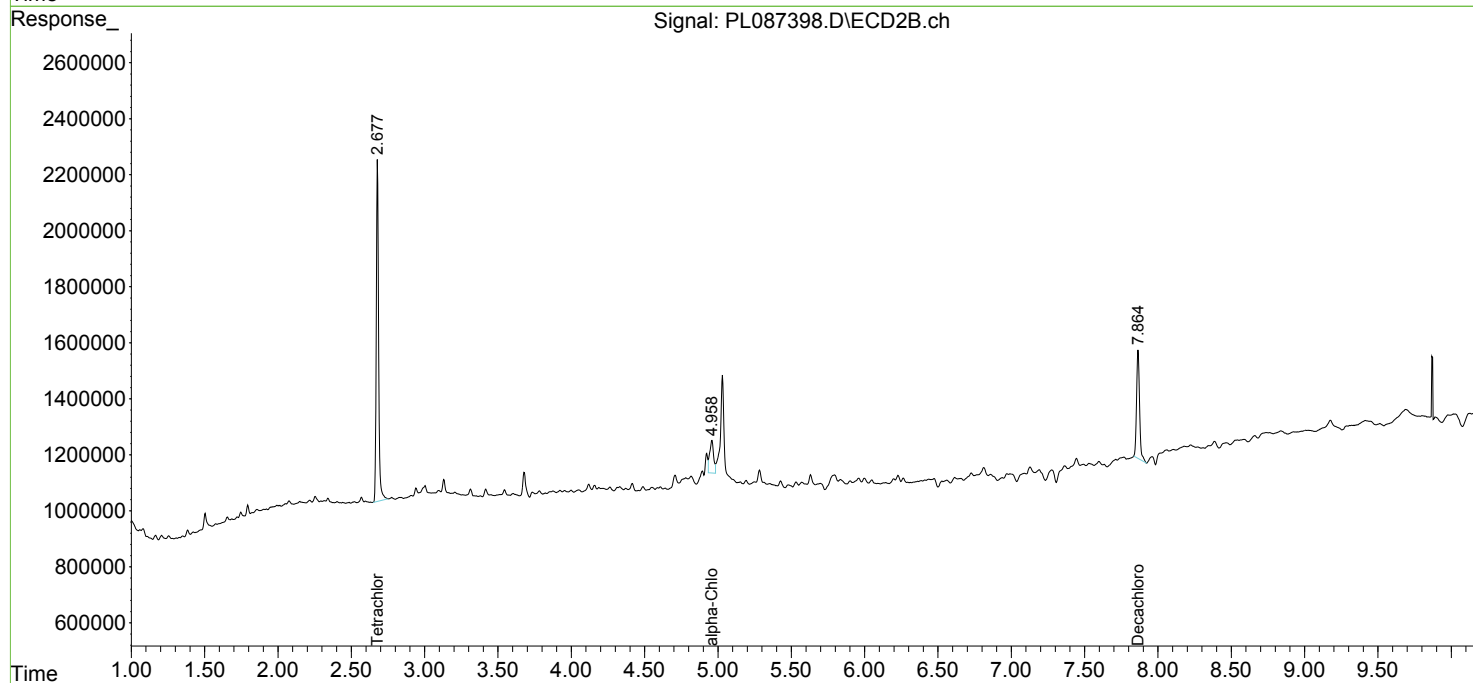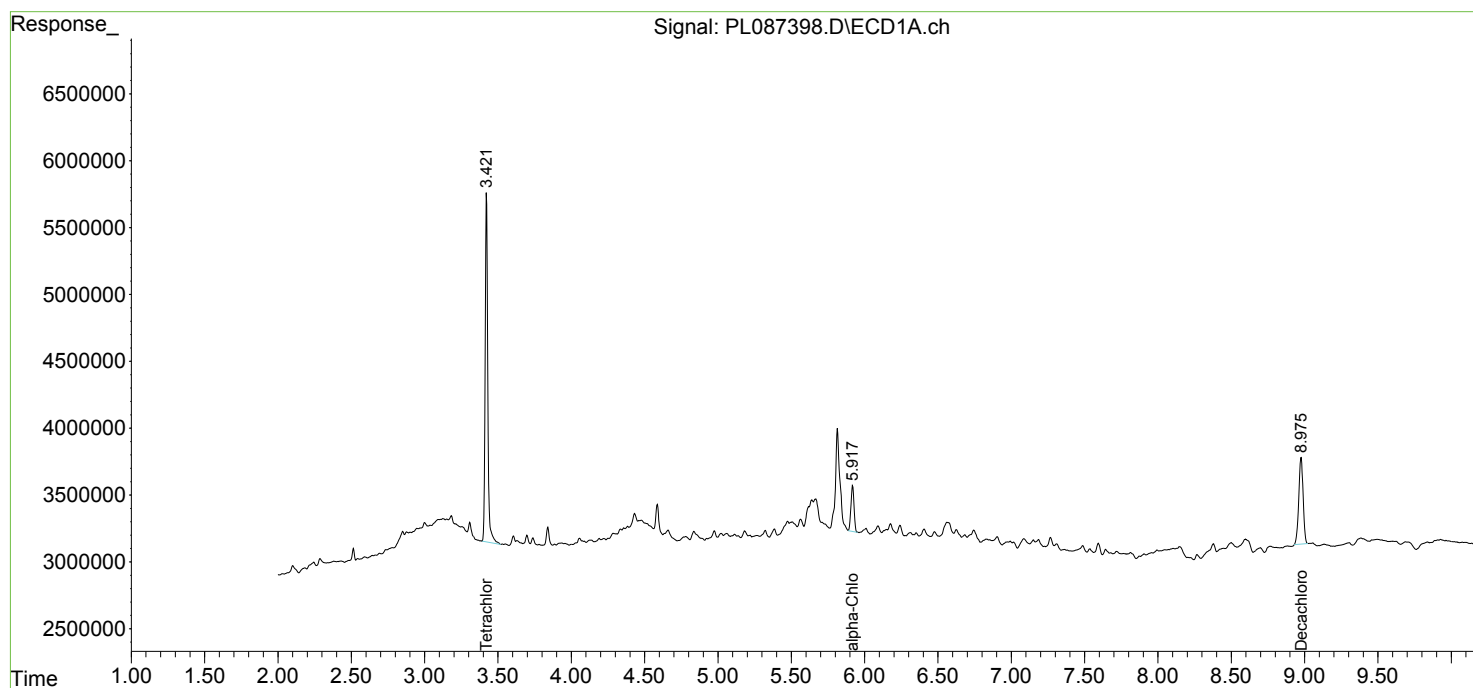

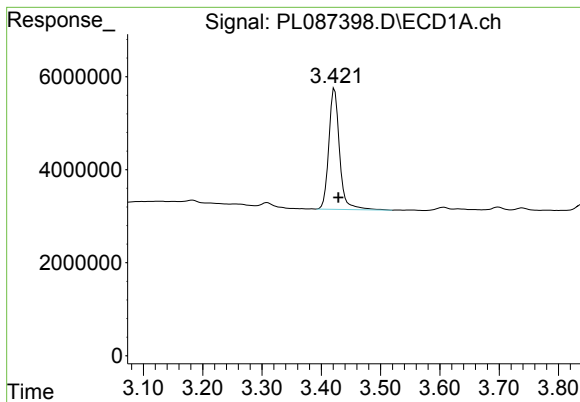


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.006 min
Response: 32632926
Conc: 8.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
GHL-SD-52-D


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

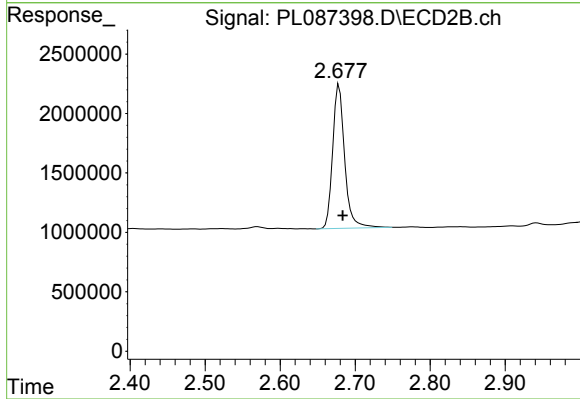


#1 Tetrachloro-m-xylene

R.T.: 2.679 min
Delta R.T.: -0.005 min
Response: 13462427
Conc: 8.00 ng/ml

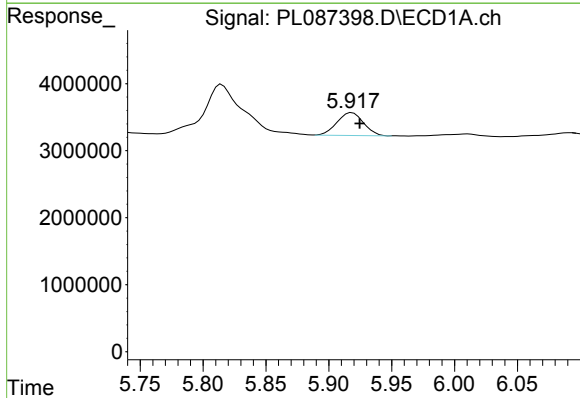


#11 alpha-Chlordane

R.T.: 5.919 min
Delta R.T.: -0.006 min
Response: 4992075
Conc: 1.04 ng/ml

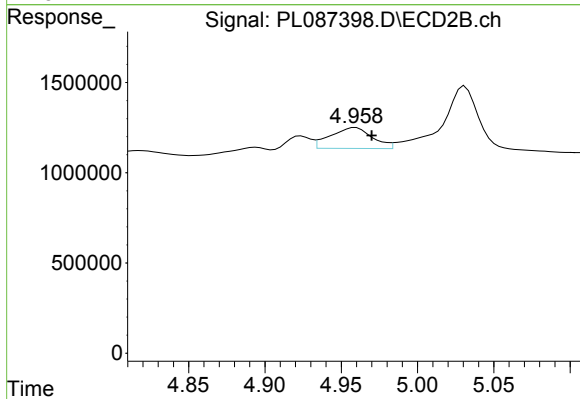

#11 alpha-Chlordane

R.T.: 4.958 min
Delta R.T.: -0.012 min
Response: 2245302
Conc: 0.97 ng/ml m

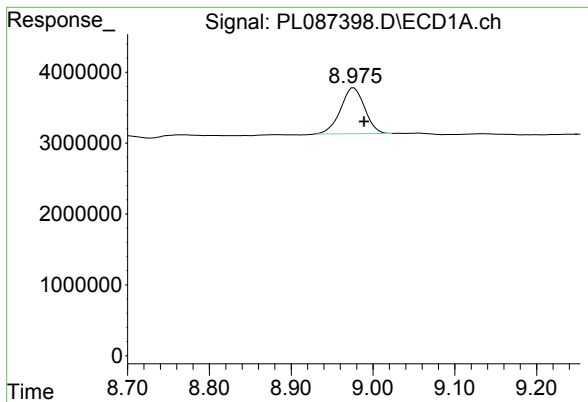


#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.013 min
Response: 13207491
Conc: 3.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
GHL-SD-52-D

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

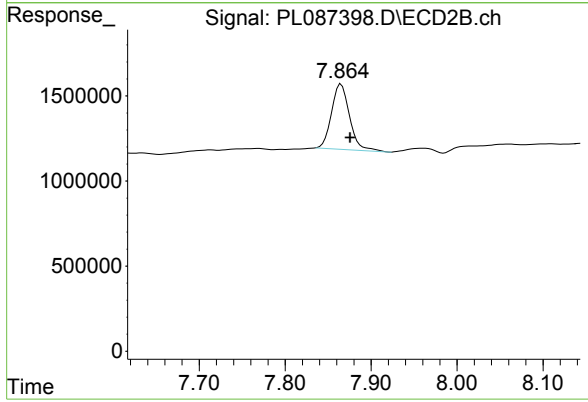

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.011 min
Response: 5594106
Conc: 3.31 ng/ml