

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122319\
 Data File : PL055173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 10:16
 Operator : SG\AJ
 Sample : K6370-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:47:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.049	110.6E6	29758857	10.521	11.263
28)	SA Decachlor...	8.314	9.148	1138.3E6	266.4E6	122.676	120.703
Target Compounds							
16)	A 4,4'-DDD	0.000	6.883	0	61126961	N.D.	32.154 #
17)	MA 4,4'-DDT	6.468	7.208f	134.1E6	33581108	13.316	17.110 #
18)	B Endrin al...	6.575f	7.109f	403.5E6	8209643	41.429	4.254 #
19)	B Endosulfa...	6.761	0.000	68476343	0	6.808	N.D. #
20)	A Methoxychlor	0.000	7.615f	0	13162266	N.D.	12.196 #
21)	B Endrin ke...	7.283f	0.000	320.2E6	0	30.546	N.D. #
22)	Mirex	0.000	8.275f	0	218.2E6	N.D.	131.622 #
27)	Chlordane-5	0.000	7.051	0	1821677	N.D.	26.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122319\
Data File : PL055173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 10:16
Operator : SG\AJ
Sample : K6370-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:47:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

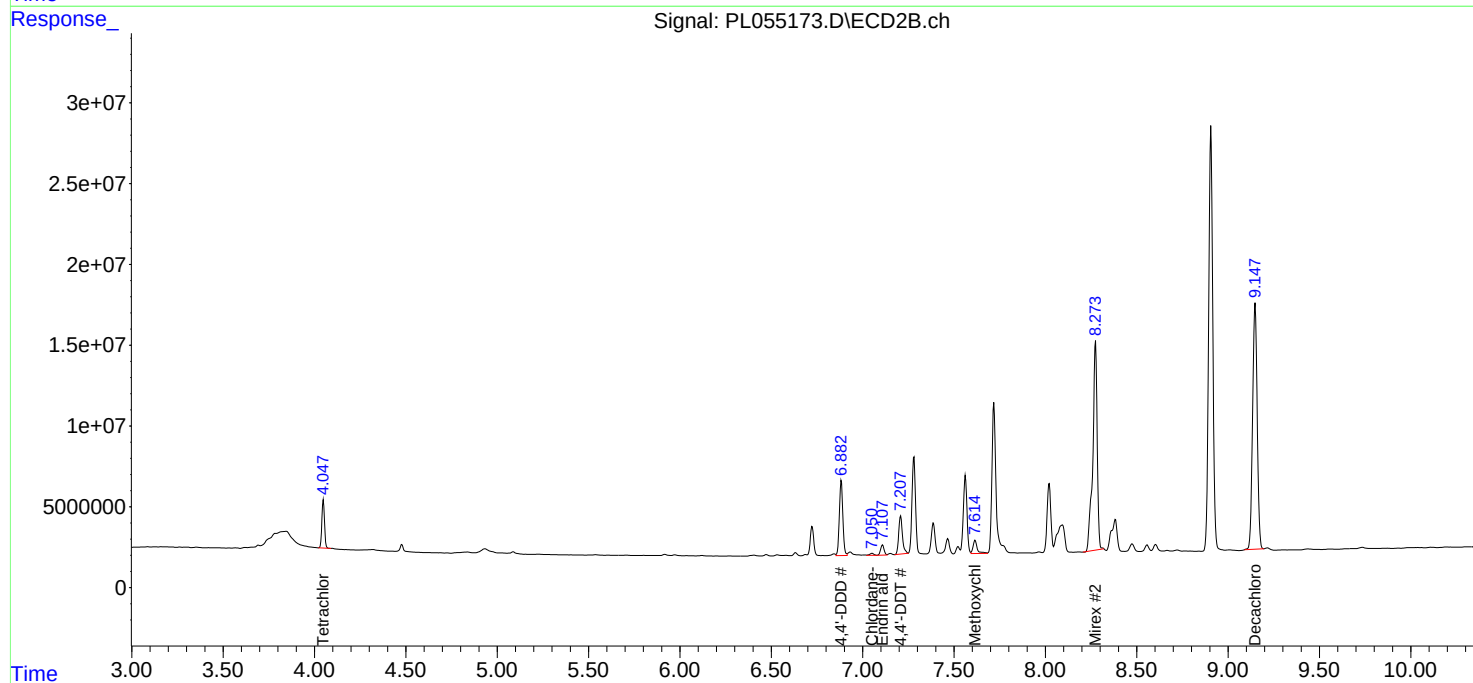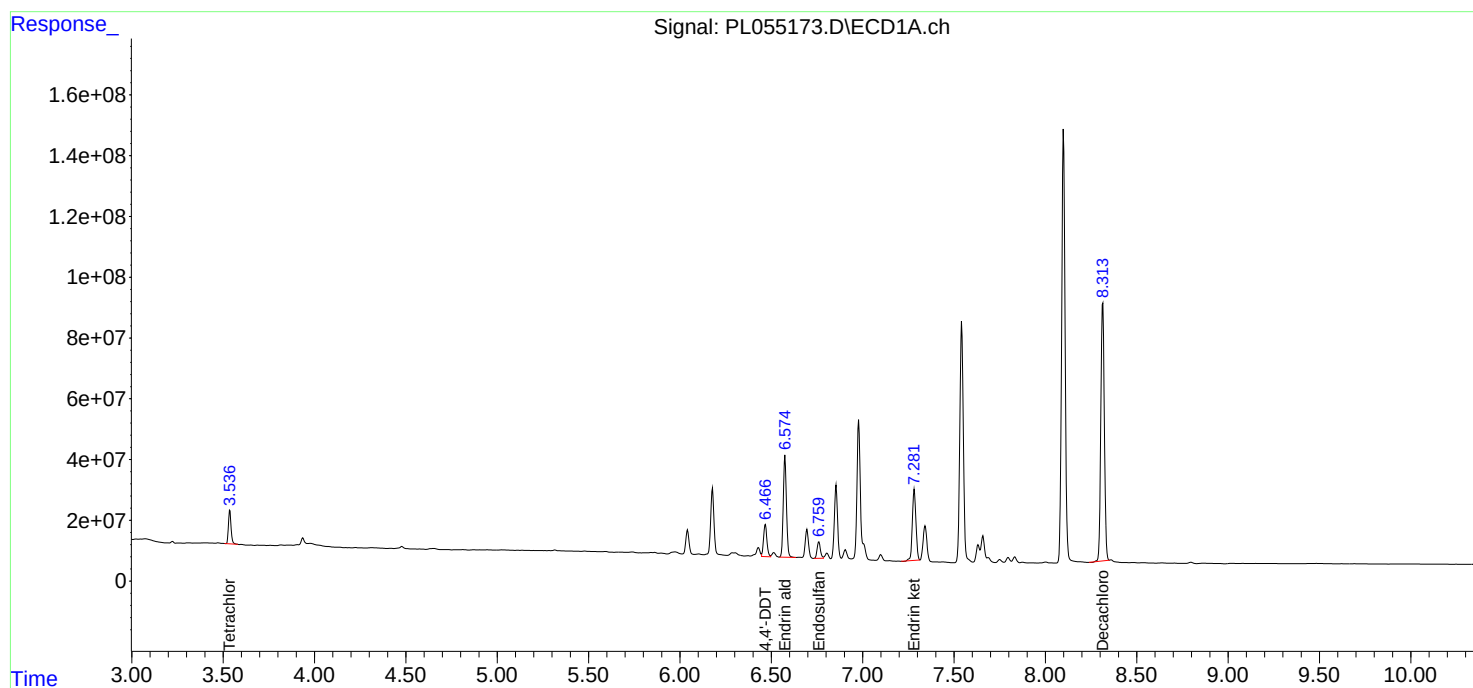


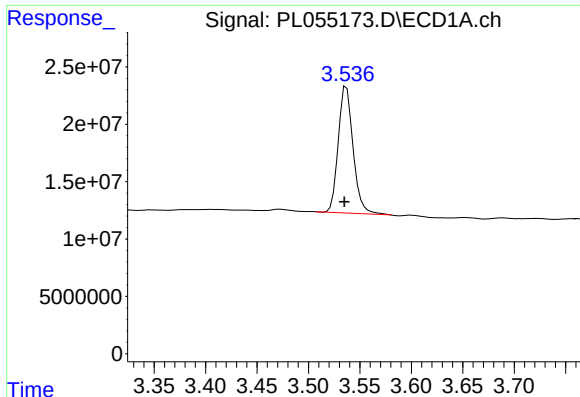

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.002 min
Response: 110642744
Conc: 10.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

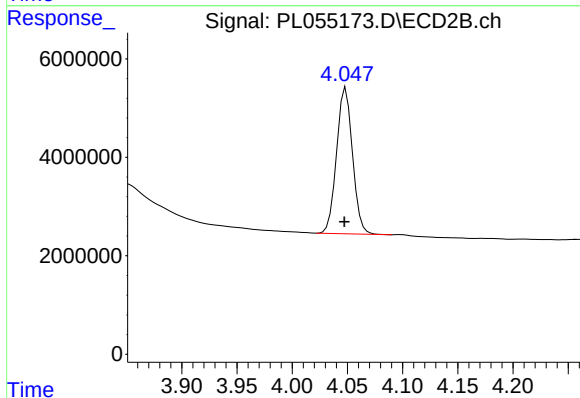


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.001 min
Response: 29758857
Conc: 11.26 ng/ml

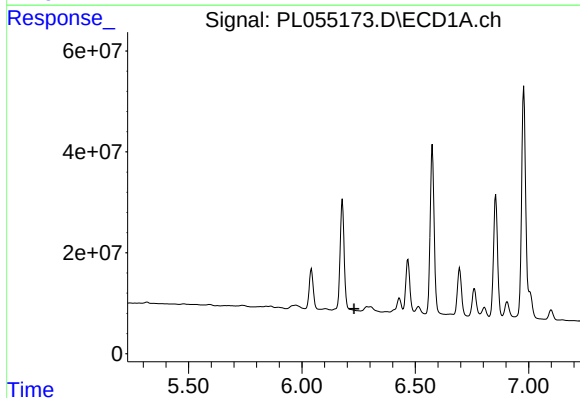


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

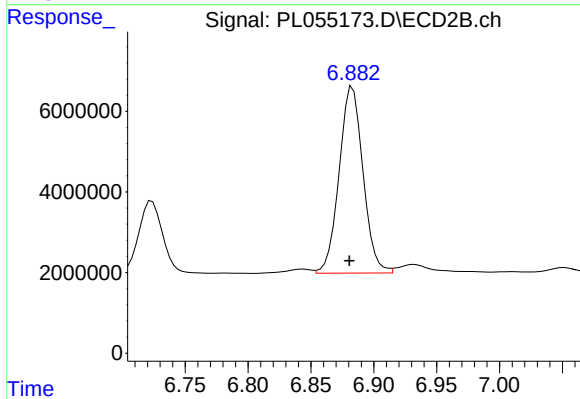

#16 4,4'-DDD


R.T.: 6.883 min
Delta R.T.: 0.003 min
Response: 61126961
Conc: 32.15 ng/ml

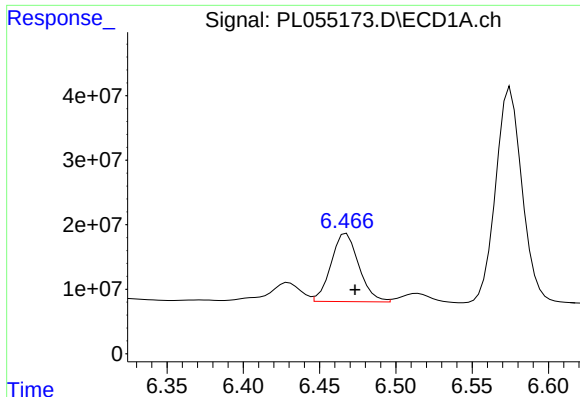

#17 4,4'-DDT


R.T.: 6.468 min
Delta R.T.: -0.006 min
Response: 134052199
Conc: 13.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

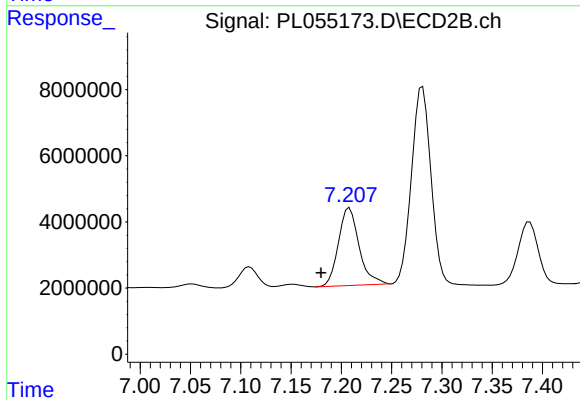


#17 4,4'-DDT

R.T.: 7.208 min
Delta R.T.: 0.028 min
Response: 33581108
Conc: 17.11 ng/ml

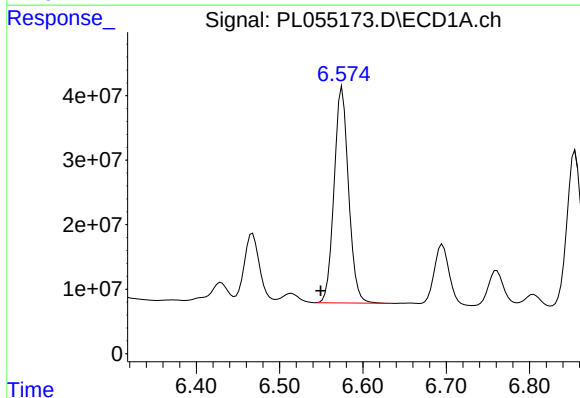


#18 Endrin aldehyde

R.T.: 6.575 min
Delta R.T.: 0.026 min
Response: 403488149
Conc: 41.43 ng/ml

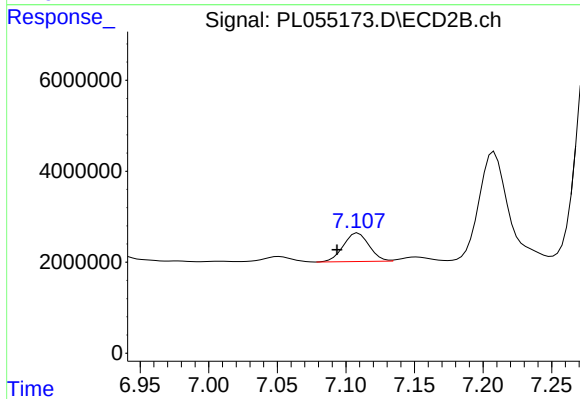

#18 Endrin aldehyde


R.T.: 7.109 min
Delta R.T.: 0.015 min
Response: 8209643
Conc: 4.25 ng/ml

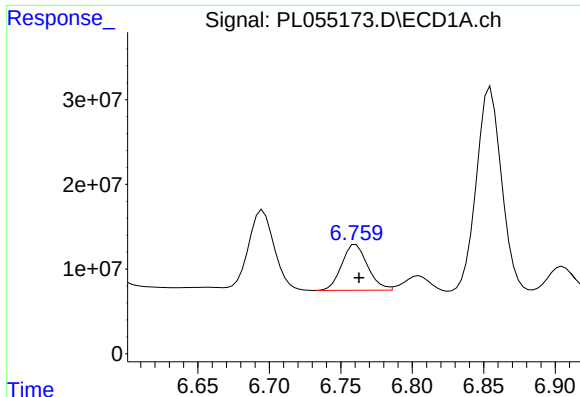

#19 Endosulfan Sulfate


R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 68476343
Conc: 6.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

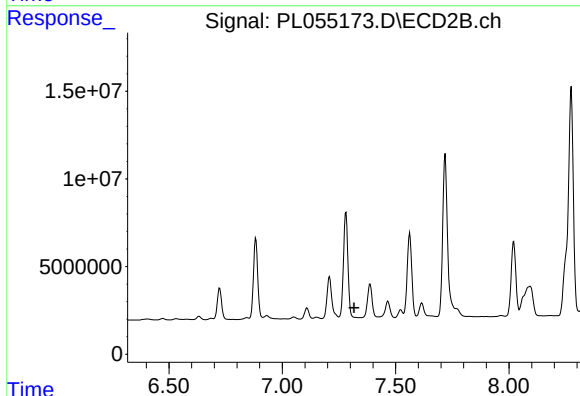


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.

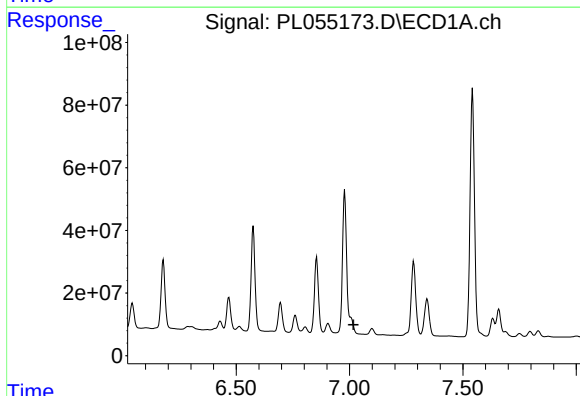


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.018 min
Response: 0
Conc: N.D.

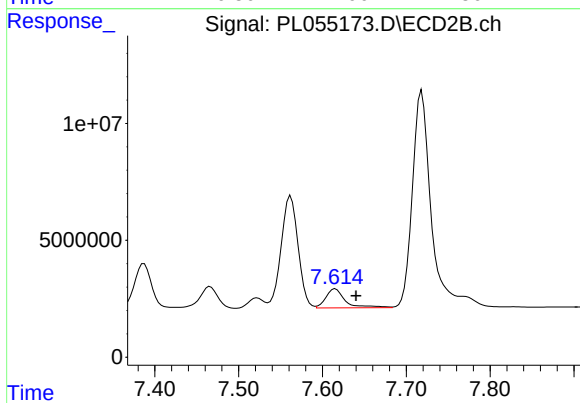

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: -0.025 min
Response: 13162266
Conc: 12.20 ng/ml

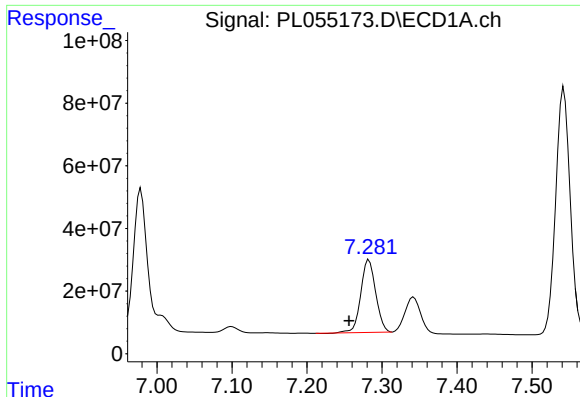

#21 Endrin ketone


R.T.: 7.283 min
Delta R.T.: 0.026 min
Response: 320172076
Conc: 30.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

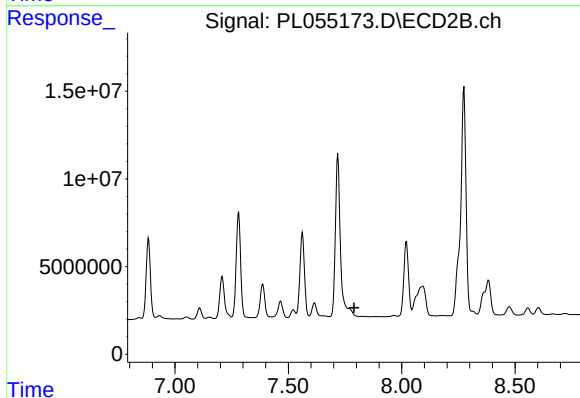


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.790 min
Response: 0
Conc: N.D.

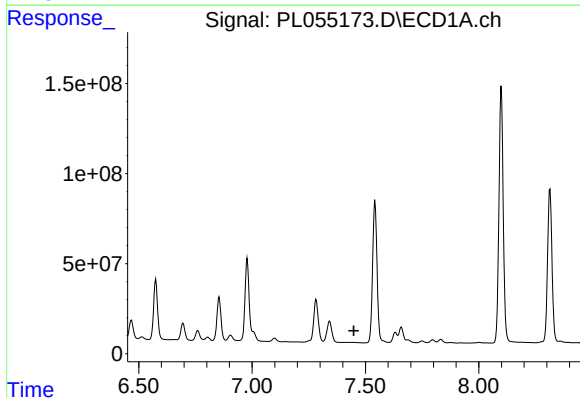


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.448 min
Response: 0
Conc: N.D.

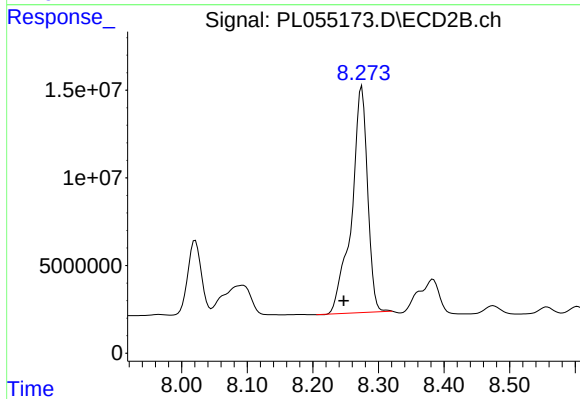

#22 Mirex


R.T.: 8.275 min
Delta R.T.: 0.028 min
Response: 218237801
Conc: 131.62 ng/ml

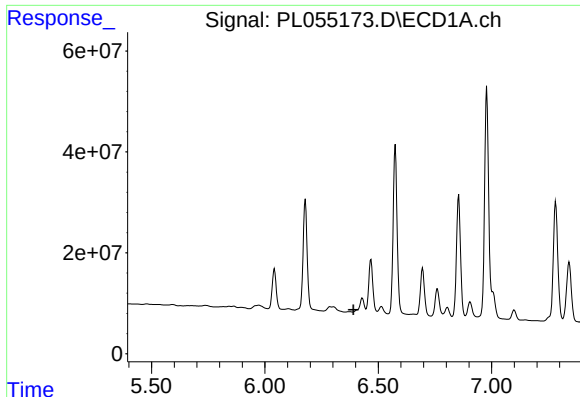

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

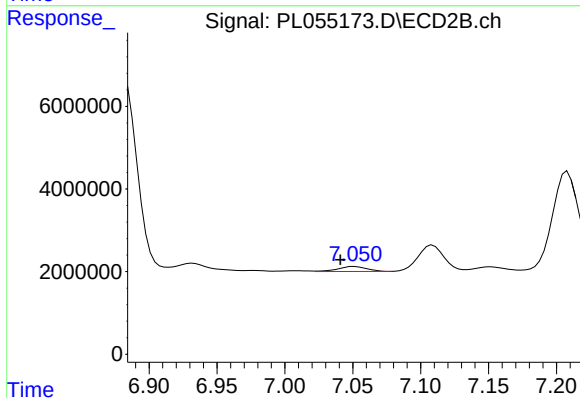


#27 Chlordane-5

R.T.: 7.051 min
Delta R.T.: 0.010 min
Response: 1821677
Conc: 26.11 ng/ml

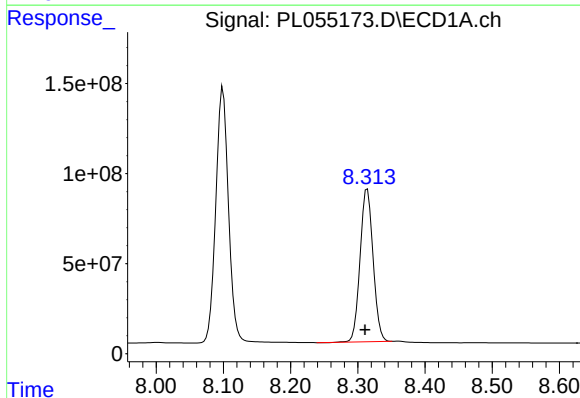

#28 Decachlorobiphenyl

R.T.: 8.314 min
Delta R.T.: 0.004 min
Response: 1138279174
Conc: 122.68 ng/ml

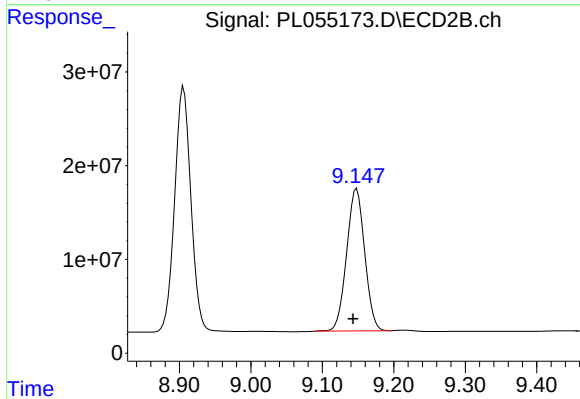

#28 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: 0.005 min
Response: 266446960
Conc: 120.70 ng/ml