

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122319\
 Data File : PL055199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 19:56
 Operator : SG\AJ
 Sample : K6386-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:52:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.050	208.0E6	55754936	19.775	21.101
28)	SA Decachlor...	8.315	9.148	170.7E6	47258948	18.392	21.409
Target Compounds							
2)	A alpha-BHC	0.000	4.460f	0	2459655	N.D.	0.668 #
8)	B Heptachlo...	0.000	5.911	0	7152578	N.D.	2.806 #
10)	B gamma-Chl...	0.000	6.169	0	3318287	N.D.	1.250 #
15)	B Endosulfa...	6.404f	0.000	94771996	0	8.075	N.D. #
18)	B Endrin al...	0.000	7.097	0	2043845	N.D.	1.059 #
24)	Chlordane-2	4.922	0.000	41287964	0	97.484	N.D. #
25)	Chlordane-3	0.000	6.169	0	3318287	N.D.	10.311 #
27)	Chlordane-5	6.404	7.029	94771996	1883425	243.212	26.993 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122319\
Data File : PL055199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 19:56
Operator : SG\AJ
Sample : K6386-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:52:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

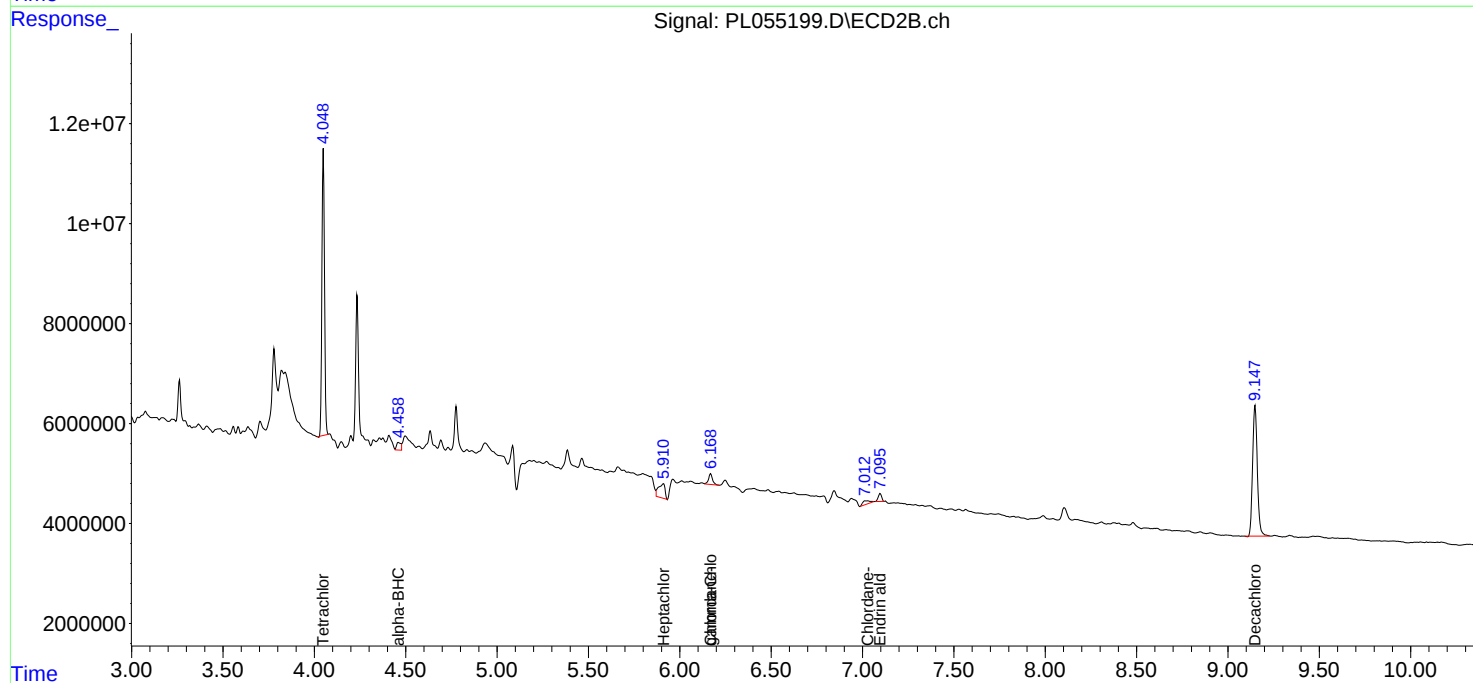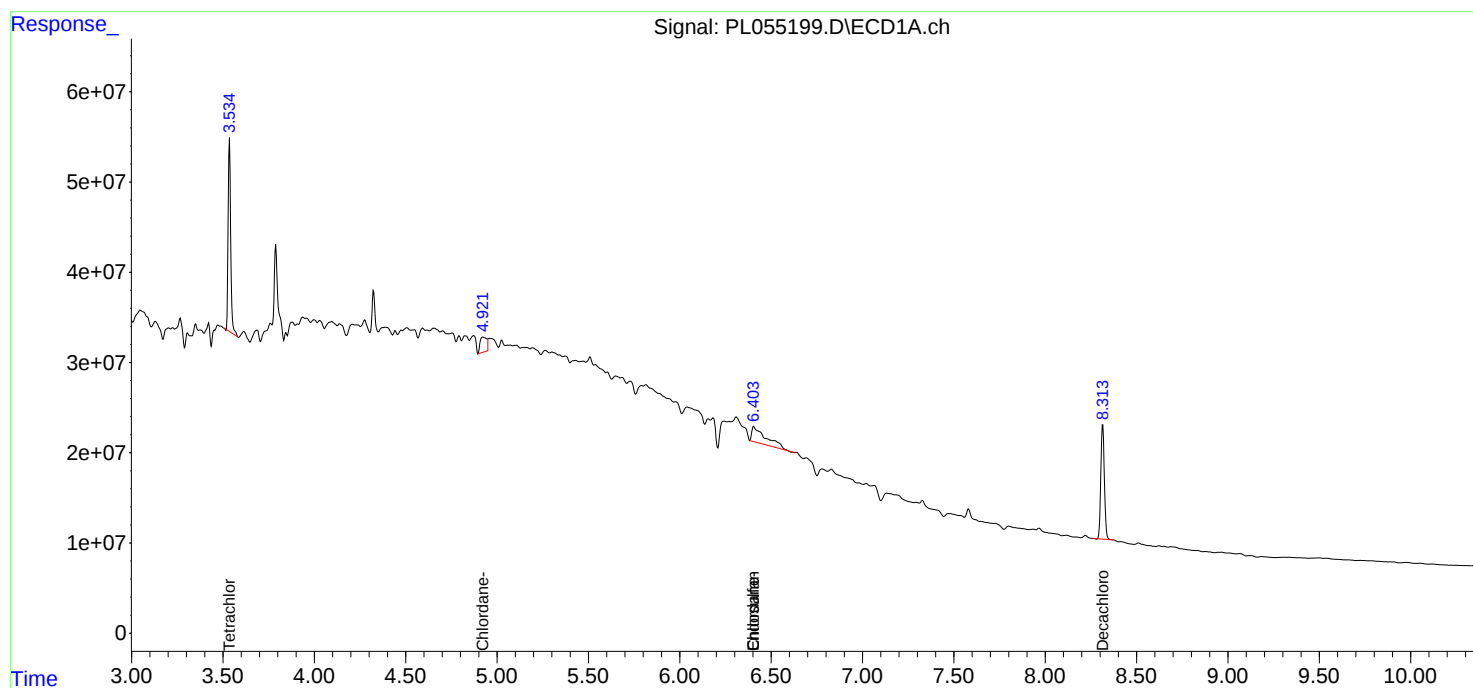


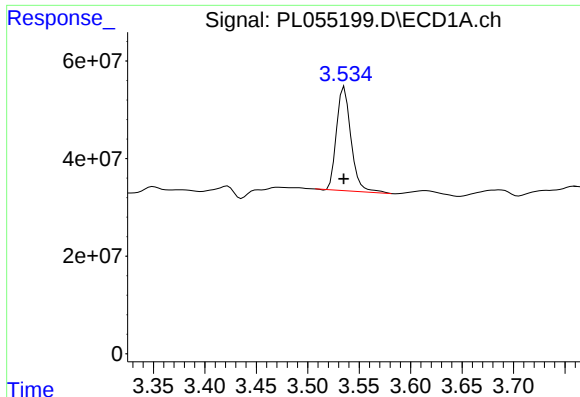

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 207962707
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

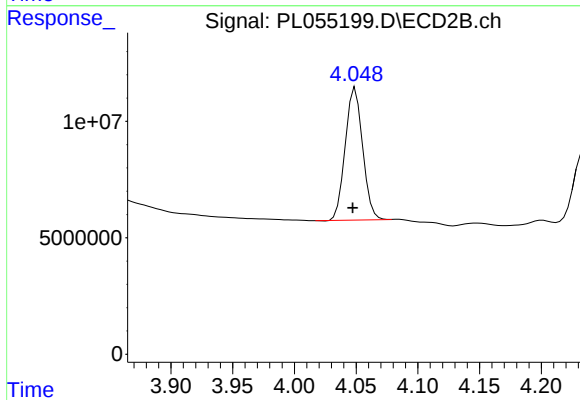


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: 0.002 min
Response: 55754936
Conc: 21.10 ng/ml

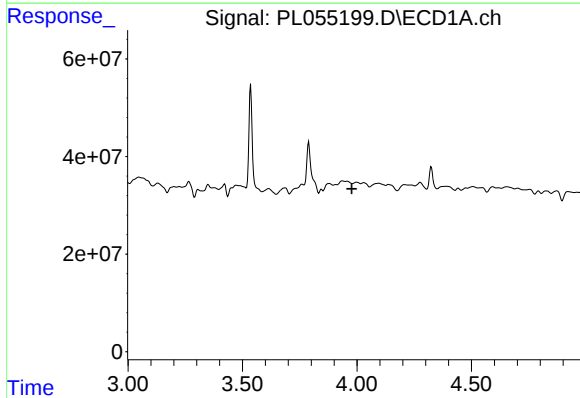


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.977 min
Response: 0
Conc: N.D.

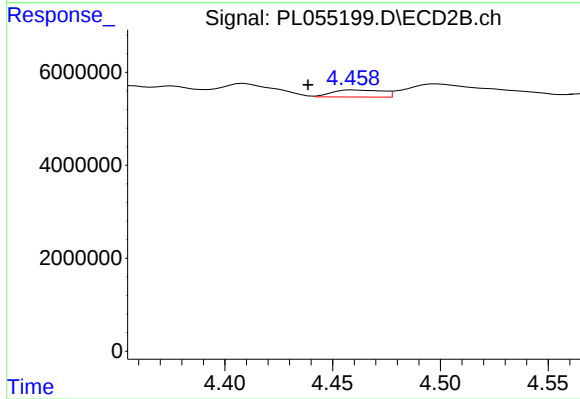

#2 alpha-BHC


R.T.: 4.460 min
Delta R.T.: 0.021 min
Response: 2459655
Conc: 0.67 ng/ml

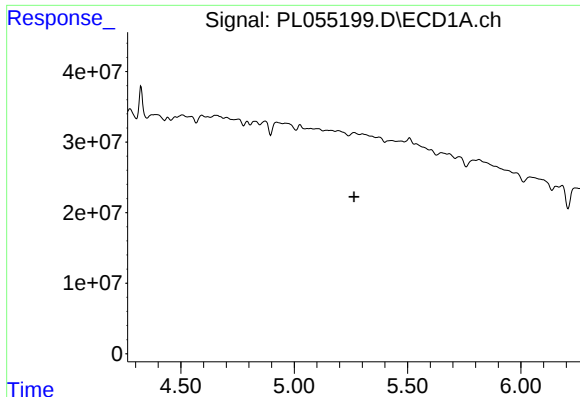

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.265 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

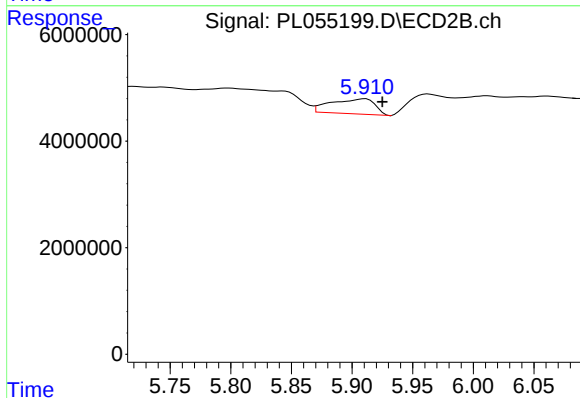


#8 Heptachlor epoxide

R.T.: 5.911 min
Delta R.T.: -0.014 min
Response: 7152578
Conc: 2.81 ng/ml

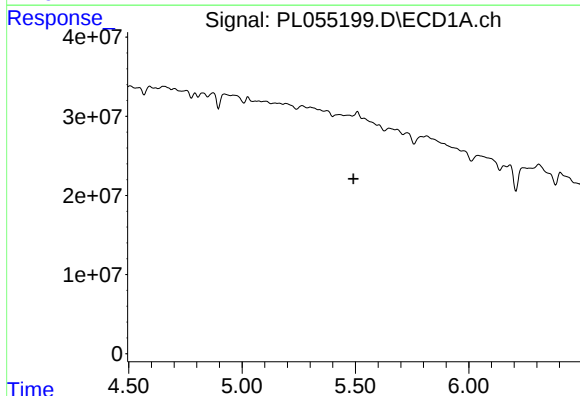


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

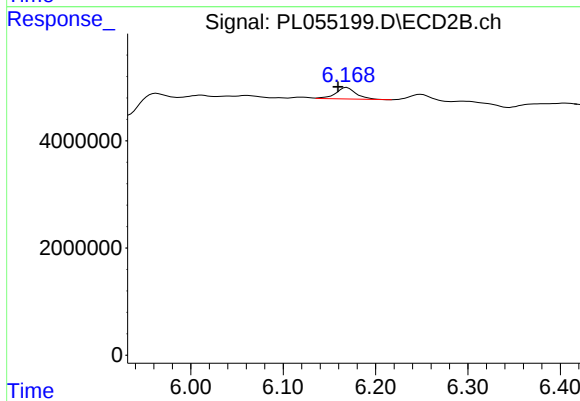

#10 gamma-Chlordane


R.T.: 6.169 min
Delta R.T.: 0.010 min
Response: 3318287
Conc: 1.25 ng/ml

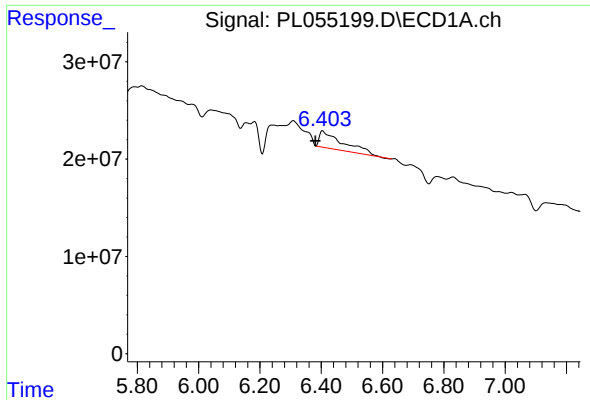

#15 Endosulfan II


R.T.: 6.404 min
Delta R.T.: 0.023 min
Response: 94771996
Conc: 8.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

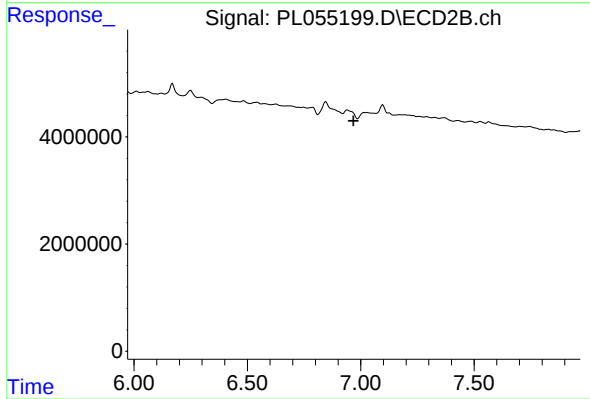


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.968 min
Response: 0
Conc: N.D.

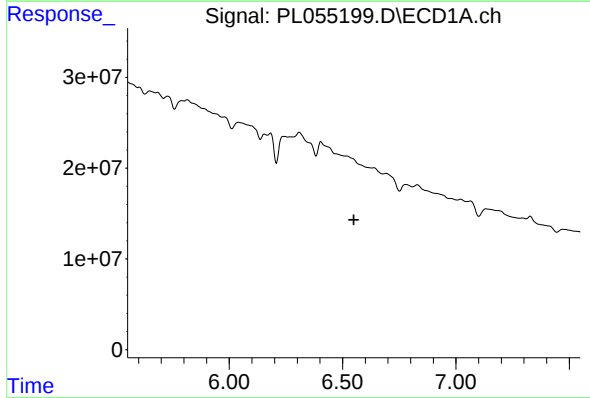


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.549 min
Response: 0
Conc: N.D.

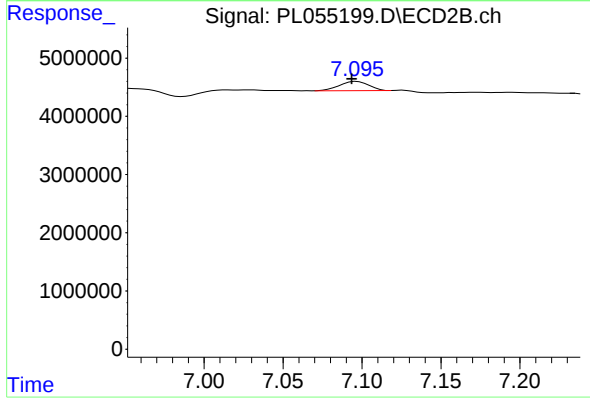

#18 Endrin aldehyde


R.T.: 7.097 min
Delta R.T.: 0.003 min
Response: 2043845
Conc: 1.06 ng/ml

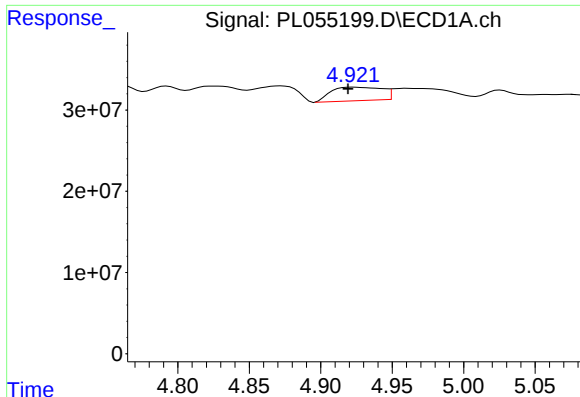

#24 Chlordane-2


R.T.: 4.922 min
Delta R.T.: 0.003 min
Response: 41287964
Conc: 97.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

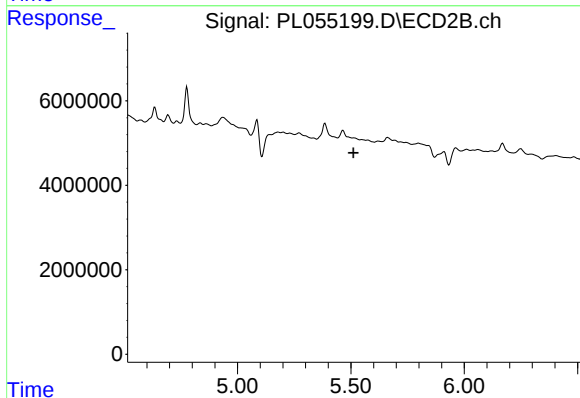


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.512 min
Response: 0
Conc: N.D.

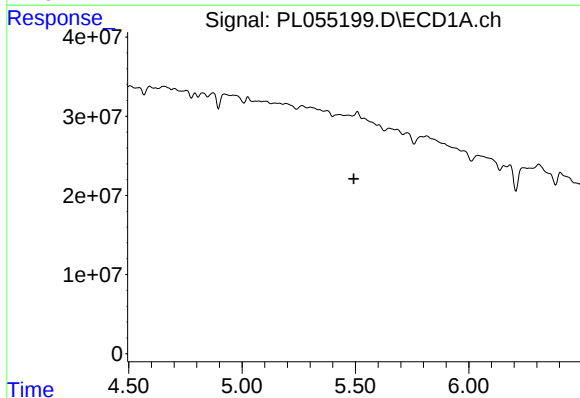


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

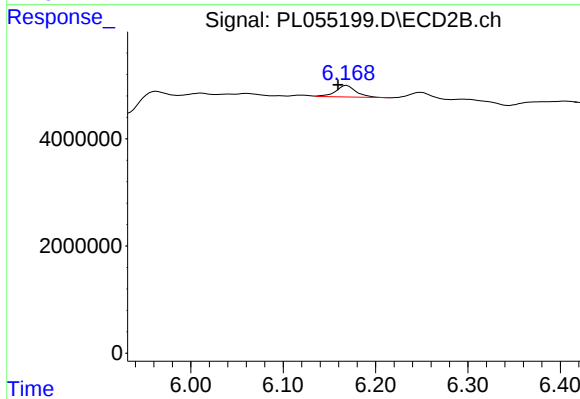

#25 Chlordane-3


R.T.: 6.169 min
Delta R.T.: 0.009 min
Response: 3318287
Conc: 10.31 ng/ml

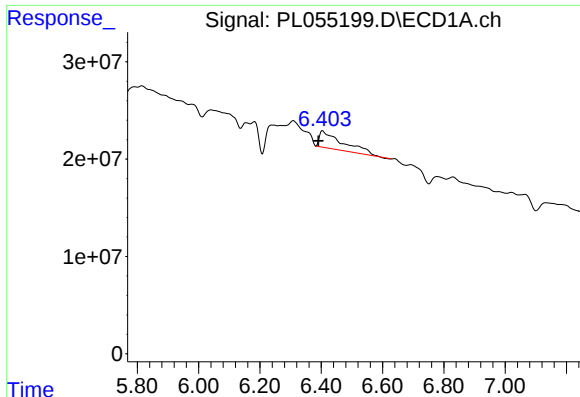

#27 Chlordane-5


R.T.: 6.404 min
Delta R.T.: 0.013 min
Response: 94771996
Conc: 243.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

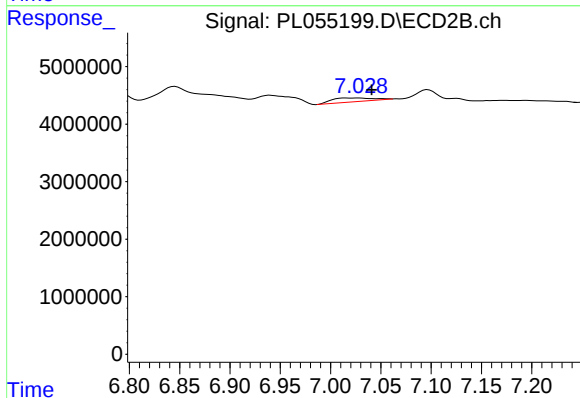


#27 Chlordane-5

R.T.: 7.029 min
Delta R.T.: -0.012 min
Response: 1883425
Conc: 26.99 ng/ml

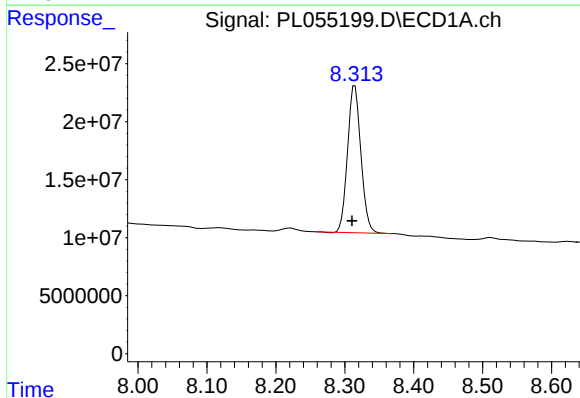

#28 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: 0.004 min
Response: 170657037
Conc: 18.39 ng/ml

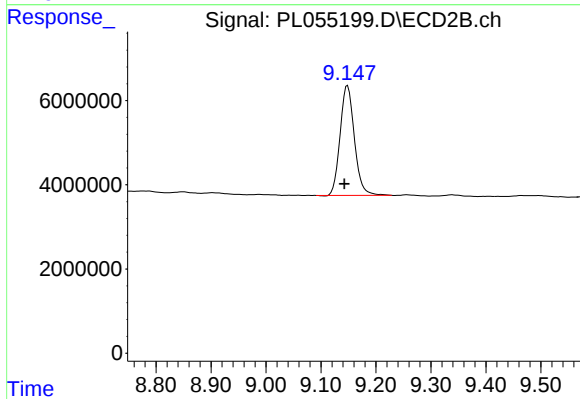

#28 Decachlorobiphenyl

R.T.: 9.148 min
Delta R.T.: 0.006 min
Response: 47258948
Conc: 21.41 ng/ml