

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122319\
 Data File : PL055180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 15:17
 Operator : SG\AJ
 Sample : K6395-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 12/24/2019 10:41:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:48:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	4.048	144.0E6	38103757	13.692	14.421
28)	SA Decachlor...	8.313	9.147	141.2E6	35678367	15.223	16.163
Target Compounds							
17)	MA 4,4'-DDT	6.473	7.180	6088808	1028079	0.605m	0.524m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122319\
Data File : PL055180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 15:17
Operator : SG\AJ
Sample : K6395-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
12/24/2019 10:41:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:48:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

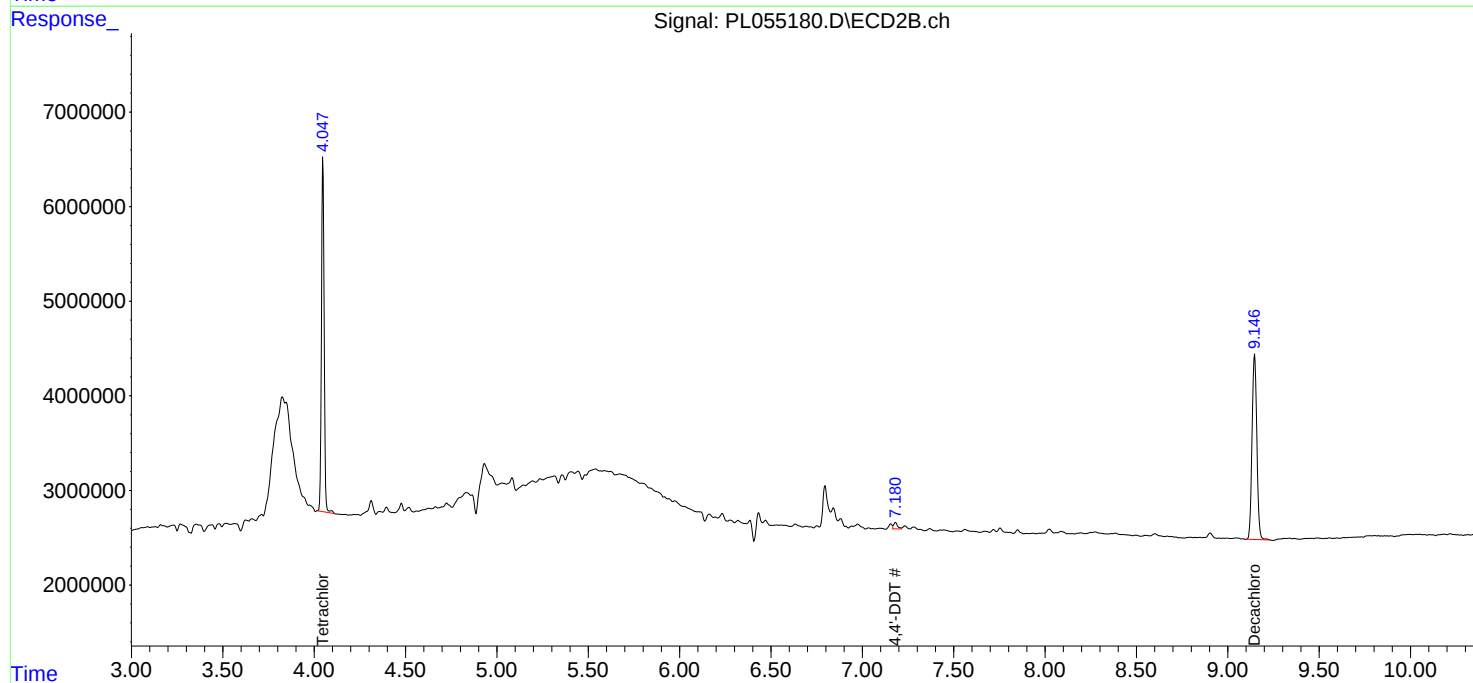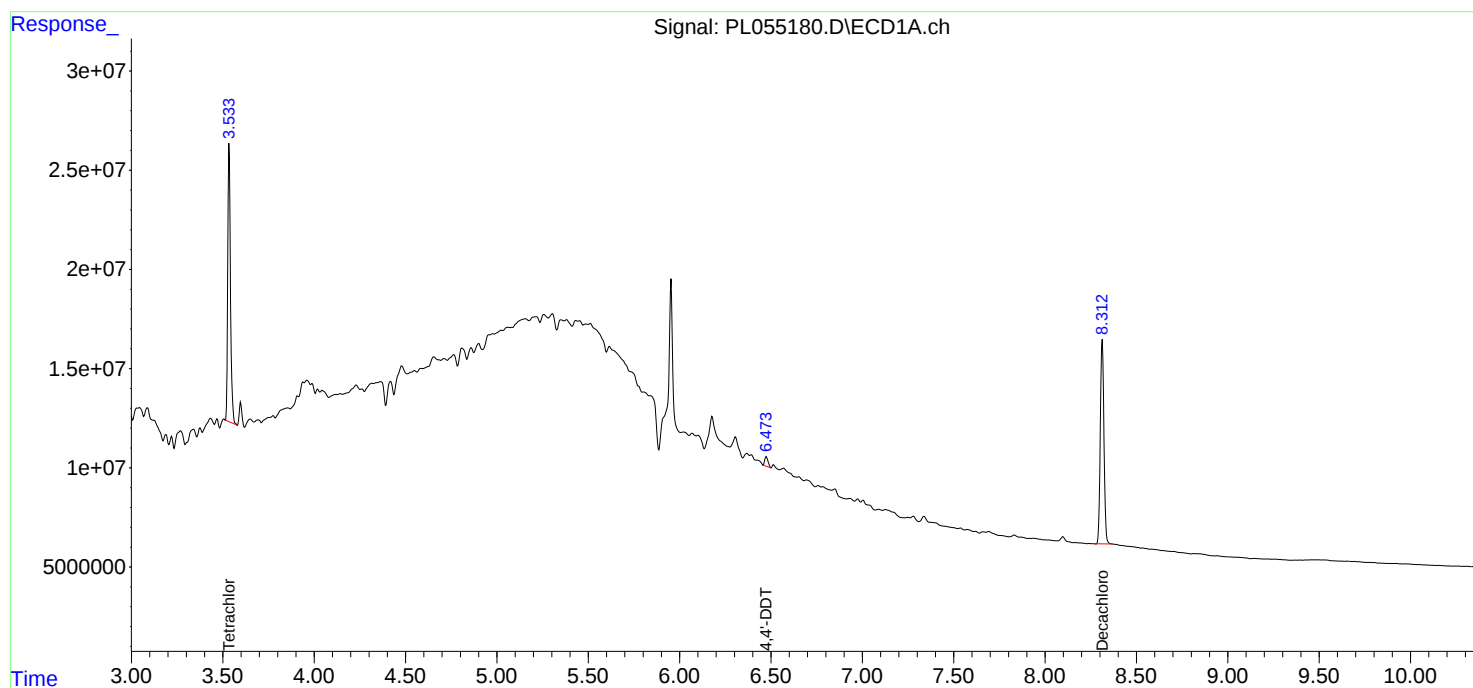

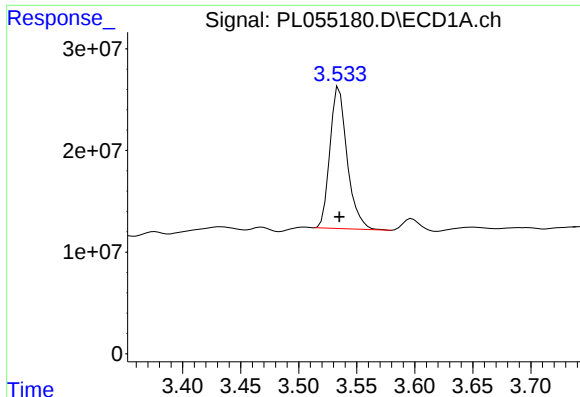


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 143995706
Conc: 13.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
12/24/2019 10:41:53 AM

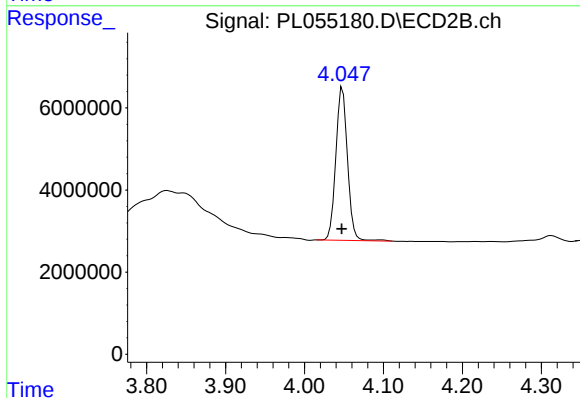


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.001 min
Response: 38103757
Conc: 14.42 ng/ml

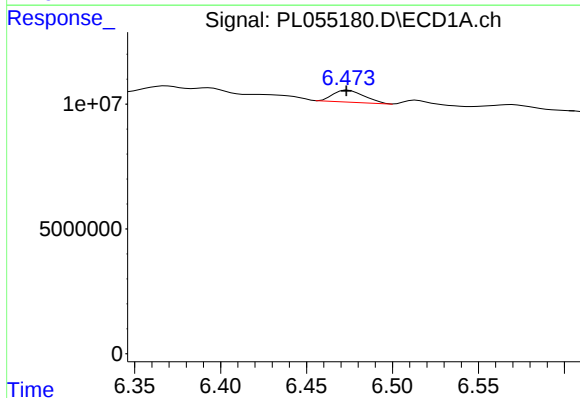


#17 4,4'-DDT

R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 6088808
Conc: 0.60 ng/ml m

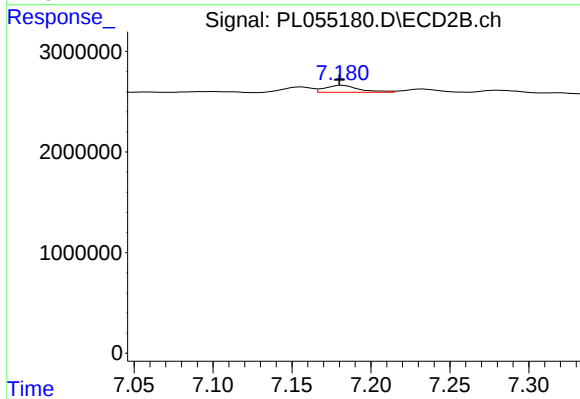

#17 4,4'-DDT

R.T.: 7.180 min
Delta R.T.: 0.000 min
Response: 1028079
Conc: 0.52 ng/ml m

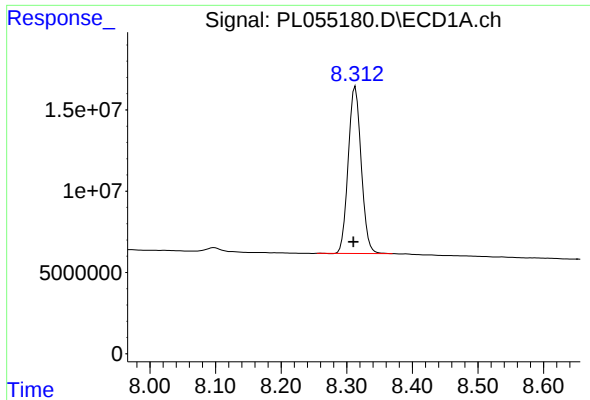

#28 Decachlorobiphenyl

R.T.: 8.313 min

Delta R.T.: 0.003 min


Response: 141246990

Conc: 15.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Ankita
12/24/2019 10:41:53 AM

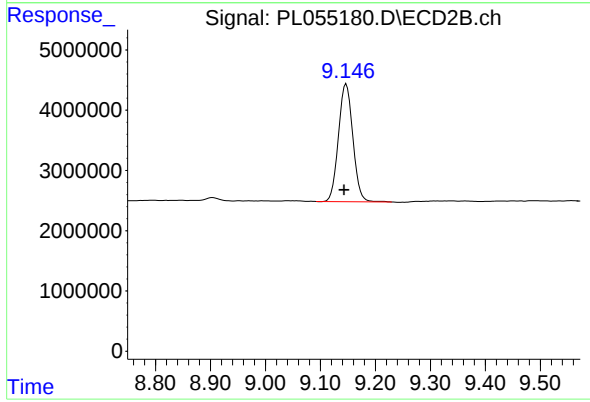

#28 Decachlorobiphenyl

R.T.: 9.147 min

Delta R.T.: 0.004 min

Response: 35678367

Conc: 16.16 ng/ml