

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122320\
 Data File : PL063771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 09:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 12:51:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.160f	0.000	30334862	0	8.074	N.D. #
10) B	gamma-Chl...	0.000	6.234f	0	26501458	N.D.	9.578 #
11) B	alpha-Chl...	0.000	6.319	0	3954927	N.D.	1.433 #
25)	Chlordane-3	0.000	6.234f	0	26501458	N.D.	77.346 #
26)	Chlordane-4	0.000	6.319	0	3954927	N.D.	9.622 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122320\
Data File : PL063771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 09:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 12:51:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

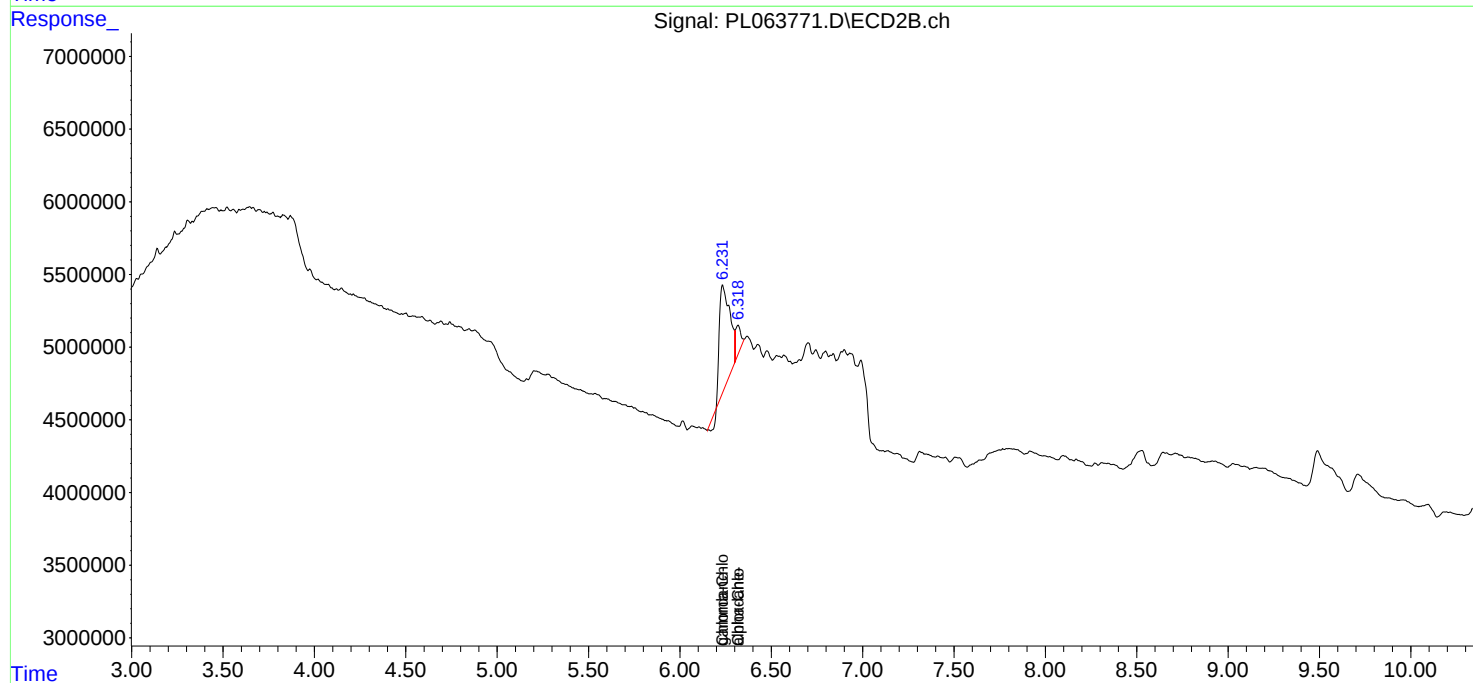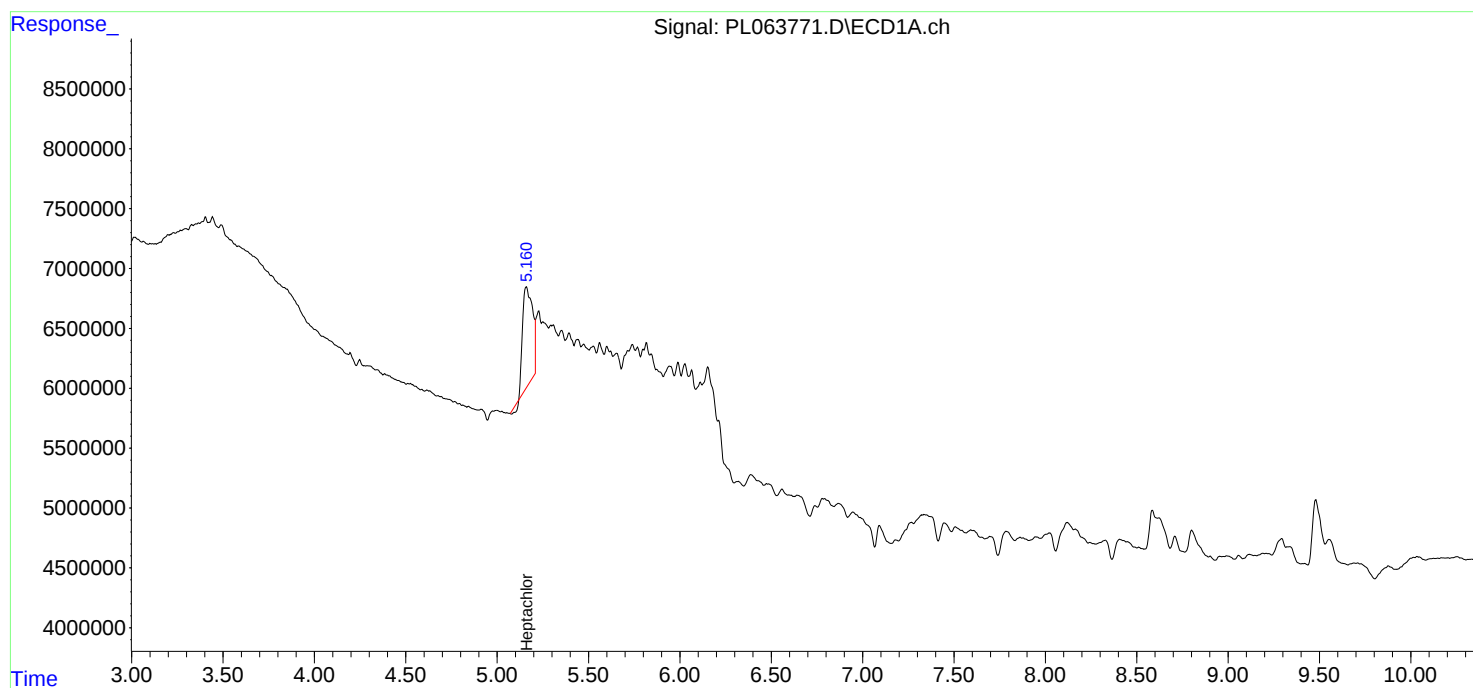


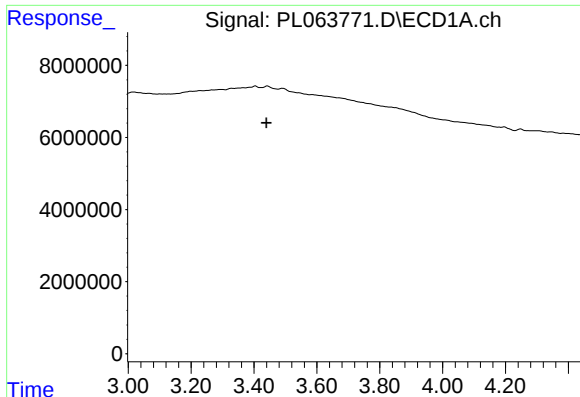

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

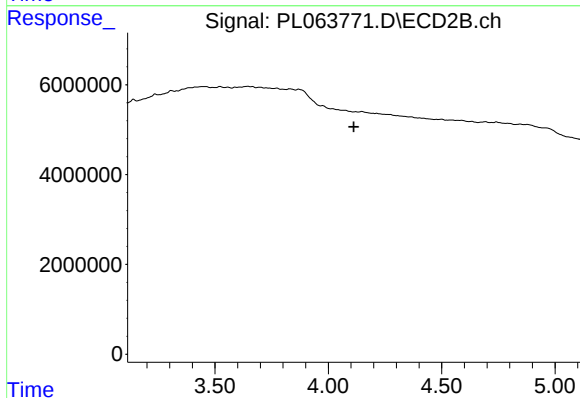


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.113 min
Response: 0
Conc: N.D.

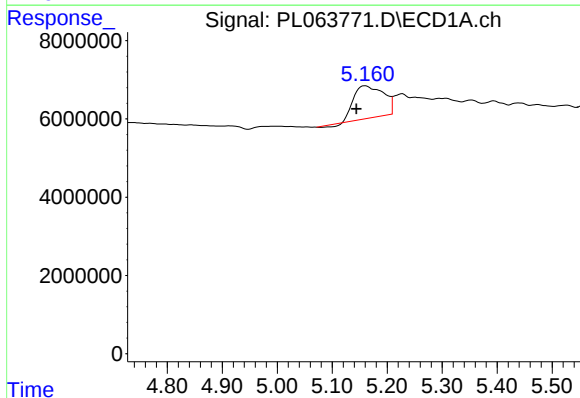


#8 Heptachlor epoxide

R.T.: 5.160 min
Delta R.T.: 0.016 min
Response: 30334862
Conc: 8.07 ng/ml

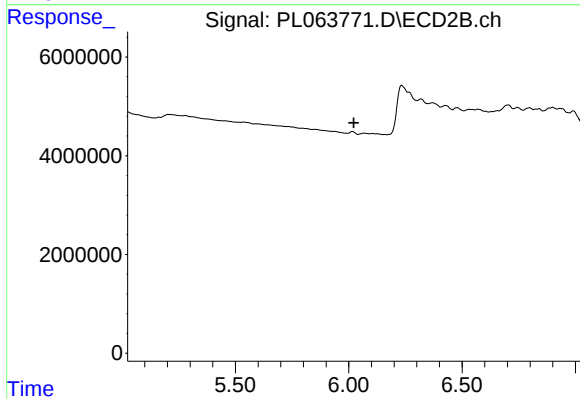

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 6.022 min
Response: 0
Conc: N.D.

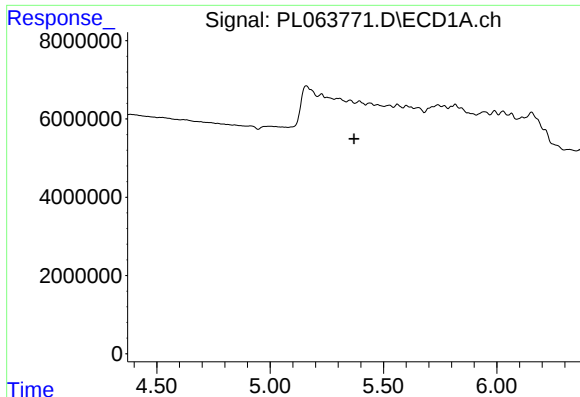

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

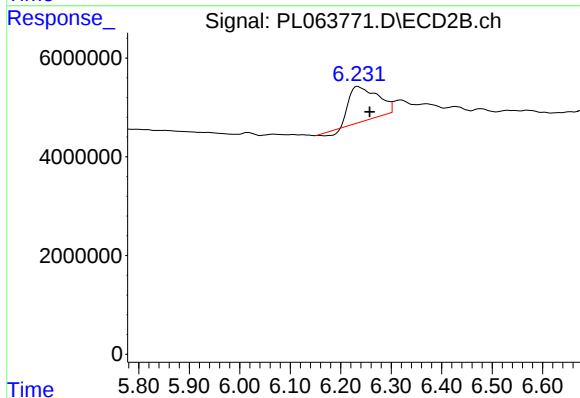


#10 gamma-Chlordane

R.T.: 6.234 min
Delta R.T.: -0.024 min
Response: 26501458
Conc: 9.58 ng/ml

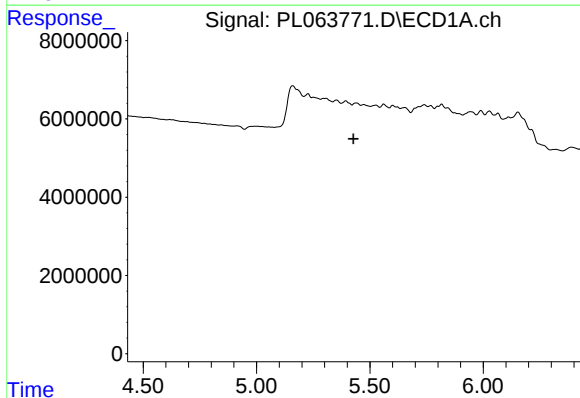


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

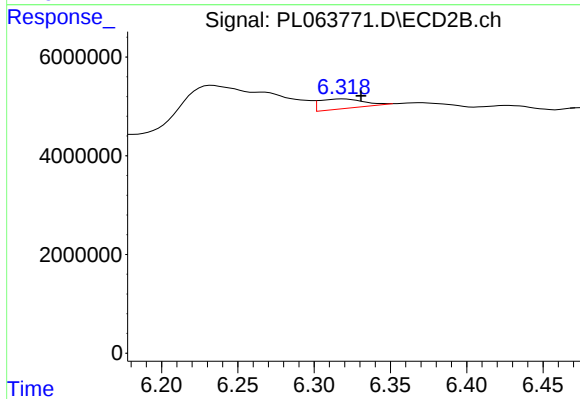

#11 alpha-Chlordane


R.T.: 6.319 min
Delta R.T.: -0.012 min
Response: 3954927
Conc: 1.43 ng/ml

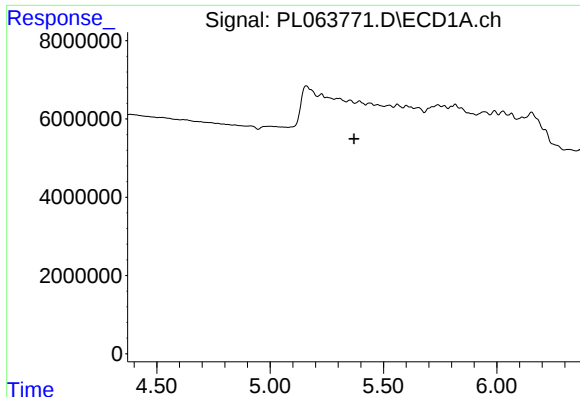

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

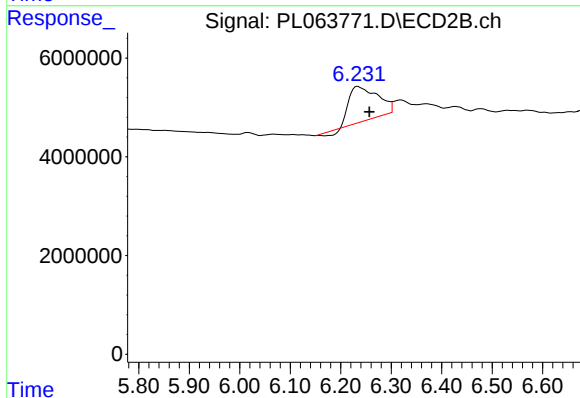


#25 Chlordane-3

R.T.: 6.234 min
Delta R.T.: -0.024 min
Response: 26501458
Conc: 77.35 ng/ml

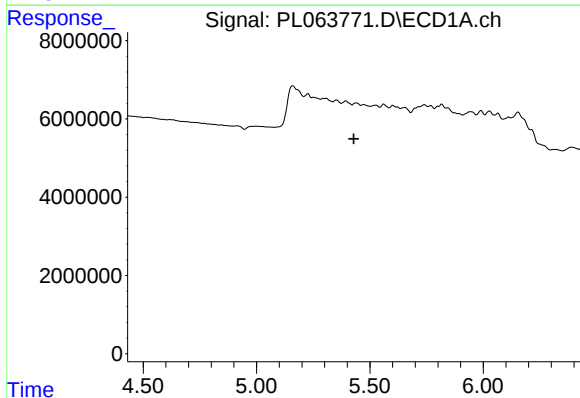


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.428 min
Response: 0
Conc: N.D.

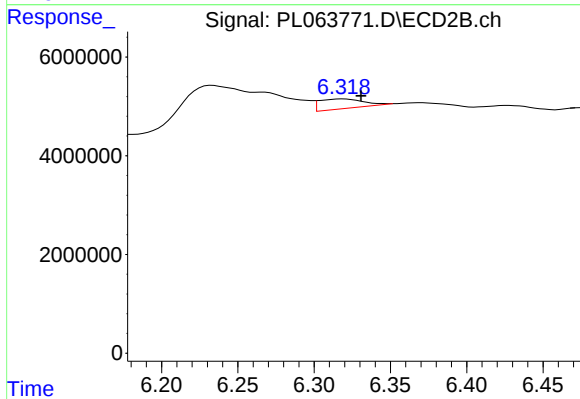

#26 Chlordane-4


R.T.: 6.319 min
Delta R.T.: -0.012 min
Response: 3954927
Conc: 9.62 ng/ml

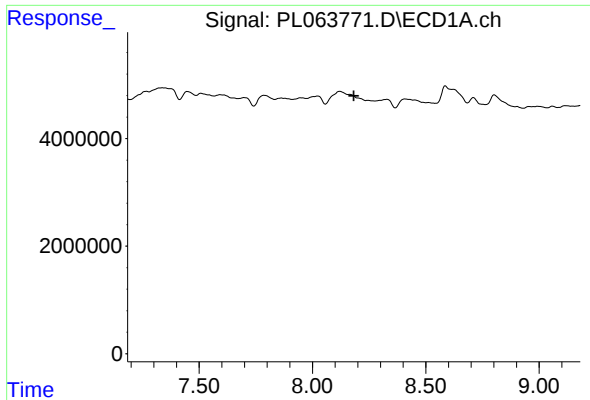

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

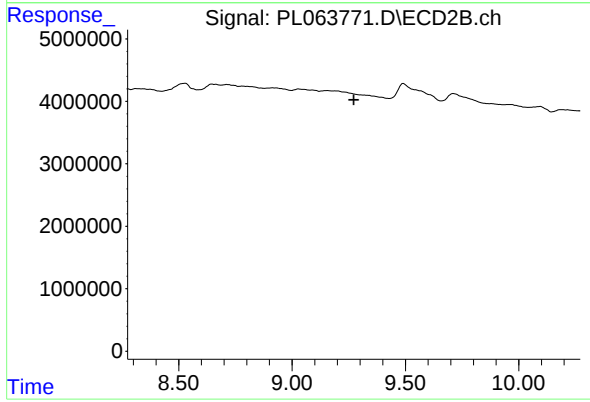

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.272 min
Response: 0
Conc: N.D.