

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122320\
 Data File : PL063794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 18:15
 Operator : AR\AJ
 Sample : L5179-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-24743

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 22:28:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	4.111	57162216	47492388	19.067	18.602
28) SA Decachlor...	8.178	9.266	38964879	27666145	14.143	14.032
Target Compounds						
6) B beta-BHC	4.377f	4.998f	5346615	4965430	2.766	2.829
23) Chlordane-1	4.312	0.000	4410888	0	43.041	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122320\
Data File : PL063794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 18:15
Operator : AR\AJ
Sample : L5179-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-24743

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 22:28:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

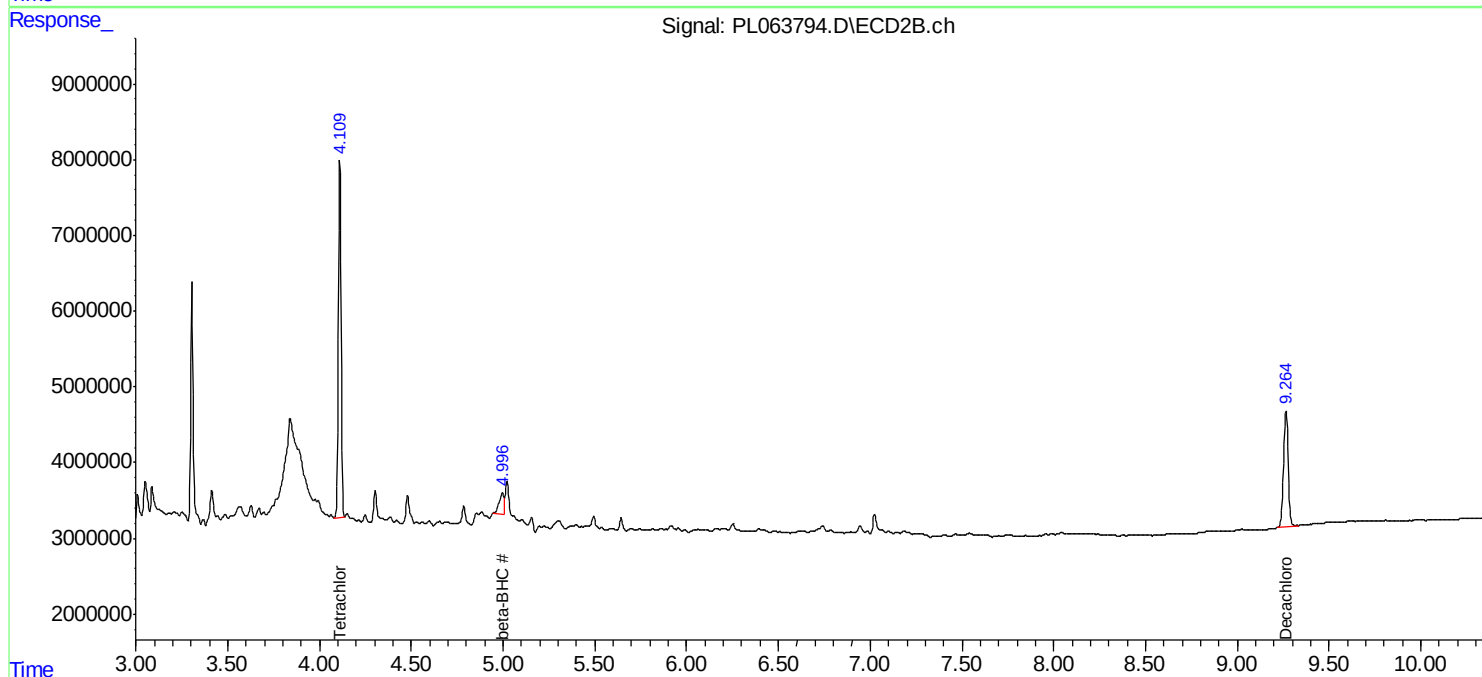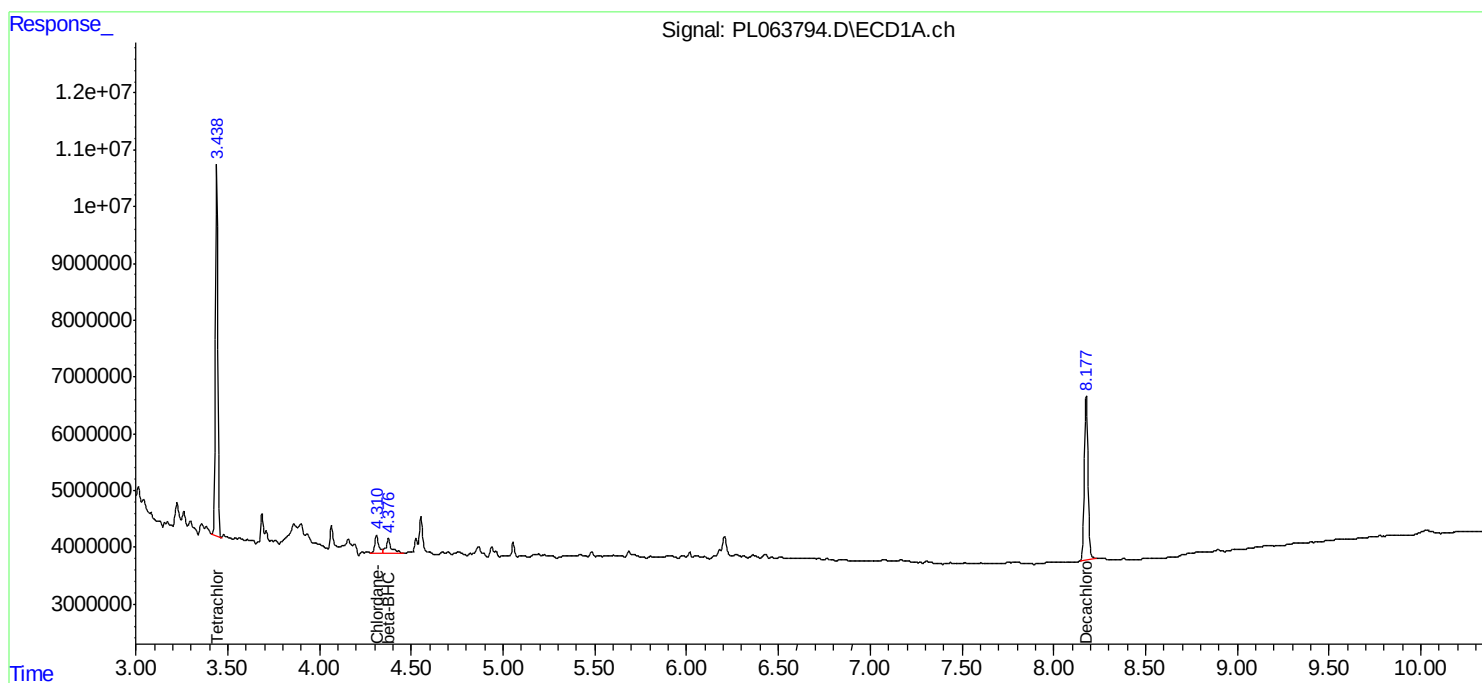


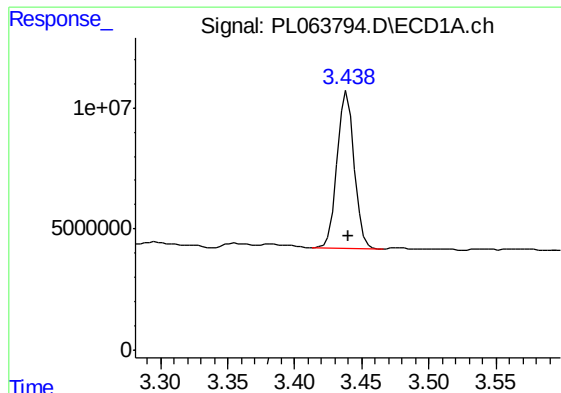

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 57162216
Conc: 19.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24743

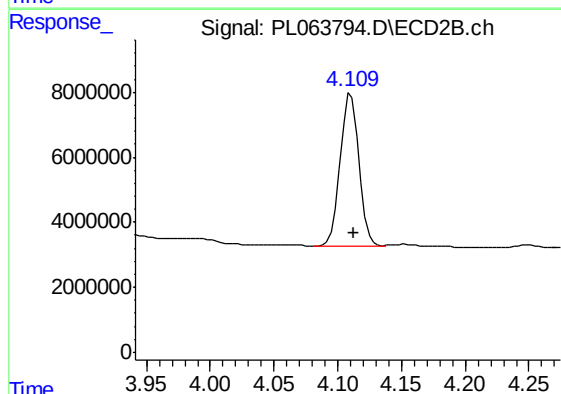


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 47492388
Conc: 18.60 ng/ml

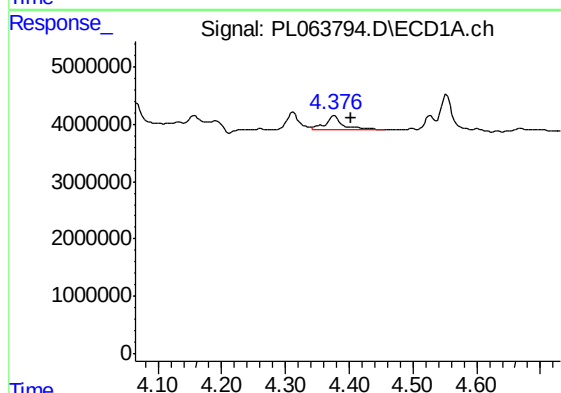


#6 beta-BHC

R.T.: 4.377 min
Delta R.T.: -0.027 min
Response: 5346615
Conc: 2.77 ng/ml

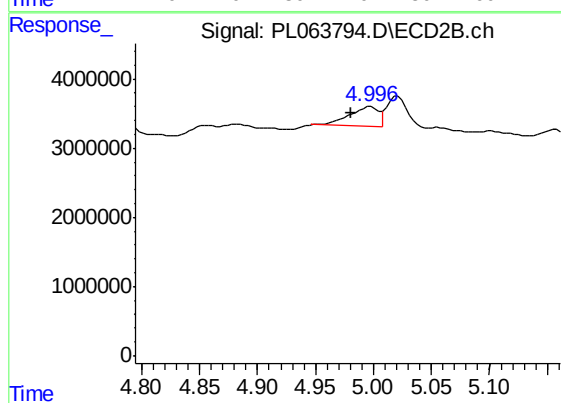

#6 beta-BHC


R.T.: 4.998 min
Delta R.T.: 0.017 min
Response: 4965430
Conc: 2.83 ng/ml

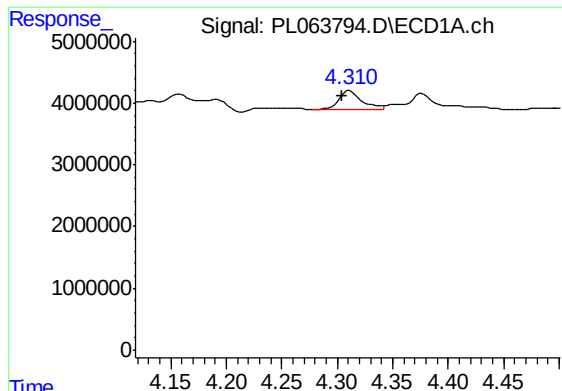

#23 Chlordane-1


R.T.: 4.312 min
Delta R.T.: 0.007 min
Response: 4410888
Conc: 43.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24743

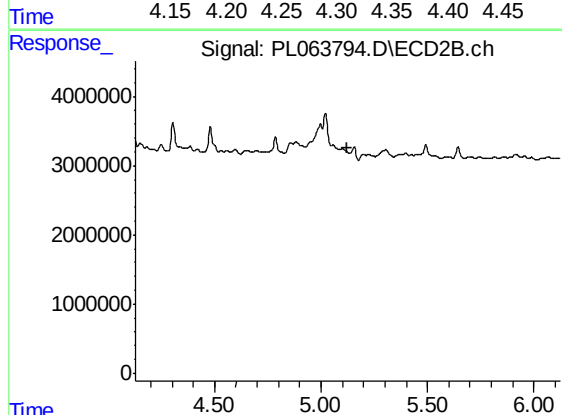


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.126 min
Response: 0
Conc: N.D.

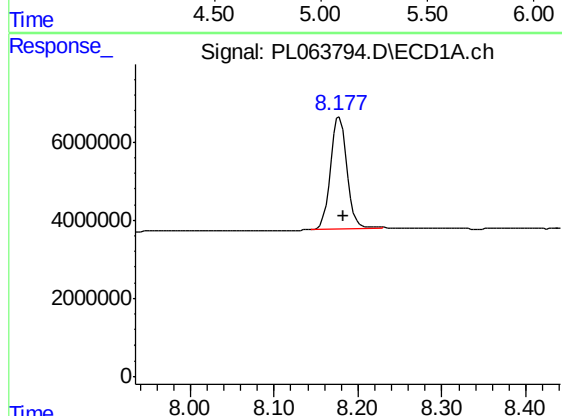

#28 Decachlorobiphenyl

R.T.: 8.178 min
Delta R.T.: -0.004 min
Response: 38964879
Conc: 14.14 ng/ml

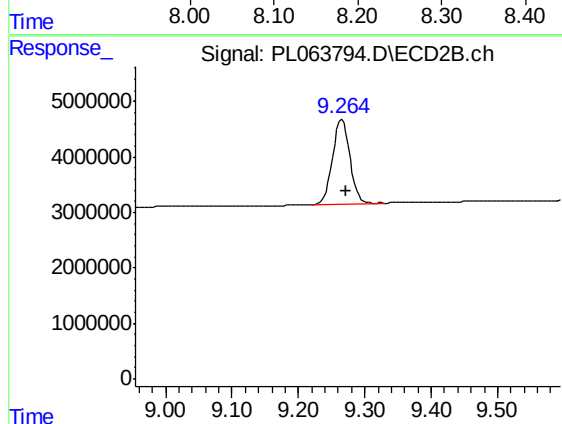

#28 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.006 min
Response: 27666145
Conc: 14.03 ng/ml