

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122320\
 Data File : PL063802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2020 20:10
 Operator : AR\AJ
 Sample : L5189-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 18

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 22:31:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.111	61733063	52846140	20.592	20.699
28)	SA Decachlor...	8.177	9.266	50456179	37031359	18.313	18.782
Target Compounds							
3)	MA gamma-BHC...	4.157	0.000	3625875	0	0.793	N.D. #
6)	B beta-BHC	0.000	4.989	0	3077948	N.D.	1.753 #
9)	A Endosulfan I	5.495	0.000	8288461	0	2.394	N.D. #
10)	B gamma-Chl...	0.000	6.254	0	3777422	N.D.	1.365 #
20)	A Methoxychlor	6.920f	0.000	5269358	0	4.011	N.D. #
25)	Chlordane-3	0.000	6.254	0	3777422	N.D.	11.025 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122320\
Data File : PL063802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2020 20:10
Operator : AR\AJ
Sample : L5189-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
18

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 22:31:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

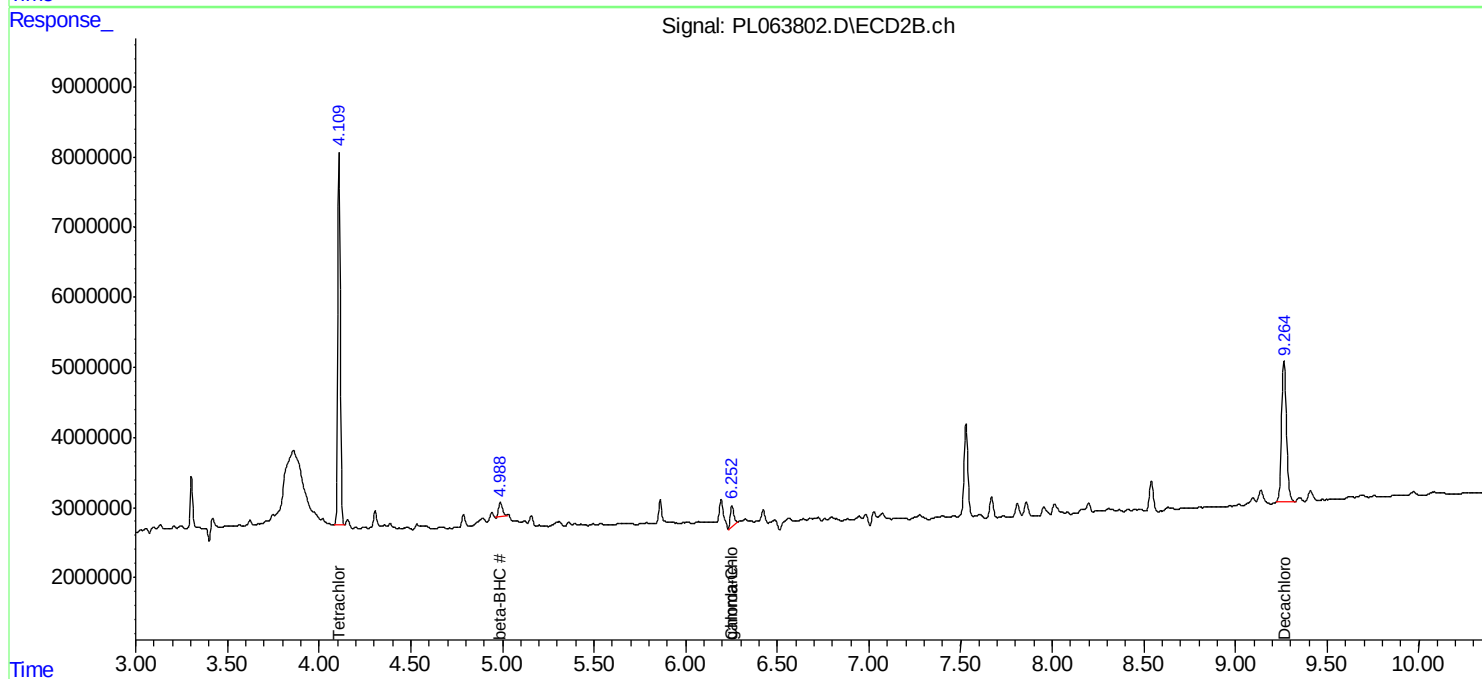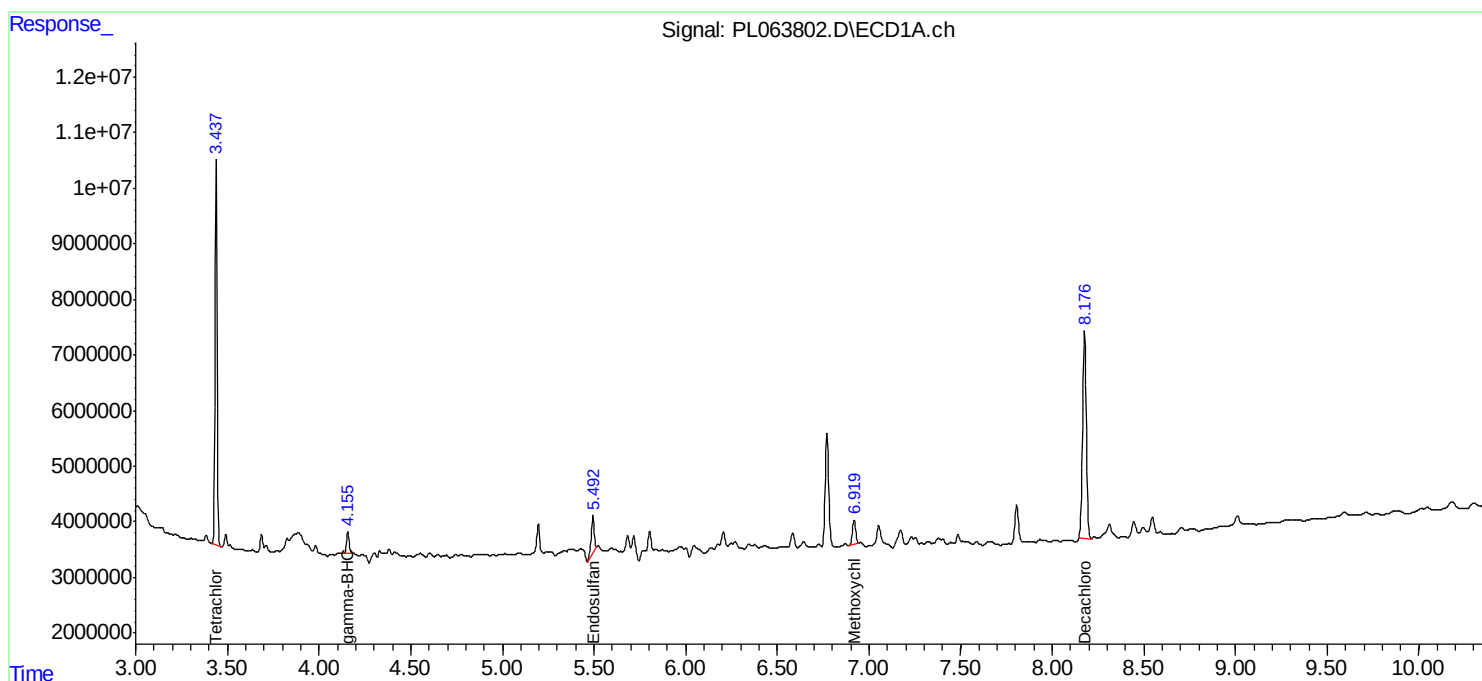


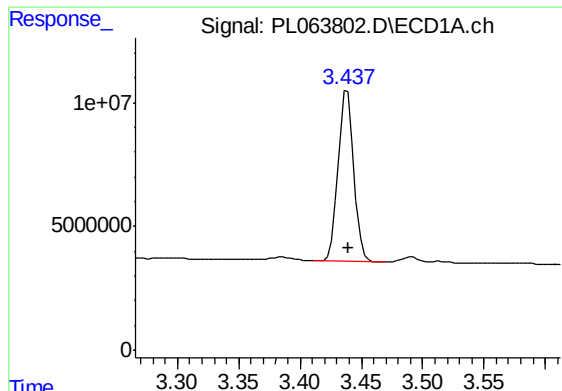

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: -0.001 min
Response: 61733063
Conc: 20.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
18

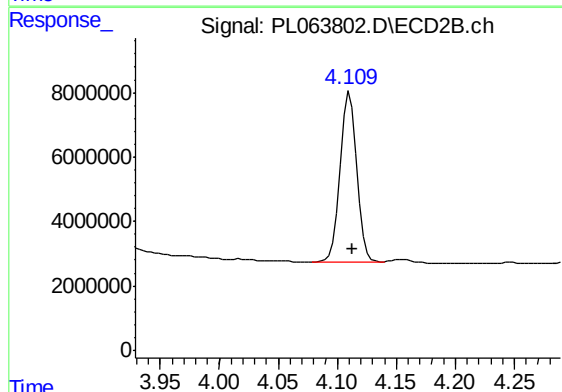


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 52846140
Conc: 20.70 ng/ml

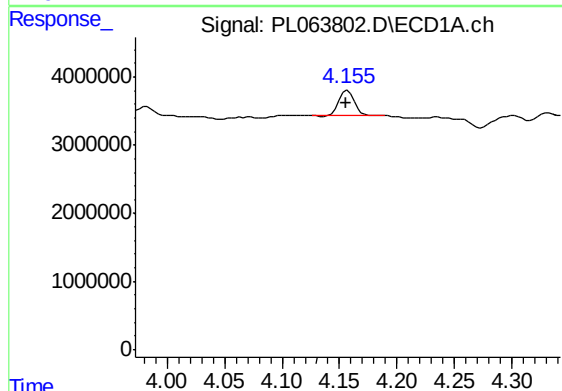


#3 gamma-BHC (Lindane)

R.T.: 4.157 min
Delta R.T.: 0.001 min
Response: 3625875
Conc: 0.79 ng/ml

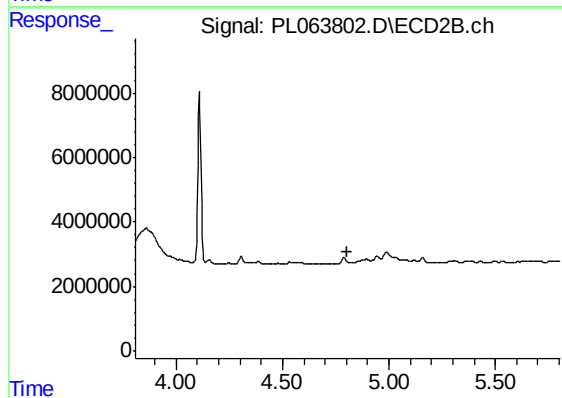

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.806 min
Response: 0
Conc: N.D.

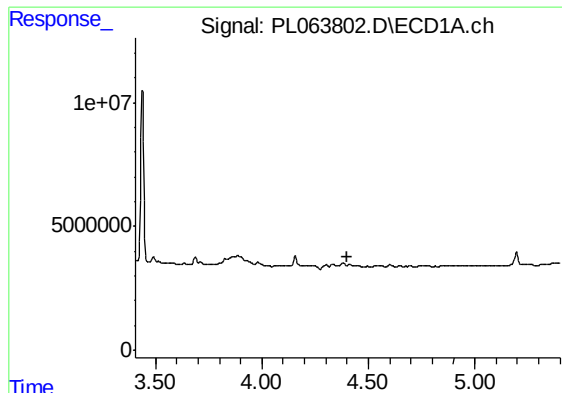

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18

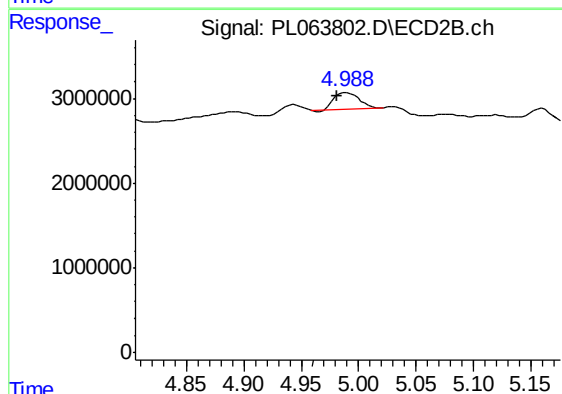


#6 beta-BHC

R.T.: 4.989 min
Delta R.T.: 0.008 min
Response: 3077948
Conc: 1.75 ng/ml

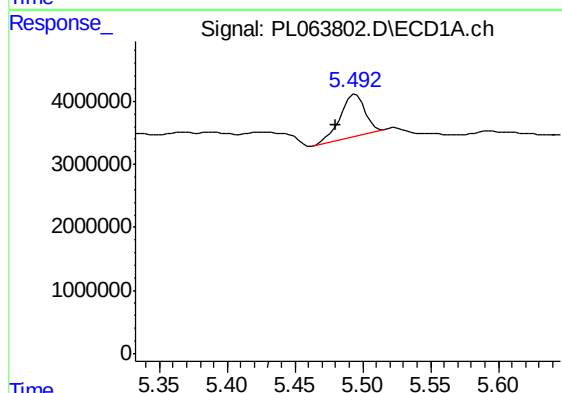


#9 Endosulfan I

R.T.: 5.495 min
Delta R.T.: 0.015 min
Response: 8288461
Conc: 2.39 ng/ml

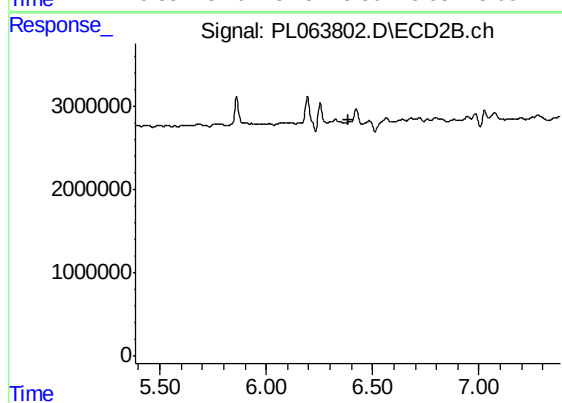

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

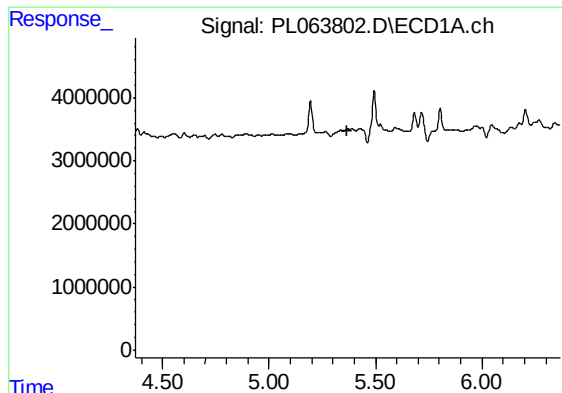

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18

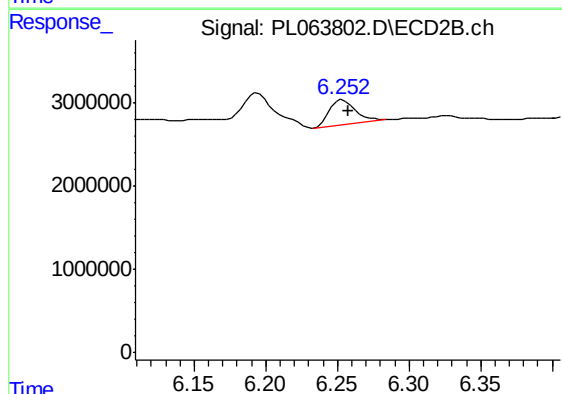


#10 gamma-Chlordane

R.T.: 6.254 min
Delta R.T.: -0.004 min
Response: 3777422
Conc: 1.37 ng/ml

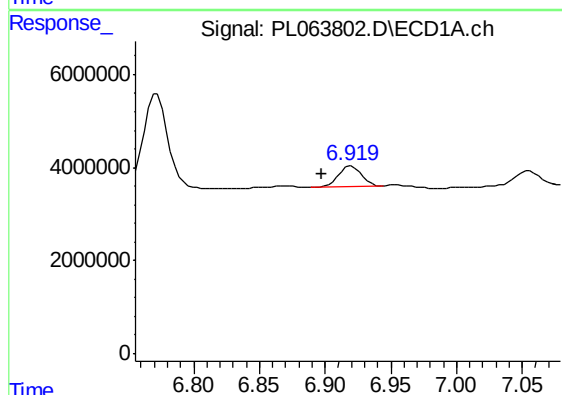


#20 Methoxychlor

R.T.: 6.920 min
Delta R.T.: 0.023 min
Response: 5269358
Conc: 4.01 ng/ml

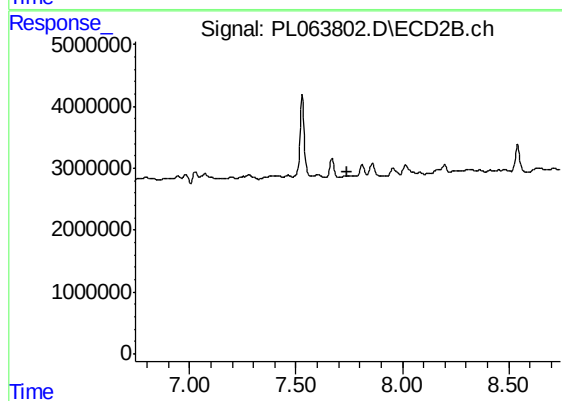

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.743 min
Response: 0
Conc: N.D.

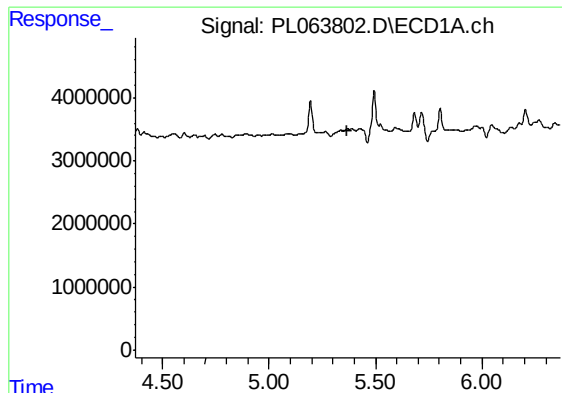

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
18

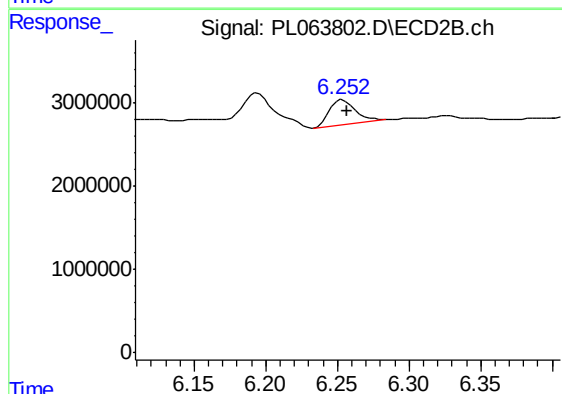


#25 Chlordane-3

R.T.: 6.254 min
Delta R.T.: -0.003 min
Response: 3777422
Conc: 11.02 ng/ml

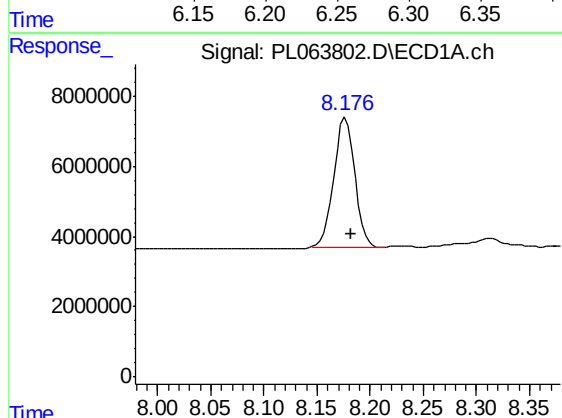

#28 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: -0.005 min
Response: 50456179
Conc: 18.31 ng/ml

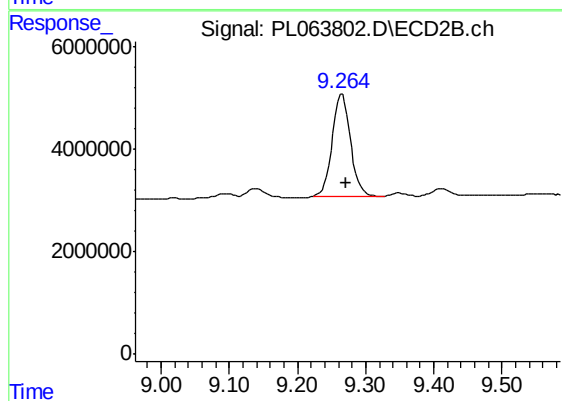

#28 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.006 min
Response: 37031359
Conc: 18.78 ng/ml