

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122321\
 Data File : PL071593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2021 08:43
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:58:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10) B	gamma-Chl...	0.000	8.232	0	142842	0.110 #
14) MA	Endrin	0.000	8.913f	0	78776	0.078 #
15) B	Endosulfa...	0.000	9.119	0	483827	0.479 #
18) B	Endrin al...	0.000	9.277f	0	392523	0.521 #
20) A	Methoxychlor	0.000	9.825	0	393896	0.785 #
21) B	Endrin ke...	0.000	9.995	0	237025	0.225 #
22)	Mirex	0.000	10.460	0	361600	0.449 #
25)	Chlordane-3	0.000	8.232	0	142842	0.816 #
27)	Chlordane-5	0.000	9.172f	0	1095872	31.191 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122321\
Data File : PL071593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2021 08:43
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:58:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

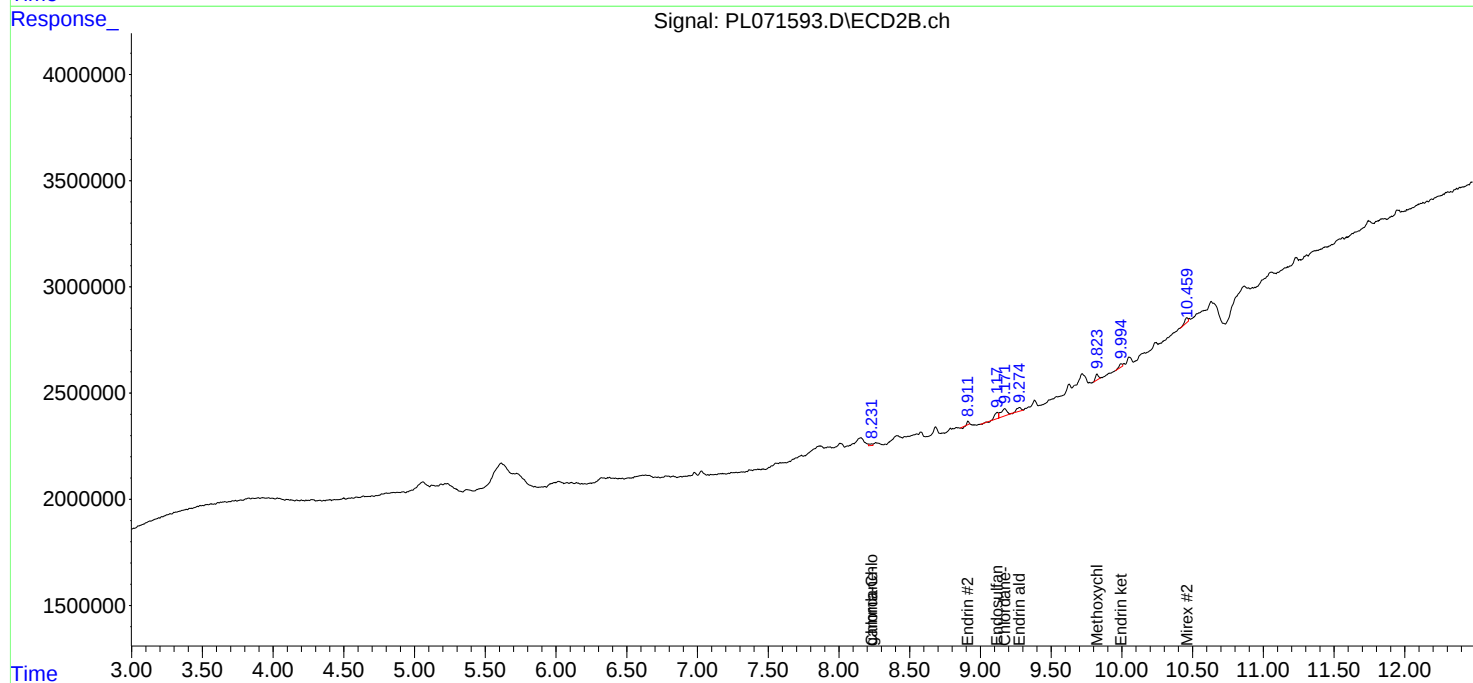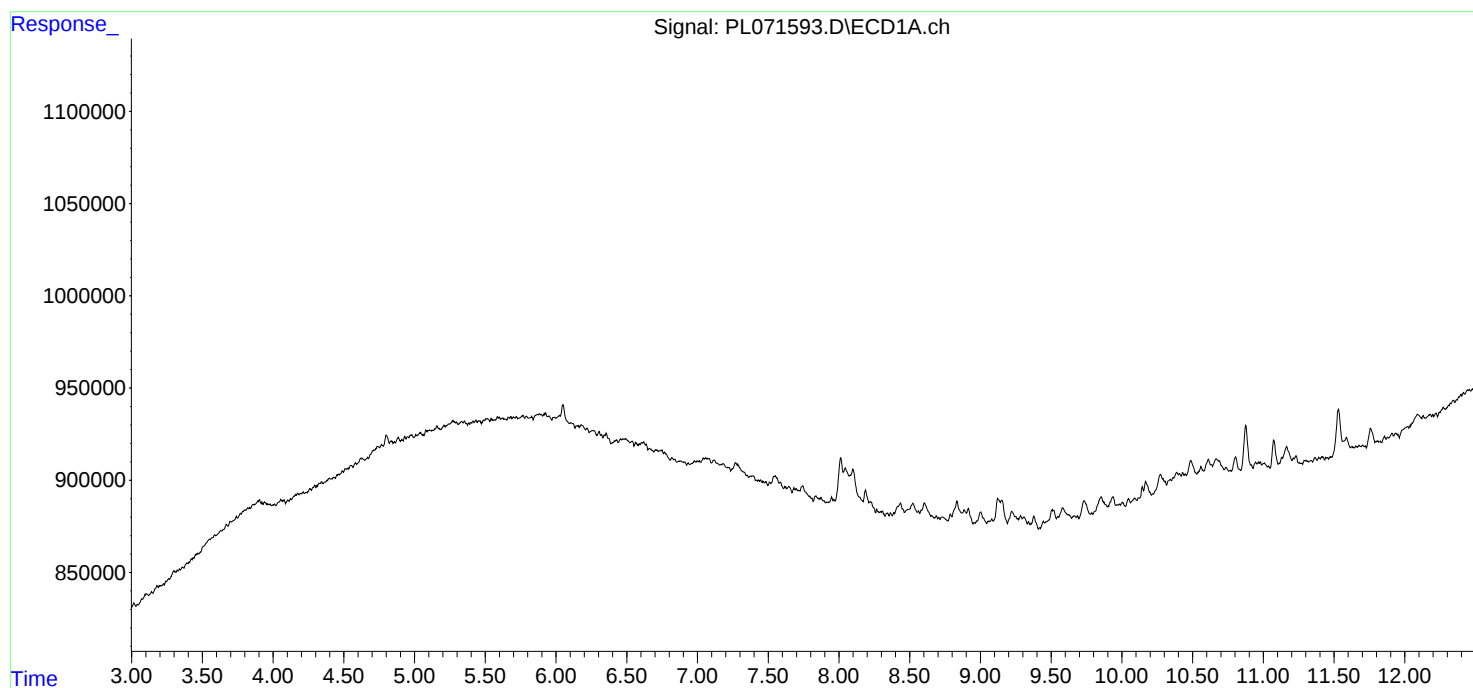


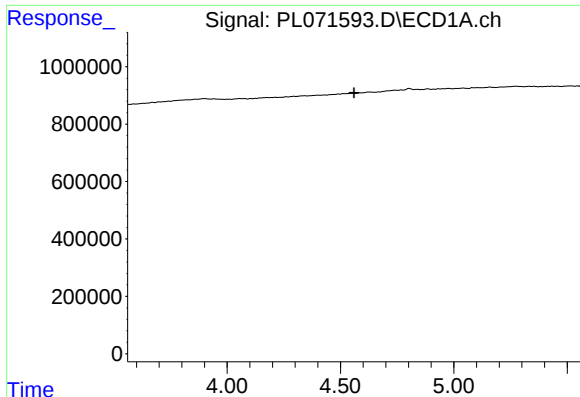

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

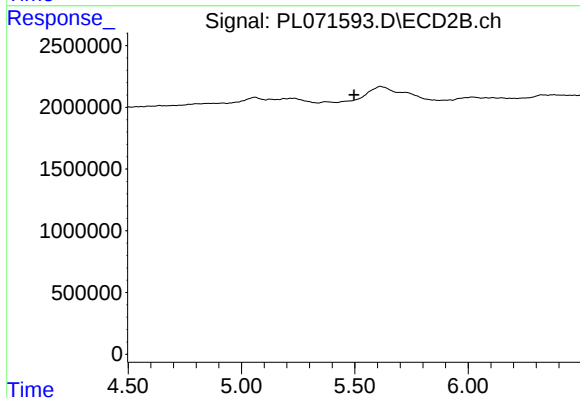


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

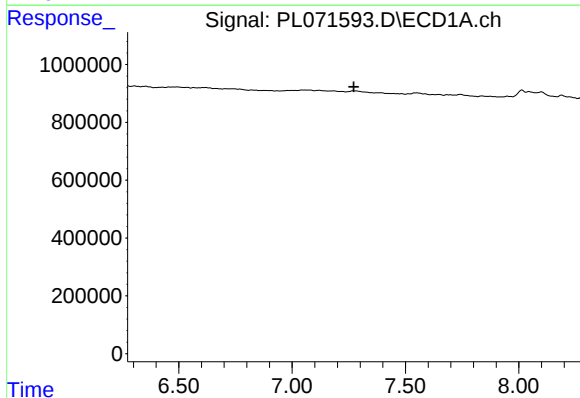


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

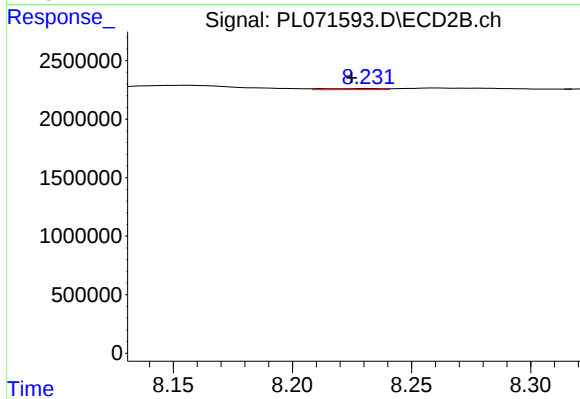

#10 gamma-Chlordane


R.T.: 8.232 min
Delta R.T.: 0.007 min
Response: 142842
Conc: 0.11 ng/ml

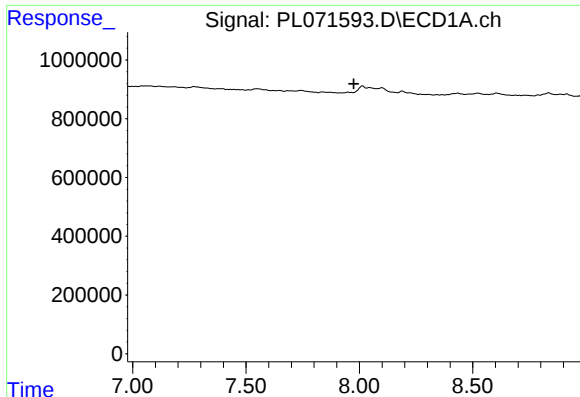

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

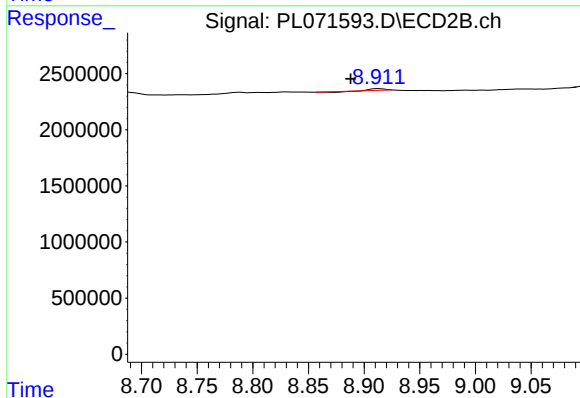


#14 Endrin

R.T.: 8.913 min
Delta R.T.: 0.025 min
Response: 78776
Conc: 0.08 ng/ml

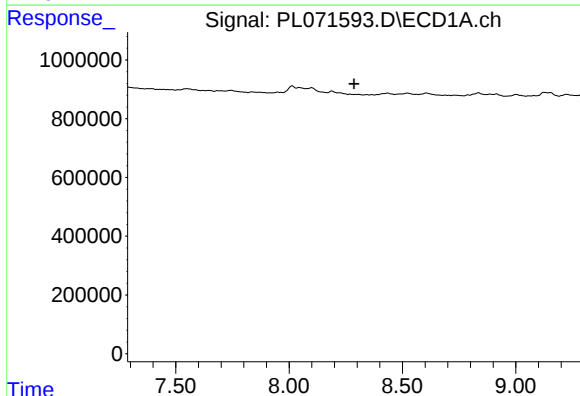


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

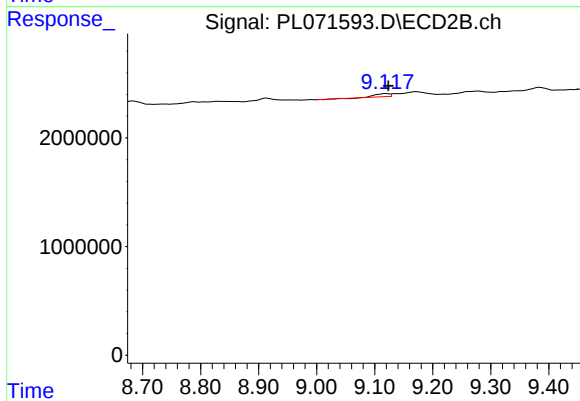

#15 Endosulfan II


R.T.: 9.119 min
Delta R.T.: -0.005 min
Response: 483827
Conc: 0.48 ng/ml

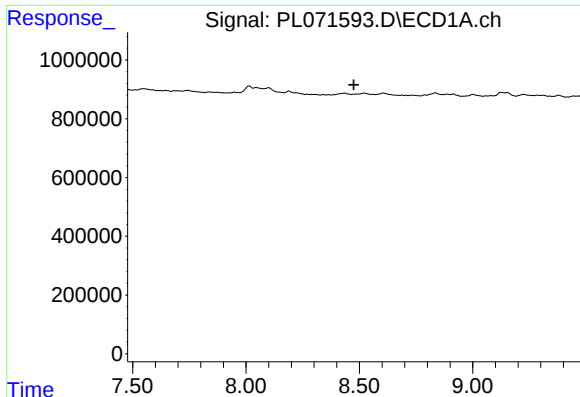

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

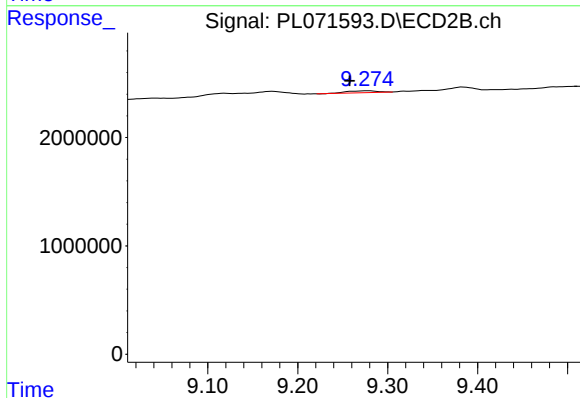


#18 Endrin aldehyde

R.T.: 9.277 min
Delta R.T.: 0.020 min
Response: 392523
Conc: 0.52 ng/ml

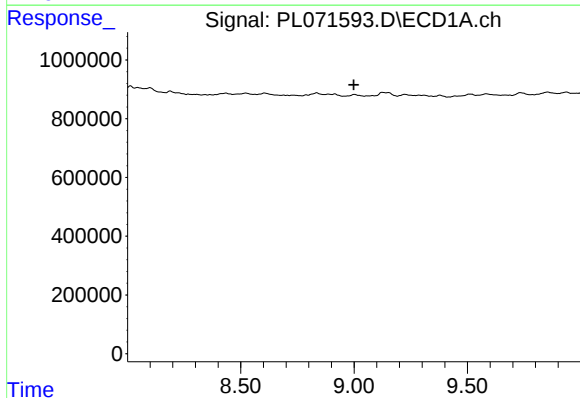


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 8.998 min
Response: 0
Conc: N.D.

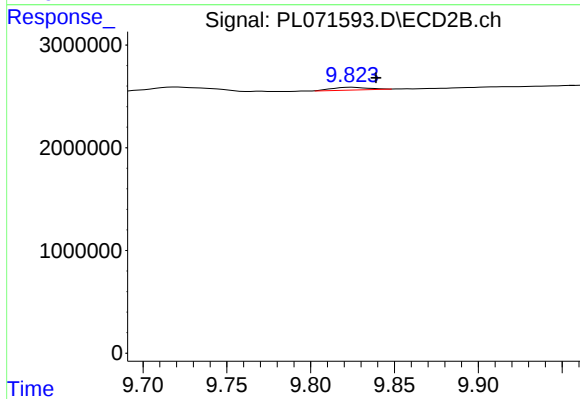

#20 Methoxychlor


R.T.: 9.825 min
Delta R.T.: -0.015 min
Response: 393896
Conc: 0.78 ng/ml

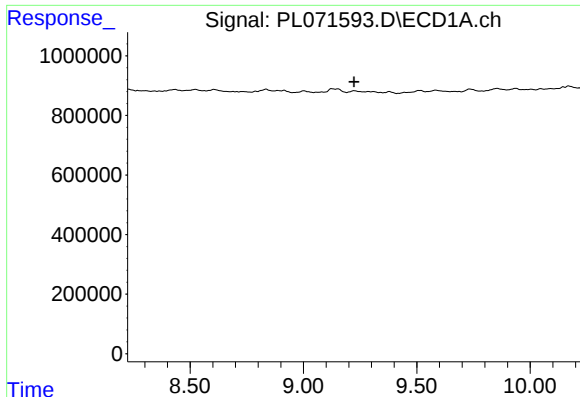

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

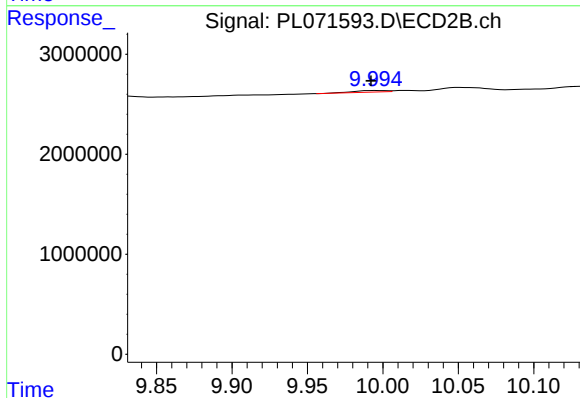


#21 Endrin ketone

R.T.: 9.995 min
Delta R.T.: 0.003 min
Response: 237025
Conc: 0.23 ng/ml

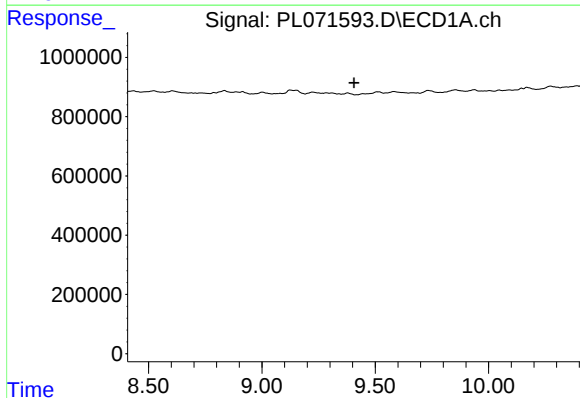


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.406 min
Response: 0
Conc: N.D.

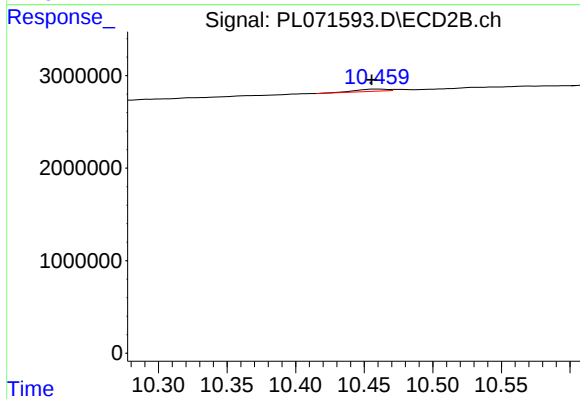

#22 Mirex


R.T.: 10.460 min
Delta R.T.: 0.005 min
Response: 361600
Conc: 0.45 ng/ml

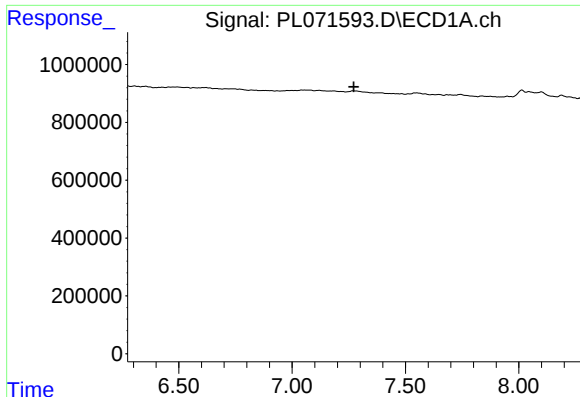

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

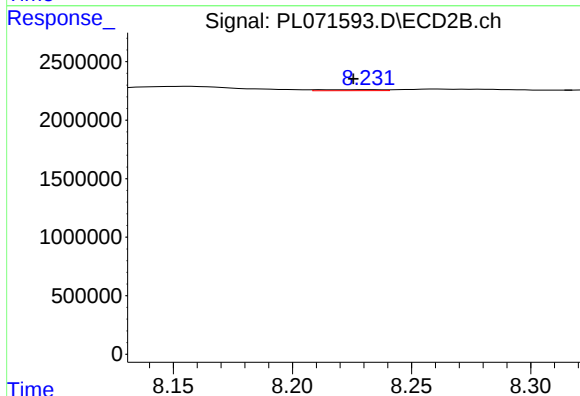


#25 Chlordane-3

R.T.: 8.232 min
Delta R.T.: 0.007 min
Response: 142842
Conc: 0.82 ng/ml

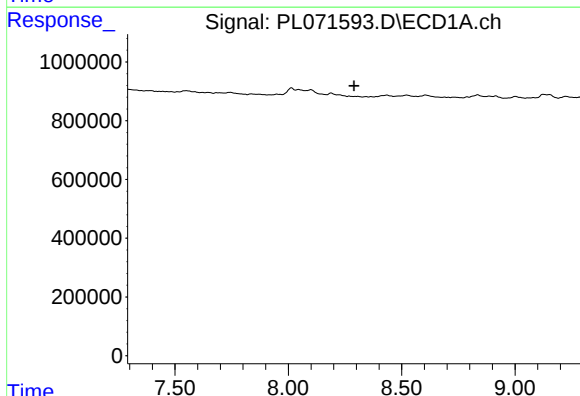


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.290 min
Response: 0
Conc: N.D.

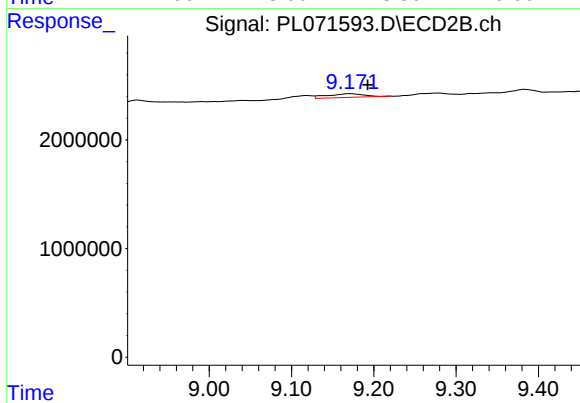

#27 Chlordane-5


R.T.: 9.172 min
Delta R.T.: -0.020 min
Response: 1095872
Conc: 31.19 ng/ml

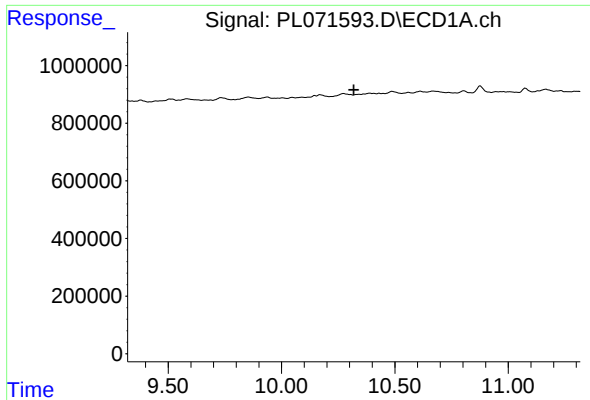

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

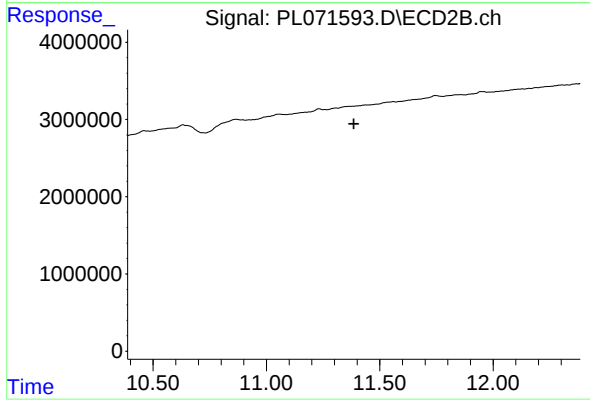

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.385 min
Response: 0
Conc: N.D.