

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122321\
 Data File : PL071606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2021 16:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 01:02:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.495	11221194	27617815	23.674	23.183
28)	SA Decachlor...	10.327	11.390	16357438	28096948	24.620	25.860
Target Compounds							
2)	A alpha-BHC	5.252	6.054f	267026	630172	0.420	0.366
4)	MA Heptachlor	6.082	7.134f	470042	124636	0.680	0.078 #
6)	B beta-BHC	6.082	0.000	470042	0	1.646	N.D. #
8)	B Heptachlo...	0.000	7.967	0	635717	N.D.	0.474 #
9)	A Endosulfan I	0.000	8.344f	0	123845	N.D.	0.103 #
14)	MA Endrin	0.000	8.914f	0	369460	N.D.	0.365 #
15)	B Endosulfa...	0.000	9.144f	0	1263077	N.D.	1.252 #
19)	B Endosulfa...	0.000	9.514f	0	100199	N.D.	0.102 #
20)	A Methoxychlor	0.000	9.828	0	177985	N.D.	0.355 #
21)	B Endrin ke...	0.000	10.017f	0	767245	N.D.	0.730 #
27)	Chlordane-5	0.000	9.168f	0	337151	N.D.	9.596 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122321\
Data File : PL071606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2021 16:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 01:02:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

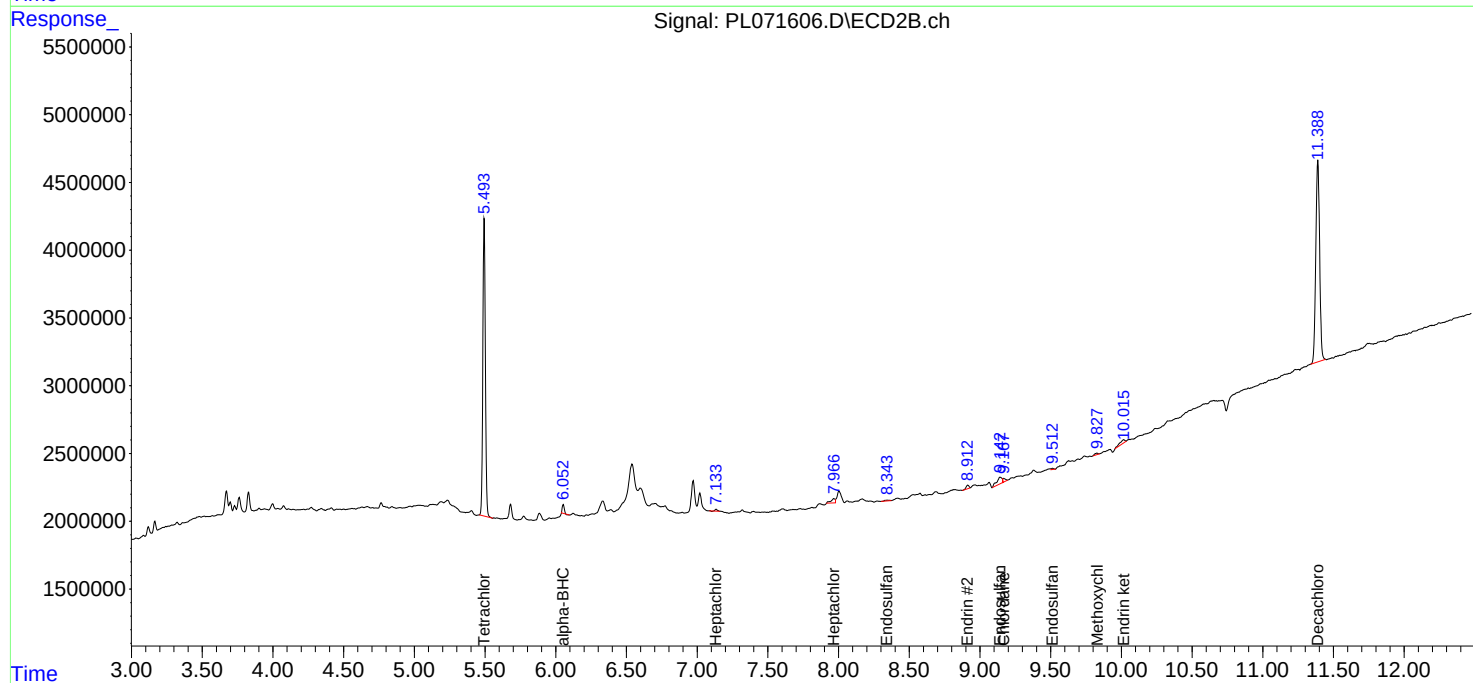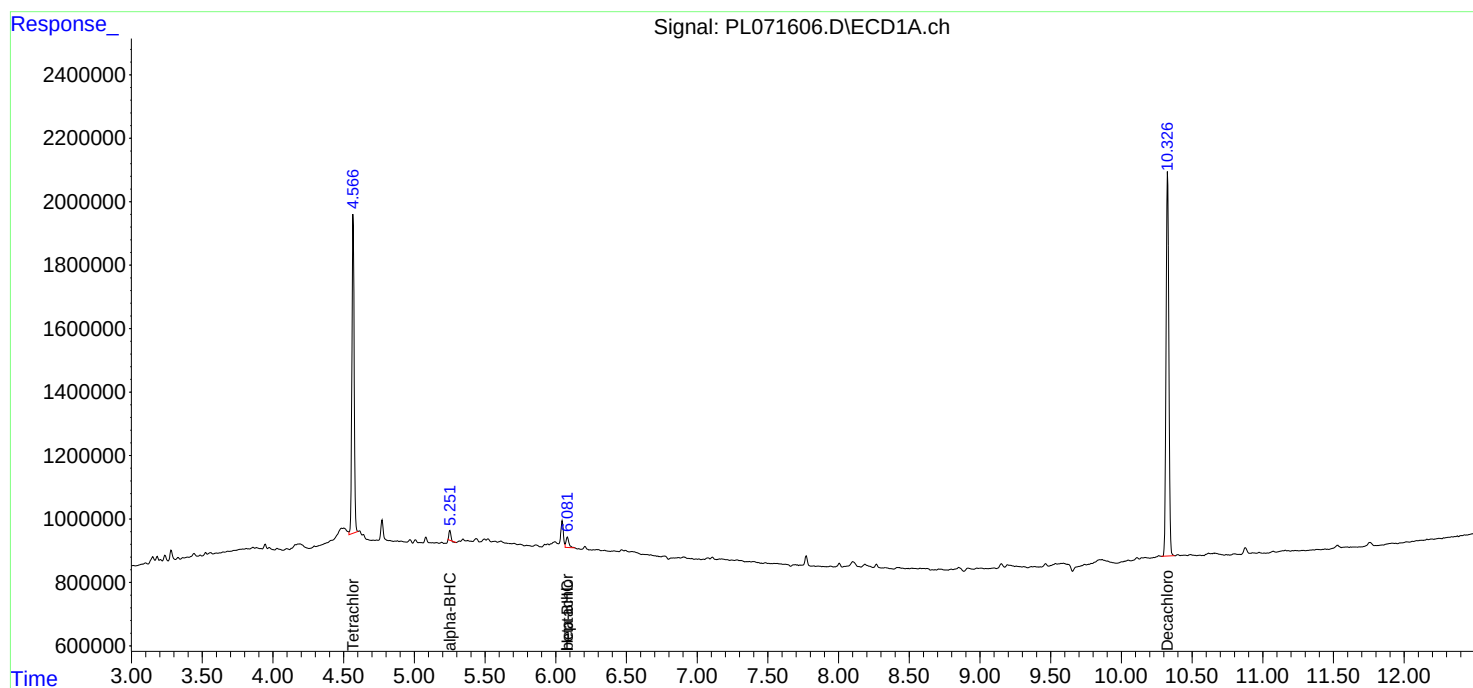


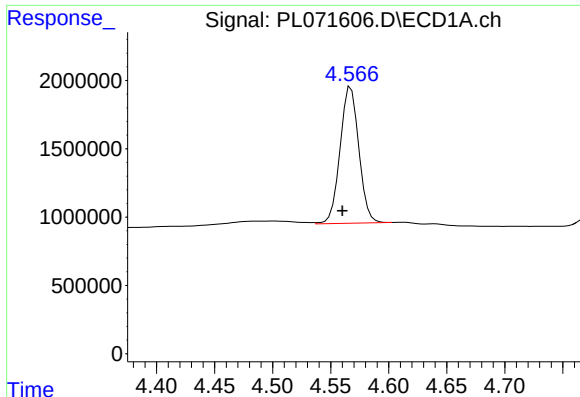

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.007 min
Response: 11221194
Conc: 23.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

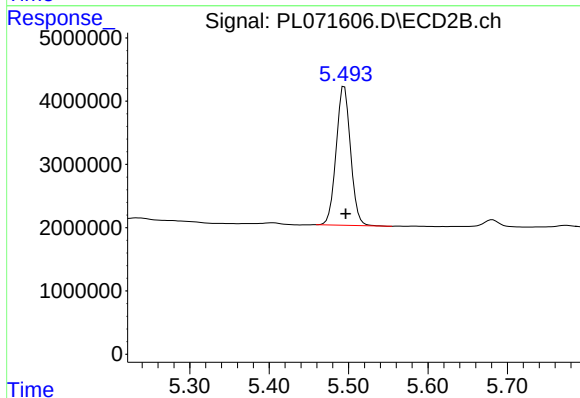


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: -0.002 min
Response: 27617815
Conc: 23.18 ng/ml

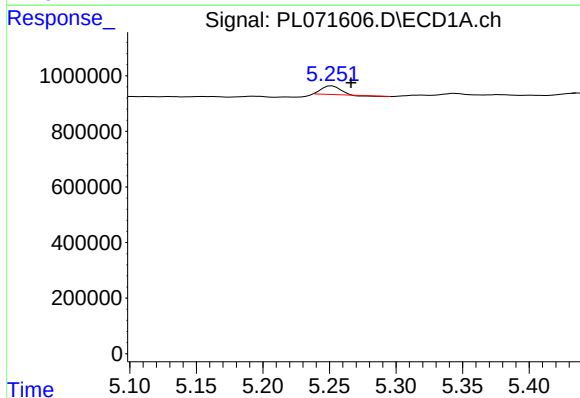


#2 alpha-BHC

R.T.: 5.252 min
Delta R.T.: -0.014 min
Response: 267026
Conc: 0.42 ng/ml

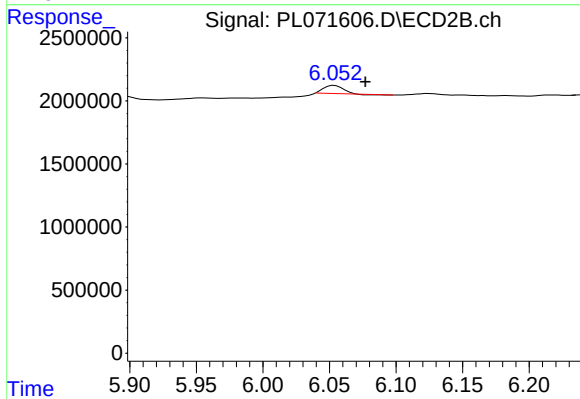

#2 alpha-BHC


R.T.: 6.054 min
Delta R.T.: -0.023 min
Response: 630172
Conc: 0.37 ng/ml

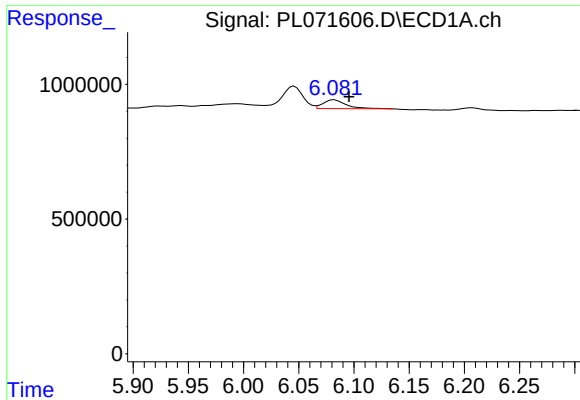

#4 Heptachlor


R.T.: 6.082 min
Delta R.T.: -0.013 min
Response: 470042
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

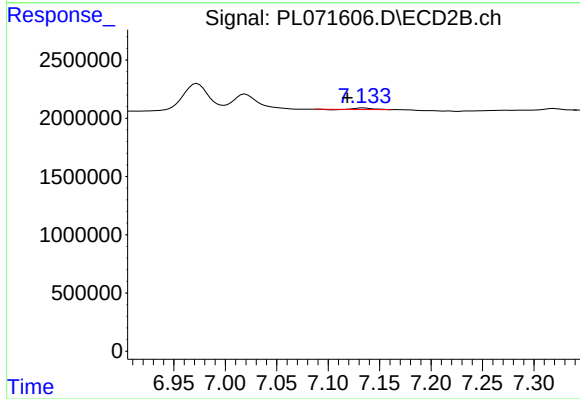


#4 Heptachlor

R.T.: 7.134 min
Delta R.T.: 0.016 min
Response: 124636
Conc: 0.08 ng/ml

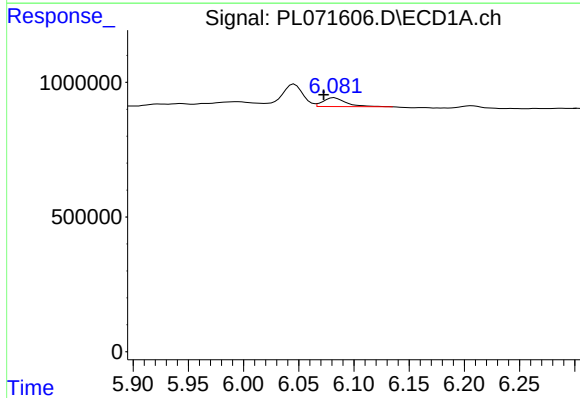


#6 beta-BHC

R.T.: 6.082 min
Delta R.T.: 0.010 min
Response: 470042
Conc: 1.65 ng/ml

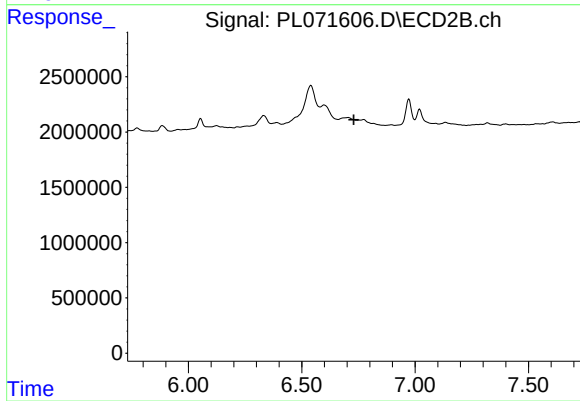

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.730 min
Response: 0
Conc: N.D.

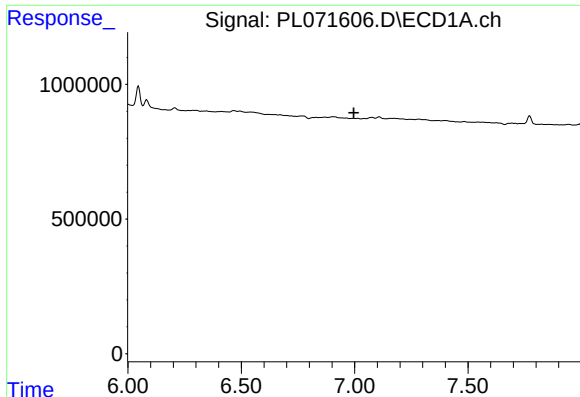

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

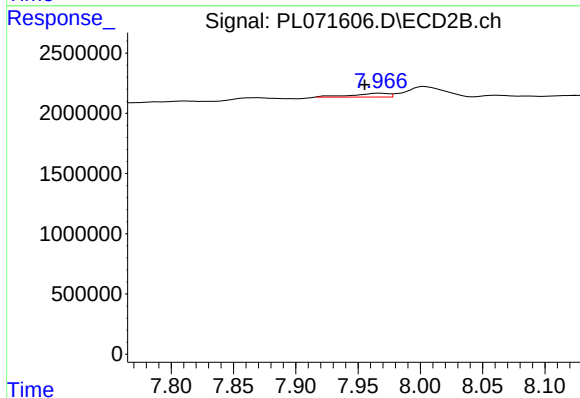


#8 Heptachlor epoxide

R.T.: 7.967 min
Delta R.T.: 0.012 min
Response: 635717
Conc: 0.47 ng/ml

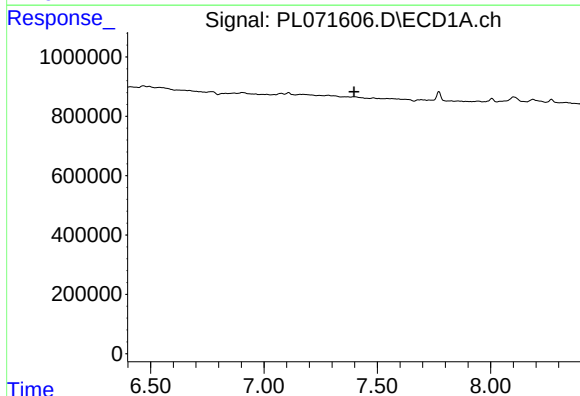


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

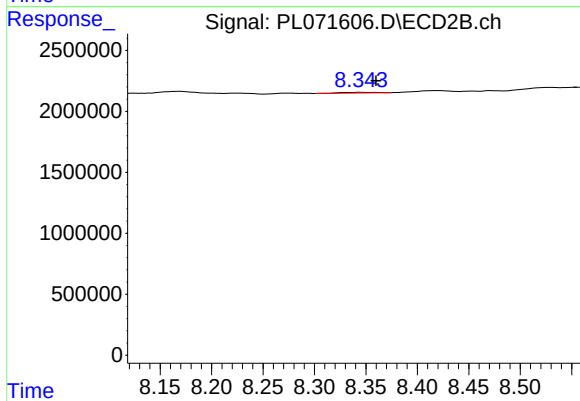

#9 Endosulfan I


R.T.: 8.344 min
Delta R.T.: -0.015 min
Response: 123845
Conc: 0.10 ng/ml

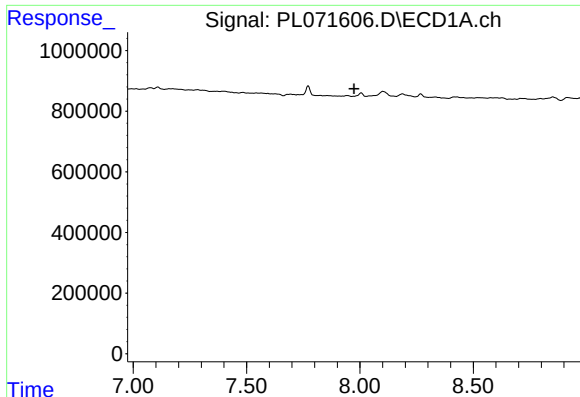

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

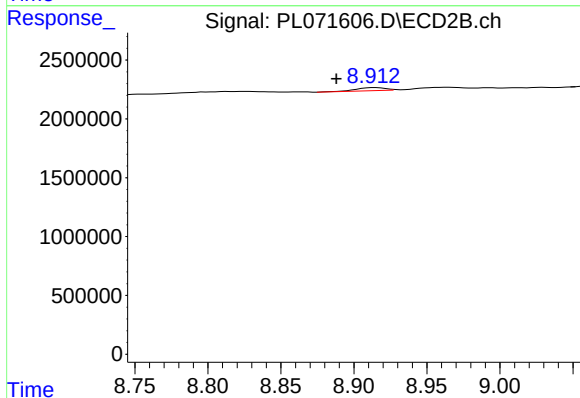


#14 Endrin

R.T.: 8.914 min
Delta R.T.: 0.026 min
Response: 369460
Conc: 0.36 ng/ml

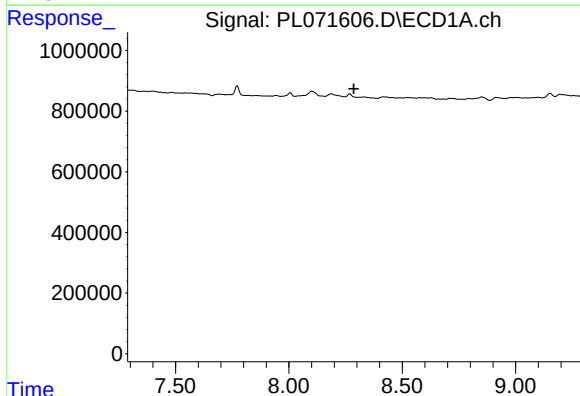


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

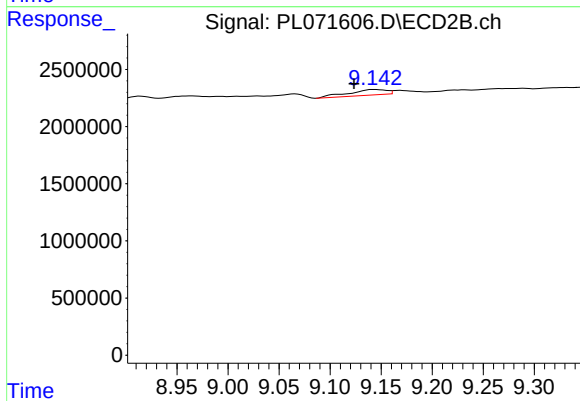

#15 Endosulfan II


R.T.: 9.144 min
Delta R.T.: 0.020 min
Response: 1263077
Conc: 1.25 ng/ml

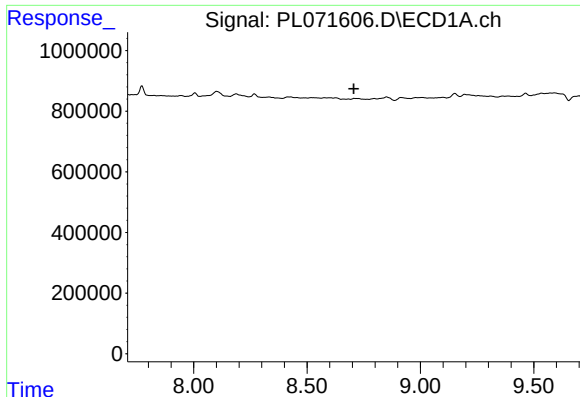

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

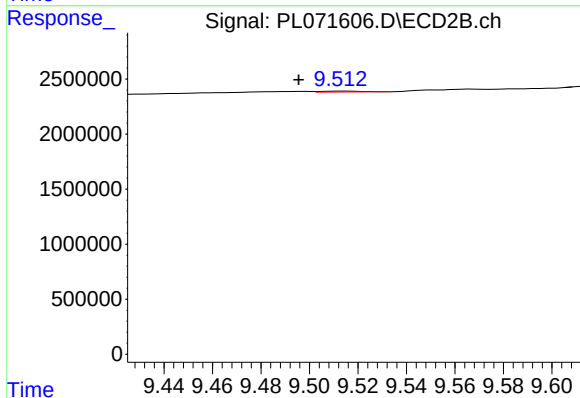


#19 Endosulfan Sulfate

R.T.: 9.514 min
Delta R.T.: 0.018 min
Response: 100199
Conc: 0.10 ng/ml

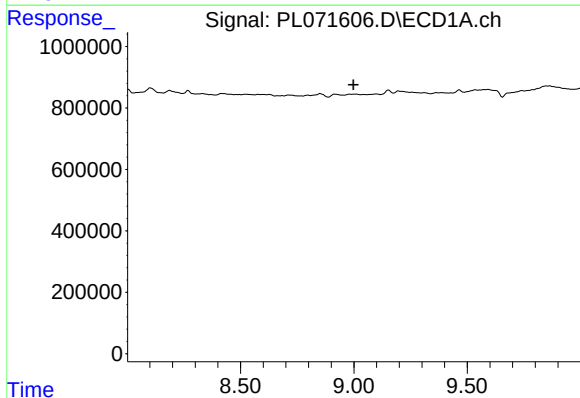


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 8.998 min
Response: 0
Conc: N.D.

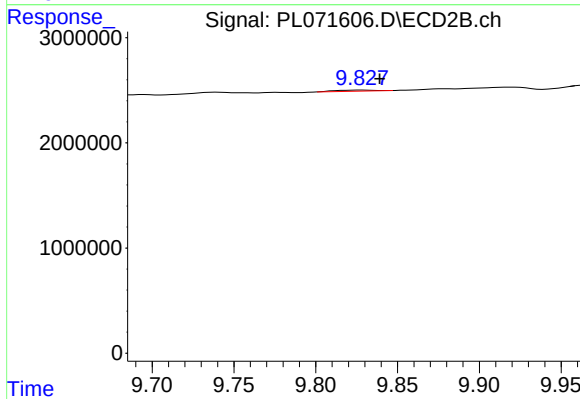

#20 Methoxychlor


R.T.: 9.828 min
Delta R.T.: -0.011 min
Response: 177985
Conc: 0.35 ng/ml

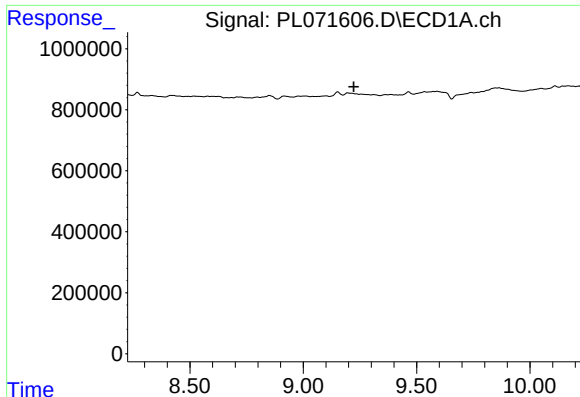

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

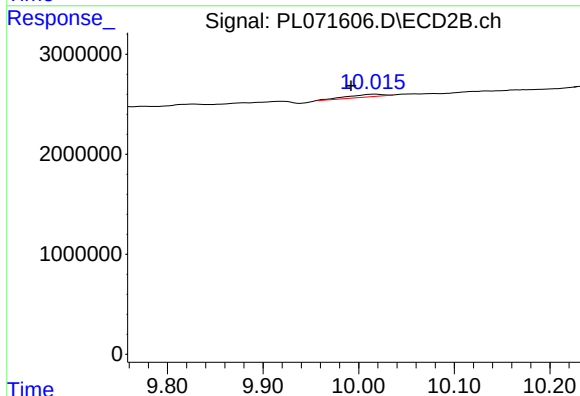


#21 Endrin ketone

R.T.: 10.017 min
Delta R.T.: 0.025 min
Response: 767245
Conc: 0.73 ng/ml

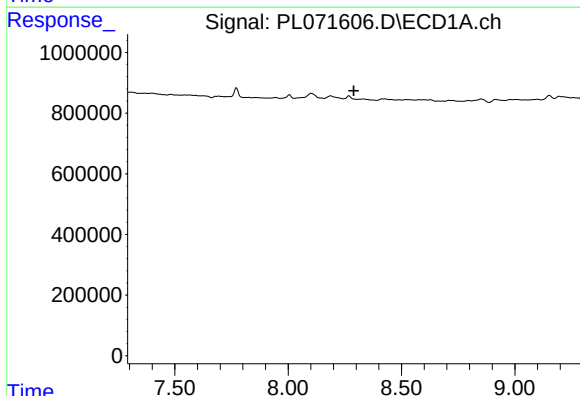


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.290 min
Response: 0
Conc: N.D.

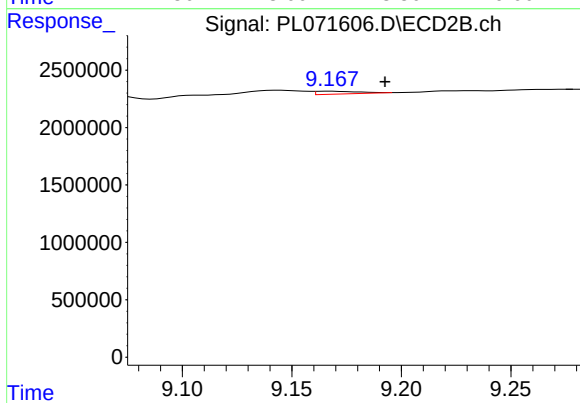

#27 Chlordane-5


R.T.: 9.168 min
Delta R.T.: -0.024 min
Response: 337151
Conc: 9.60 ng/ml

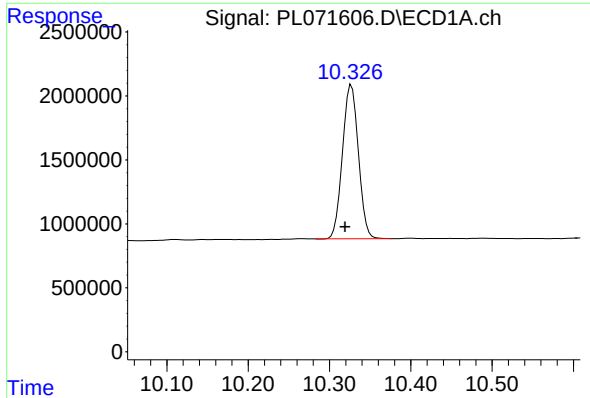

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.008 min
Response: 16357438
Conc: 24.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

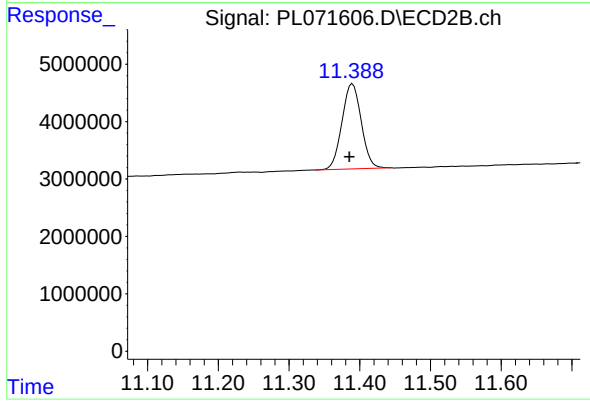

#28 Decachlorobiphenyl

R.T.: 11.390 min
Delta R.T.: 0.005 min
Response: 28096948
Conc: 25.86 ng/ml